


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003038.D
Acq On : 09 Oct 2018 21:51
Operator : MJ/SJ
Sample : J5157-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD0

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:49 PM

Quant Time: Oct 10 02:08:25 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

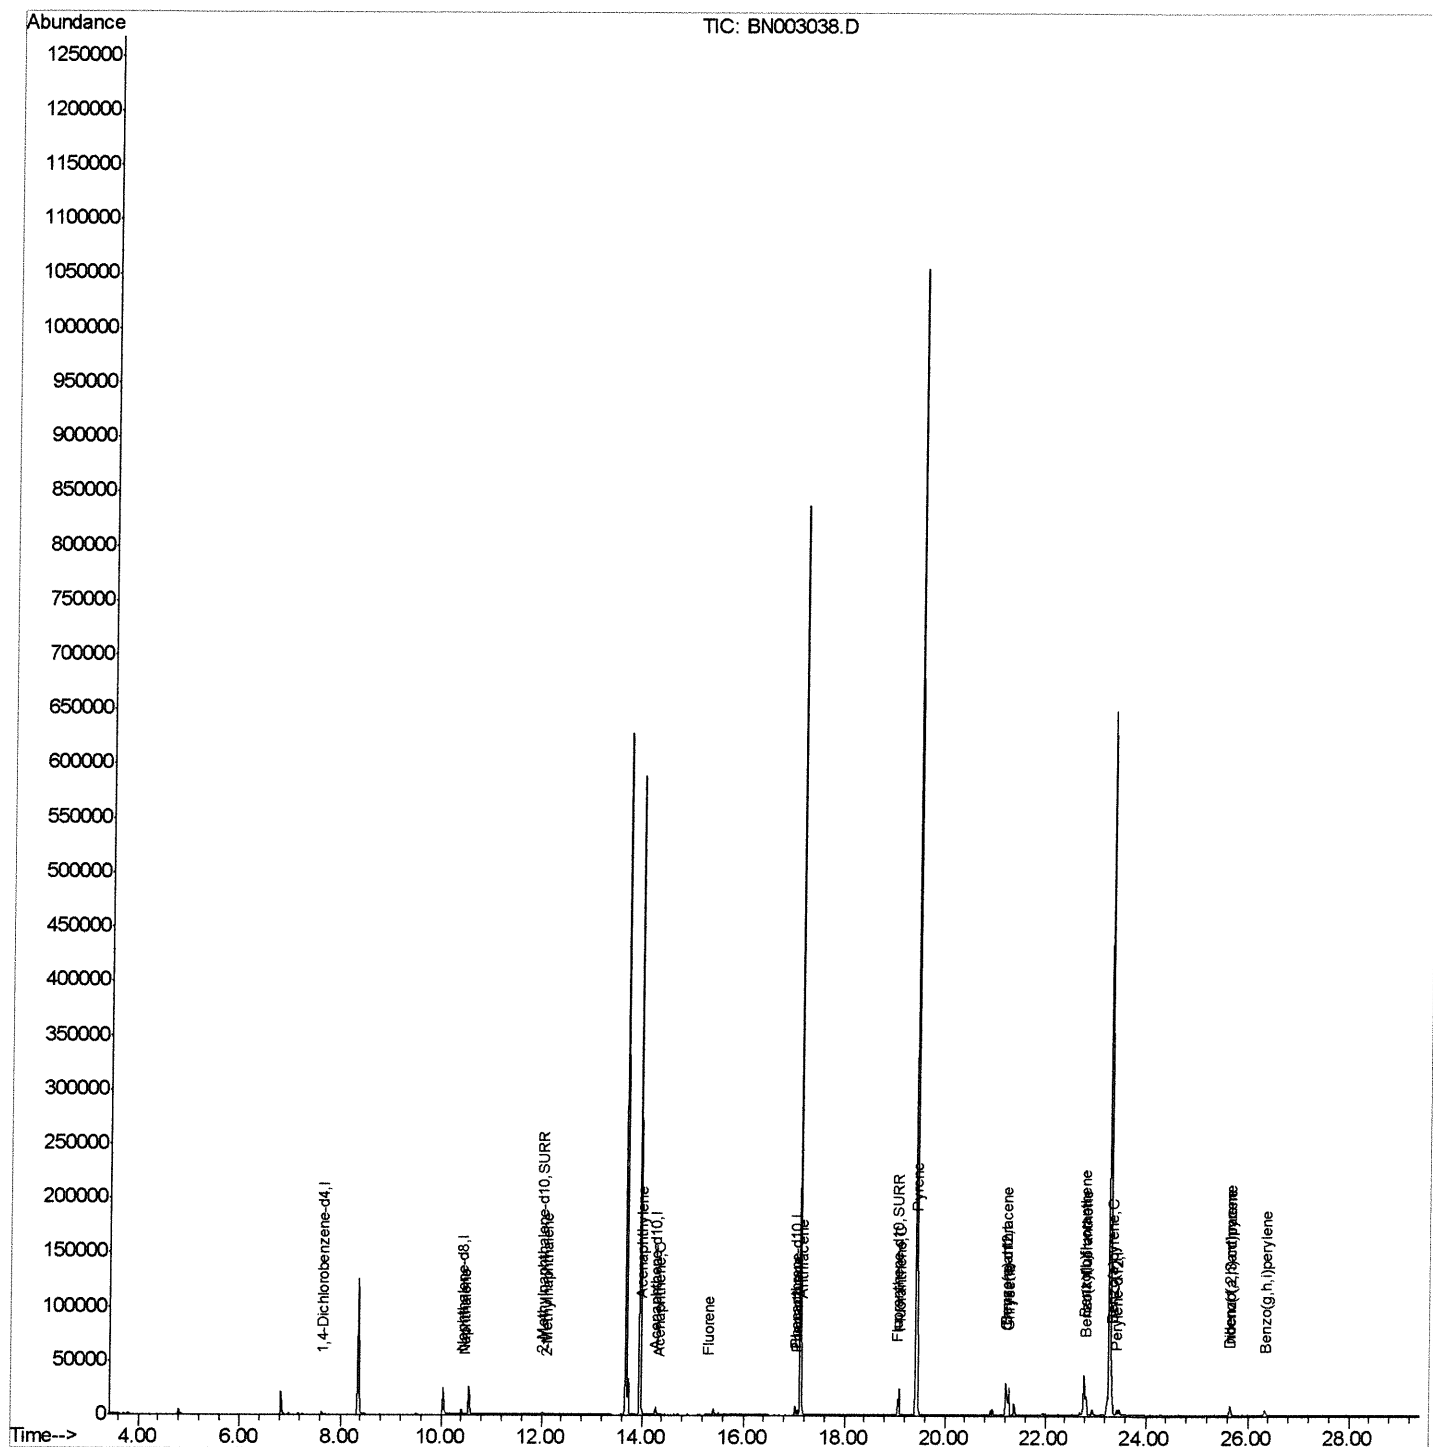

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003038.D
 Acq On : 09 Oct 2018 21:51
 Operator : MJ/SJ
 Sample : J5157-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:49 PM

Quant Time: Oct 10 01:38:04 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

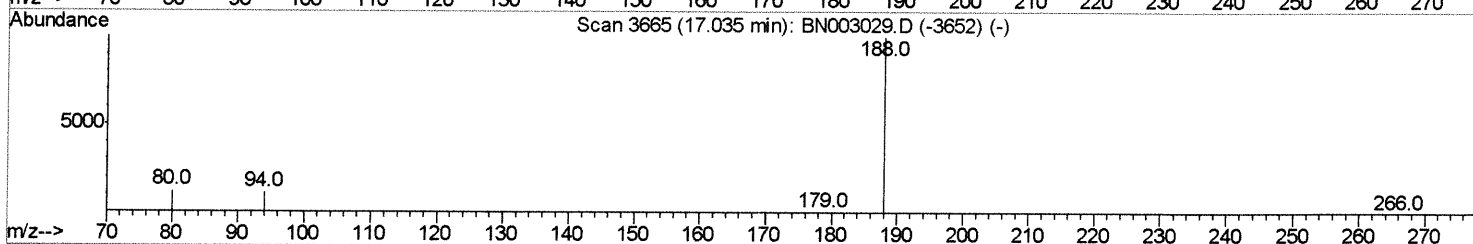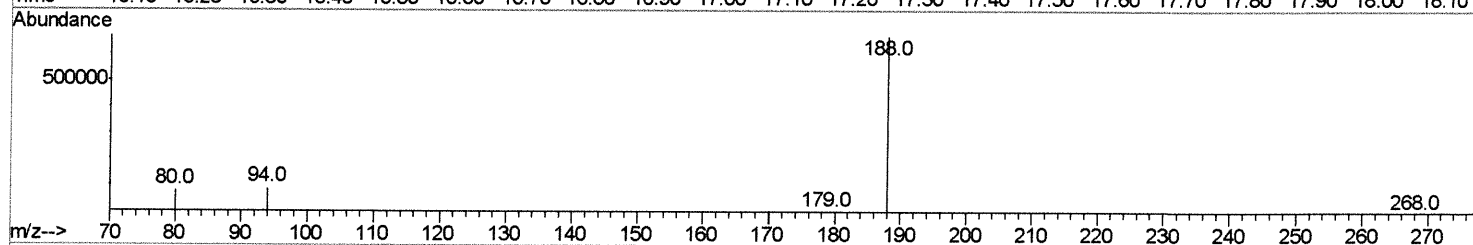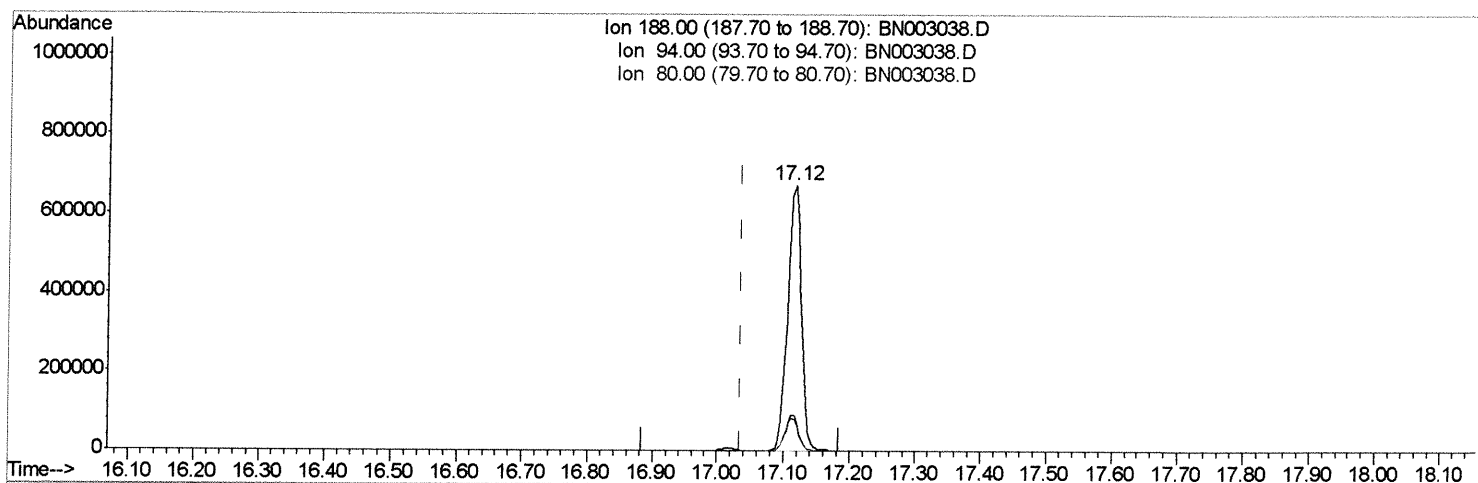

TIC: BN003038.D

(10) Phenanthrene-d10 (I)
 17.116min (+0.080) 0.40ng/ul
 response 959084

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	13.03
80.00	12.70	11.84
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003038.D
 Acq On : 09 Oct 2018 21:51
 Operator : MJ/SJ
 Sample : J5157-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:49 PM

Quant Time: Oct 10 01:38:04 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

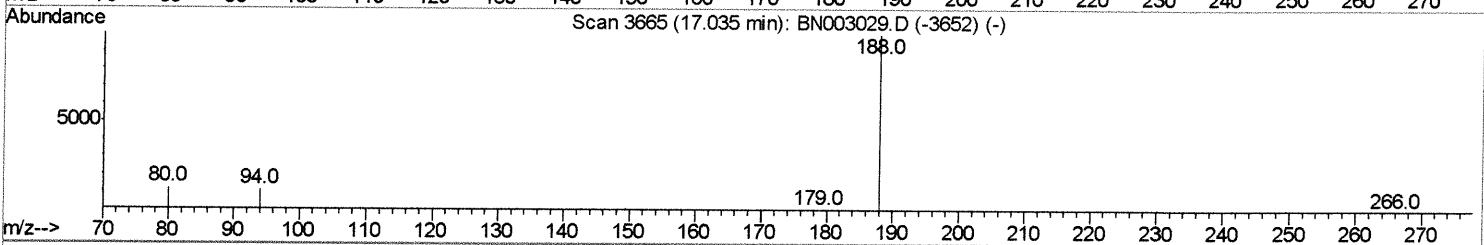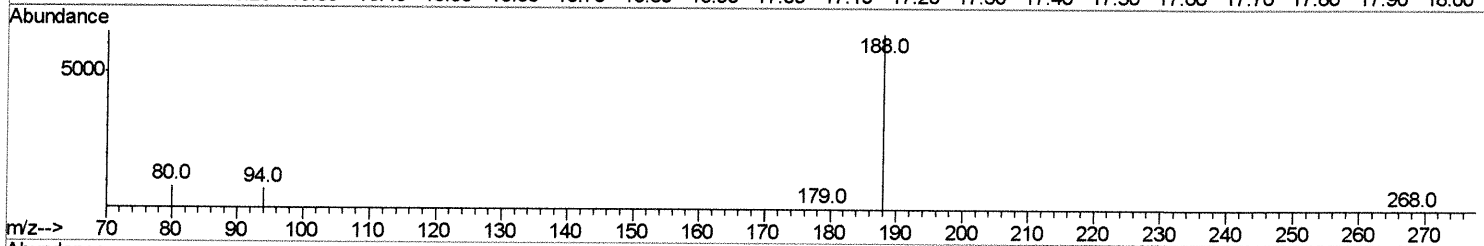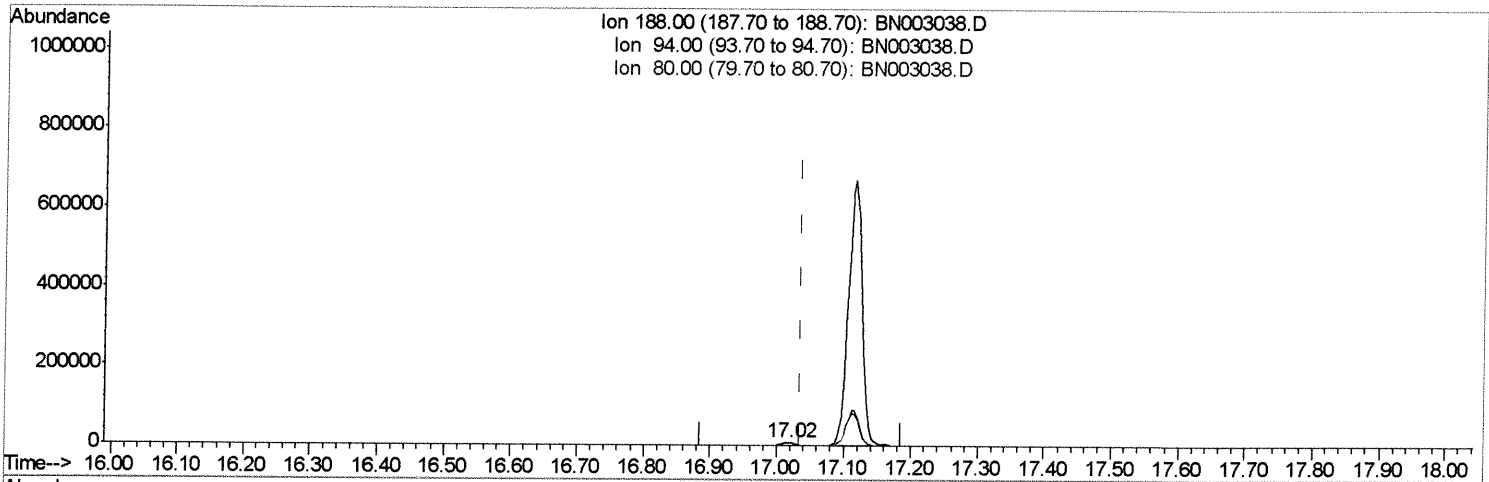

TIC: BN003038.D

(10) Phenanthrene-d10 (I)

17.019min (-0.017) 0.40ng/ul m *SJ 10/12/18*

response 9447

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	11.84
80.00	12.70	13.30
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003038.D
 Acq On : 09 Oct 2018 21:51
 Operator : MJ/SJ
 Sample : J5157-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:49 PM

Quant Time: Oct 10 02:05:44 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

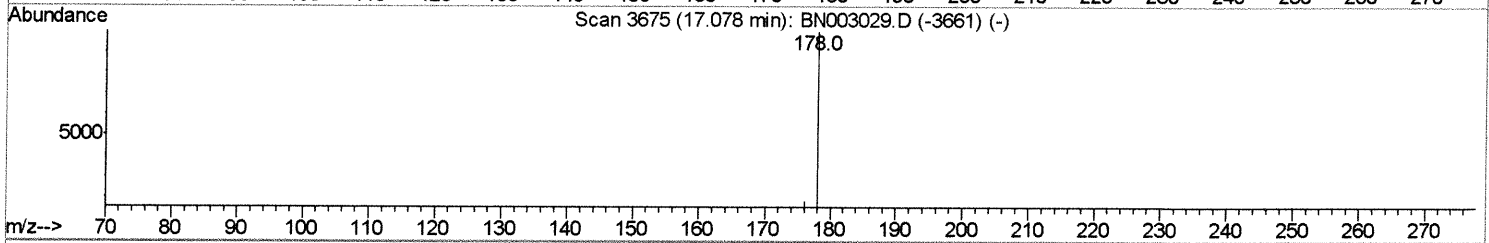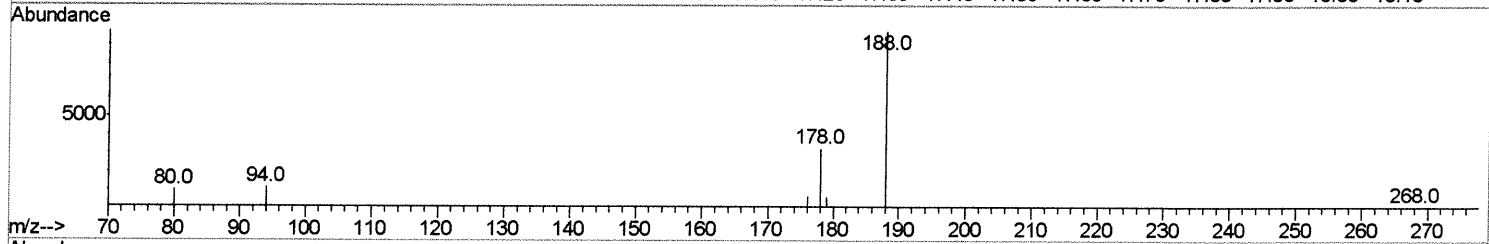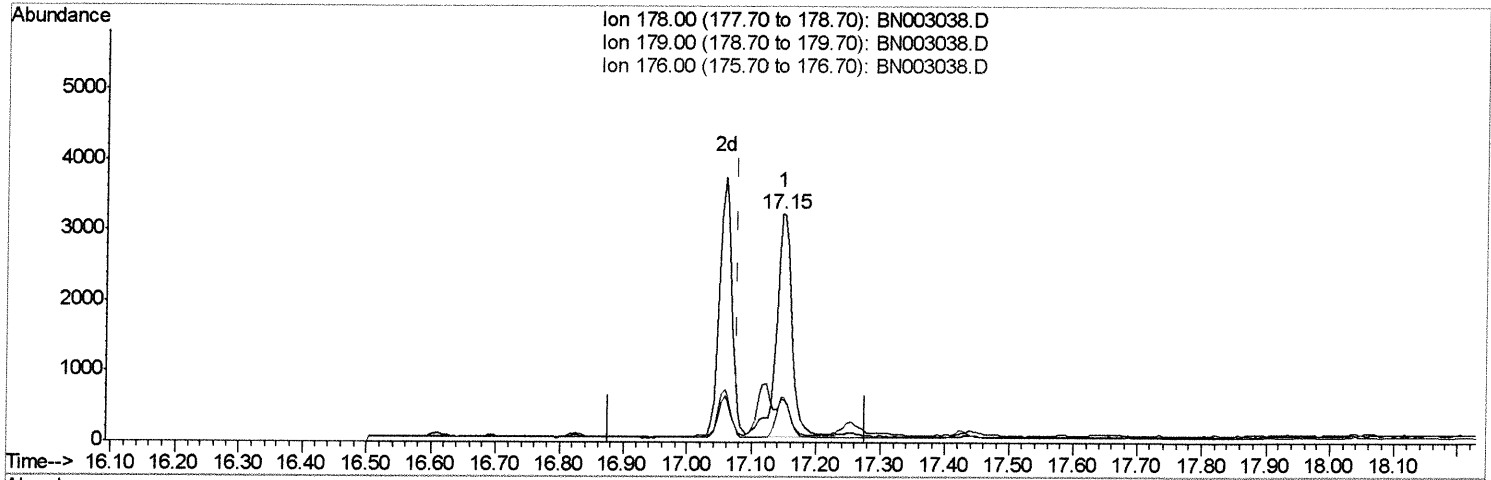

TIC: BN003038.D

(12) Phenanthrene

17.145min (+0.068) 0.20ng/ul

response 5373

Ion	Exp%	Act%
178.00	100	100
179.00	16.10	18.82
176.00	19.30	19.93
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003038.D
 Acq On : 09 Oct 2018 21:51
 Operator : MJ/SJ
 Sample : J5157-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:49 PM

Quant Time: Oct 10 02:05:44 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

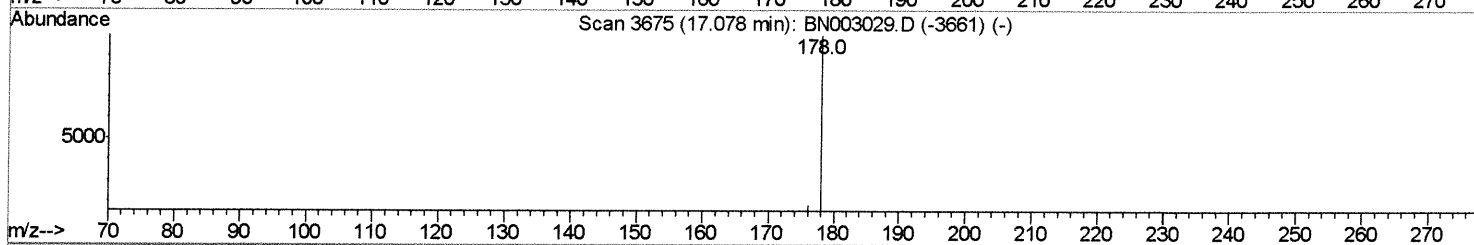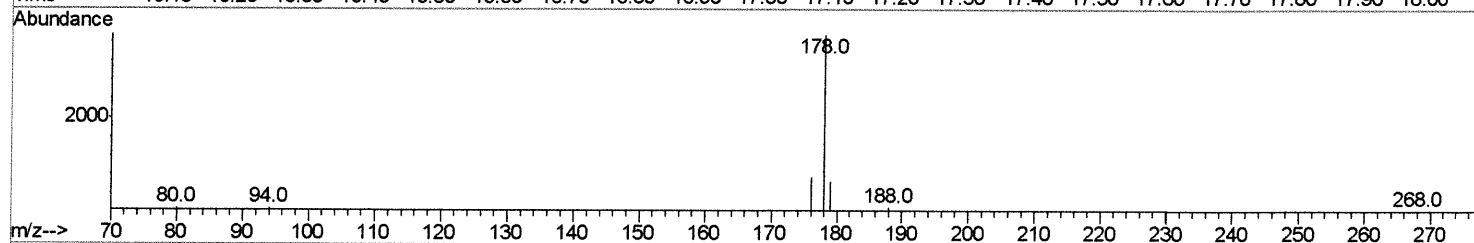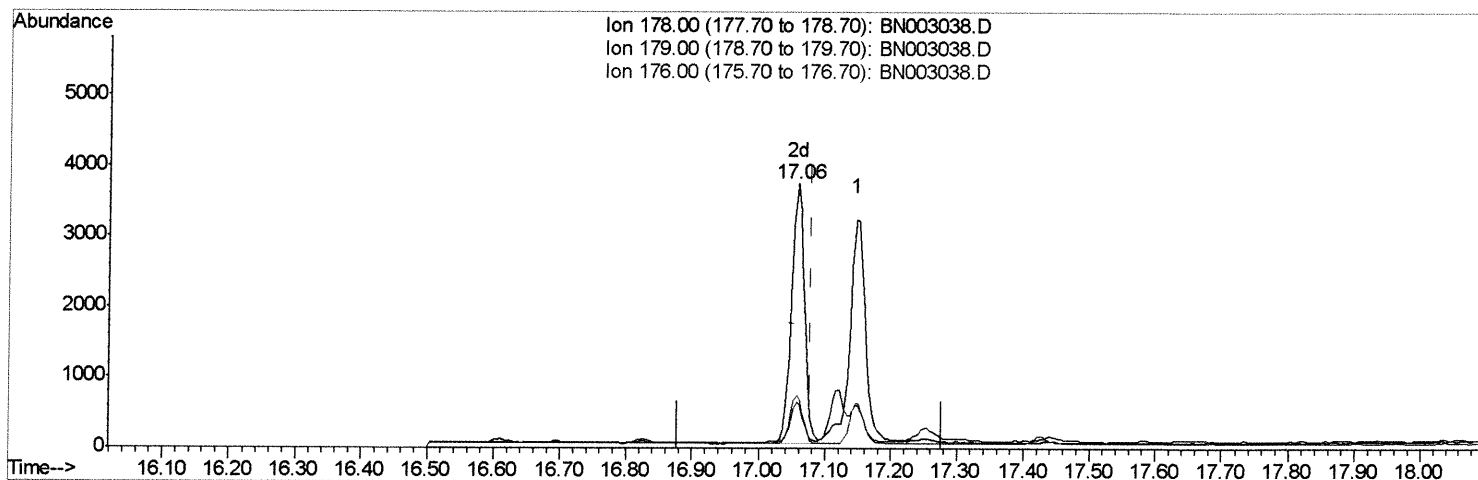

TIC: BN003038.D

(12) Phenanthrene

17.057min (-0.021) 0.19ng/ul m

SJ 10/12/18

response 4995

Ion	Exp%	Act%
178.00	100	100
179.00	16.10	17.62
176.00	19.30	19.96
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003038.D
Acq On : 09 Oct 2018 21:51
Operator : MJ/SJ
Sample : J5157-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD0

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:49 PM

Quant Time: Oct 10 02:05:44 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

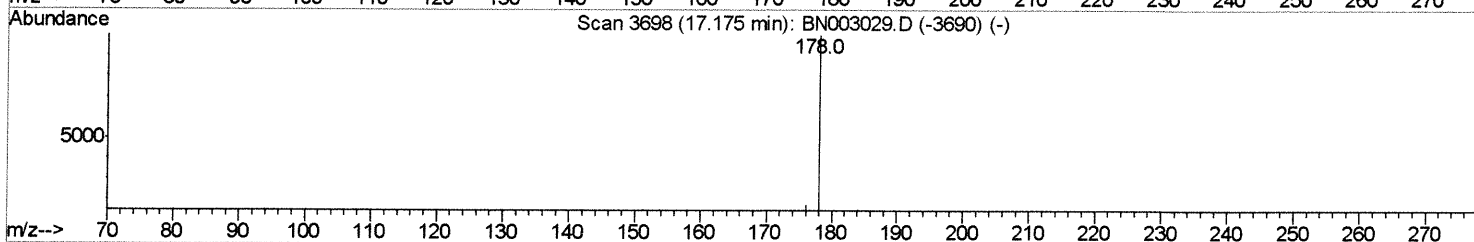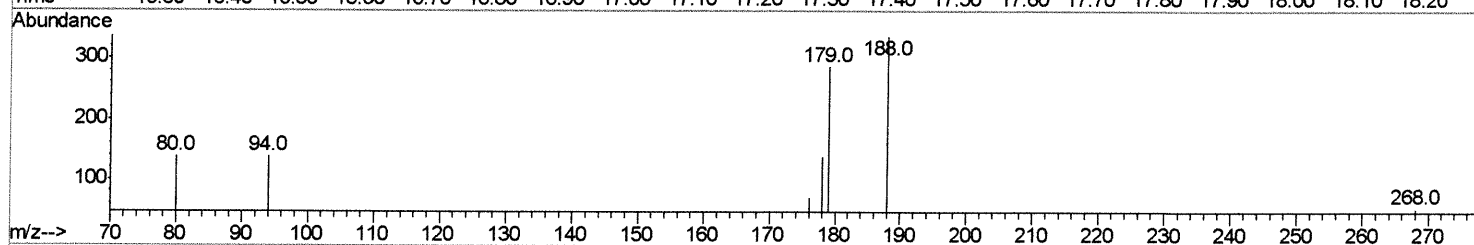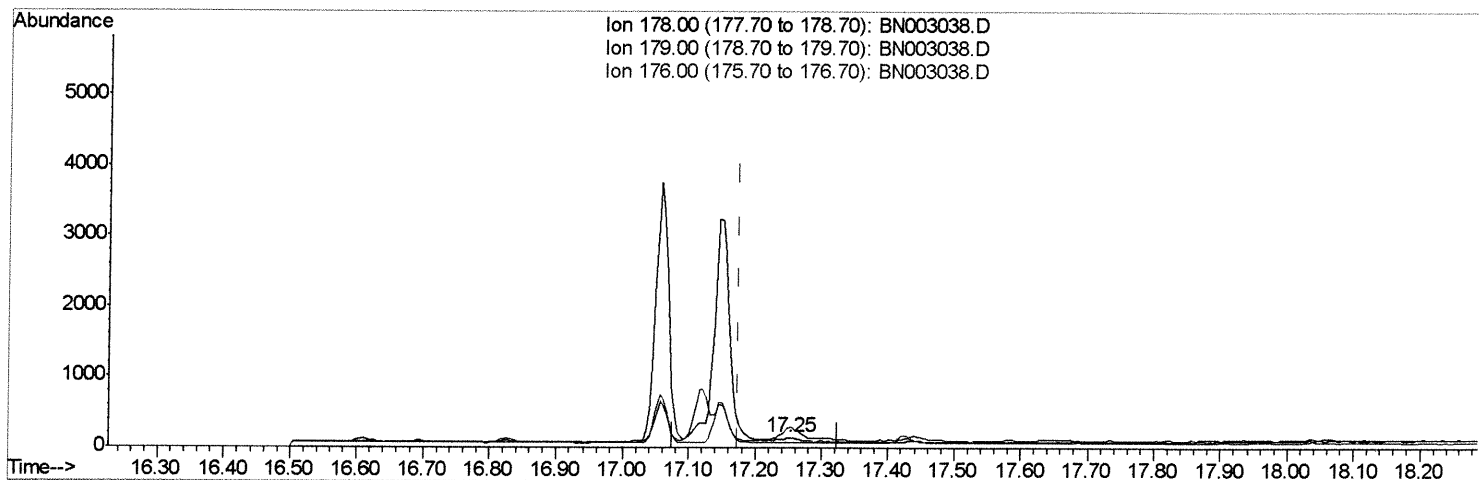

TIC: BN003038.D

(13) Anthracene

17.251min (+0.076) 0.00ng/ul

response 93

Ion	Exp%	Act%
178.00	100	100
179.00	16.30	205.76#
176.00	19.10	51.08#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003038.D
 Acq On : 09 Oct 2018 21:51
 Operator : MJ/SJ
 Sample : J5157-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:49 PM

Quant Time: Oct 10 02:05:44 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

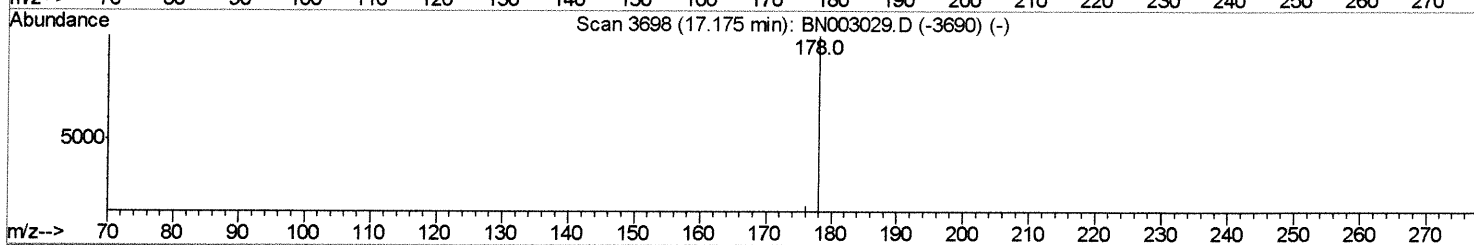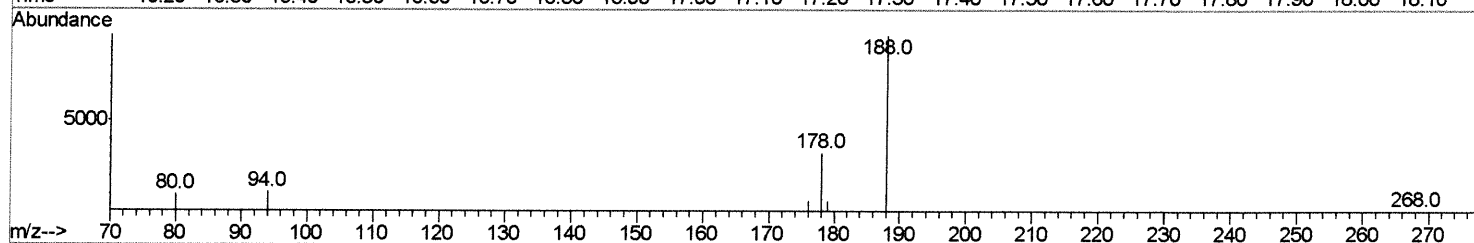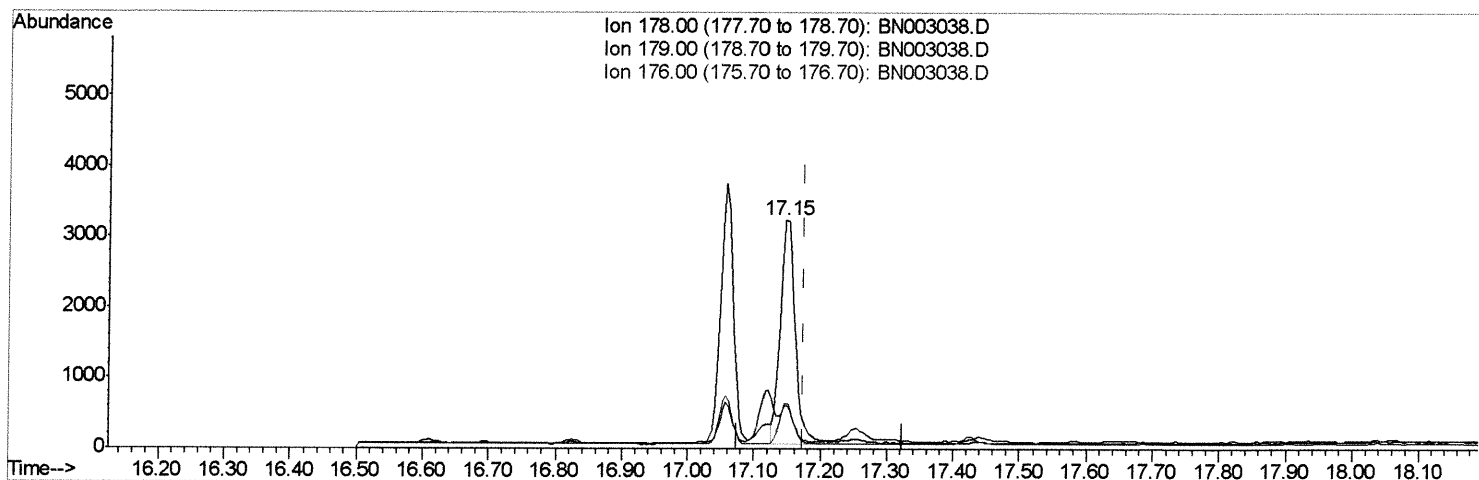

TIC: BN003038.D

(13) Anthracene

17.145min (-0.029) 0.20ng/ul m

51 10/12/18

response 4961

Ion	Exp%	Act%
178.00	100	100
179.00	16.30	18.82
176.00	19.10	19.93
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003038.D
 Acq On : 09 Oct 2018 21:51
 Operator : MJ/SJ
 Sample : J5157-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:49 PM

Quant Time: Oct 10 02:05:44 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

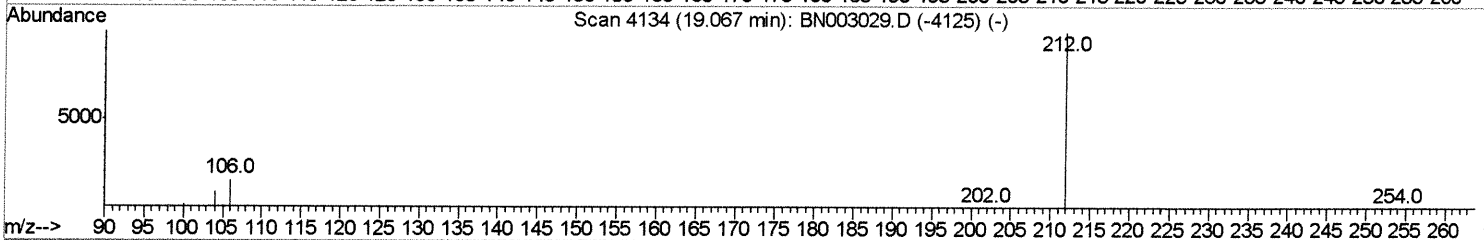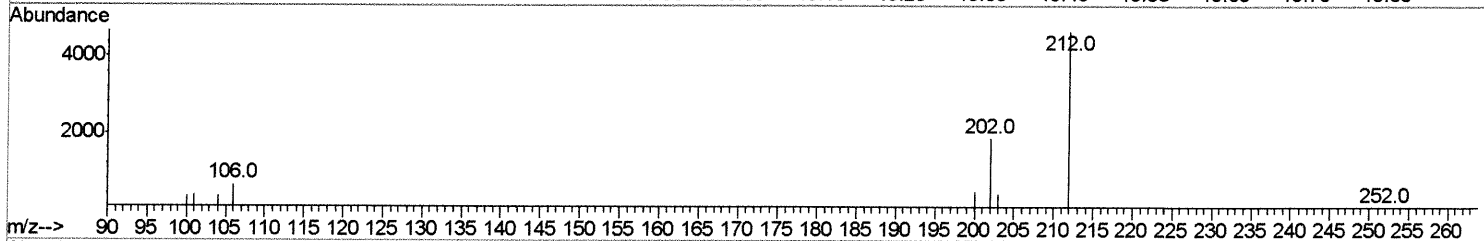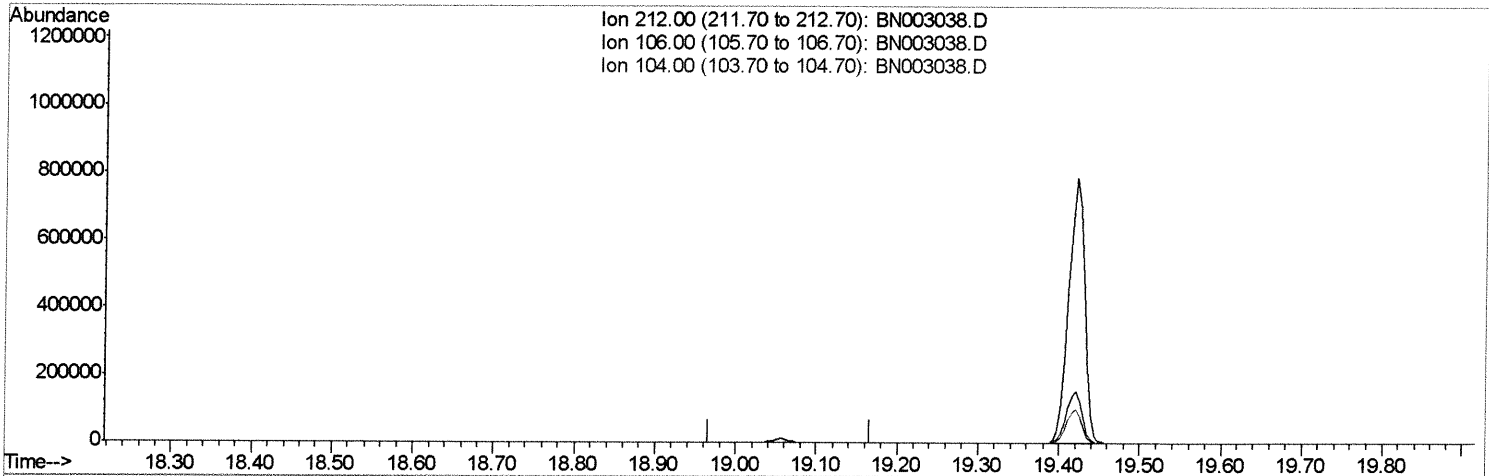

TIC: BN003038.D

(14) Fluoranthene-d10 (SURR)

19.067min (-19.067) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	15.40	0.00#
104.00	8.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003038.D
Acq On : 09 Oct 2018 21:51
Operator : MJ/SJ
Sample : J5157-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD0

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:49 PM

Quant Time: Oct 10 02:05:44 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

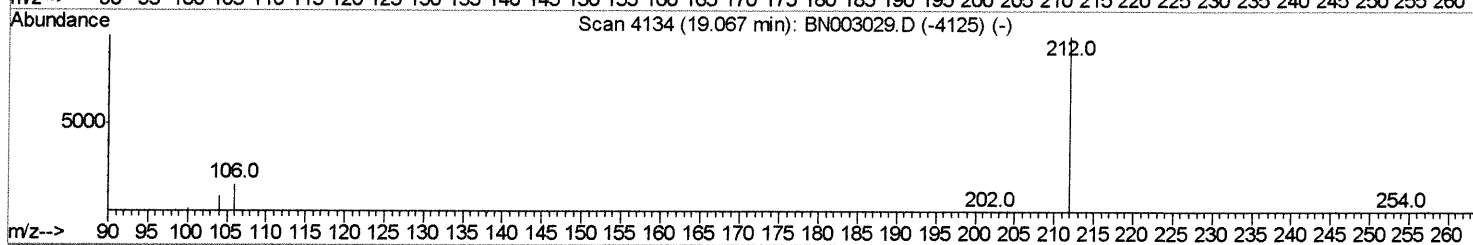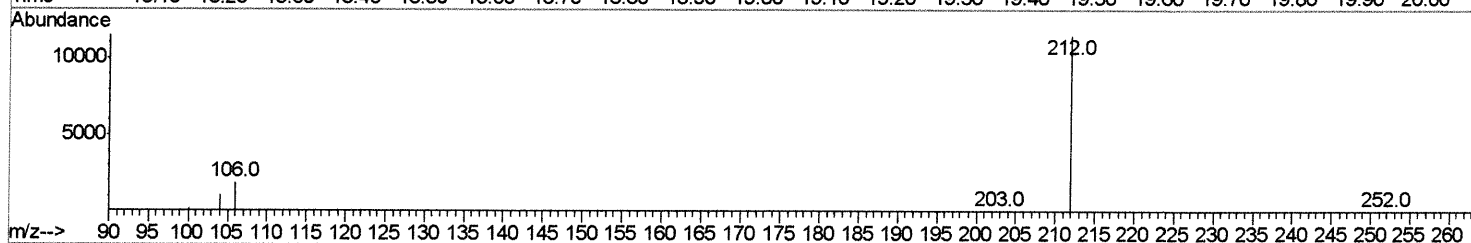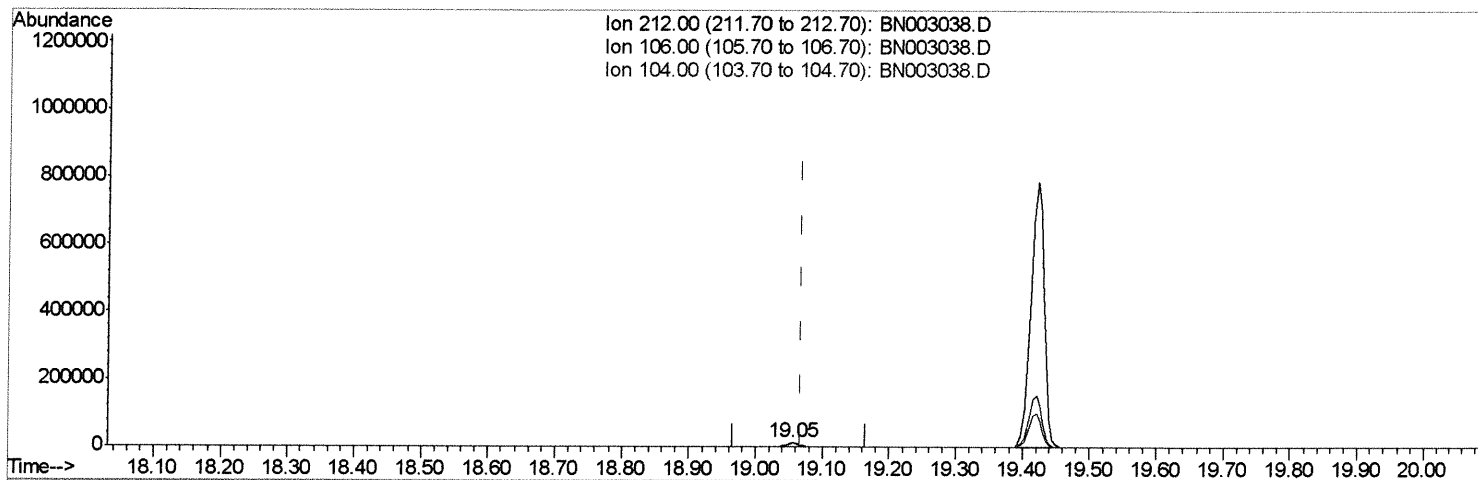

TIC: BN003038.D

(14) Fluoranthene-d10 (SURR)

19.053min (-0.014) 0.58ng/ul m

SJ 10/12/18

response 15795

Ion	Exp%	Act%
212.00	100	100
106.00	15.40	0.00#
104.00	8.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003038.D
Acq On : 09 Oct 2018 21:51
Operator : MJ/SJ
Sample : J5157-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD0

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:49 PM

Quant Time: Oct 10 02:05:44 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

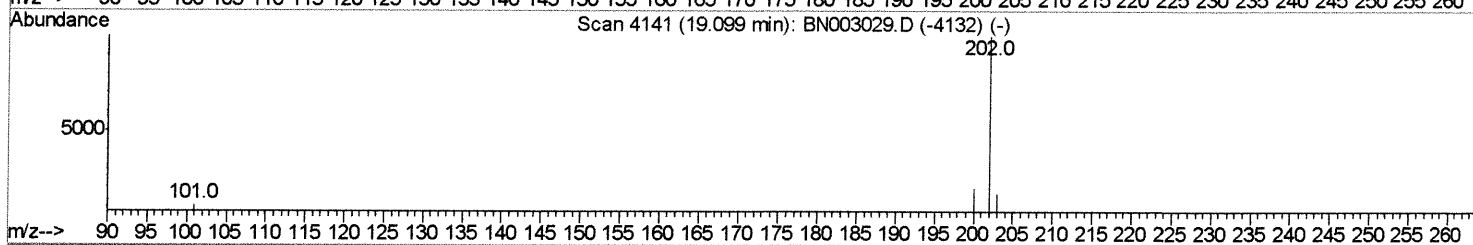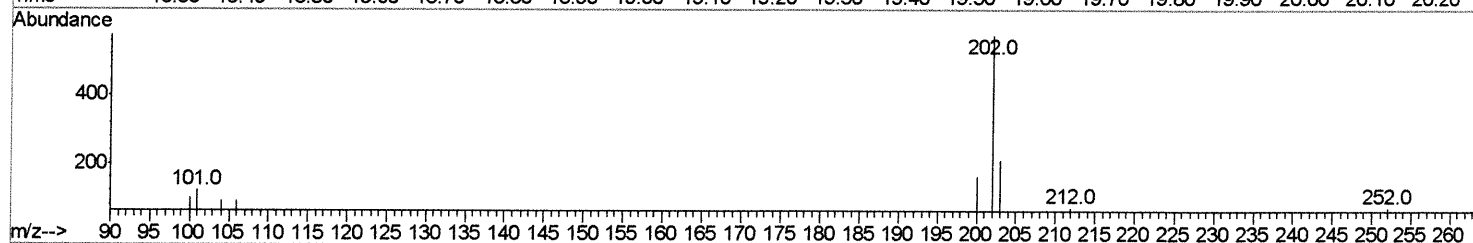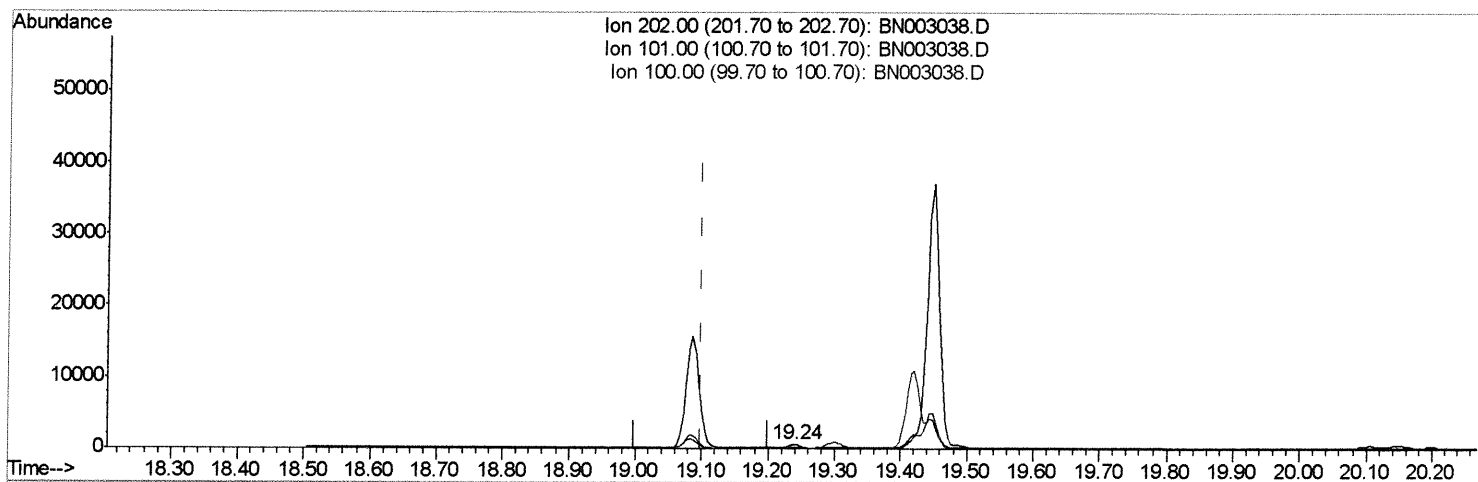

TIC: BN003038.D

(15) Fluoranthene (C)

19.239min (+0.140) 0.02ng/ul

response 599

Ion	Exp%	Act%
202.00	100	100
101.00	12.30	20.97
100.00	9.10	17.50
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003038.D
 Acq On : 09 Oct 2018 21:51
 Operator : MJ/SJ
 Sample : J5157-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:49 PM

Quant Time: Oct 10 02:05:44 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

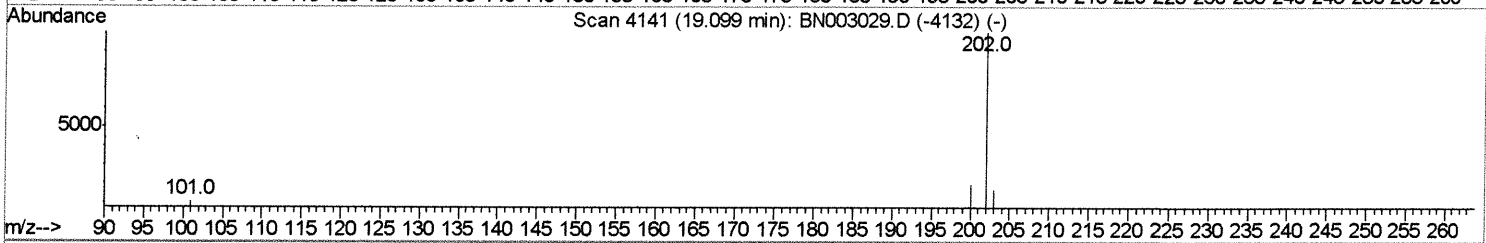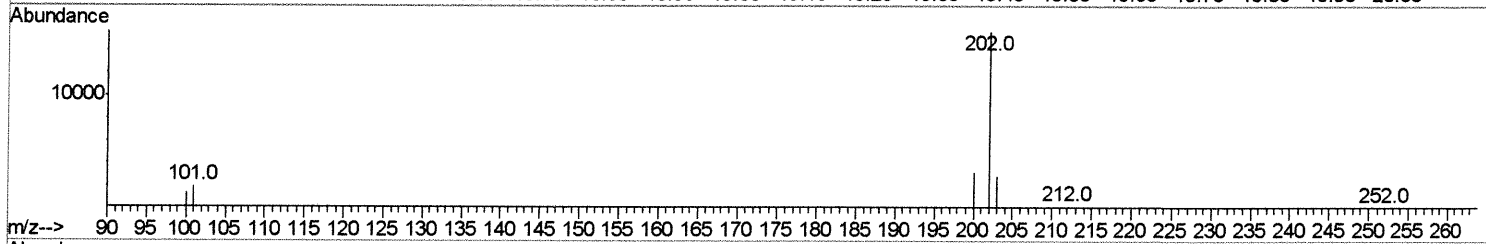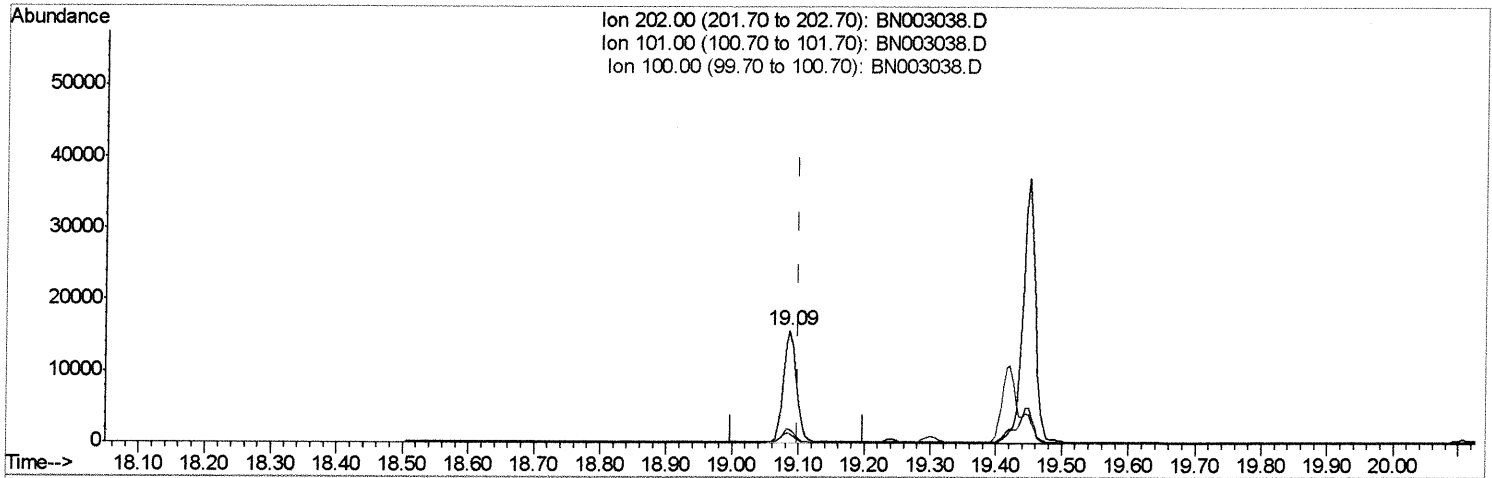

TIC: BN003038.D

(15) Fluoranthene (C)

19.086min (-0.014) 0.70ng/ul m *SJ 10/12/18*

response 21756

Ion	Exp%	Act%
202.00	100	100
101.00	12.30	12.05
100.00	9.10	8.91
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003038.D
 Acq On : 09 Oct 2018 21:51
 Operator : MJ/SJ
 Sample : J5157-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:49 PM

Quant Time: Oct 10 02:05:44 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

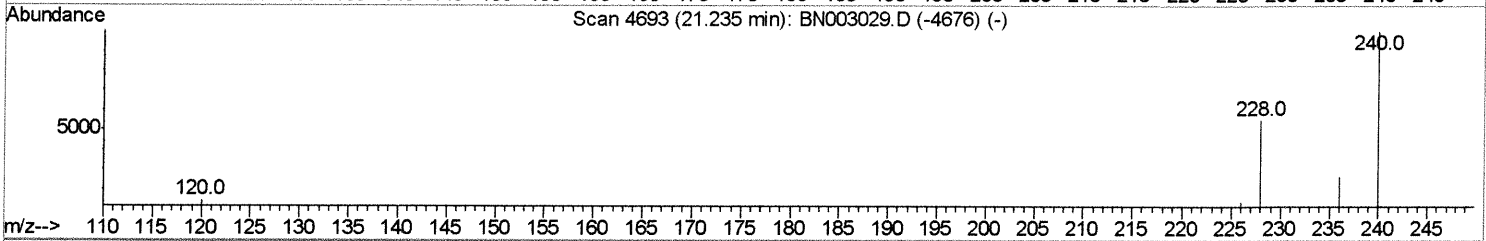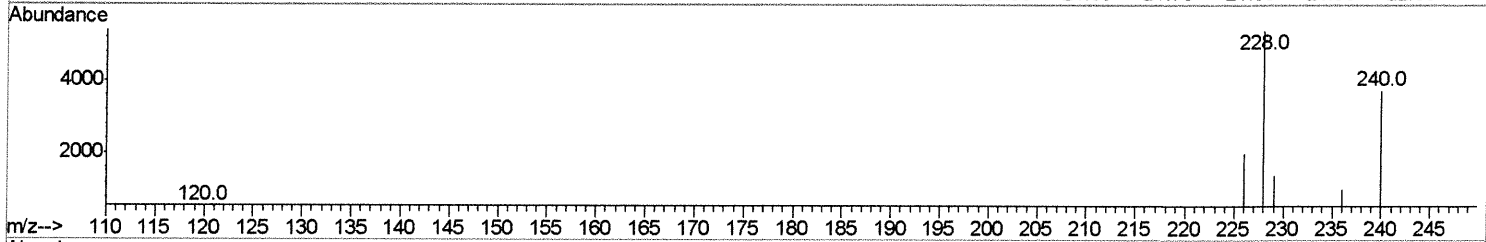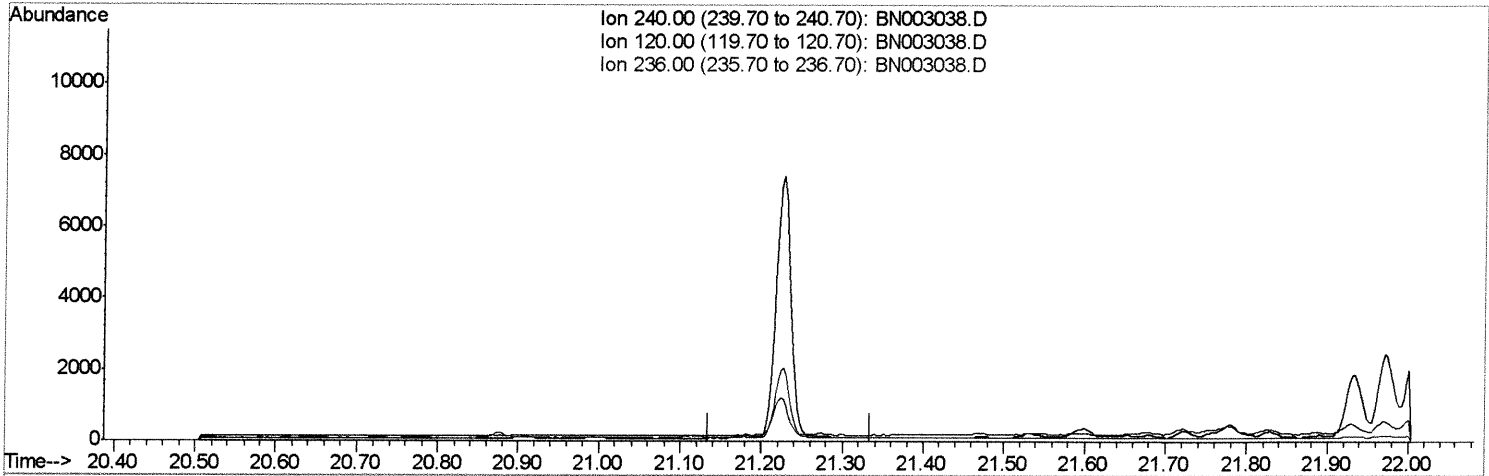

TIC: BN003038.D

(16) Chrysene-d12 (I)

21.235min (-21.235) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	16.40	0.00#
236.00	28.10	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003038.D
 Acq On : 09 Oct 2018 21:51
 Operator : MJ/SJ
 Sample : J5157-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:49 PM

Quant Time: Oct 10 02:05:44 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

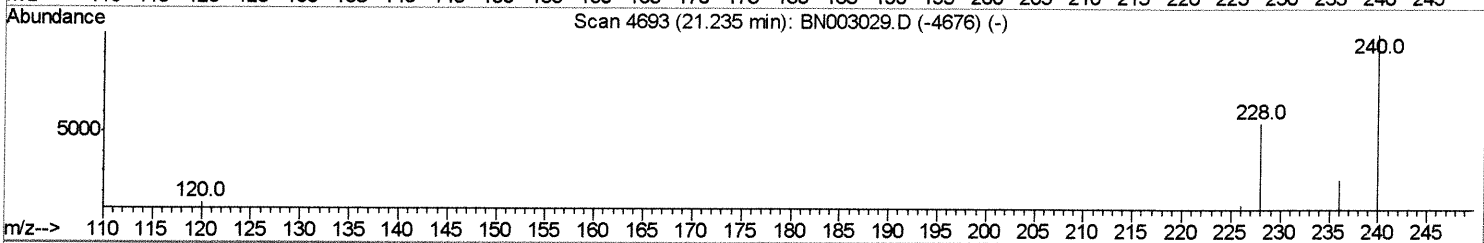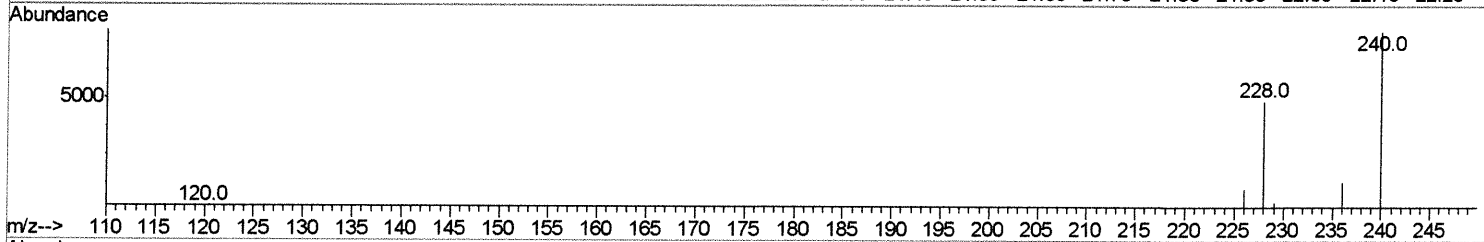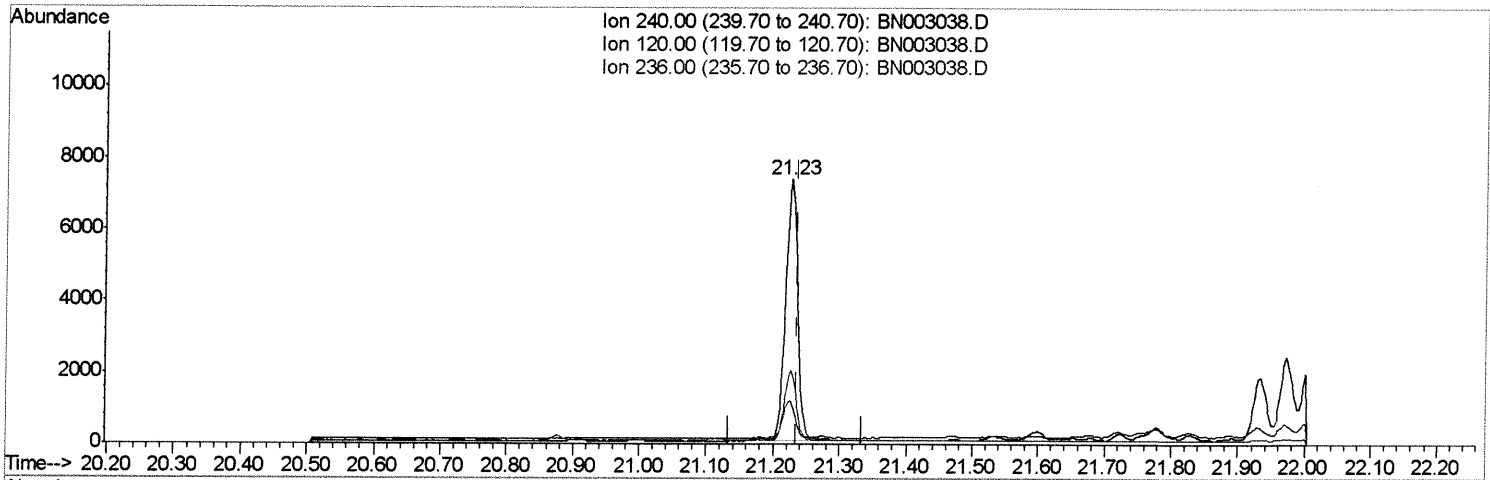

TIC: BN003038.D

(16) Chrysene-d12 (I)

21.226min (-0.009) 0.40ng/ul m *SJ 10/12/18*

response 9112

Ion	Exp%	Act%
240.00	100	100
120.00	16.40	15.74
236.00	28.10	27.74
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003038.D
Acq On : 09 Oct 2018 21:51
Operator : MJ/SJ
Sample : J5157-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD0

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:49 PM

Quant Time: Oct 10 02:07:00 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

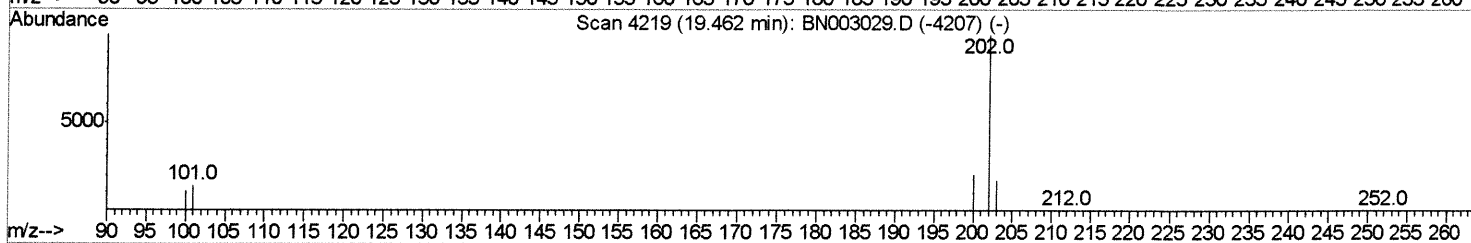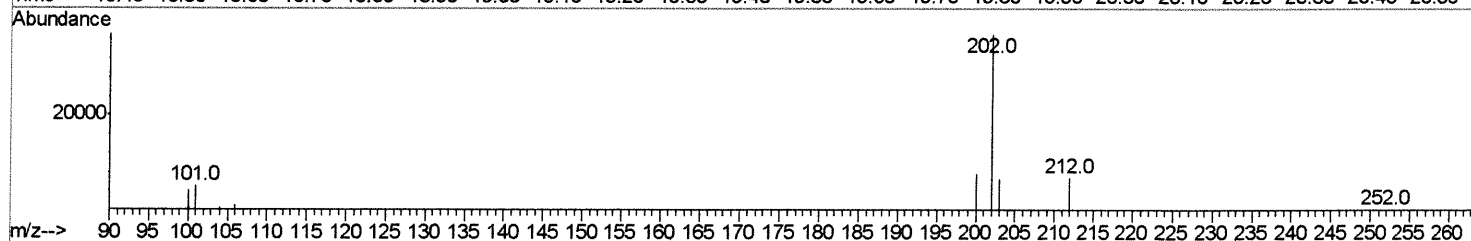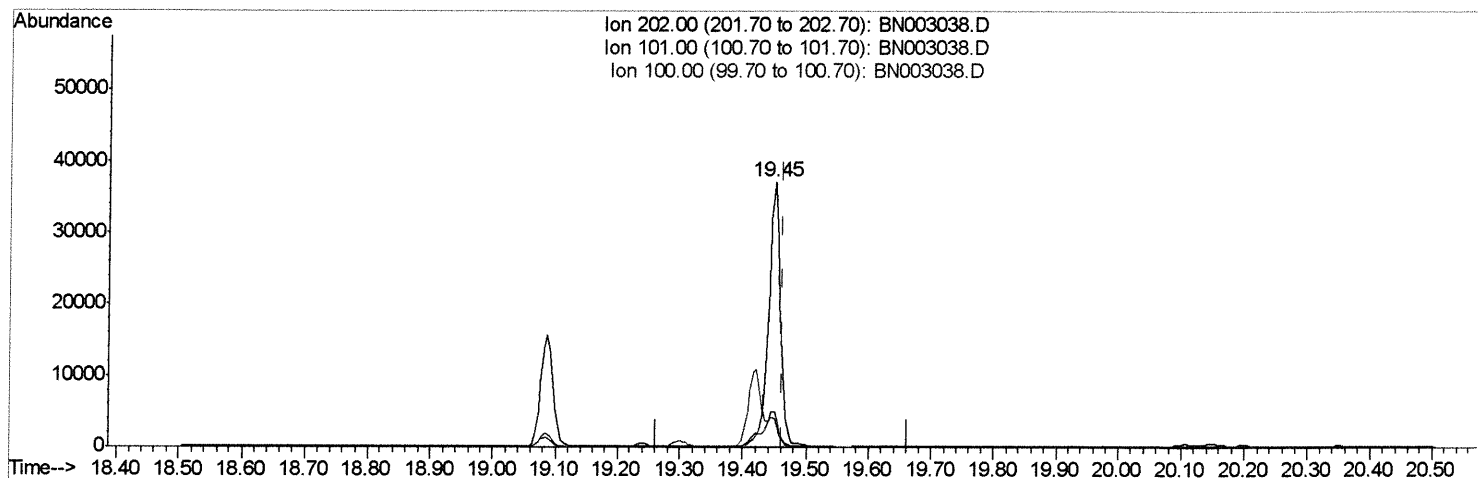

TIC: BN003038.D

(17) Pyrene

19.448min (-0.014) 1.40ng/ul

response 49380

Ion	Exp%	Act%
202.00	100	100
101.00	14.90	13.53
100.00	12.40	10.89
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003038.D
 Acq On : 09 Oct 2018 21:51
 Operator : MJ/SJ
 Sample : J5157-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:49 PM

Quant Time: Oct 10 02:07:00 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

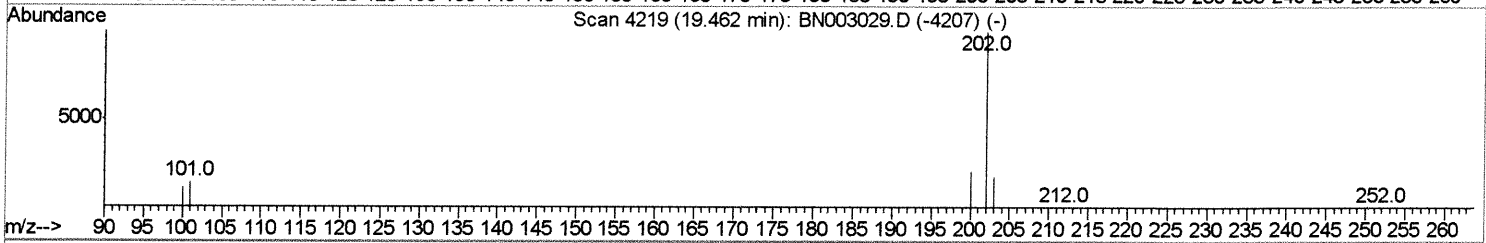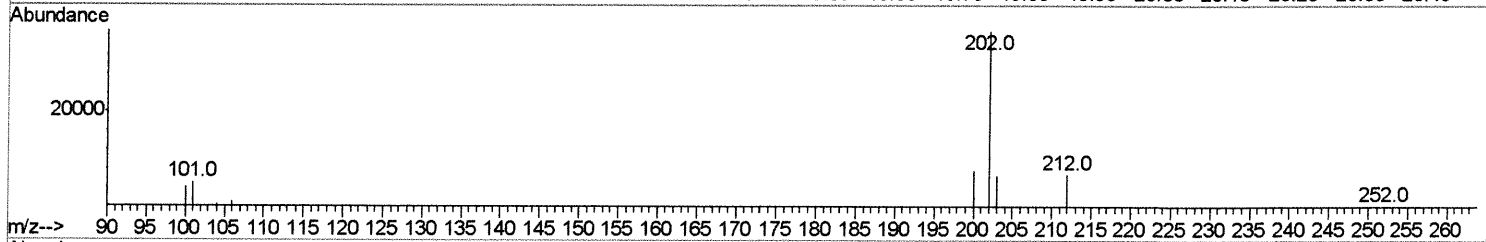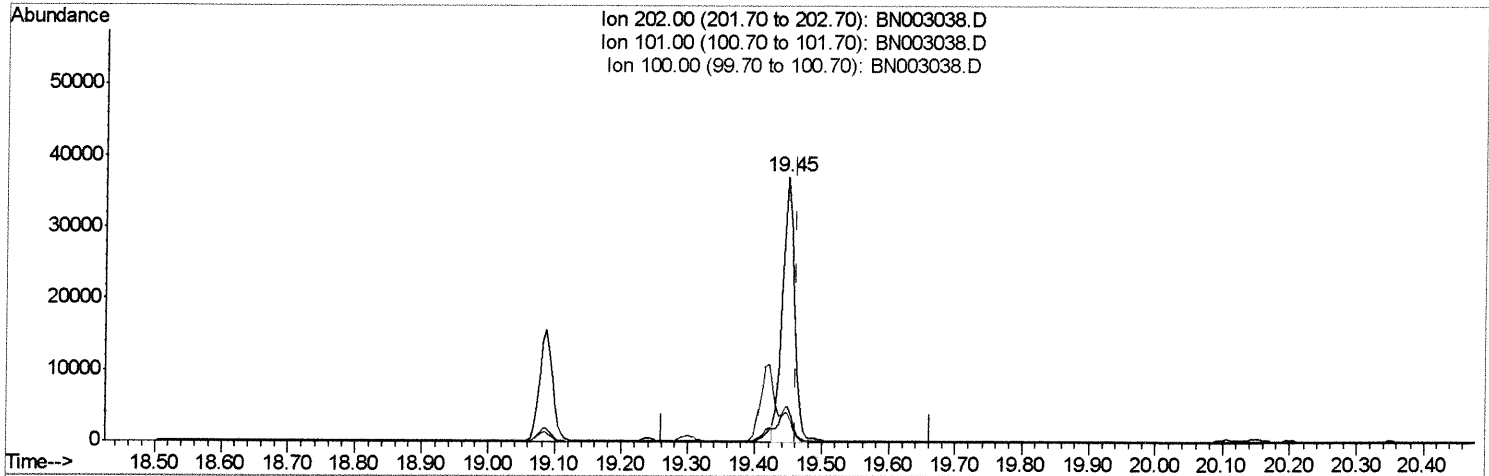

TIC: BN003038.D

(17) Pyrene

19.448min (-0.014) 1.34ng/ul m

5J10/12/18

response 47300

Ion	Exp%	Act%
202.00	100	100
101.00	14.90	13.53
100.00	12.40	10.89
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003038.D
 Acq On : 09 Oct 2018 21:51
 Operator : MJ/SJ
 Sample : J5157-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:49 PM

Quant Time: Oct 10 02:07:00 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

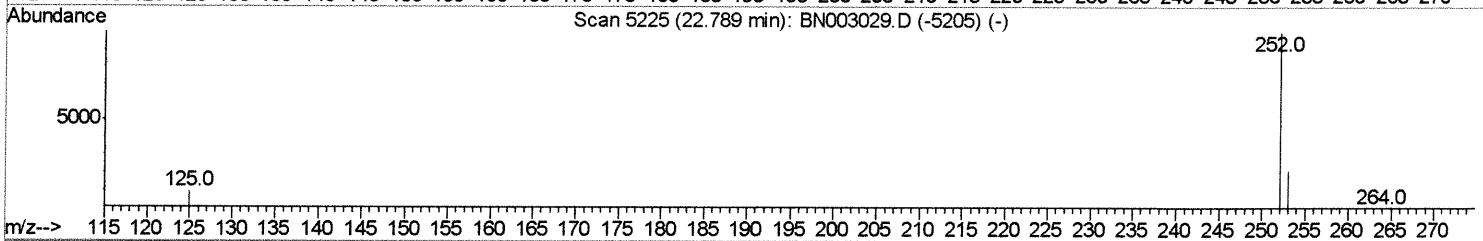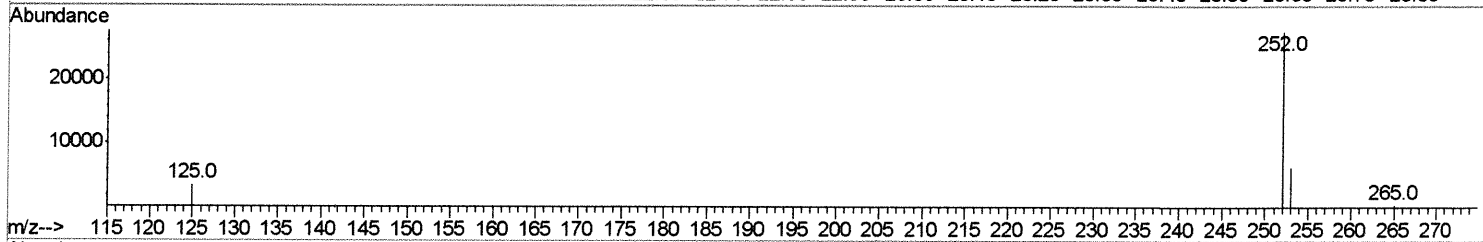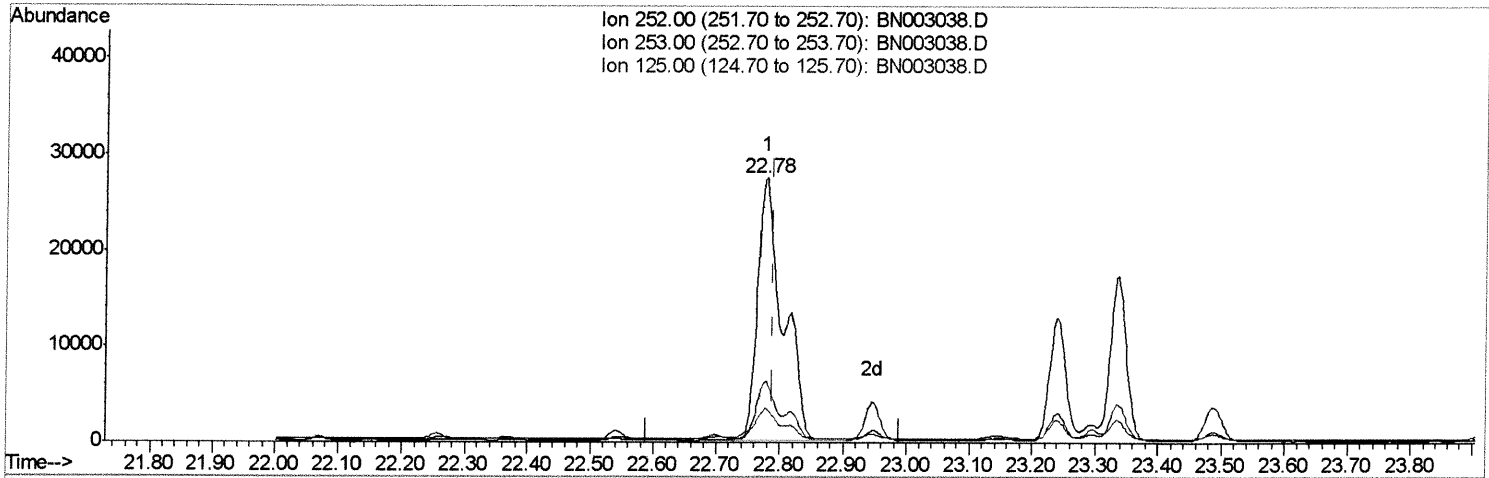

TIC: BN003038.D

(21) Benzo(b)fluoranthene
 22.778min (-0.012) 2.55ng/ul
 response 76210

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	23.20
125.00	17.10	12.72
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003038.D
 Acq On : 09 Oct 2018 21:51
 Operator : MJ/SJ
 Sample : J5157-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:49 PM

Quant Time: Oct 10 02:07:00 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

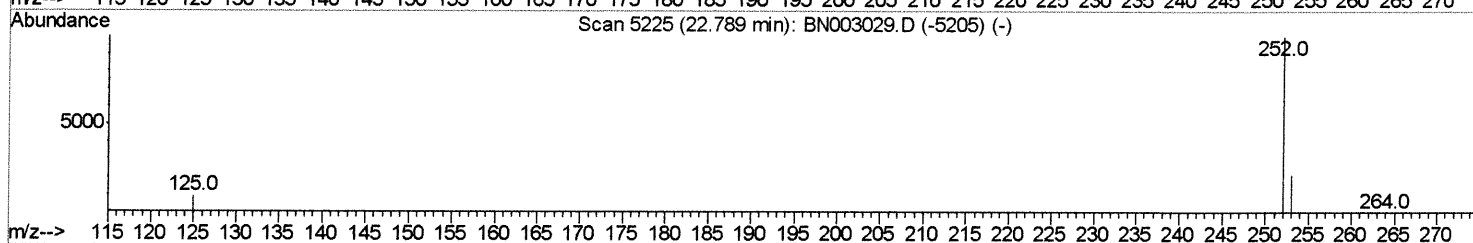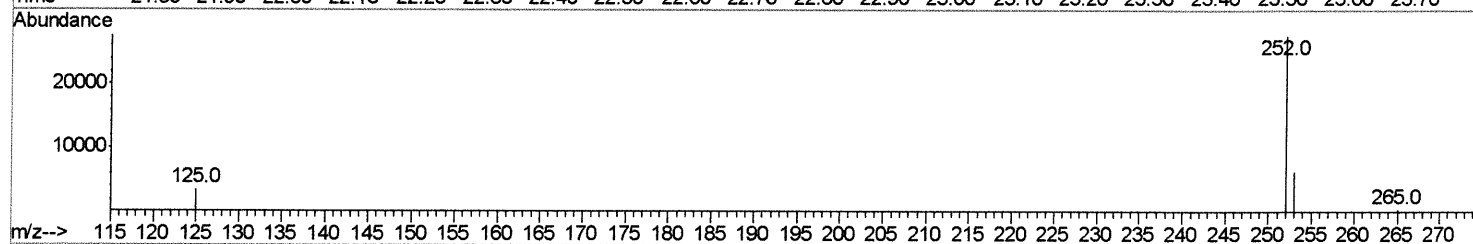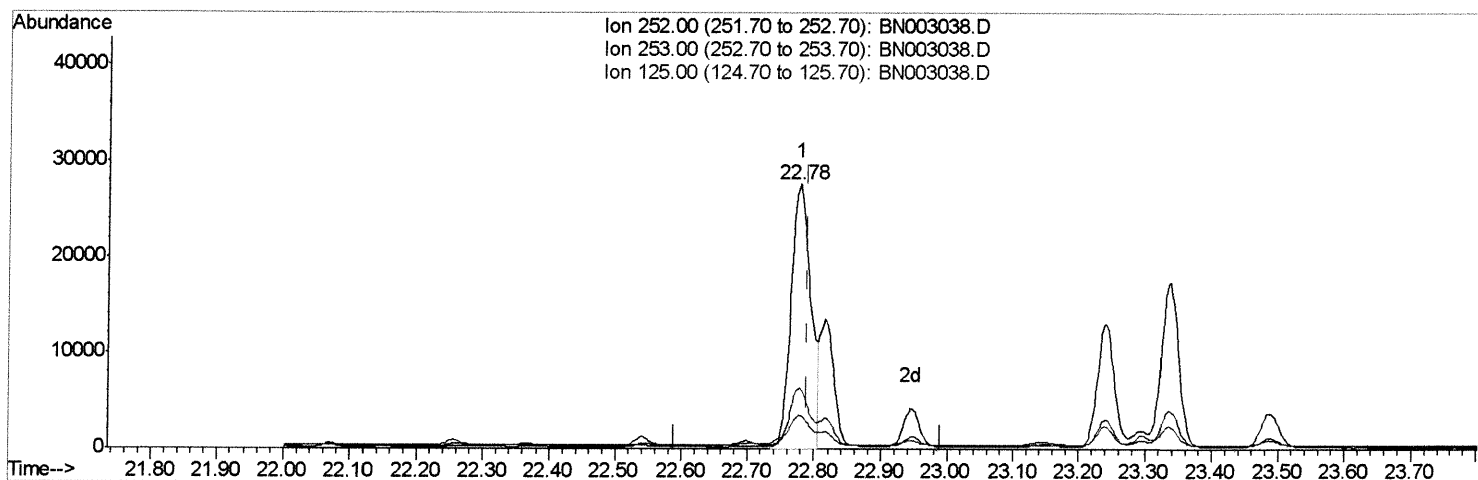

TIC: BN003038.D

(21) Benzo(b)fluoranthene

22.778min (-0.012) 1.90ng/ul m

SJ 10/12/18

response 56937

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	23.20
125.00	17.10	12.72
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003038.D
 Acq On : 09 Oct 2018 21:51
 Operator : MJ/SJ
 Sample : J5157-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:49 PM

Quant Time: Oct 10 02:07:00 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

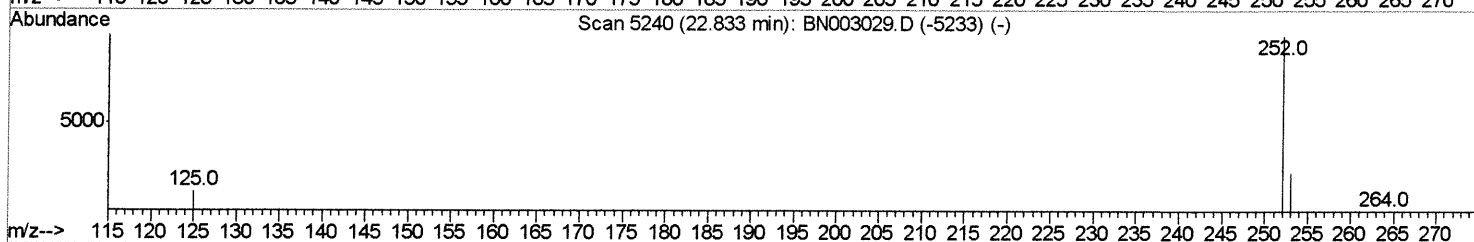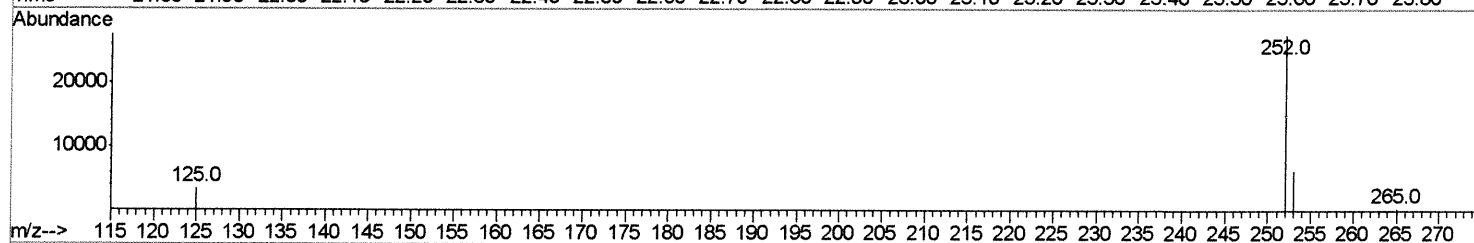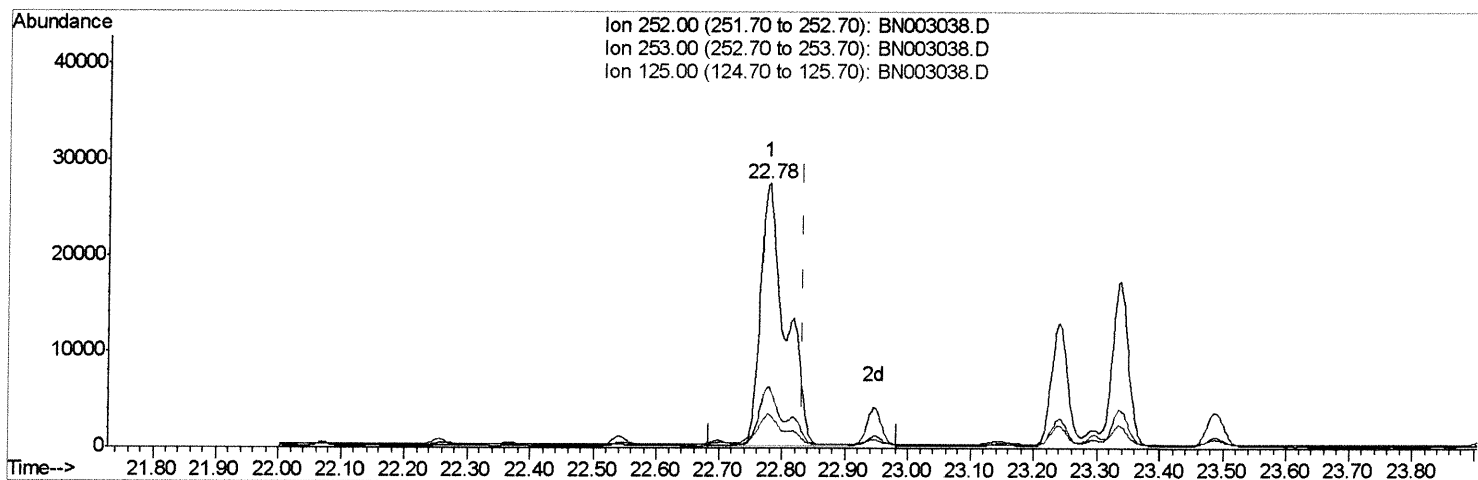

TIC: BN003038.D

(22) Benzo(k)fluoranthene
 22.778min (-0.055) 2.46ng/ui
 response 76210

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	23.20
125.00	17.60	12.72#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003038.D
Acq On : 09 Oct 2018 21:51
Operator : MJ/SJ
Sample : J5157-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD0

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:49 PM

Quant Time: Oct 10 02:07:00 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

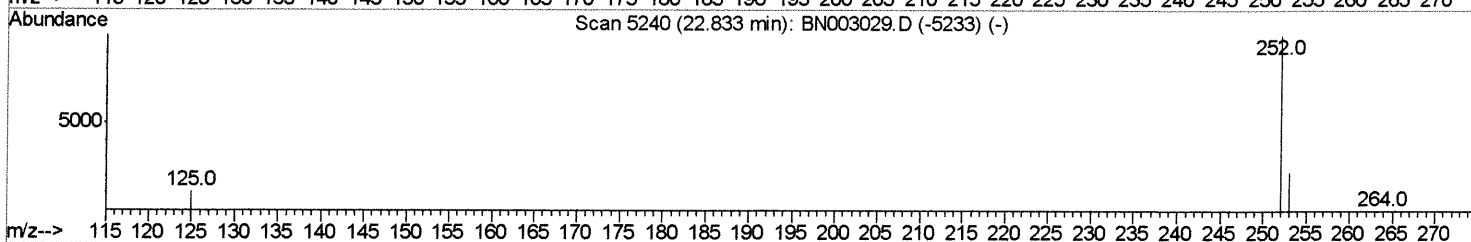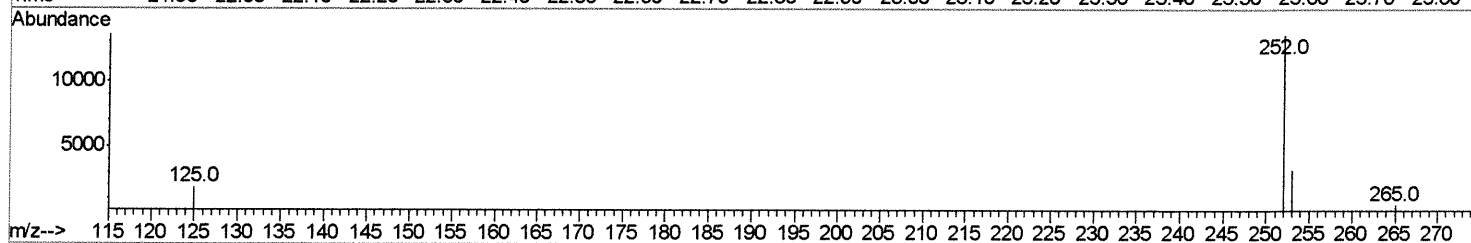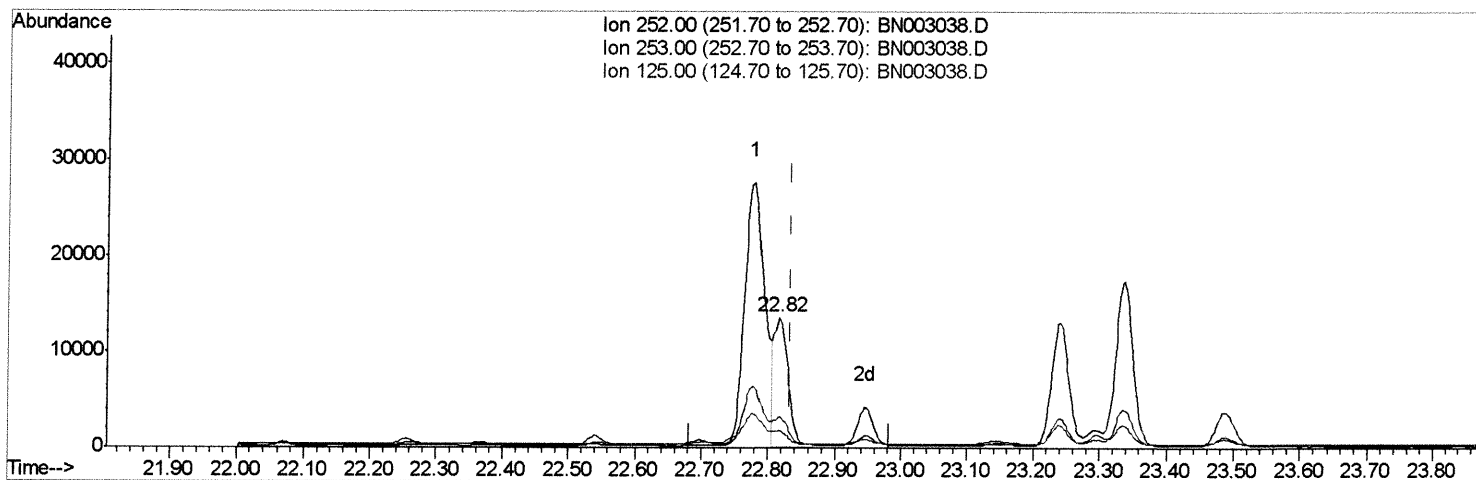

TIC: BN003038.D

(22) Benzo(k)fluoranthene

22.816min (-0.017) 0.65ng/ul m

SJ 10/14/18

response 20053

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	23.66
125.00	17.60	13.50#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003038.D
 Acq On : 09 Oct 2018 21:51
 Operator : MJ/SJ
 Sample : J5157-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD0

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:49 PM

Quant Time: Oct 10 02:08:25 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	1573	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.39	136	6606	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.26	164	4174	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.02	188	9447m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.23	240	9112m	0.40	ng/ul	0.00
20) Perylene-d12	23.44	264	8313	0.40	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.01	152	5556	0.54	ng/ul	-0.02
14) Fluoranthene-d10	19.05	212	15795m	0.58	ng/ul	-0.01

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
3) Naphthalene	10.44	128	1459	0.086	ng/ul#	91
5) 2-Methylnaphthalene	12.09	142	245	0.021	ng/ul	92
7) Acenaphthylene	13.98	152	3339	0.175	ng/ul	98
8) Acenaphthene	14.32	153	435	0.030	ng/ul#	94
9) Fluorene	15.32	166	603	0.036	ng/ul#	96
12) Phenanthrene	17.06	178	4995m	0.190	ng/ul	99
13) Anthracene	17.15	178	4961m	0.199	ng/ul	
15) Fluoranthene	19.09	202	21756m	0.704	ng/ul	
17) Pyrene	19.45	202	47300m	1.337	ng/ul	100
18) Benzo(a)anthracene	21.21	228	25327	0.864	ng/ul	
19) Chrysene	21.26	228	27718	0.931	ng/ul	88
21) Benzo(b)fluoranthene	22.78	252	56937m	1.902	ng/ul	
22) Benzo(k)fluoranthene	22.82	252	20053m	0.646	ng/ul	93
23) Benzo(a)pyrene	23.34	252	31161	1.161	ng/ul#	
24) Indeno(1,2,3-cd)pyrene	25.66	276	13764	0.446	ng/ul#	89
25) Dibenzo(a,h)anthracene	25.65	278	3716	0.151	ng/ul#	
26) Benzo(a,h,i)perylene	26.33	276	10665	0.410	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed