


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003039.D
Acq On : 09 Oct 2018 22:26
Operator : MJ/SJ
Sample : J5157-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD1

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:50 PM

Quant Time: Oct 10 02:12:33 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

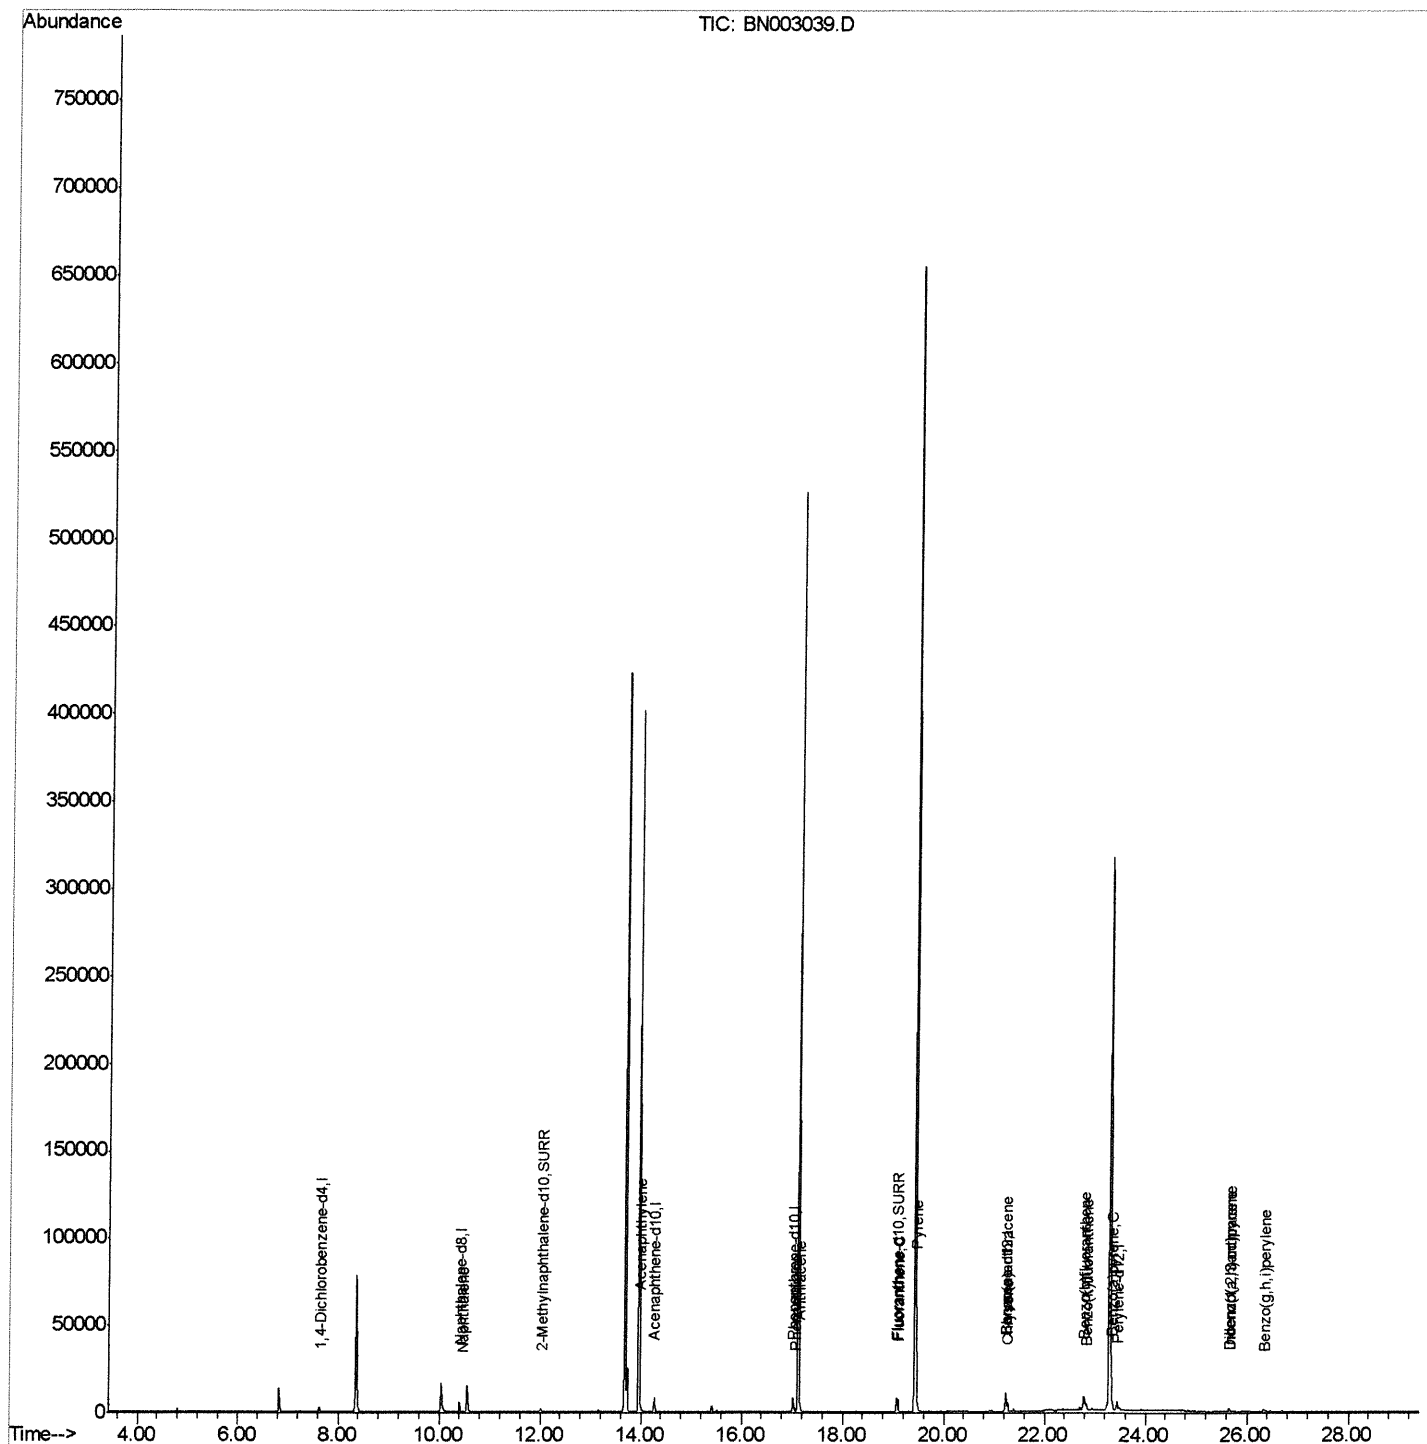

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003039.D
 Acq On : 09 Oct 2018 22:26
 Operator : MJ/SJ
 Sample : J5157-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD1

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:50 PM

Quant Time: Oct 10 01:38:12 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

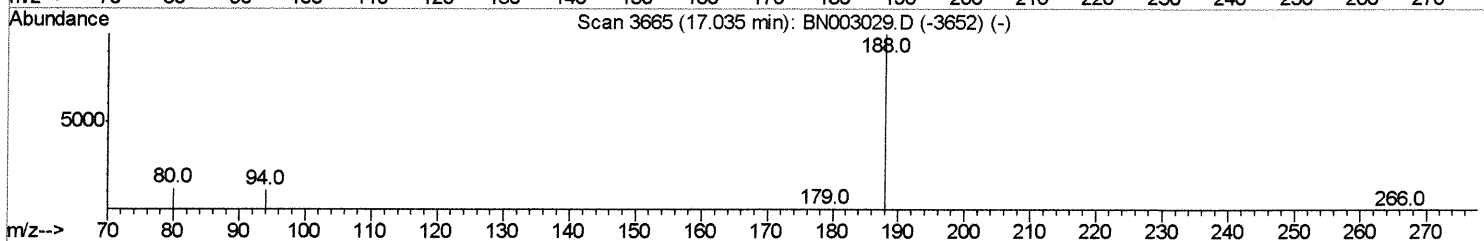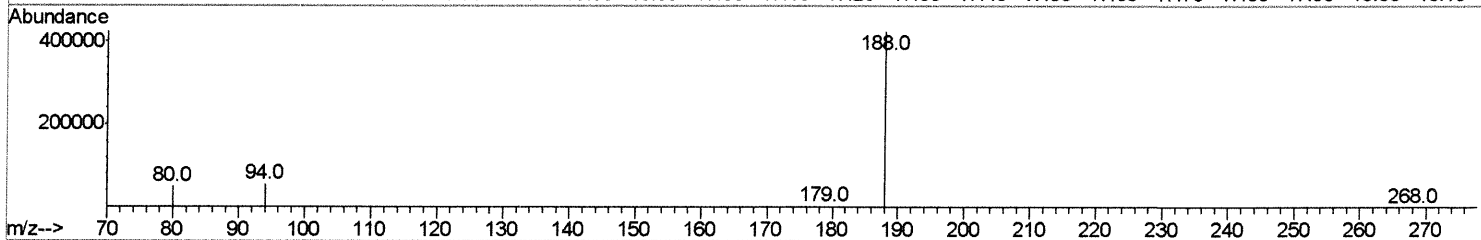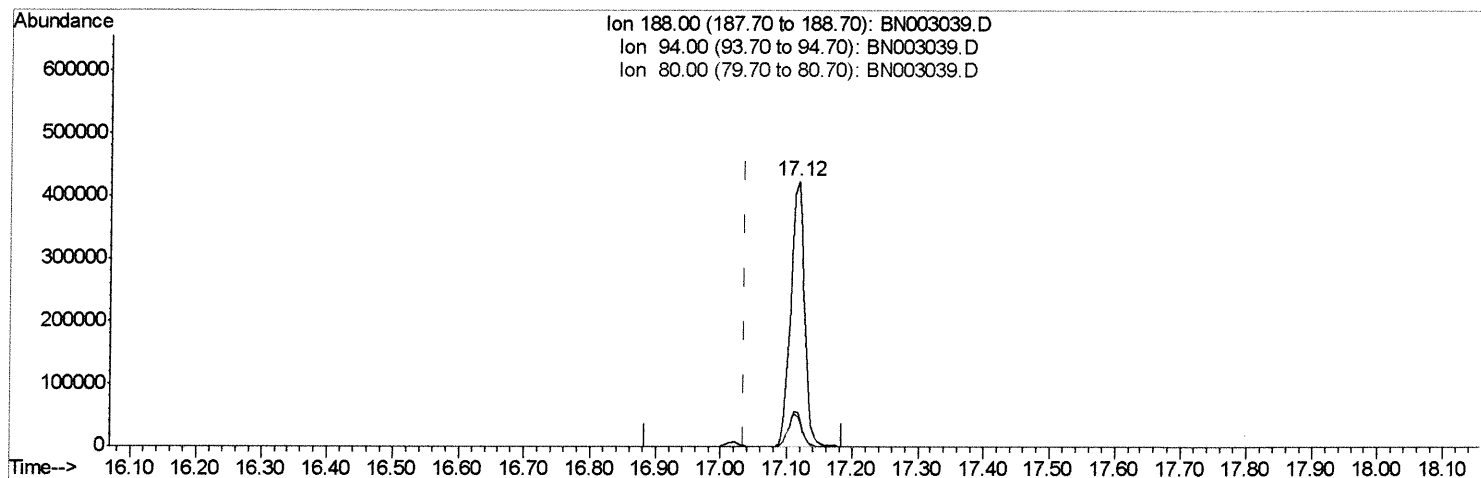

TIC: BN003039.D

(10) Phenanthrene-d10 (I)

17.116min (+0.080) 0.40ng/ul

response 610696

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	12.76
80.00	12.70	11.47
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003039.D
 Acq On : 09 Oct 2018 22:26
 Operator : MJ/SJ
 Sample : J5157-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD1

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:50 PM

Quant Time: Oct 10 01:38:12 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

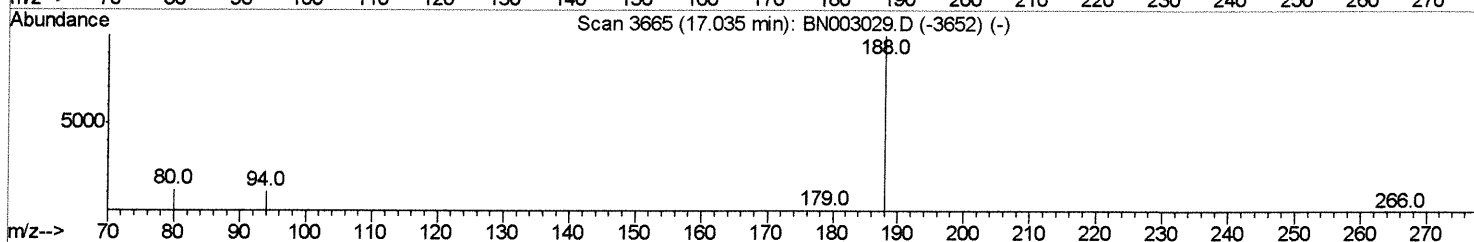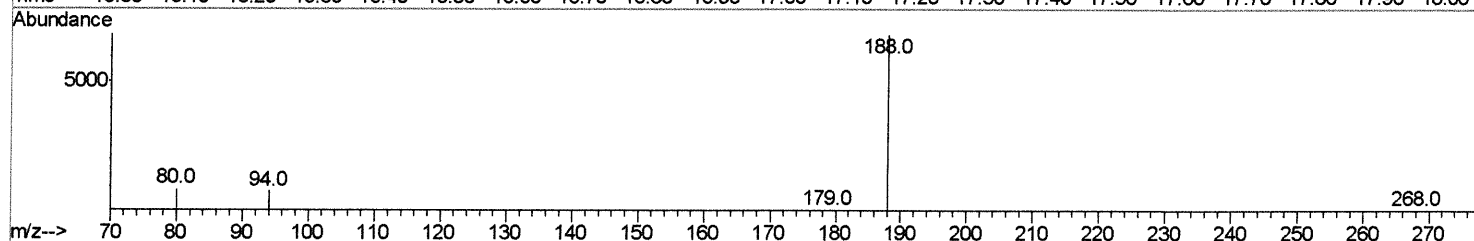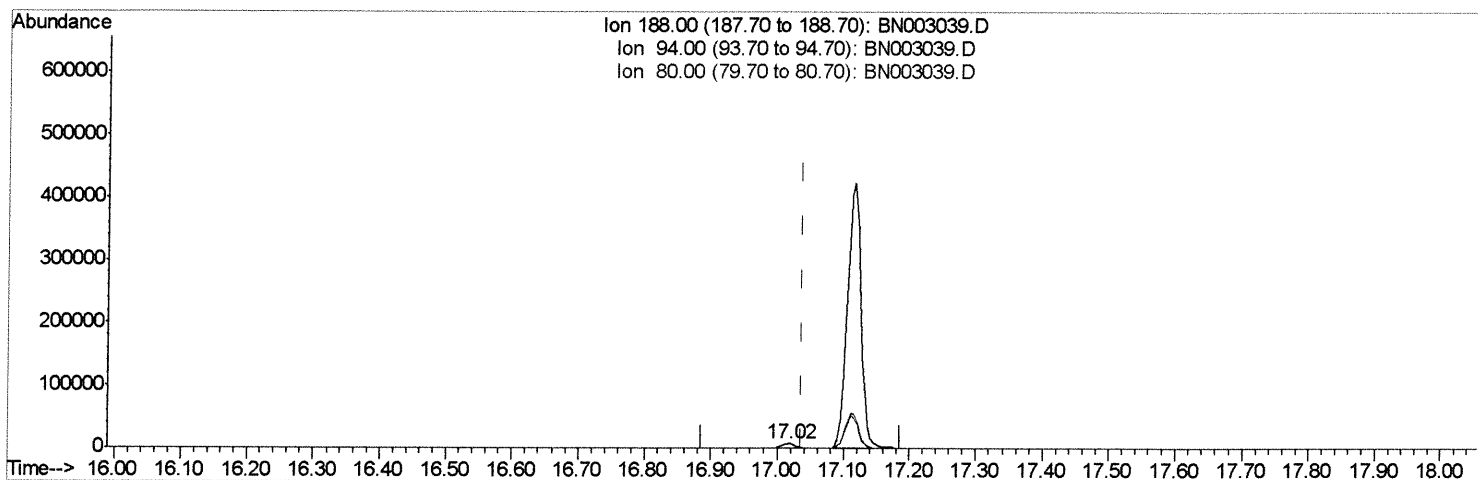

TIC: BN003039.D

(10) Phenanthrene-d10 (I)

17.019min (-0.017) 0.40ng/ul m

SJ 10/12/18

response 10123

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	11.43
80.00	12.70	12.49
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003039.D
Acq On : 09 Oct 2018 22:26
Operator : MJ/SJ
Sample : J5157-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD1

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:50 PM

Quant Time: Oct 10 02:09:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

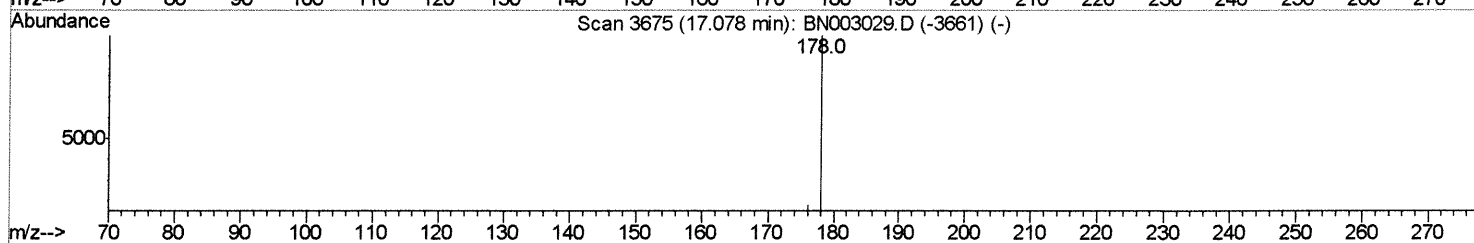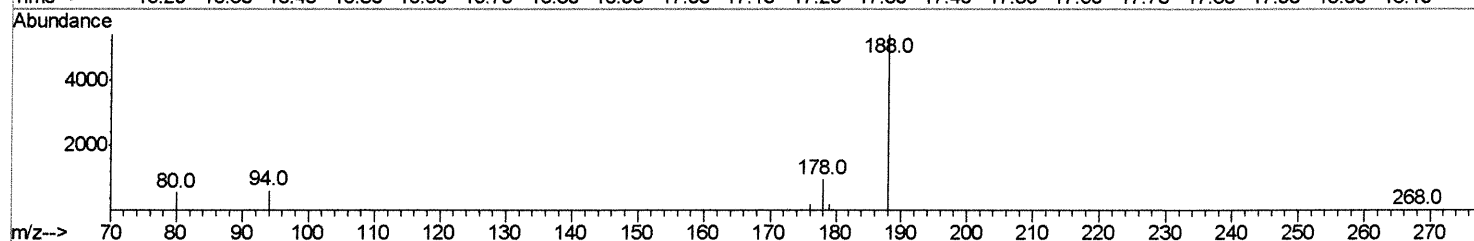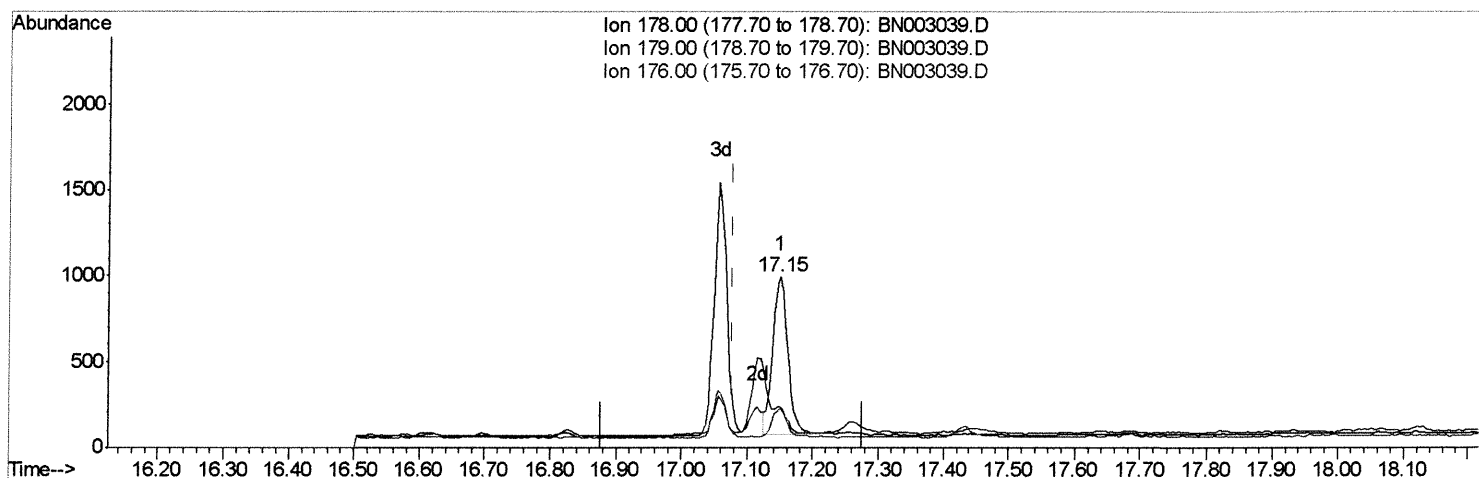

TIC: BN003039.D

(12) Phenanthrene

17.149min (+0.072) 0.05ng/ul

response 1481

Ion	Exp%	Act%
178.00	100	100
179.00	16.10	23.89#
176.00	19.30	23.49#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003039.D
 Acq On : 09 Oct 2018 22:26
 Operator : MJ/SJ
 Sample : J5157-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD1

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:50 PM

Quant Time: Oct 10 02:09:31 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

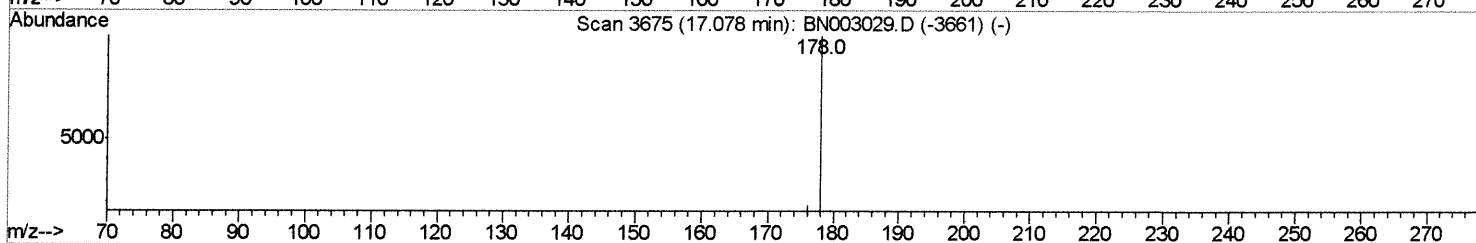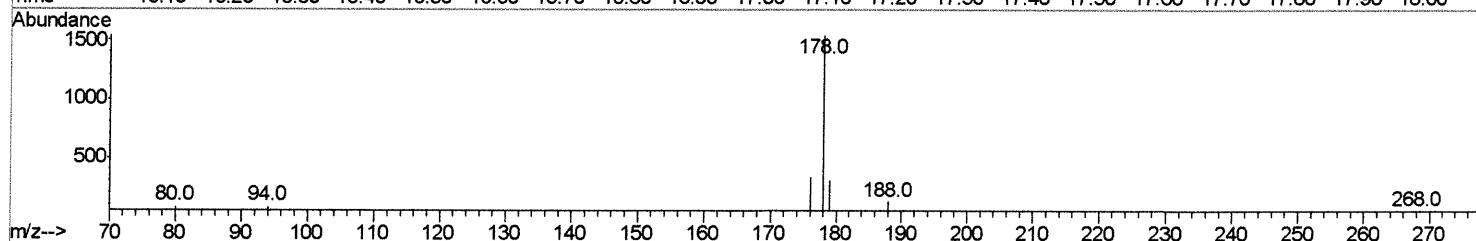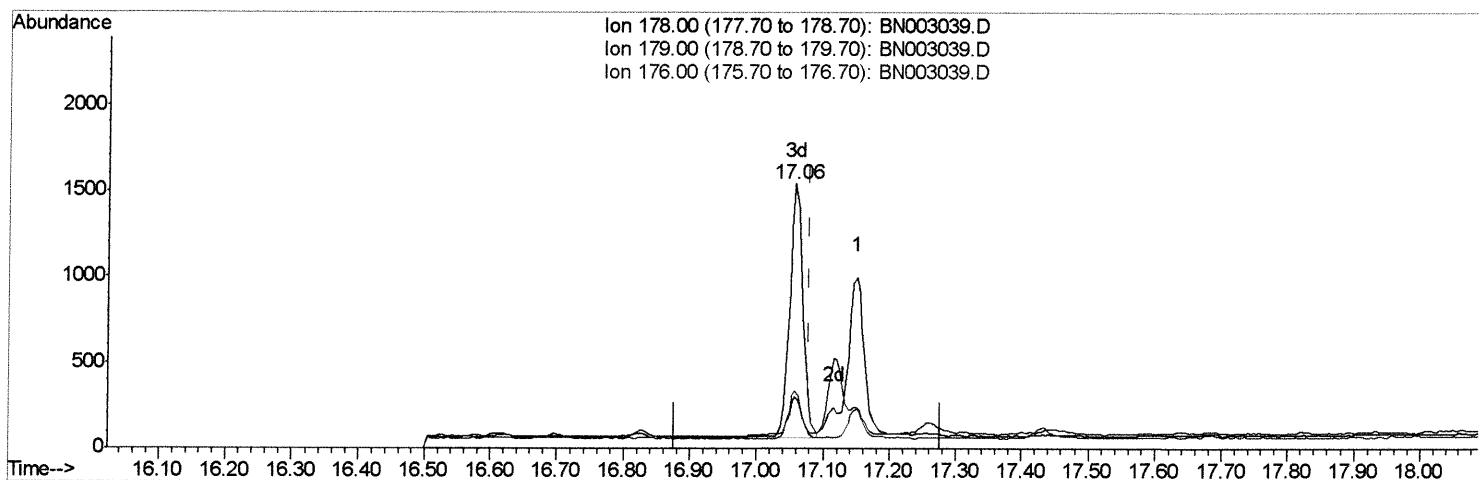

TIC: BN003039.D

(12) Phenanthrene

17.057min (-0.021) 0.07ng/ul m *SJ 10/12/18*

response 2039

Ion	Exp%	Act%
178.00	100	100
179.00	16.10	19.40#
176.00	19.30	21.87
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003039.D
Acq On : 09 Oct 2018 22:26
Operator : MJ/SJ
Sample : J5157-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD1

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:50 PM

Quant Time: Oct 10 02:09:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

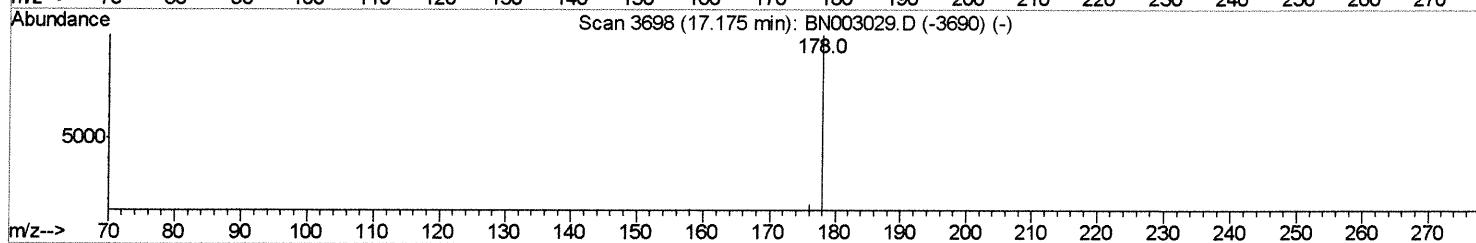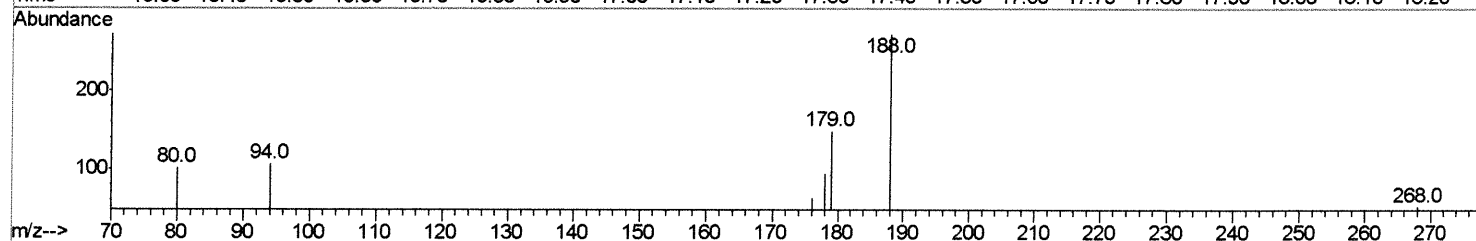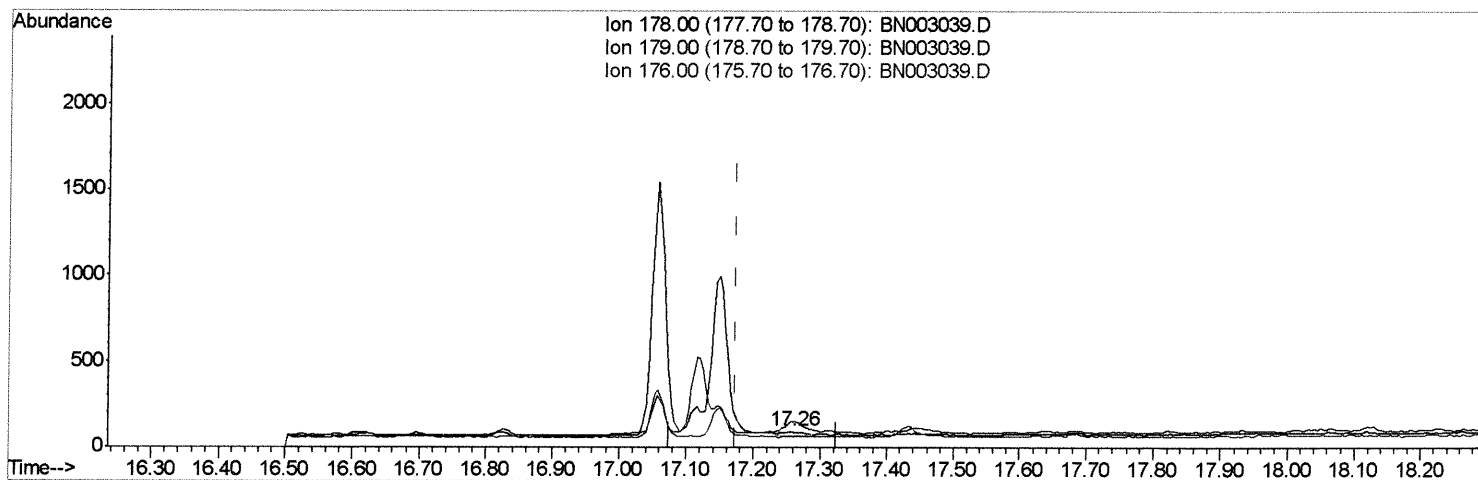

TIC: BN003039.D

(13) Anthracene

17.259min (+0.084) 0.00ng/ul

response 35

Ion	Exp%	Act%
178.00	100	100
179.00	16.30	157.45#
176.00	19.10	68.09#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003039.D
Acq On : 09 Oct 2018 22:26
Operator : MJ/SJ
Sample : J5157-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD1

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:50 PM

Quant Time: Oct 10 02:09:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

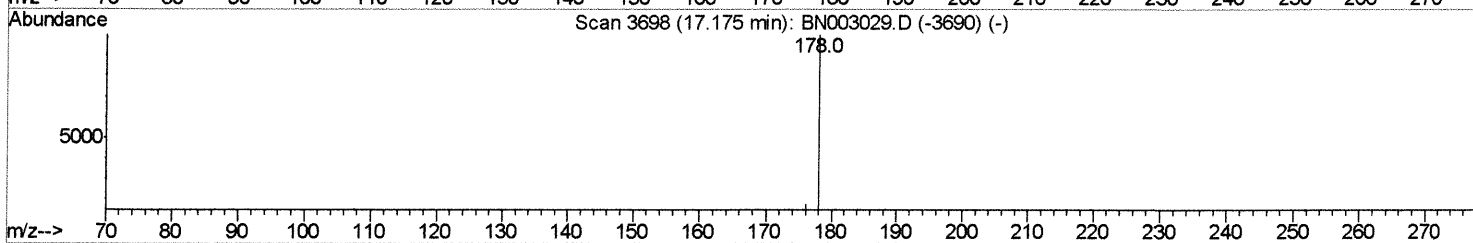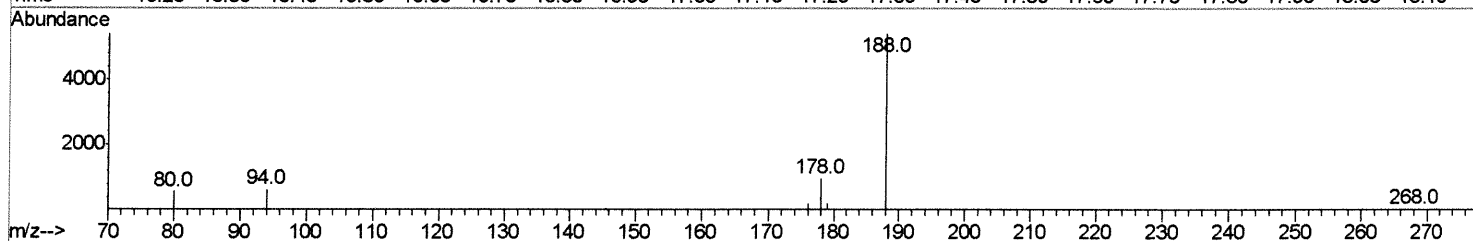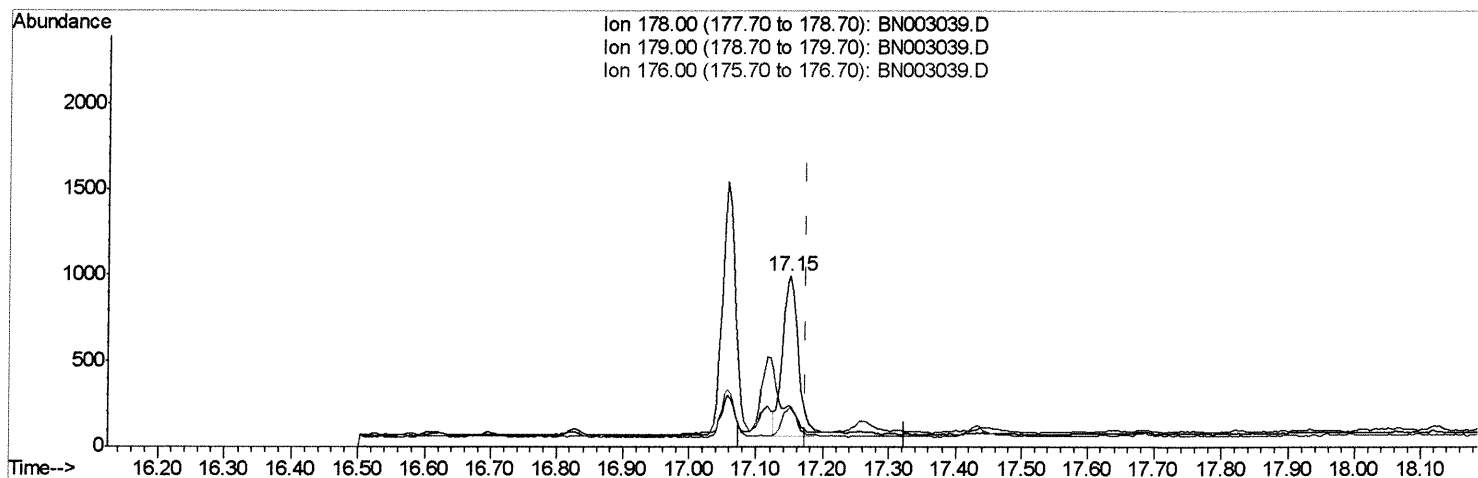

TIC: BN003039.D

(13) Anthracene

17.149min (-0.025) 0.06ng/ul m

SJ 10/12/18

response 1519

Ion	Exp%	Act%
178.00	100	100
179.00	16.30	23.89#
176.00	19.10	23.49#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003039.D
 Acq On : 09 Oct 2018 22:26
 Operator : MJ/SJ
 Sample : J5157-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD1

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:50 PM

Quant Time: Oct 10 02:09:31 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

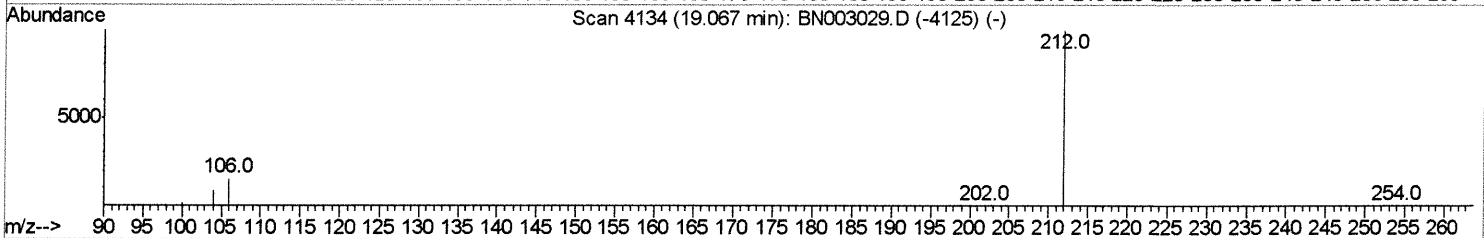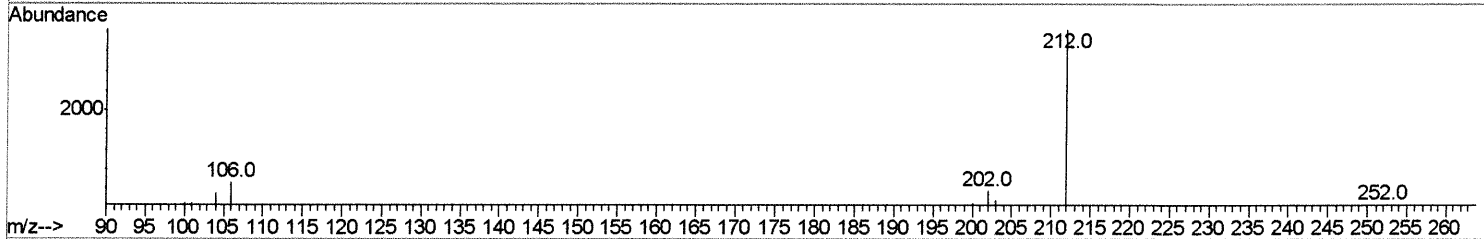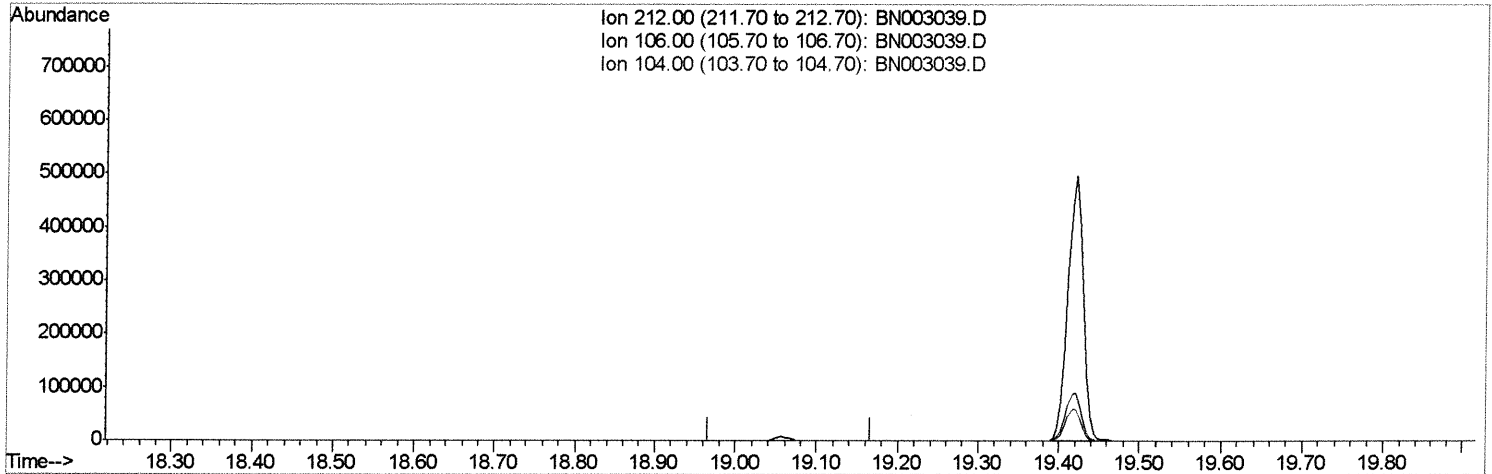

TIC: BN003039.D

(14) Fluoranthene-d10 (SURR)

19.067min (-19.067) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	15.40	0.00#
104.00	8.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003039.D
Acq On : 09 Oct 2018 22:26
Operator : MJ/SJ
Sample : J5157-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
C0AD1

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:50 PM

Quant Time: Oct 10 02:09:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

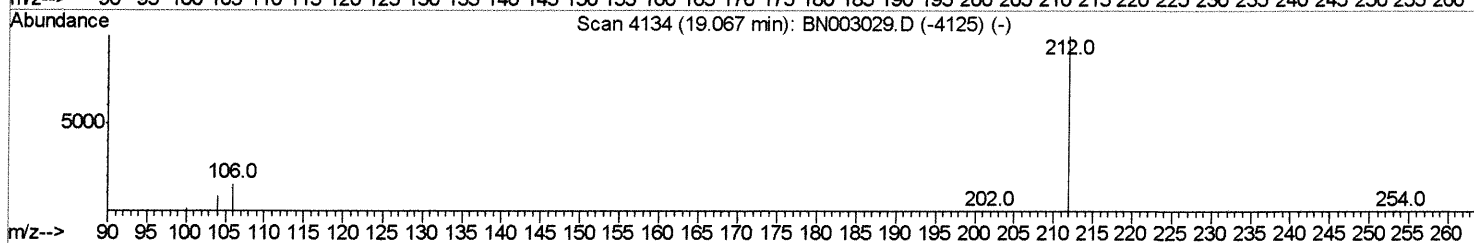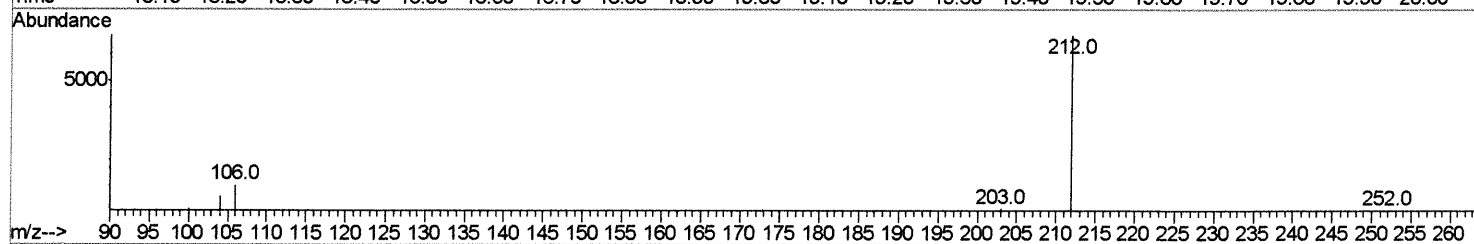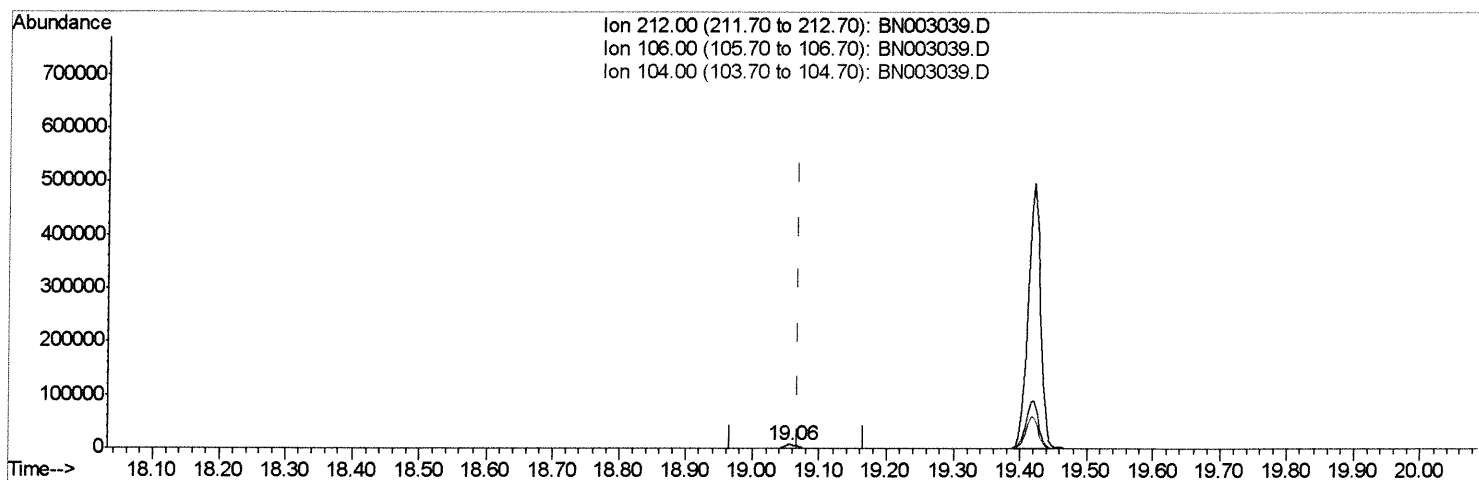

TIC: BN003039.D

(14) Fluoranthene-d10 (SURR)

19.058min (-0.009) 0.33ng/ul m

SJ 10/12/18

response 9496

Ion	Exp%	Act%
212.00	100	100
106.00	15.40	0.00#
104.00	8.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003039.D
 Acq On : 09 Oct 2018 22:26
 Operator : MJ/SJ
 Sample : J5157-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD1

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:50 PM

Quant Time: Oct 10 02:09:31 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

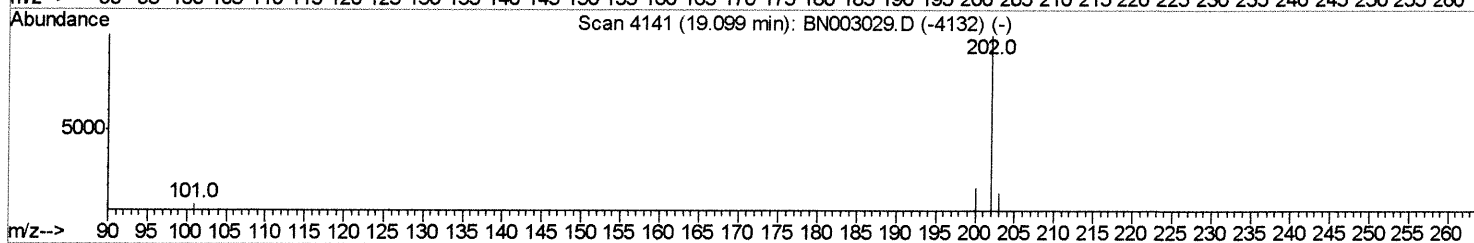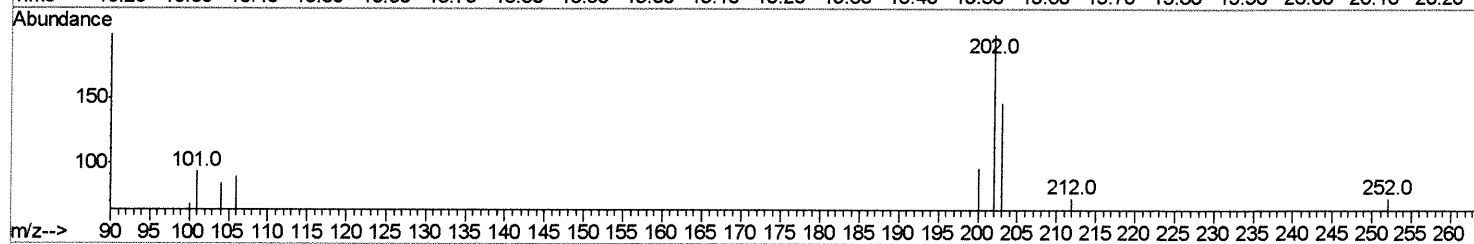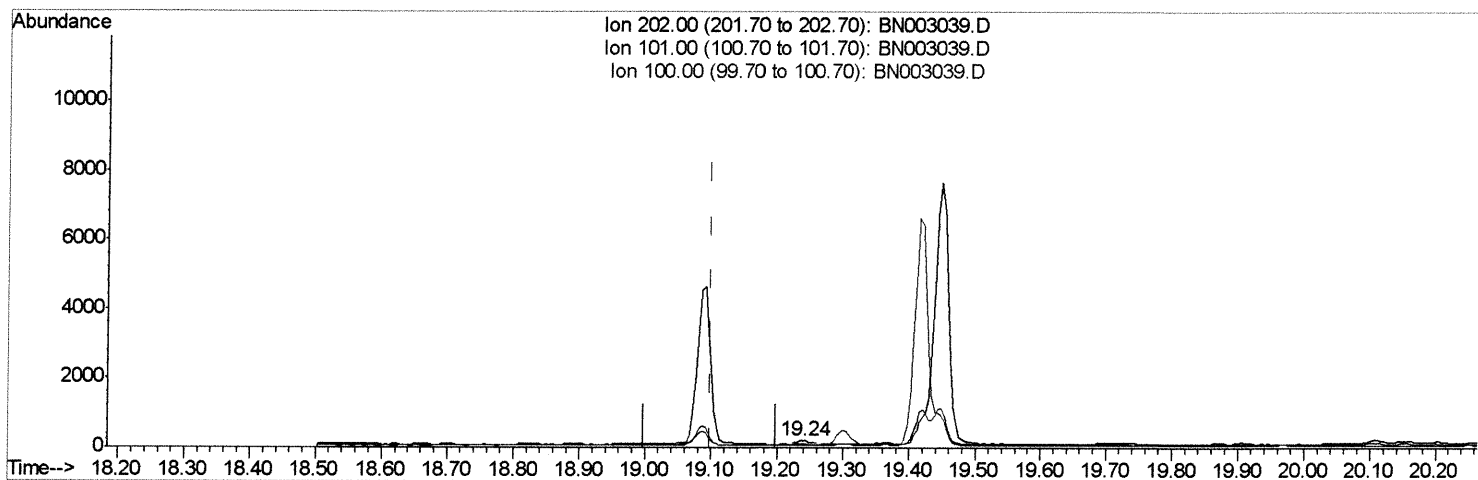

TIC: BN003039.D

(15) Fluoranthene (C)

19.239min (+0.139) 0.01ng/ul

response 170

Ion	Exp%	Act%
202.00	100	100
101.00	12.30	46.50#
100.00	9.10	34.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003039.D
 Acq On : 09 Oct 2018 22:26
 Operator : MJ/SJ
 Sample : J5157-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD1

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:50 PM

Quant Time: Oct 10 02:09:31 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

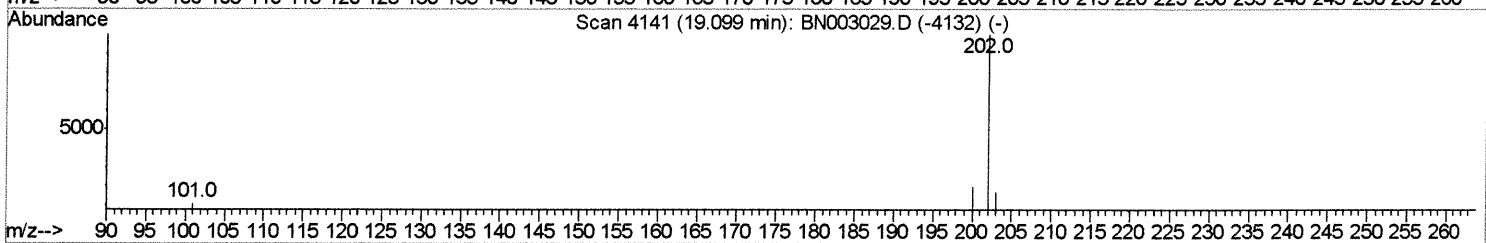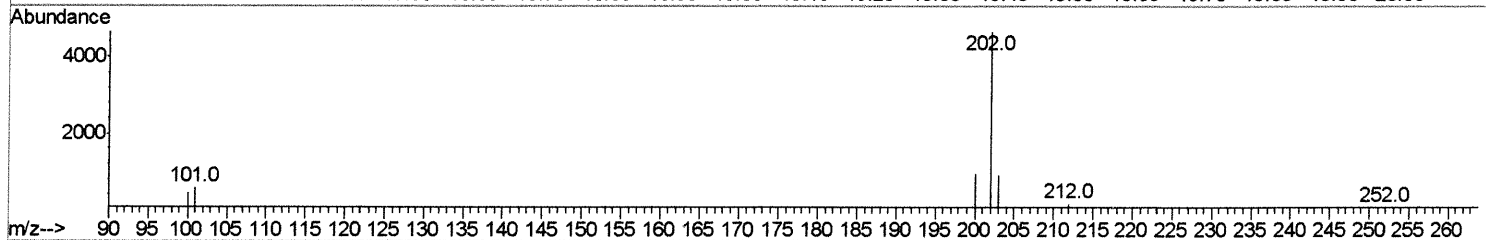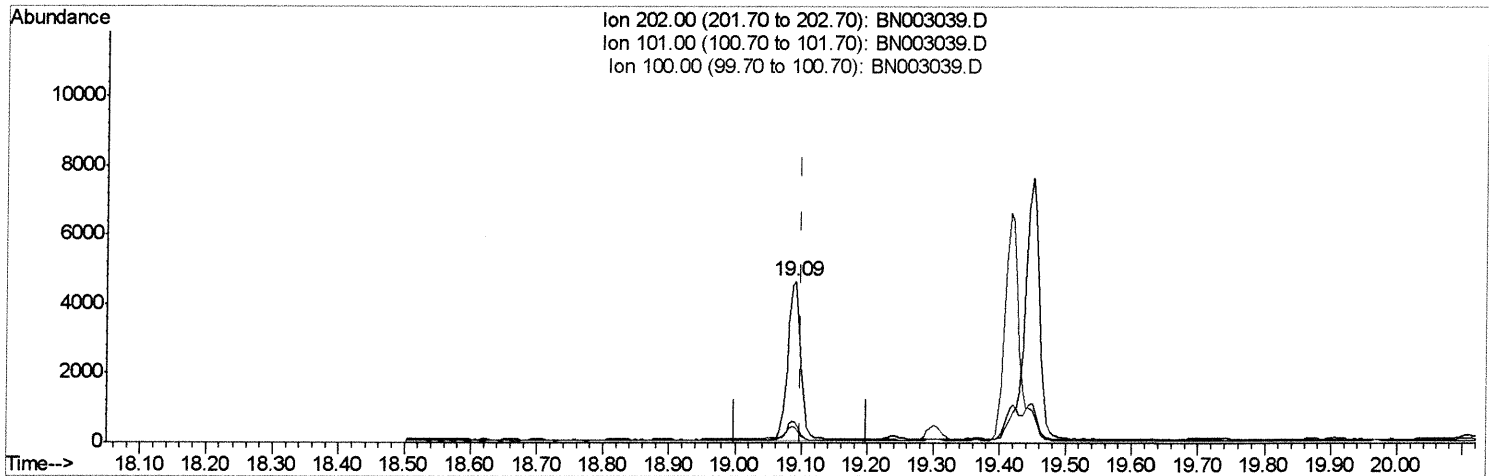

TIC: BN003039.D

(15) Fluoranthene (C)

19.090min (-0.009) 0.19ng/ul m

5/10/12/14

response 6323

Ion	Exp%	Act%
202.00	100	100
101.00	12.30	12.34
100.00	9.10	9.34
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003039.D
Acq On : 09 Oct 2018 22:26
Operator : MJ/SJ
Sample : J5157-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD1

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:50 PM

Quant Time: Oct 10 02:09:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

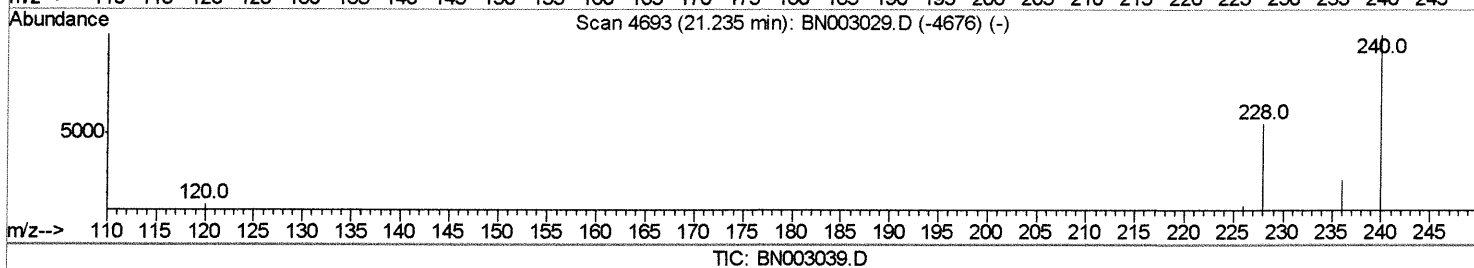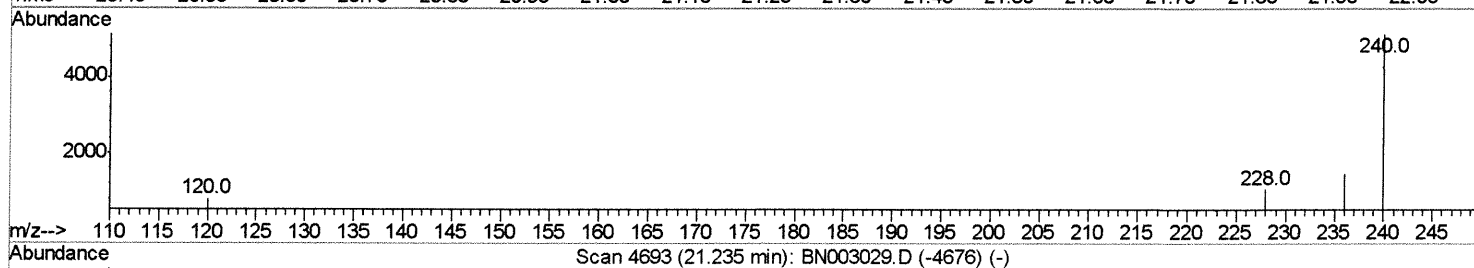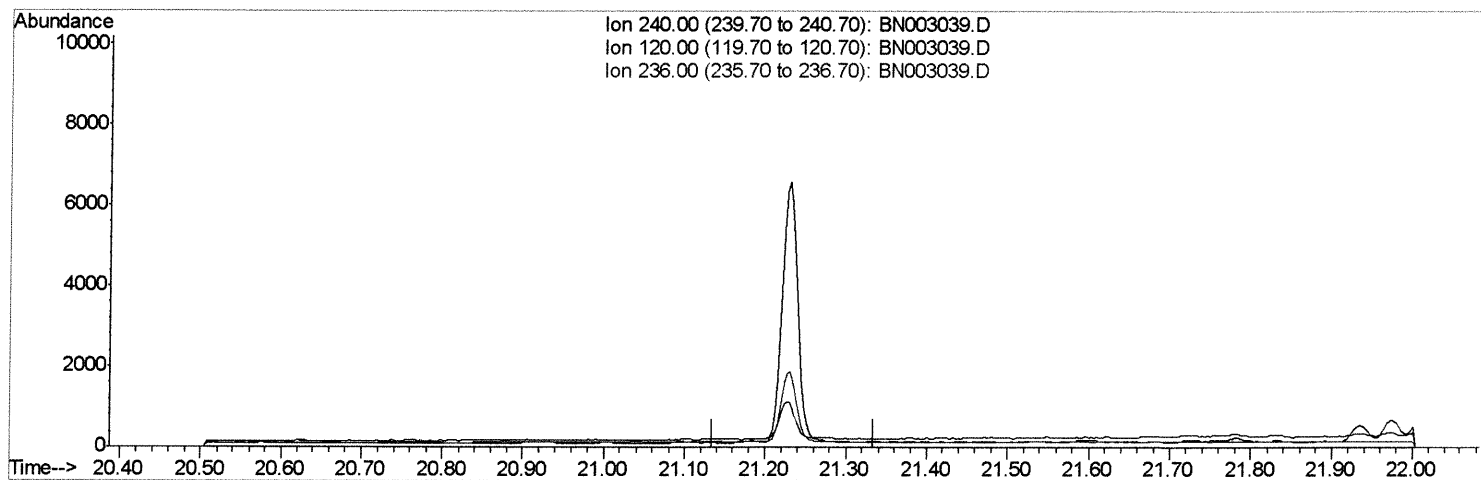

(16) Chrysene-d12 (I)

21.235min (-21.235) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	16.40	0.00#
236.00	28.10	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003039.D
 Acq On : 09 Oct 2018 22:26
 Operator : MJ/SJ
 Sample : J5157-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD1

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:50 PM

Quant Time: Oct 10 02:09:31 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

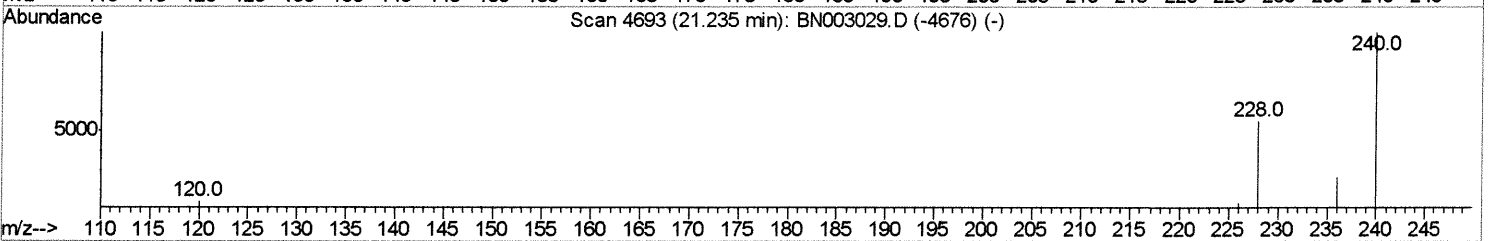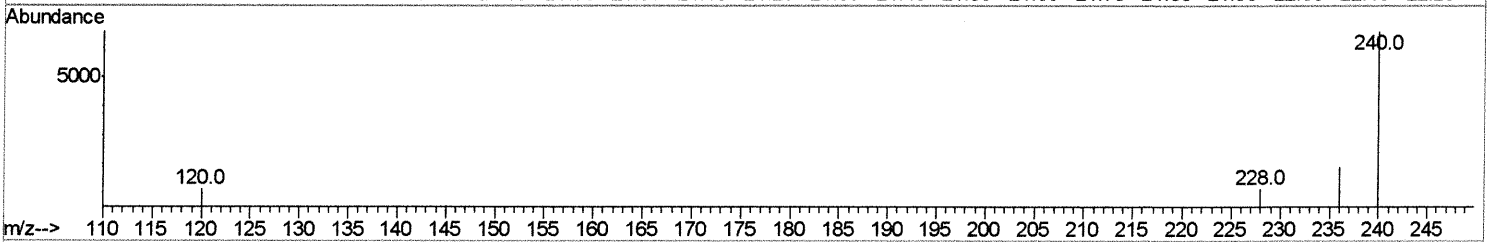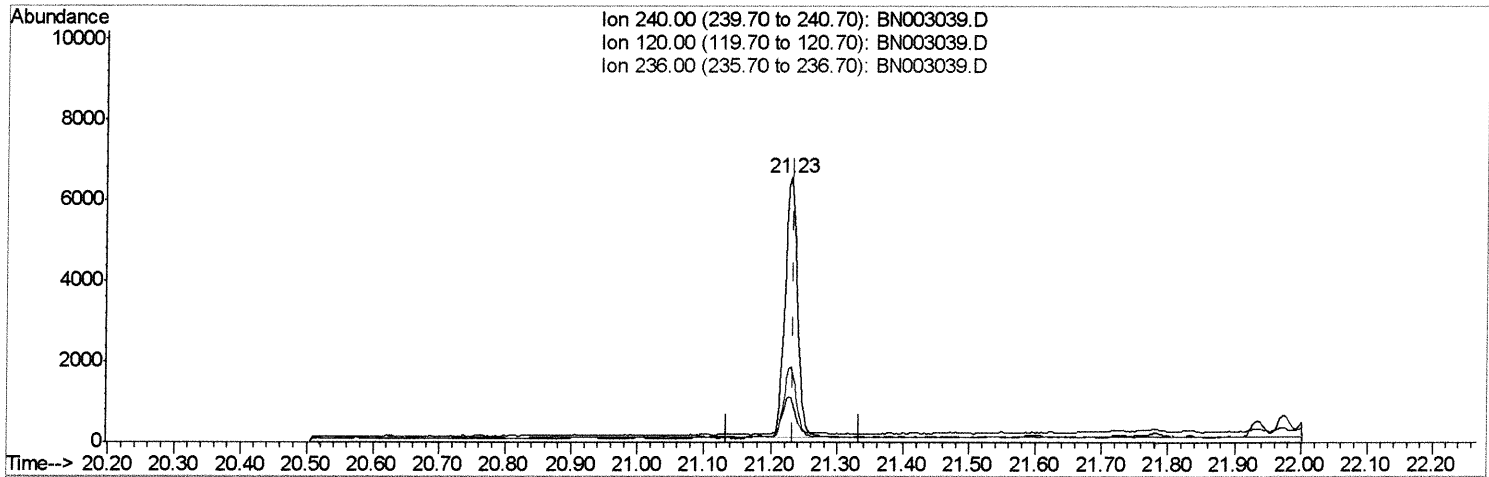

TIC: BN003039.D

(16) Chrysene-d12 (I)

21.229min (-0.006) 0.40ng/ul m *SJ 10/12/18*

response 8453

Ion	Exp%	Act%
240.00	100	100
120.00	16.40	16.79
236.00	28.10	28.54
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003039.D
 Acq On : 09 Oct 2018 22:26
 Operator : MJ/SJ
 Sample : J5157-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD1

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:50 PM

Quant Time: Oct 10 02:11:05 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

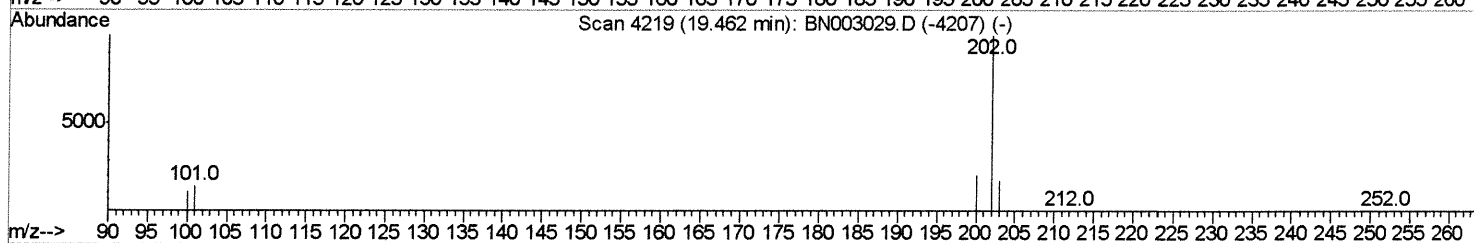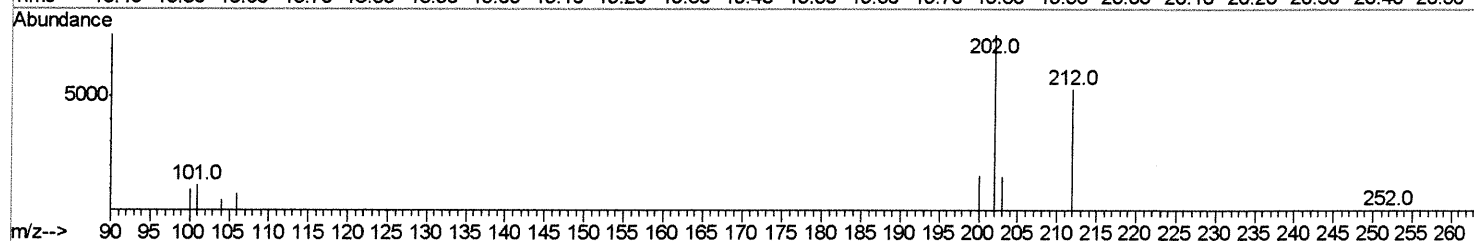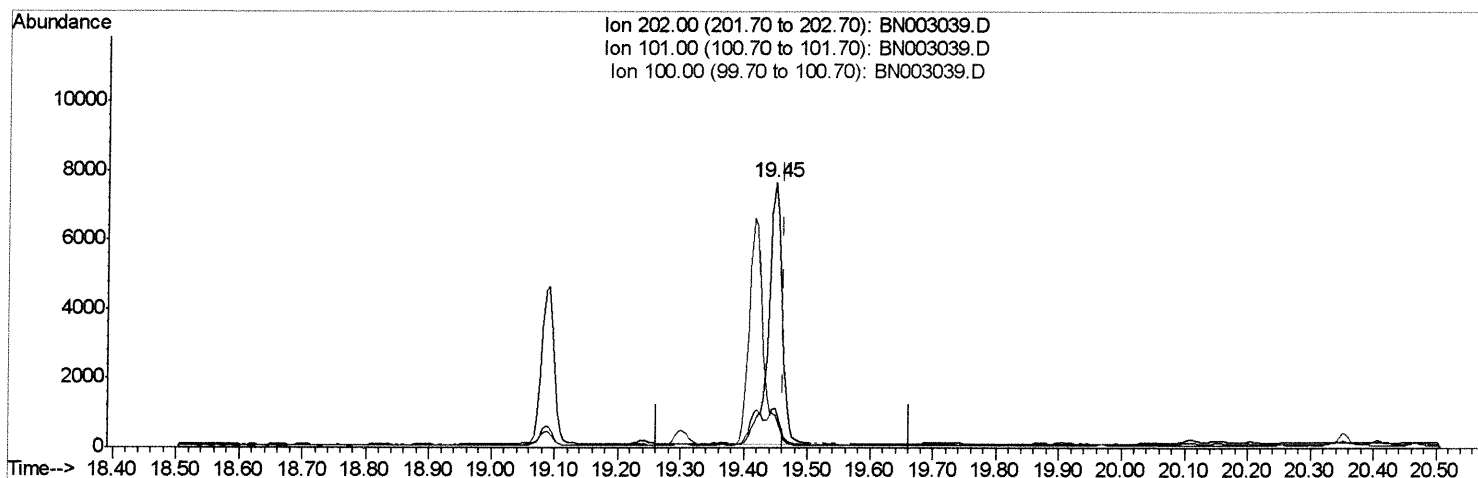

TIC: BN003039.D

(17) Pyrene

19.448min (-0.014) 0.35ng/ul

response 11594

Ion	Exp%	Act%
202.00	100	100
101.00	14.90	14.87
100.00	12.40	12.35
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003039.D
 Acq On : 09 Oct 2018 22:26
 Operator : MJ/SJ
 Sample : J5157-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD1

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:50 PM

Quant Time: Oct 10 02:11:05 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

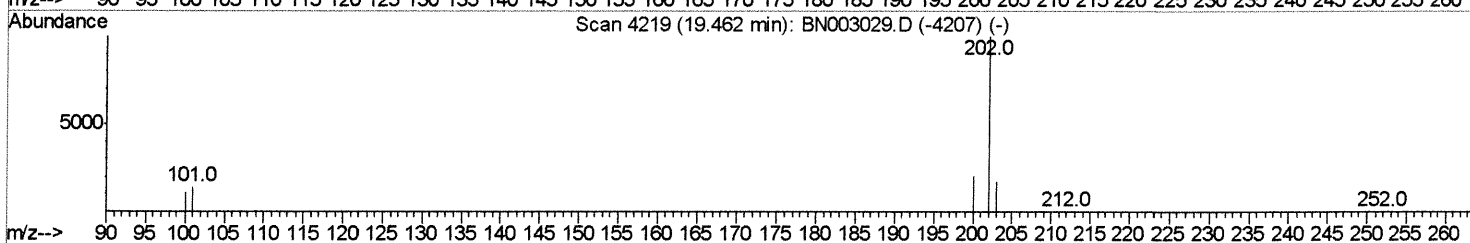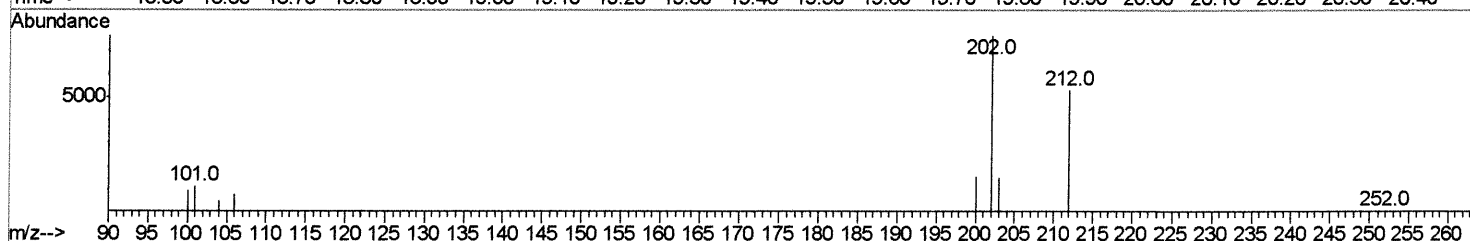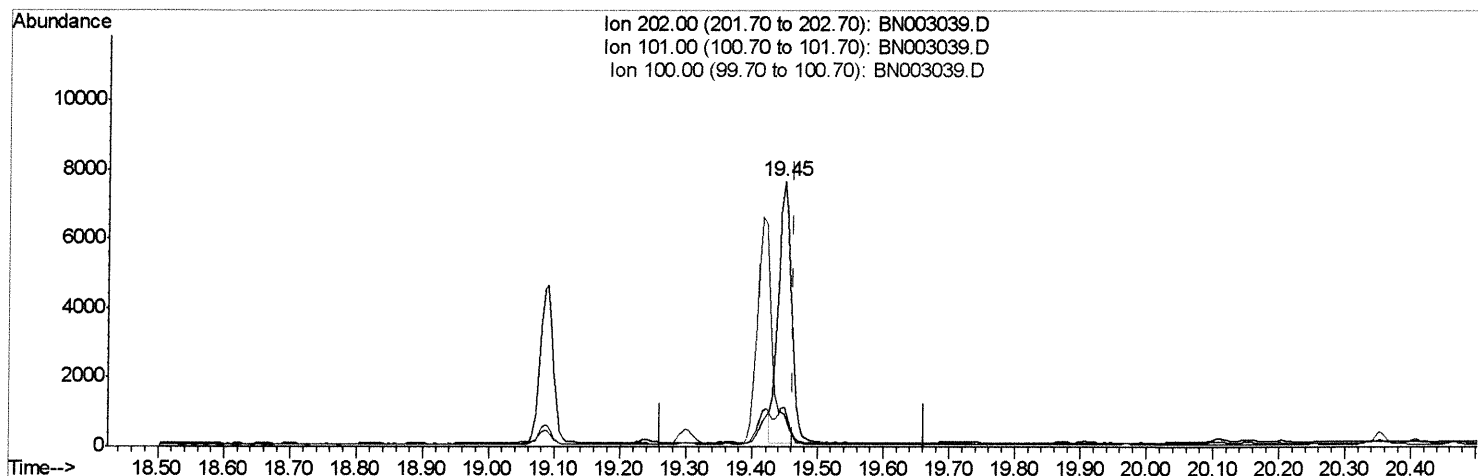

TIC: BN003039.D

(17) Pyrene

19.448min (-0.014) 0.33ng/ul m

5/10/12/18

response 10682

Ion	Exp%	Act%
202.00	100	100
101.00	14.90	14.87
100.00	12.40	12.35
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003039.D
Acq On : 09 Oct 2018 22:26
Operator : MJ/SJ
Sample : J5157-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD1

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:50 PM

Quant Time: Oct 10 02:11:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

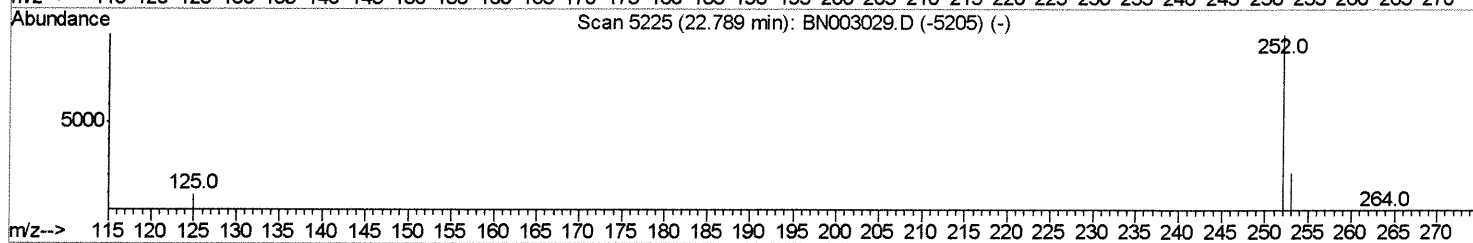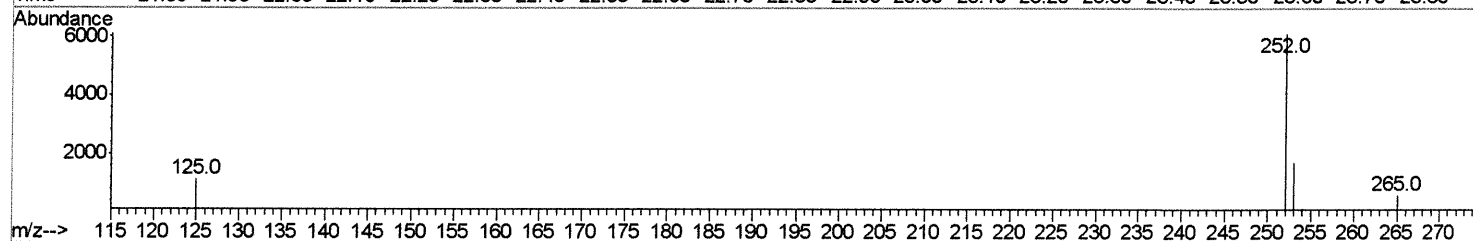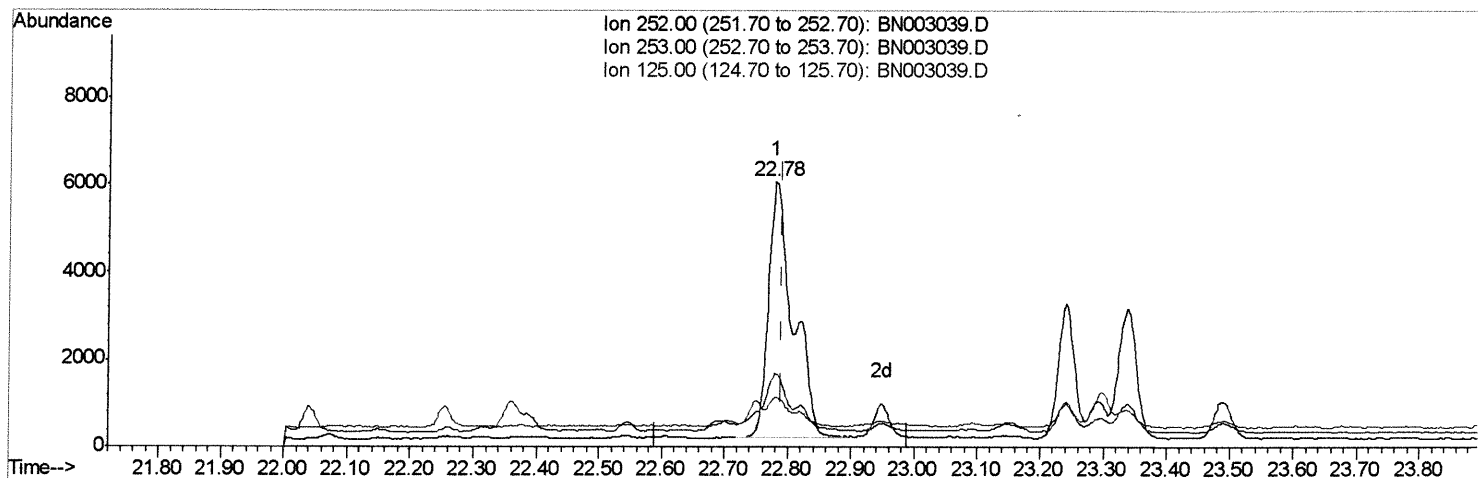

TIC: BN003039.D

(21) Benzo(b)fluoranthene

22.778min (-0.012) 0.65ng/ul

response 15897

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	27.83
125.00	17.10	18.70
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003039.D
Acq On : 09 Oct 2018 22:26
Operator : MJ/SJ
Sample : J5157-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD1

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:50 PM

Quant Time: Oct 10 02:11:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

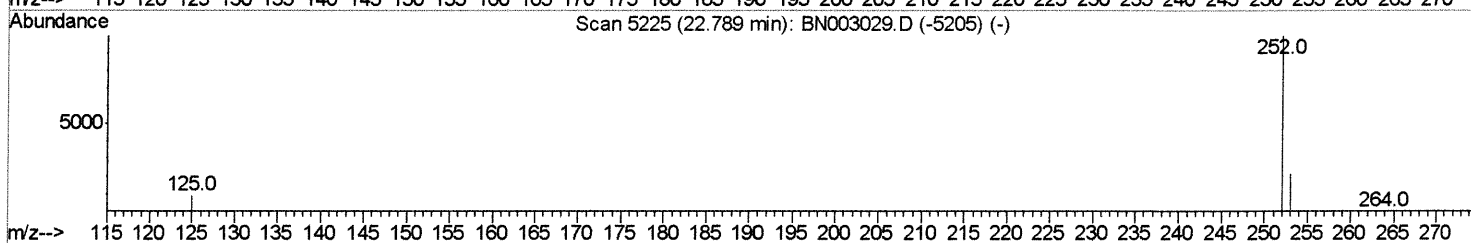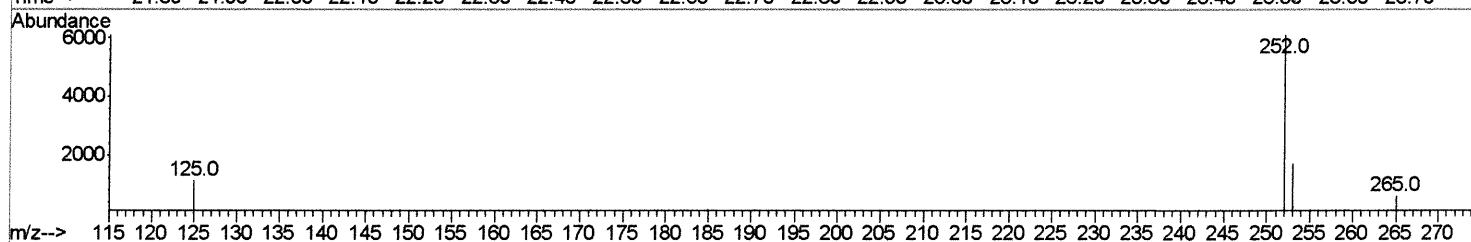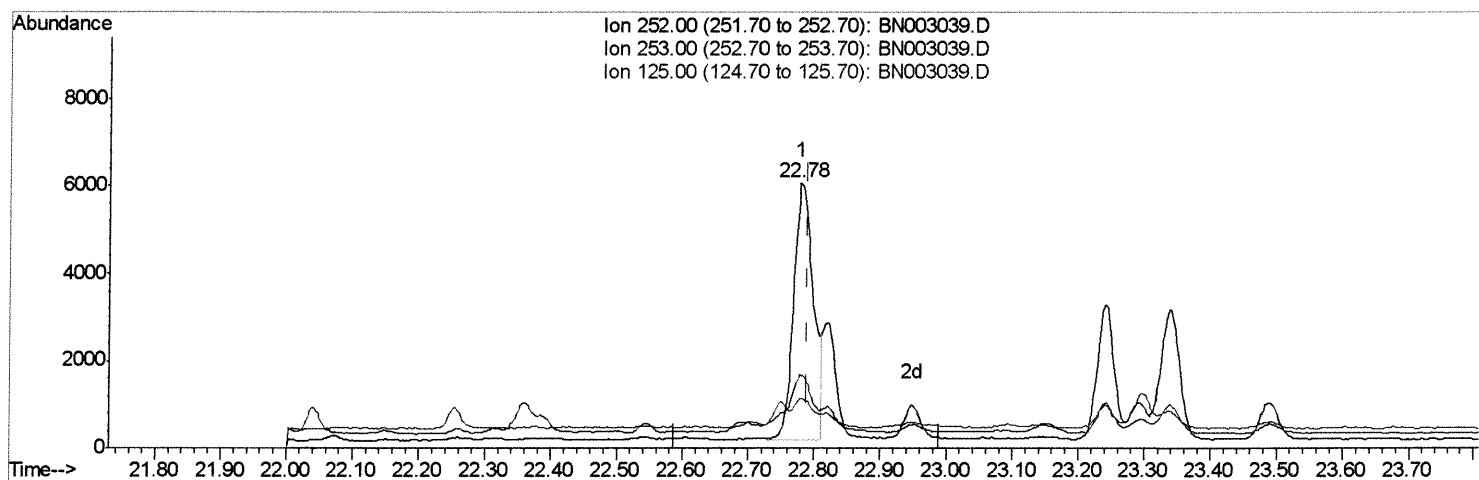

TIC: BN003039.D

(21) Benzo(b)fluoranthene

22.778min (-0.012) 0.50ng/ul m

5 J10/12/18

response 12309

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	27.83
125.00	17.10	18.70
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003039.D
Acq On : 09 Oct 2018 22:26
Operator : MJ/SJ
Sample : J5157-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD1

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:50 PM

Quant Time: Oct 10 02:11:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

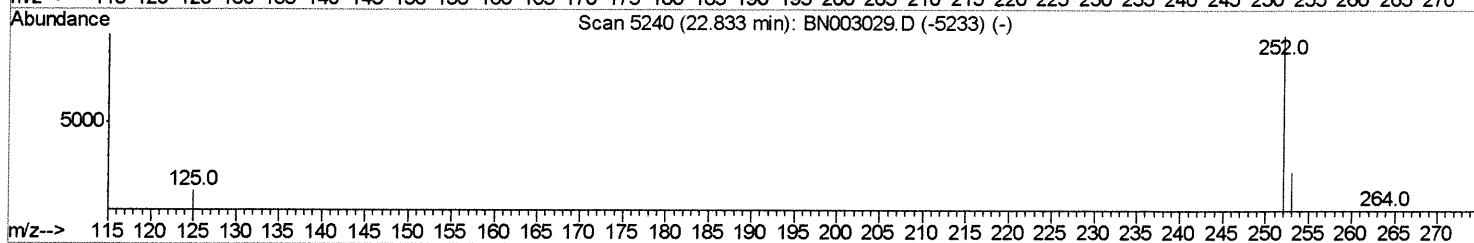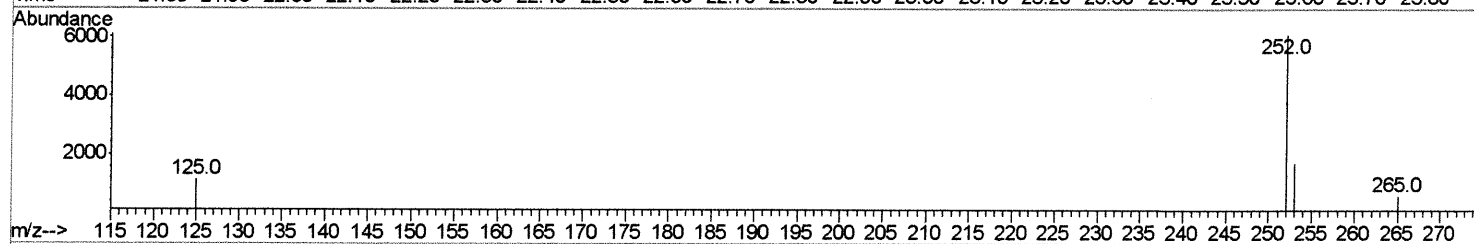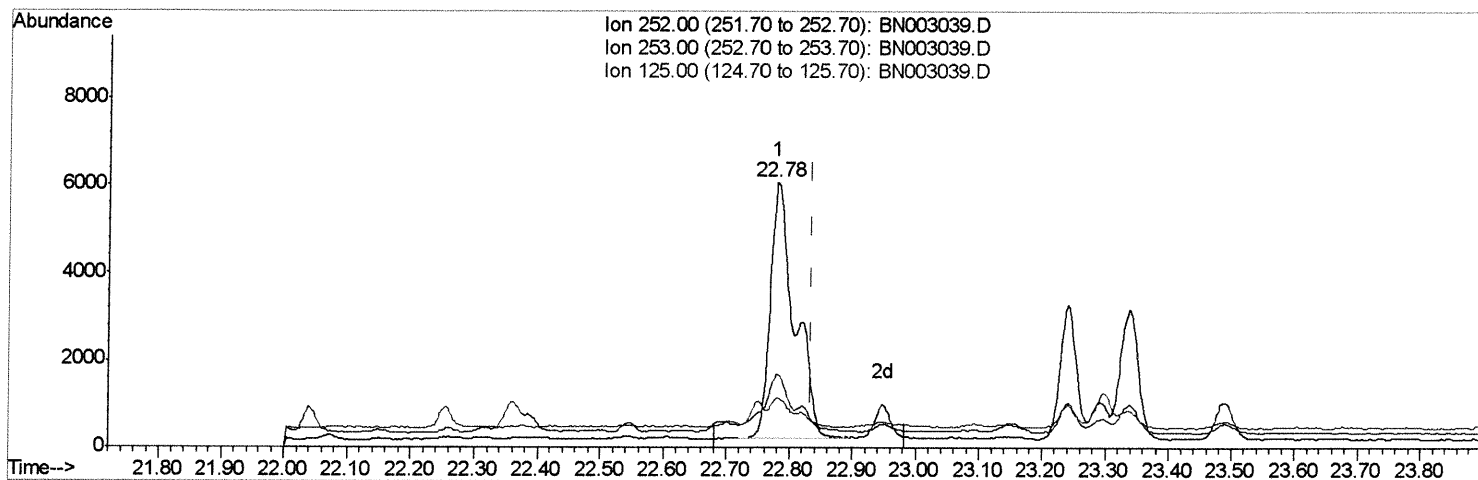

TIC: BN003039.D

(22) Benzo(k)fluoranthene

22.778min (-0.056) 0.62ng/ul

response 15897

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	27.83
125.00	17.60	18.70
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003039.D
 Acq On : 09 Oct 2018 22:26
 Operator : MJ/SJ
 Sample : J5157-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD1

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:50 PM

Quant Time: Oct 10 02:11:05 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

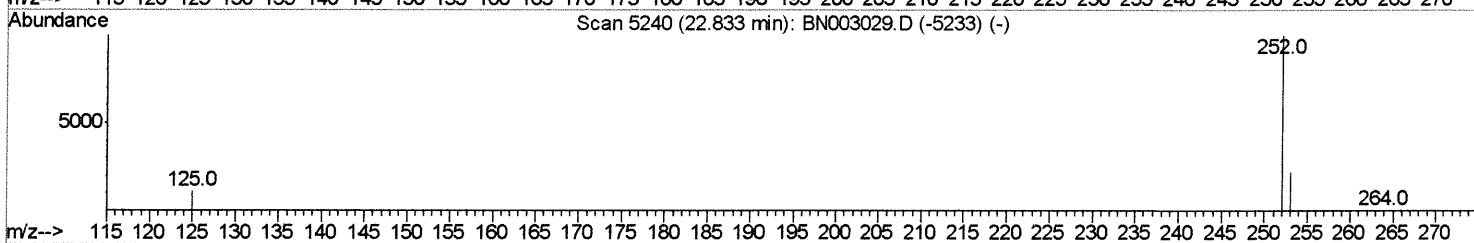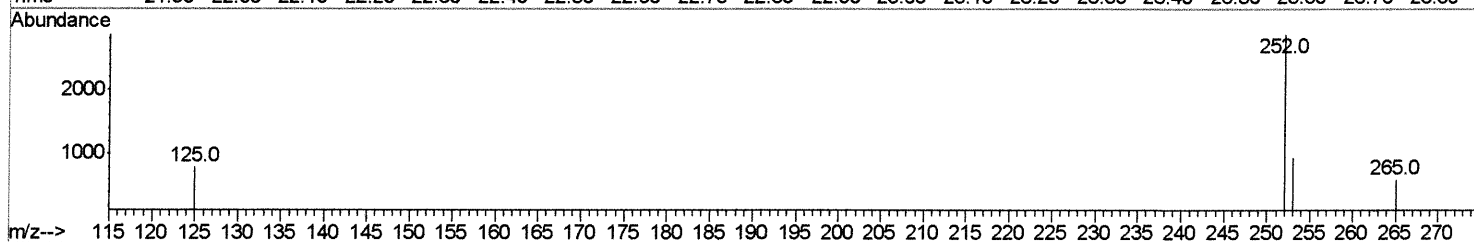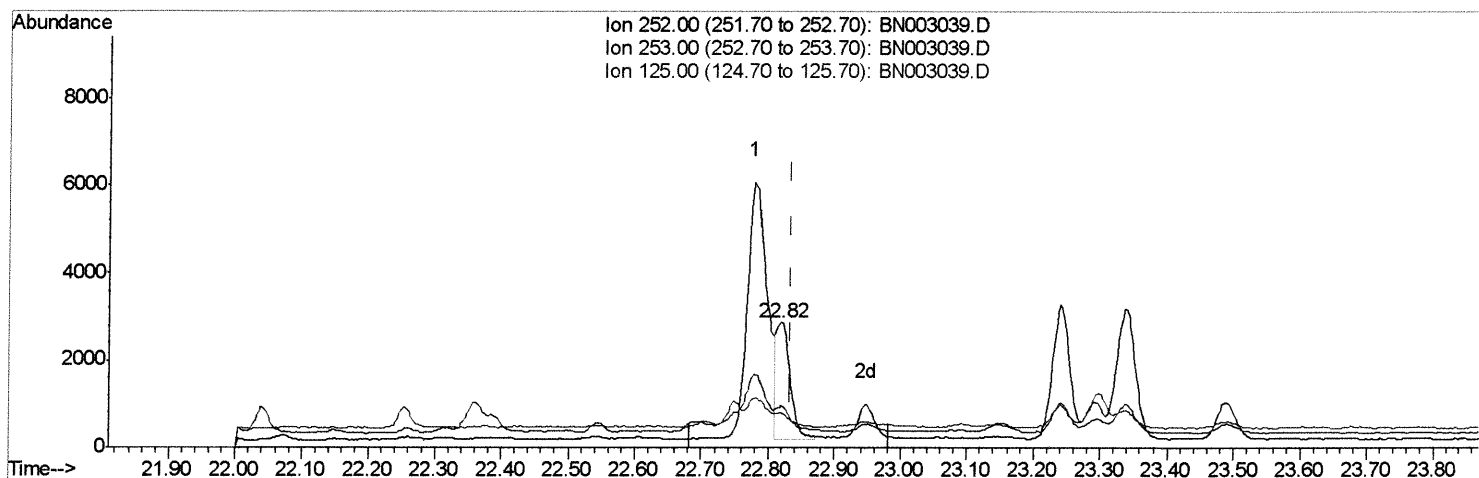

(22) Benzo(k)fluoranthene

22.819min (-0.015) 0.15ng/ul m

SJ 10/12/18

response 3708

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	33.43#
125.00	17.60	27.76#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003039.D
 Acq On : 09 Oct 2018 22:26
 Operator : MJ/SJ
 Sample : J5157-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD1

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:50 PM

Quant Time: Oct 10 02:12:33 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	1767	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.39	136	7569	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.26	164	4506	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.02	188	10123m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.23	240	8453m	0.40	ng/ul	0.00
20) Perylene-d12	23.44	264	6817	0.40	ng/ul	-0.01

> SJ 10/12/18

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.01	152	3754	0.32	ng/ul	-0.01
14) Fluoranthene-d10	19.06	212	9496m	0.33	ng/ul	0.00

> SJ 10/12/18

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Naphthalene	10.44	128	550	0.028	ng/ul#	71
7) Acenaphthylene	13.98	152	761	0.037	ng/ul#	79
12) Phenanthrene	17.06	178	2039m	0.072	ng/ul	
13) Anthracene	17.15	178	1519m	0.057	ng/ul	
15) Fluoranthene	19.09	202	6323m	0.191	ng/ul	
17) Pyrene	19.45	202	10682m	0.325	ng/ul	
18) Benzo(a)anthracene	21.21	228	3765	0.138	ng/ul#	88
19) Chrysene	21.27	228	5653	0.205	ng/ul#	92
21) Benzo(b)fluoranthene	22.78	252	12309m	0.501	ng/ul	
22) Benzo(k)fluoranthene	22.82	252	3708m	0.146	ng/ul	
23) Benzo(a)pyrene	23.34	252	6053	0.275	ng/ul#	92
24) Indeno(1,2,3-cd)pyrene	25.66	276	3124	0.124	ng/ul#	94
25) Dibenzo(a,h)anthracene	25.65	278	940	0.046	ng/ul#	26
26) Benzo(a,h,i)perylene	26.33	276	2636	0.124	ng/ul#	84

> SJ 10/12/18

> SJ 10/12/18

(#) = qualifier out of range (m) = manual integration (+) = signals summed