

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003041.D
 Acq On : 09 Oct 2018 23:37
 Operator : MJ/SJ
 Sample : J5157-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD3

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:52 PM

Quant Time: Oct 10 02:25:33 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

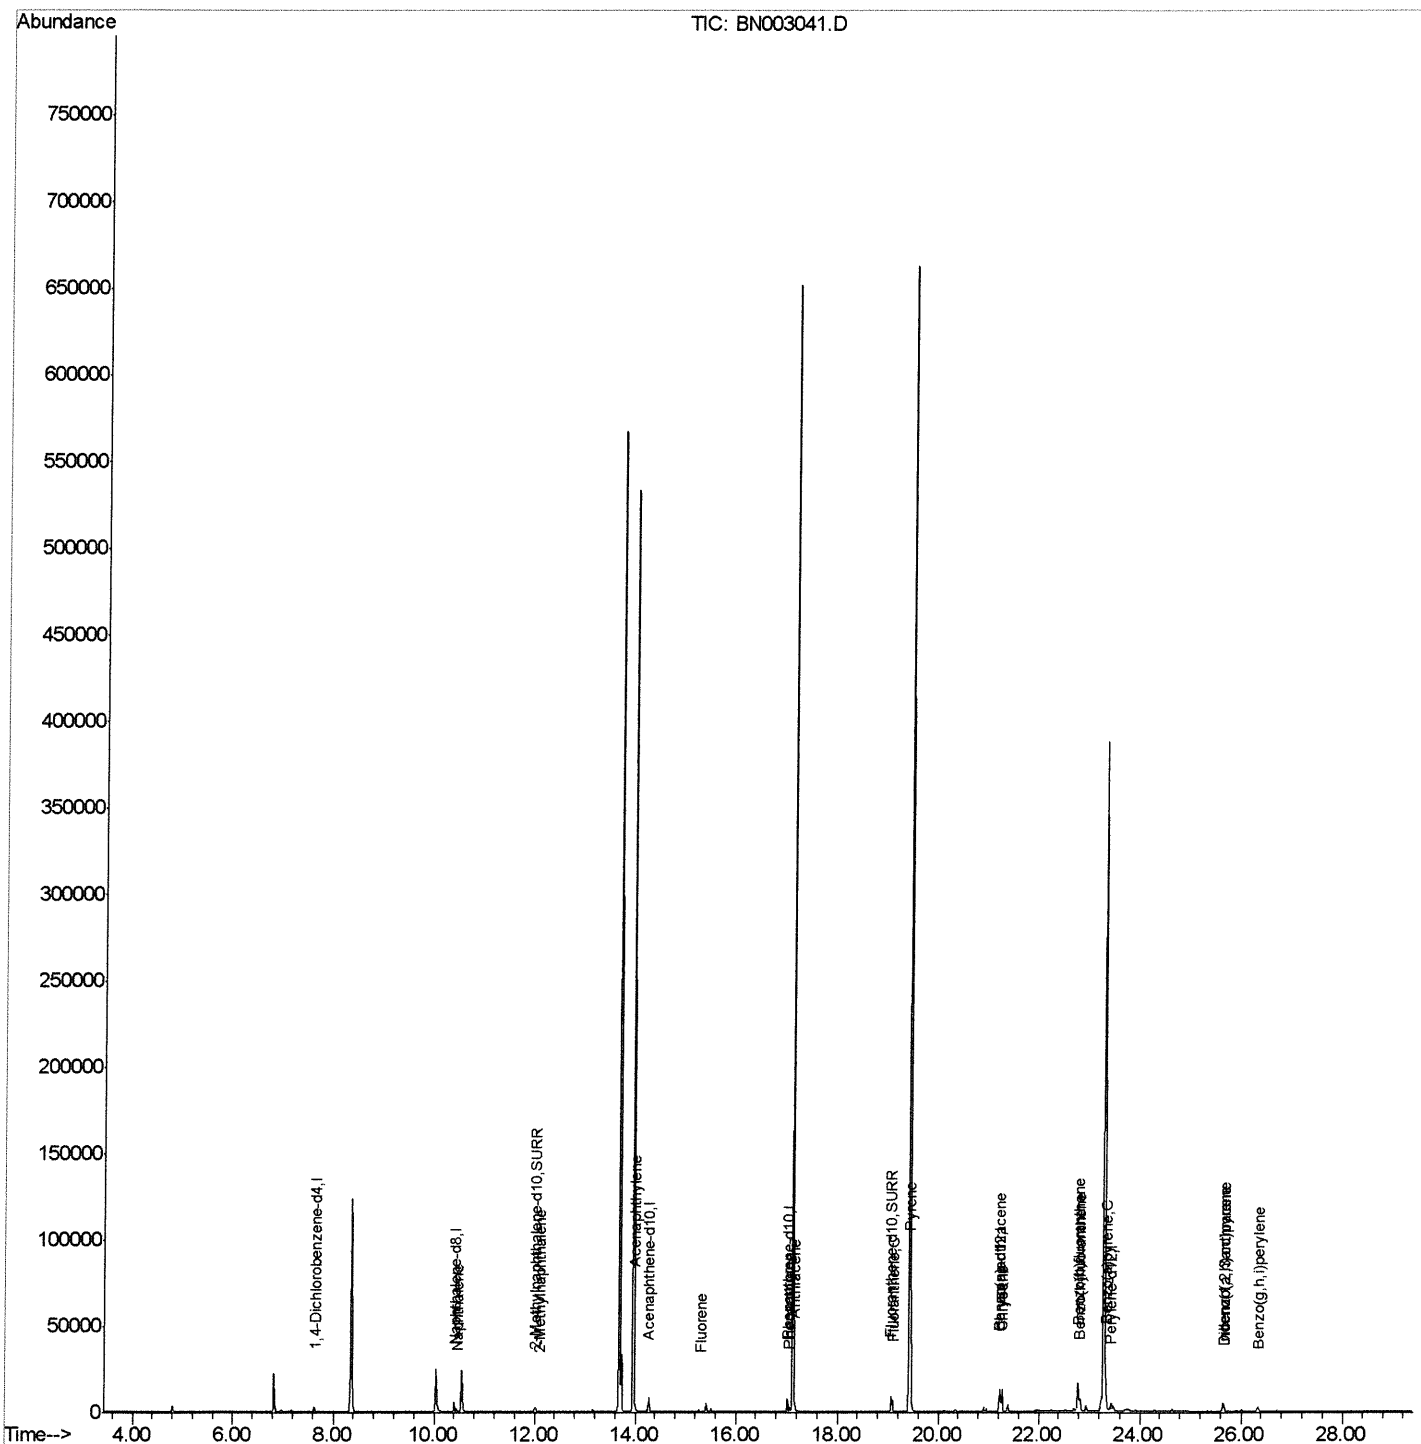

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003041.D
 Acq On : 09 Oct 2018 23:37
 Operator : MJ/SJ
 Sample : J5157-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD3

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:52 PM

Quant Time: Oct 10 01:38:21 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

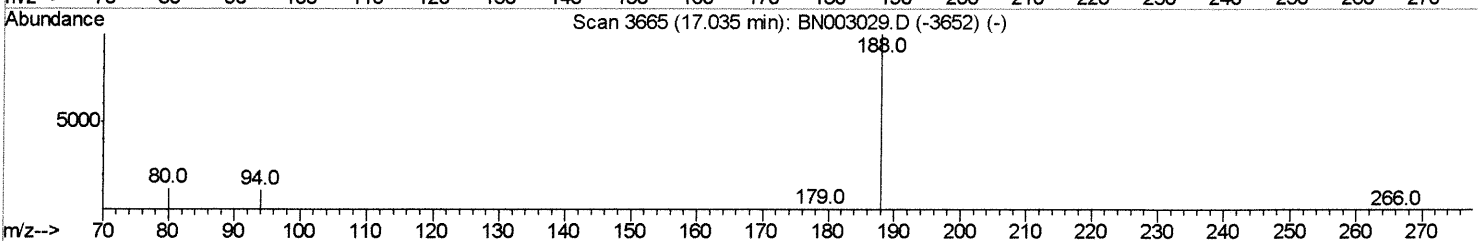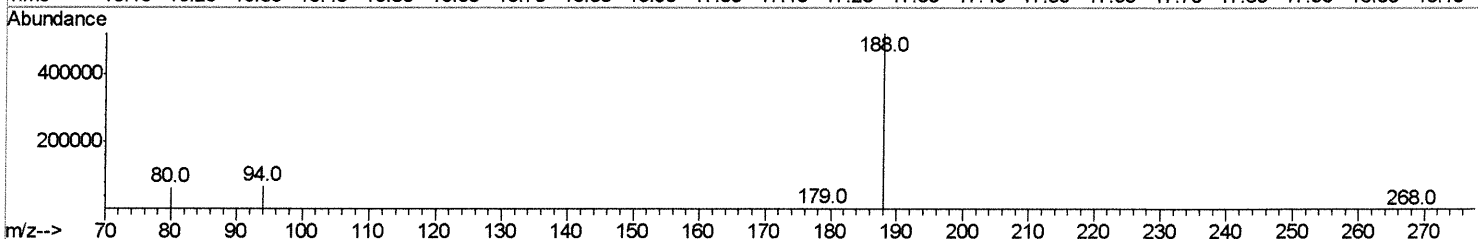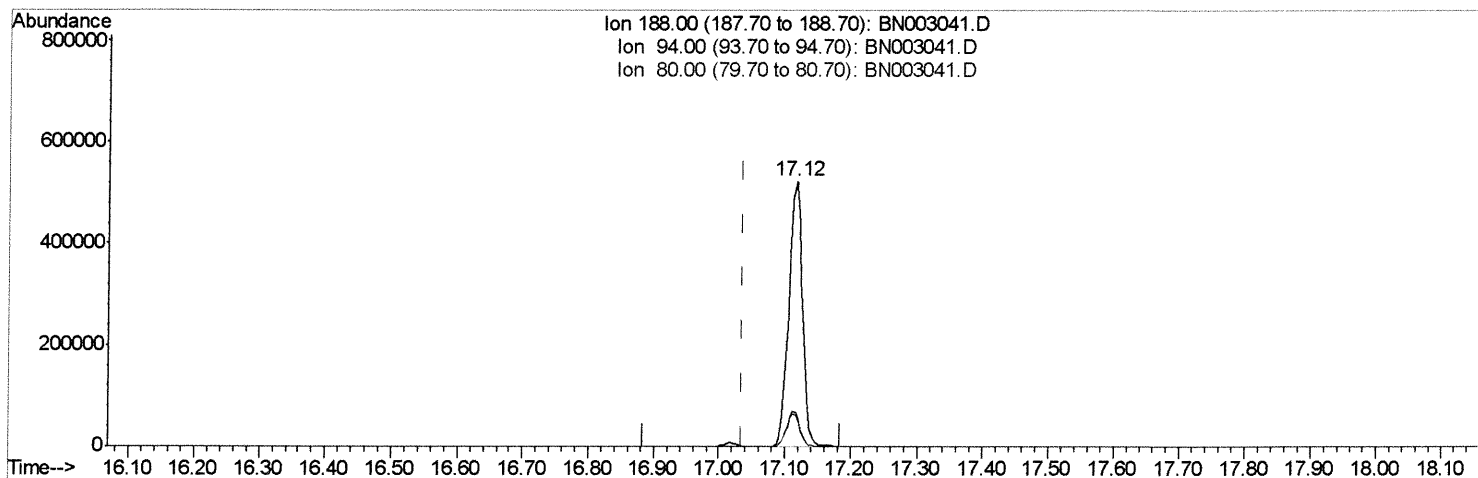

TIC: BN003041.D

(10) Phenanthrene-d10 (I)
 17.116min (+0.080) 0.40ng/ul
 response 747396

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	12.94
80.00	12.70	11.79
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003041.D
Acq On : 09 Oct 2018 23:37
Operator : MJ/SJ
Sample : J5157-11
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD3

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:52 PM

Quant Time: Oct 10 01:38:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

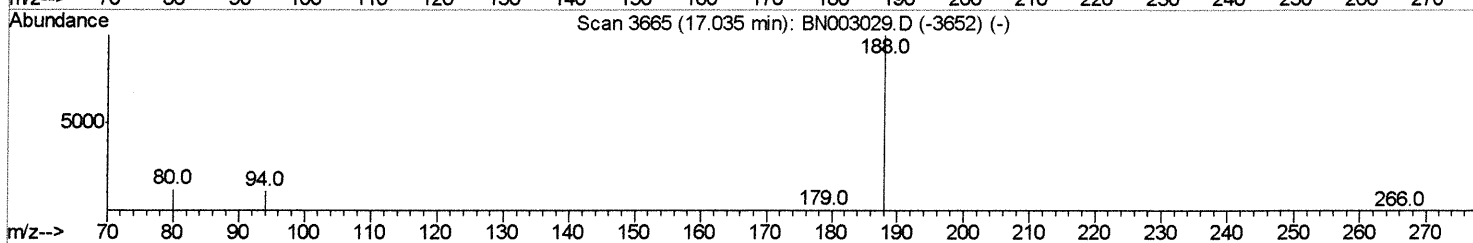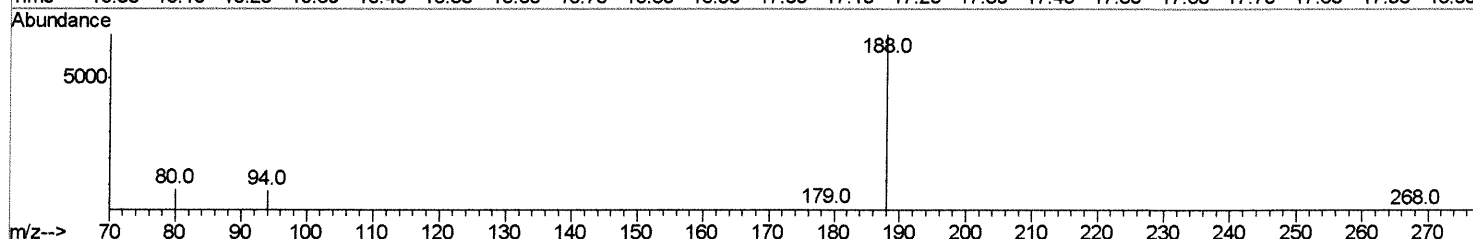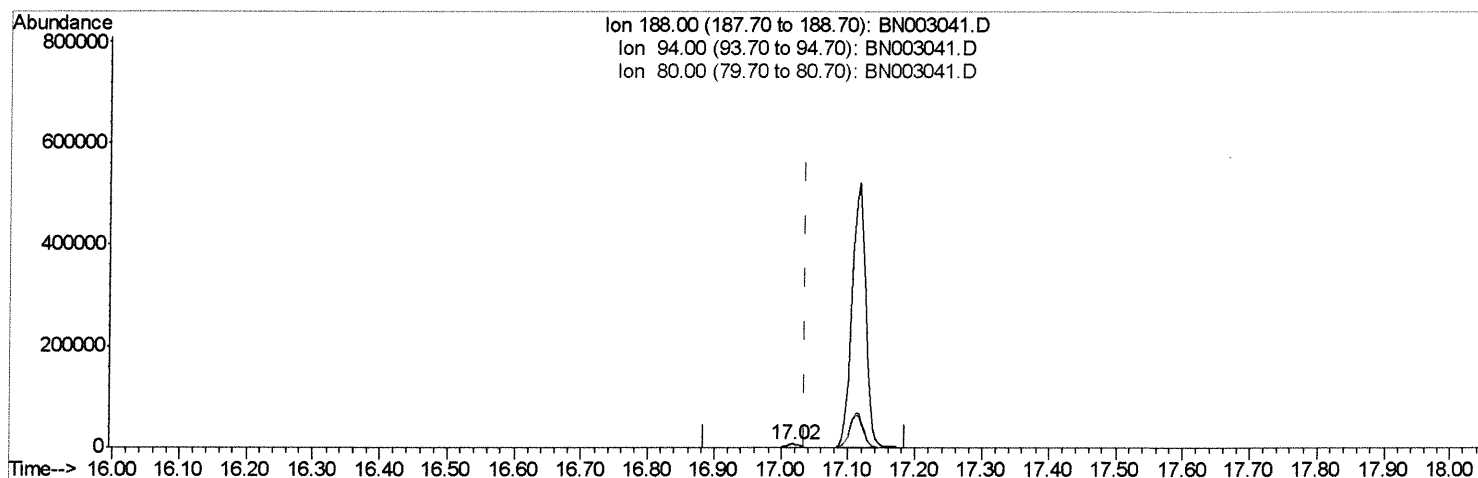

TIC: BN003041.D

(10) Phenanthrene-d10 (I)

17.018min (-0.017) 0.40ng/ul m

5110/12/18

response 9365

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	11.68
80.00	12.70	12.49
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003041.D
Acq On : 09 Oct 2018 23:37
Operator : MJ/SJ
Sample : J5157-11
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD3

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:52 PM

Quant Time: Oct 10 02:22:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

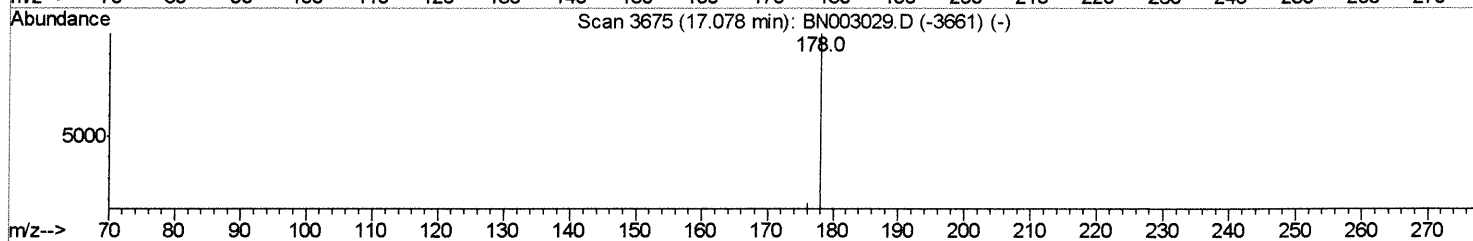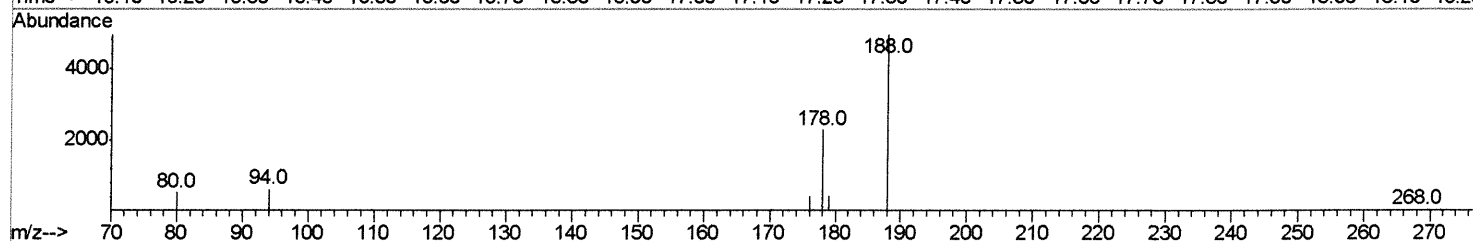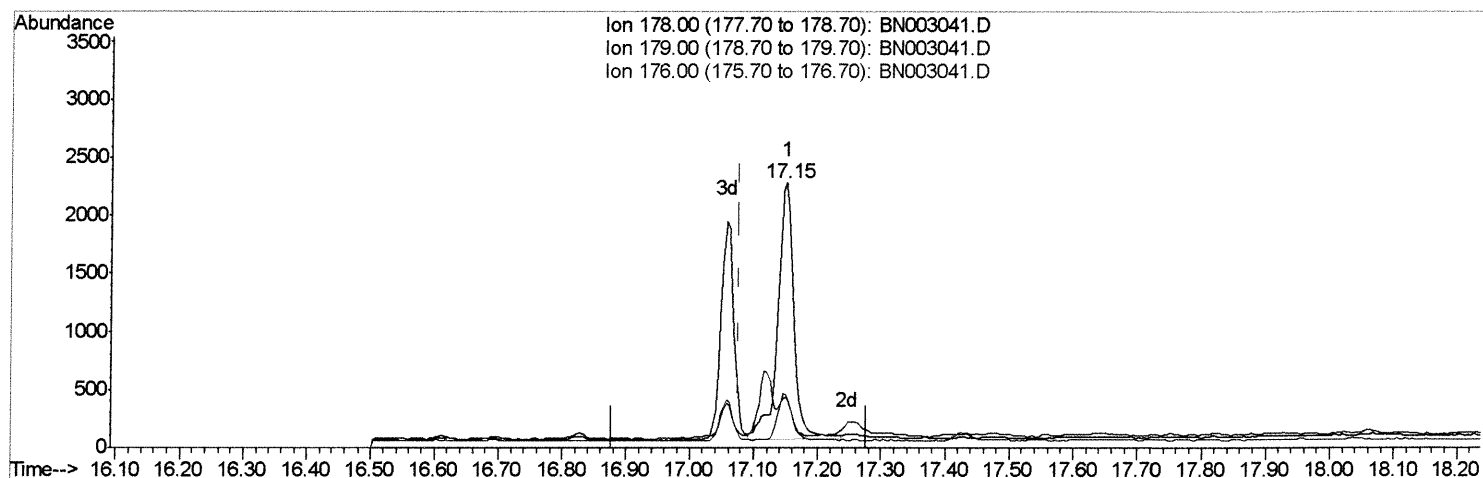

TIC: BN003041.D

(12) Phenanthrene

17.149min (+0.072) 0.15ng/ul

response 3856

Ion	Exp%	Act%
178.00	100	100
179.00	16.10	19.14
176.00	19.30	20.02
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003041.D
Acq On : 09 Oct 2018 23:37
Operator : MJ/SJ
Sample : J5157-11
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD3

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:52 PM

Quant Time: Oct 10 02:22:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

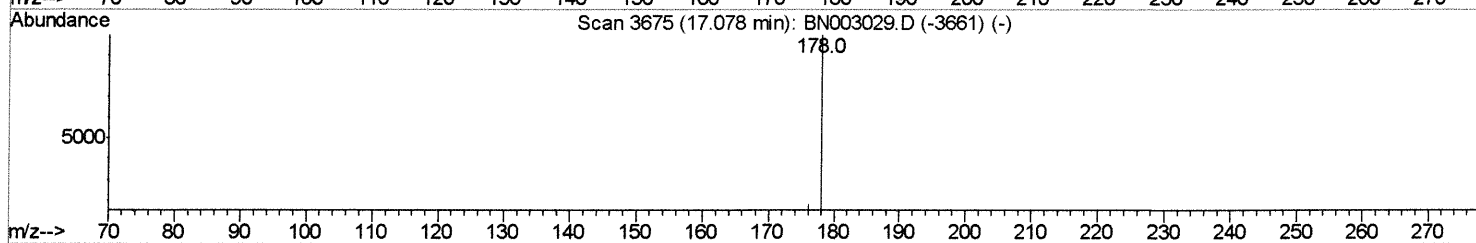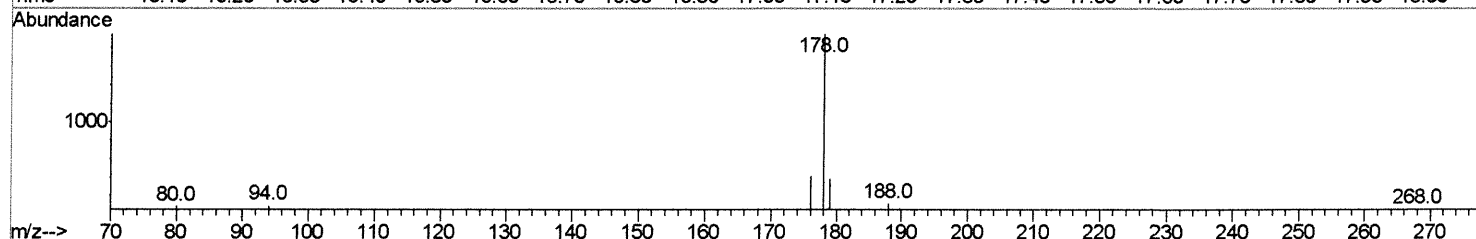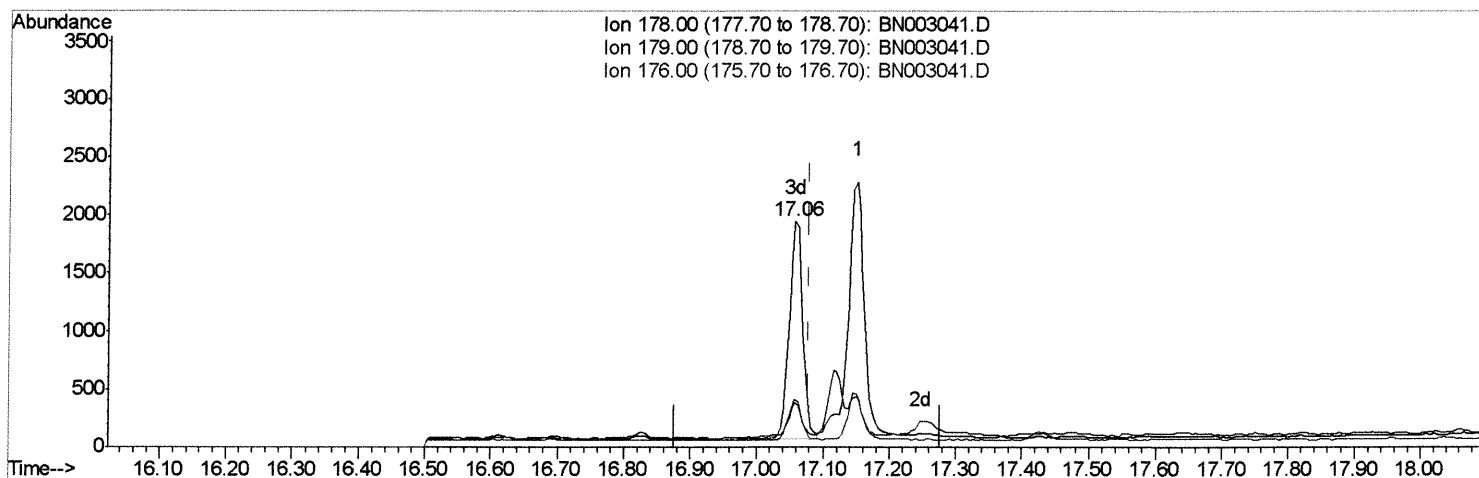

TIC: BN003041.D

(12) Phenanthrene

17.056min (-0.021) 0.10ng/ul m

SJ 10/12/18

response 2659

Ion	Exp%	Act%
178.00	100	100
179.00	16.10	19.55#
176.00	19.30	21.14
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003041.D
 Acq On : 09 Oct 2018 23:37
 Operator : MJ/SJ
 Sample : J5157-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD3

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:52 PM

Quant Time: Oct 10 02:22:51 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

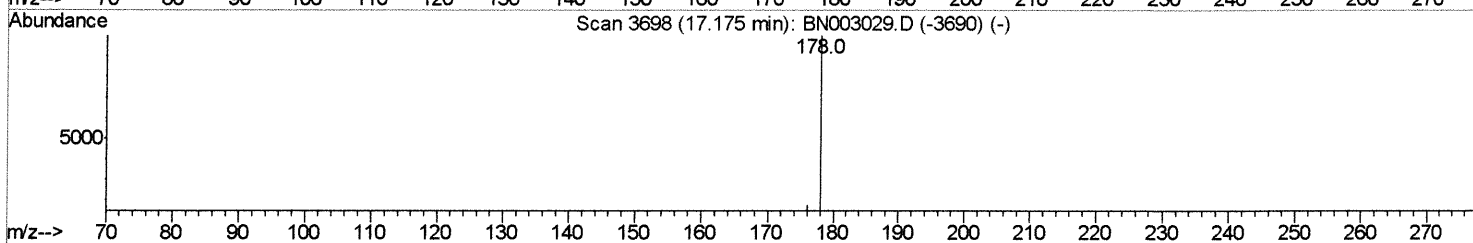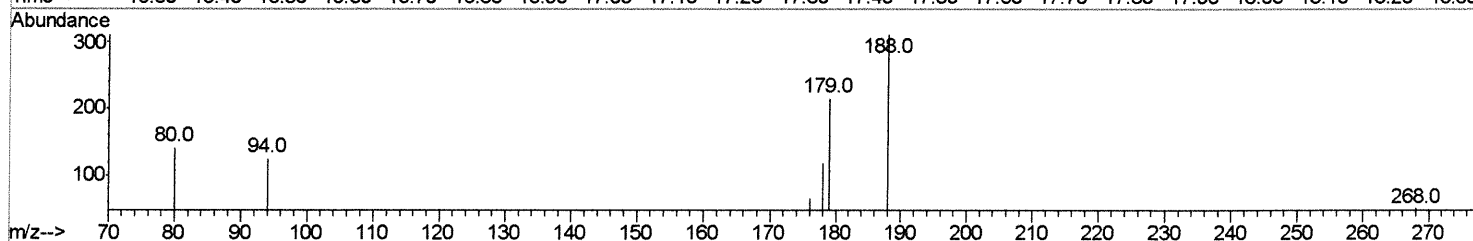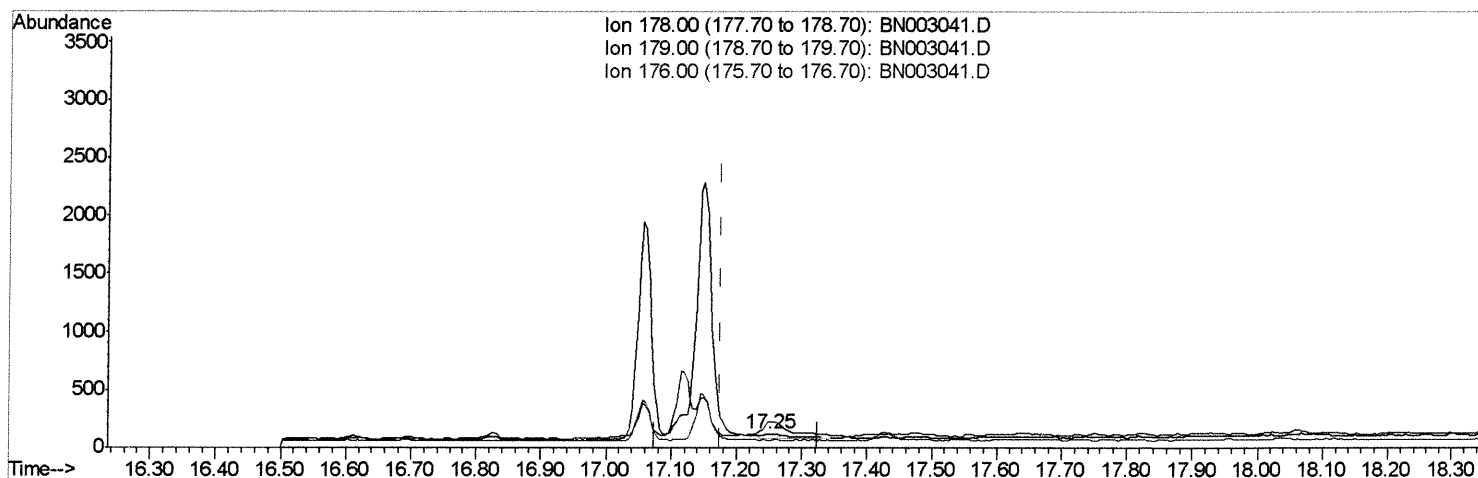

TIC: BN003041.D

(13) Anthracene

17.246min (+0.072) 0.00ng/ul

response 117

Ion	Exp%	Act%
178.00	100	100
179.00	16.30	182.20#
176.00	19.10	55.08#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003041.D
 Acq On : 09 Oct 2018 23:37
 Operator : MJ/SJ
 Sample : J5157-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD3

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:52 PM

Quant Time: Oct 10 02:22:51 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

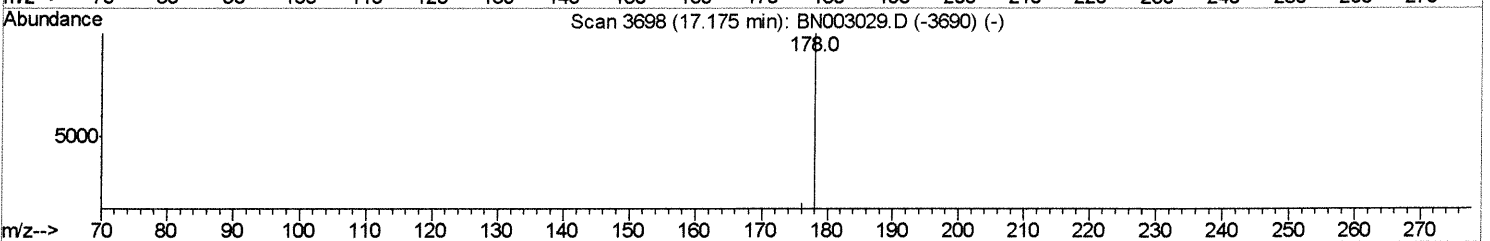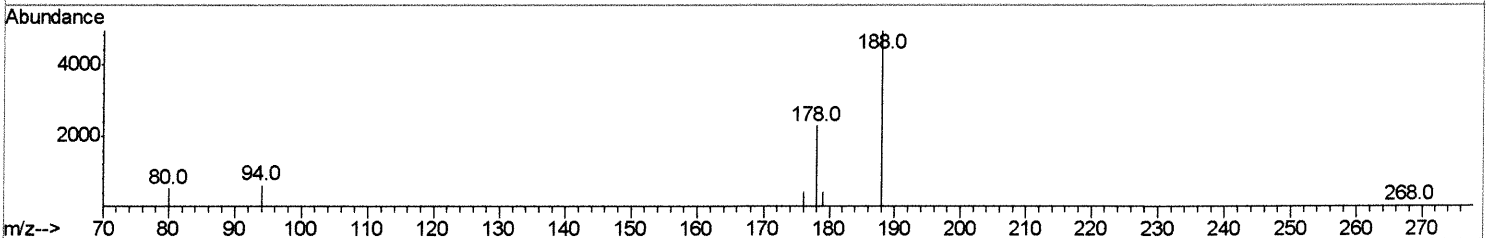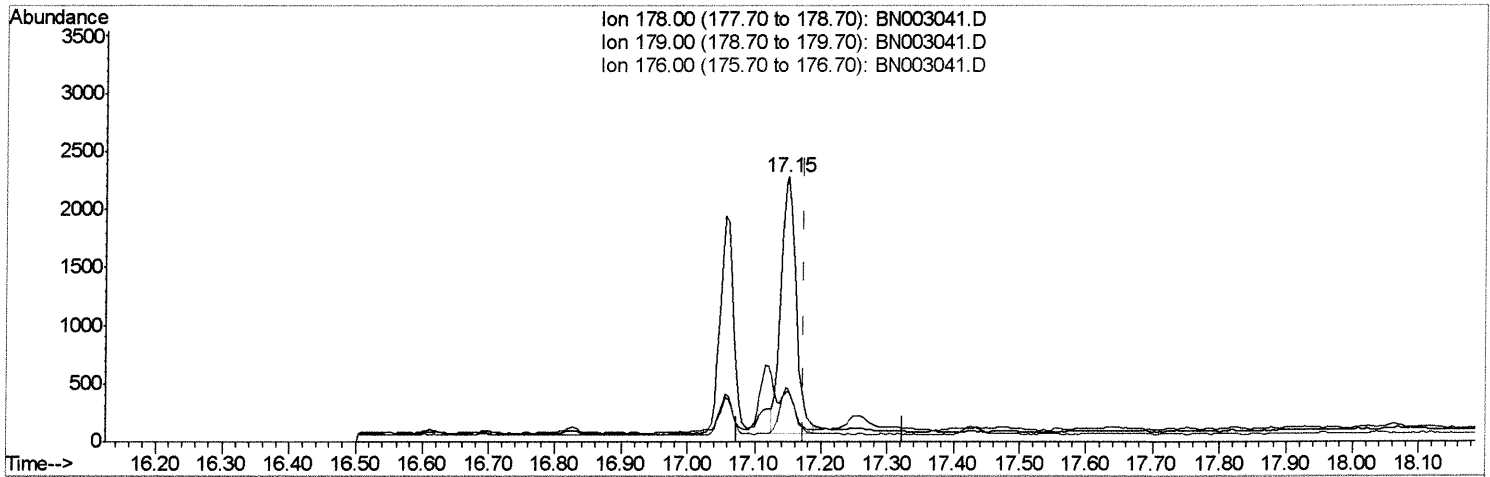

TIC: BN003041.D

(13) Anthracene

17.149min (-0.025) 0.14ng/ul m

SJ 10/12/18

response 3477

Ion	Exp%	Act%
178.00	100	100
179.00	16.30	19.14
176.00	19.10	20.02
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003041.D
 Acq On : 09 Oct 2018 23:37
 Operator : MJ/SJ
 Sample : J5157-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD3

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:52 PM

Quant Time: Oct 10 02:22:51 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

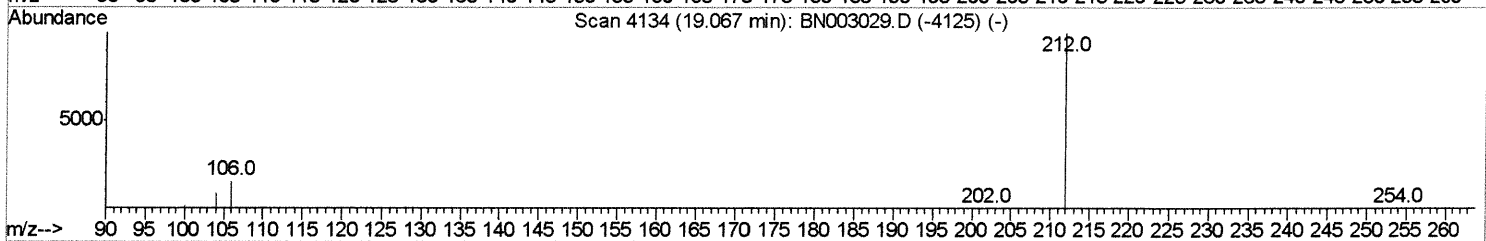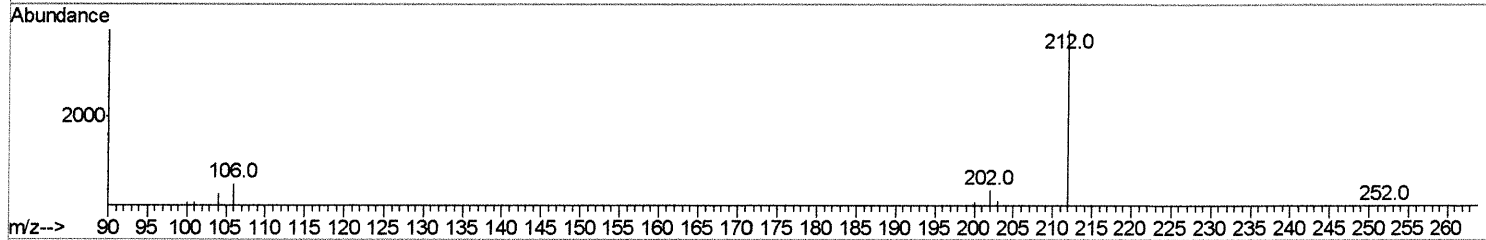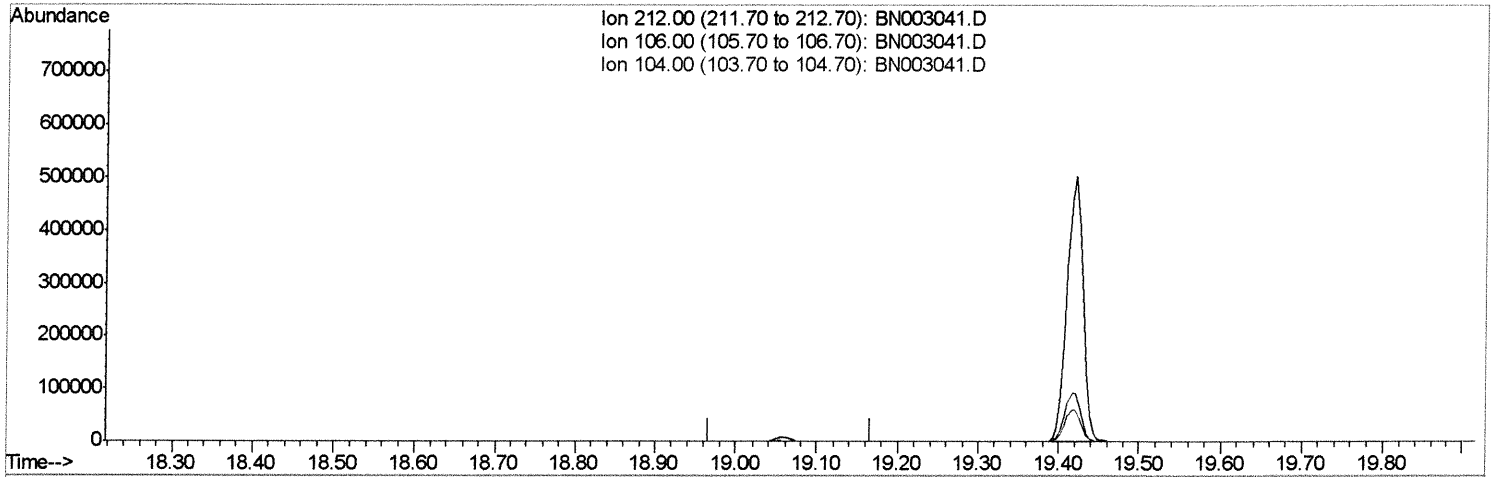

TIC: BN003041.D

(14) Fluoranthene-d10 (SURR)

19.067min (-19.067) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	15.40	0.00#
104.00	8.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003041.D
 Acq On : 09 Oct 2018 23:37
 Operator : MJ/SJ
 Sample : J5157-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 C0AD3

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:52 PM

Quant Time: Oct 10 02:22:51 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

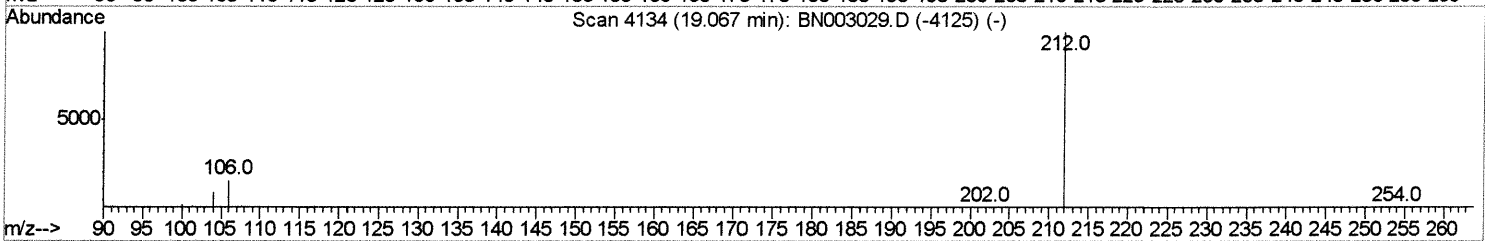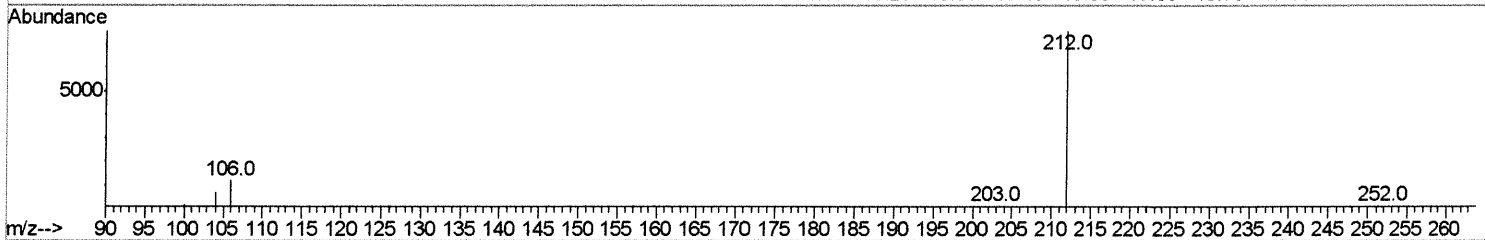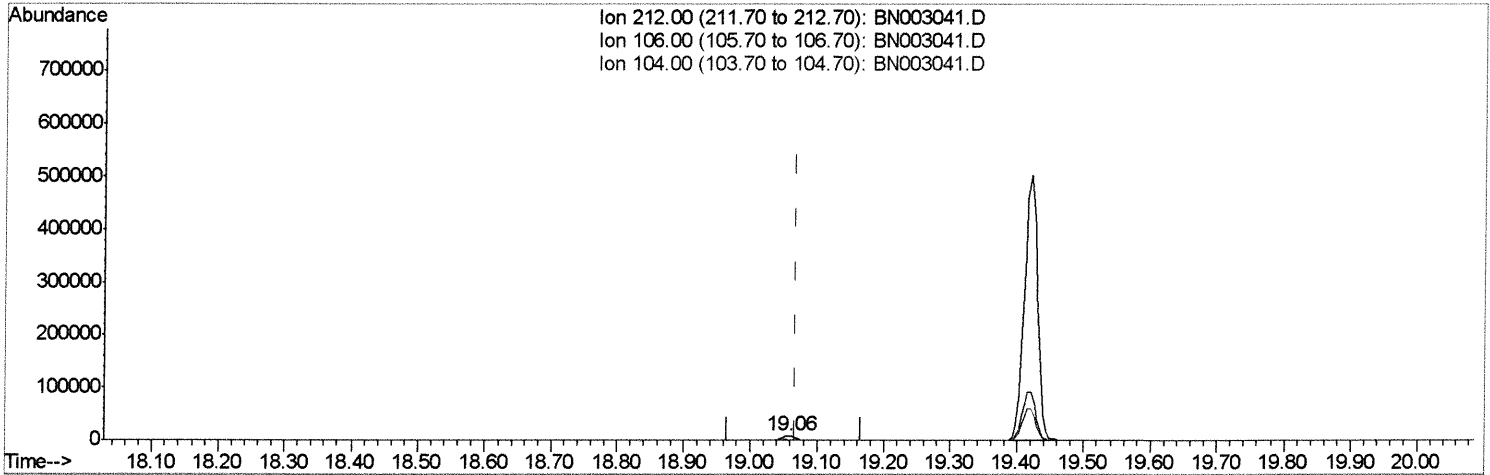

TIC: BN003041.D

(14) Fluoranthene-d10 (SURR)

19.058min (-0.009) 0.38ng/ul m

response 10256

Ion Exp% Act%

212.00 100 100

106.00 15.40 0.00#

104.00 8.60 0.00#

0.00 0.00 0.00

SJ 10/12/18

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003041.D
Acq On : 09 Oct 2018 23:37
Operator : MJ/SJ
Sample : J5157-11
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD3

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:52 PM

Quant Time: Oct 10 02:22:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

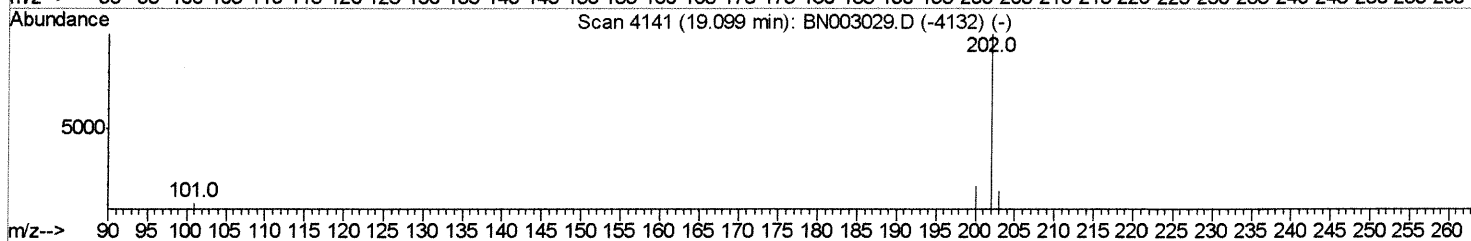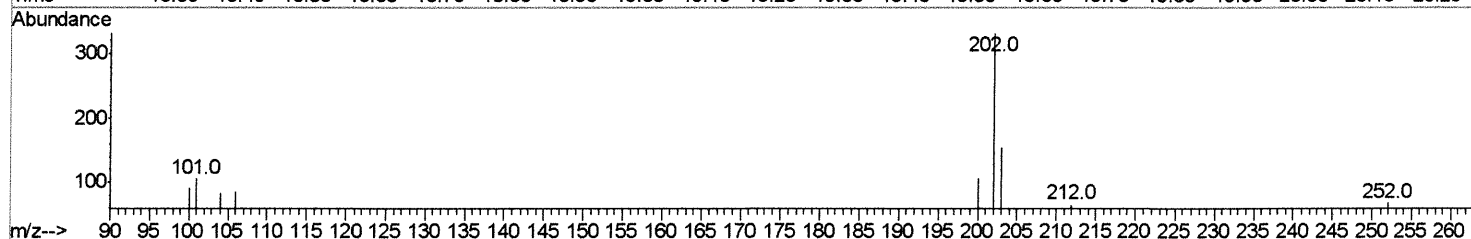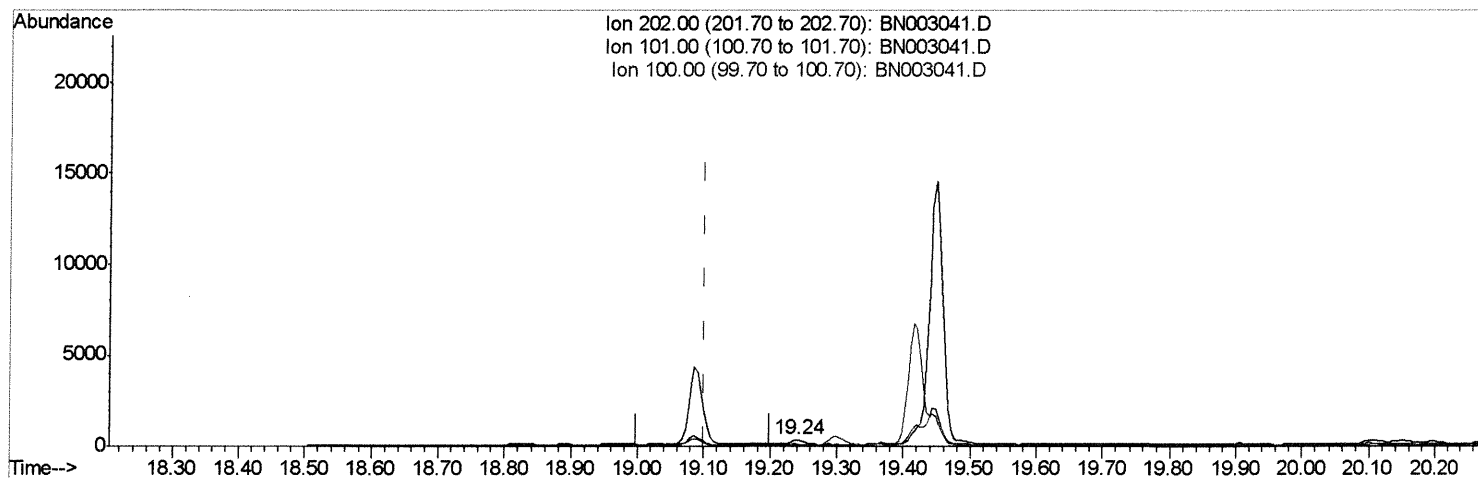

TIC: BN003041.D

(15) Fluoranthene (C)

19.239min (+0.139) 0.01ng/ul

response 335

Ion	Exp%	Act%
202.00	100	100
101.00	12.30	31.63
100.00	9.10	27.11
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003041.D
 Acq On : 09 Oct 2018 23:37
 Operator : MJ/SJ
 Sample : J5157-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD3

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:52 PM

Quant Time: Oct 10 02:22:51 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

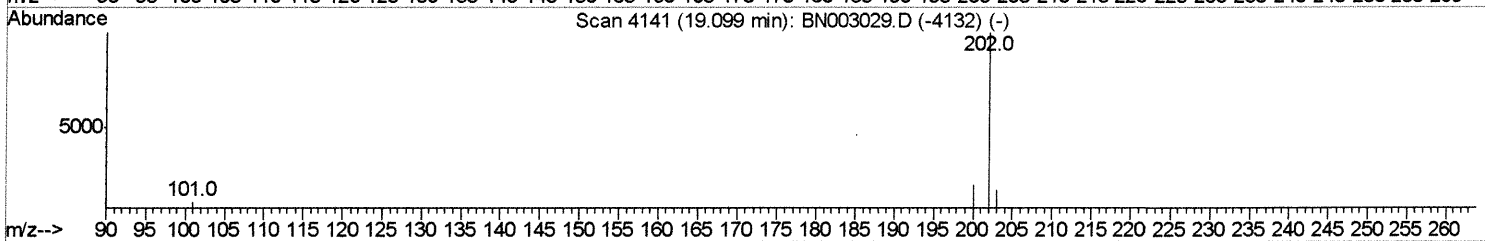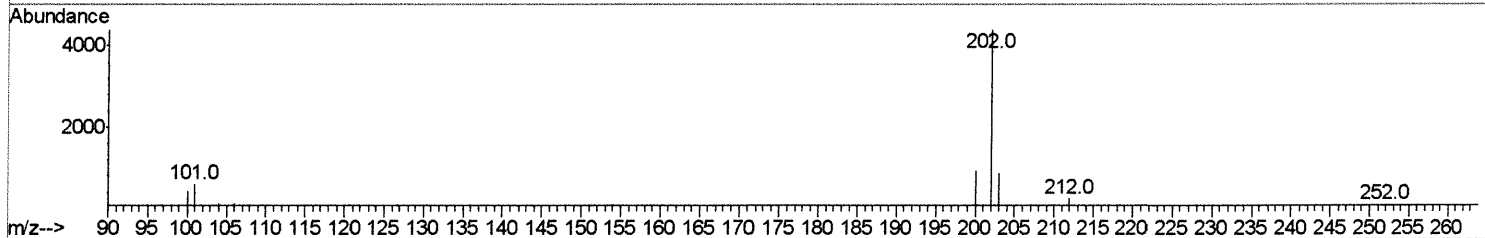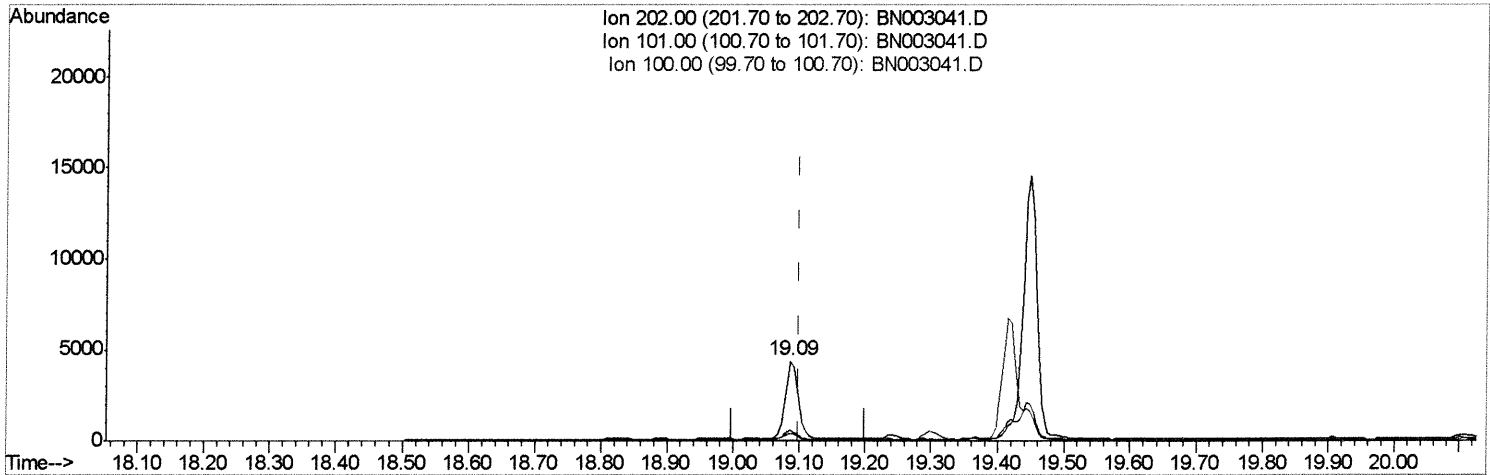

TIC: BN003041.D

(15) Fluoranthene (C)

19.085min (-0.014) 0.20ng/ul m

SG 10/12/18

response 6033

Ion	Exp%	Act%
202.00	100	100
101.00	12.30	13.44
100.00	9.10	9.80
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003041.D
 Acq On : 09 Oct 2018 23:37
 Operator : MJ/SJ
 Sample : J5157-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD3

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:52 PM

Quant Time: Oct 10 02:22:51 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

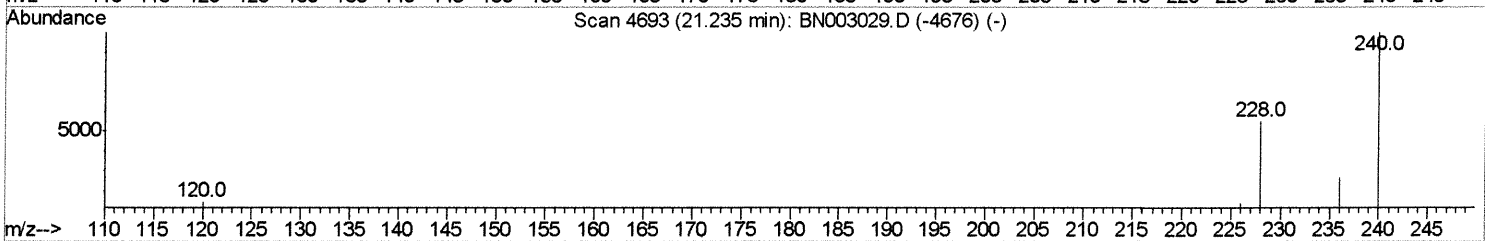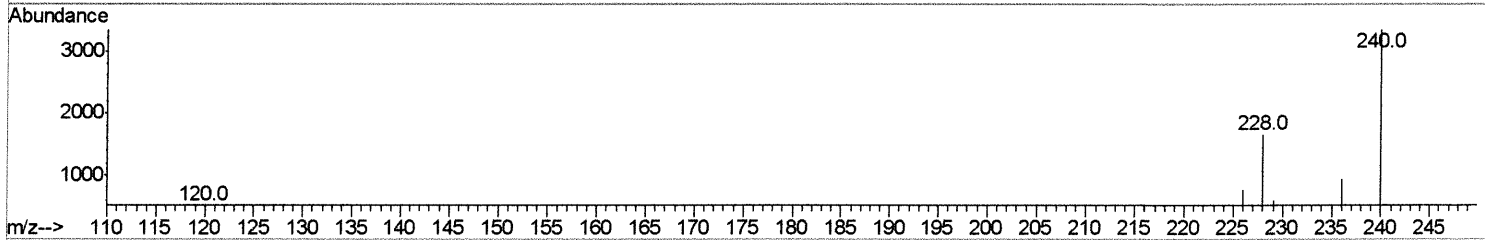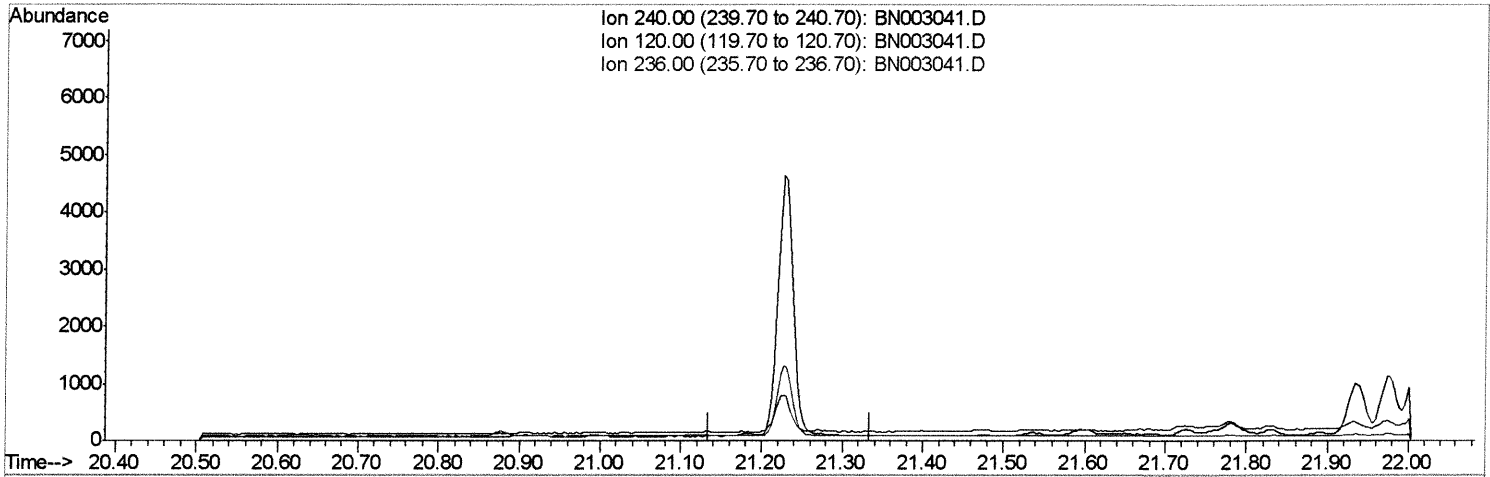

(16) Chrysene-d12 (I)

21.235min (-21.235) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	16.40	0.00#
236.00	28.10	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003041.D
 Acq On : 09 Oct 2018 23:37
 Operator : MJ/SJ
 Sample : J5157-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD3

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:52 PM

Quant Time: Oct 10 02:22:51 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

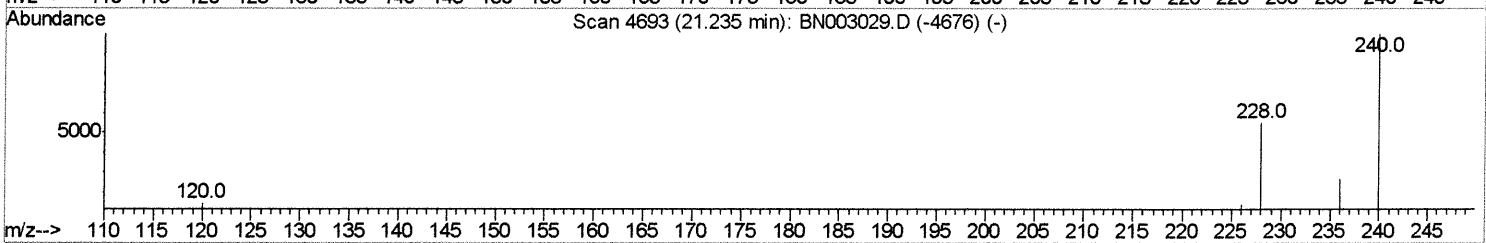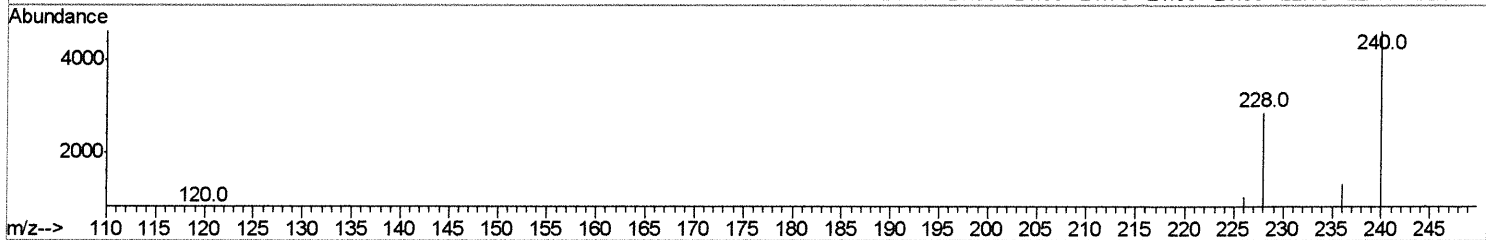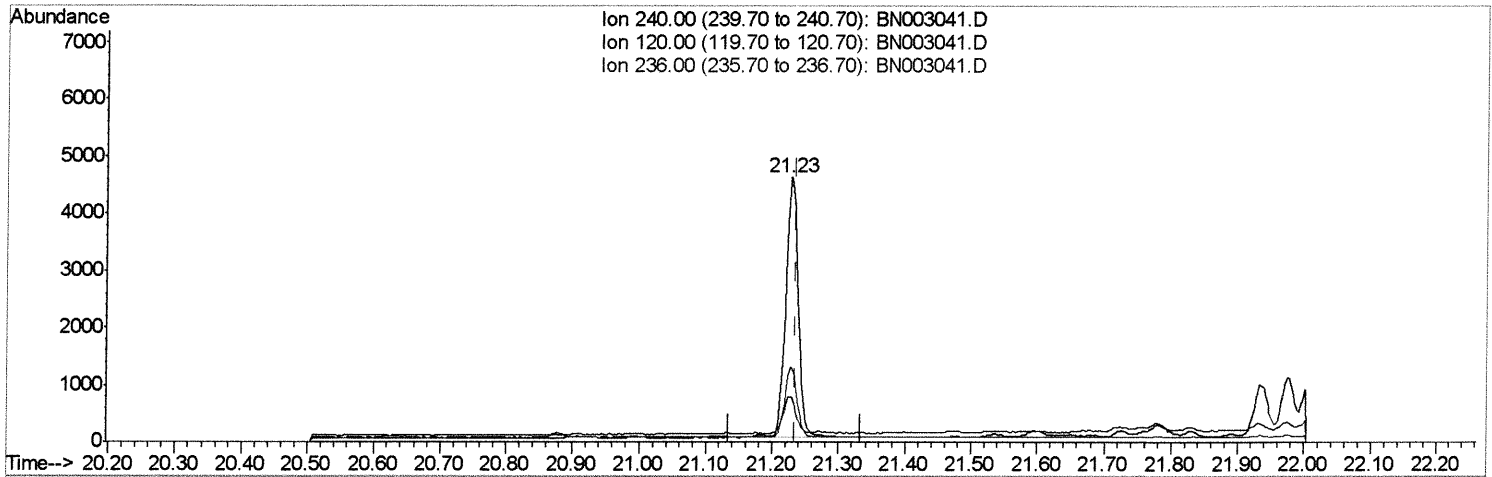

TIC: BN003041.D

(16) Chrysene-d12 (I)

21.226min (-0.009) 0.40ng/ul m

response 5885

Ion	Exp%	Act%
240.00	100	100
120.00	16.40	17.49
236.00	28.10	28.42
0.00	0.00	0.00

SJ 10/12/18

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003041.D
Acq On : 09 Oct 2018 23:37
Operator : MJ/SJ
Sample : J5157-11
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD3

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:52 PM

Quant Time: Oct 10 02:24:25 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

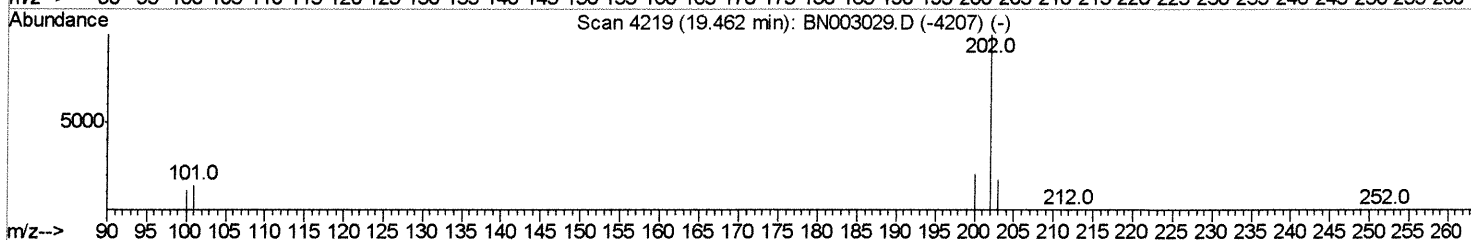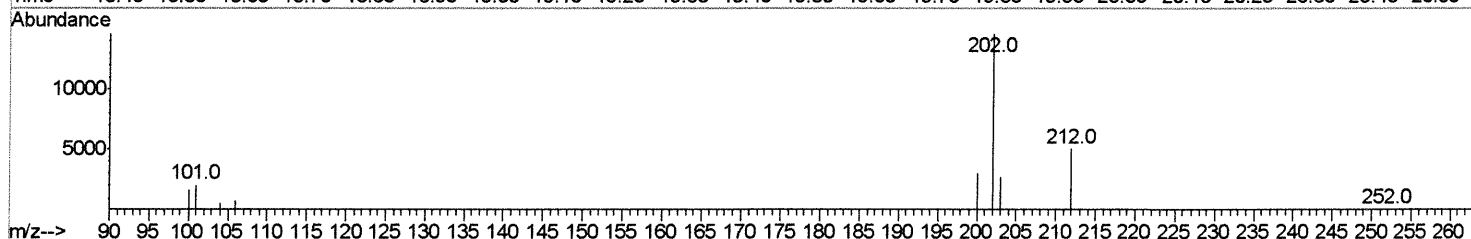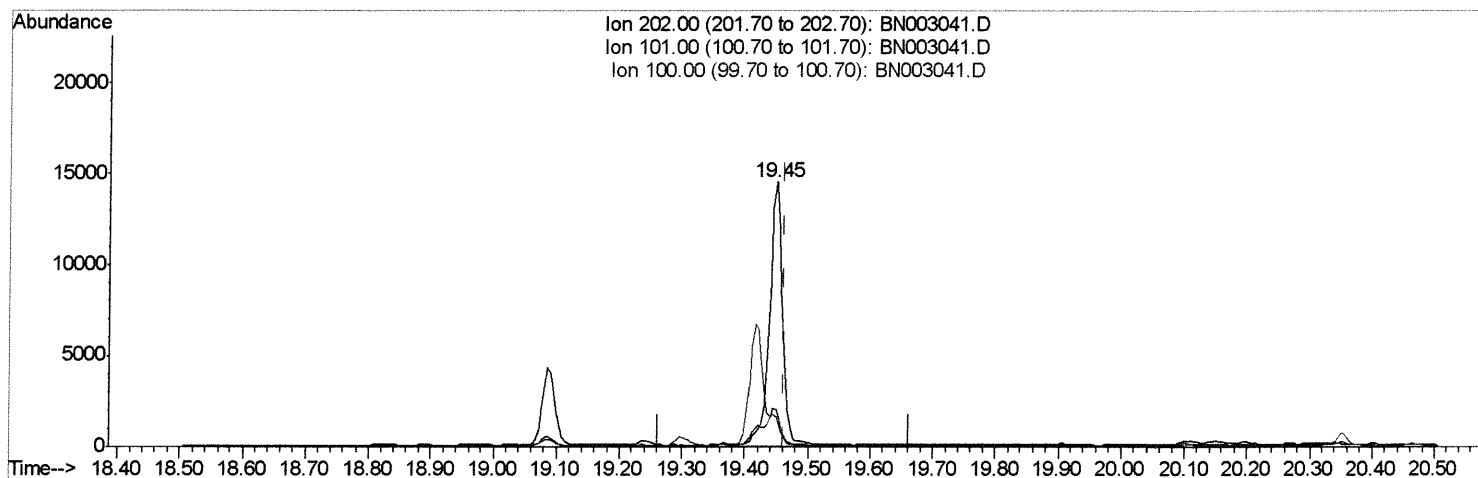

TIC: BN003041.D

(17) Pyrene

19.448min (-0.014) 0.92ng/ul

response 21137

Ion	Exp%	Act%
202.00	100	100
101.00	14.90	14.13
100.00	12.40	11.58
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003041.D
Acq On : 09 Oct 2018 23:37
Operator : MJ/SJ
Sample : J5157-11
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD3

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:52 PM

Quant Time: Oct 10 02:24:25 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

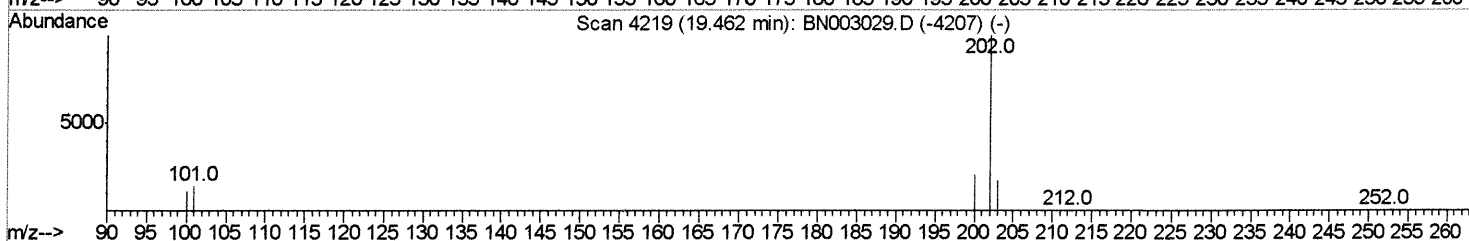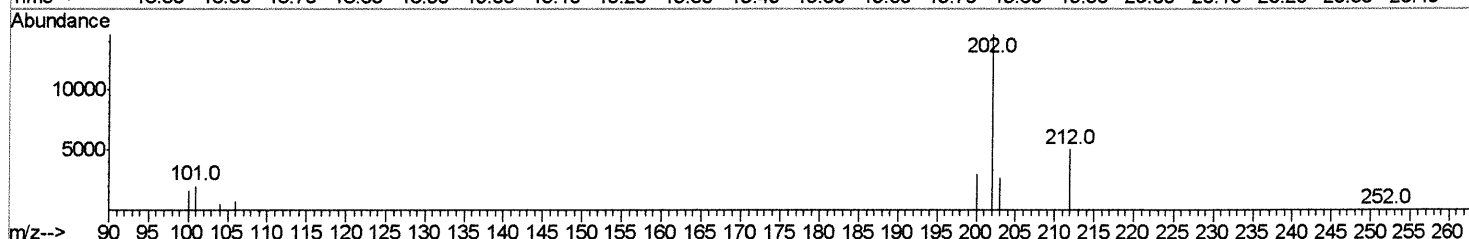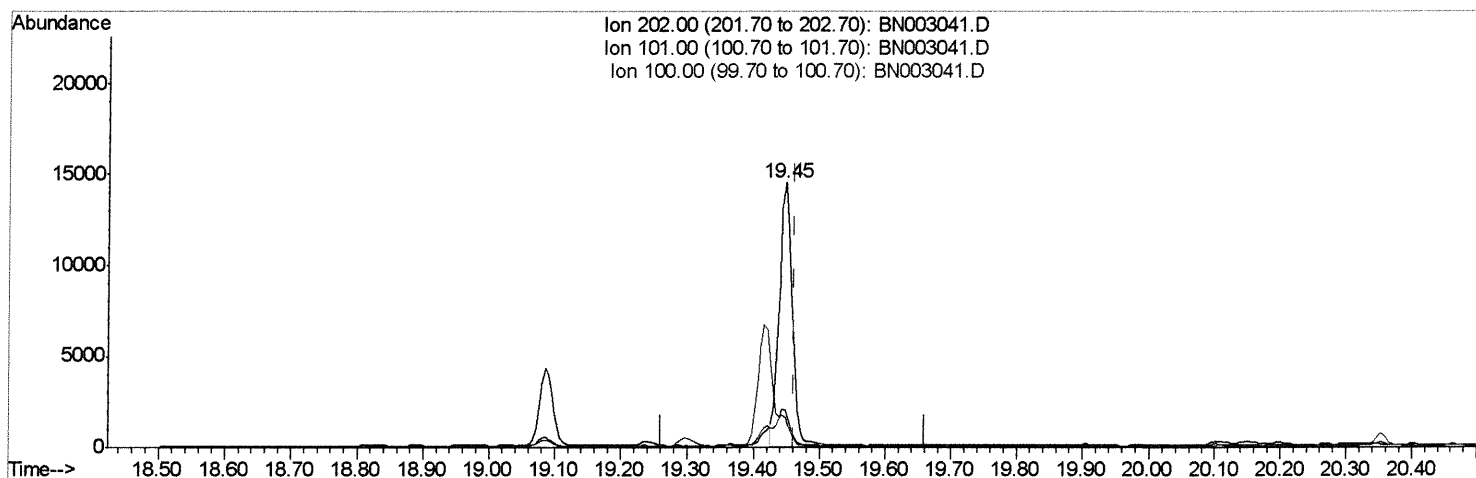

TIC: BN003041.D

(17) Pyrene

19.448min (-0.014) 0.88ng/ul m

SD 10/12/18

response 20156

Ion	Exp%	Act%
202.00	100	100
101.00	14.90	14.13
100.00	12.40	11.58
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003041.D
 Acq On : 09 Oct 2018 23:37
 Operator : MJ/SJ
 Sample : J5157-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD3

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:52 PM

Quant Time: Oct 10 02:24:25 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

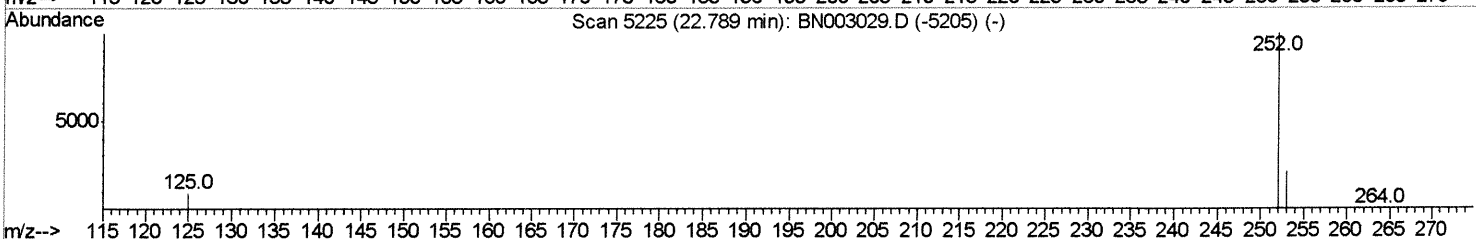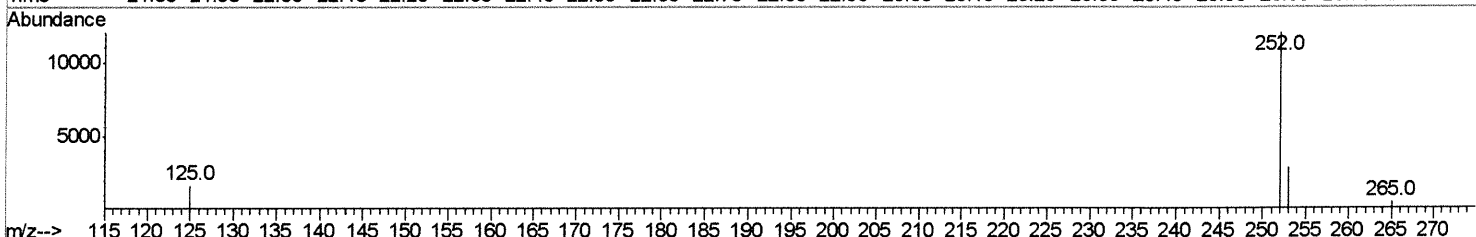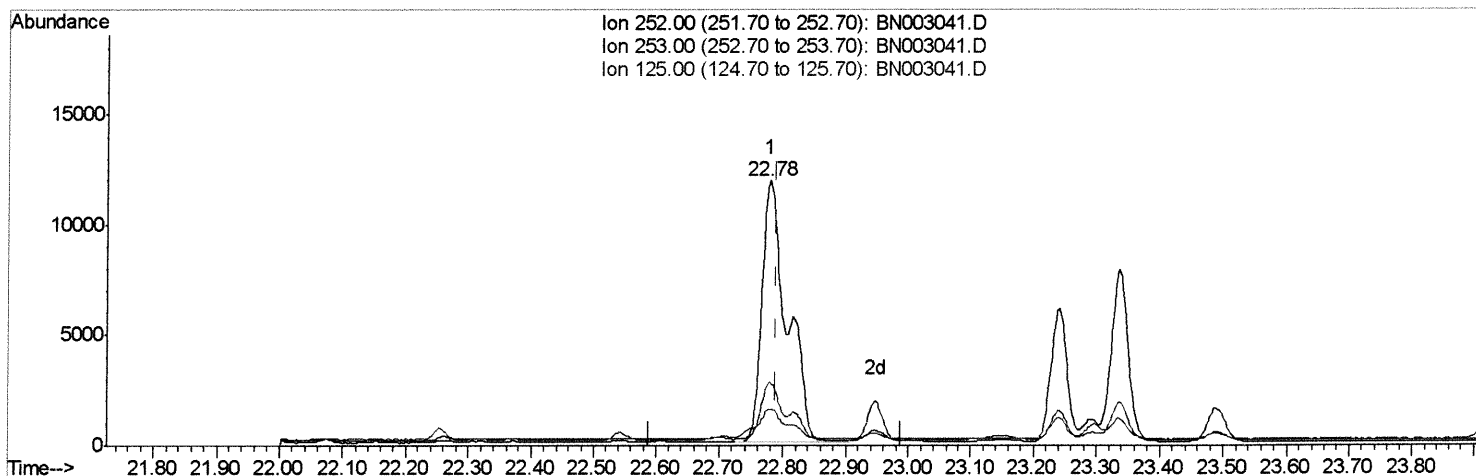

(21) Benzo(b)fluoranthene
 22.778min (-0.012) 1.41ng/ul
 response 32858

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	24.07
125.00	17.10	13.70
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003041.D
 Acq On : 09 Oct 2018 23:37
 Operator : MJ/SJ
 Sample : J5157-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD3

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:52 PM

Quant Time: Oct 10 02:24:25 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

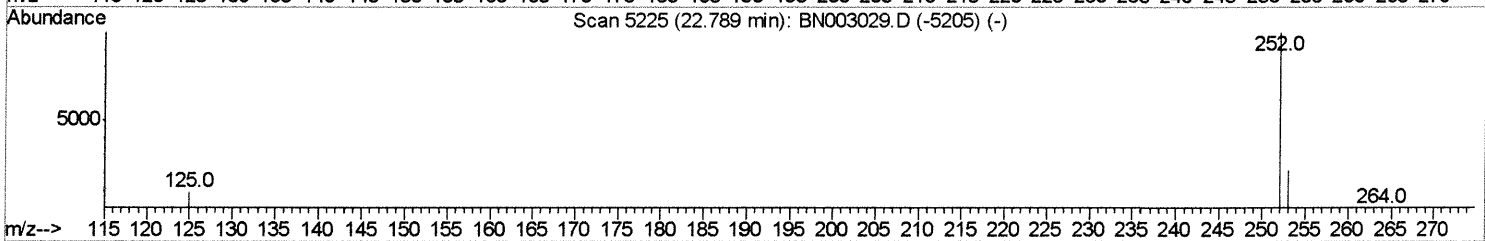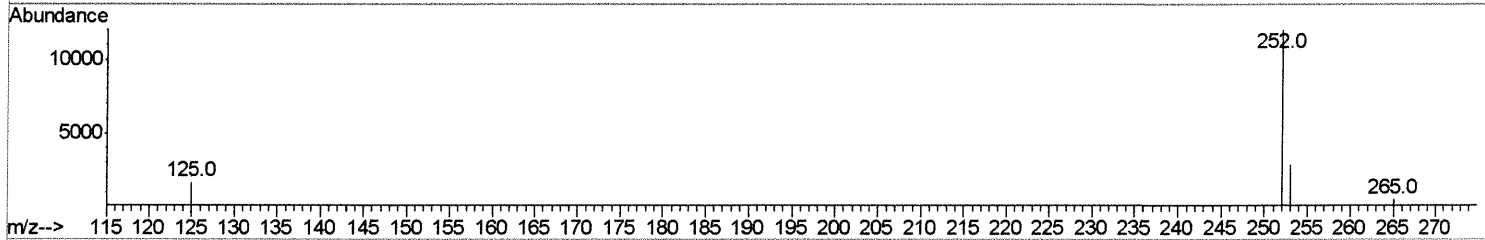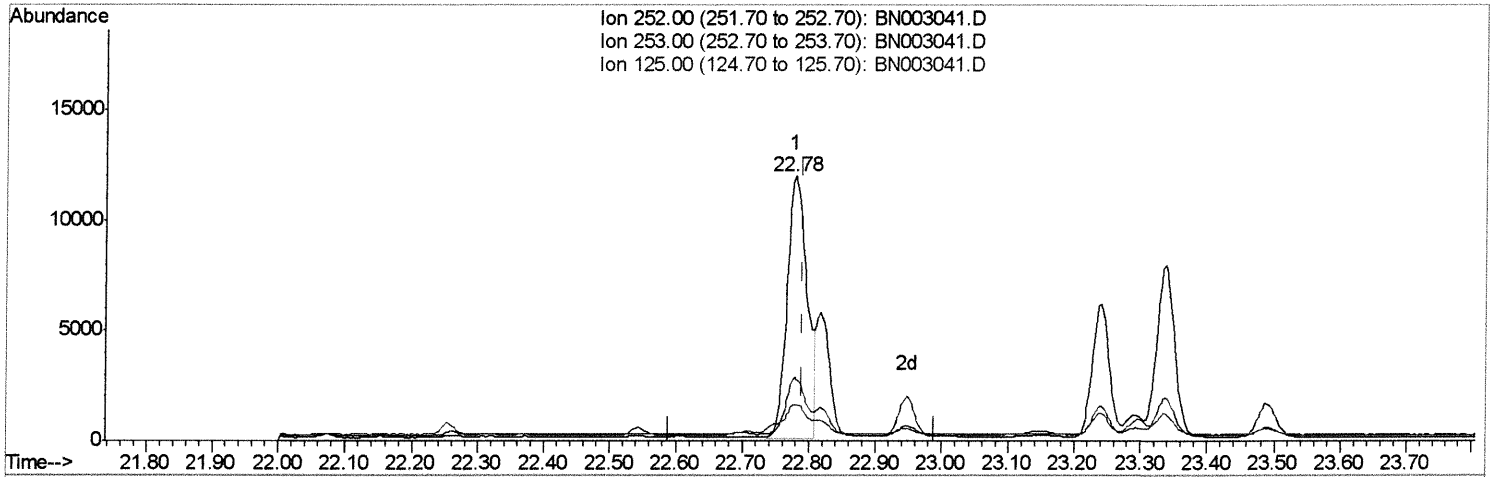

TIC: BN003041.D

(21) Benzo(b)fluoranthene

22.778min (-0.012) 1.06ng/ul m

5/10/12/18

response 24768

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	24.07
125.00	17.10	13.70
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003041.D
 Acq On : 09 Oct 2018 23:37
 Operator : MJ/SJ
 Sample : J5157-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD3

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:52 PM

Quant Time: Oct 10 02:24:25 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

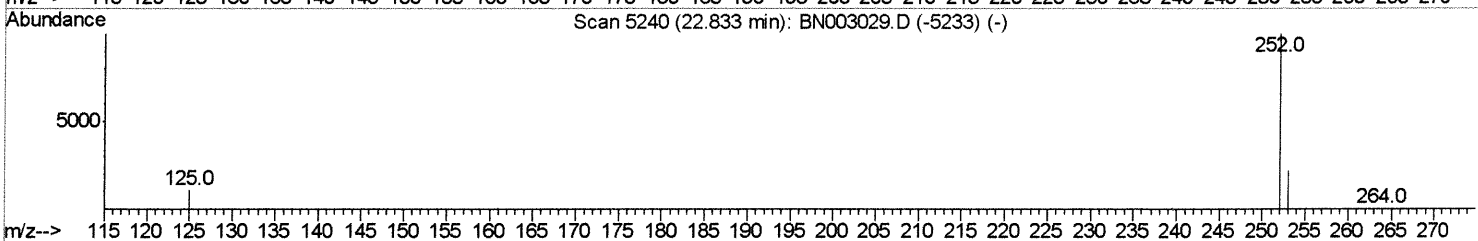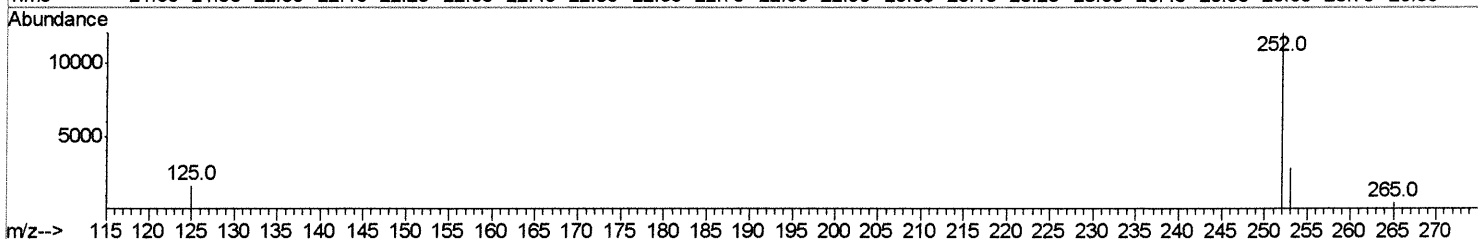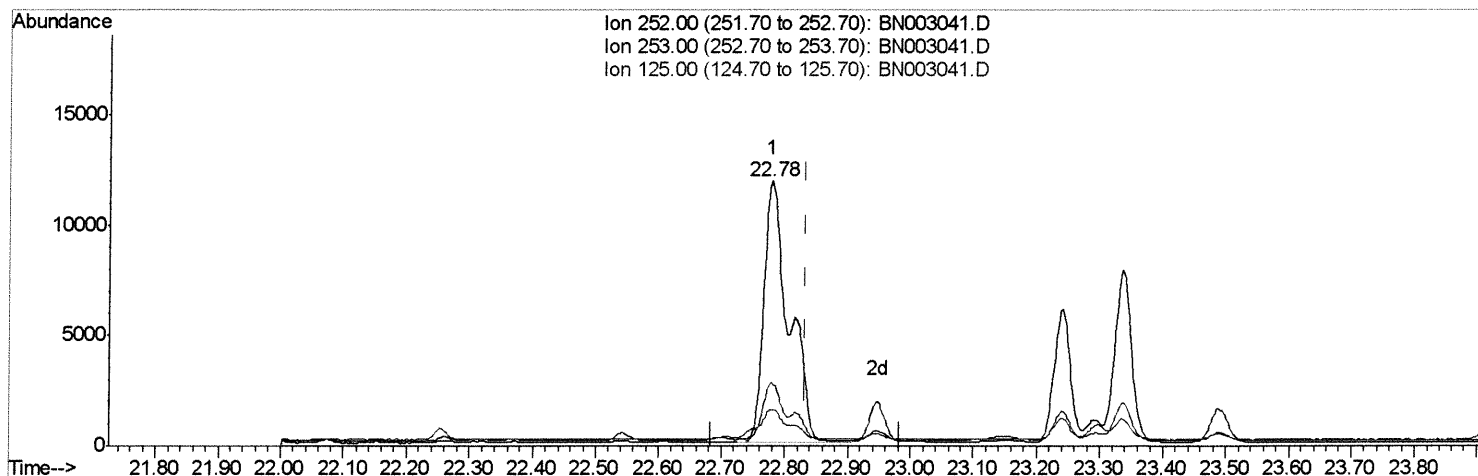

TIC: BN003041.D

(22) Benzo(k)fluoranthene
 22.778min (-0.056) 1.36ng/ul
 response 32858

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	24.07
125.00	17.60	13.70#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003041.D
 Acq On : 09 Oct 2018 23:37
 Operator : MJ/SJ
 Sample : J5157-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD3

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:52 PM

Quant Time: Oct 10 02:24:25 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

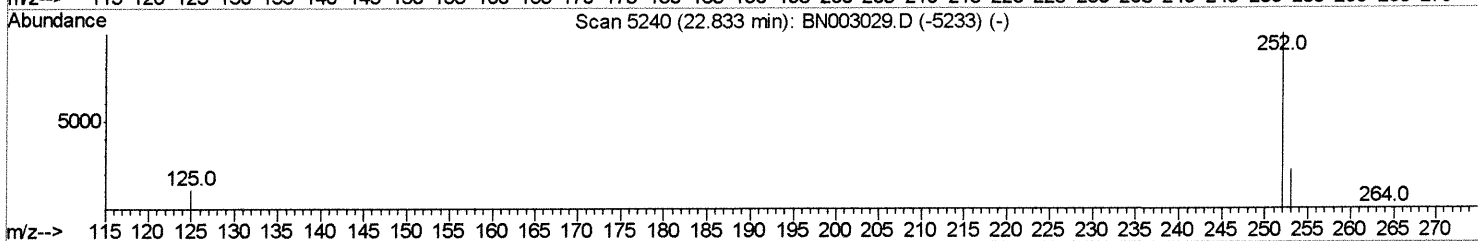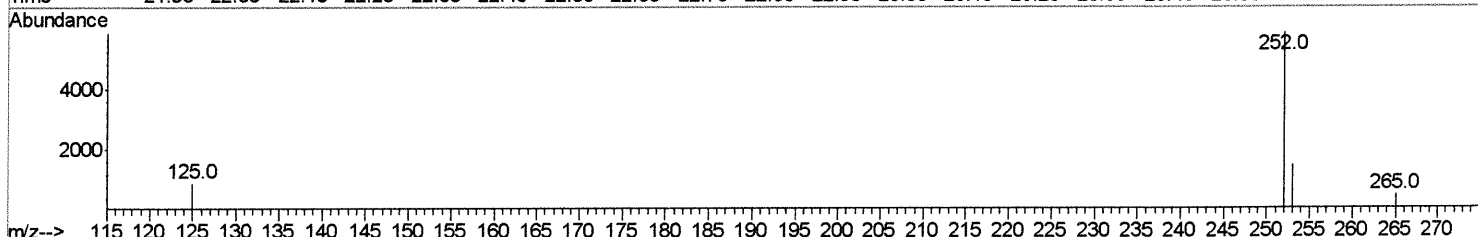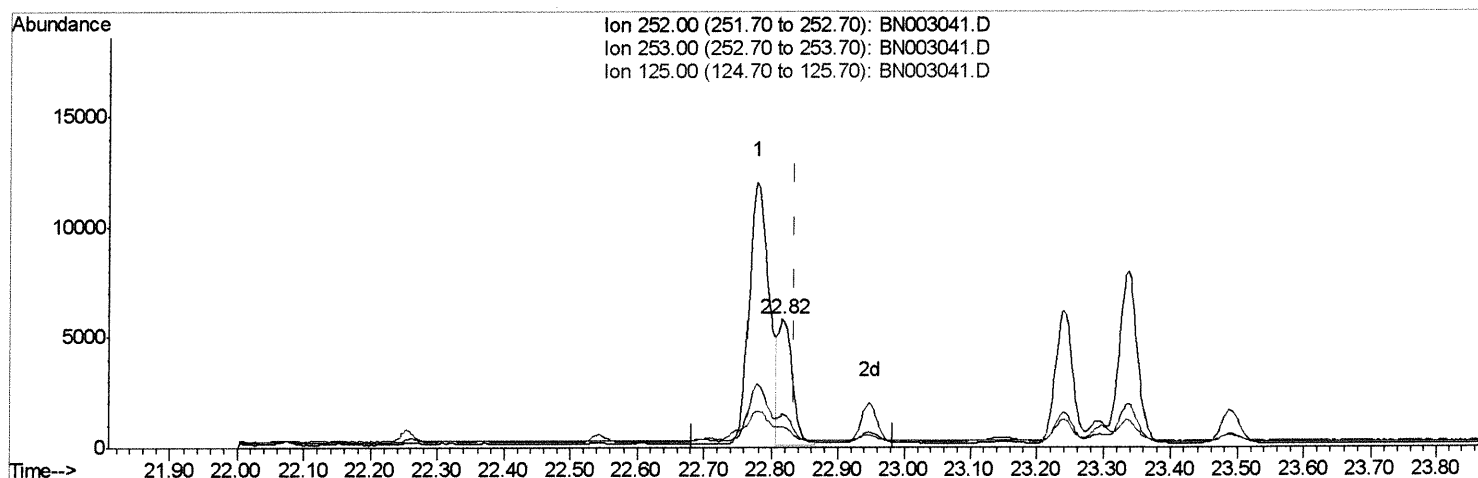

TIC: BN003041.D

(22) Benzo(k)fluoranthene

22.816min (-0.018) 0.34ng/ul m

5/10/12/18

response 8324

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	25.81
125.00	17.60	15.88
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003041.D
 Acq On : 09 Oct 2018 23:37
 Operator : MJ/SJ
 Sample : J5157-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD3

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:52 PM

Quant Time: Oct 10 02:25:33 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	1939	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.39	136	8093	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.26	164	4683	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.02	188	9365m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.23	240	5885m	0.40	ng/ul	0.00
20) Perylene-d12	23.44	264	6471	0.40	ng/ul	-0.01

Svstem Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methvl naphthalene-d10	12.01	152	5244	0.42	ng/ul	-0.02
14) Fluoranthene-d10	19.06	212	10256m	0.38	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
3) Naphthalene	10.44	128	2804	0.135	ng/ul	98
5) 2-Methvl naphthalene	12.08	142	315	0.022	ng/ul	99
7) Acenaphthylene	13.98	152	1632	0.076	ng/ul#	89
9) Fluorene	15.32	166	509	0.027	ng/ul#	92
12) Phenanthrene	17.06	178	2659m	0.102	ng/ul	} SJ 10/12/18
13) Anthracene	17.15	178	3477m	0.141	ng/ul	
15) Fluoranthene	19.09	202	6033m	0.197	ng/ul	
17) Pyrene	19.45	202	20156m	0.882	ng/ul	} SJ 10/12/18
18) Benzo(a)anthracene	21.21	228	10398	0.549	ng/ul	
19) Chrysene	21.26	228	13589	0.707	ng/ul	99
21) Benzo(b)fluoranthene	22.78	252	24768m	1.063	ng/ul	> SJ 10/12/18
22) Benzo(k)fluoranthene	22.82	252	8324m	0.345	ng/ul	
23) Benzo(a)pyrene	23.34	252	14877	0.712	ng/ul#	90
24) Indeno(1,2,3-cd)pyrene	25.66	276	7173	0.299	ng/ul#	93
25) Dibenzo(a,h)anthracene	25.66	278	2134	0.111	ng/ul#	74
26) Benzo(g,h,i)perylene	26.33	276	5926	0.293	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed