

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003042.D
 Acq On : 10 Oct 2018 00:12
 Operator : MJ/SJ
 Sample : J5157-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD4

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:53 PM

Quant Time: Oct 10 02:29:44 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

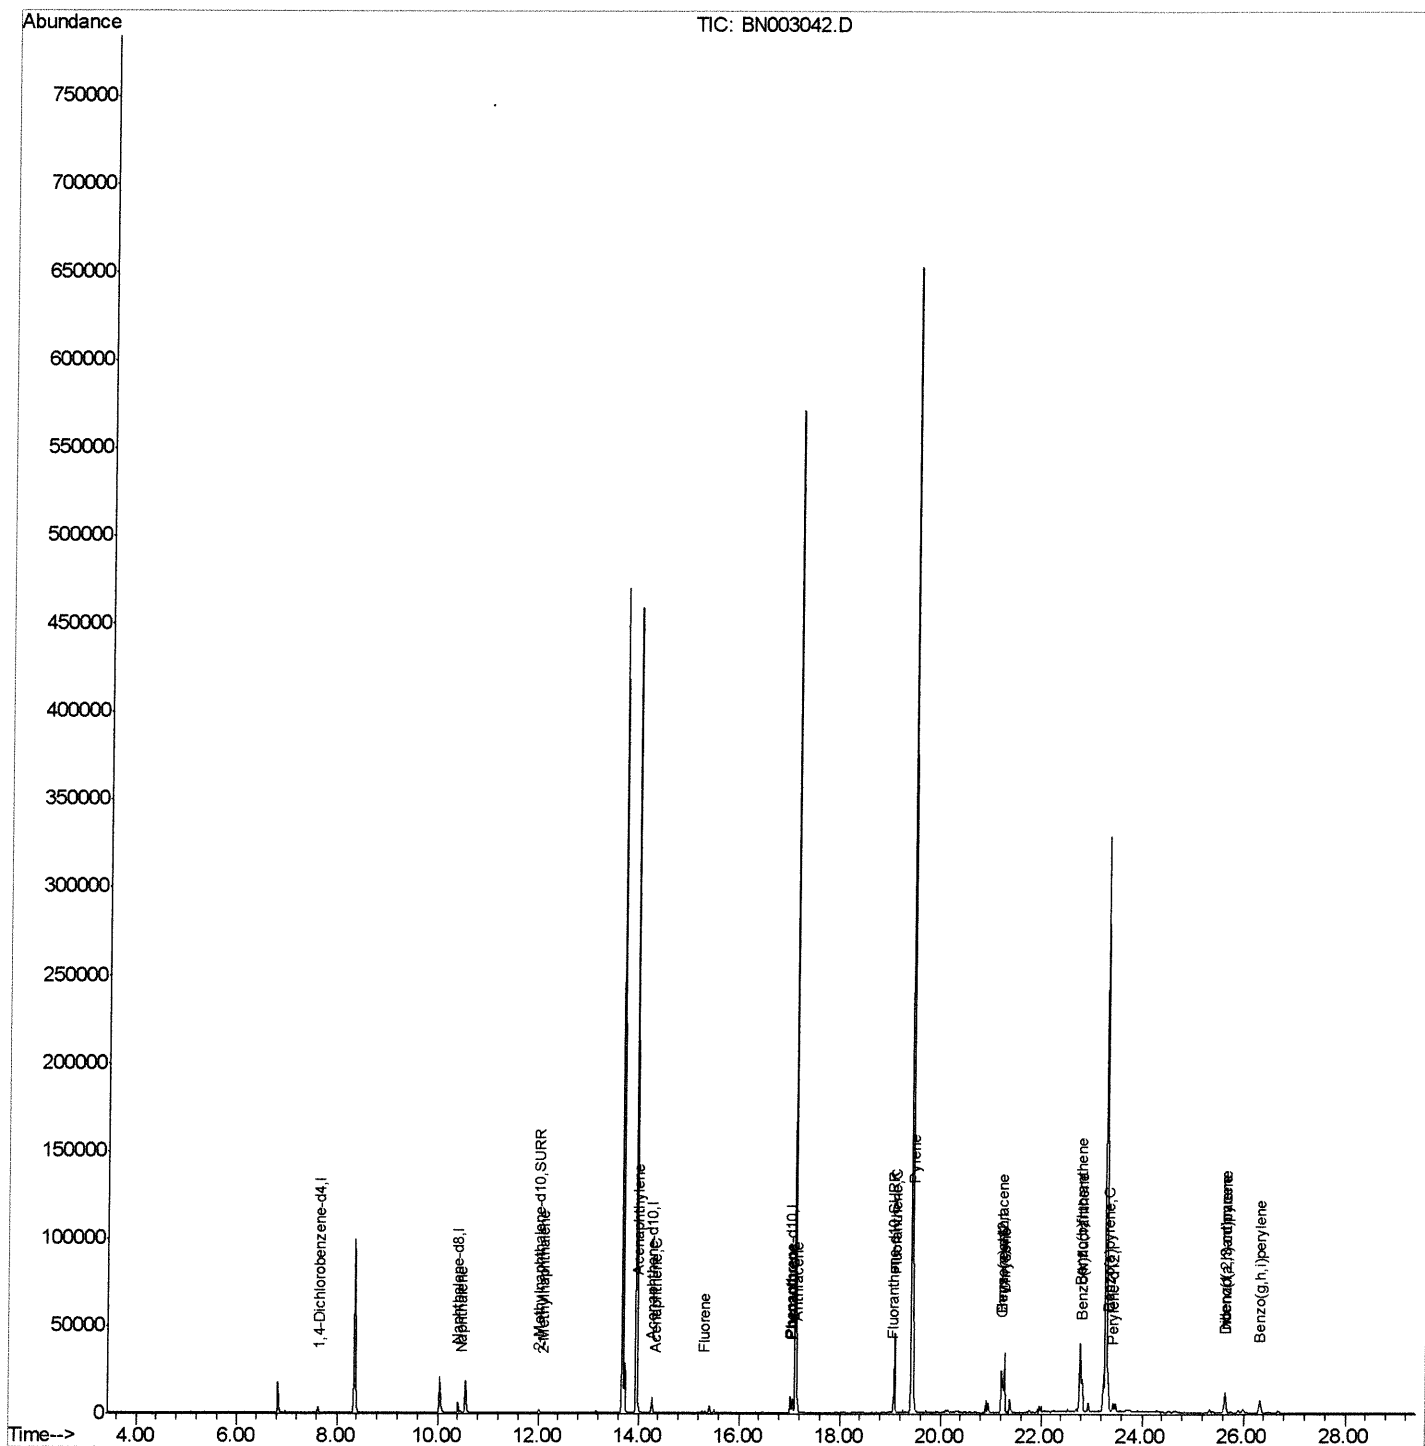

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003042.D
Acq On : 10 Oct 2018 00:12
Operator : MJ/SJ
Sample : J5157-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD4

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:53 PM

Quant Time: Oct 10 01:38:27 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

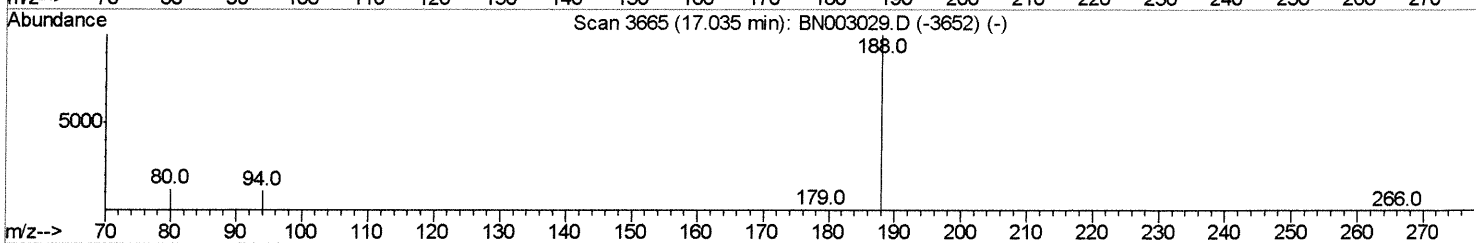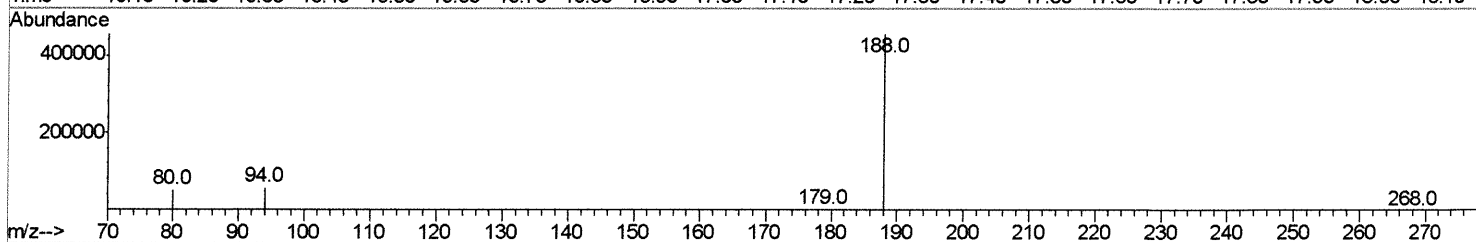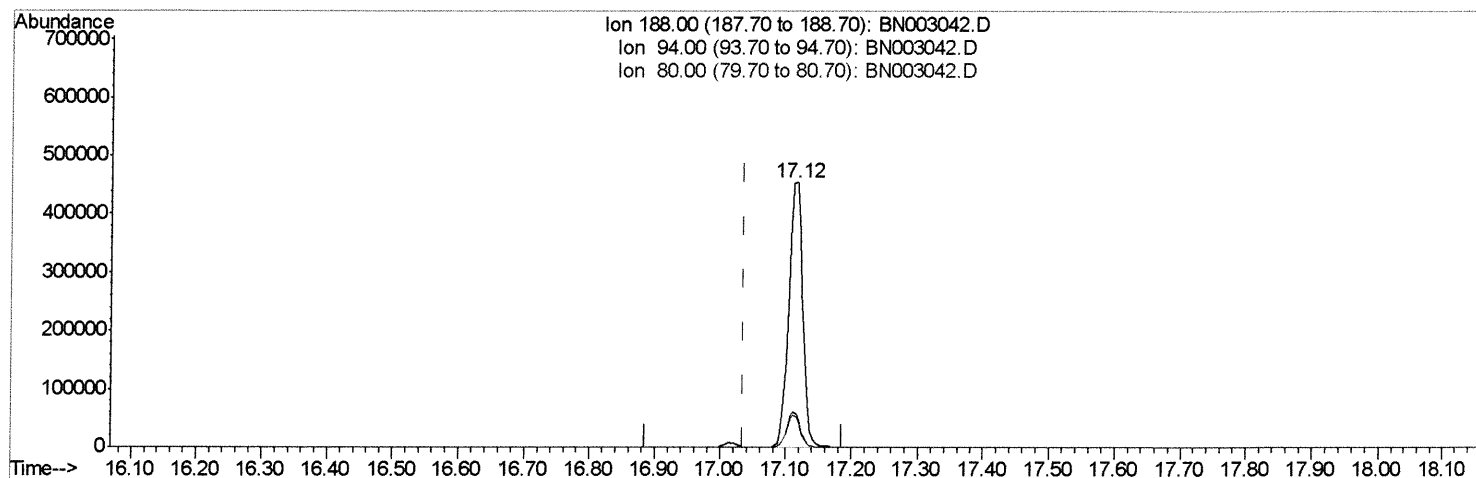

TIC: BN003042.D

(10) Phenanthrene-d10 (I)

17.115min (+0.080) 0.40ng/ul

response 671677

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	12.43
80.00	12.70	11.27
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003042.D
 Acq On : 10 Oct 2018 00:12
 Operator : MJ/SJ
 Sample : J5157-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD4

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:53 PM

Quant Time: Oct 10 01:38:27 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

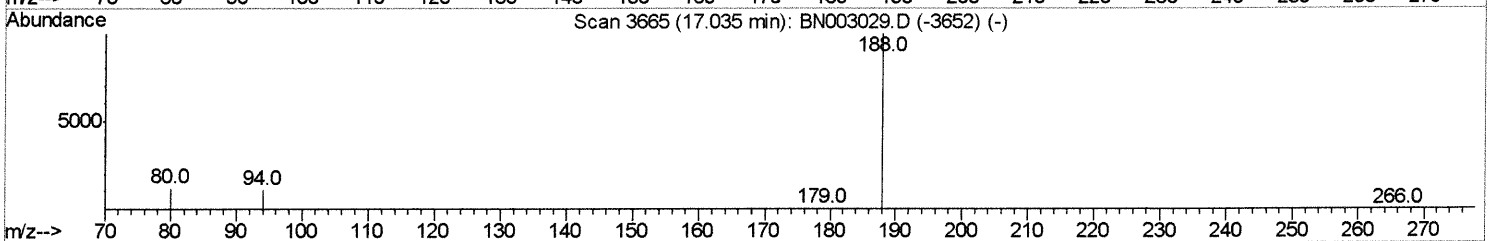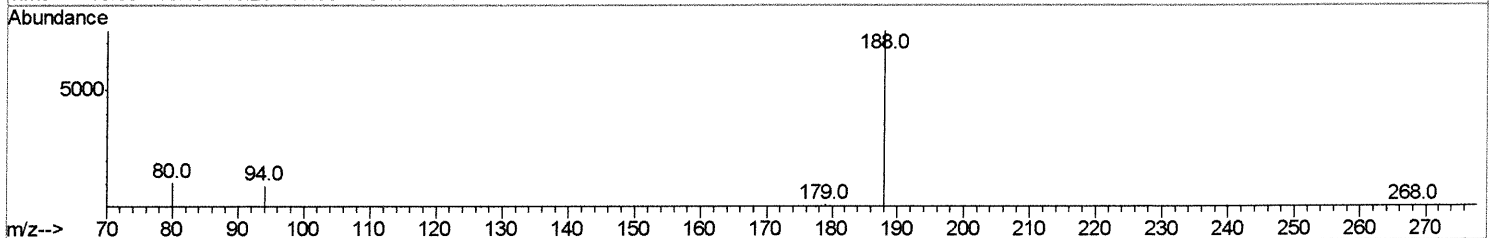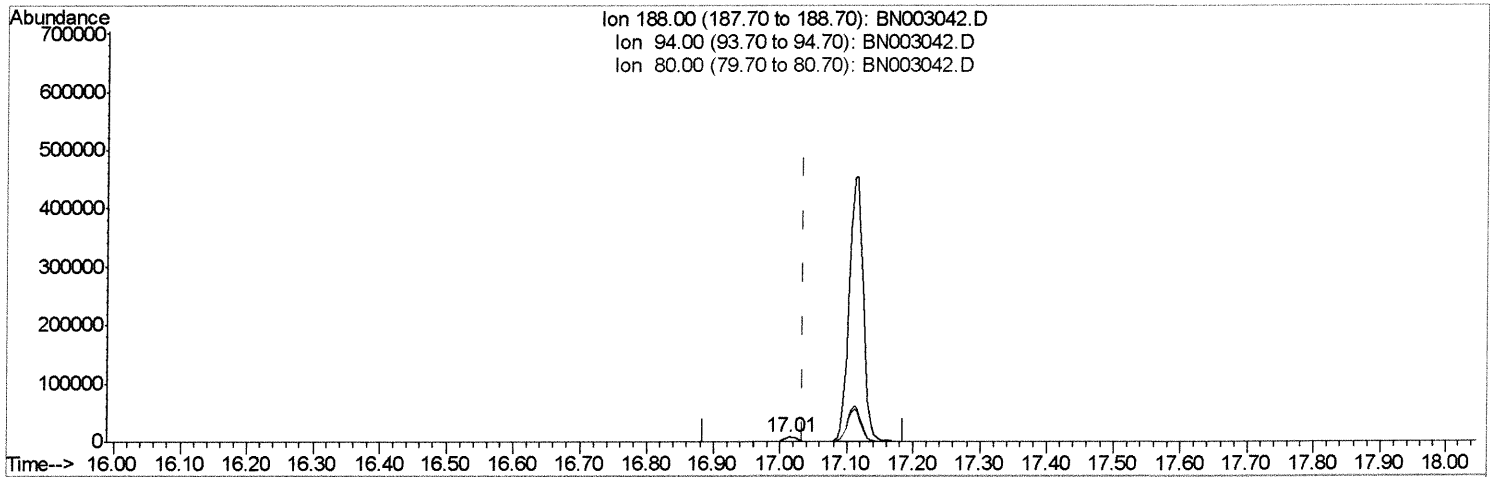

TIC: BN003042.D

(10) Phenanthrene-d10 (I)

17.014min (-0.021) 0.40ng/ul m

SJ 10/12/18

response 10533

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	12.53
80.00	12.70	14.15
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003042.D
 Acq On : 10 Oct 2018 00:12
 Operator : MJ/SJ
 Sample : J5157-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD4

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:53 PM

Quant Time: Oct 10 02:26:29 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

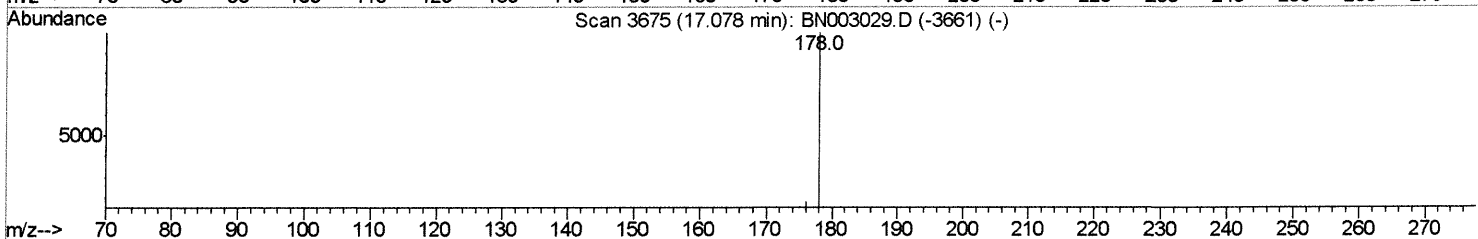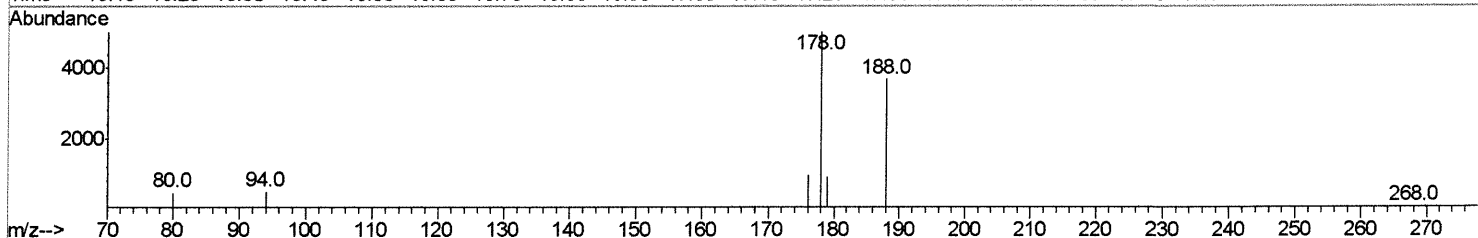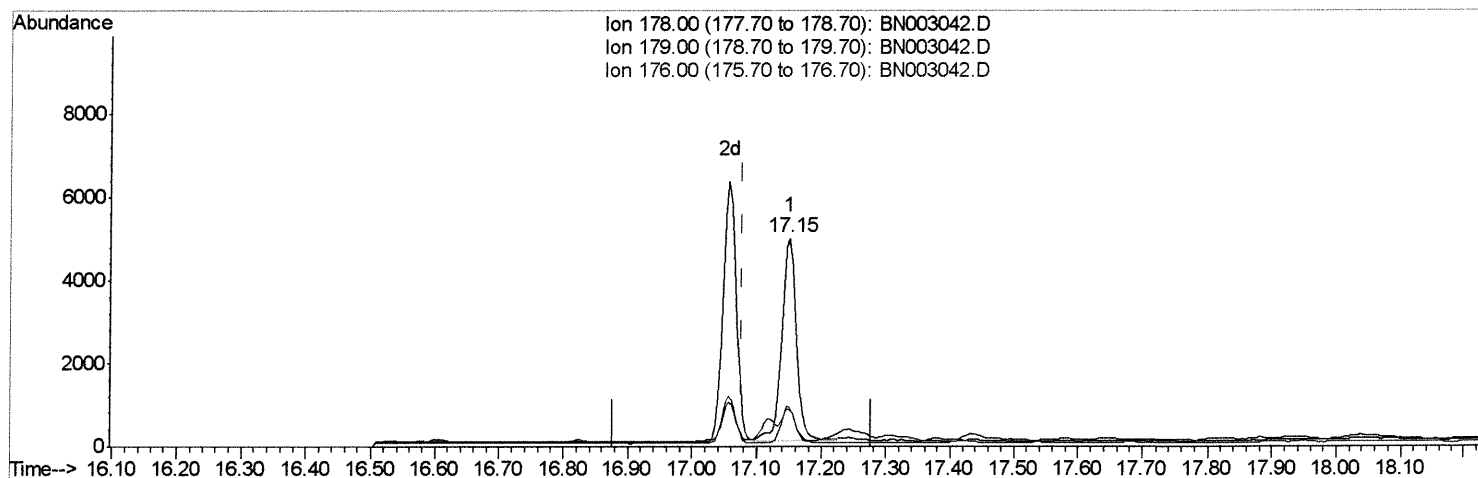

TIC: BN003042.D

(12) Phenanthrene

17.149min (+0.071) 0.26ng/ul

response 7612

Ion	Exp%	Act%
178.00	100	100
179.00	16.10	17.88
176.00	19.30	19.09
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003042.D
 Acq On : 10 Oct 2018 00:12
 Operator : MJ/SJ
 Sample : J5157-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD4

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:53 PM

Quant Time: Oct 10 02:26:29 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

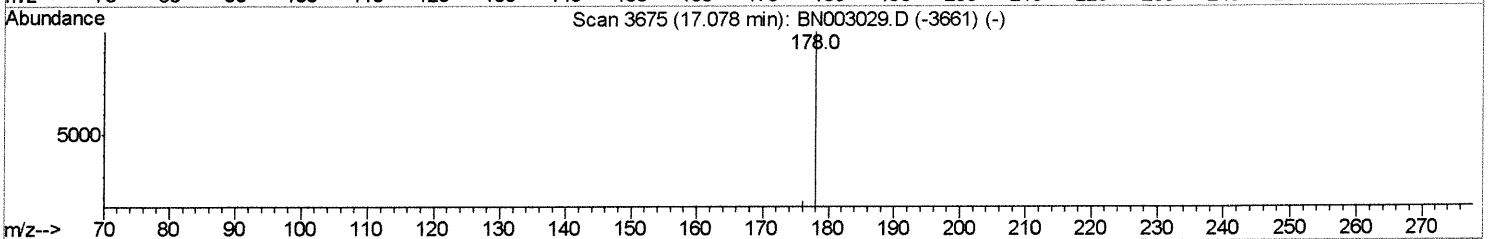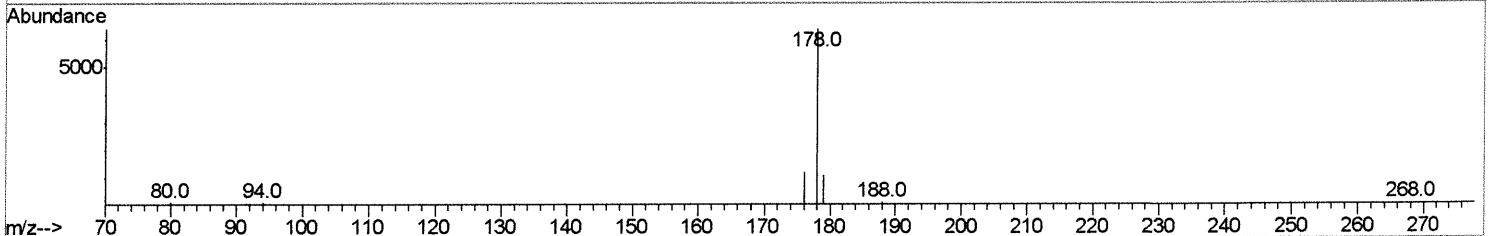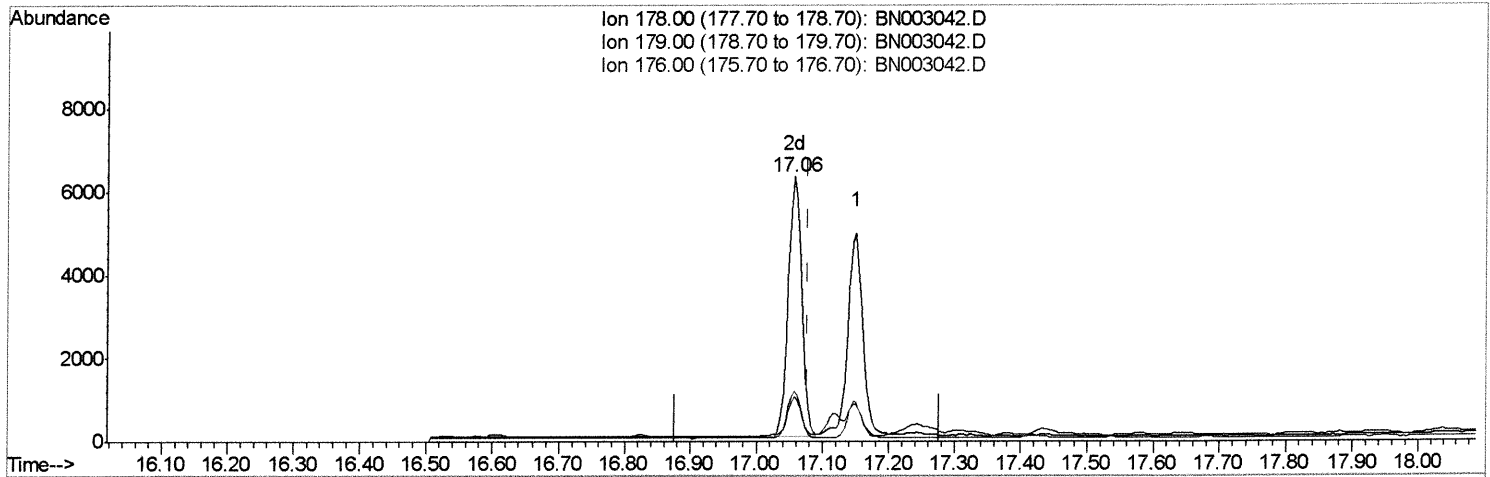

TIC: BN003042.D

(12) Phenanthrene

17.056min (-0.021) 0.30ng/ul m *3110/12/18*

response 8874

Ion	Exp%	Act%
178.00	100	100
179.00	16.10	17.05
176.00	19.30	19.09
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003042.D
 Acq On : 10 Oct 2018 00:12
 Operator : MJ/SJ
 Sample : J5157-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD4

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:53 PM

Quant Time: Oct 10 02:26:29 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

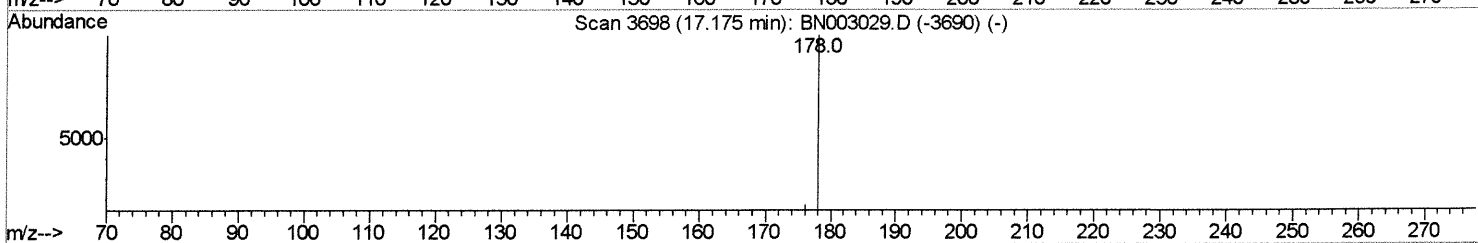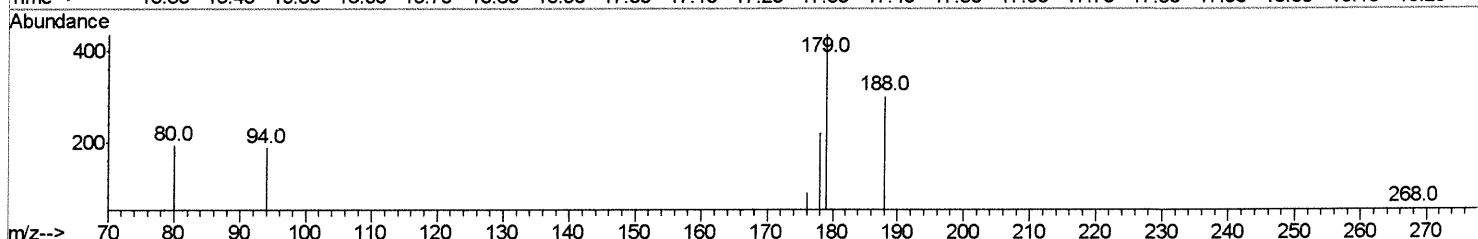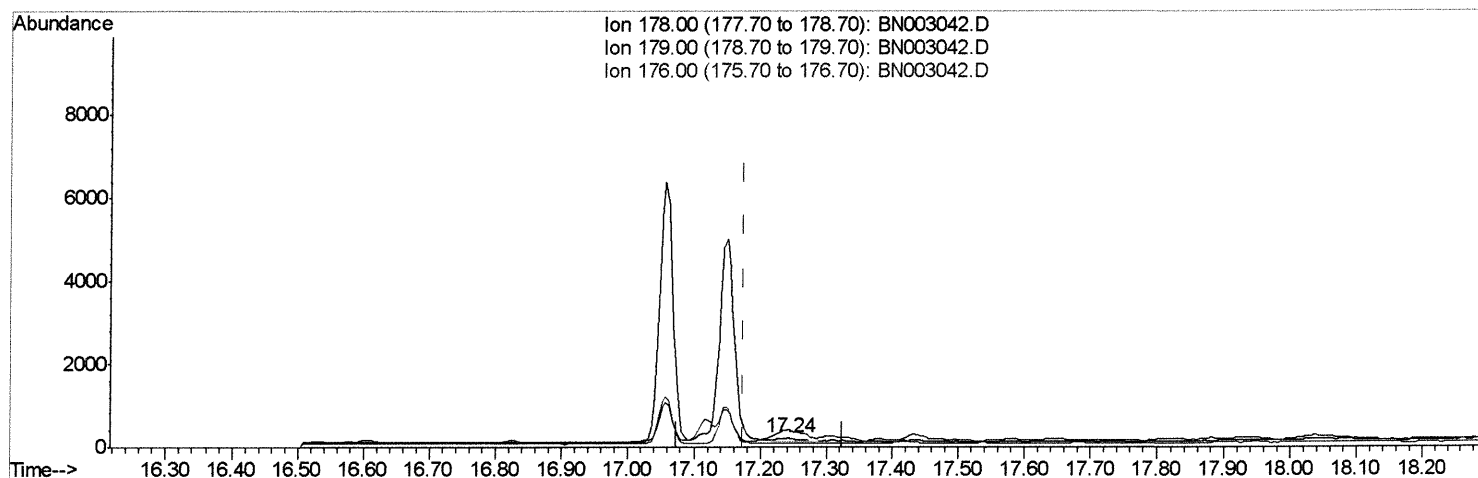

TIC: BN003042.D

(13) Anthracene

17.242min (+0.067) 0.01ng/ul

response 150

Ion	Exp%	Act%
178.00	100	100
179.00	16.30	198.19#
176.00	19.10	39.82#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003042.D
 Acq On : 10 Oct 2018 00:12
 Operator : MJ/SJ
 Sample : J5157-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD4

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:53 PM

Quant Time: Oct 10 02:26:29 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

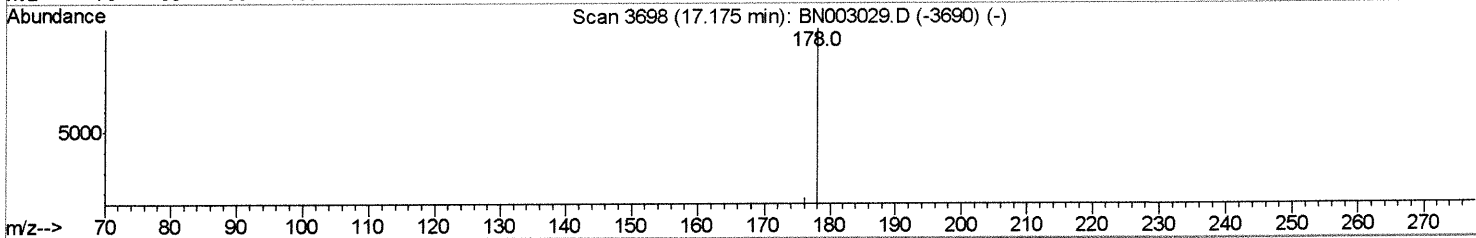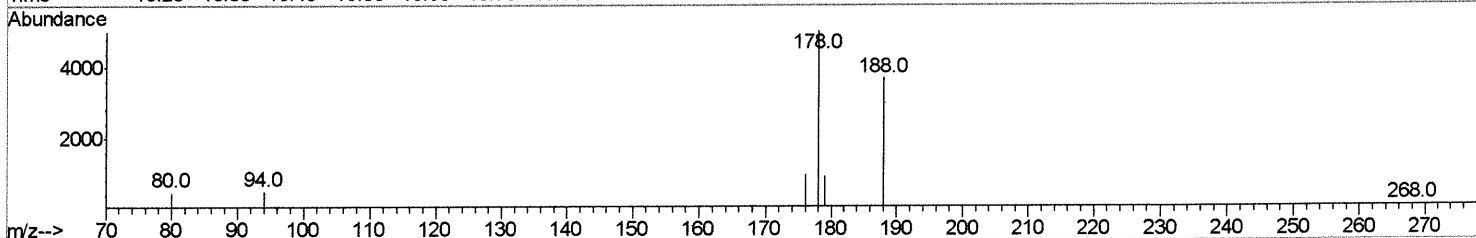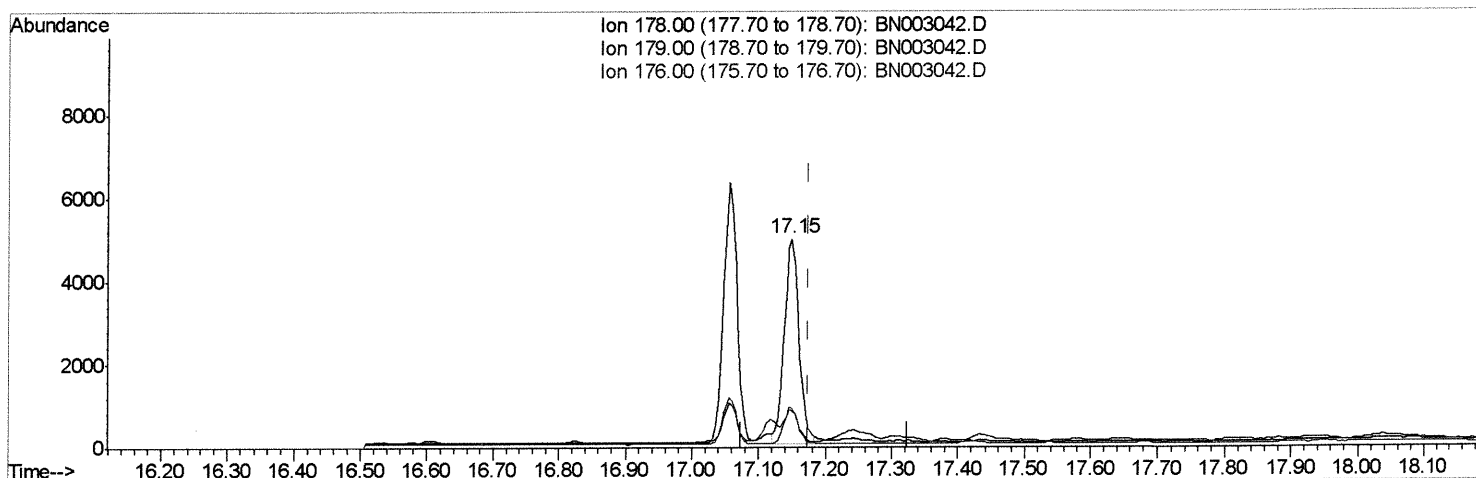

(13) Anthracene

17.149min (-0.026) 0.28ng/ul m *57 10/12/18*

response 7652

Ion	Exp%	Act%
178.00	100	100
179.00	16.30	17.88
176.00	19.10	19.09
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003042.D
 Acq On : 10 Oct 2018 00:12
 Operator : MJ/SJ
 Sample : J5157-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD4

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:53 PM

Quant Time: Oct 10 02:26:29 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

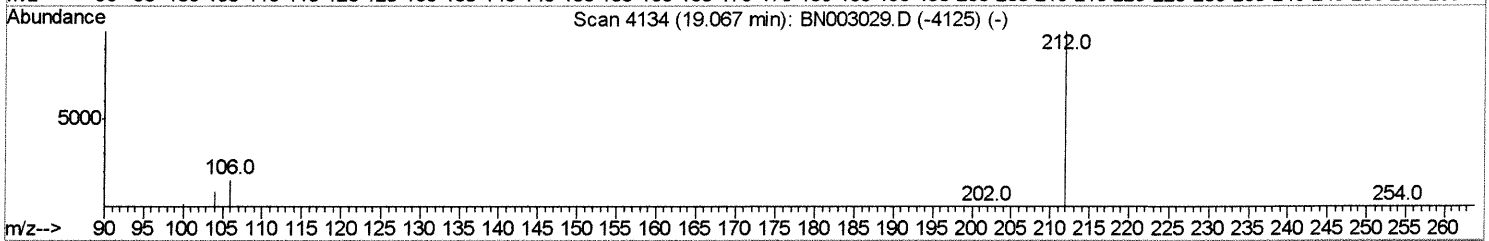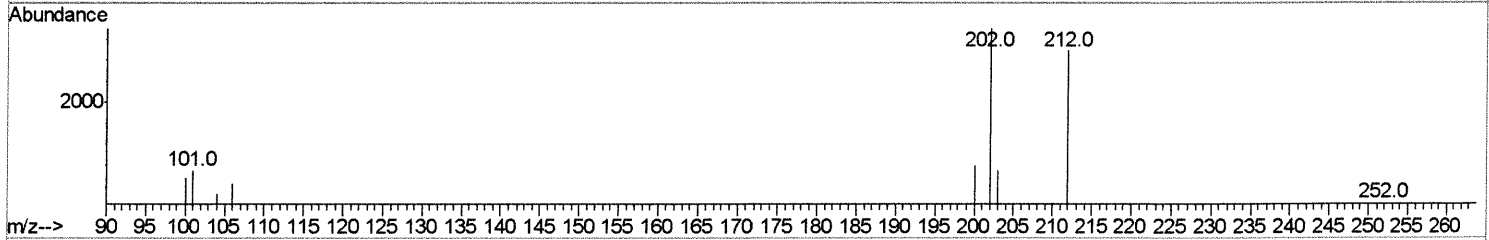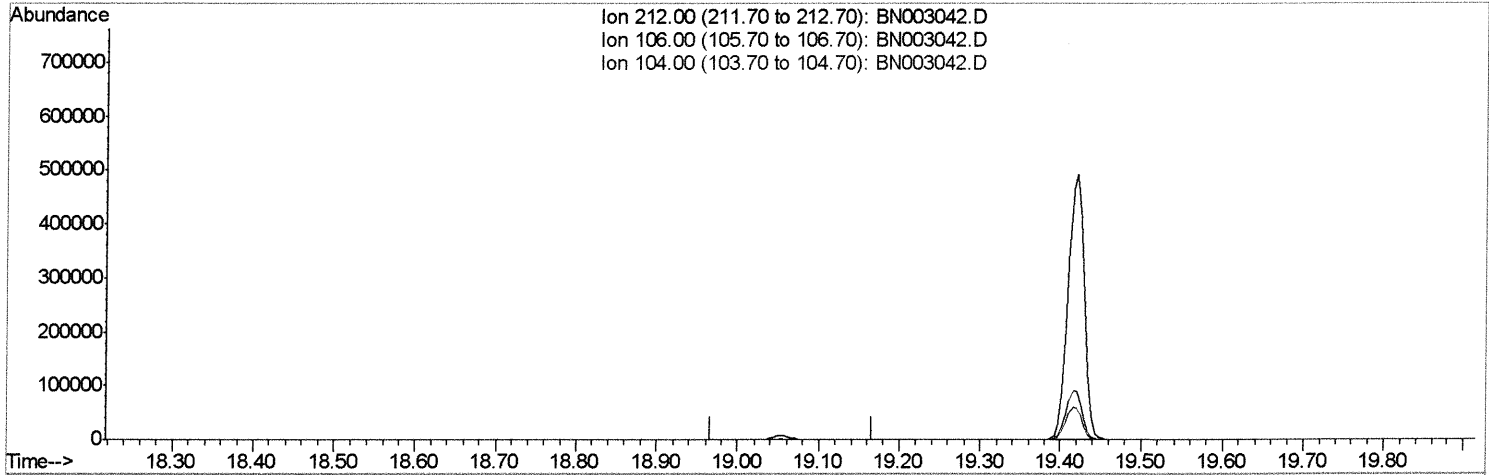

TIC: BN003042.D

(14) Fluoranthene-d10 (SURR)

19.067min (-19.067) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	15.40	0.00#
104.00	8.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003042.D
 Acq On : 10 Oct 2018 00:12
 Operator : MJ/SJ
 Sample : J5157-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD4

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:53 PM

Quant Time: Oct 10 02:26:29 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

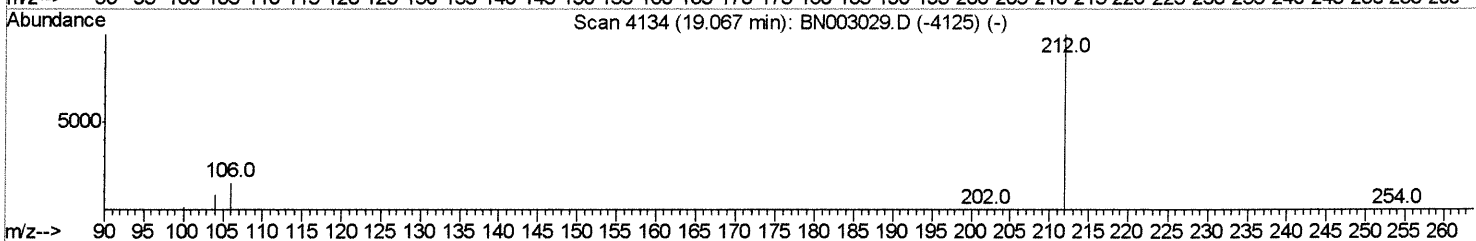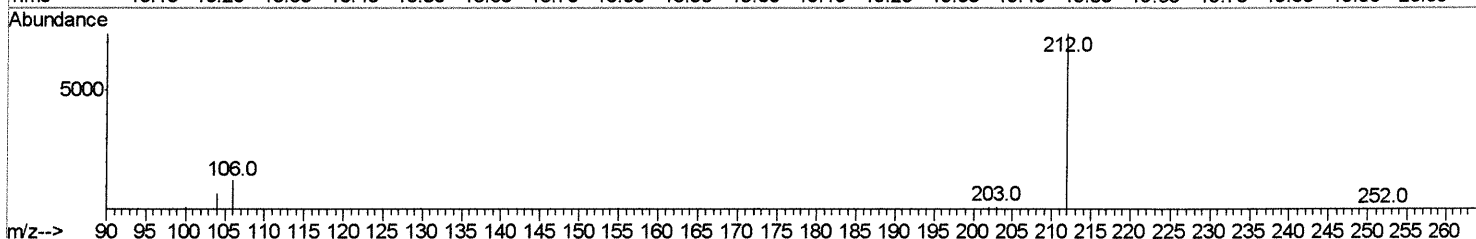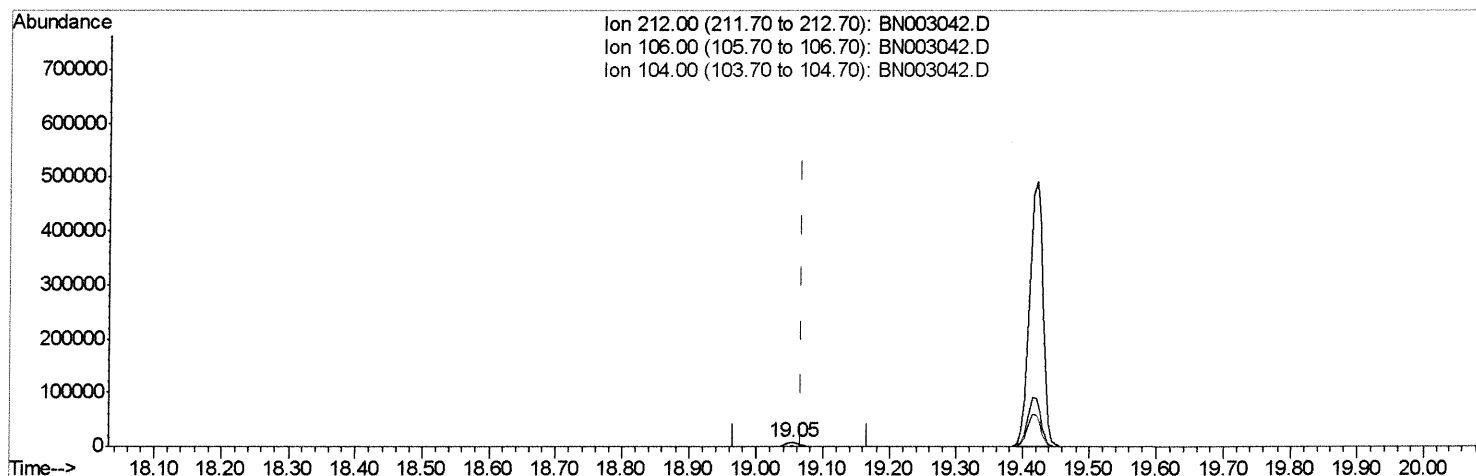

TIC: BN003042.D

(14) Fluoranthene-d10 (SURR)

19.053min (-0.014) 0.34ng/ul m

SJ 10/12/18

response 10269

Ion	Exp%	Act%
212.00	100	100
106.00	15.40	0.00#
104.00	8.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003042.D
 Acq On : 10 Oct 2018 00:12
 Operator : MJ/SJ
 Sample : J5157-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD4

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:53 PM

Quant Time: Oct 10 02:26:29 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

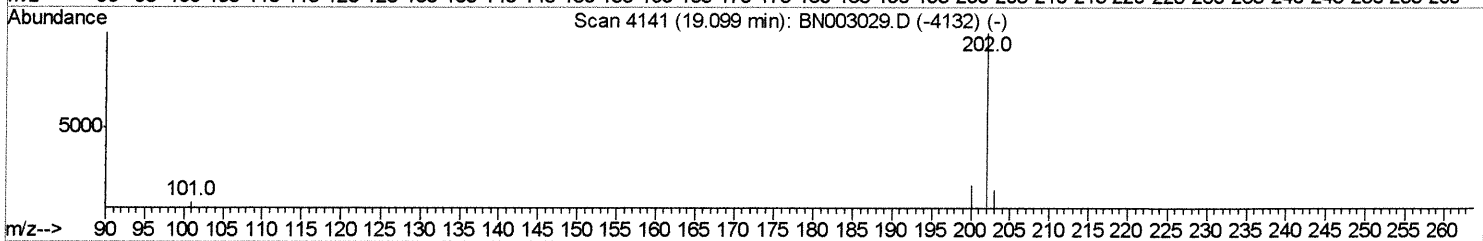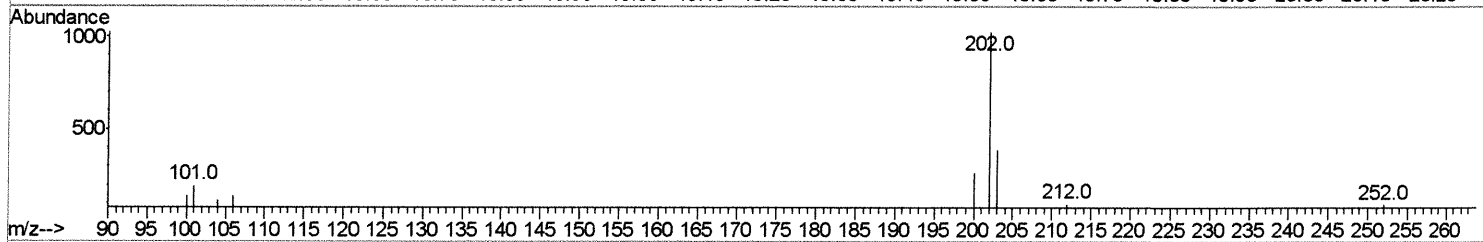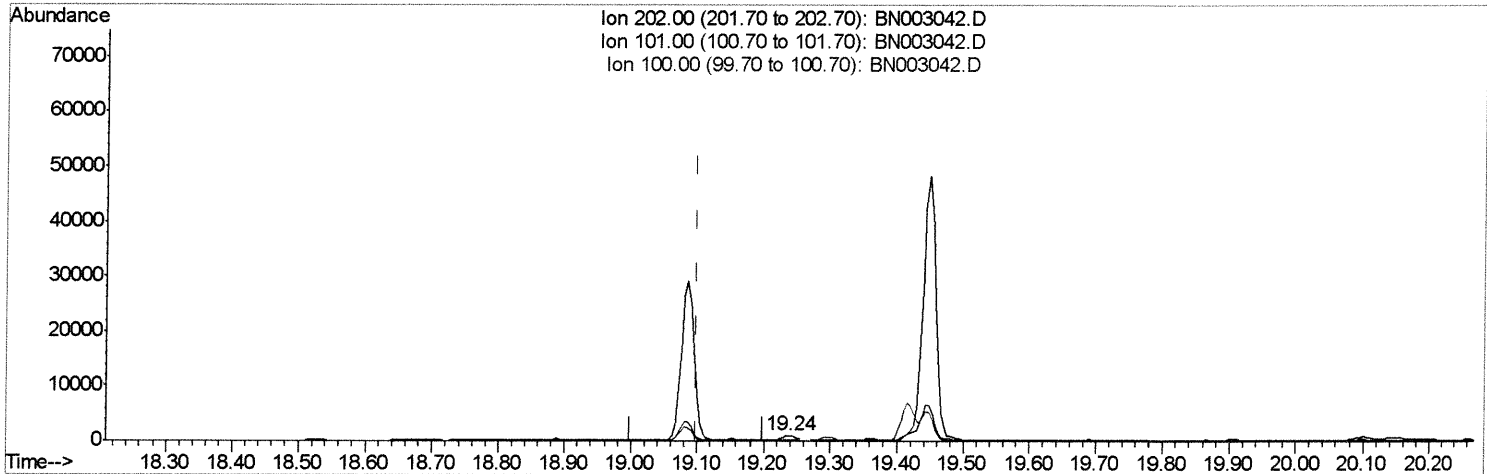

TIC: BN003042.D

(15) Fluoranthene (C)

19.238min (+0.139) 0.03ng/ui

response 1086

Ion	Exp%	Act%
202.00	100	100
101.00	12.30	18.87
100.00	9.10	13.88
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003042.D
 Acq On : 10 Oct 2018 00:12
 Operator : MJ/SJ
 Sample : J5157-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD4

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:53 PM

Quant Time: Oct 10 02:26:29 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

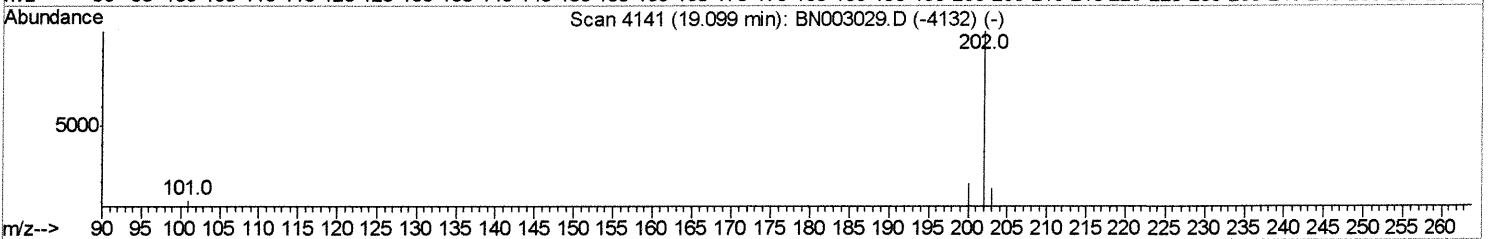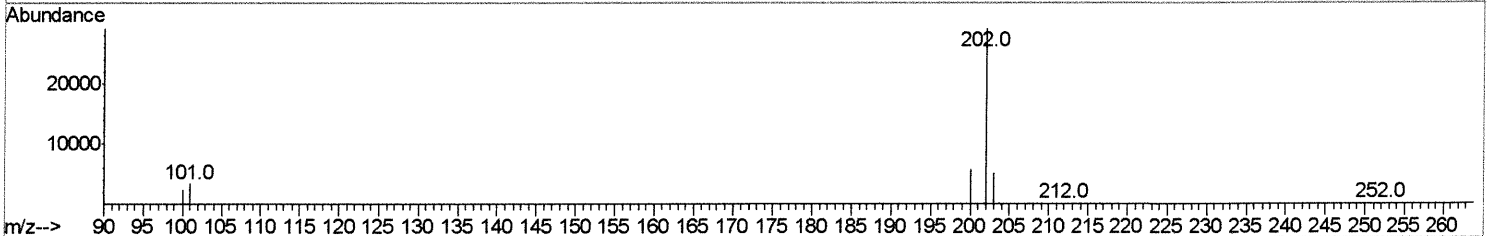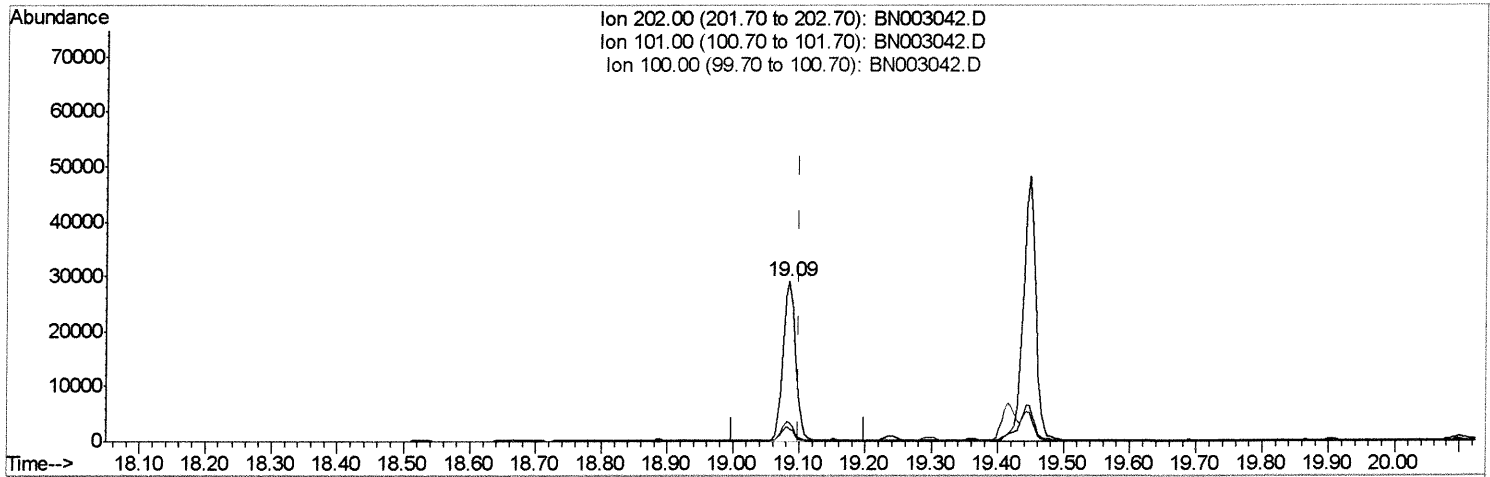

(15) Fluoranthene (C)

19.085min (-0.014) 1.13ng/ul m *SJ 10/12/18*

response 38990

Ion	Exp%	Act%
202.00	100	100
101.00	12.30	11.81
100.00	9.10	8.59
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003042.D
Acq On : 10 Oct 2018 00:12
Operator : MJ/SJ
Sample : J5157-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD4

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:53 PM

Quant Time: Oct 10 02:26:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

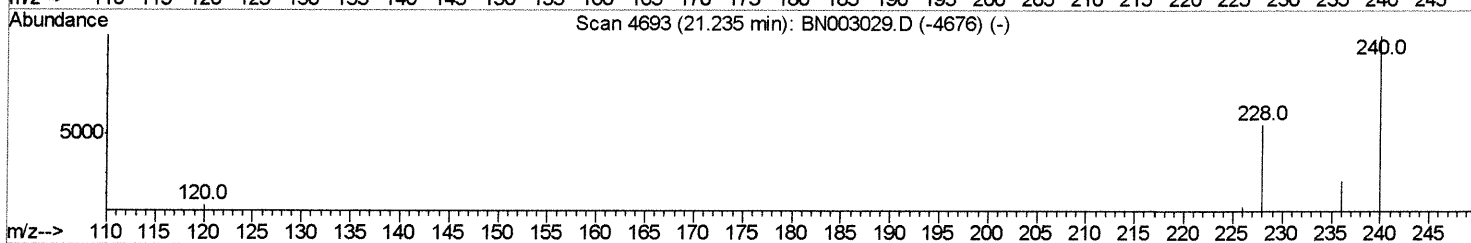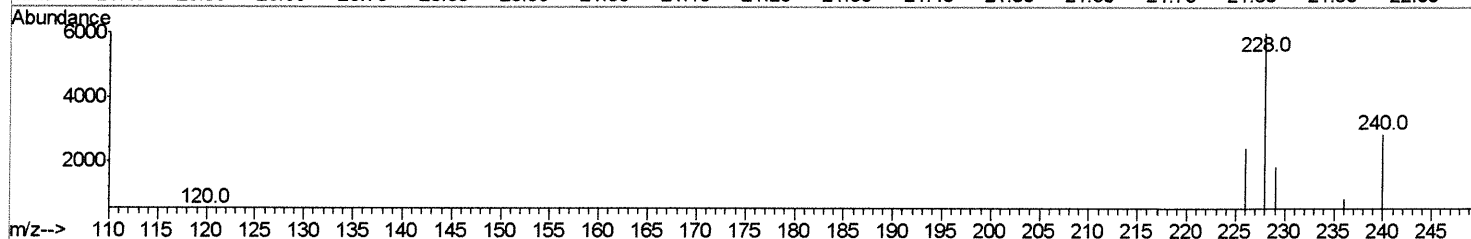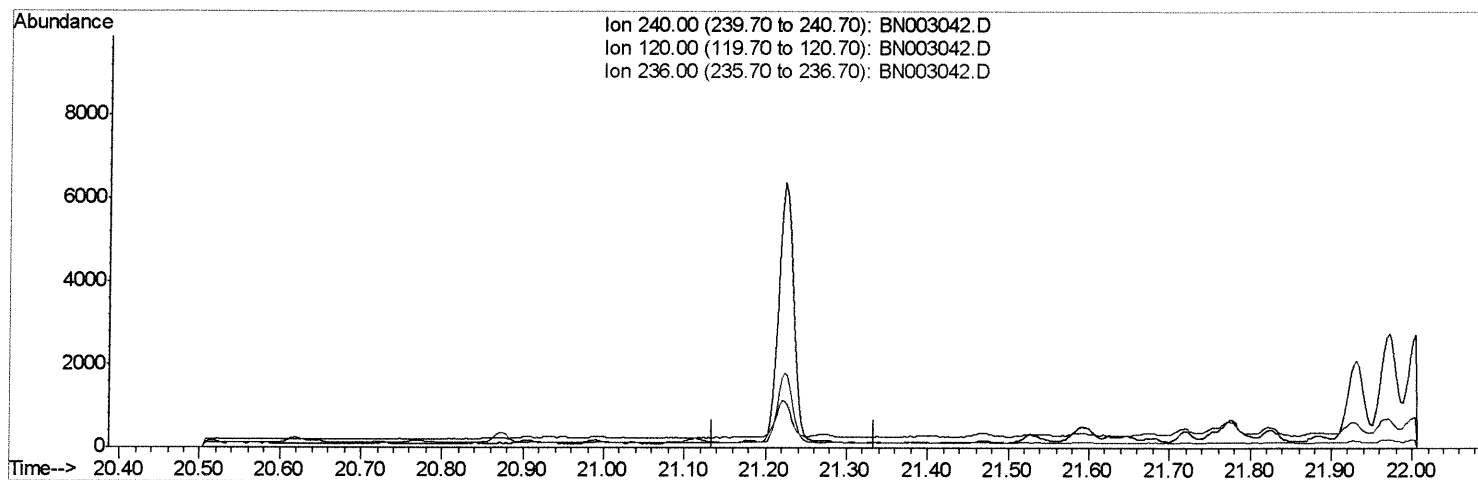

TIC: BN003042.D

(16) Chrysene-d12 (I)

21.235min (-21.235) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	16.40	0.00#
236.00	28.10	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003042.D
Acq On : 10 Oct 2018 00:12
Operator : MJ/SJ
Sample : J5157-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD4

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:53 PM

Quant Time: Oct 10 02:26:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

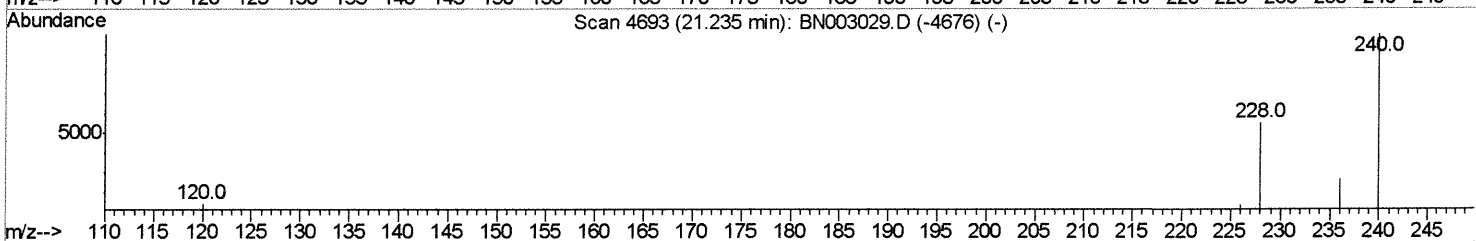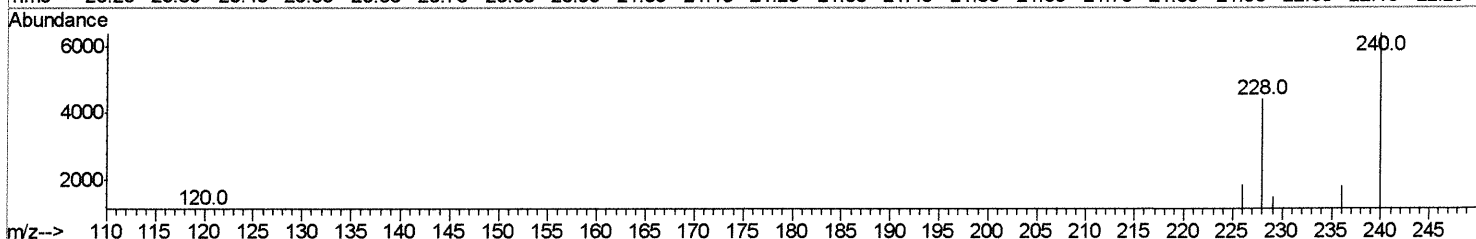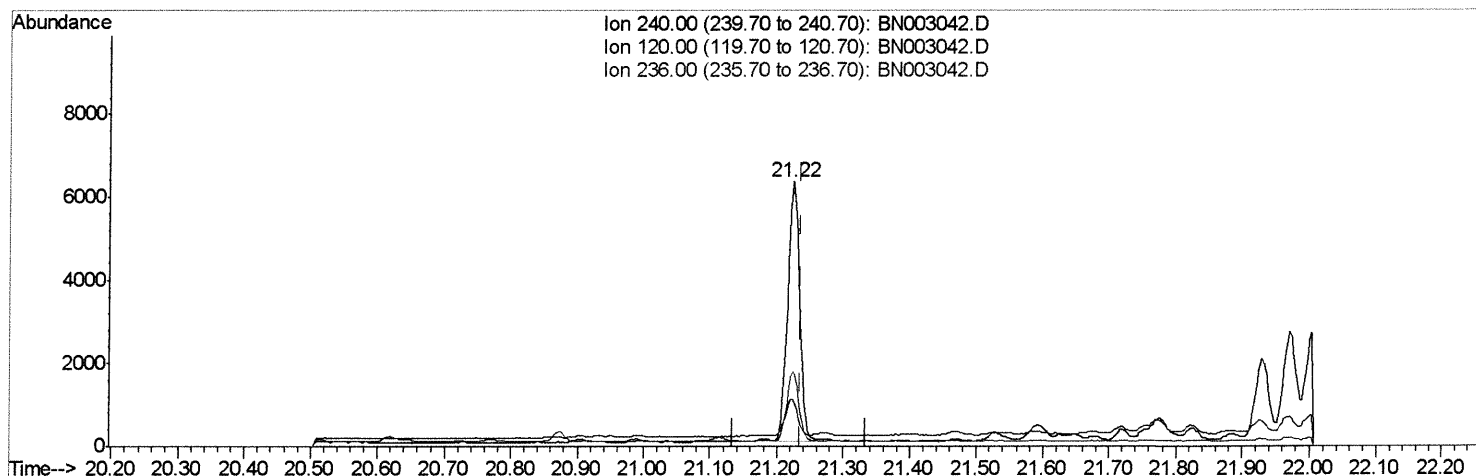

TIC: BN003042.D

(16) Chrysene-d12 (I)

21.223min (-0.012) 0.40ng/ul m

SJ10/12/18

response 7863

Ion	Exp%	Act%
240.00	100	100
120.00	16.40	17.78
236.00	28.10	28.36
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003042.D
 Acq On : 10 Oct 2018 00:12
 Operator : MJ/SJ
 Sample : J5157-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 C0AD4

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:53 PM

Quant Time: Oct 10 02:27:47 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

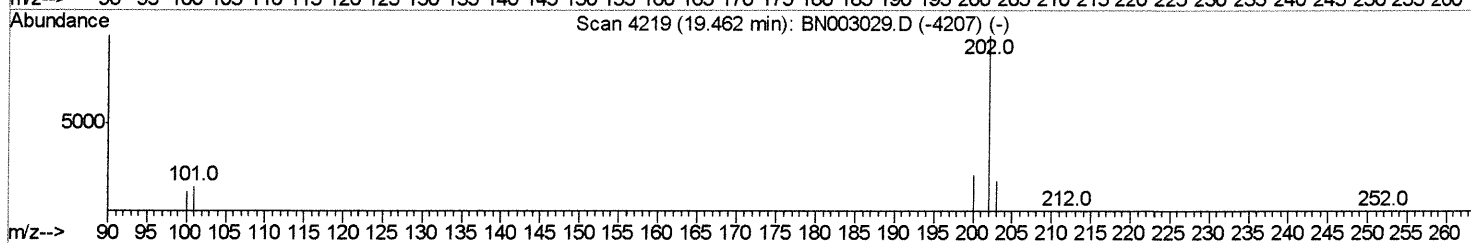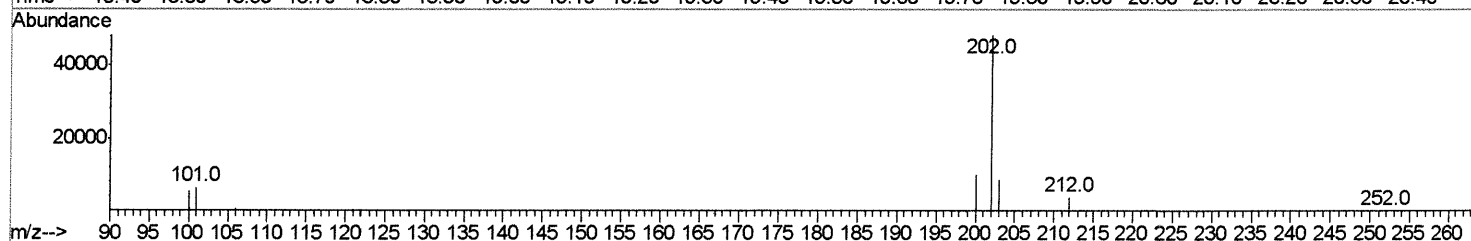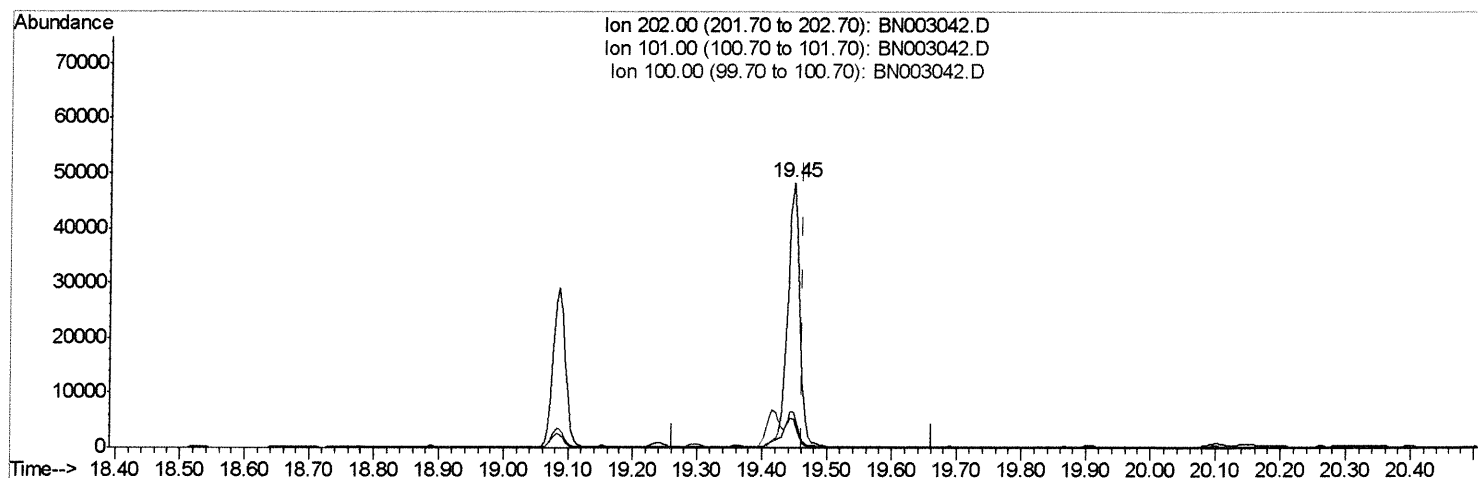

TIC: BN003042.D

(17) Pyrene

19.448min (-0.014) 2.11ng/ul

response 64501

Ion	Exp%	Act%
202.00	100	100
101.00	14.90	13.47
100.00	12.40	10.76
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003042.D
 Acq On : 10 Oct 2018 00:12
 Operator : MJ/SJ
 Sample : J5157-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD4

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:53 PM

Quant Time: Oct 10 02:27:47 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

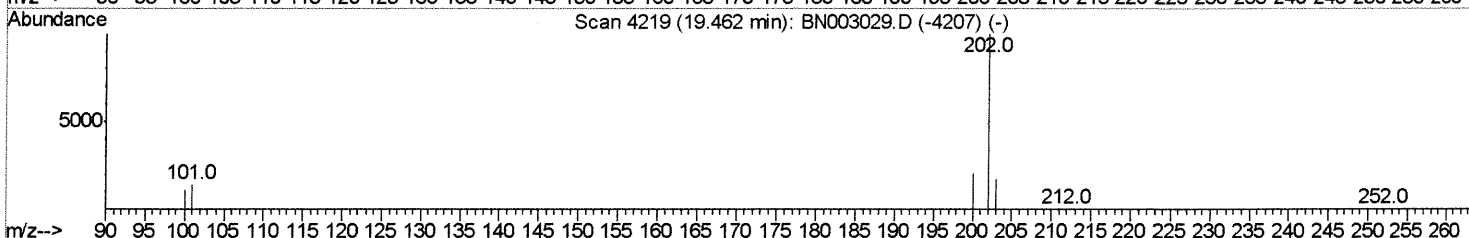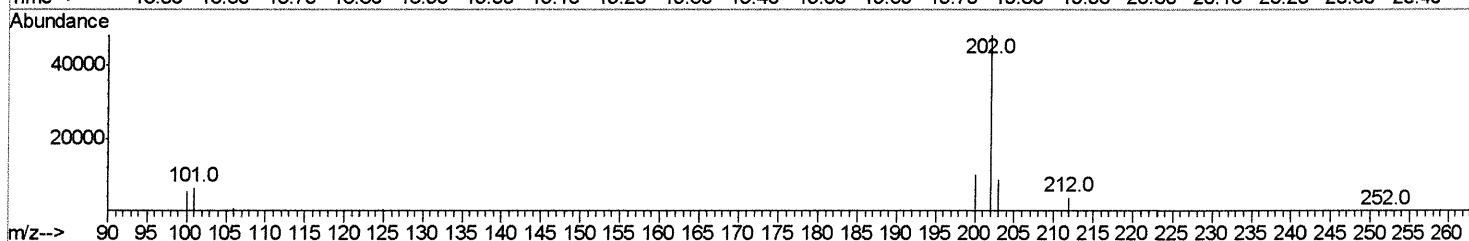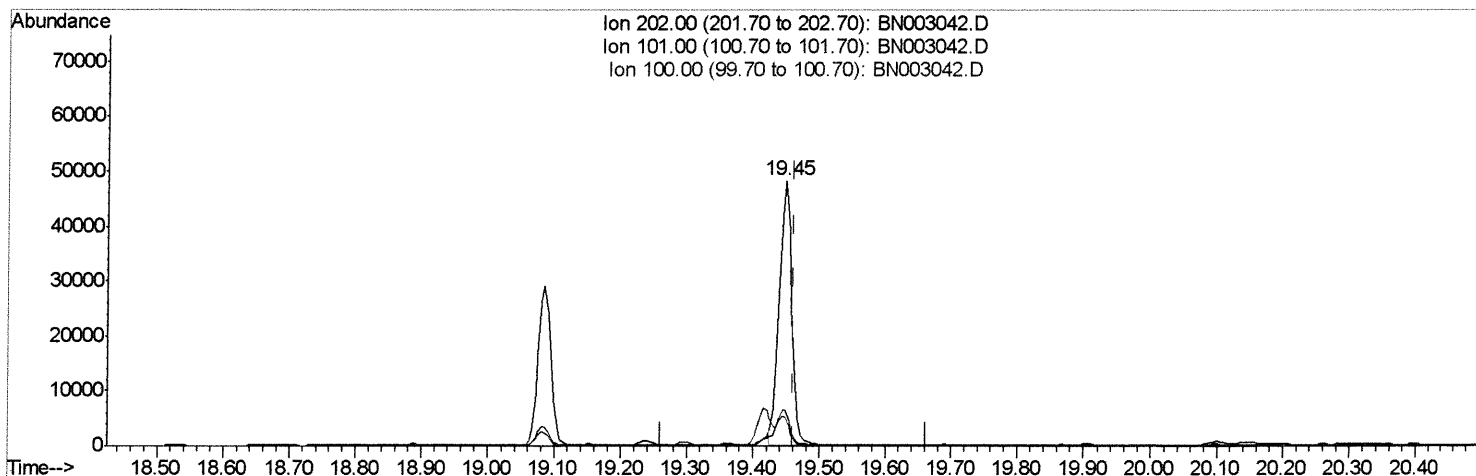

TIC: BN003042.D

(17) Pyrene

19.448min (-0.014) 2.04ng/ul m

SJ 10/12/18

response 62346

Ion	Exp%	Act%
202.00	100	100
101.00	14.90	13.47
100.00	12.40	10.76
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003042.D
 Acq On : 10 Oct 2018 00:12
 Operator : MJ/SJ
 Sample : J5157-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD4

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:53 PM

Quant Time: Oct 10 02:27:47 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

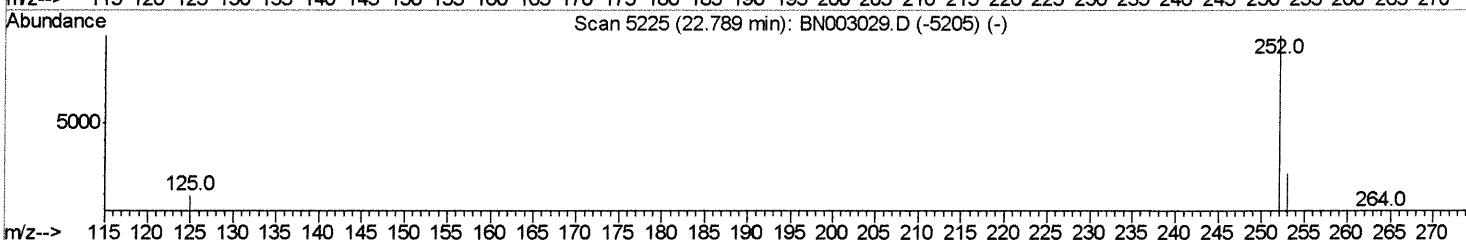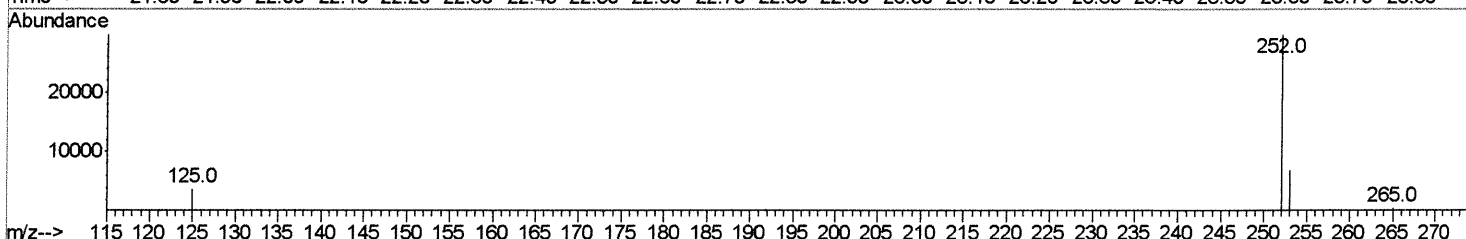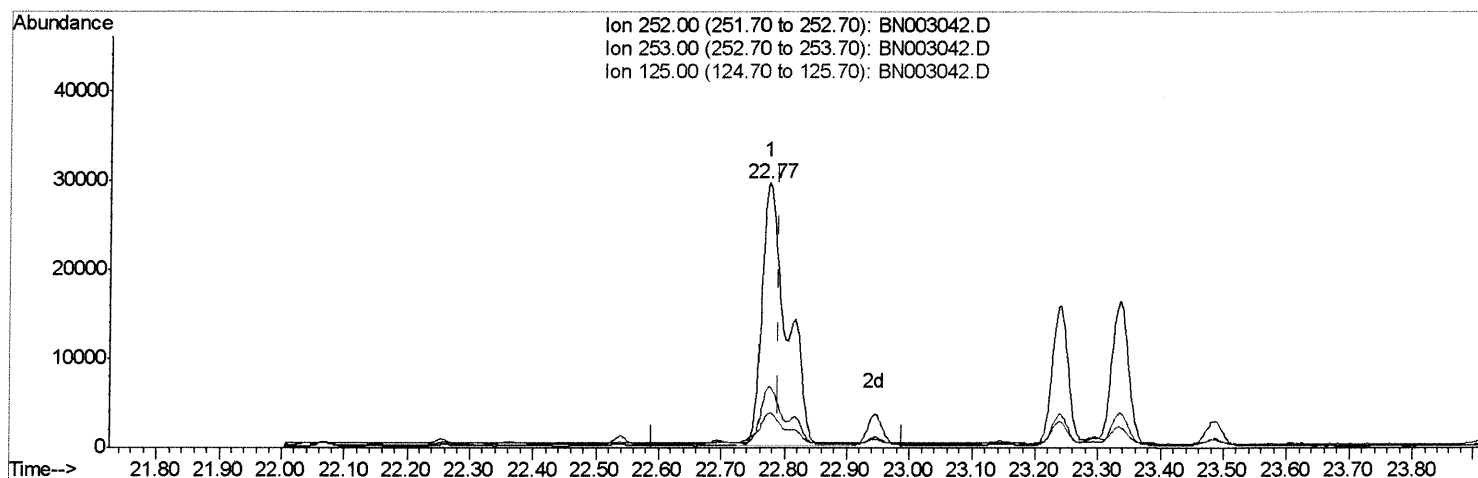

TIC: BN003042.D

(21) Benzo(b)fluoranthene
 22.775min (-0.015) 3.27ng/ul
 response 82176

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	23.18
125.00	17.10	12.92
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003042.D
 Acq On : 10 Oct 2018 00:12
 Operator : MJ/SJ
 Sample : J5157-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD4

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:53 PM

Quant Time: Oct 10 02:27:47 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

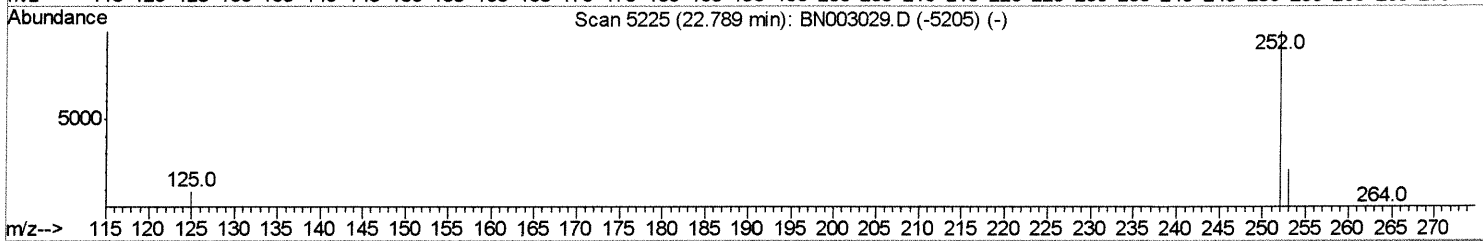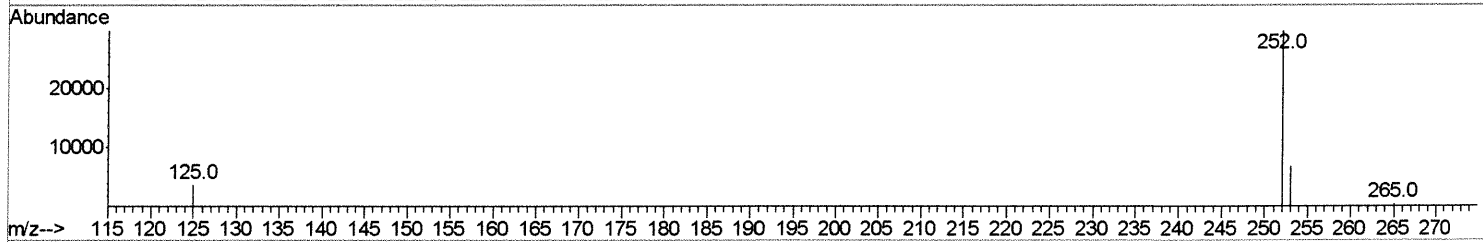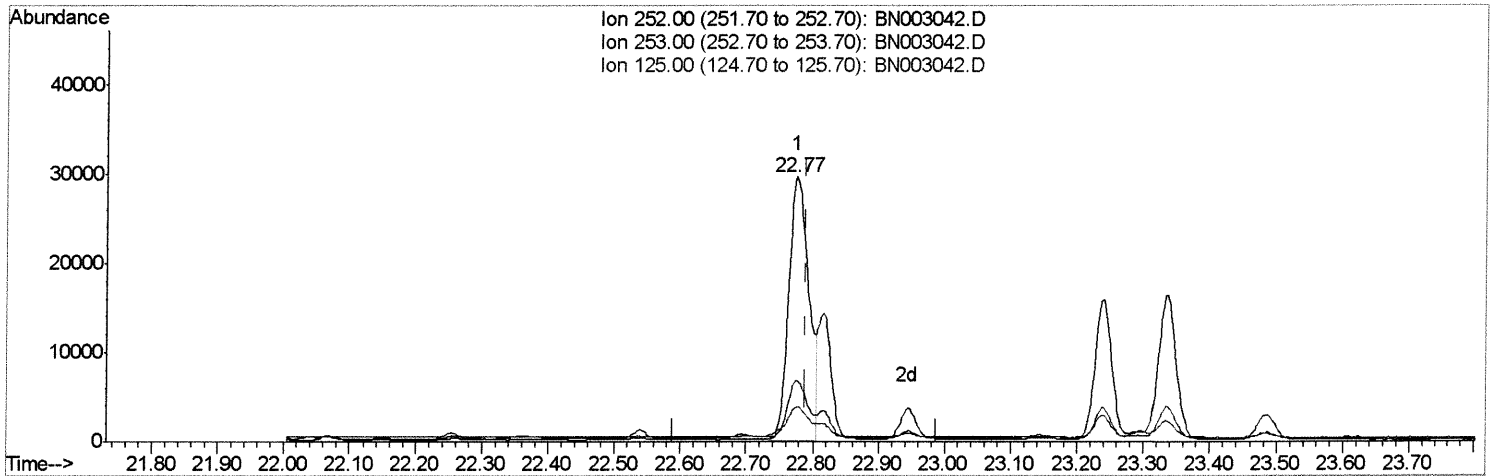

(21) Benzo(b)fluoranthene

22.775min (-0.015) 2.49ng/ul m

SJ 10/12/18

response 62404

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	23.18
125.00	17.10	12.92
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003042.D
 Acq On : 10 Oct 2018 00:12
 Operator : MJ/SJ
 Sample : J5157-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD4

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:53 PM

Quant Time: Oct 10 02:27:47 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

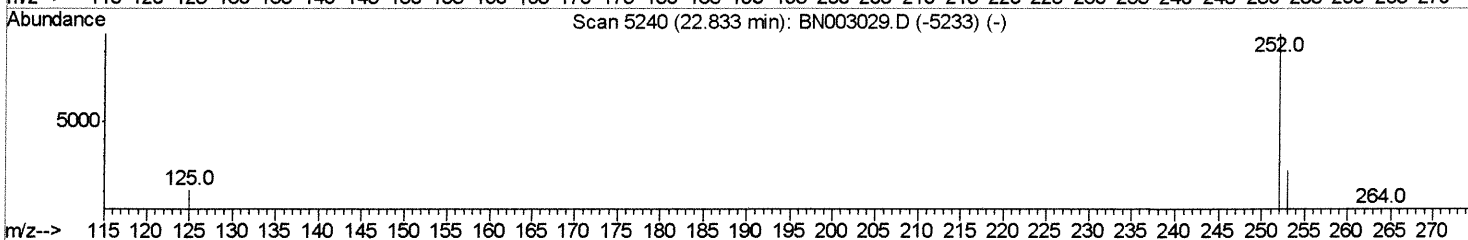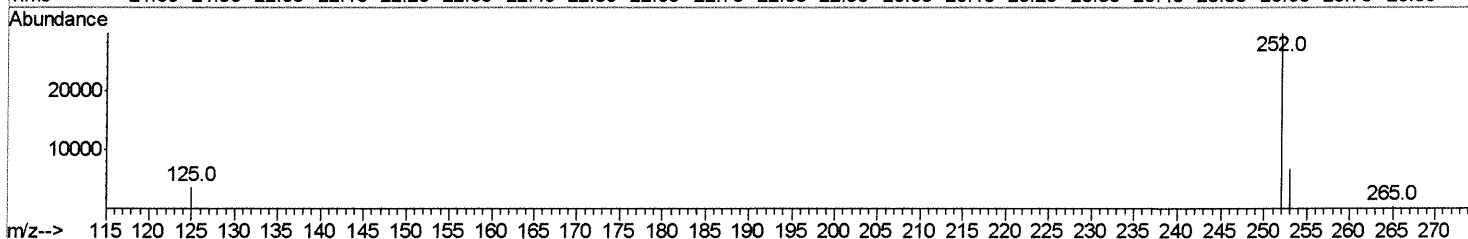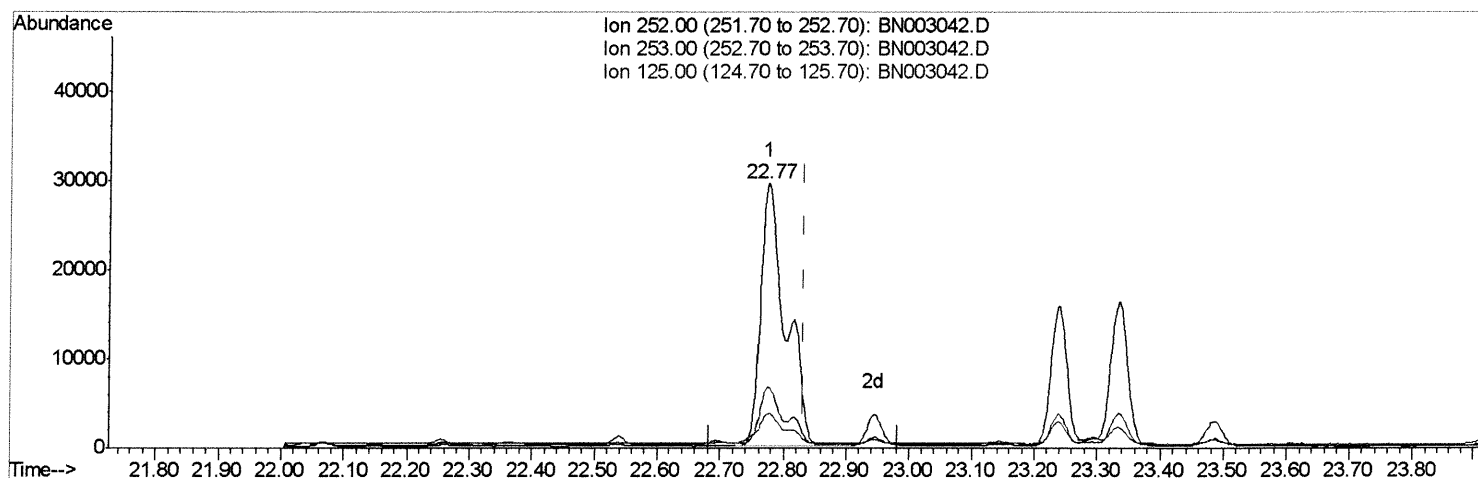

TIC: BN003042.D

(22) Benzo(k)fluoranthene
 22.775min (-0.059) 3.16ng/ul
 response 82176

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	23.18
125.00	17.60	12.92#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003042.D
 Acq On : 10 Oct 2018 00:12
 Operator : MJ/SJ
 Sample : J5157-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD4

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:53 PM

Quant Time: Oct 10 02:27:47 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

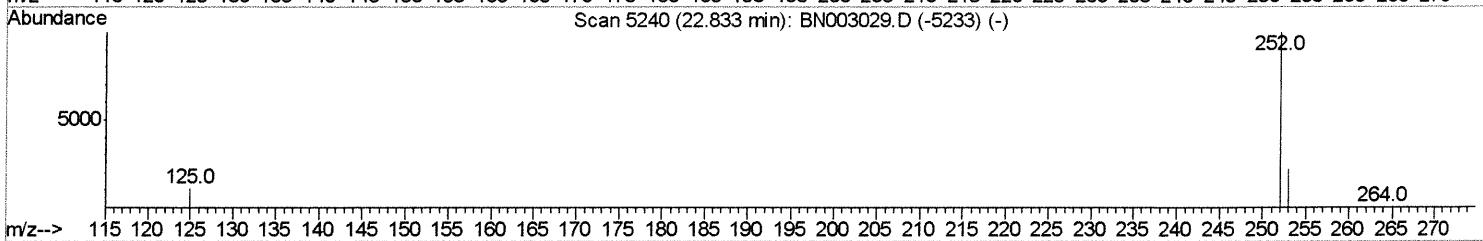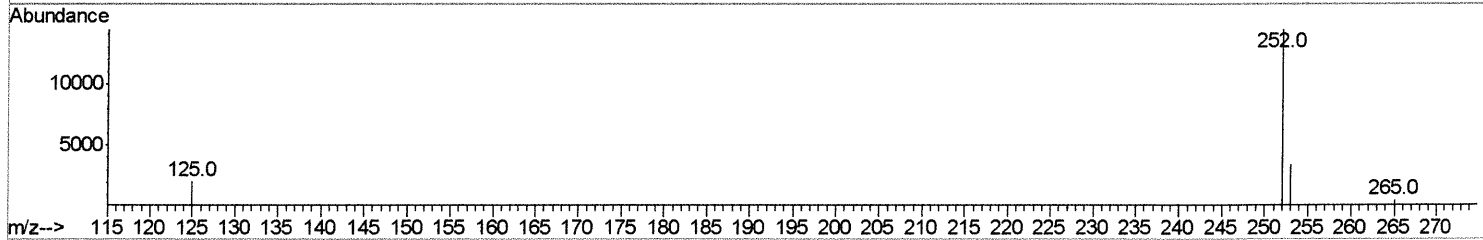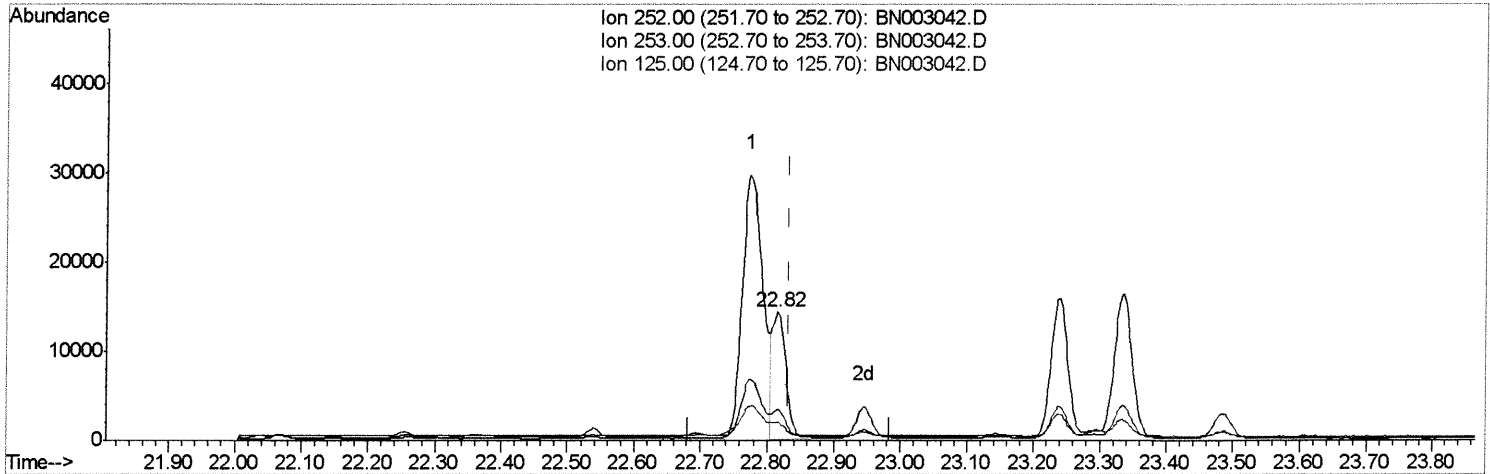

(22) Benzo(k)fluoranthene

22.815min (-0.018) 0.78ng/ul m

SJ 10/12/18

response 20354

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	24.02
125.00	17.60	14.08
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003042.D
 Acq On : 10 Oct 2018 00:12
 Operator : MJ/SJ
 Sample : J5157-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD4

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:53 PM

Quant Time: Oct 10 02:29:44 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	2010	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.39	136	8440	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.26	164	4944	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.01	188	10533m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.22	240	7863m	0.40	ng/ul	-0.01
20) Perylene-d12	23.44	264	6968	0.40	ng/ul	-0.02

Sytem Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.01	152	4364	0.33	ng/ul	-0.02
14) Fluoranthene-d10	19.05	212	10269m	0.34	ng/ul	-0.01

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
3) Naphthalene	10.44	128	1695	0.078	ng/ul#	93
5) 2-Methylnaphthalene	12.08	142	523	0.035	ng/ul	95
7) Acenaphthylene	13.98	152	3395	0.150	ng/ul	96
8) Acenaphthene	14.32	153	609	0.035	ng/ul	96
9) Fluorene	15.32	166	946	0.048	ng/ul#	94
12) Phenanthrene	17.06	178	8874m	0.302	ng/ul	
13) Anthracene	17.15	178	7652m	0.276	ng/ul	
15) Fluoranthene	19.09	202	38990m	1.132	ng/ul	
17) Pyrene	19.45	202	62346m	2.041	ng/ul	
18) Benzo(a)anthracene	21.21	228	18721	0.740	ng/ul	96
19) Chrysene	21.26	228	35350	1.376	ng/ul	99
21) Benzo(b)fluoranthene	22.77	252	62404m	2.487	ng/ul	
22) Benzo(k)fluoranthene	22.82	252	20354m	0.782	ng/ul	
23) Benzo(a)pyrene	23.34	252	30691	1.365	ng/ul#	88
24) Indeno(1,2,3-cd)pyrene	25.65	276	17832	0.690	ng/ul#	94
25) Dibenzo(a,h)anthracene	25.64	278	5122	0.248	ng/ul	93
26) Benzo(a,h,i)perylene	26.32	276	14679	0.674	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed