

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003043.D
 Acq On : 10 Oct 2018 00:47
 Operator : MJ/SJ
 Sample : J5157-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD5

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:54 PM

Quant Time: Oct 10 02:33:34 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

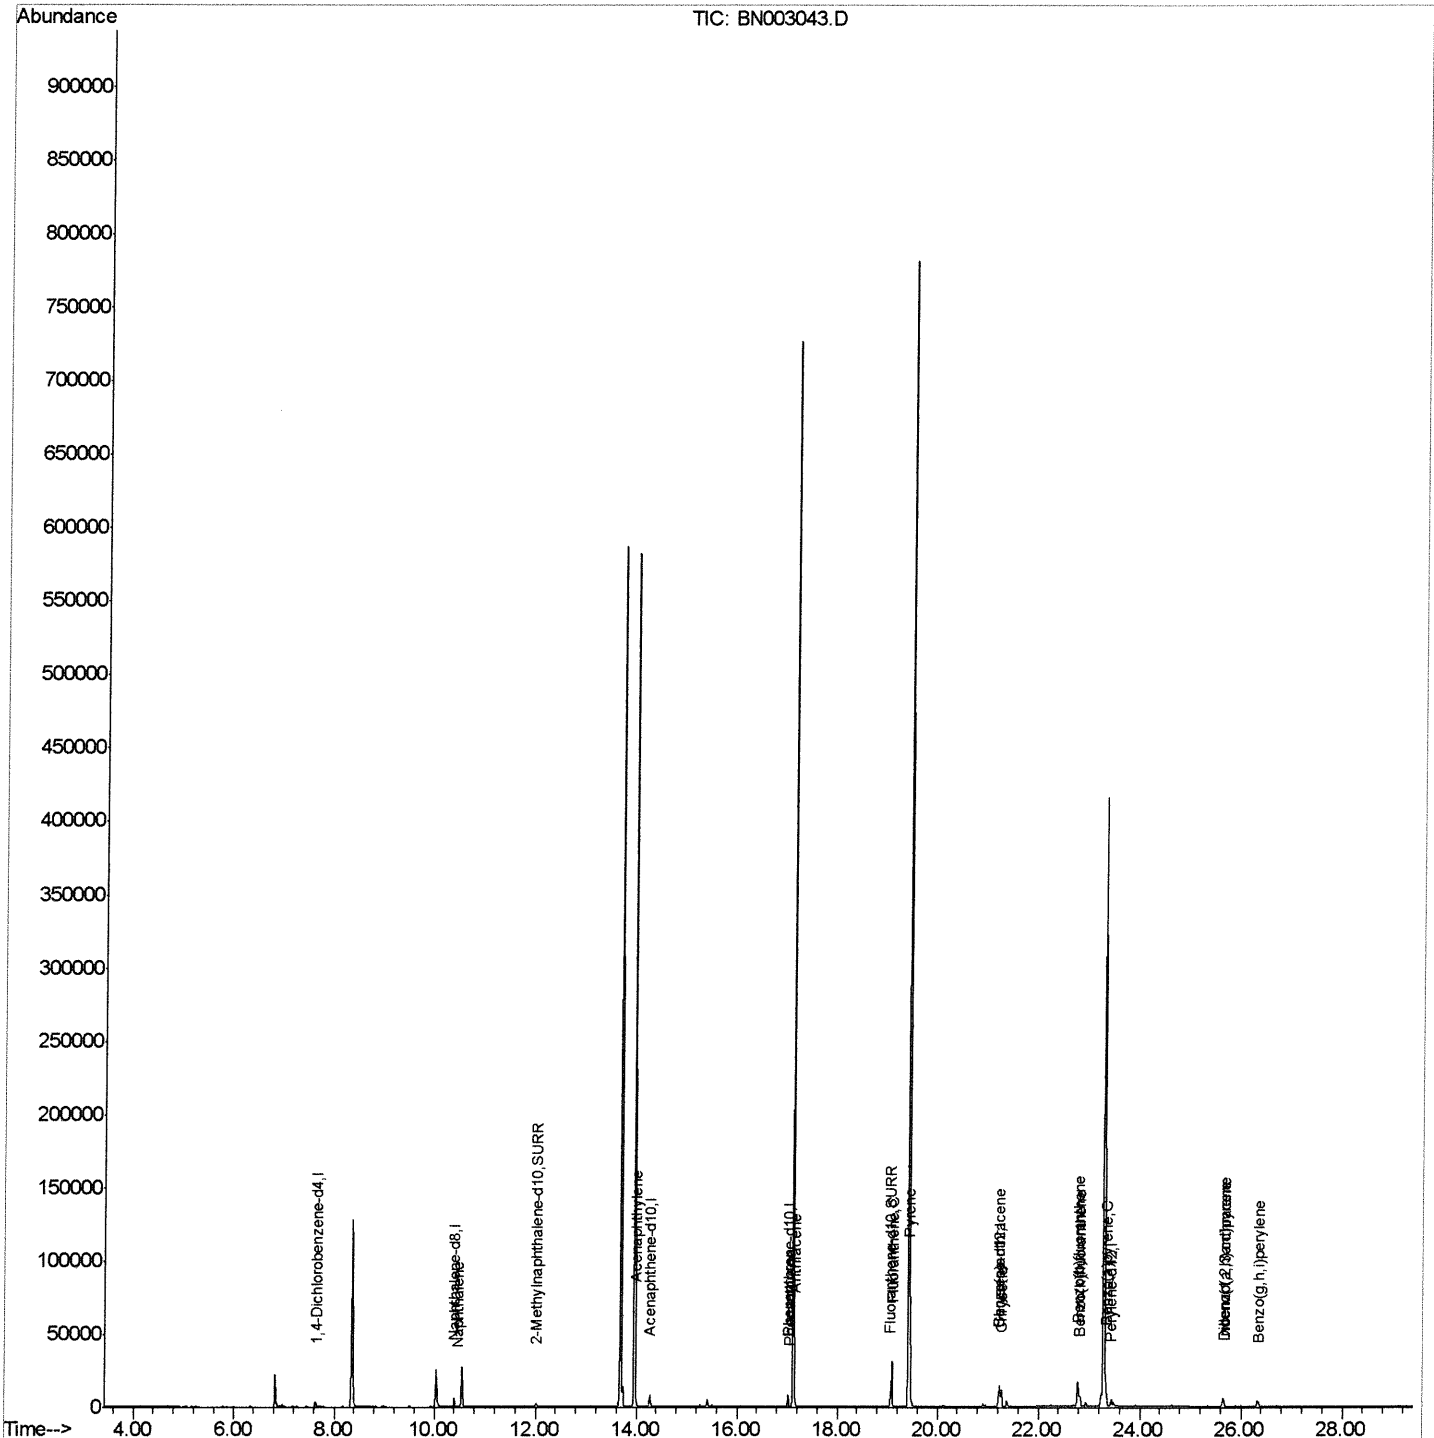

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003043.D
 Acq On : 10 Oct 2018 00:47
 Operator : MJ/SJ
 Sample : J5157-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD5

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:54 PM

Quant Time: Oct 10 01:38:33 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

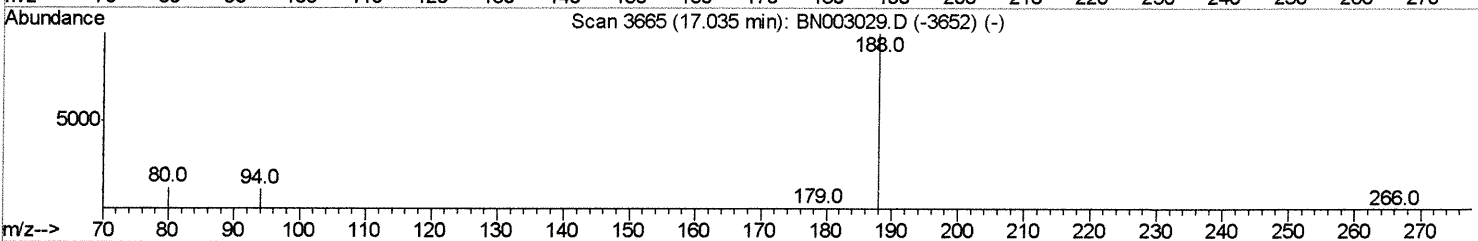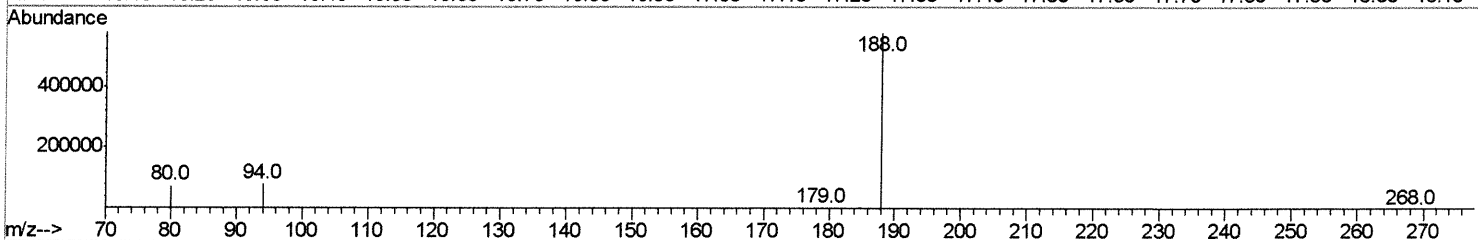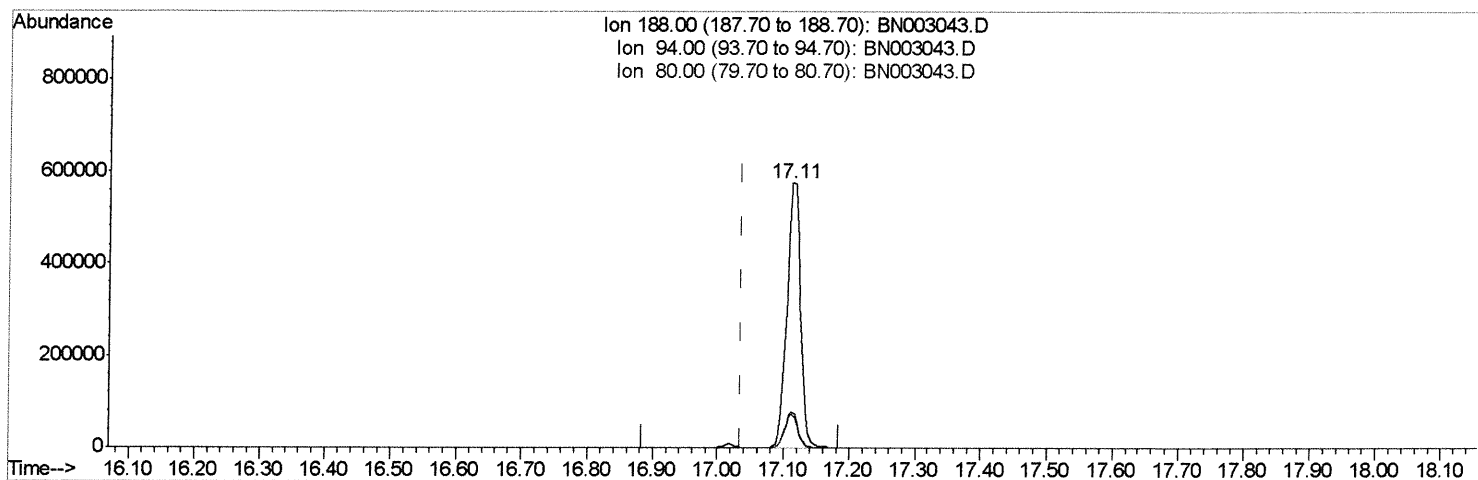

TIC: BN003043.D

(10) Phenanthrene-d10 (I)
 17.111min (+0.076) 0.40ng/ul
 response 823723

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	13.67
80.00	12.70	12.52
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003043.D
 Acq On : 10 Oct 2018 00:47
 Operator : MJ/SJ
 Sample : J5157-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD5

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:54 PM

Quant Time: Oct 10 01:38:33 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

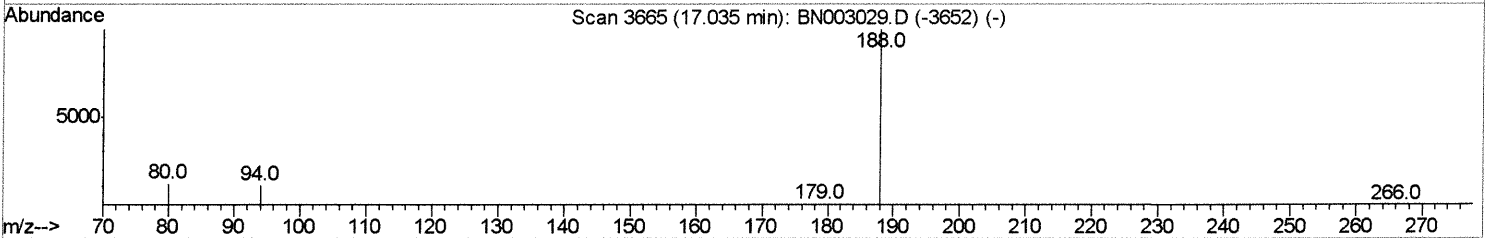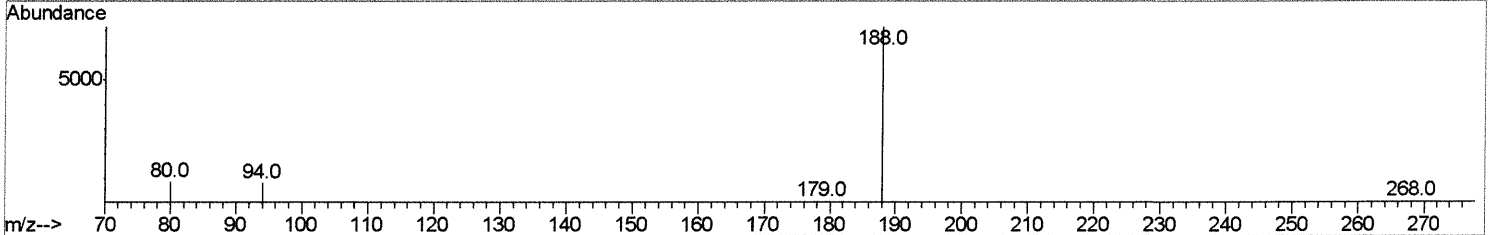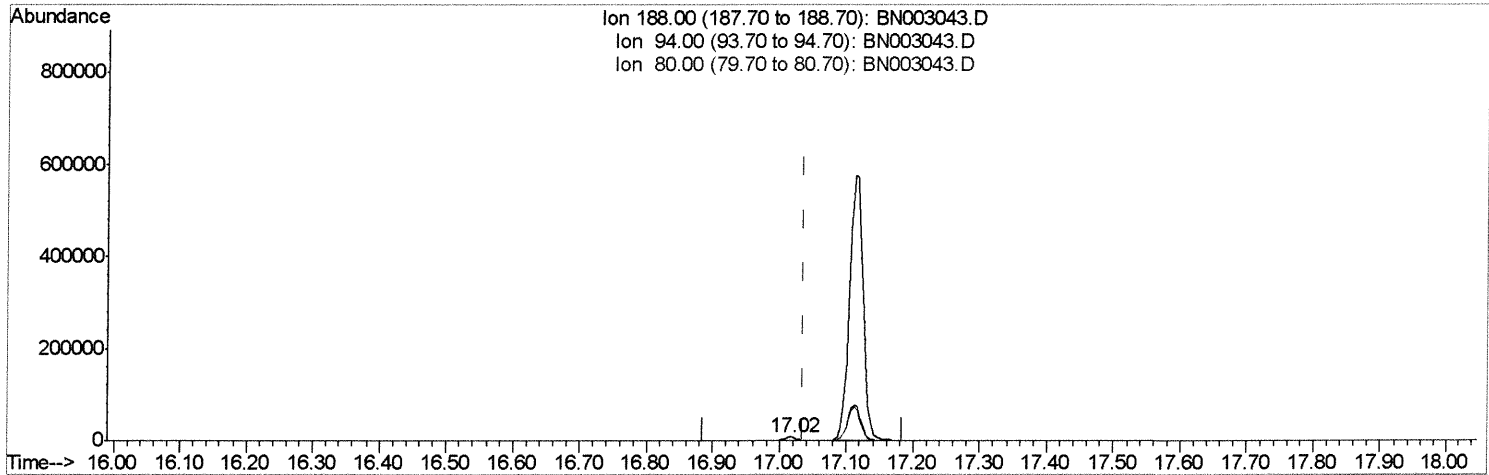

TIC: BN003043.D

(10) Phenanthrene-d10 (I)

17.019min (-0.017) 0.40ng/ul m *SJ 10/12/18*

response 10234

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	11.26
80.00	12.70	12.20
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003043.D
Acq On : 10 Oct 2018 00:47
Operator : MJ/SJ
Sample : J5157-13
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD5

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:54 PM

Quant Time: Oct 10 02:30:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

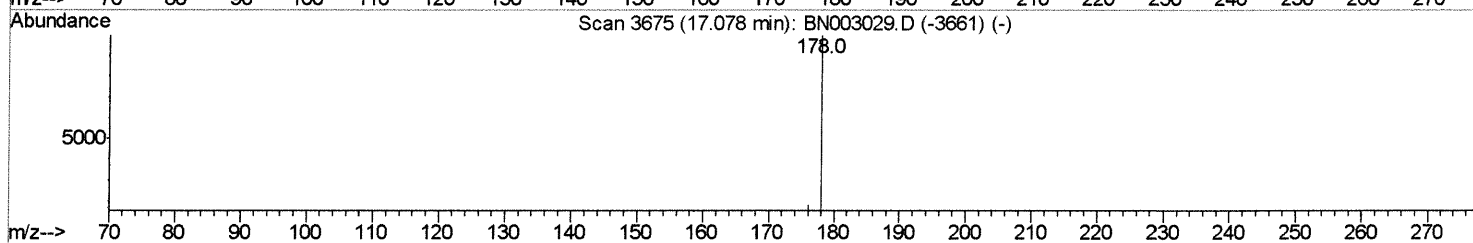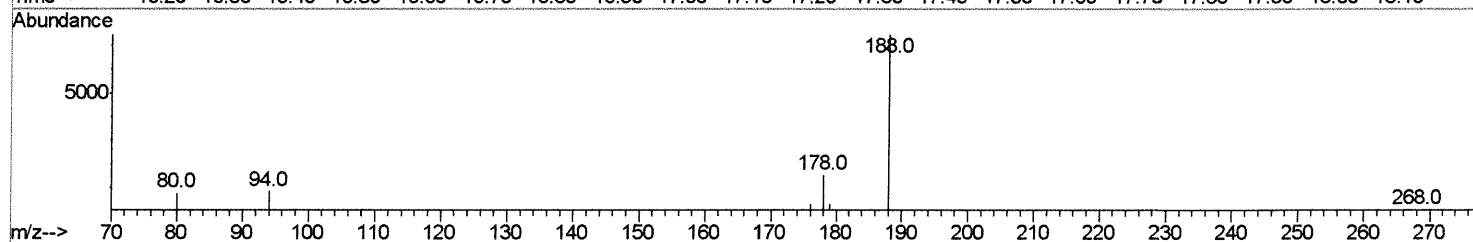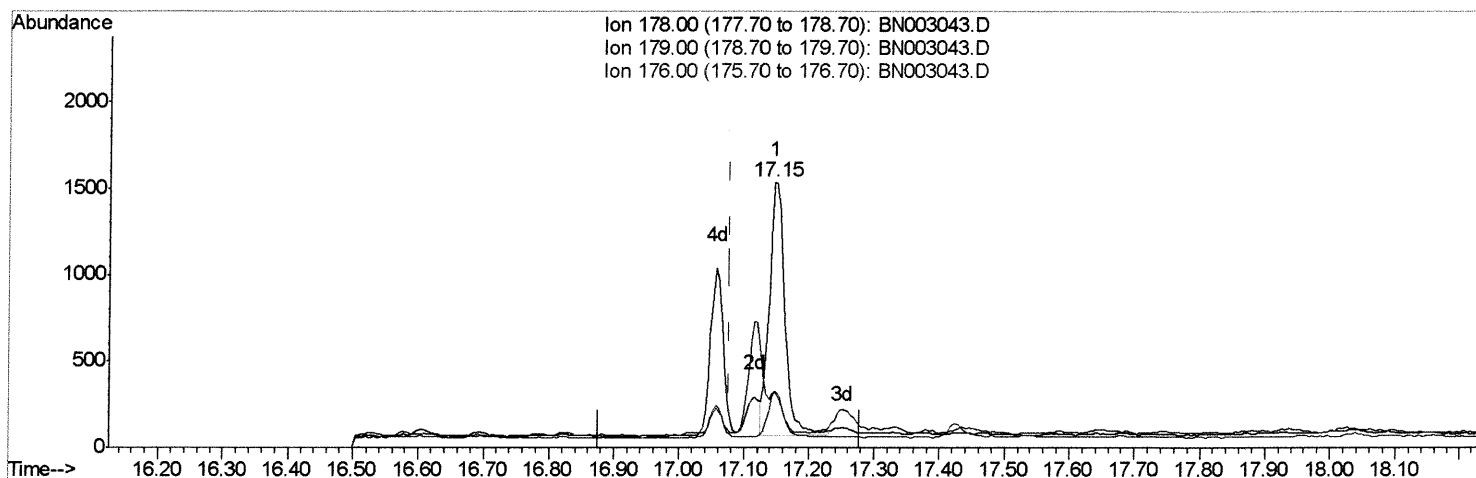

TIC: BN003043.D

(12) Phenanthrene

17.145min (+0.068) 0.09ng/ul

response 2458

Ion	Exp%	Act%
178.00	100	100
179.00	16.10	20.94#
176.00	19.30	21.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003043.D
Acq On : 10 Oct 2018 00:47
Operator : MJ/SJ
Sample : J5157-13
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD5

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:54 PM

Quant Time: Oct 10 02:30:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

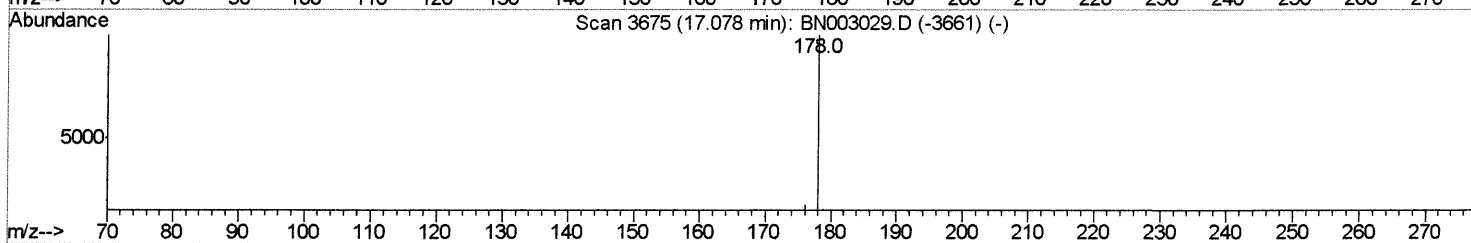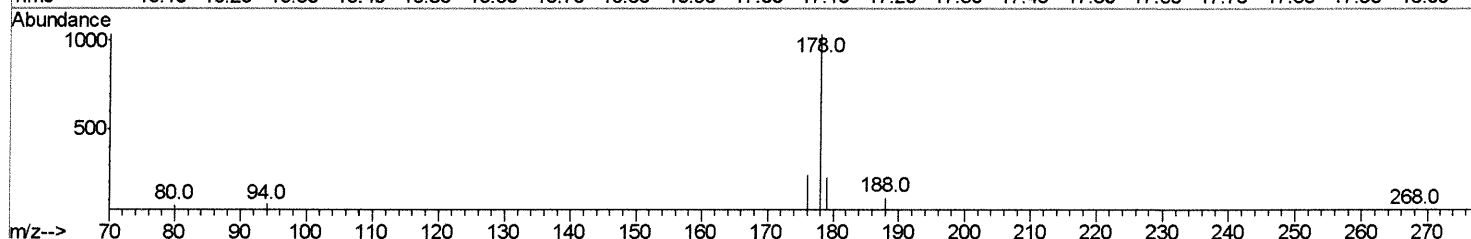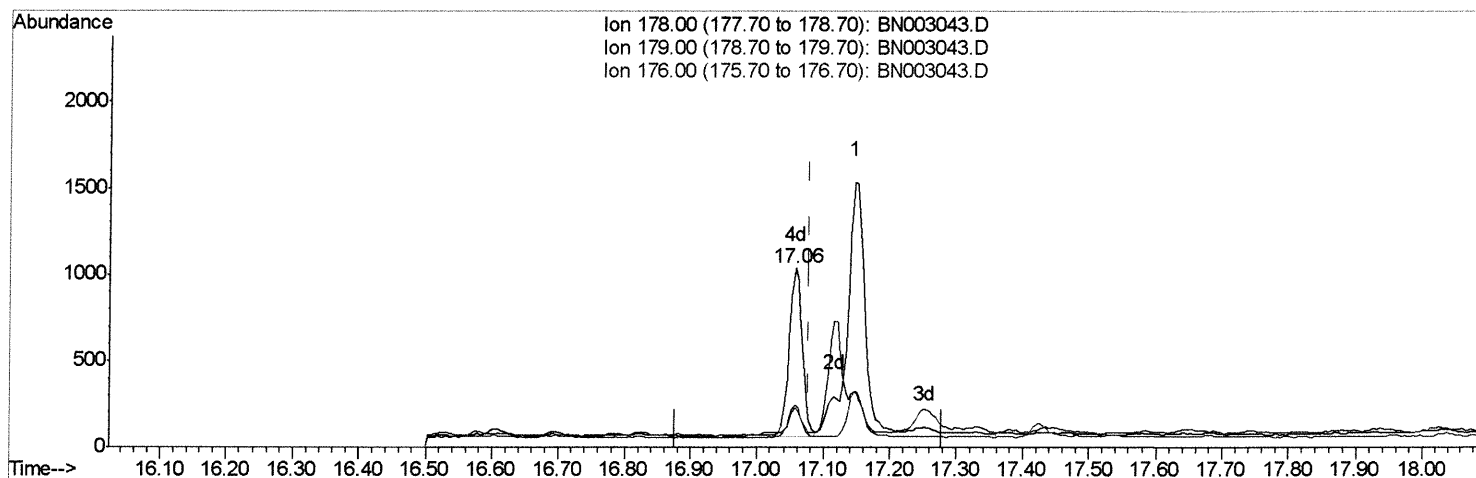

TIC: BN003043.D

(12) Phenanthrene

17.057min (-0.021) 0.05ng/ul m

SJ 10/12/18

response 1350

Ion	Exp%	Act%
178.00	100	100
179.00	16.10	22.01#
176.00	19.30	23.65#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003043.D
 Acq On : 10 Oct 2018 00:47
 Operator : MJ/SJ
 Sample : J5157-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD5

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:54 PM

Quant Time: Oct 10 02:30:35 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

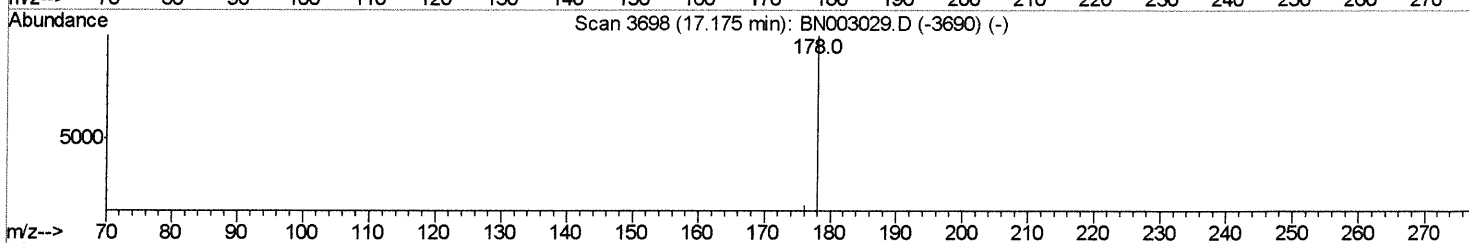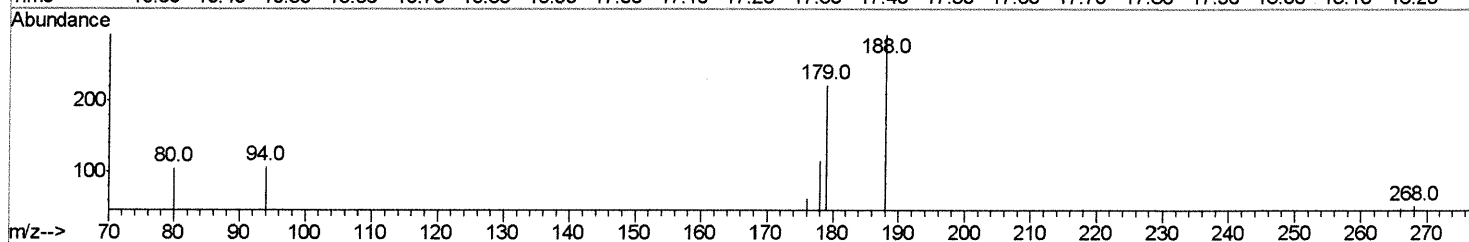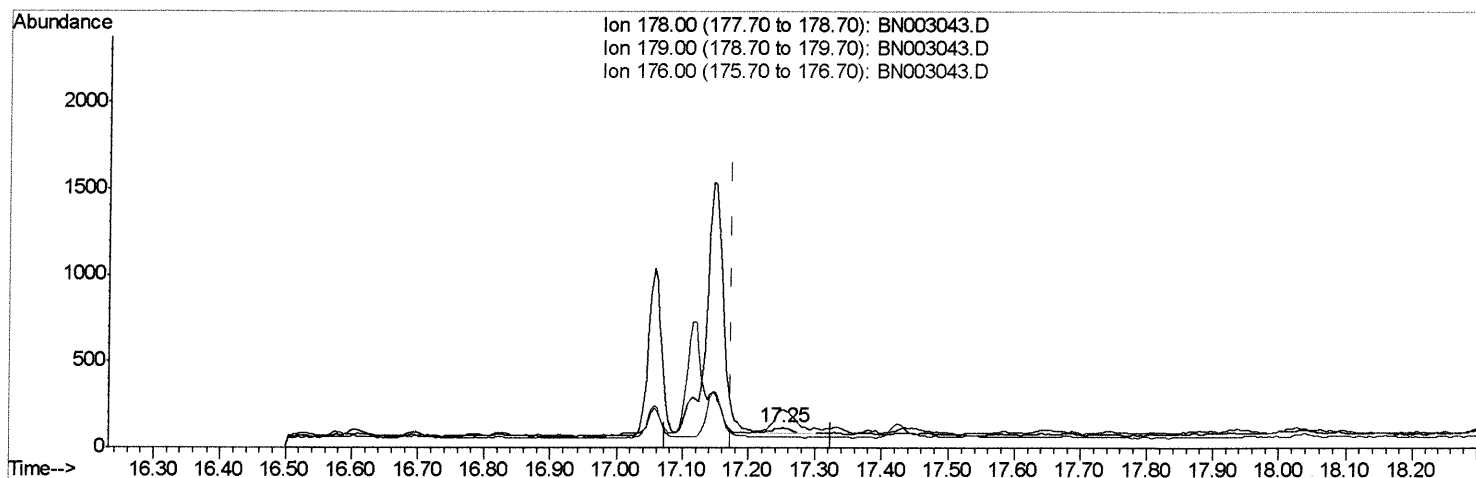

TIC: BN003043.D

(13) Anthracene

17.251min (+0.076) 0.00ng/ul

response 65

Ion	Exp%	Act%
178.00	100	100
179.00	16.30	191.38#
176.00	19.10	54.31#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003043.D
Acq On : 10 Oct 2018 00:47
Operator : MJ/SJ
Sample : J5157-13
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD5

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:54 PM

Quant Time: Oct 10 02:30:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

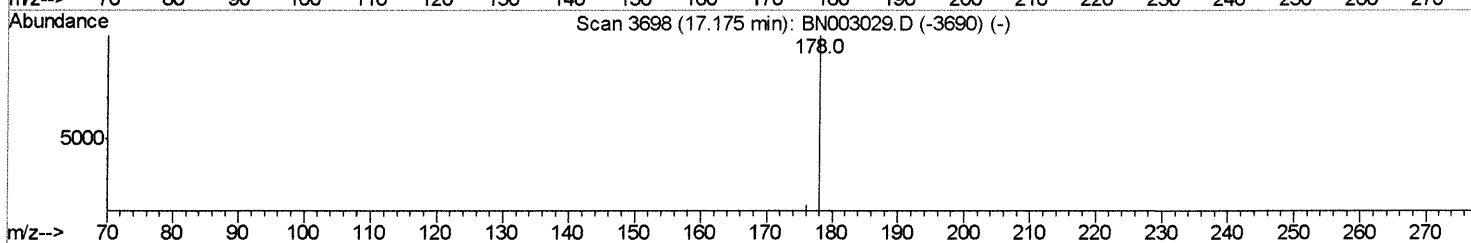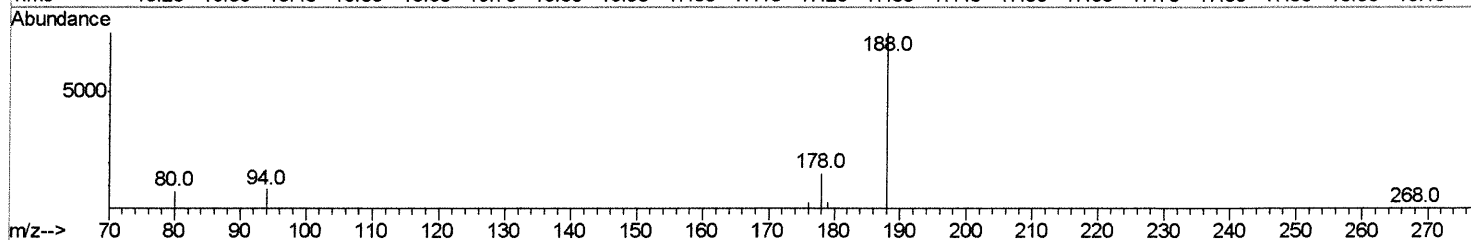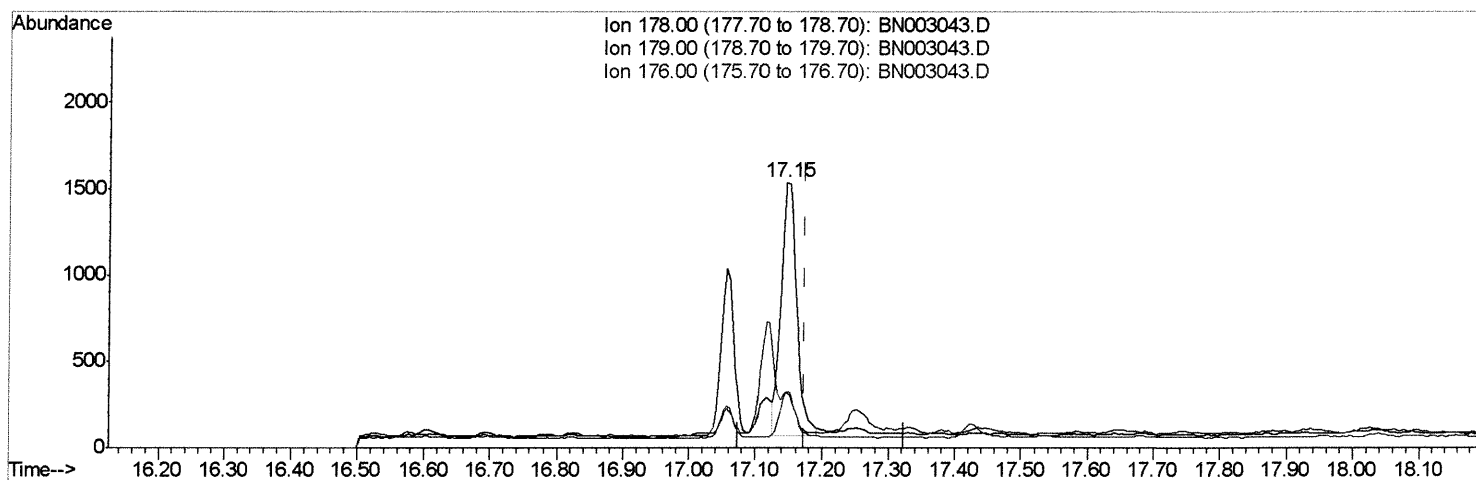

TIC: BN003043.D

(13) Anthracene

17.145min (-0.030) 0.09ng/ul m

5J10/12/18

response 2432

Ion	Exp%	Act%
178.00	100	100
179.00	16.30	20.94#
176.00	19.10	21.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003043.D
Acq On : 10 Oct 2018 00:47
Operator : MJ/SJ
Sample : J5157-13
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD5

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:54 PM

Quant Time: Oct 10 02:30:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

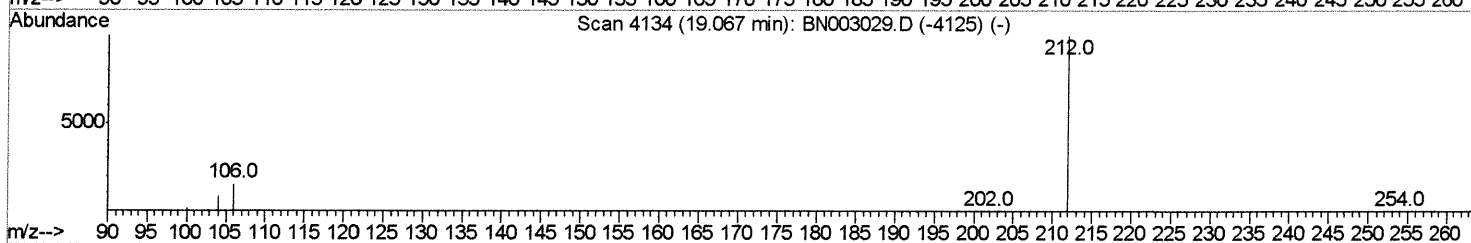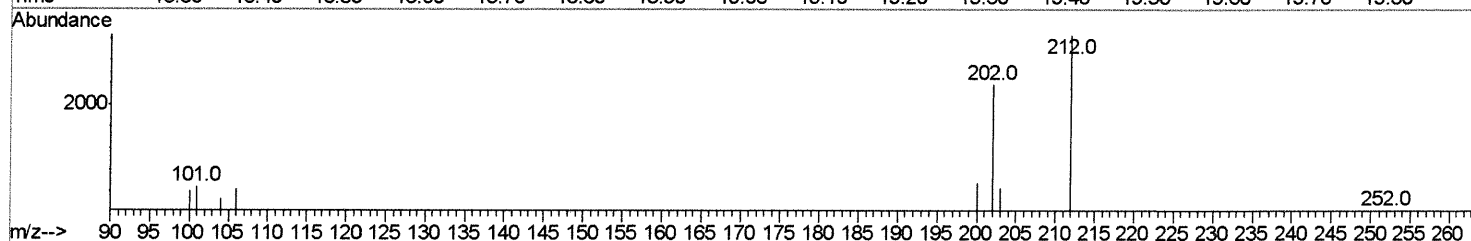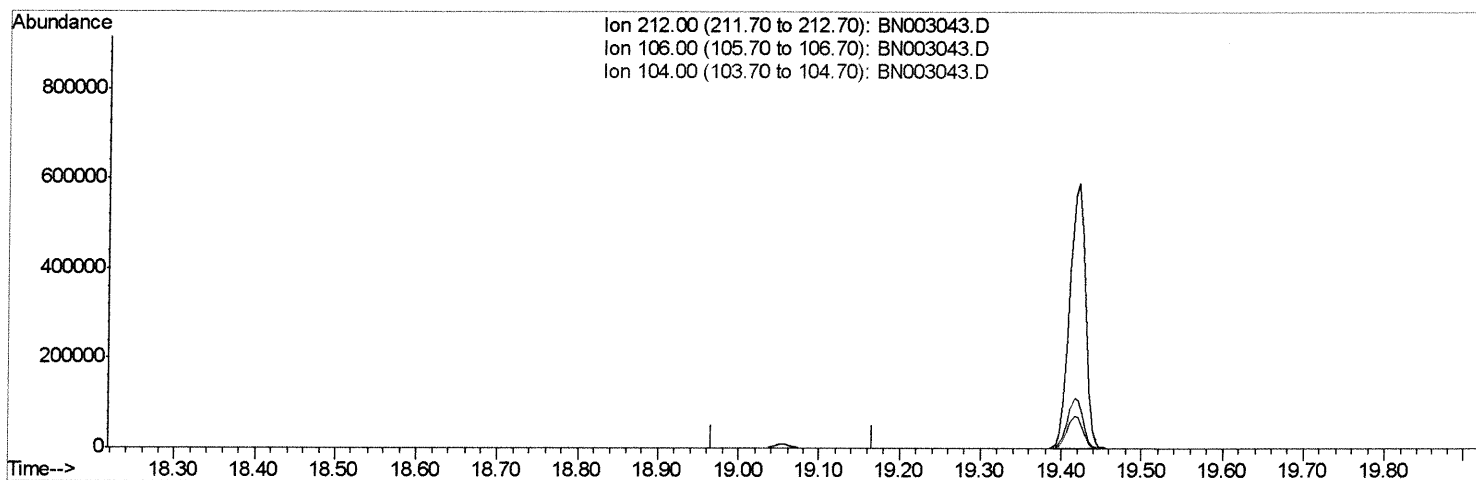

TIC: BN003043.D

(14) Fluoranthene-d10 (SURR)

19.067min (-19.067) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	15.40	0.00#
104.00	8.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003043.D
 Acq On : 10 Oct 2018 00:47
 Operator : MJ/SJ
 Sample : J5157-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD5

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:54 PM

Quant Time: Oct 10 02:30:35 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

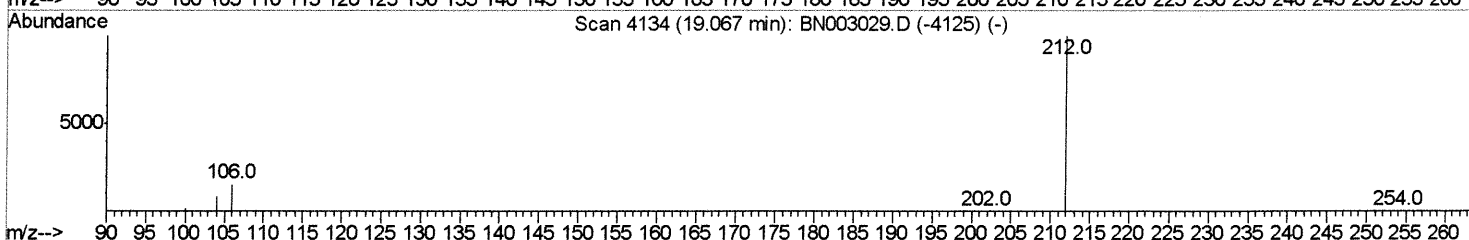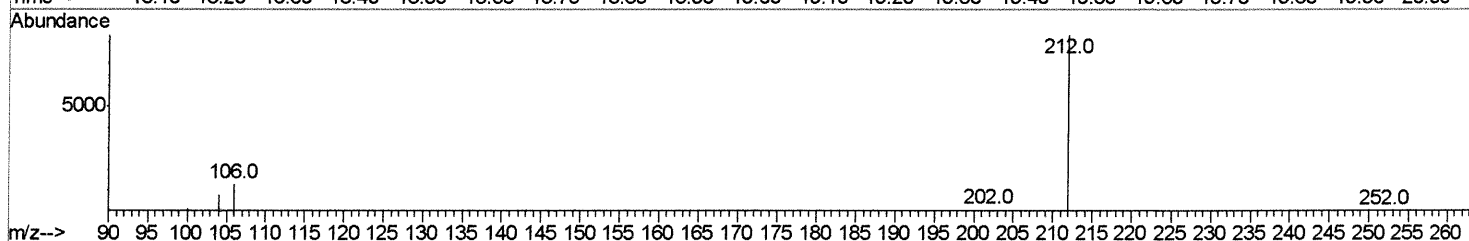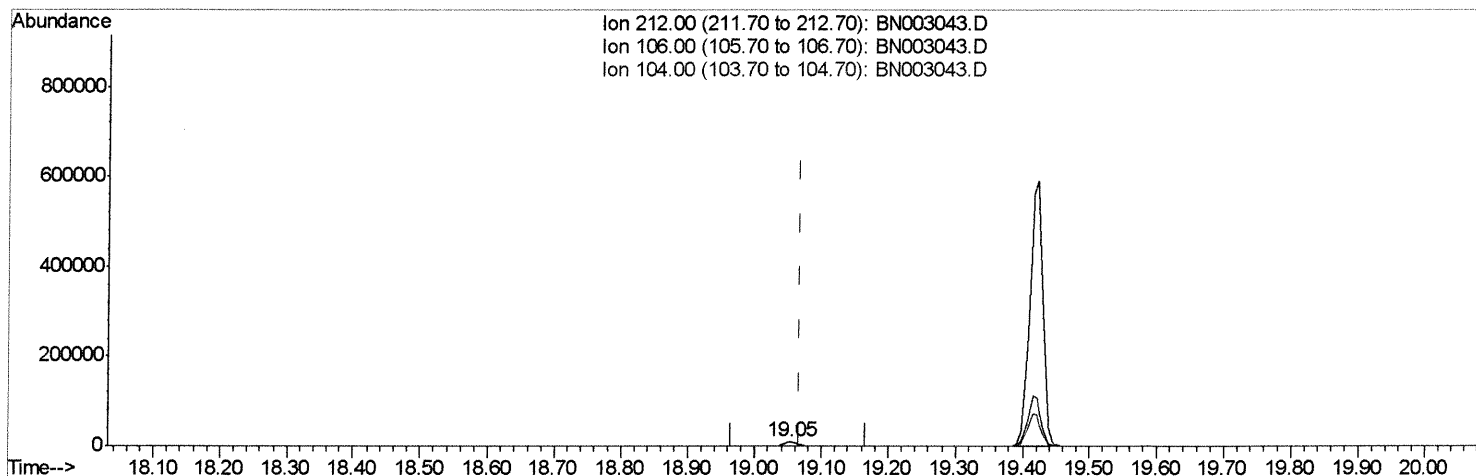

TIC: BN003043.D

(14) Fluoranthene-d10 (SURR)

19.053min (-0.014) 0.40ng/ul m

SJ 10/12/18

response 11768

Ion	Exp%	Act%
212.00	100	100
106.00	15.40	0.00#
104.00	8.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003043.D
Acq On : 10 Oct 2018 00:47
Operator : MJ/SJ
Sample : J5157-13
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD5

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:54 PM

Quant Time: Oct 10 02:30:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

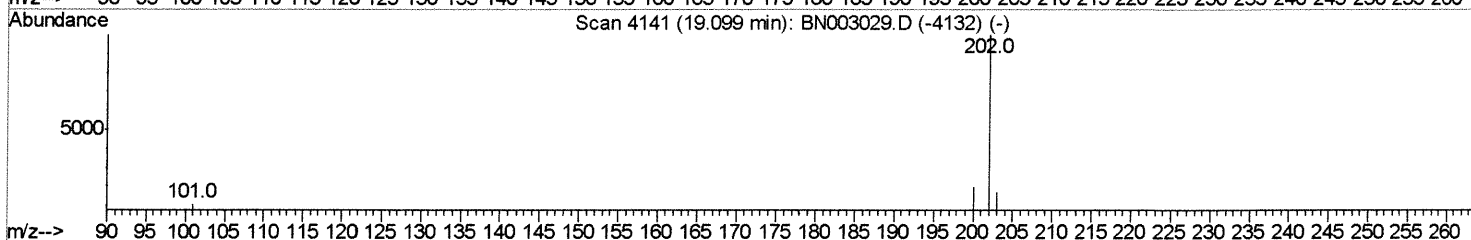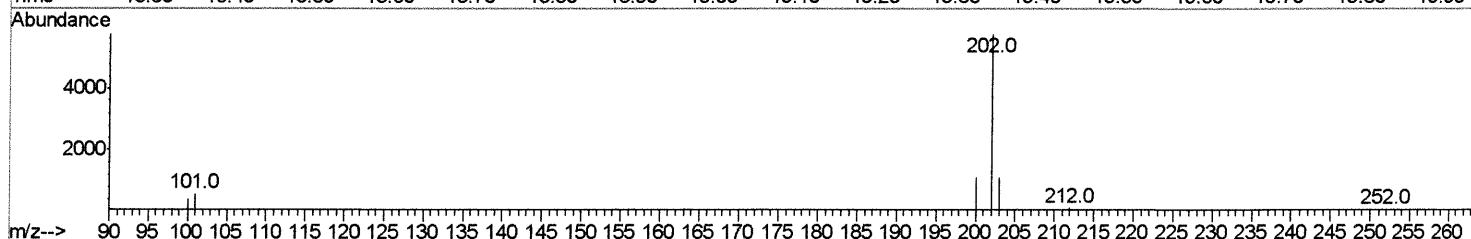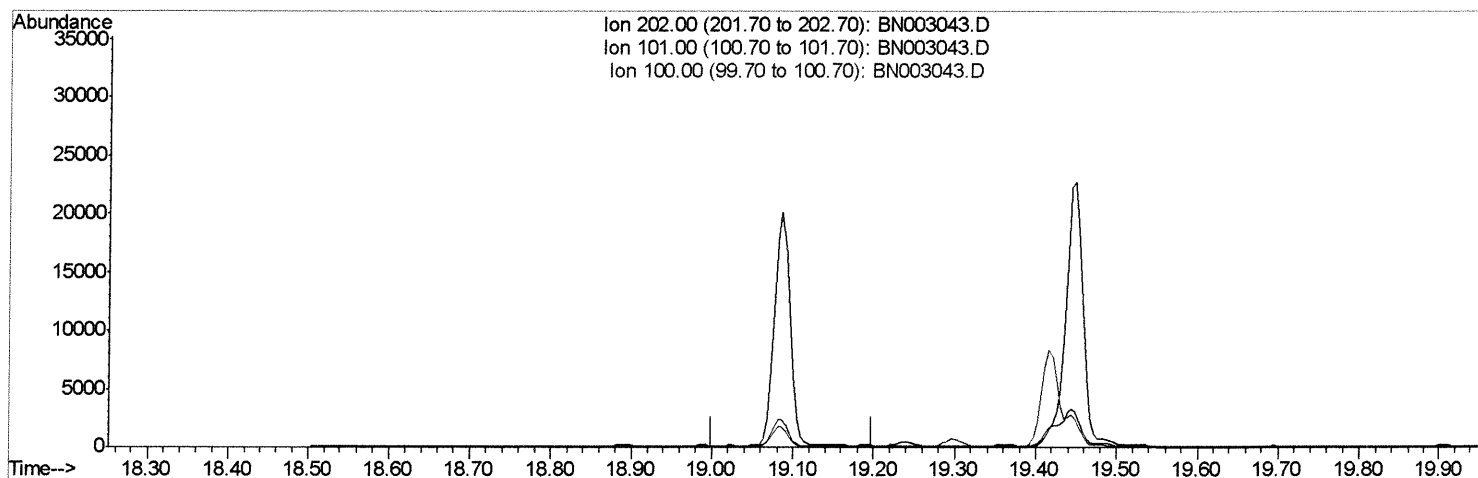

TIC: BN003043.D

(15) Fluoranthene (C)

19.099min (-19.099) 0.00ng/ul

response 0

Ion	Exp%	Act%
202.00	100	0.00
101.00	12.30	0.00
100.00	9.10	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003043.D
 Acq On : 10 Oct 2018 00:47
 Operator : MJ/SJ
 Sample : J5157-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD5

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:54 PM

Quant Time: Oct 10 02:30:35 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

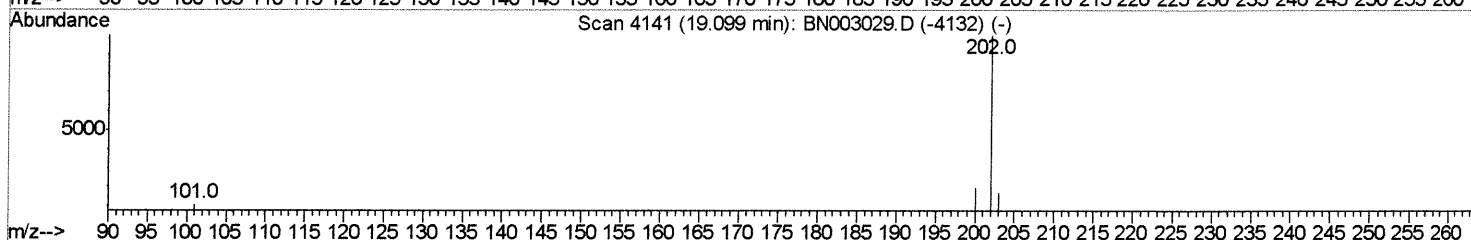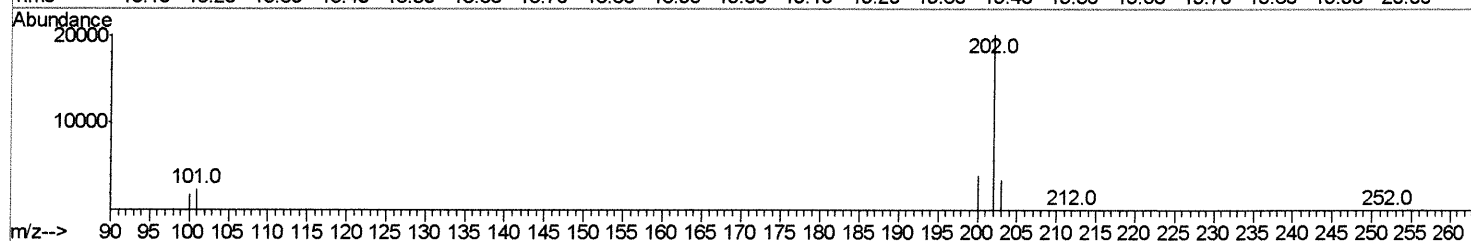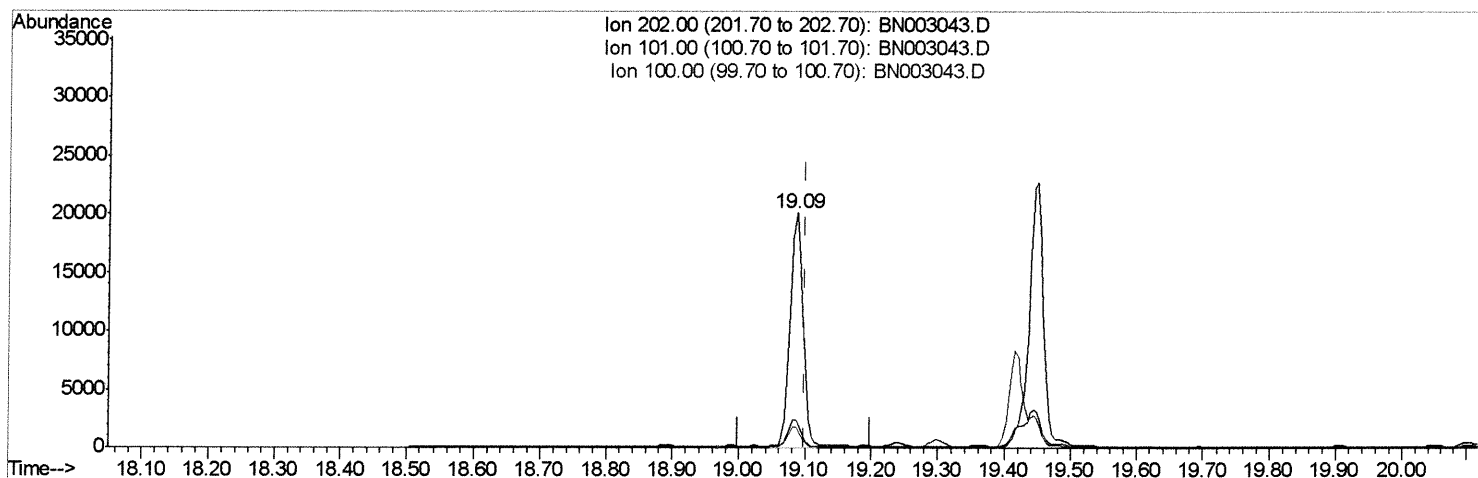

TIC: BN003043.D

(15) Fluoranthene (C)

19.086min (-0.014) 0.81ng/ul m

5/10/12/18

response 27148

Ion	Exp%	Act%
202.00	100	100
101.00	12.30	11.96
100.00	9.10	8.86
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003043.D
Acq On : 10 Oct 2018 00:47
Operator : MJ/SJ
Sample : J5157-13
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD5

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:54 PM

Quant Time: Oct 10 02:30:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

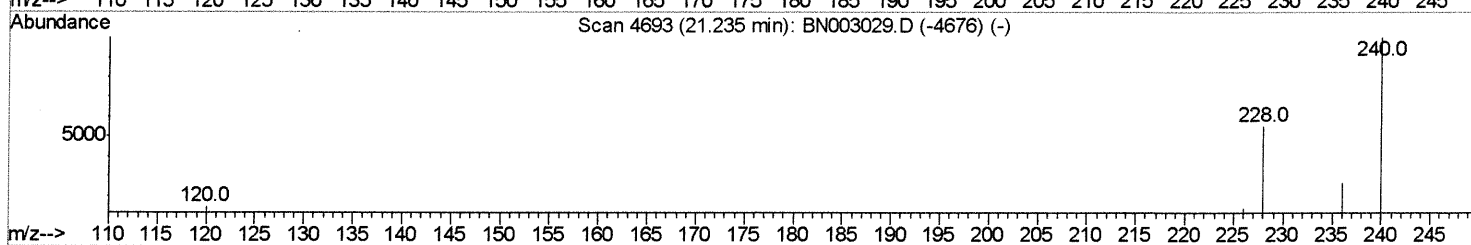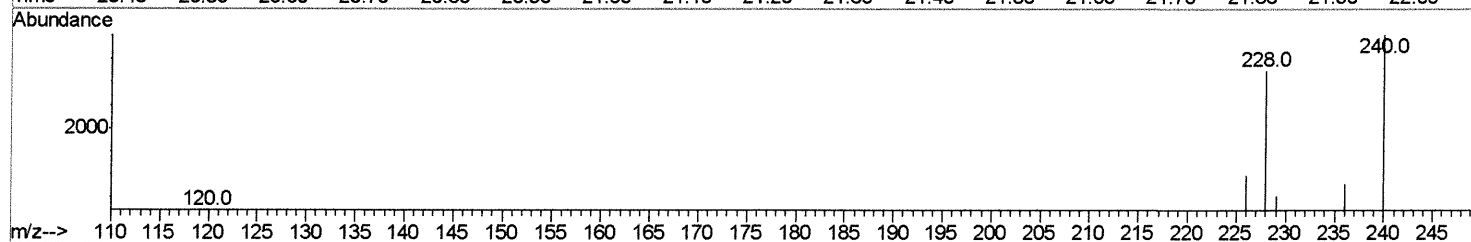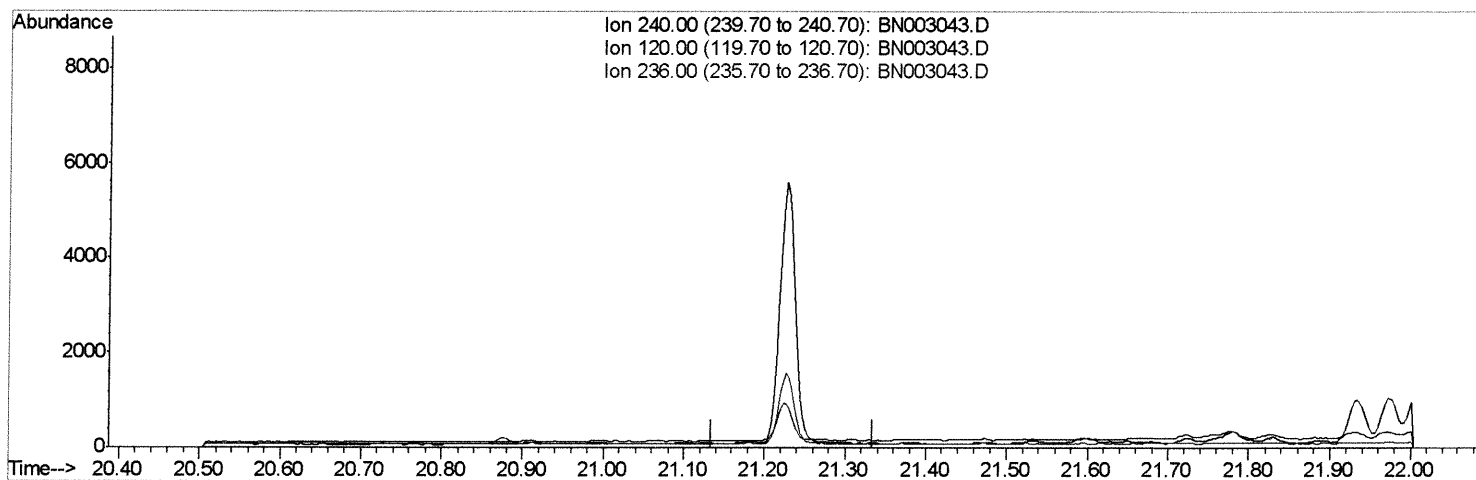

TIC: BN003043.D

(16) Chrysene-d12 (I)

21.235min (-21.235) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	16.40	0.00#
236.00	28.10	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003043.D
Acq On : 10 Oct 2018 00:47
Operator : MJ/SJ
Sample : J5157-13
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD5

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:54 PM

Quant Time: Oct 10 02:30:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

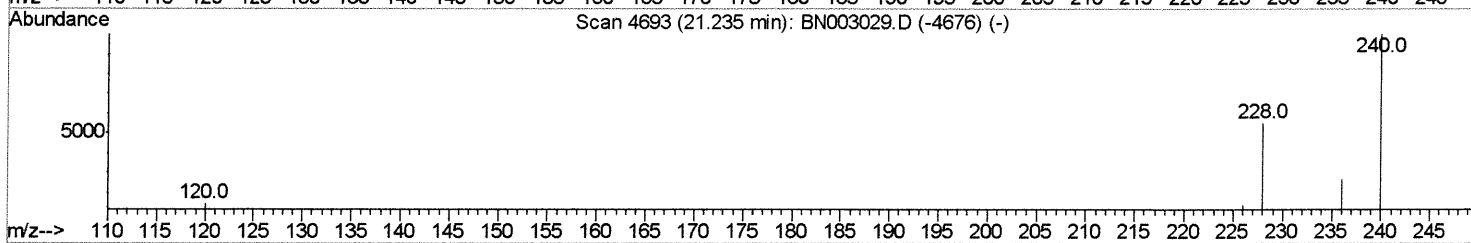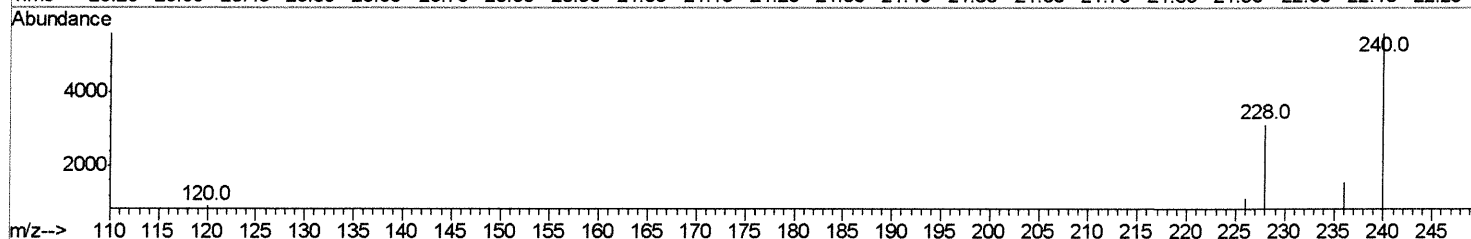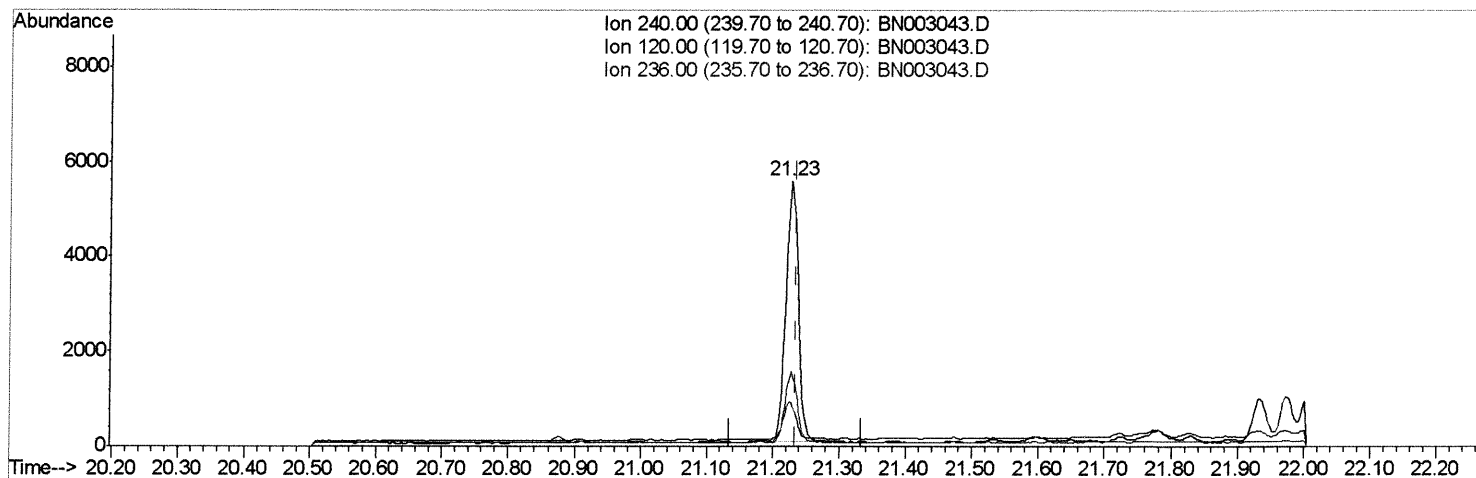

TIC: BN003043.D

(16) Chrysene-d12 (I)

21.226min (-0.009) 0.40ng/ul m

SJ 10/12/18

response 7117

Ion	Exp%	Act%
240.00	100	100
120.00	16.40	16.51
236.00	28.10	28.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003043.D
Acq On : 10 Oct 2018 00:47
Operator : MJ/SJ
Sample : J5157-13
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD5

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:54 PM

Quant Time: Oct 10 02:32:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

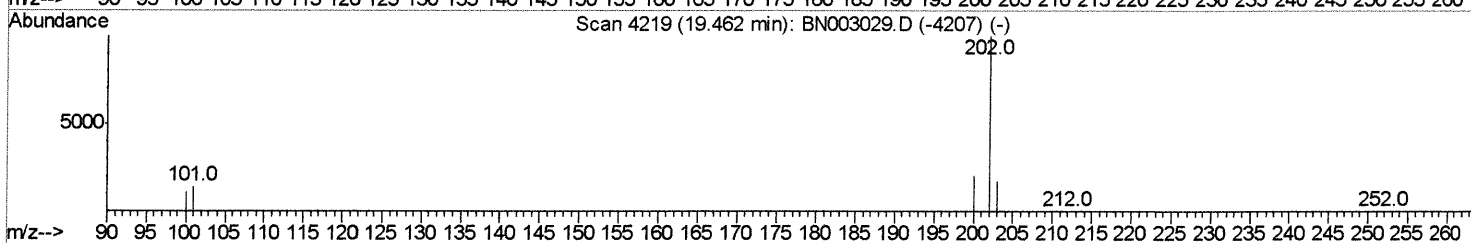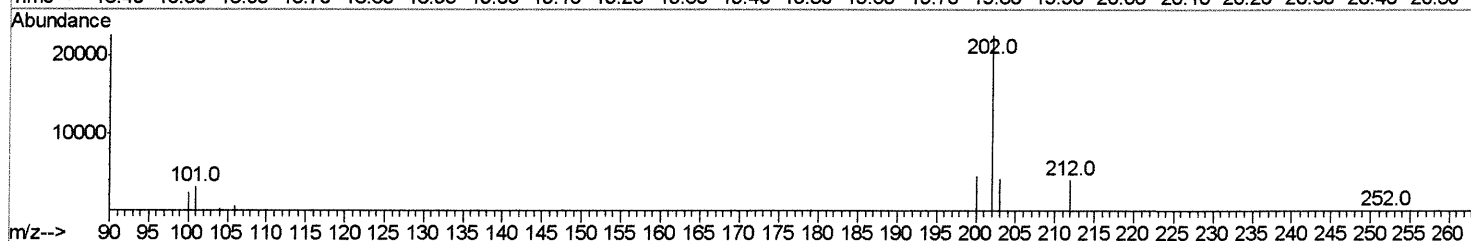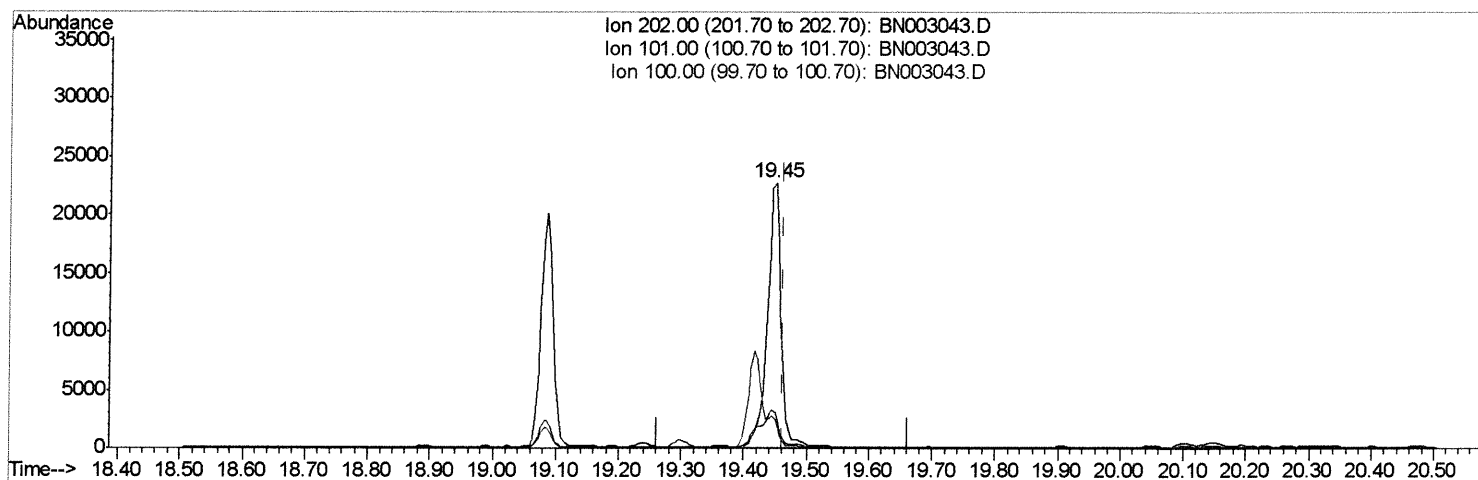

TIC: BN003043.D

(17) Pyrene

19.448min (-0.014) 1.26ng/ul

response 34757

Ion	Exp%	Act%
202.00	100	100
101.00	14.90	13.81
100.00	12.40	10.83
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003043.D
 Acq On : 10 Oct 2018 00:47
 Operator : MJ/SJ
 Sample : J5157-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD5

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:54 PM

Quant Time: Oct 10 02:32:05 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

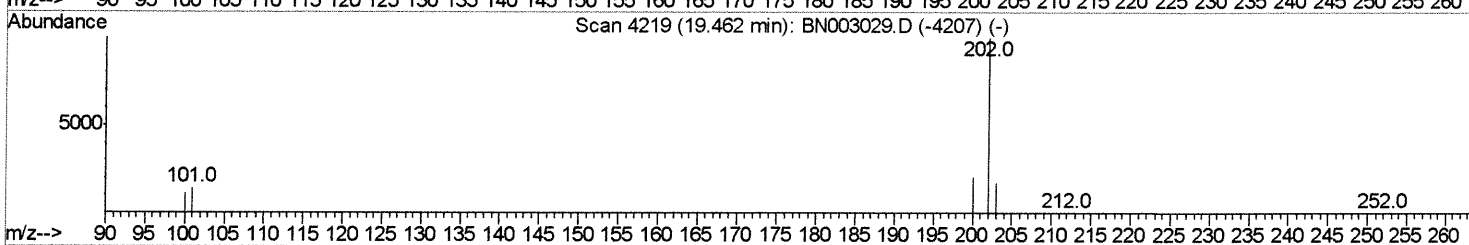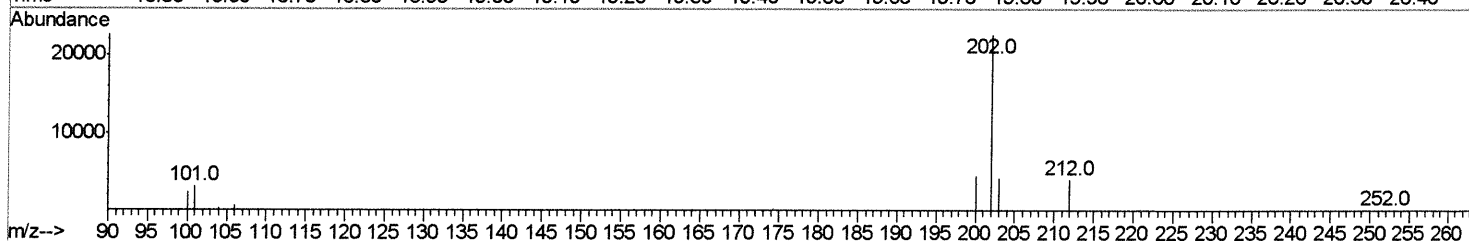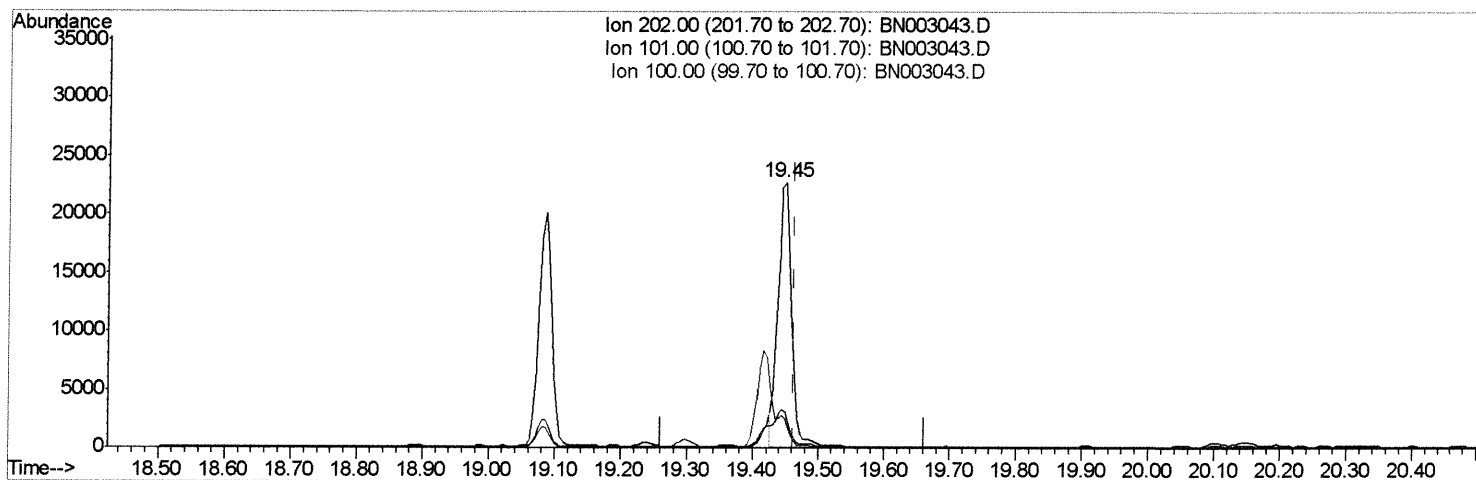

TIC: BN003043.D

(17) Pyrene

19.448min (-0.014) 1.18ng/ul m

SJ 10/12/18

response 32572

Ion	Exp%	Act%
202.00	100	100
101.00	14.90	13.81
100.00	12.40	10.83
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003043.D
Acq On : 10 Oct 2018 00:47
Operator : MJ/SJ
Sample : J5157-13
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD5

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:54 PM

Quant Time: Oct 10 02:32:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

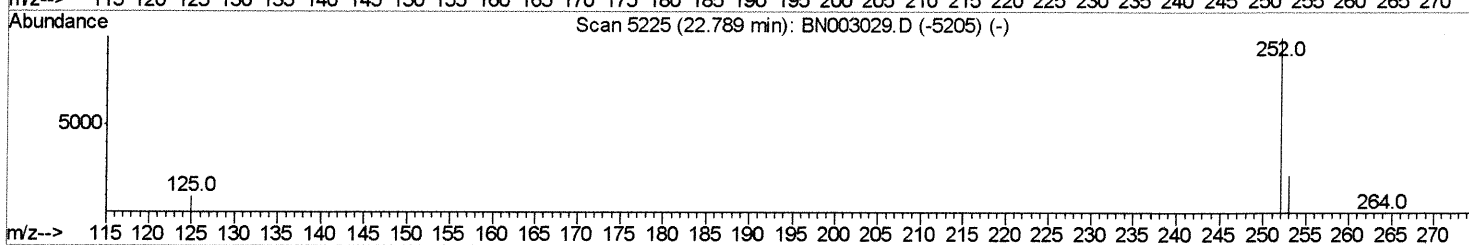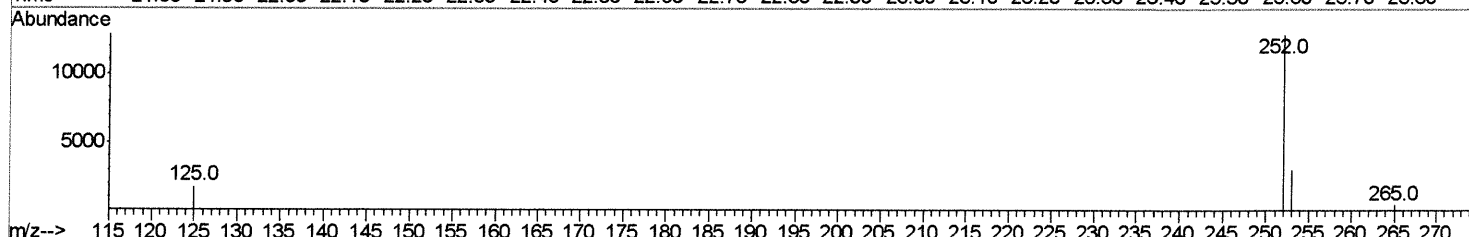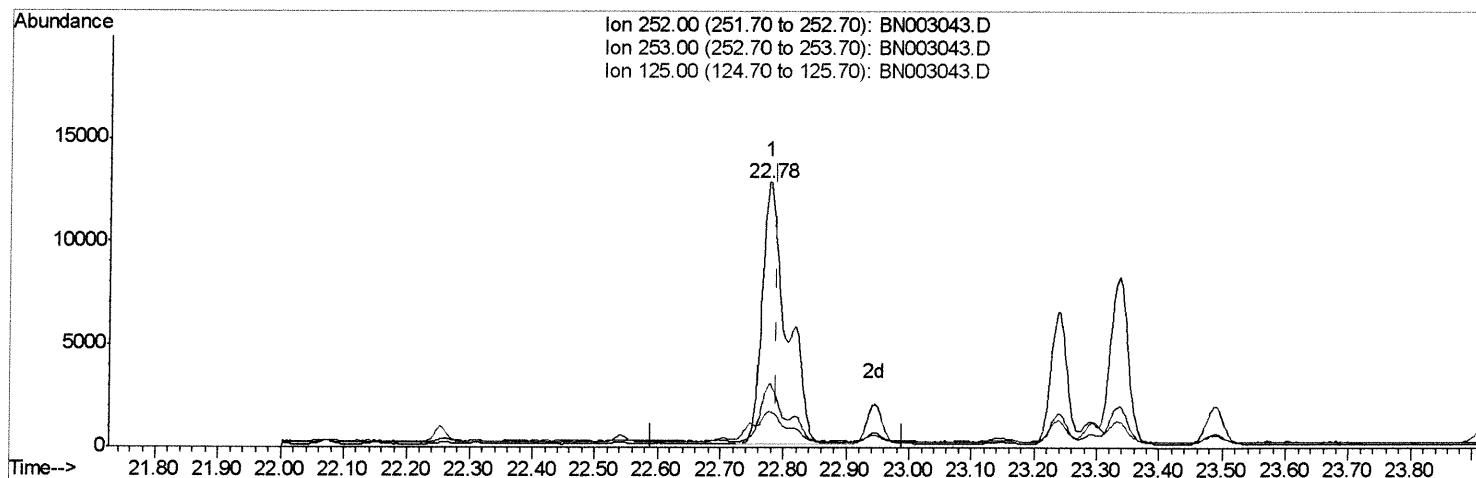

TIC: BN003043.D

(21) Benzo(b)fluoranthene

22.778min (-0.012) 1.47ng/ul

response 35069

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	23.89
125.00	17.10	13.85
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003043.D
 Acq On : 10 Oct 2018 00:47
 Operator : MJ/SJ
 Sample : J5157-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD5

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:54 PM

Quant Time: Oct 10 02:32:05 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

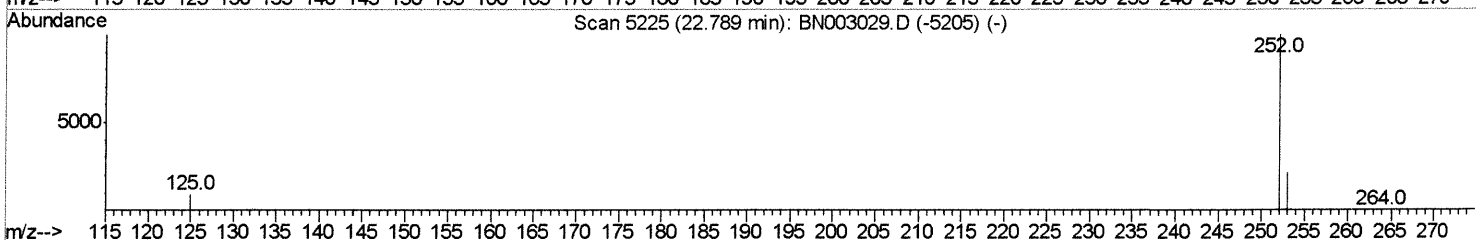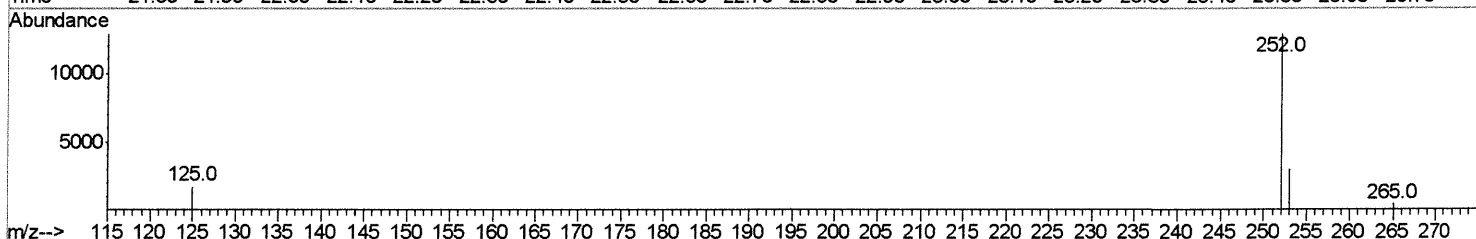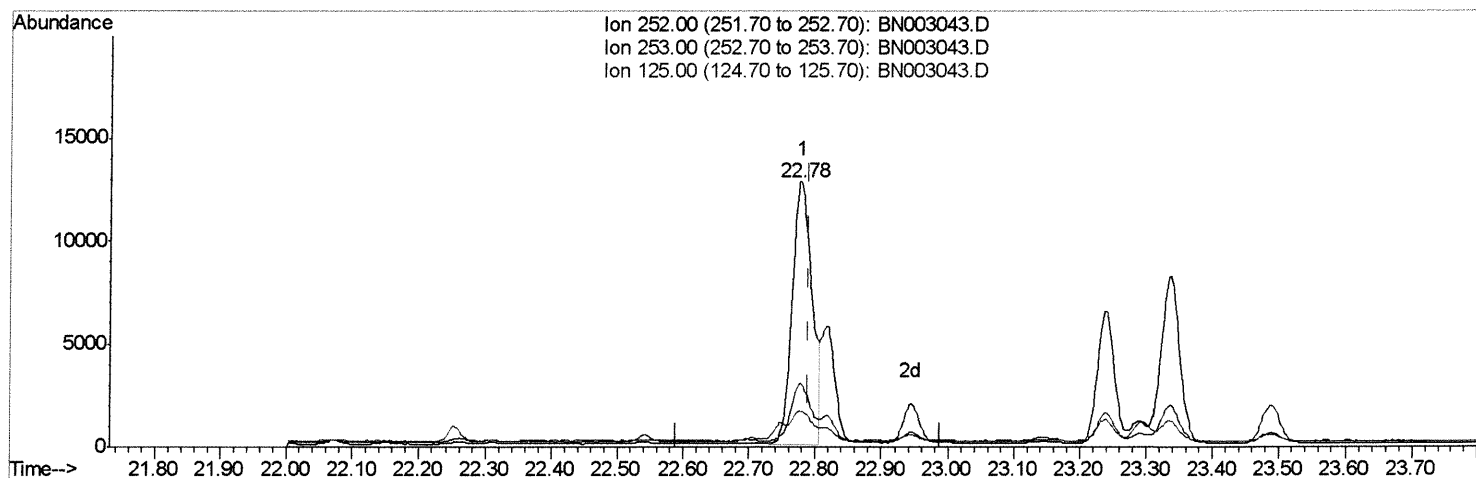

TIC: BN003043.D

(21) Benzo(b)fluoranthene

22.778min (-0.012) 1.11ng/ul m *SJ 10/12/18*

response 26408

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	23.89
125.00	17.10	13.85
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003043.D
Acq On : 10 Oct 2018 00:47
Operator : MJ/SJ
Sample : J5157-13
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD5

Manual Integrations
APPROVED

Sohil
10/10/2018 4:57:54 PM

Quant Time: Oct 10 02:32:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 01:34:31 2018
Response via : Initial Calibration

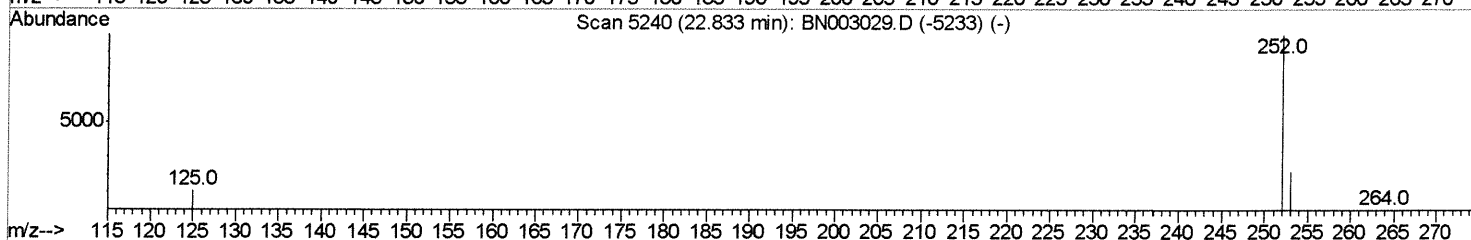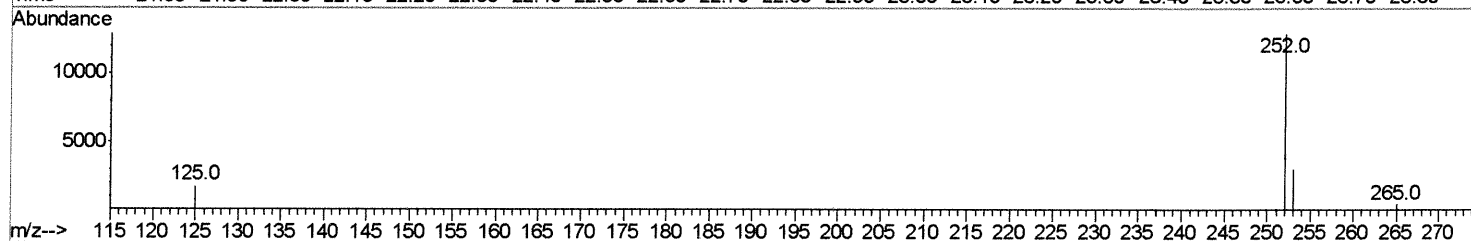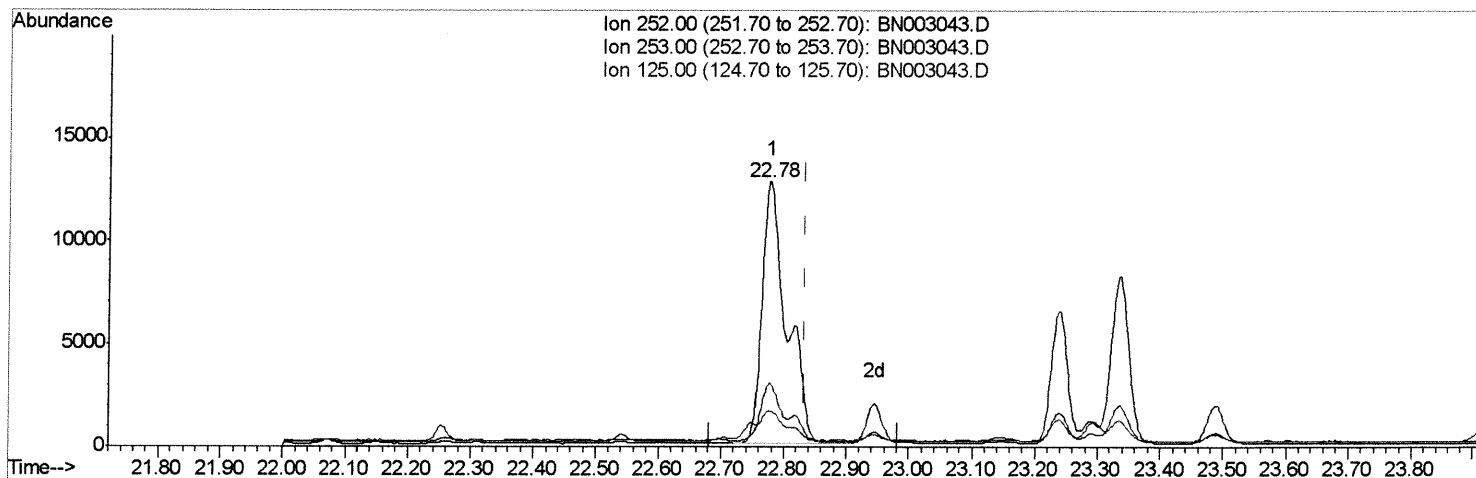

TIC: BN003043.D

(22) Benzo(k)fluoranthene

22.778min (-0.056) 1.42ng/ul

response 35082

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	23.89
125.00	17.60	13.85#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003043.D
 Acq On : 10 Oct 2018 00:47
 Operator : MJ/SJ
 Sample : J5157-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD5

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:54 PM

Quant Time: Oct 10 02:32:05 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

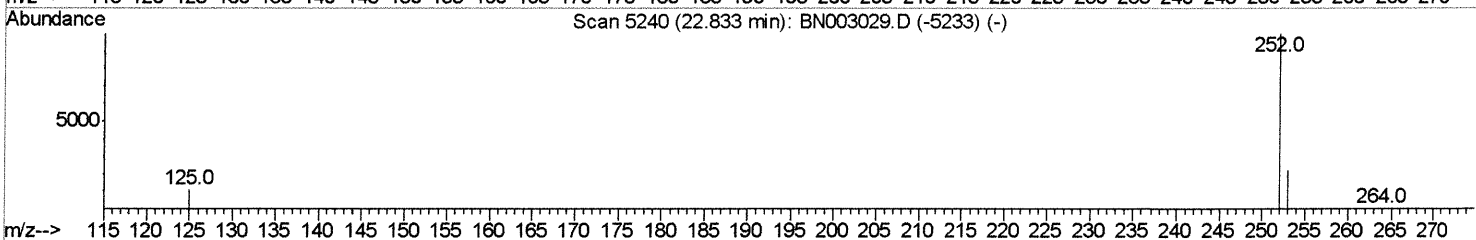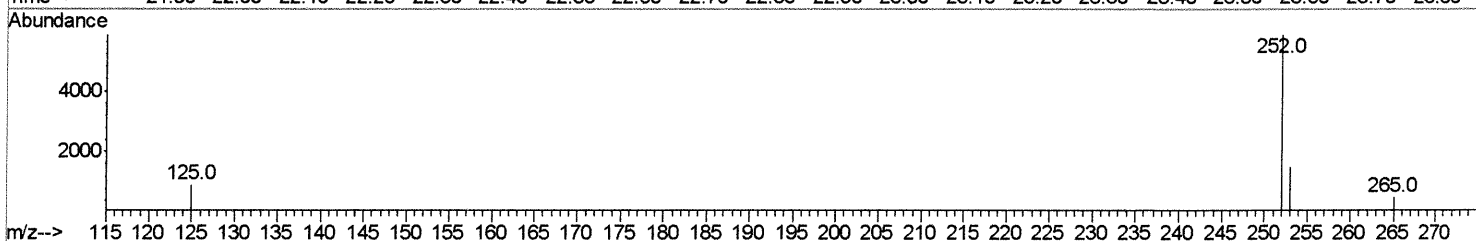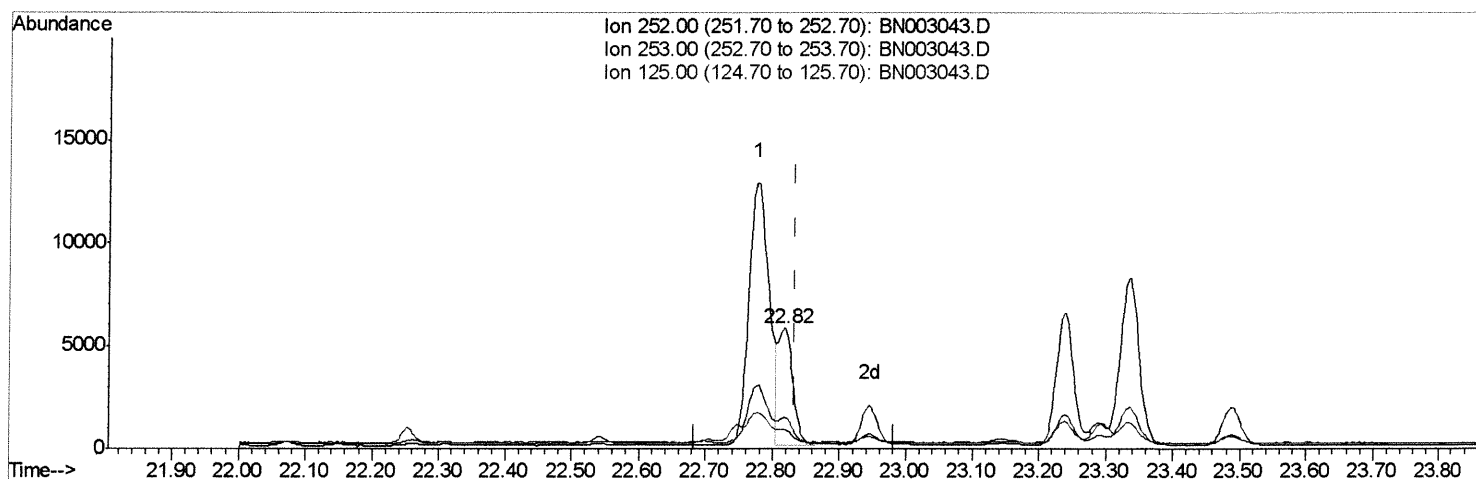

TIC: BN003043.D

(22) Benzo(k)fluoranthene

22.819min (-0.015) 0.35ng/ul m

5710/12/18

response 8547

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	25.61
125.00	17.60	15.62
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003043.D
 Acq On : 10 Oct 2018 00:47
 Operator : MJ/SJ
 Sample : J5157-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD5

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:57:54 PM

Quant Time: Oct 10 02:33:34 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 01:34:31 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	2008	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.39	136	8321	0.40	ng/ul	-0.03
6) Acenaphthene-d10	14.26	164	4898	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.02	188	10234m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.23	240	7117m	0.40	ng/ul	0.00
20) Perylene-d12	23.44	264	6617	0.40	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.01	152	5392	0.42	ng/ul	-0.02
14) Fluoranthene-d10	19.05	212	11768m	0.40	ng/ul	-0.01

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
3) Naphthalene	10.44	128	1348	0.063	ng/ul#	90
7) Acenaphthylene	13.98	152	2005	0.089	ng/ul#	92
12) Phenanthrene	17.06	178	1350m	0.047	ng/ul	
13) Anthracene	17.15	178	2432m	0.090	ng/ul	
15) Fluoranthene	19.09	202	27148m	0.811	ng/ul	
17) Pyrene	19.45	202	32572m	1.178	ng/ul	
18) Benzo(a)anthracene	21.21	228	11779	0.514	ng/ul	98
19) Chrysene	21.26	228	13351	0.574	ng/ul	98
21) Benzo(b)fluoranthene	22.78	252	26408m	1.108	ng/ul	
22) Benzo(k)fluoranthene	22.82	252	8547m	0.346	ng/ul	
23) Benzo(a)pyrene	23.34	252	16292	0.763	ng/ul#	90
24) Indeno(1,2,3-cd)pyrene	25.66	276	9157	0.373	ng/ul#	93
25) Dibenzo(a,h)anthracene	25.65	278	2743	0.140	ng/ul#	82
26) Benzo(a,h,i)perylene	26.33	276	8631	0.417	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed