

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003049.D
 Acq On : 10 Oct 2018 04:20
 Operator : MJ/SJ
 Sample : J5115-17
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC60

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:58:19 PM

Quant Time: Oct 10 09:02:30 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 08:36:11 2018
 Response via : Initial Calibration

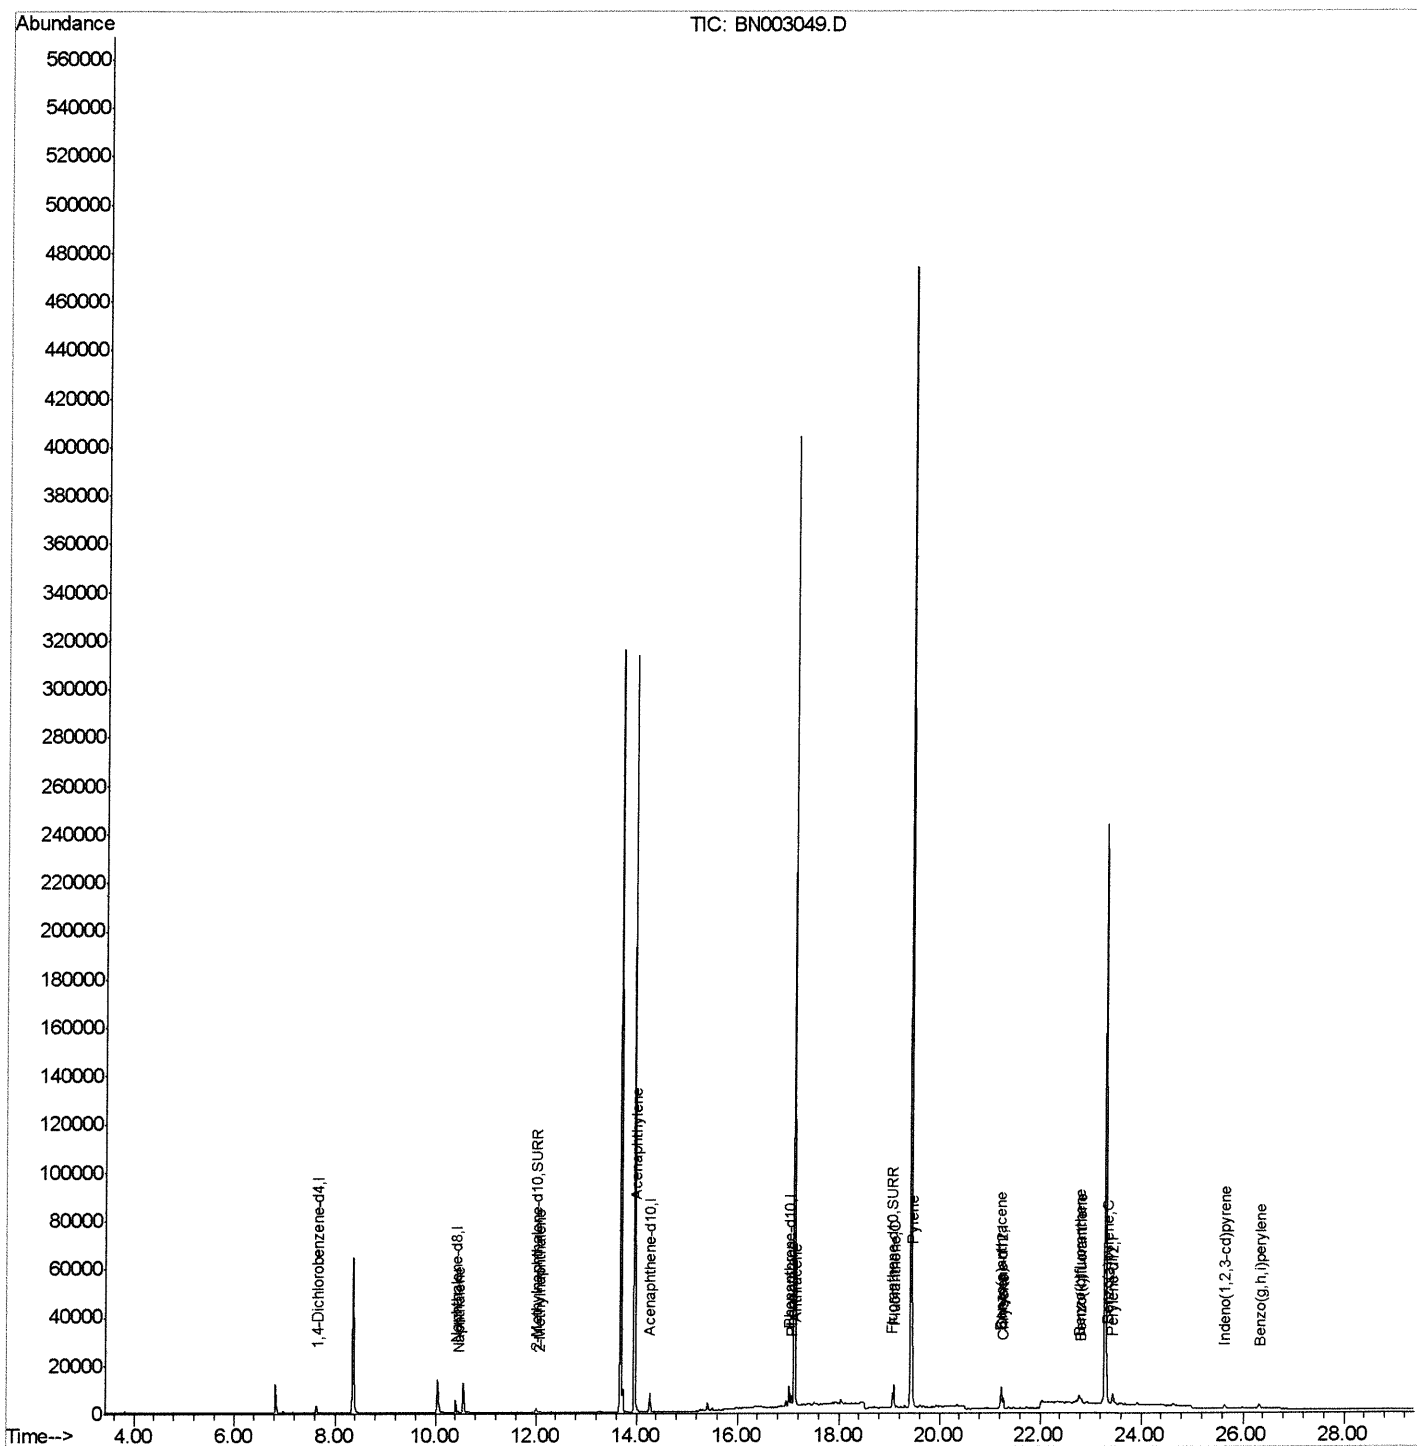

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003049.D
 Acq On : 10 Oct 2018 04:20
 Operator : MJ/SJ
 Sample : J5115-17
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC60

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:58:19 PM

Quant Time: Oct 10 08:38:58 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 08:36:11 2018
 Response via : Initial Calibration

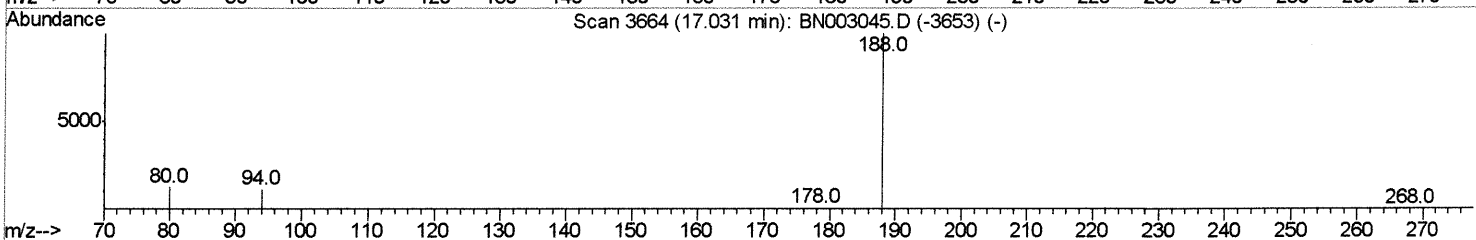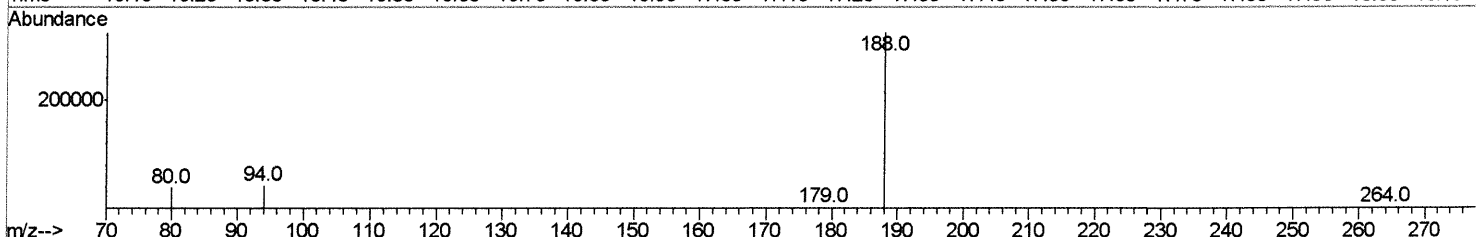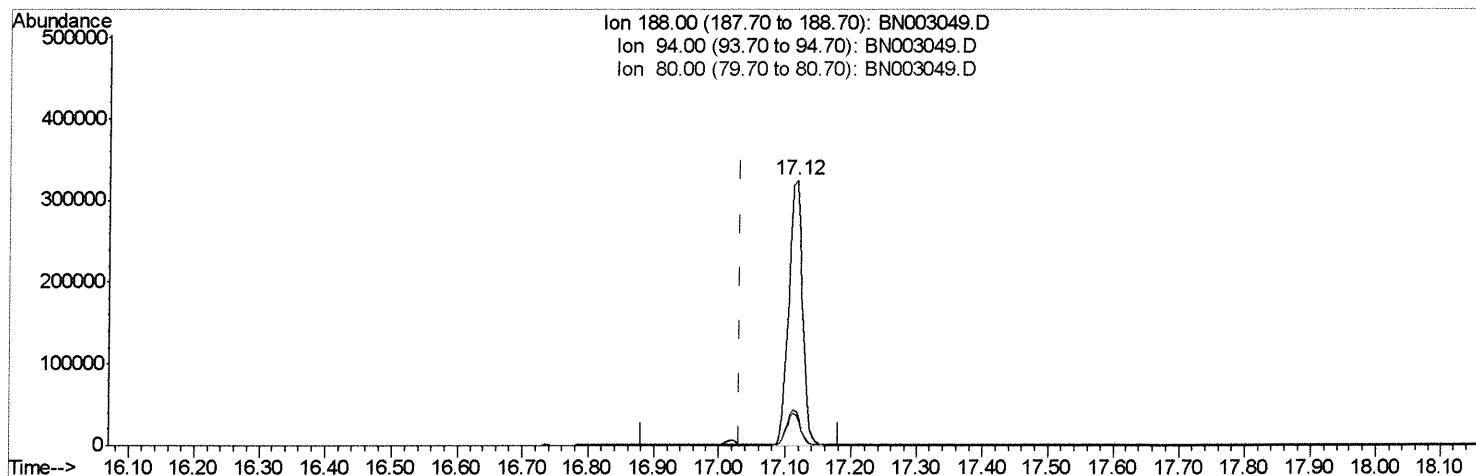

TIC: BN003049.D

(10) Phenanthrene-d10 (I)
 17.116min (+0.085) 0.40ng/ul
 response 466256

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	12.72
80.00	12.70	11.43
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003049.D
 Acq On : 10 Oct 2018 04:20
 Operator : MJ/SJ
 Sample : J5115-17
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC60

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:58:19 PM

Quant Time: Oct 10 08:38:58 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 08:36:11 2018
 Response via : Initial Calibration

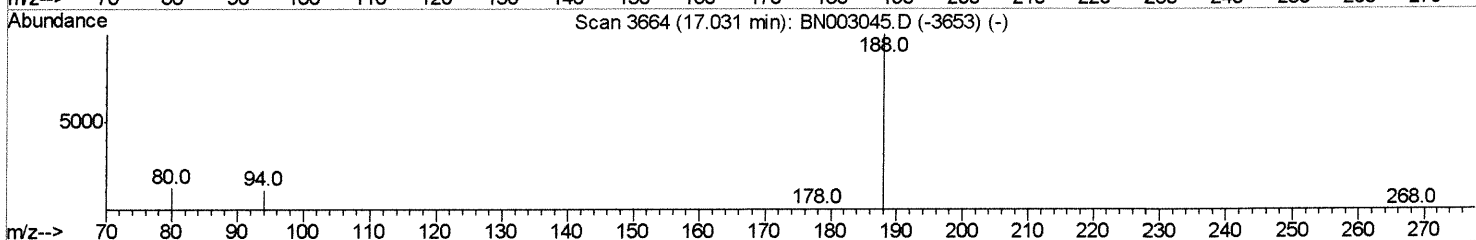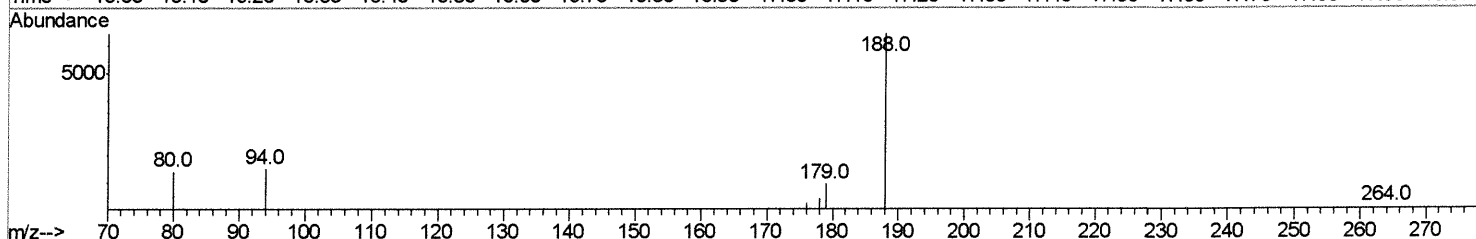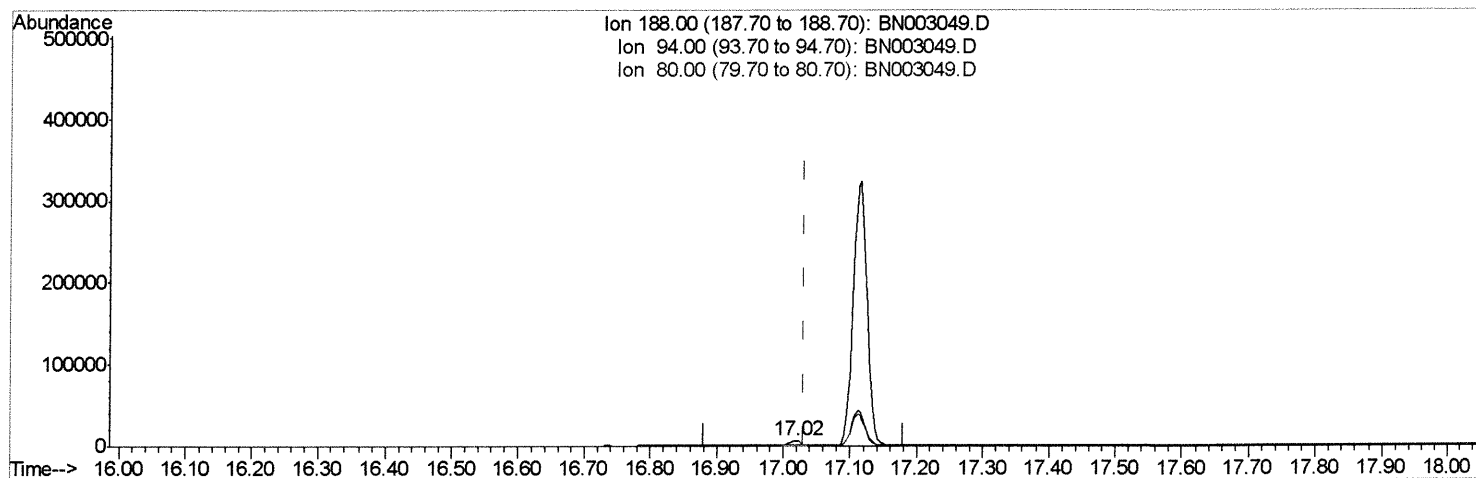

TIC: BN003049.D

(10) Phenanthrene-d10 (I)

17.019min (-0.013) 0.40ng/ul m

5110/12/18

response 9564

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	23.82#
80.00	12.70	22.23#
0.00	0.00	0.00

```

Data Path   : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File   : BN003049.D
Acq On      : 10 Oct 2018   04:20
Operator    : MJ/SJ
Sample      : J5115-17
Misc        :
ALS Vial    : 21      Sample Multiplier: 1

```

Sohil
10/10/2018 4:58:19 PM



Abundance

Ion 178.00 (177.70 to 178.70): BN003049.D
Ion 179.00 (178.70 to 179.70): BN003049.D
Ion 176.00 (175.70 to 176.70): BN003049.D

5000
4000
3000
2000
1000
0

2d
1
17.15

Time--> 16.20 16.30 16.40 16.50 16.60 16.70 16.80 16.90 17.00 17.10 17.20 17.30 17.40 17.50 17.60 17.70 17.80 17.90 18.00 18.10

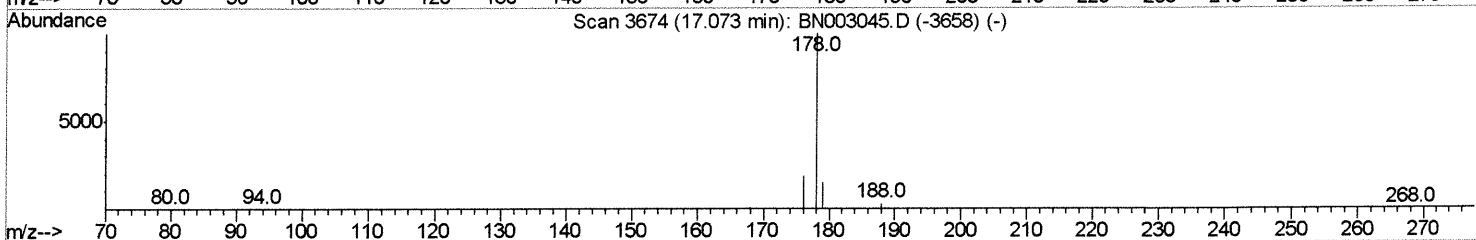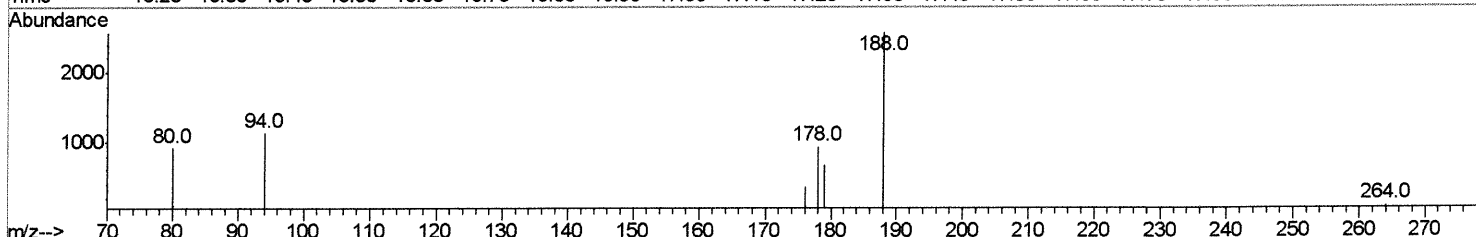

(12) Phenanthrene
17.150min (+0.076) 0.03ng/ul
response 866

Ion	Exp%	Act%
178.00	100	100
179.00	16.10	71.50#
176.00	19.30	39.06#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003049.D
Acq On : 10 Oct 2018 04:20
Operator : MJ/SJ
Sample : J5115-17
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC60

Manual Integrations
APPROVED

Sohil
10/10/2018 4:58:19 PM

Quant Time: Oct 10 08:59:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 08:36:11 2018
Response via : Initial Calibration

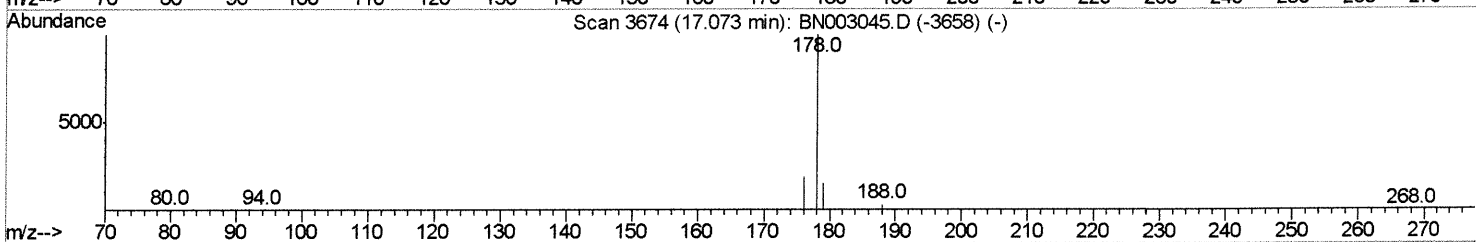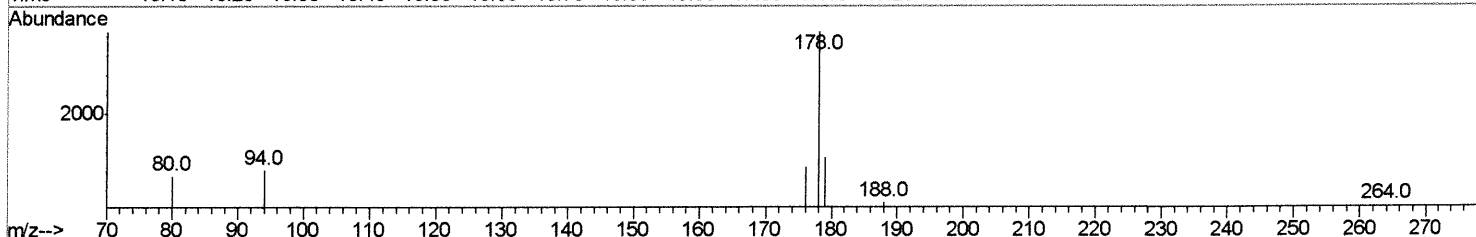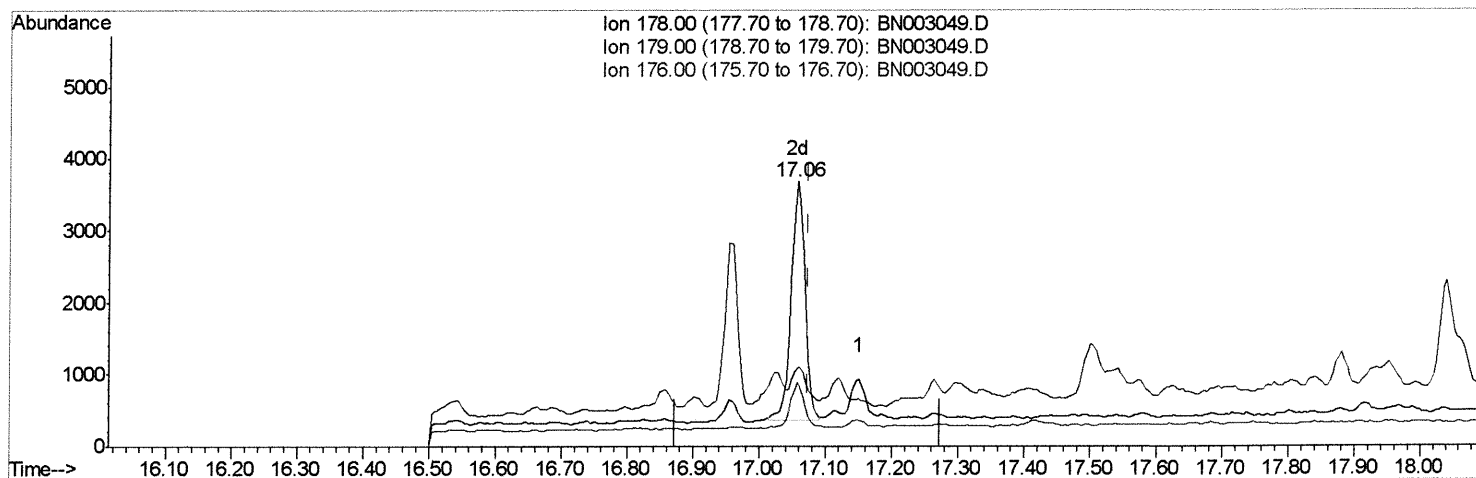

TIC: BN003049.D

(12) Phenanthrene

17.057min (-0.017) 0.18ng/ul m

SJ 10/12/18

response 4817

Ion	Exp%	Act%
178.00	100	100
179.00	16.10	29.48#
176.00	19.30	24.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003049.D
Acq On : 10 Oct 2018 04:20
Operator : MJ/SJ
Sample : J5115-17
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
JLC60

Manual Integrations
APPROVED

Sohil
10/10/2018 4:58:19 PM

Quant Time: Oct 10 08:59:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 08:36:11 2018
Response via : Initial Calibration

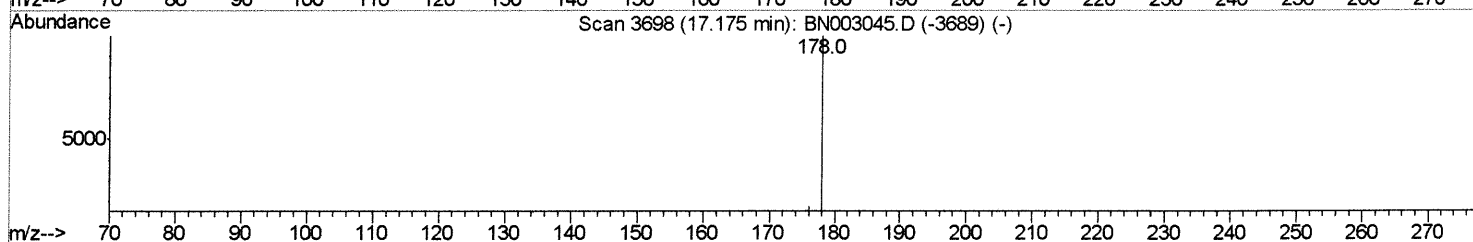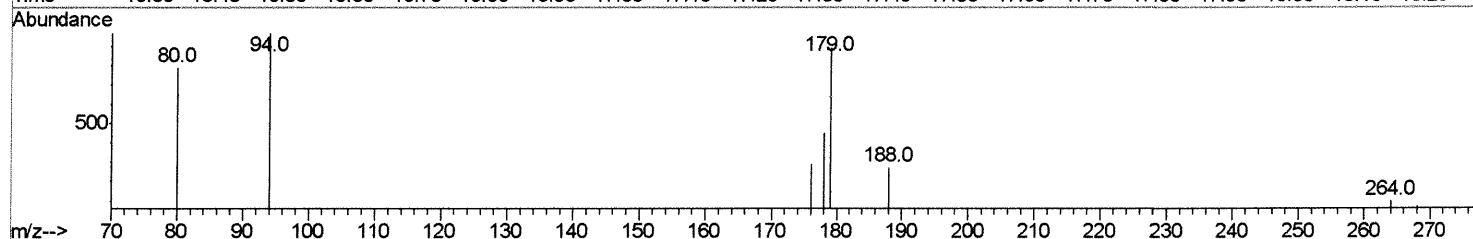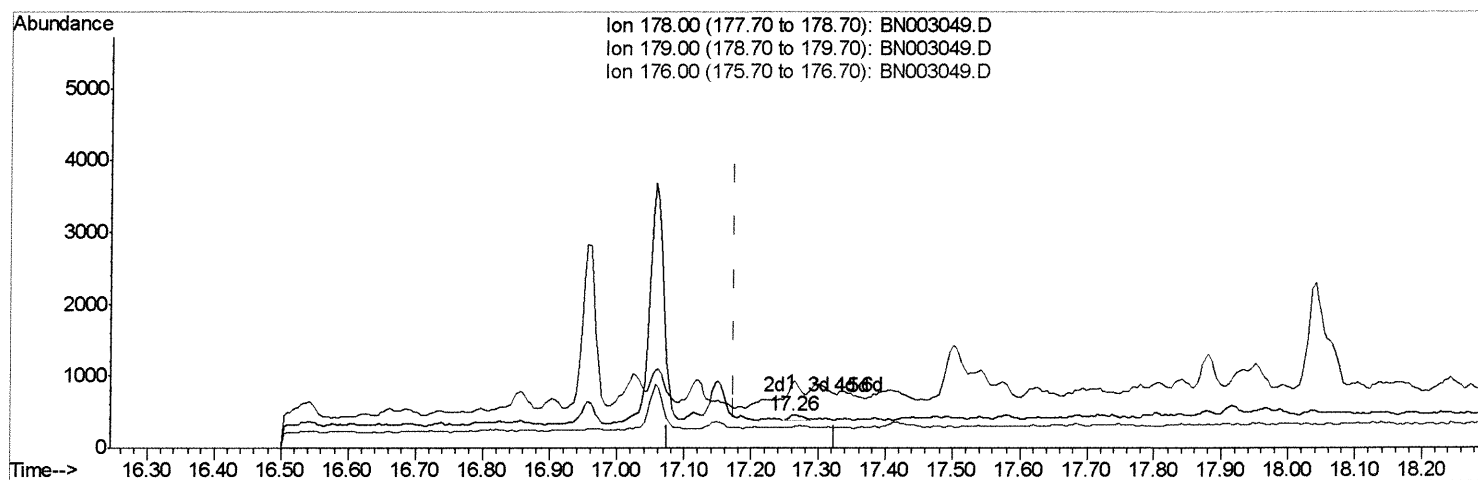

TIC: BN003049.D

(13) Anthracene

17.259min (+0.085) 0.00ng/ul

response 104

Ion	Exp%	Act%
178.00	100	100
179.00	16.30	197.12#
176.00	19.10	63.50#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003049.D
Acq On : 10 Oct 2018 04:20
Operator : MJ/SJ
Sample : J5115-17
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC60

Manual Integrations
APPROVED

Sohil
10/10/2018 4:58:19 PM

Quant Time: Oct 10 08:59:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 08:36:11 2018
Response via : Initial Calibration

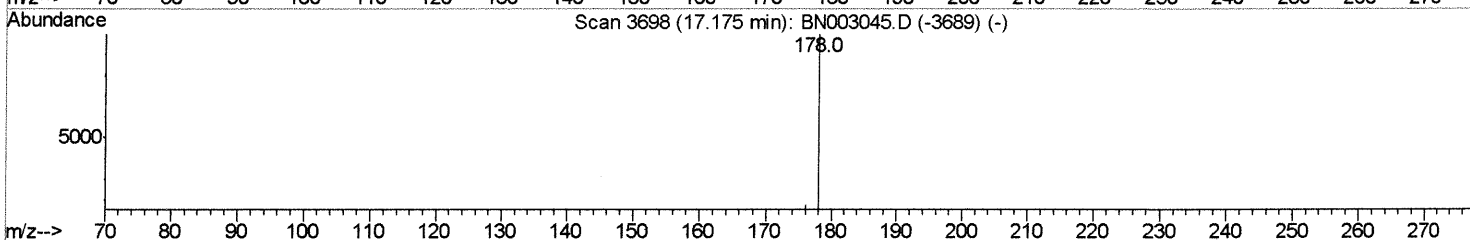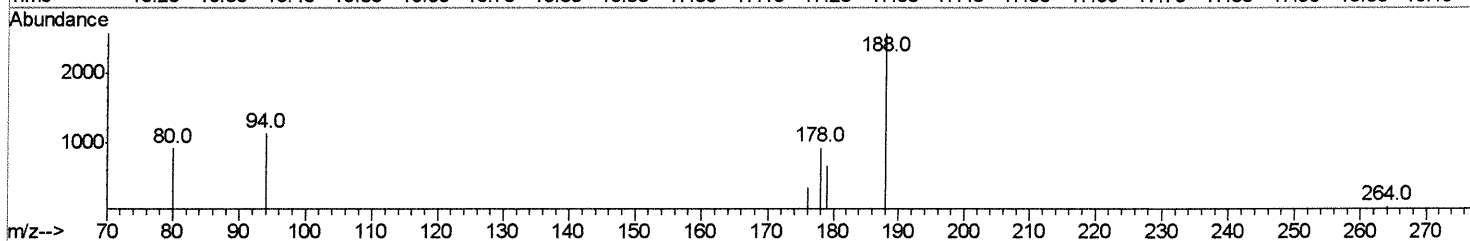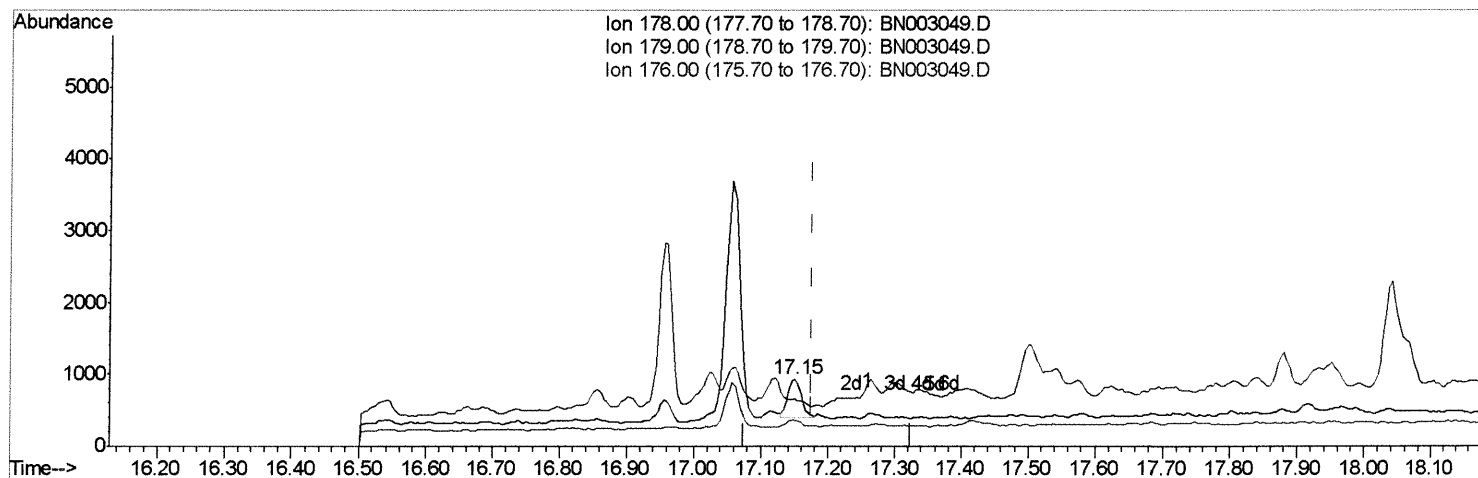

TIC: BN003049.D

(13) Anthracene

17.150min (-0.025) 0.03ng/ul m

5/10/12/18

response 743

Ion	Exp%	Act%
178.00	100	100
179.00	16.30	71.50#
176.00	19.10	39.06#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003049.D
 Acq On : 10 Oct 2018 04:20
 Operator : MJ/SJ
 Sample : J5115-17
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC60

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:58:19 PM

Quant Time: Oct 10 08:59:30 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 08:36:11 2018
 Response via : Initial Calibration

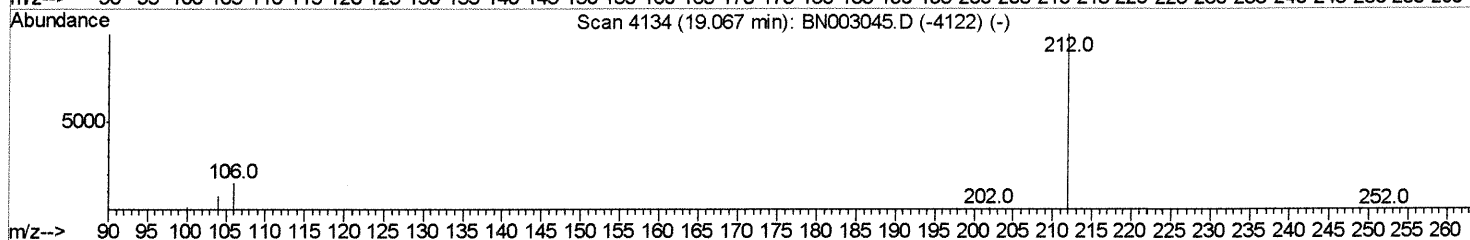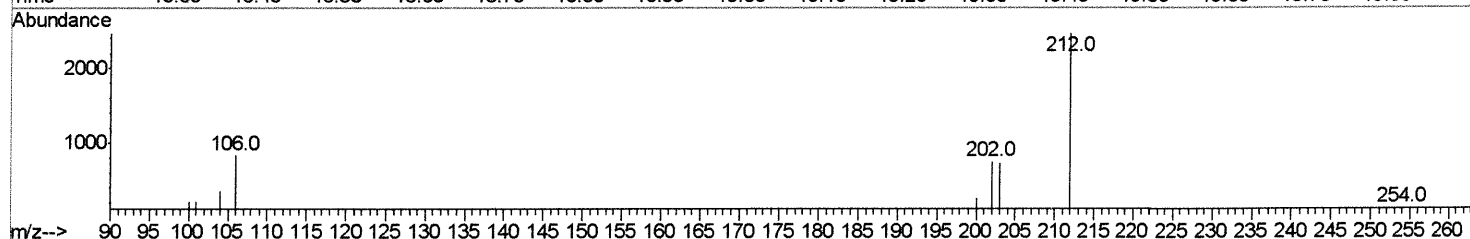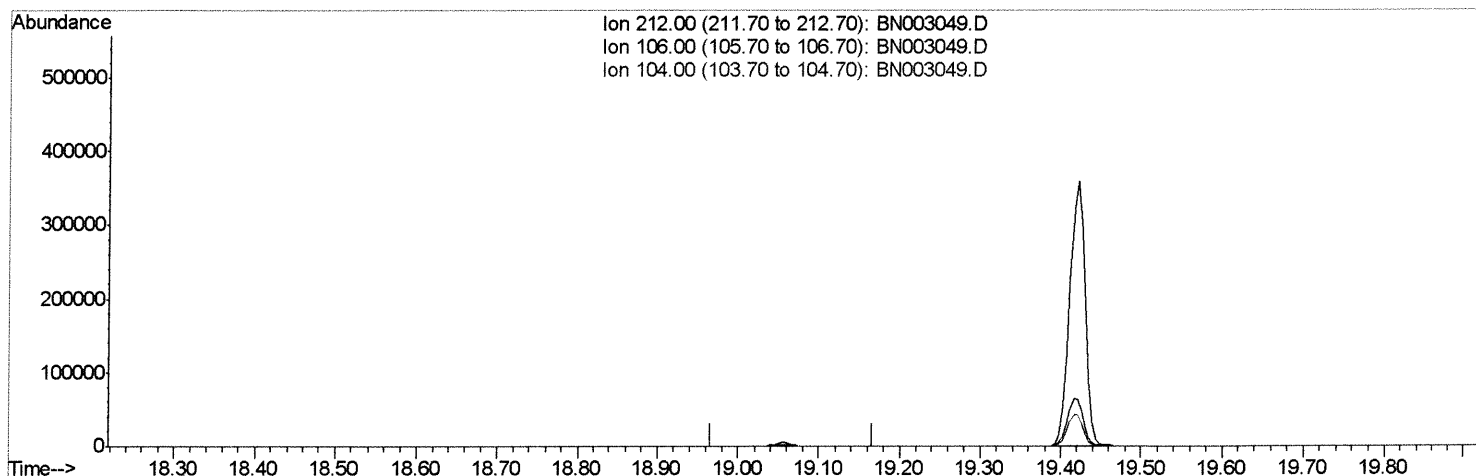

TIC: BN003049.D

(14) Fluoranthene-d10 (SURR)

19.067min (-19.067) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	15.40	0.00#
104.00	8.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003049.D
 Acq On : 10 Oct 2018 04:20
 Operator : MJ/SJ
 Sample : J5115-17
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC60

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:58:19 PM

Quant Time: Oct 10 08:59:30 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 08:36:11 2018
 Response via : Initial Calibration

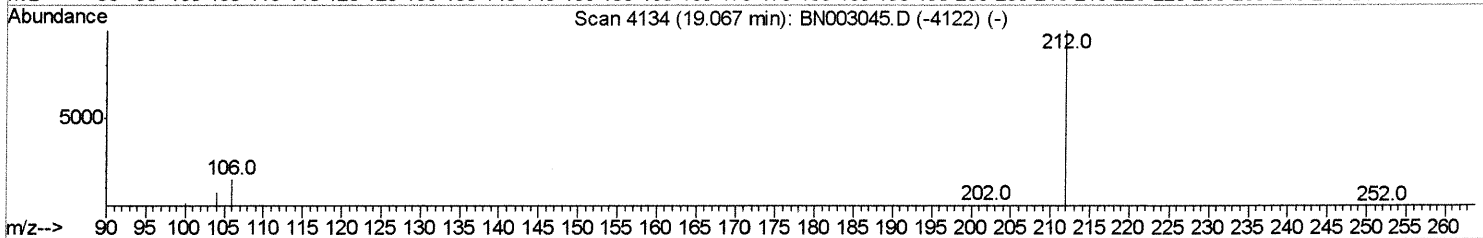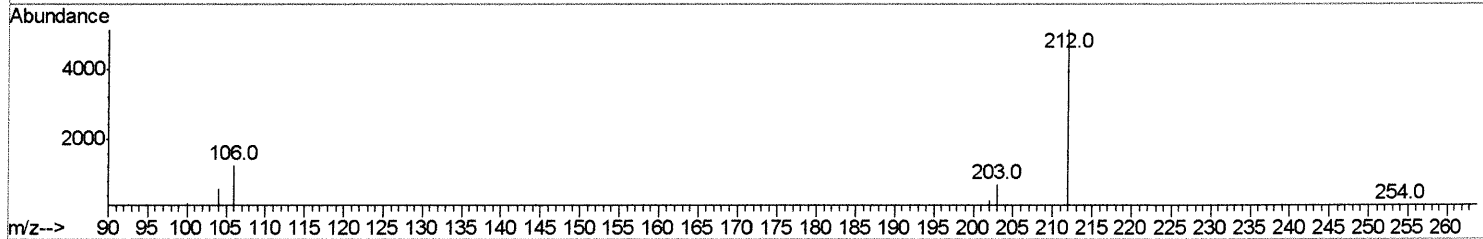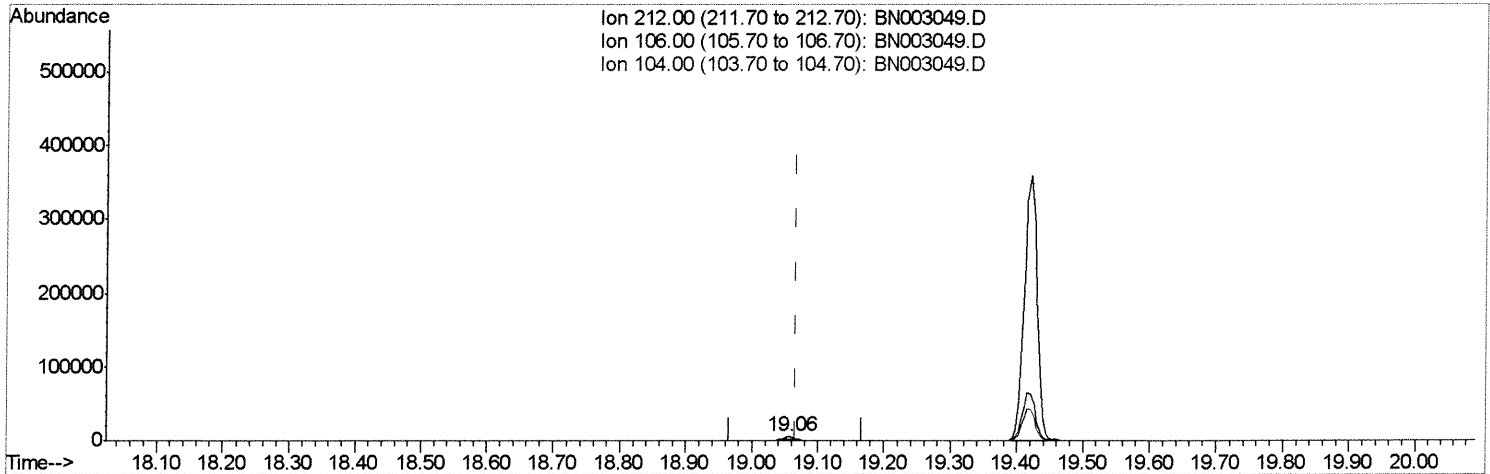

TIC: BN003049.D

(14) Fluoranthene-d10 (SURR)

19.058min (-0.009) 0.26ng/ul m *SJ 10/12/18*

response 7188

Ion	Exp%	Act%
212.00	100	100
106.00	15.40	0.00#
104.00	8.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003049.D
 Acq On : 10 Oct 2018 04:20
 Operator : MJ/SJ
 Sample : J5115-17
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC60

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:58:19 PM

Quant Time: Oct 10 08:59:30 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 08:36:11 2018
 Response via : Initial Calibration

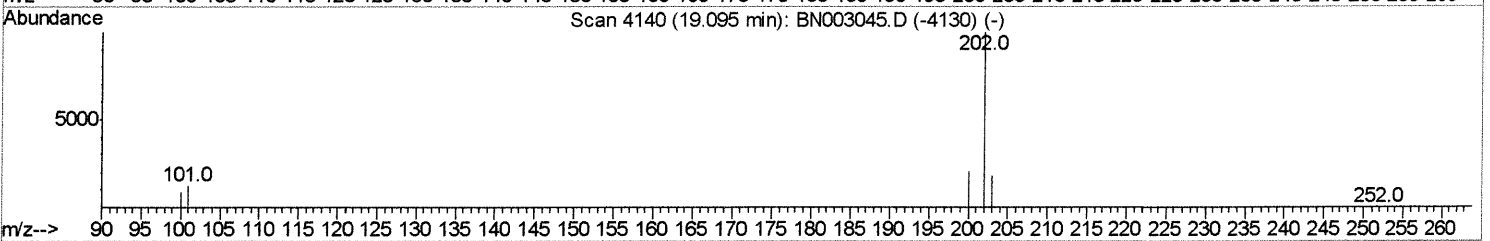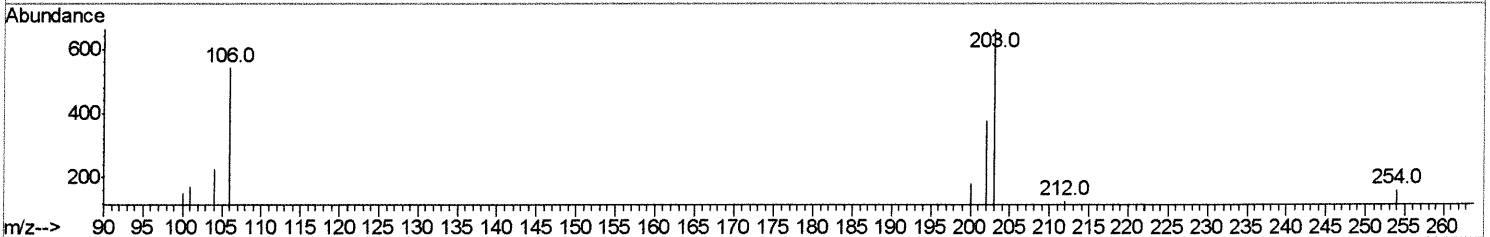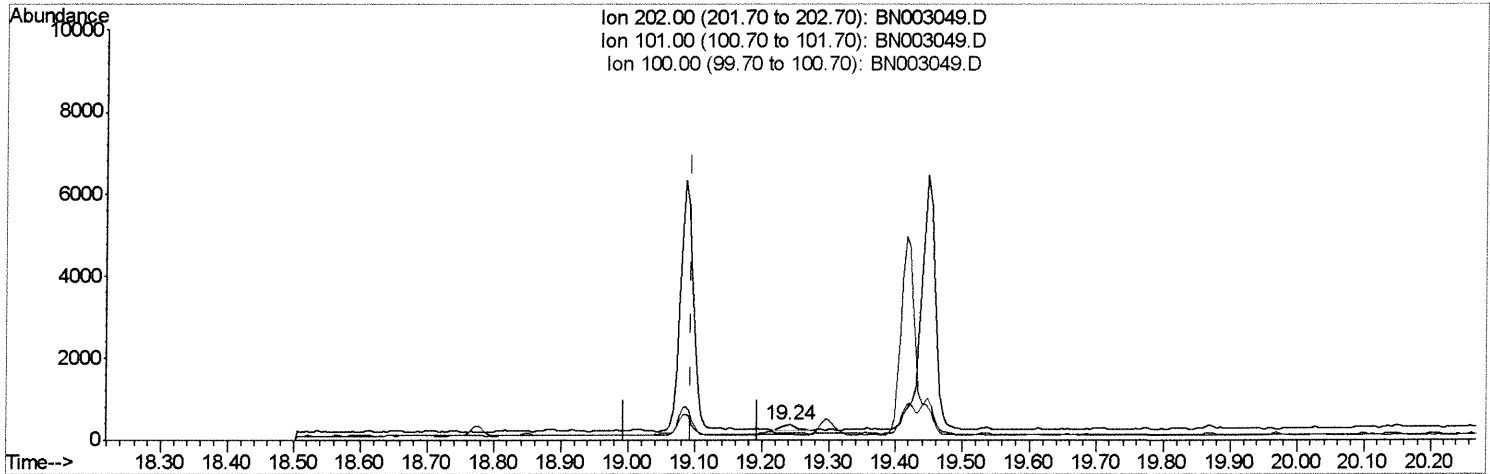

TIC: BN003049.D

(15) Fluoranthene (C)

19.239min (+0.144) 0.01ng/ul

response 202

Ion	Exp%	Act%
202.00	100	100
101.00	12.30	44.85#
100.00	9.10	40.63#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003049.D
 Acq On : 10 Oct 2018 04:20
 Operator : MJ/SJ
 Sample : J5115-17
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC60

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:58:19 PM

Quant Time: Oct 10 08:59:30 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 08:36:11 2018
 Response via : Initial Calibration

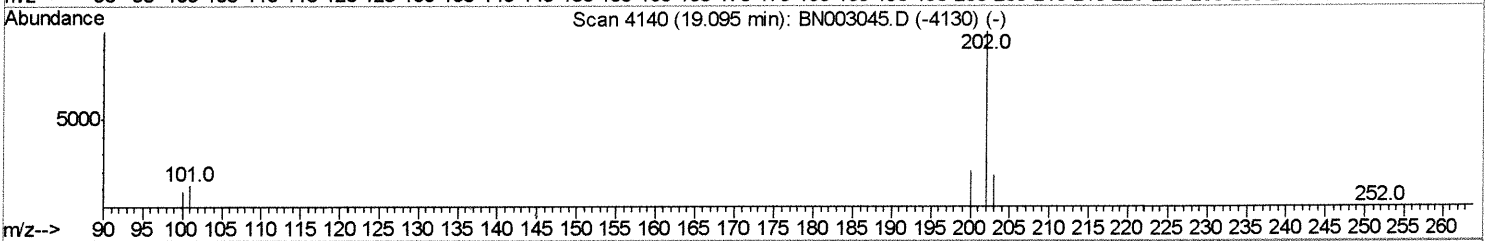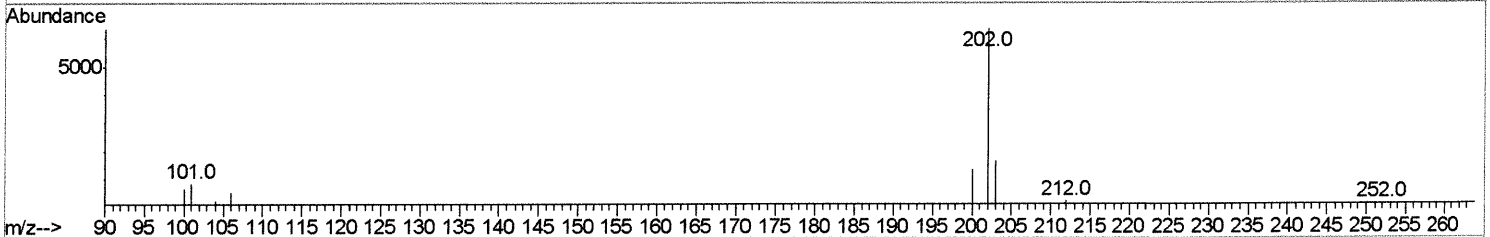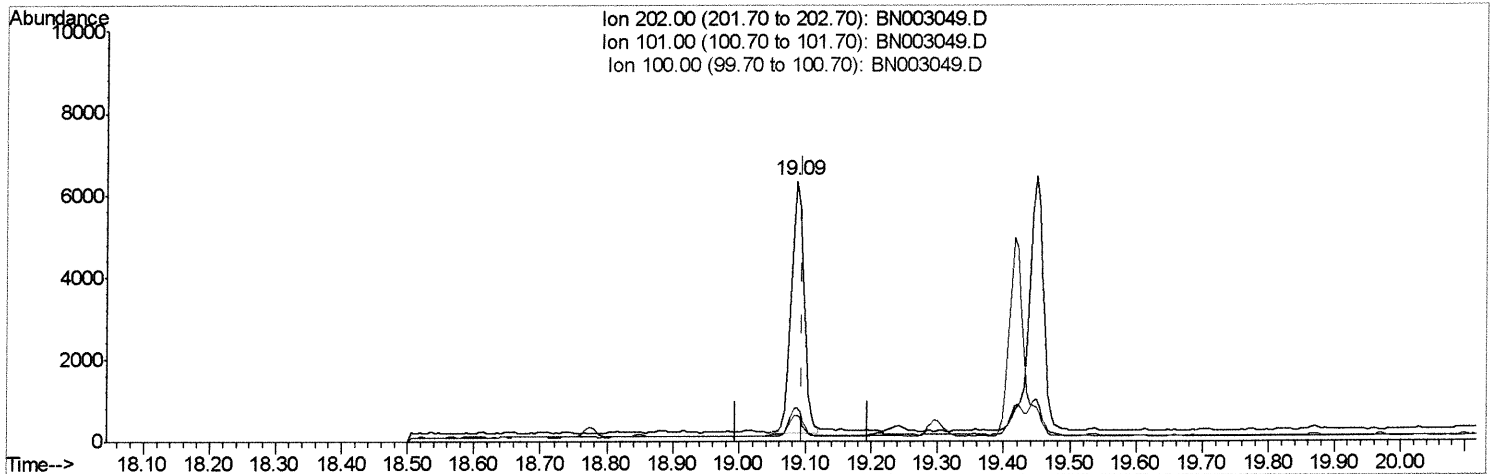

TIC: BN003049.D

(15) Fluoranthene (C)

19.086min (-0.009) 0.27ng/ul m

SJ 10/12/18

response 8367

Ion	Exp%	Act%
202.00	100	100
101.00	12.30	13.17
100.00	9.10	10.20
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003049.D
 Acq On : 10 Oct 2018 04:20
 Operator : MJ/SJ
 Sample : J5115-17
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC60

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:58:19 PM

Quant Time: Oct 10 08:59:30 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 08:36:11 2018
 Response via : Initial Calibration

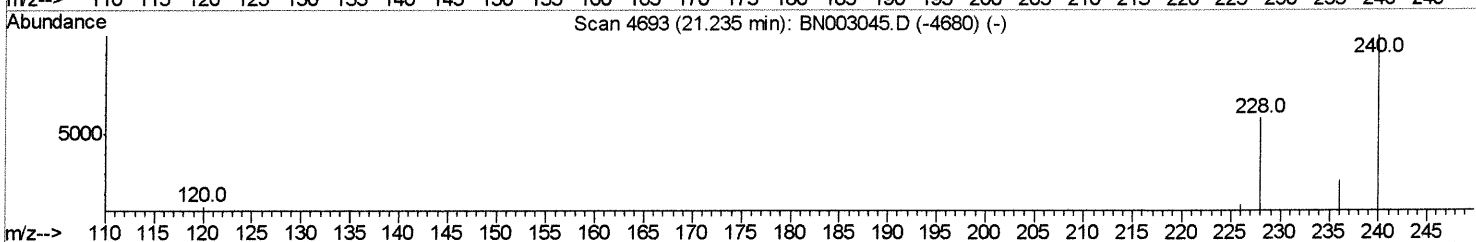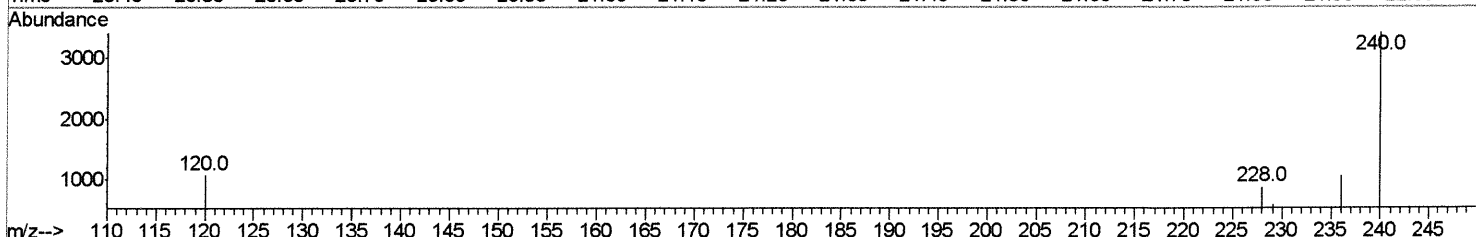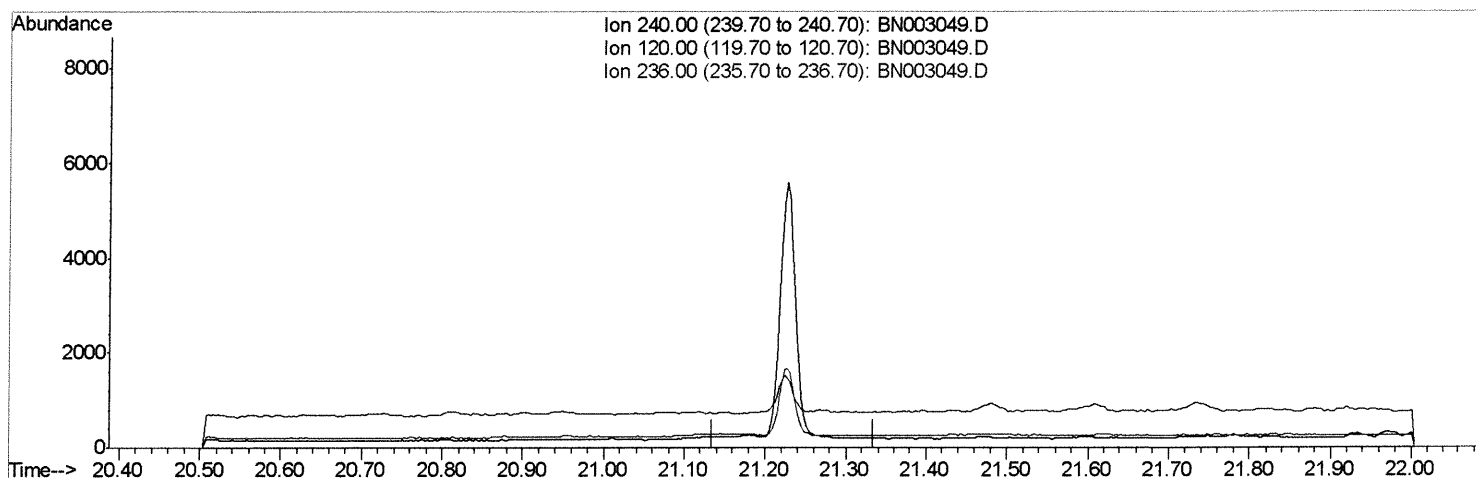

TIC: BN003049.D

(16) Chrysene-d12 (I)

21.235min (-21.235) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	16.40	0.00#
236.00	28.10	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003049.D
 Acq On : 10 Oct 2018 04:20
 Operator : MJ/SJ
 Sample : J5115-17
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC60

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:58:19 PM

Quant Time: Oct 10 08:59:30 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 08:36:11 2018
 Response via : Initial Calibration

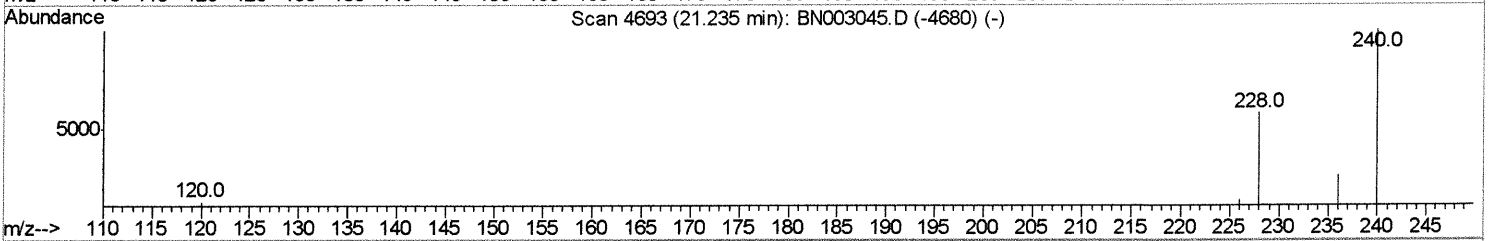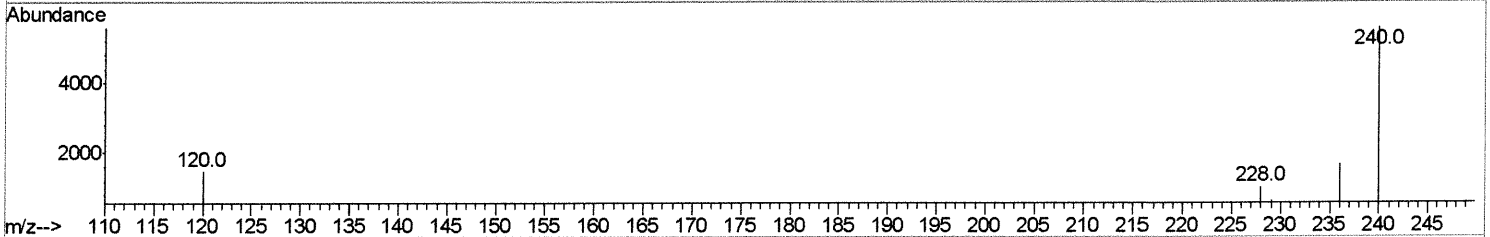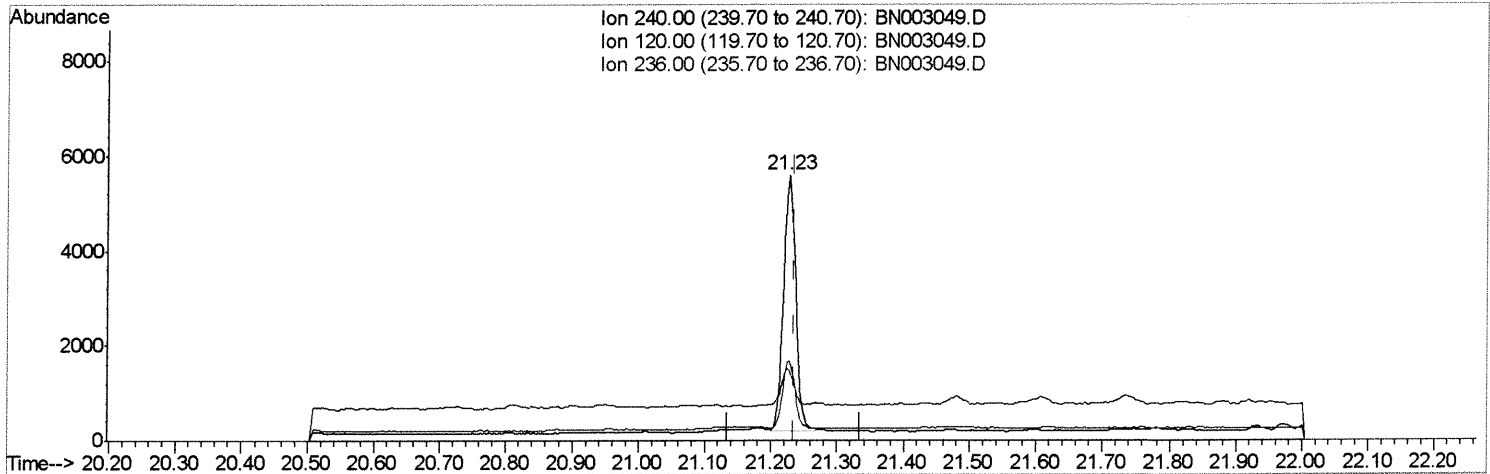

TIC: BN003049.D

(16) Chrysene-d12 (I)

21.226min (-0.009) 0.40ng/ul m

SJ 10/12/18

response 6812

Ion	Exp%	Act%
240.00	100	100
120.00	16.40	26.59#
236.00	28.10	29.91
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003049.D
 Acq On : 10 Oct 2018 04:20
 Operator : MJ/SJ
 Sample : J5115-17
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC60

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:58:19 PM

Quant Time: Oct 10 09:00:55 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 08:36:11 2018
 Response via : Initial Calibration

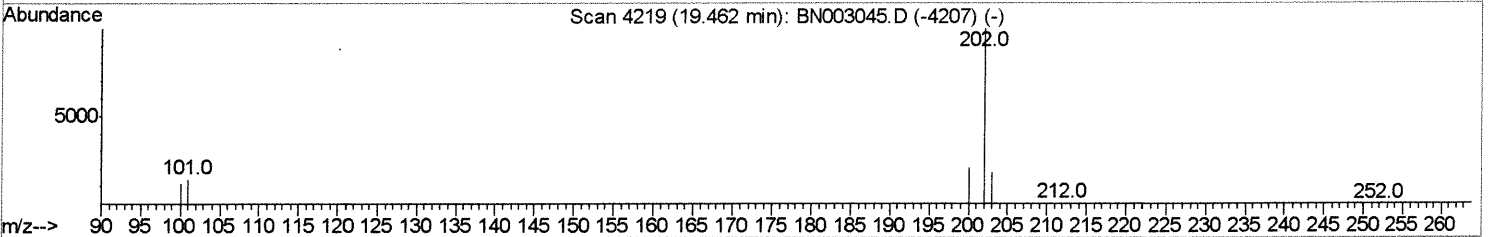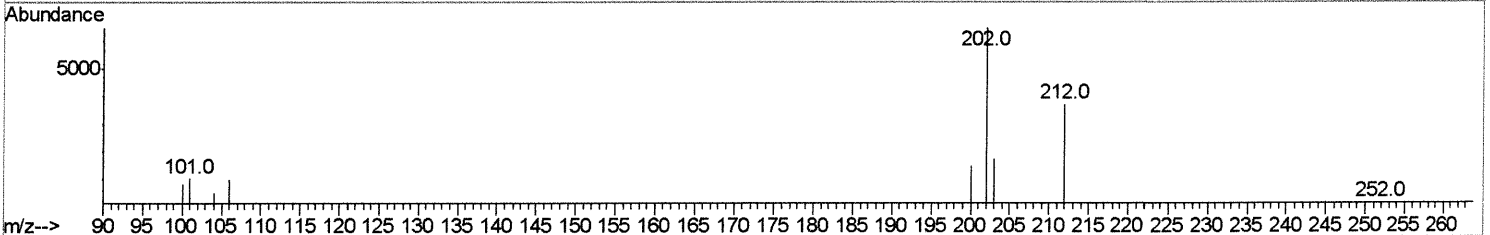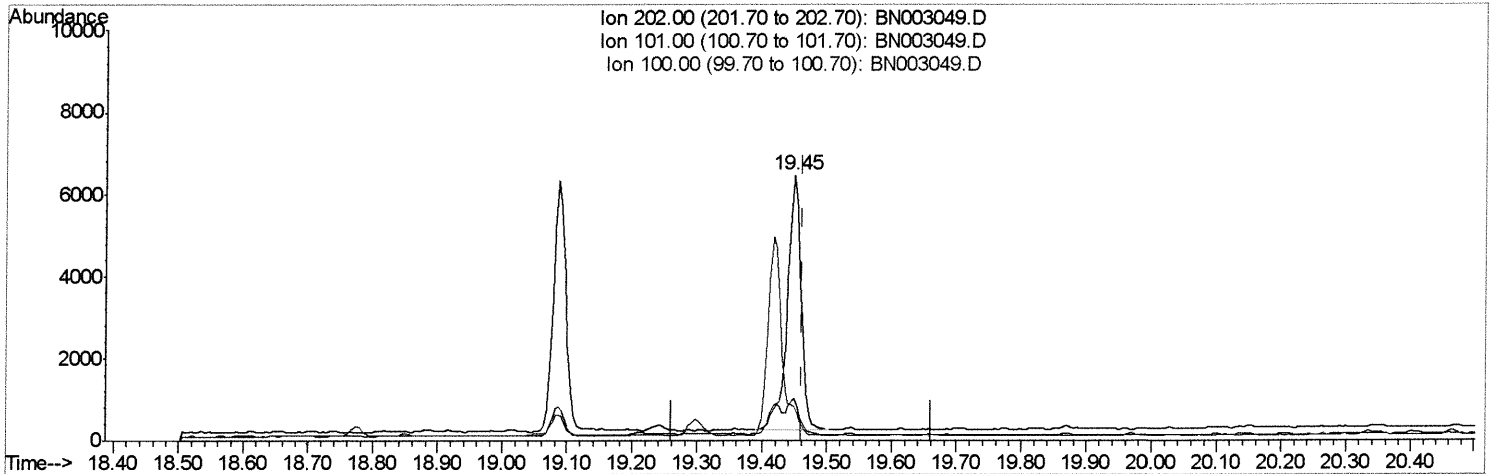

TIC: BN003049.D

(17) Pyrene

19.448min (-0.014) 0.35ng/ul

response 9379

Ion	Exp%	Act%
202.00	100	100
101.00	14.90	15.81
100.00	12.40	12.91
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003049.D
 Acq On : 10 Oct 2018 04:20
 Operator : MJ/SJ
 Sample : J5115-17
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC60

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:58:19 PM

Quant Time: Oct 10 09:00:55 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 08:36:11 2018
 Response via : Initial Calibration

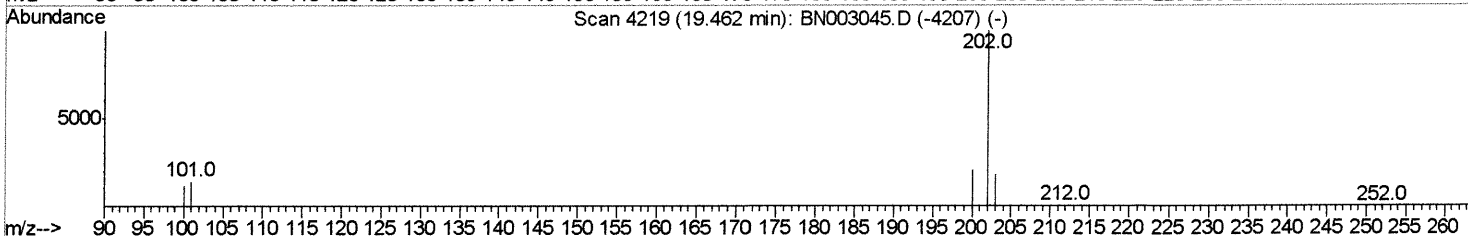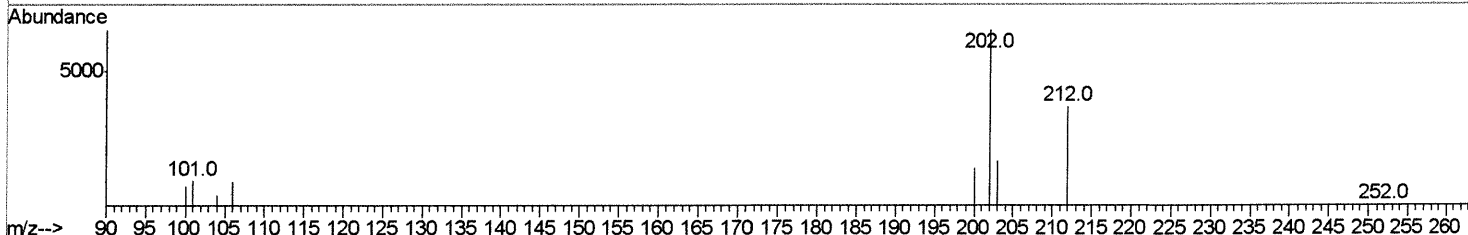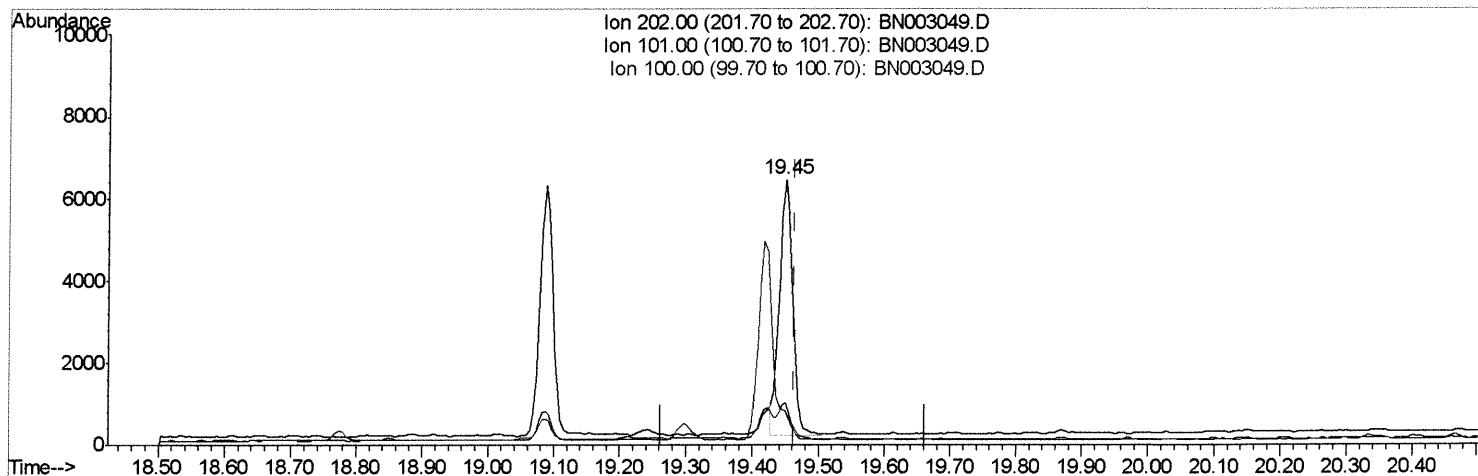

TIC: BN003049.D

(17) Pyrene

19.448min (-0.014) 0.33ng/ul m

SJ 10/12/18

response 8793

Ion	Exp%	Act%
202.00	100	100
101.00	14.90	15.81
100.00	12.40	12.91
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003049.D
 Acq On : 10 Oct 2018 04:20
 Operator : MJ/SJ
 Sample : J5115-17
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC60

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:58:19 PM

Quant Time: Oct 10 09:00:55 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 08:36:11 2018
 Response via : Initial Calibration

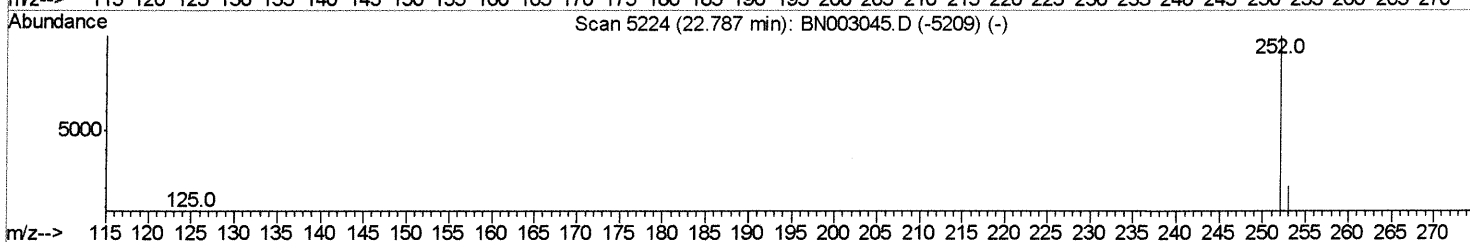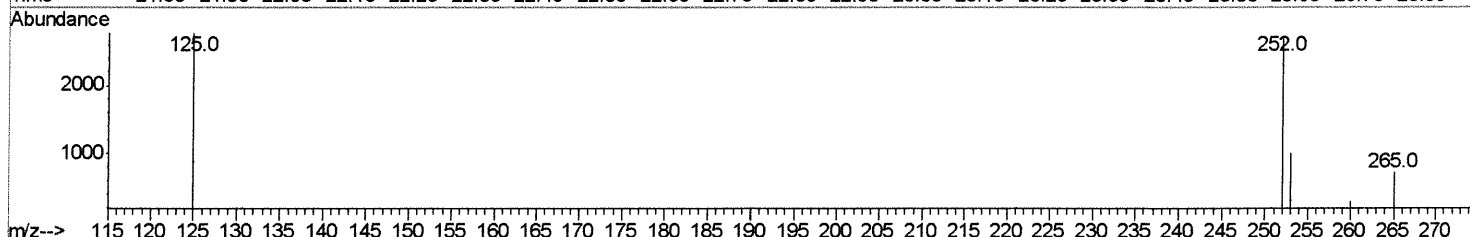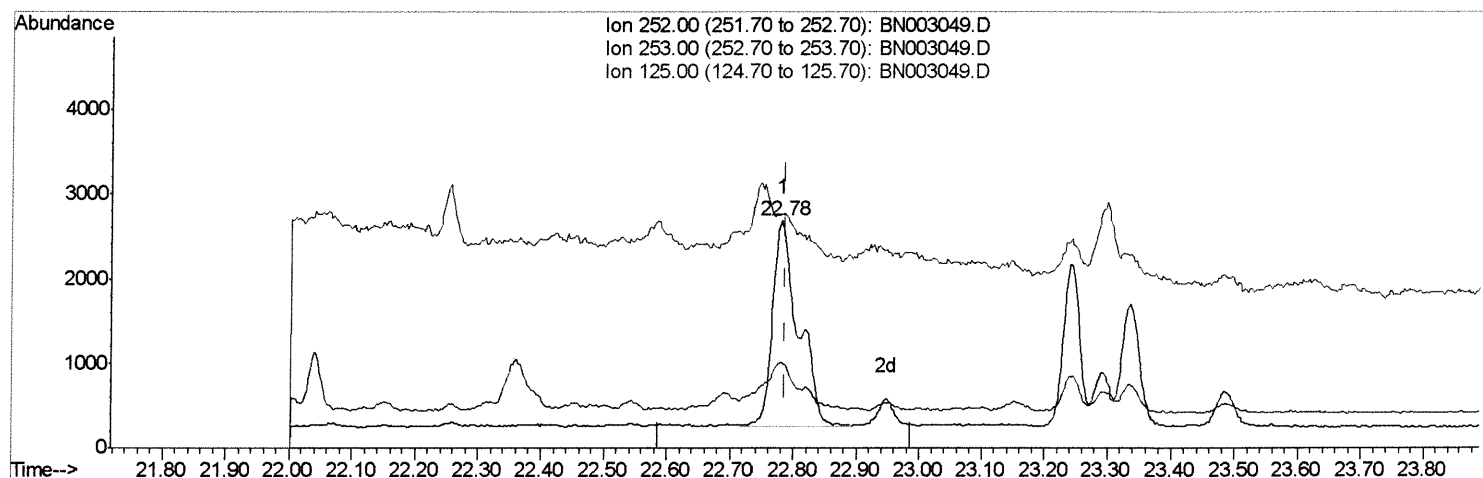

TIC: BN003049.D

(21) Benzo(b)fluoranthene
 22.781min (-0.006) 0.34ng/ul
 response 6917

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	37.47
125.00	17.10	102.97#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003049.D
 Acq On : 10 Oct 2018 04:20
 Operator : MJ/SJ
 Sample : J5115-17
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC60

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:58:19 PM

Quant Time: Oct 10 09:00:55 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 08:36:11 2018
 Response via : Initial Calibration

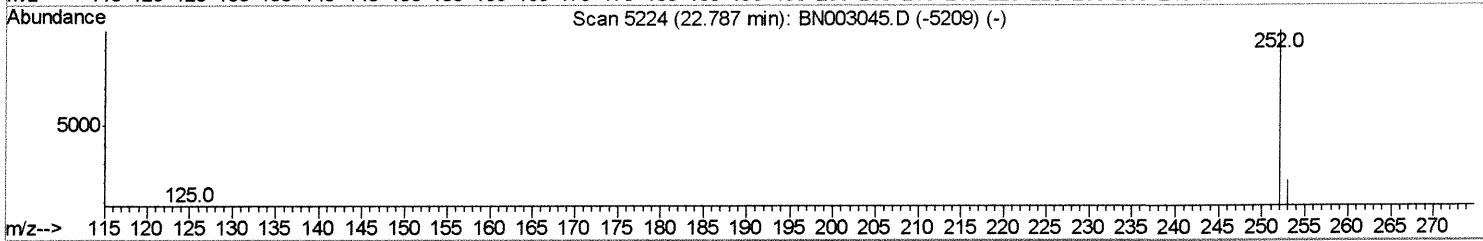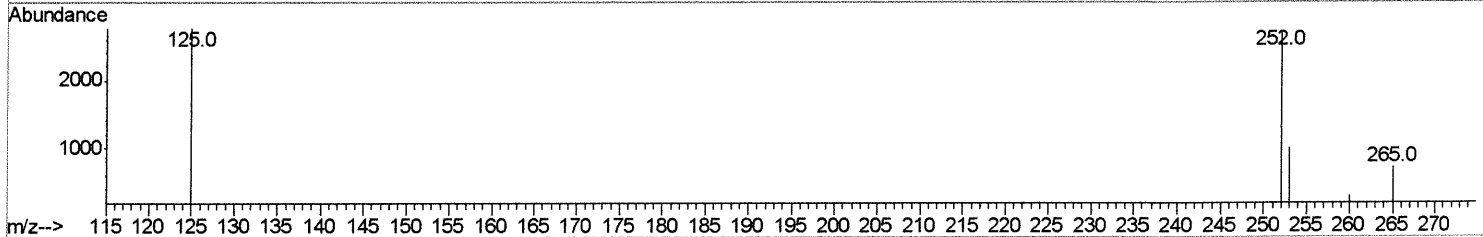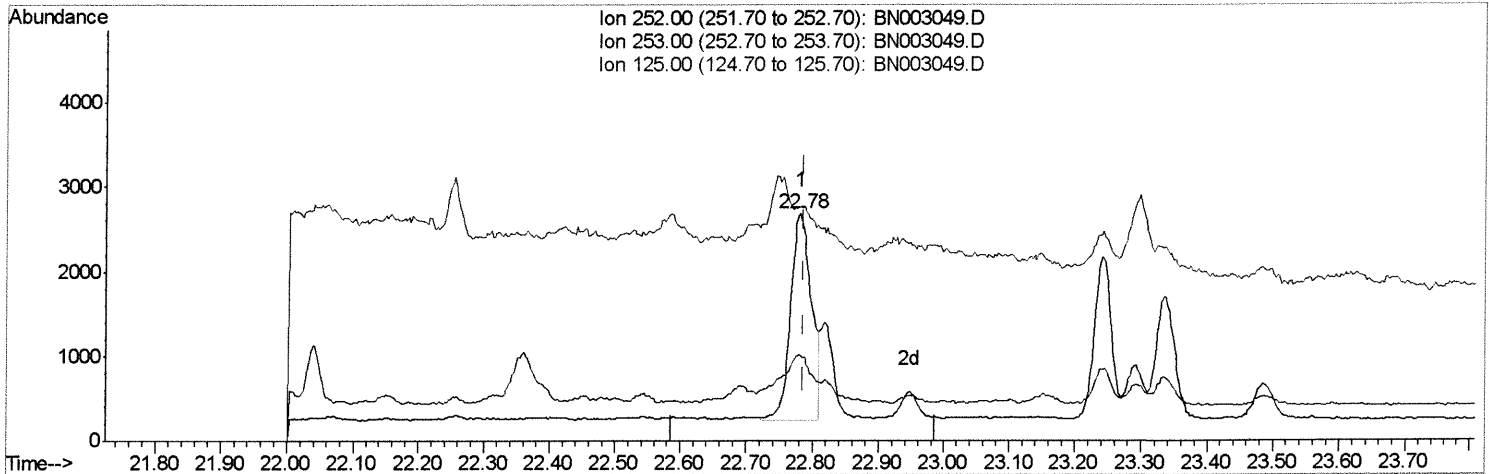

TIC: BN003049.D

(21) Benzo(b)fluoranthene
 22.781min (-0.006) 0.27ng/ul m
 response 5455

SJ 10/12/18

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	37.47
125.00	17.10	102.97#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003049.D
 Acq On : 10 Oct 2018 04:20
 Operator : MJ/SJ
 Sample : J5115-17
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC60

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:58:19 PM

Quant Time: Oct 10 09:00:55 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 08:36:11 2018
 Response via : Initial Calibration

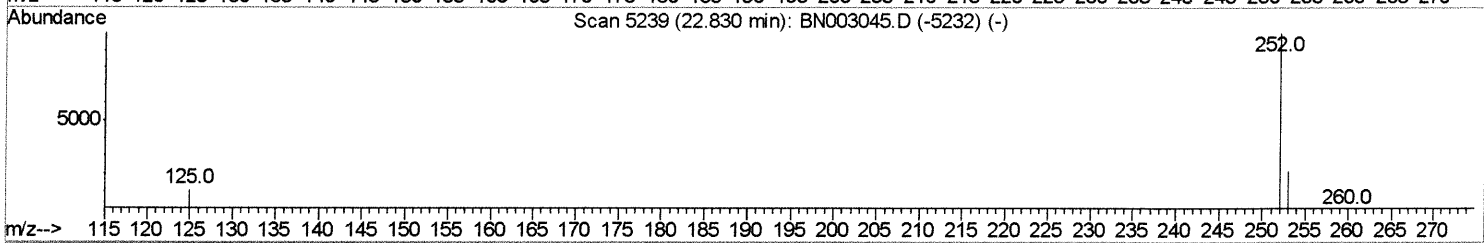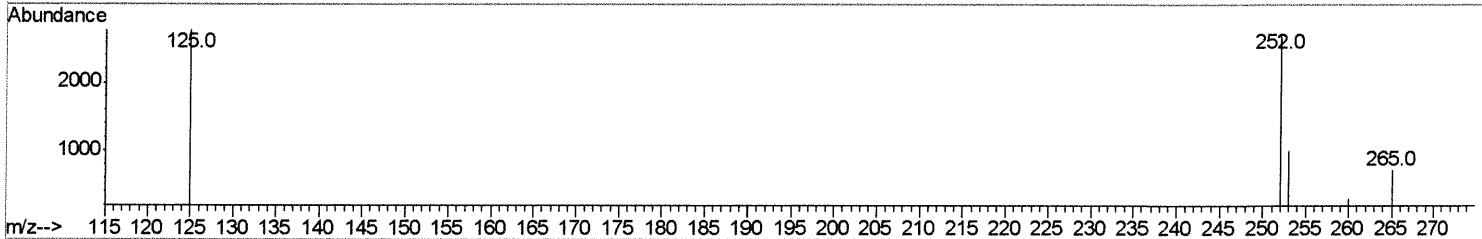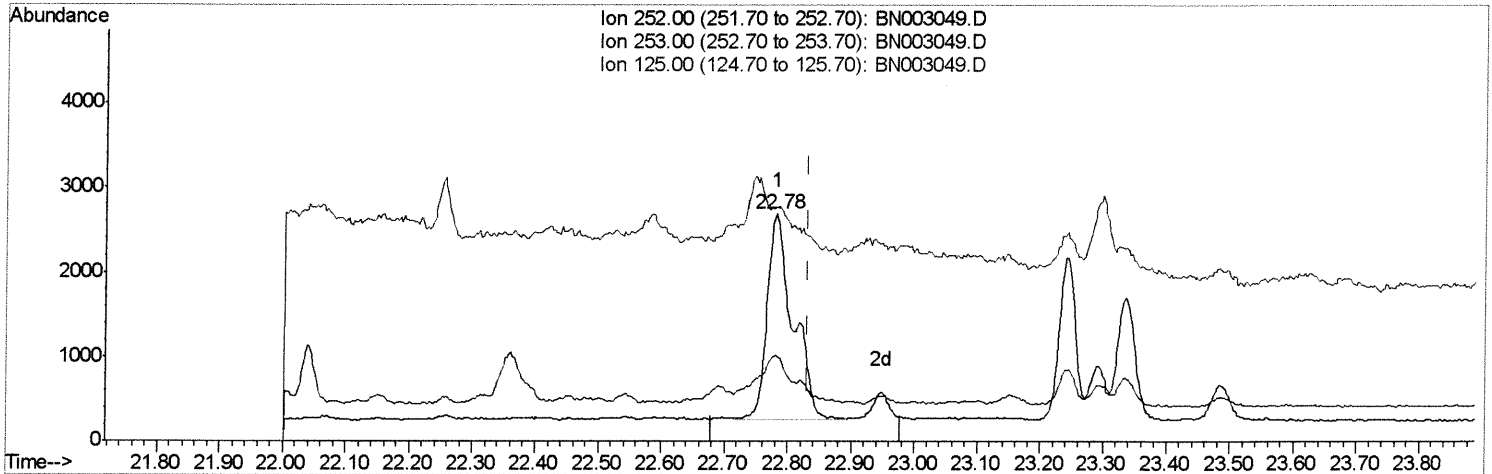

TIC: BN003049.D

(22) Benzo(k)fluoranthene
 22.781min (-0.050) 0.33ng/ul
 response 6917

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	37.47#
125.00	17.60	102.97#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003049.D
 Acq On : 10 Oct 2018 04:20
 Operator : MJ/SJ
 Sample : J5115-17
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC60

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:58:19 PM

Quant Time: Oct 10 09:00:55 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 08:36:11 2018
 Response via : Initial Calibration

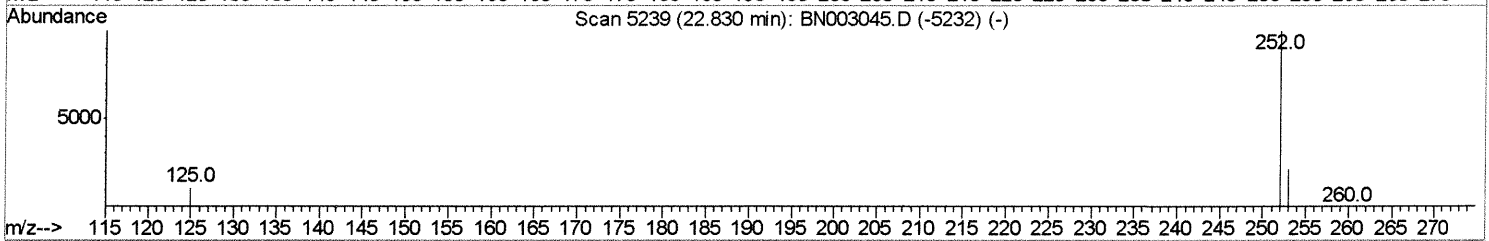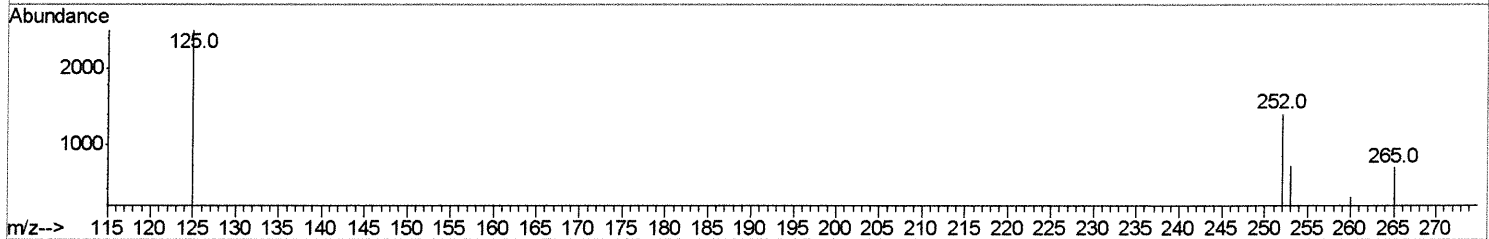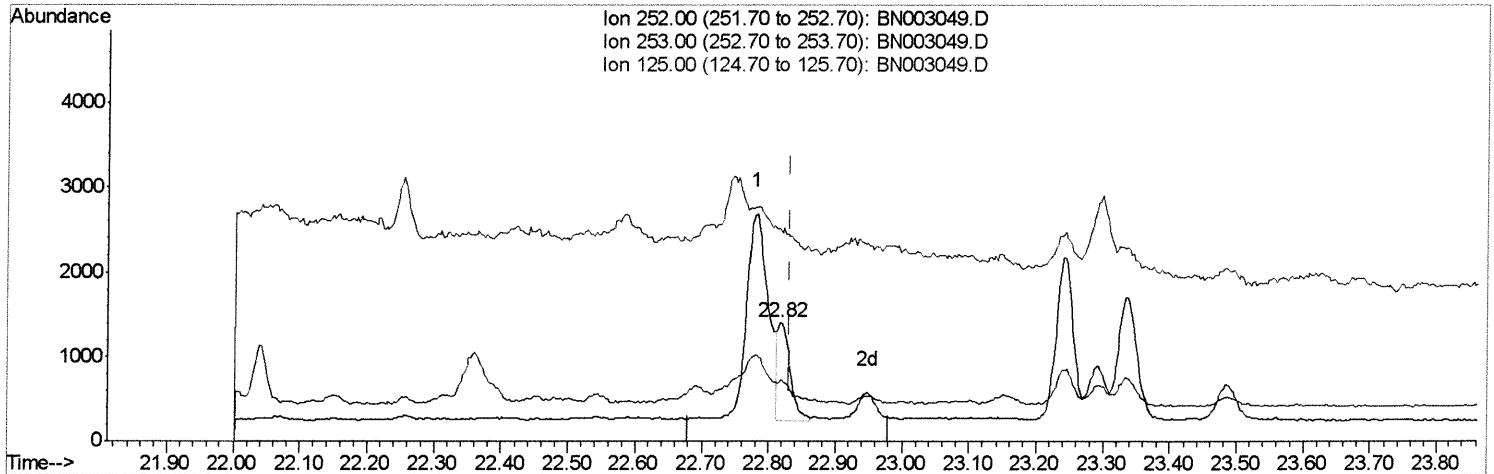

TIC: BN003049.D

(22) Benzo(k)fluoranthene

22.816min (-0.014) 0.07ng/ul m

response 1528

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	50.96#
125.00	17.60	180.06#
0.00	0.00	0.00

3310/12/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003049.D
 Acq On : 10 Oct 2018 04:20
 Operator : MJ/SJ
 Sample : J5115-17
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC60

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:58:19 PM

Quant Time: Oct 10 09:02:30 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 08:36:11 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	1832	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.39	136	7622	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.26	164	4404	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.02	188	9564m	0.40	ng/ul	-0.01
16) Chrysene-d12	21.23	240	6812m	0.40	ng/ul	0.00
20) Perylene-d12	23.44	264	5671	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.01	152	3000	0.25	ng/ul	0.00
14) Fluoranthene-d10	19.06	212	7188m	0.26	ng/ul	0.00
Target Compounds						
					Ovalue	
3) Naphthalene	10.44	128	1169	0.060	ng/ul#	87
5) 2-Methylnaphthalene	12.08	142	531	0.039	ng/ul	97
7) Acenaphthylene	13.98	152	583	0.029	ng/ul#	65
12) Phenanthrene	17.06	178	4817m	0.181	ng/ul	} SS10/12/18
13) Anthracene	17.15	178	743m	0.030	ng/ul	
15) Fluoranthene	19.09	202	8367m	0.268	ng/ul	
17) Pyrene	19.45	202	8793m	0.332	ng/ul	} SS10/12/18
18) Benzo(a)anthracene	21.21	228	3698	0.169	ng/ul#	
19) Chrysene	21.26	228	4475	0.201	ng/ul#	84
21) Benzo(b)fluoranthene	22.78	252	5455m	0.267	ng/ul	} SS10/12/18
22) Benzo(k)fluoranthene	22.82	252	1528m	0.072	ng/ul	
23) Benzo(a)pyrene	23.33	252	2864	0.156	ng/ul#	1
24) Indeno(1,2,3-cd)pyrene	25.65	276	2697	0.128	ng/ul#	94
26) Benzo(g,h,i)perylene	26.33	276	3299	0.186	ng/ul#	70

(#) = qualifier out of range (m) = manual integration (+) = signals summed