


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003051.D
Acq On : 10 Oct 2018 05:30
Operator : MJ/SJ
Sample : J5115-18
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC61

Manual Integrations
APPROVED

Sohil
10/10/2018 4:58:39 PM

Quant Time: Oct 10 09:10:34 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 08:36:11 2018
Response via : Initial Calibration

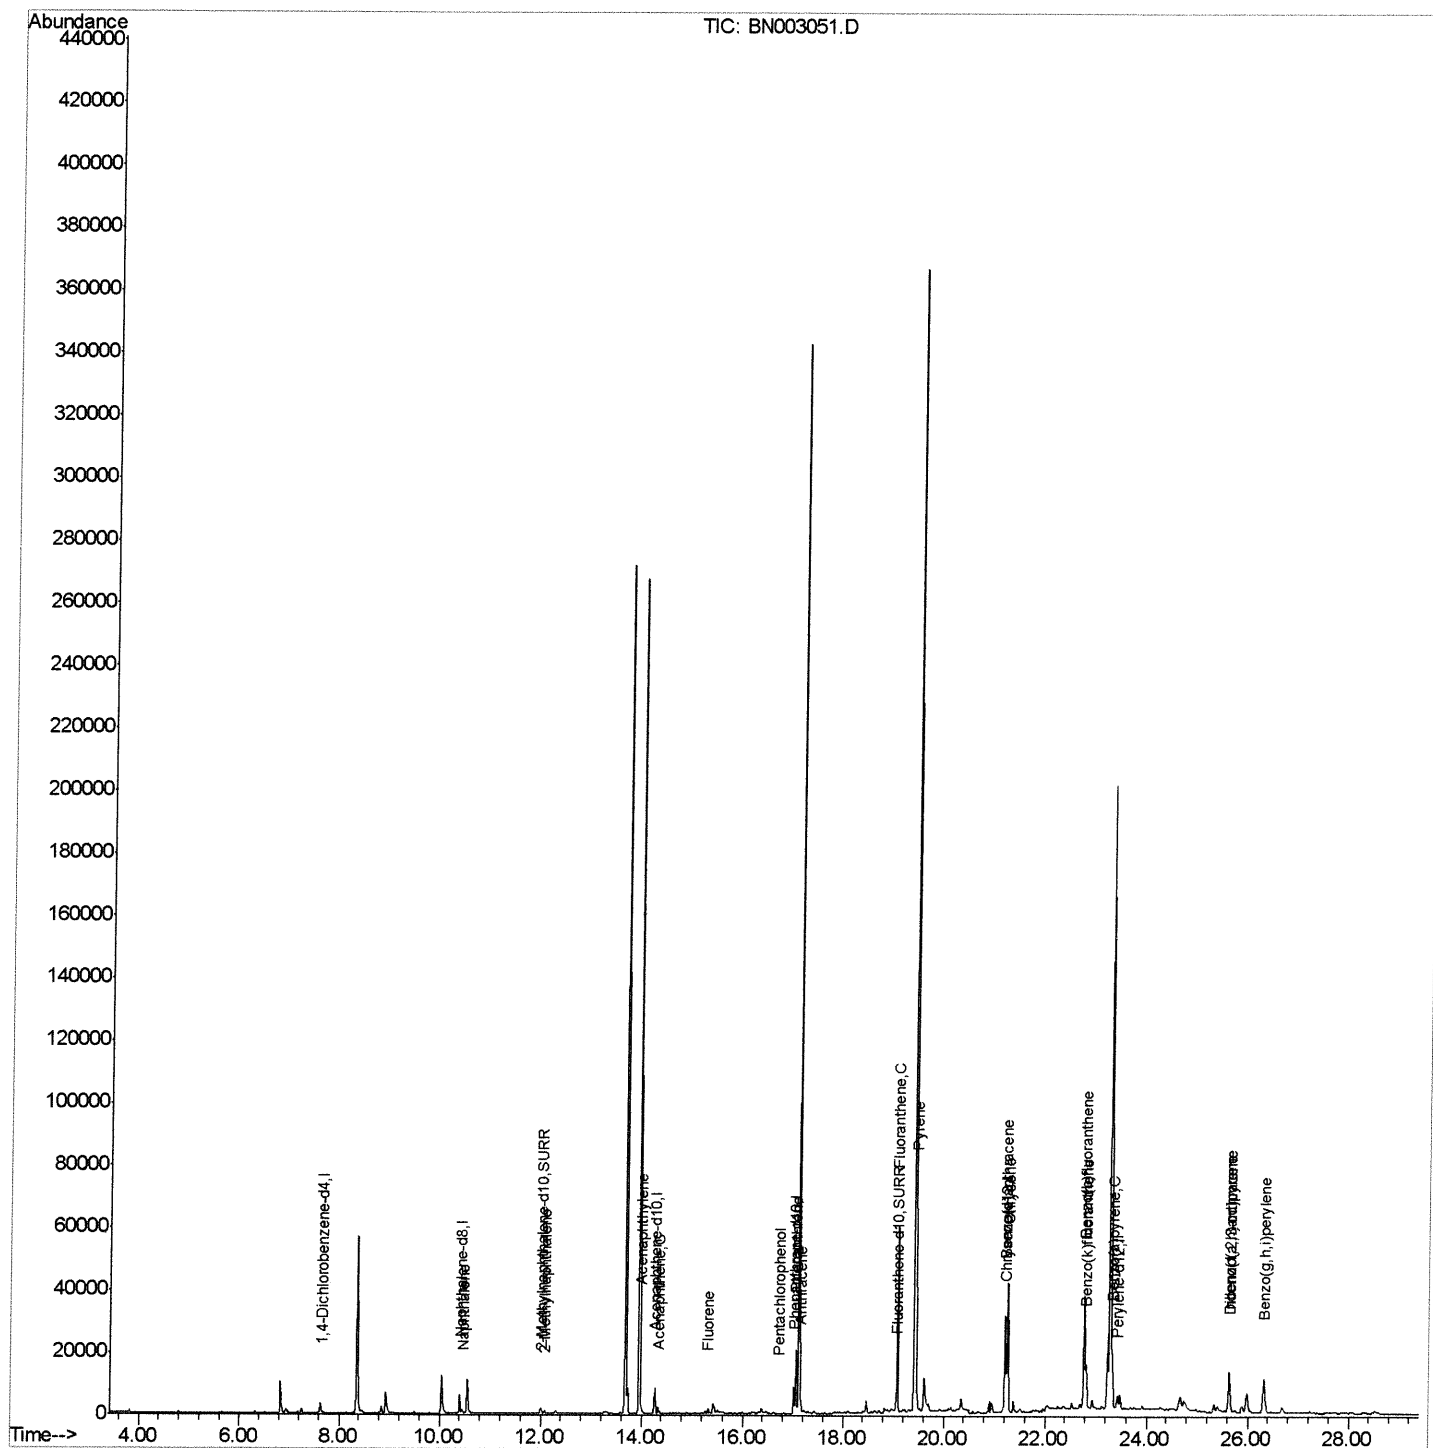

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003051.D
Acq On : 10 Oct 2018 05:30
Operator : MJ/SJ
Sample : J5115-18
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC61

Manual Integrations
APPROVED

Sohil
10/10/2018 4:58:39 PM

Quant Time: Oct 10 08:39:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 08:36:11 2018
Response via : Initial Calibration

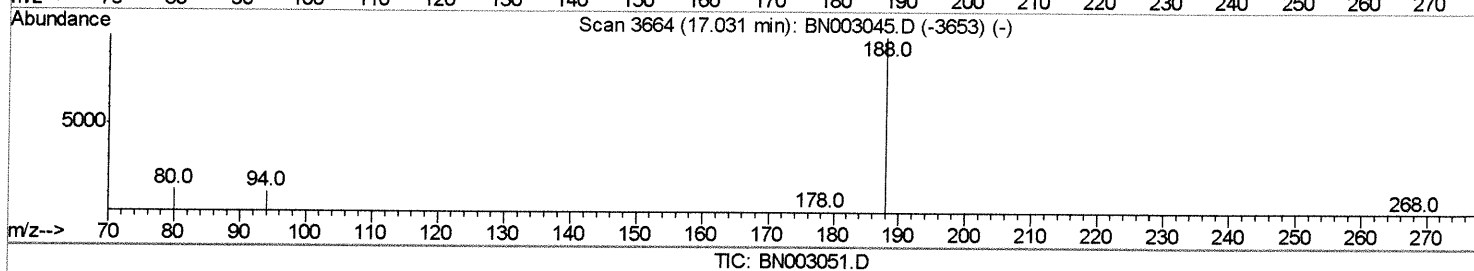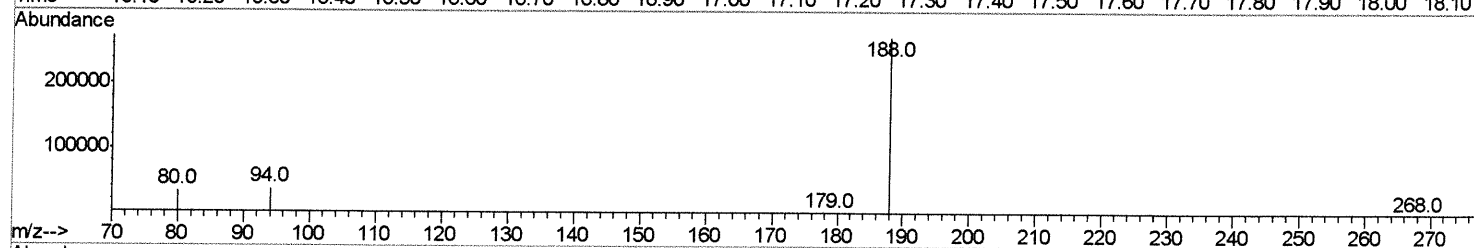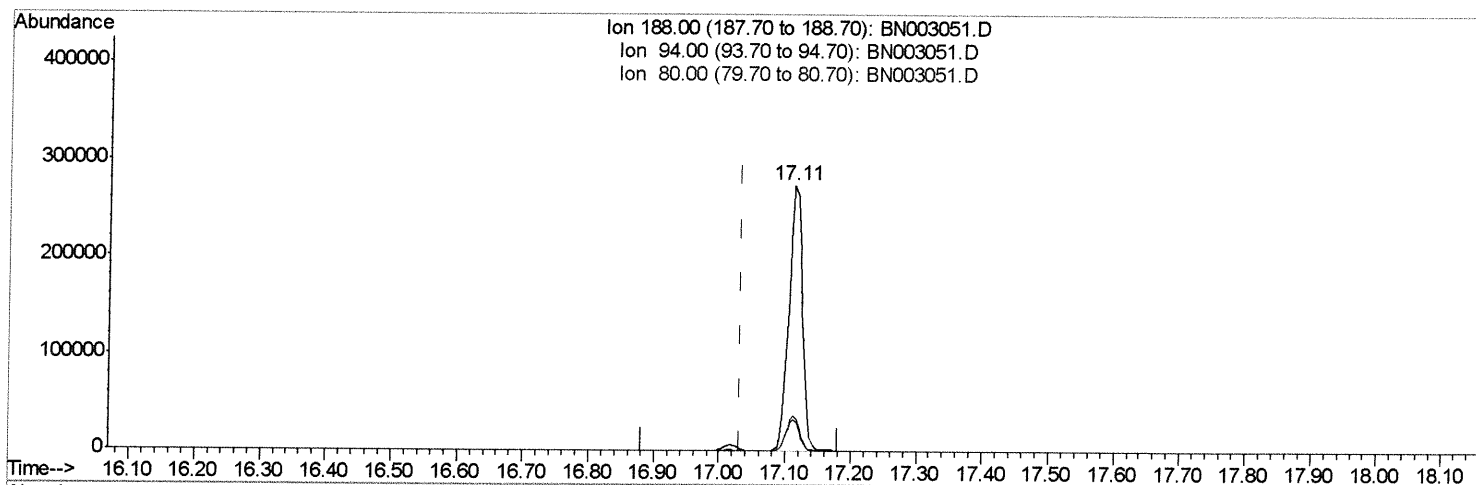

(10) Phenanthrene-d10 (I)

17.111min (+0.080) 0.40ng/ul

response 388394

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	13.09
80.00	12.70	11.93
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003051.D
Acq On : 10 Oct 2018 05:30
Operator : MJ/SJ
Sample : J5115-18
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC61

Manual Integrations
APPROVED

Sohil
10/10/2018 4:58:39 PM

Quant Time: Oct 10 08:39:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 08:36:11 2018
Response via : Initial Calibration

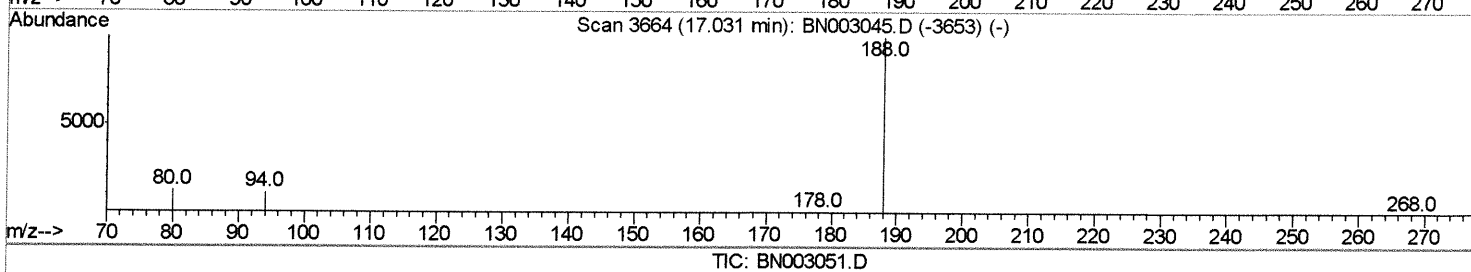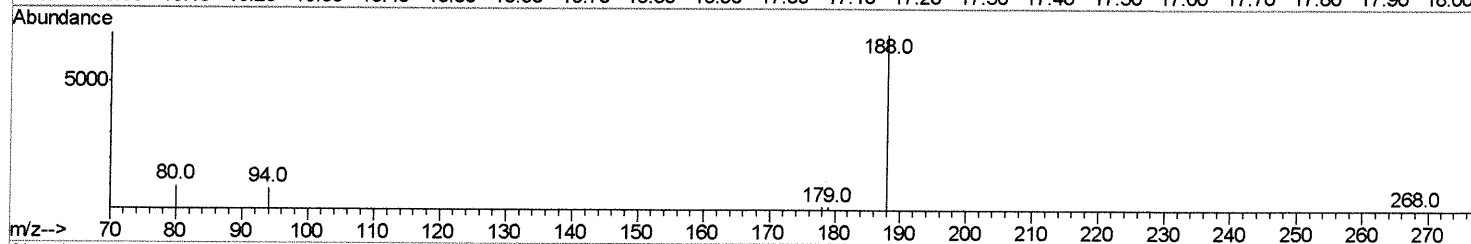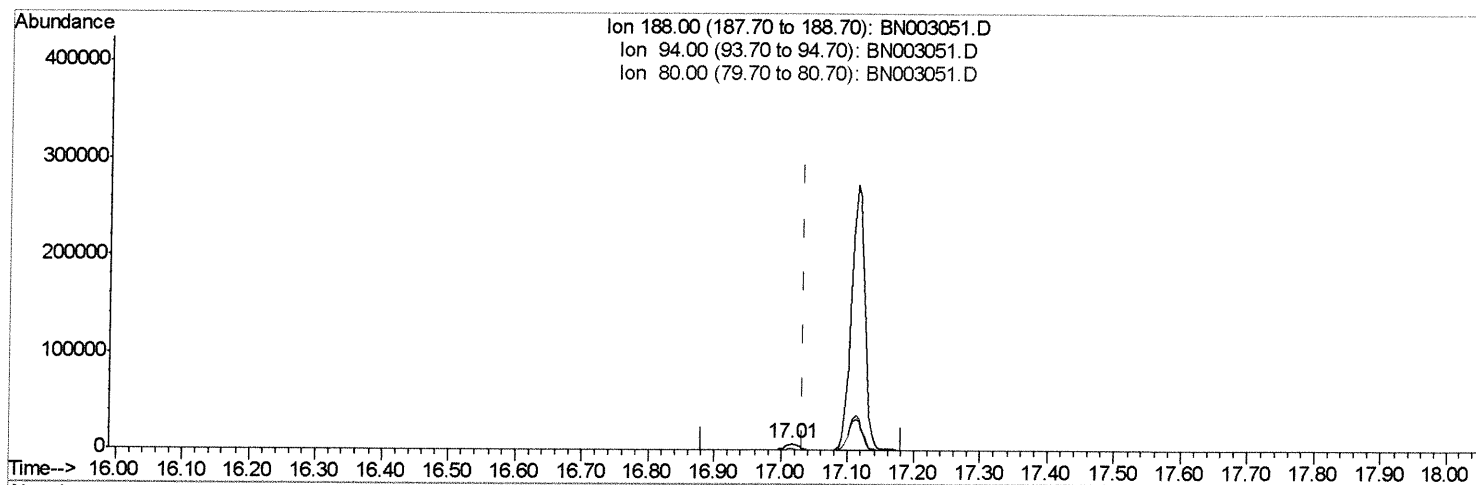

(10) Phenanthrene-d10 (I)

17.014min (-0.017) 0.40ng/ul m

5/10/12/18

response 9507

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	12.54
80.00	12.70	13.76
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003051.D
Acq On : 10 Oct 2018 05:30
Operator : MJ/SJ
Sample : J5115-18
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
JLC61

Manual Integrations
APPROVED

Sohil
10/10/2018 4:58:39 PM

Quant Time: Oct 10 09:08:03 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 08:36:11 2018
Response via : Initial Calibration

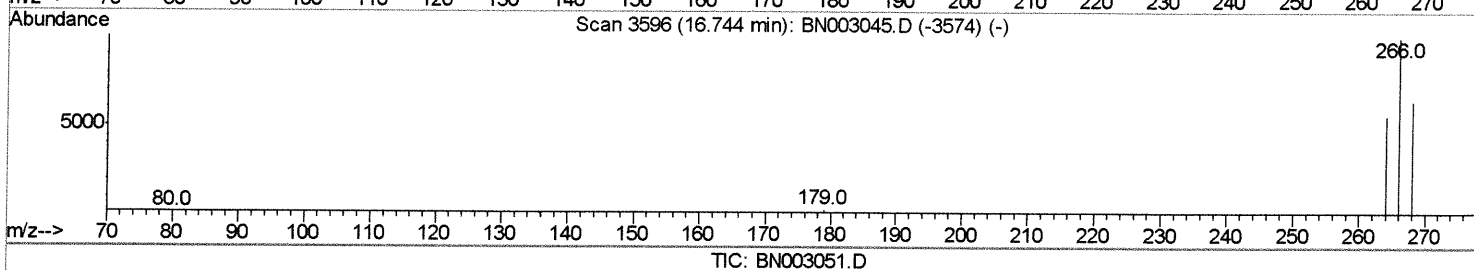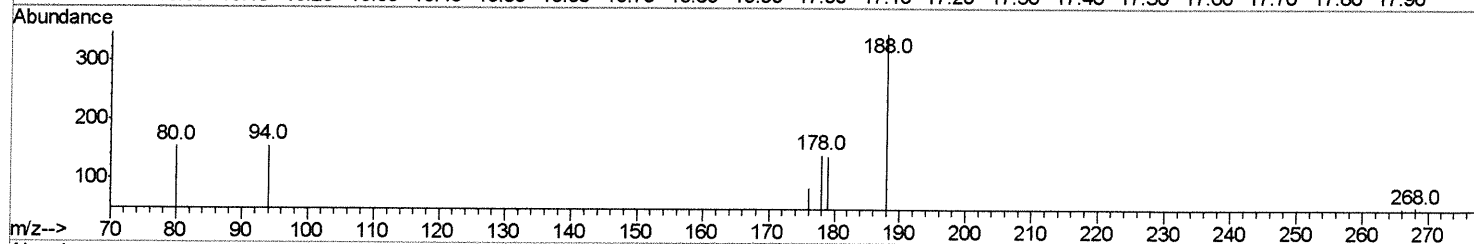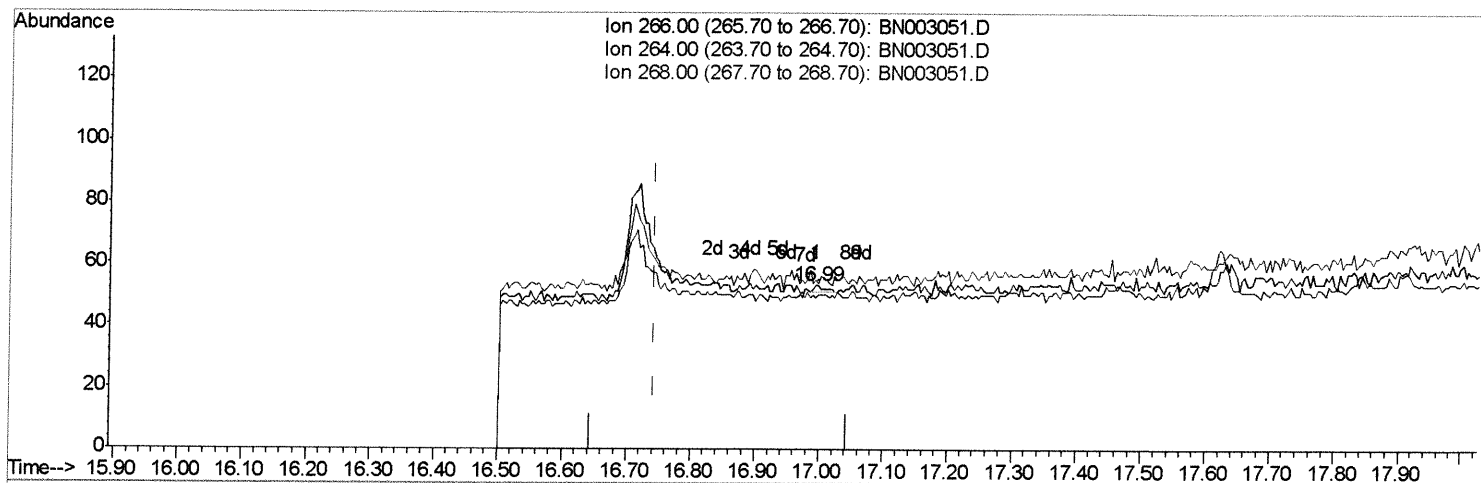

(11) Pentachlorophenol

16.993min (+0.249) 0.00ng/ul

response 3

Ion	Exp%	Act%
266.00	100	100
264.00	65.60	66.67
268.00	60.70	66.67
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003051.D
 Acq On : 10 Oct 2018 05:30
 Operator : MJ/SJ
 Sample : J5115-18
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC61

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:58:39 PM

Quant Time: Oct 10 09:08:03 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 08:36:11 2018
 Response via : Initial Calibration

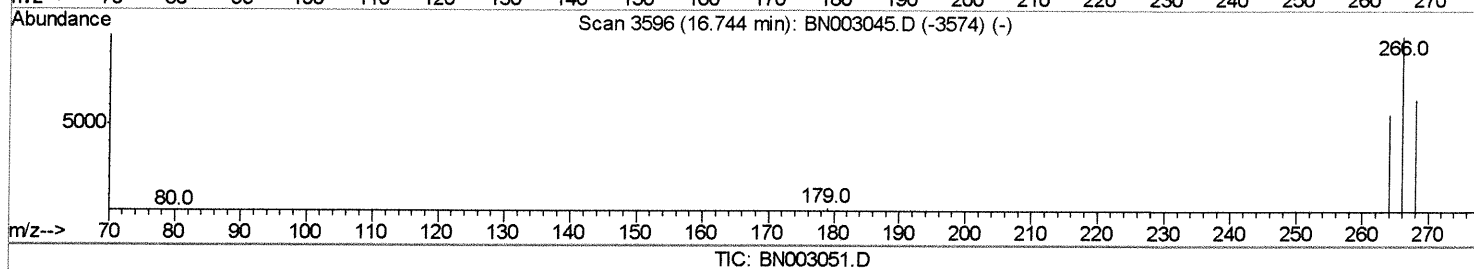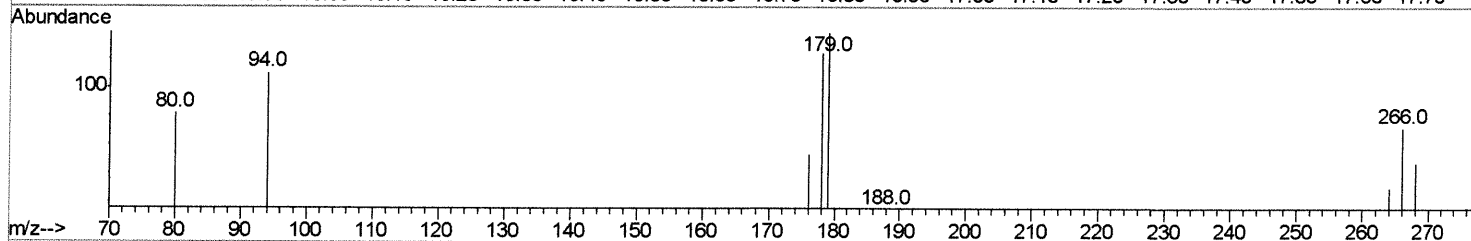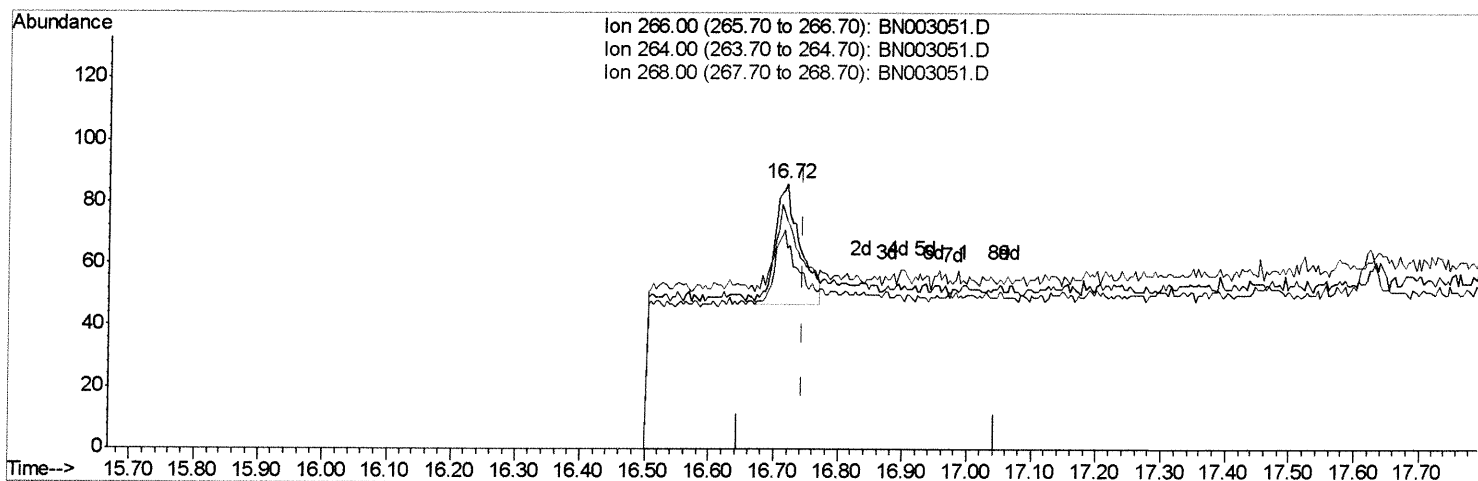

TIC: BN003051.D

(11) Pentachlorophenol

16.719min (-0.025) 0.11ng/ul m

SJ 10/12/18

response 106

Ion	Exp%	Act%
266.00	100	100
264.00	65.60	1.89#
268.00	60.70	1.89#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003051.D
Acq On : 10 Oct 2018 05:30
Operator : MJ/SJ
Sample : J5115-18
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC61

Manual Integrations
APPROVED

Sohil
10/10/2018 4:58:39 PM

Quant Time: Oct 10 09:08:03 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 08:36:11 2018
Response via : Initial Calibration

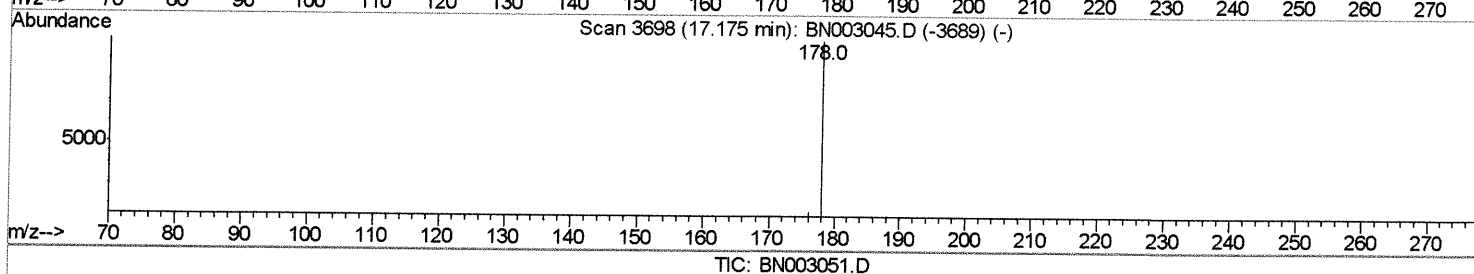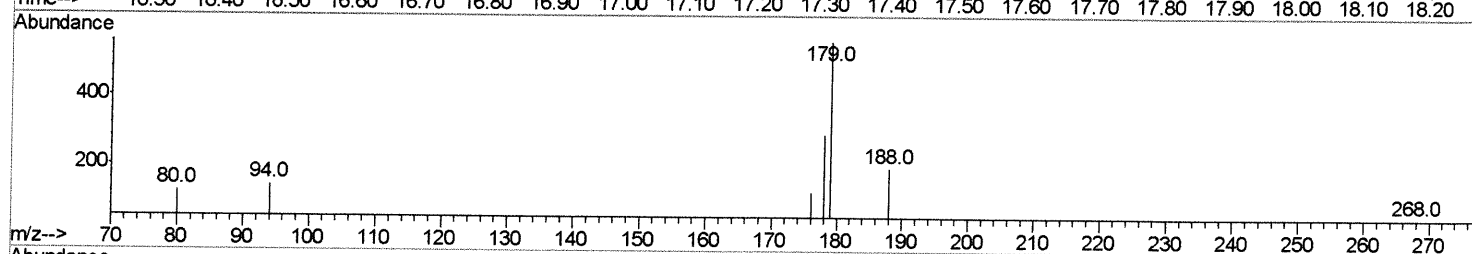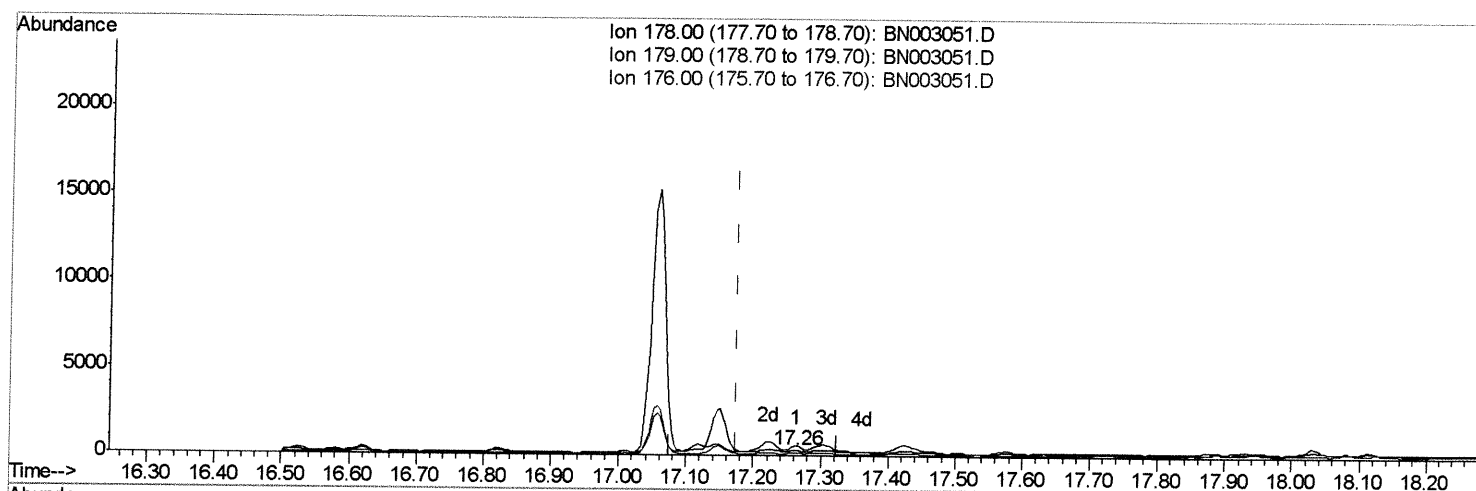

(13) Anthracene

17.263min (+0.089) 0.01ng/ul

response 157

Ion	Exp%	Act%
178.00	100	100
179.00	16.30	191.81#
176.00	19.10	42.32#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003051.D
Acq On : 10 Oct 2018 05:30
Operator : MJ/SJ
Sample : J5115-18
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
JLC61

Manual Integrations
APPROVED

Sohil
10/10/2018 4:58:39 PM

Quant Time: Oct 10 09:08:03 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 08:36:11 2018
Response via : Initial Calibration

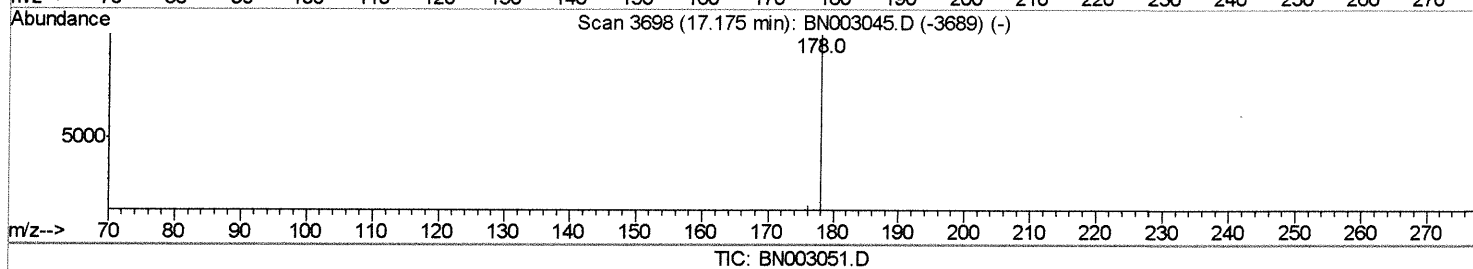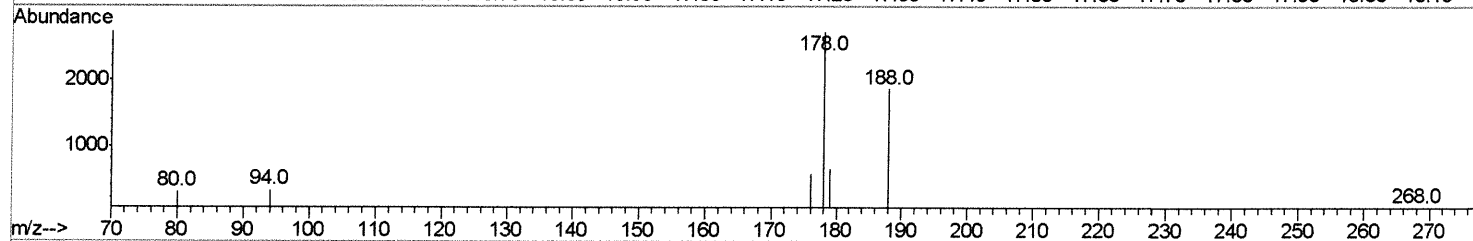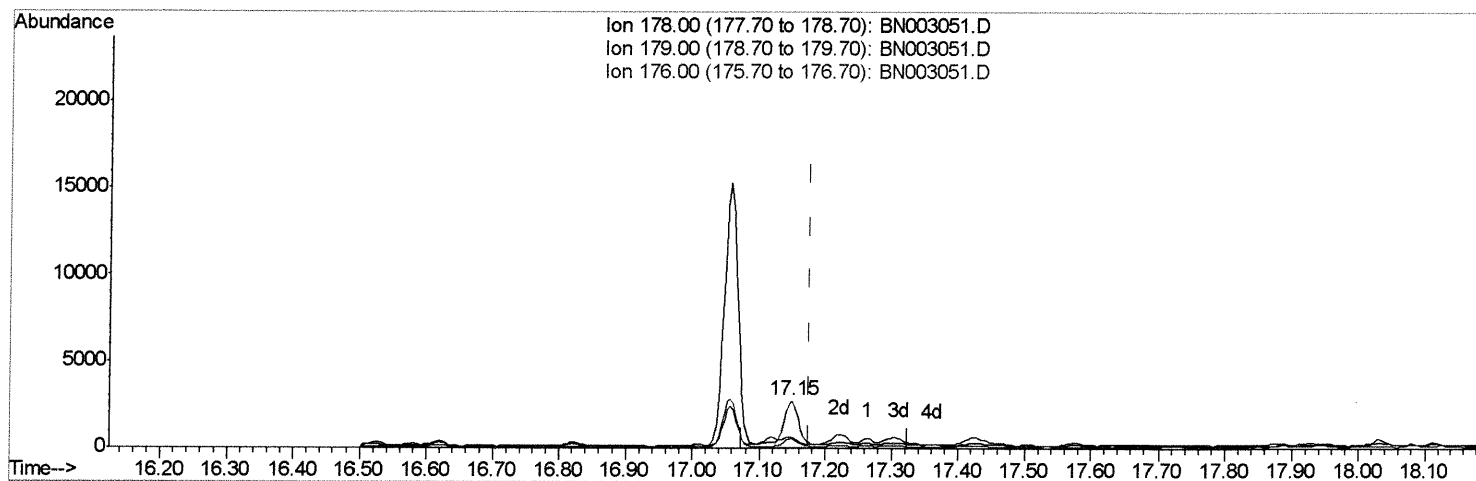

TIC: BN003051.D

(13) Anthracene

17.149min (-0.025) 0.17ng/ul m

SJ 10/12/18

response 4169

Ion	Exp%	Act%
178.00	100	100
179.00	16.30	23.67#
176.00	19.10	20.61
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003051.D
Acq On : 10 Oct 2018 05:30
Operator : MJ/SJ
Sample : J5115-18
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC61

Manual Integrations
APPROVED

Sohil
10/10/2018 4:58:39 PM

Quant Time: Oct 10 09:08:03 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 08:36:11 2018
Response via : Initial Calibration

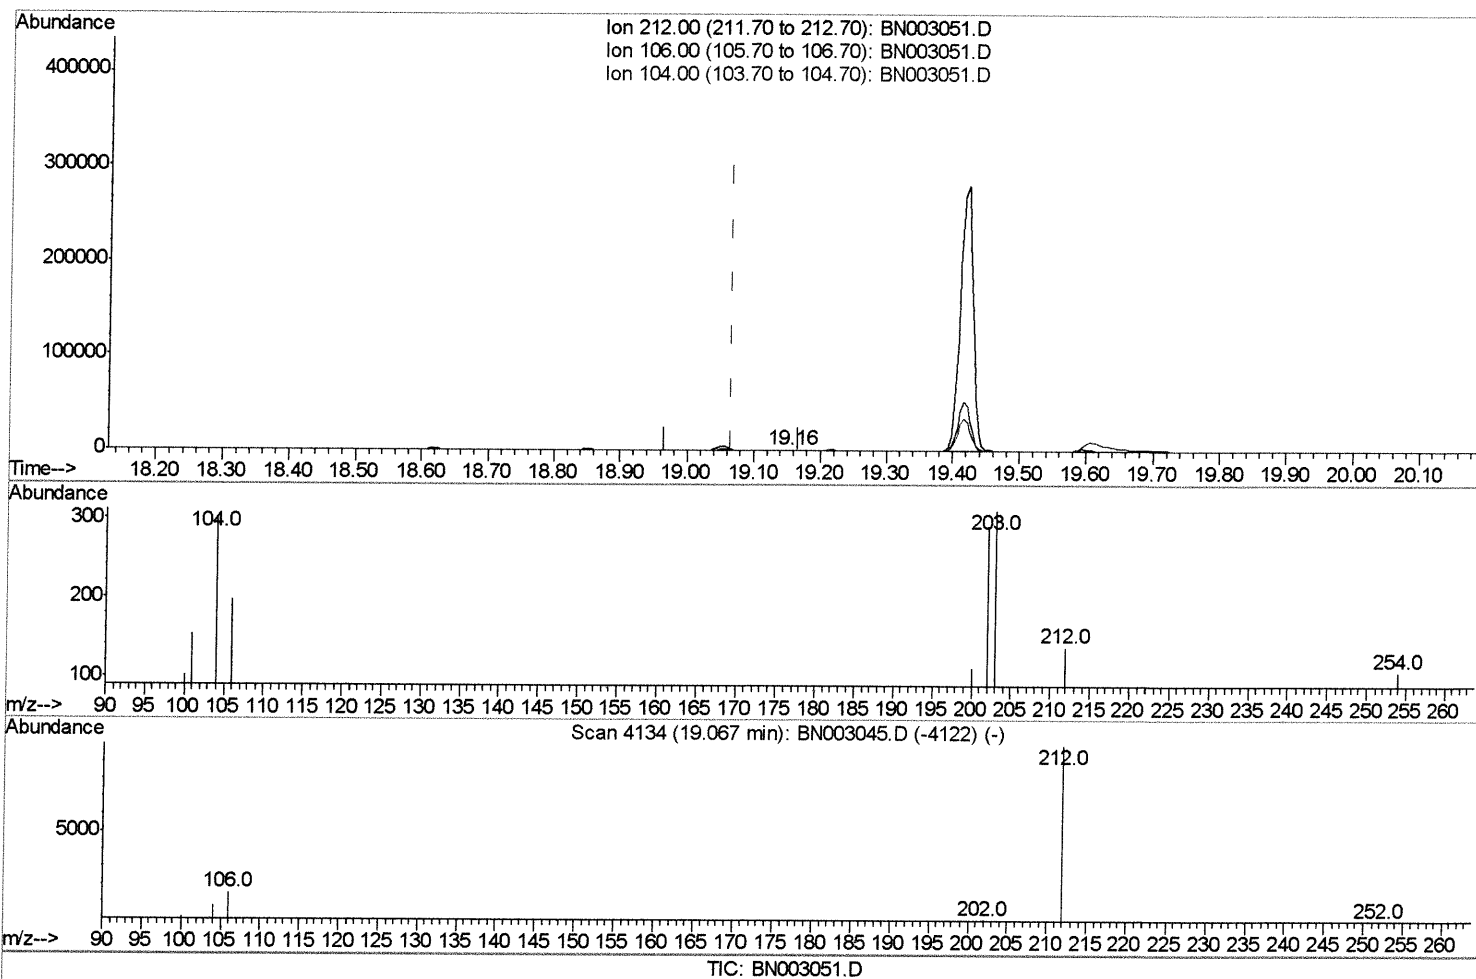

(14) Fluoranthene-d10 (SURR)

19.155min (+0.088) 0.00ng/ul

response 104

Ion	Exp%	Act%
212.00	100	100
106.00	15.40	0.00#
104.00	8.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003051.D
Acq On : 10 Oct 2018 05:30
Operator : MJ/SJ
Sample : J5115-18
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC61

Manual Integrations
APPROVED

Sohil
10/10/2018 4:58:39 PM

Quant Time: Oct 10 09:08:03 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 08:36:11 2018
Response via : Initial Calibration

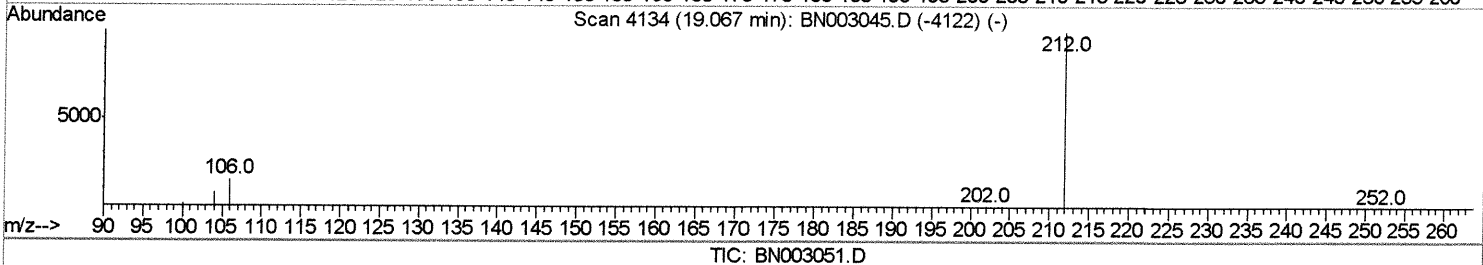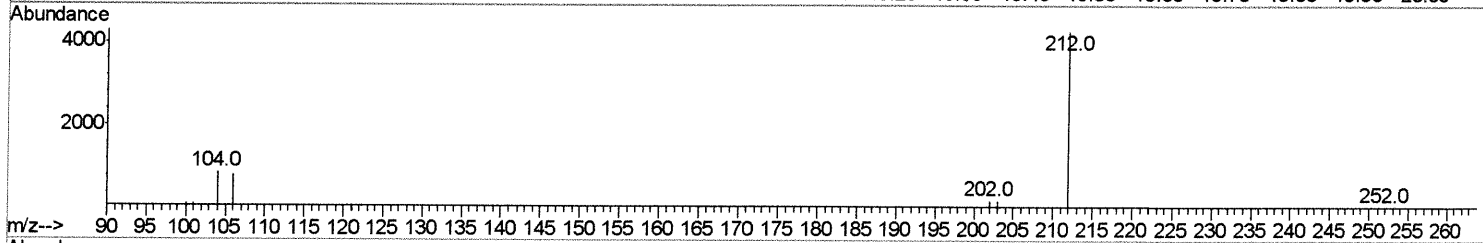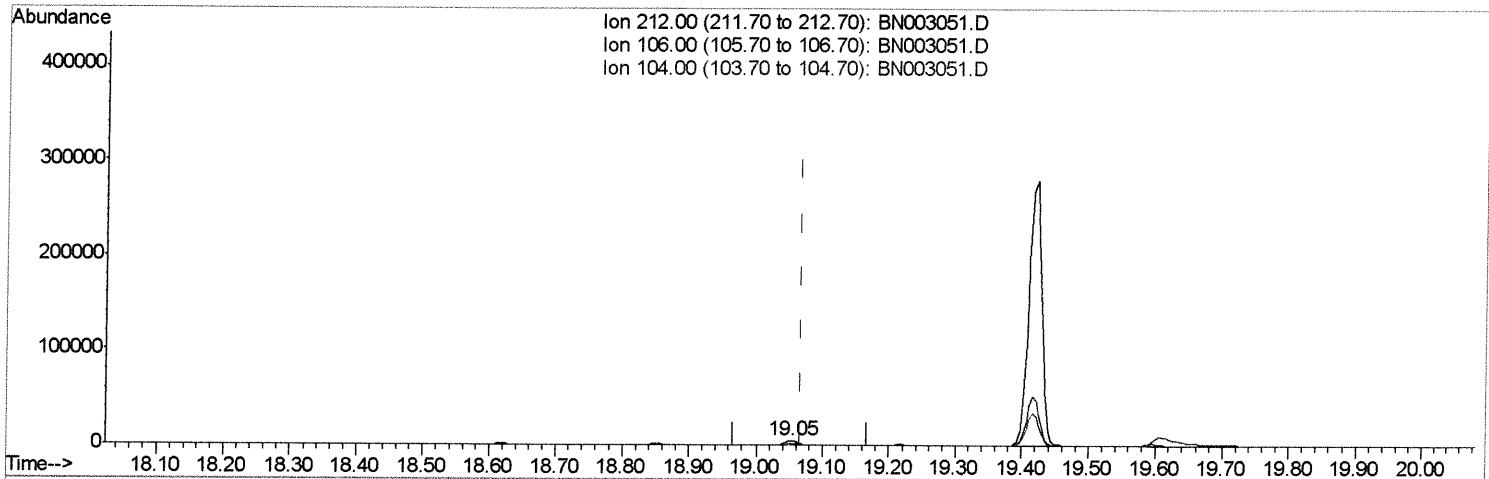

(14) Fluoranthene-d10 (SURRE)

19.053min (-0.014) 0.20ng/ul m

SJ 10/12/18

response 5457

Ion	Exp%	Act%
212.00	100	100
106.00	15.40	0.00#
104.00	8.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003051.D
 Acq On : 10 Oct 2018 05:30
 Operator : MJ/SJ
 Sample : J5115-18
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC61

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:58:39 PM

Quant Time: Oct 10 09:08:03 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 08:36:11 2018
 Response via : Initial Calibration

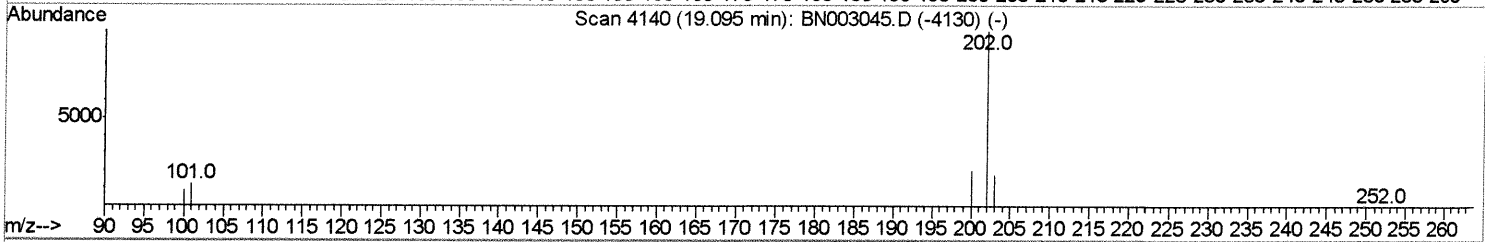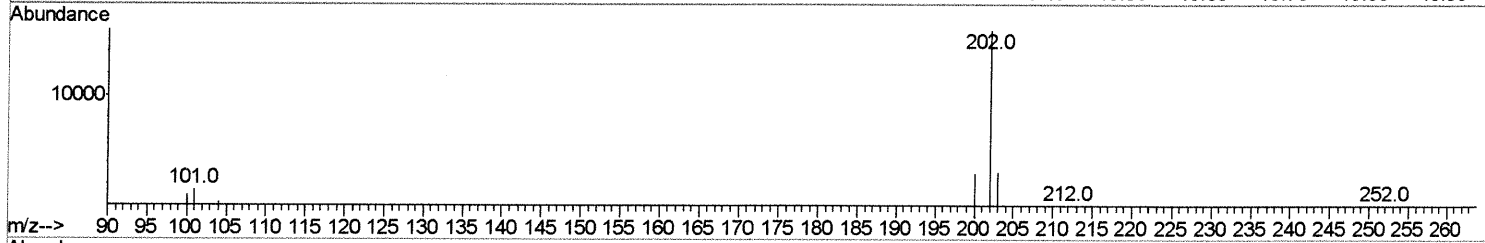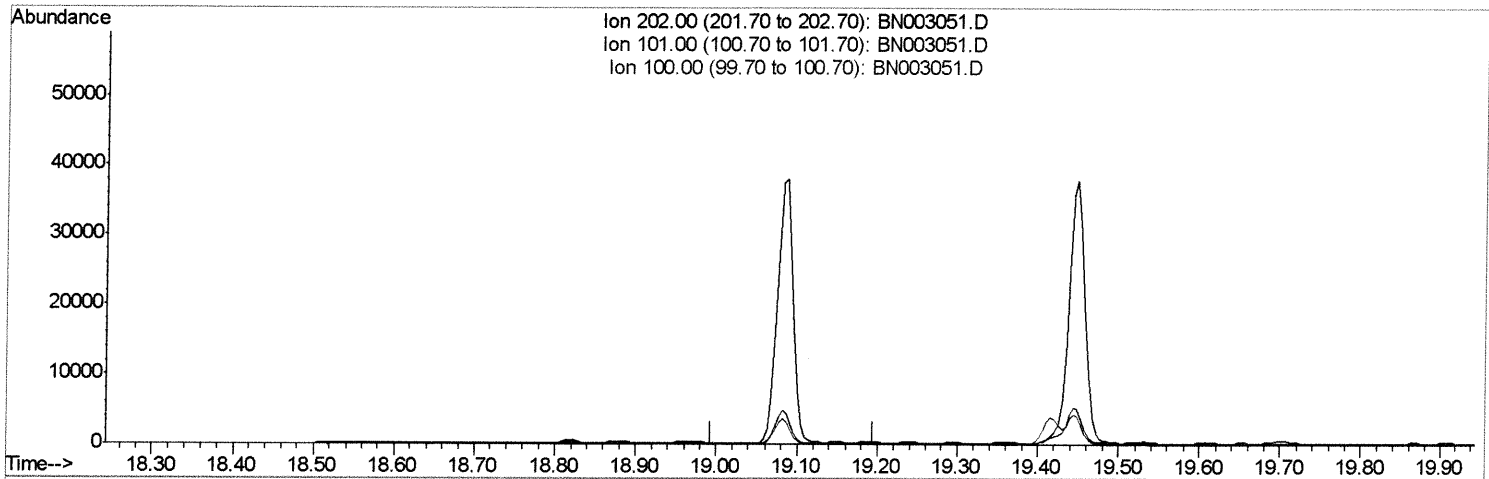

TIC: BN003051.D

(15) Fluoranthene (C)

19.095min (-19.095) 0.00ng/ul

response 0

Ion	Exp%	Act%
202.00	100	0.00
101.00	12.30	0.00
100.00	9.10	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003051.D
Acq On : 10 Oct 2018 05:30
Operator : MJ/SJ
Sample : J5115-18
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC61

Manual Integrations
APPROVED

Sohil
10/10/2018 4:58:39 PM

Quant Time: Oct 10 09:08:03 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 08:36:11 2018
Response via : Initial Calibration

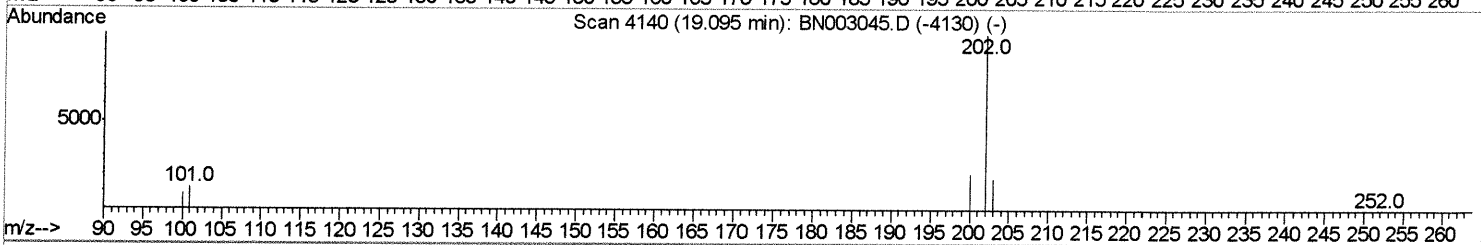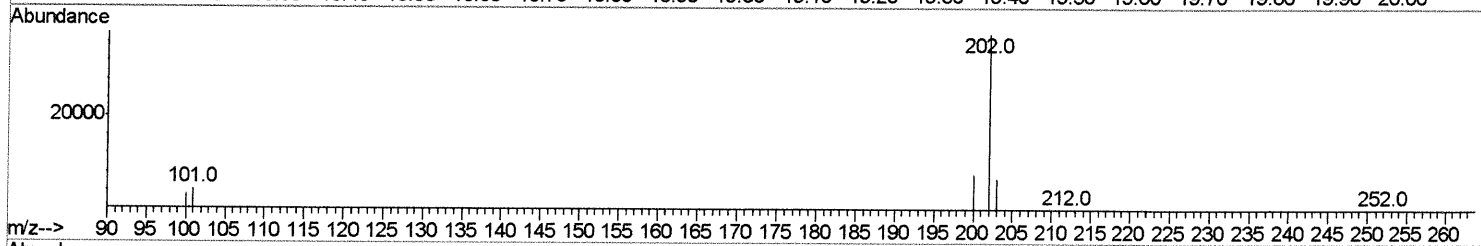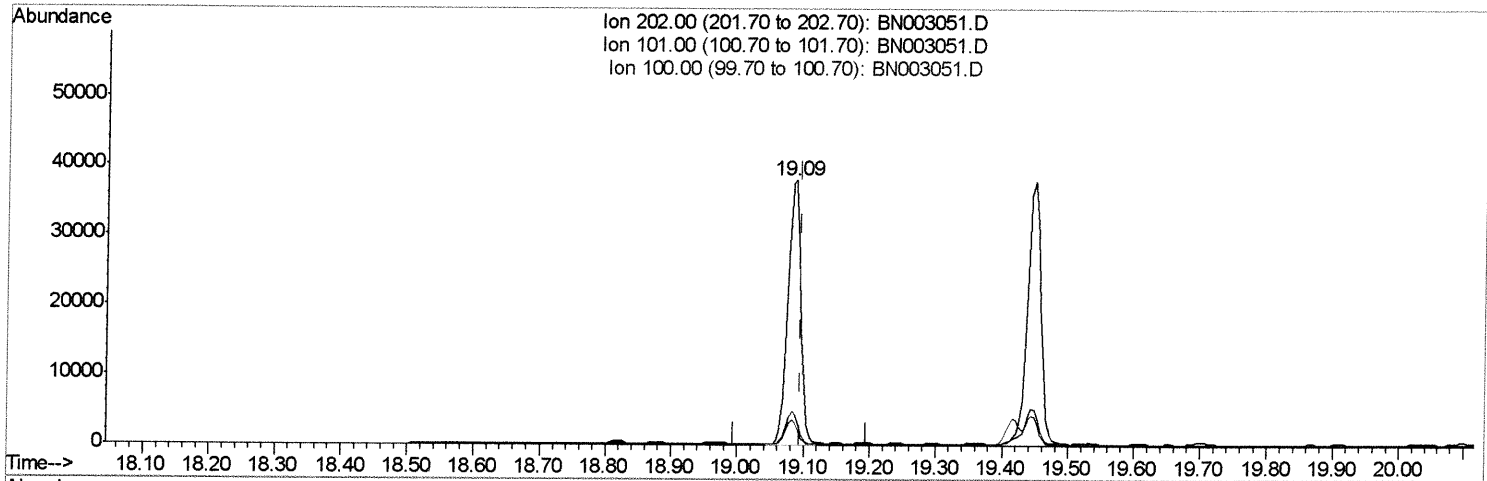

TIC: BN003051.D

(15) Fluoranthene (C)

19.086min (-0.009) 1.65ng/ul m

5 J 10/12/18

response 51154

Ion	Exp%	Act%
202.00	100	100
101.00	12.30	11.47
100.00	9.10	8.26
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003051.D
Acq On : 10 Oct 2018 05:30
Operator : MJ/SJ
Sample : J5115-18
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC61

Manual Integrations
APPROVED

Sohil
10/10/2018 4:58:39 PM

Quant Time: Oct 10 09:08:03 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 08:36:11 2018
Response via : Initial Calibration

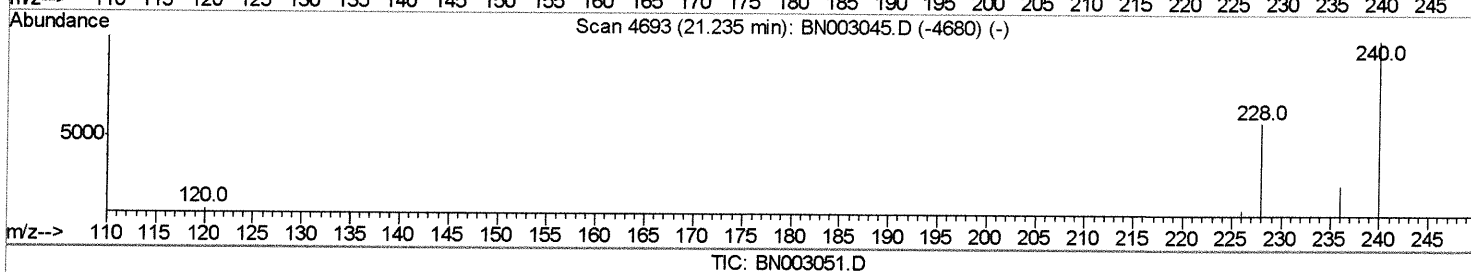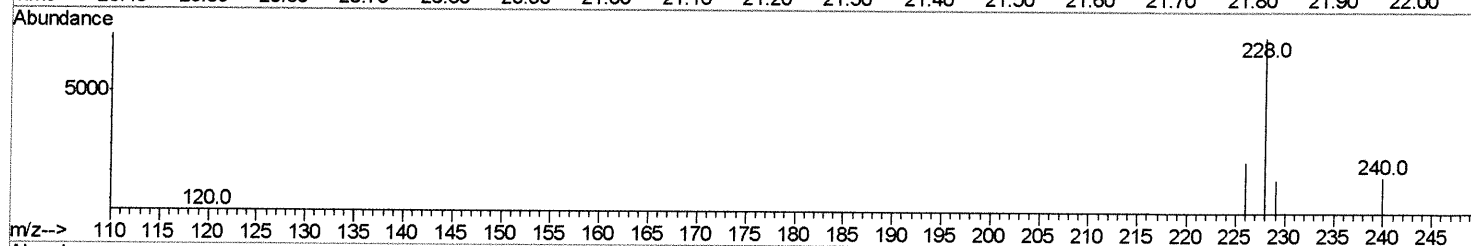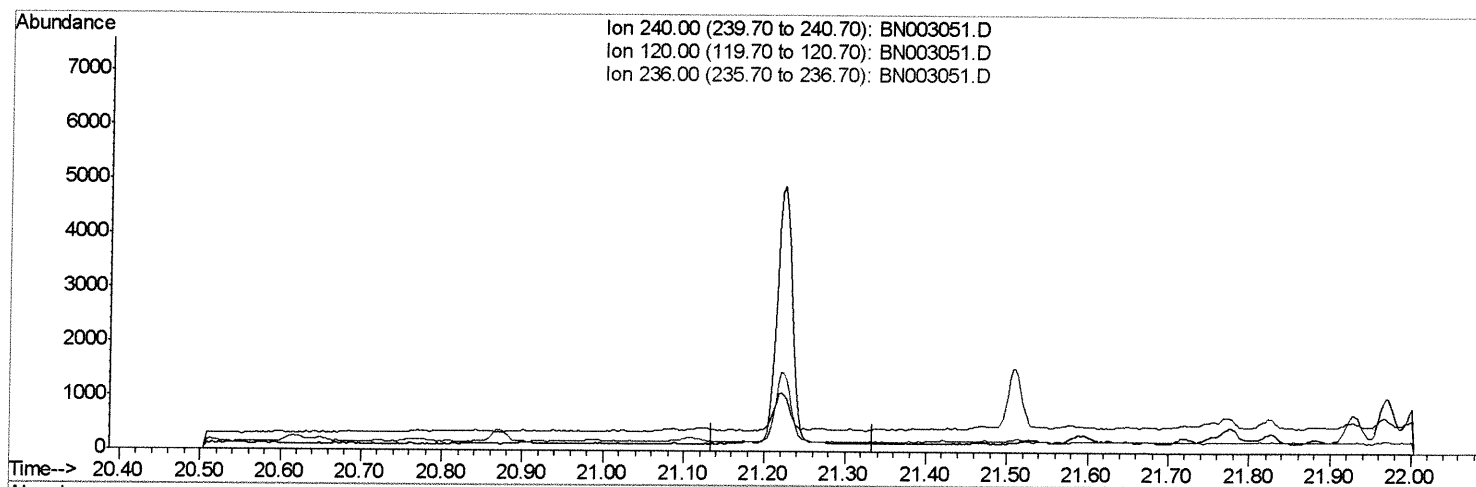

(16) Chrysene-d12 (I)

21.235min (-21.235) 0.00ng/ui

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	16.40	0.00#
236.00	28.10	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003051.D
Acq On : 10 Oct 2018 05:30
Operator : MJ/SJ
Sample : J5115-18
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC61

Manual Integrations
APPROVED

Sohil
10/10/2018 4:58:39 PM

Quant Time: Oct 10 09:08:03 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 08:36:11 2018
Response via : Initial Calibration

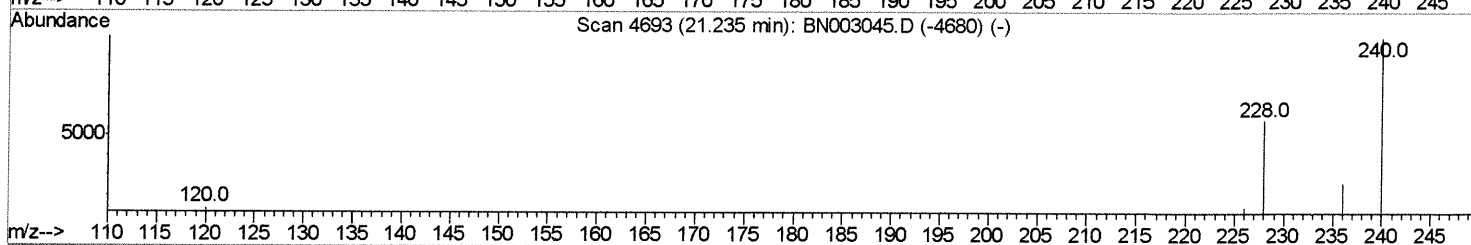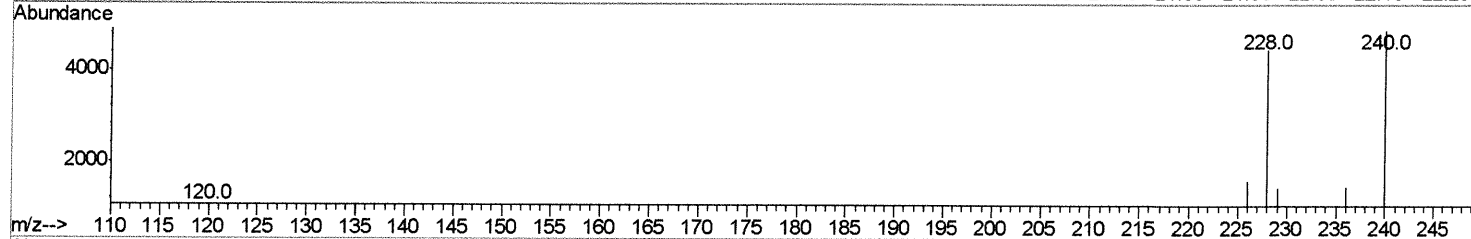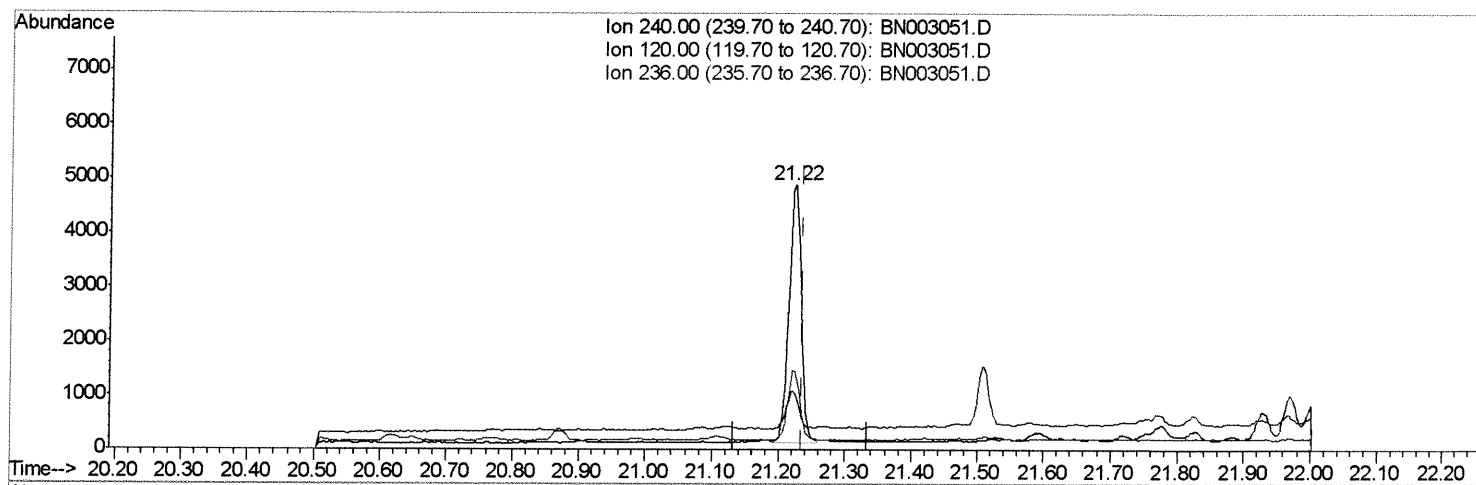

TIC: BN003051.D

(16) Chrysene-d12 (I)

21.223min (-0.012) 0.40ng/ul m

5010/12/18

response 6100

Ion	Exp%	Act%
240.00	100	100
120.00	16.40	21.34#
236.00	28.10	29.73
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003051.D
Acq On : 10 Oct 2018 05:30
Operator : MJ/SJ
Sample : J5115-18
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC61

Manual Integrations
APPROVED

Sohil
10/10/2018 4:58:39 PM

Quant Time: Oct 10 09:09:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 08:36:11 2018
Response via : Initial Calibration

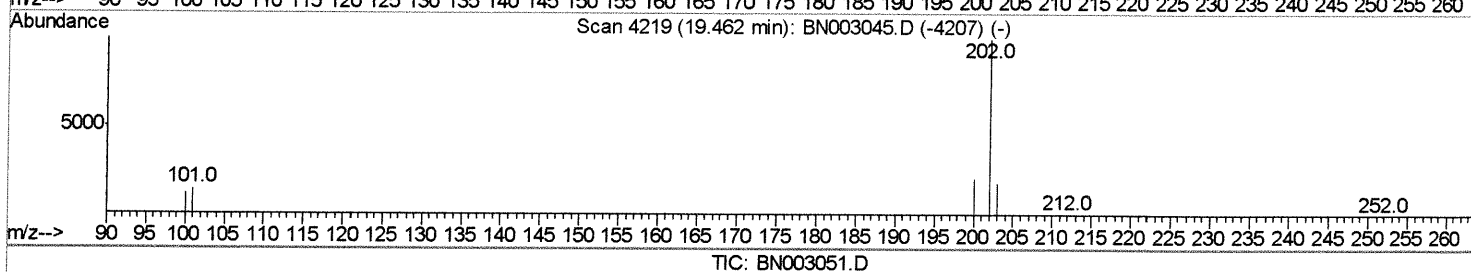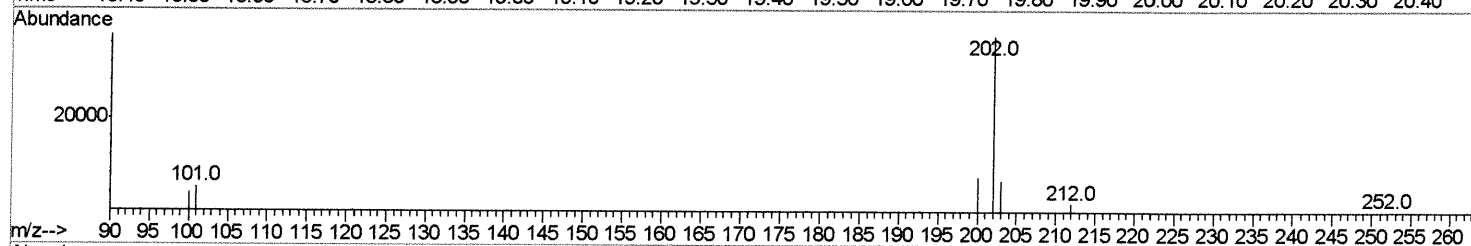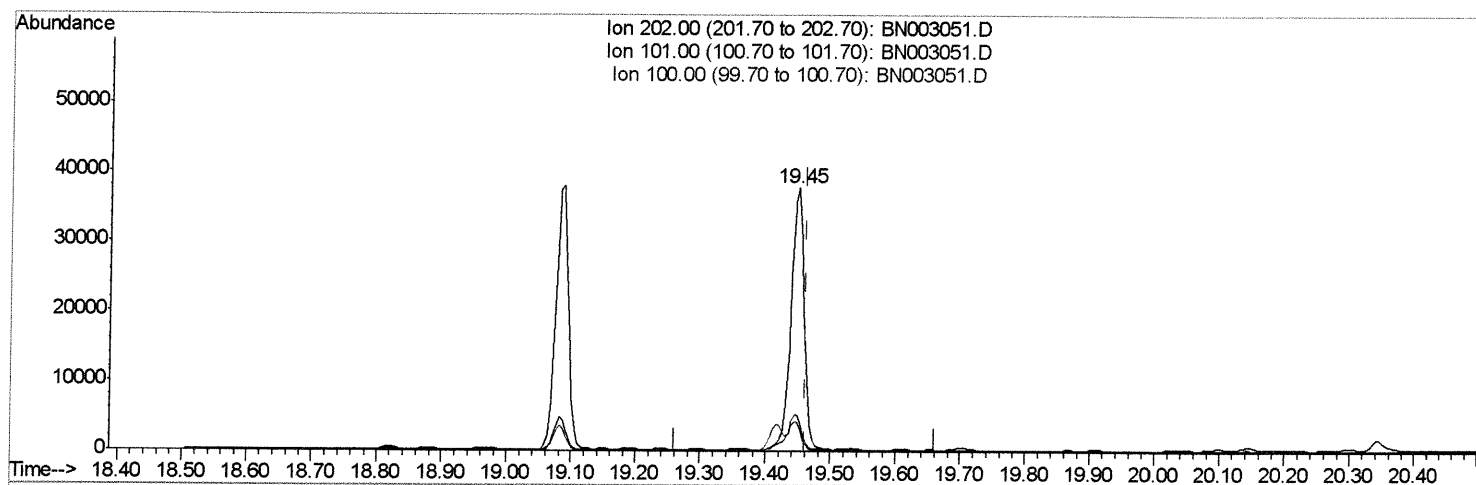

(17) Pyrene

19.448min (-0.014) 2.24ng/ul

response 53110

Ion	Exp%	Act%
202.00	100	100
101.00	14.90	13.62
100.00	12.40	10.78
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003051.D
Acq On : 10 Oct 2018 05:30
Operator : MJ/SJ
Sample : J5115-18
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC61

Manual Integrations
APPROVED

Sohil
10/10/2018 4:58:39 PM

Quant Time: Oct 10 09:09:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 08:36:11 2018
Response via : Initial Calibration

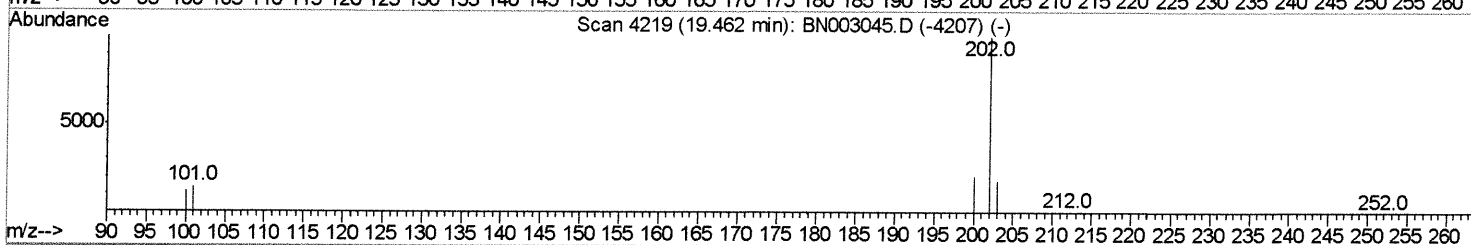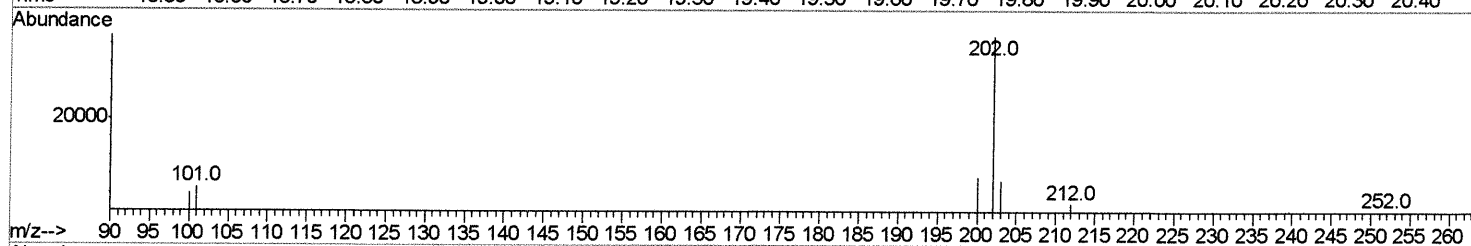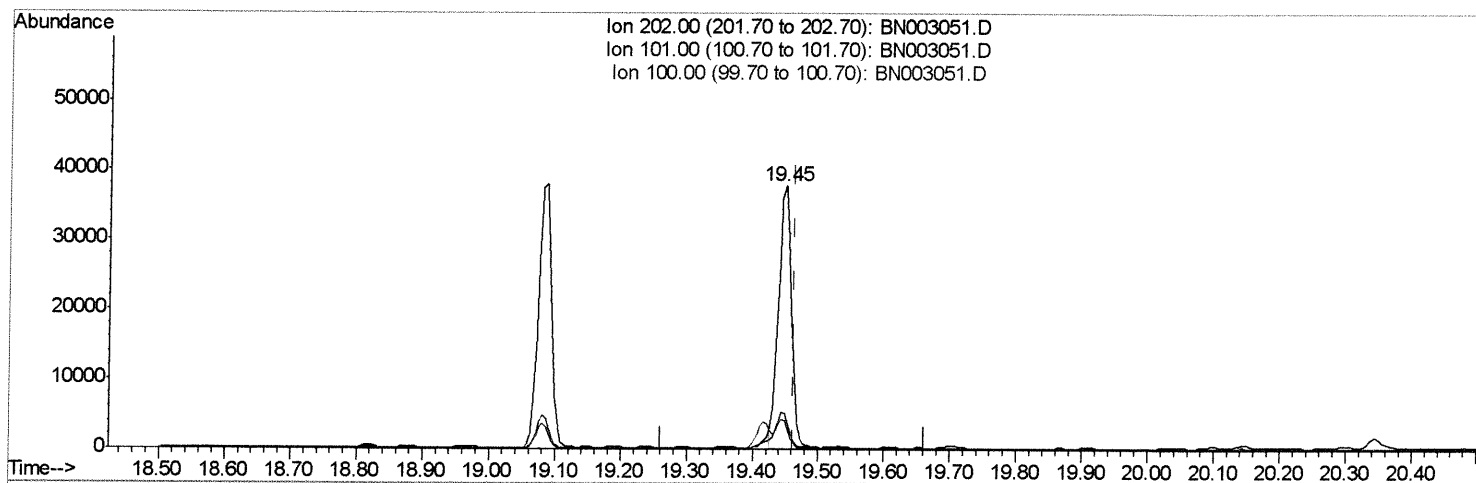

TIC: BN003051.D

(17) Pyrene

19.448min (-0.014) 2.17ng/ul m

SJ10/12/18

response 51497

Ion	Exp%	Act%
202.00	100	100
101.00	14.90	13.62
100.00	12.40	10.78
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003051.D
Acq On : 10 Oct 2018 05:30
Operator : MJ/SJ
Sample : J5115-18
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC61

Manual Integrations
APPROVED

Sohil
10/10/2018 4:58:39 PM

Quant Time: Oct 10 09:09:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 08:36:11 2018
Response via : Initial Calibration

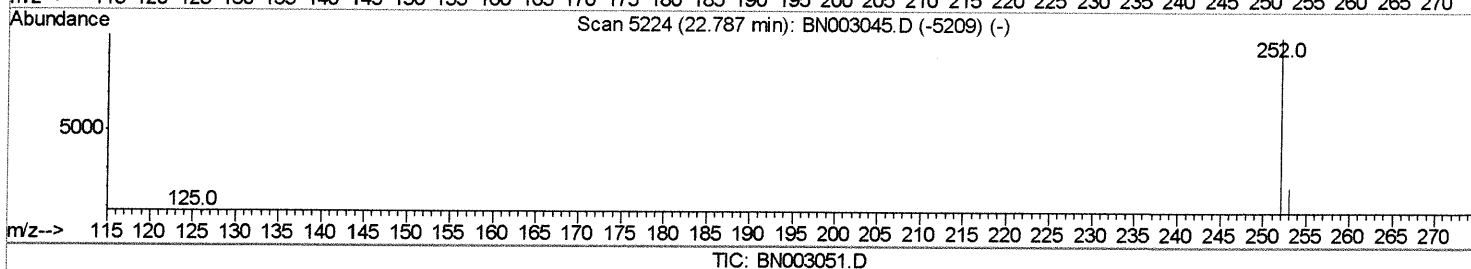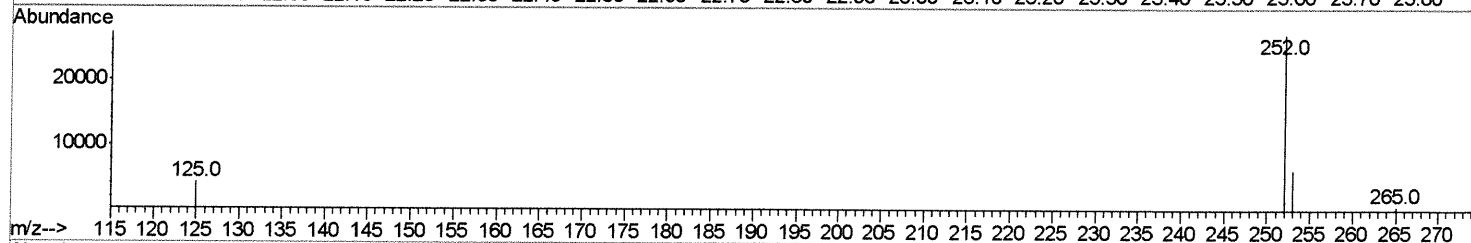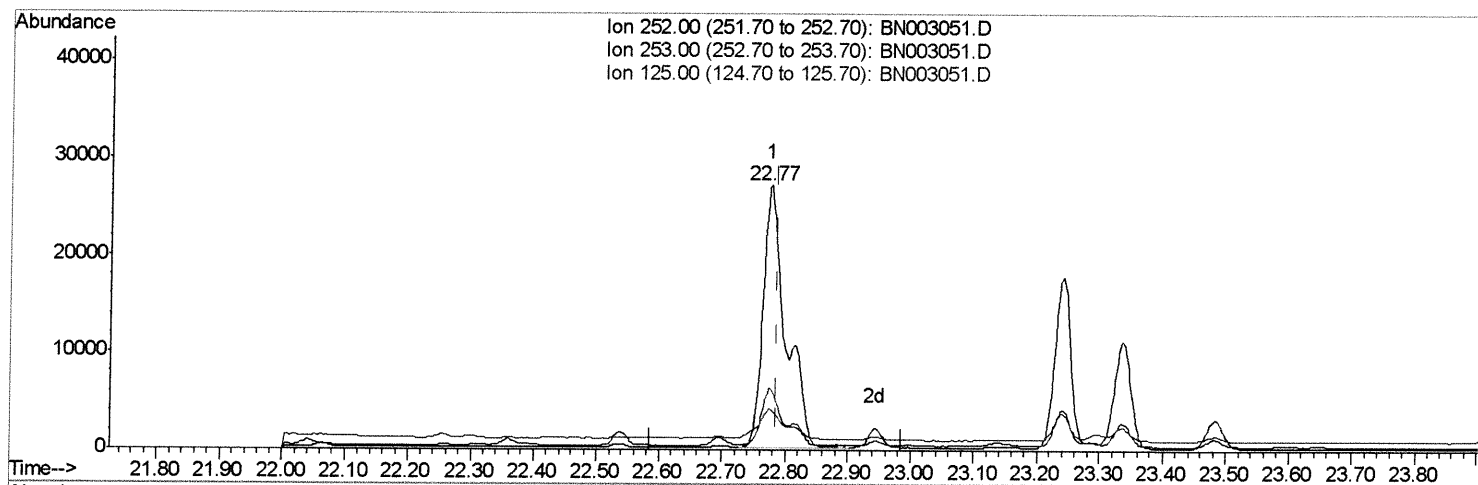

(21) Benzo(b)fluoranthene

22.775min (-0.012) 3.39ng/ul

response 68797

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	23.36
125.00	17.10	15.32
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003051.D
Acq On : 10 Oct 2018 05:30
Operator : MJ/SJ
Sample : J5115-18
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC61

Manual Integrations
APPROVED

Sohil
10/10/2018 4:58:39 PM

Quant Time: Oct 10 09:09:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 08:36:11 2018
Response via : Initial Calibration

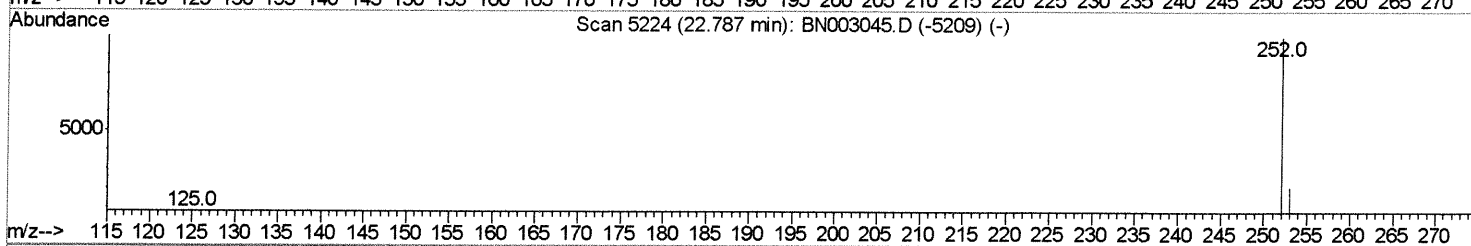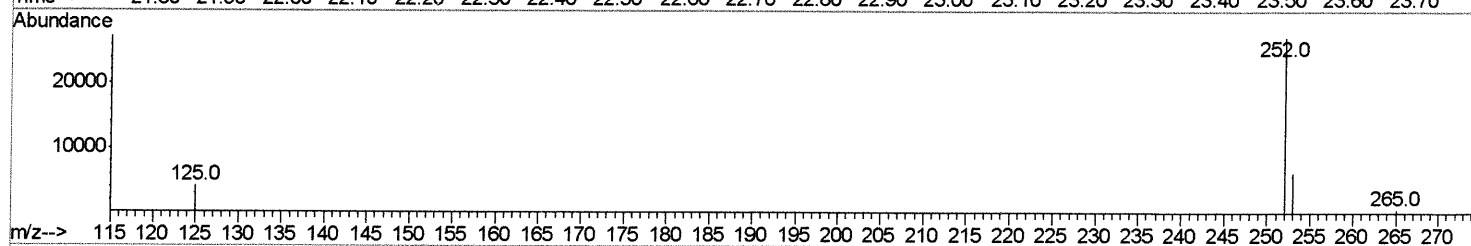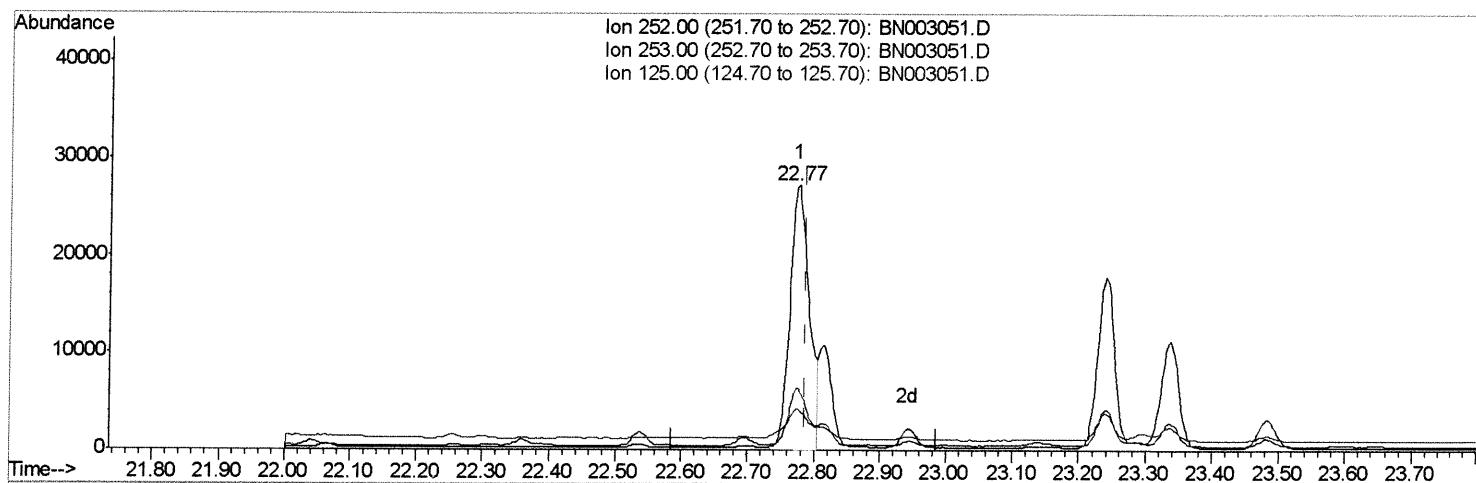

TIC: BN003051.D

(21) Benzo(b)fluoranthene

22.775min (-0.012) 2.72ng/ul m

5/10/12/18

response 55080

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	23.36
125.00	17.10	15.32
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003051.D
 Acq On : 10 Oct 2018 05:30
 Operator : MJ/SJ
 Sample : J5115-18
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC61

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:58:39 PM

Quant Time: Oct 10 09:09:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 08:36:11 2018
 Response via : Initial Calibration

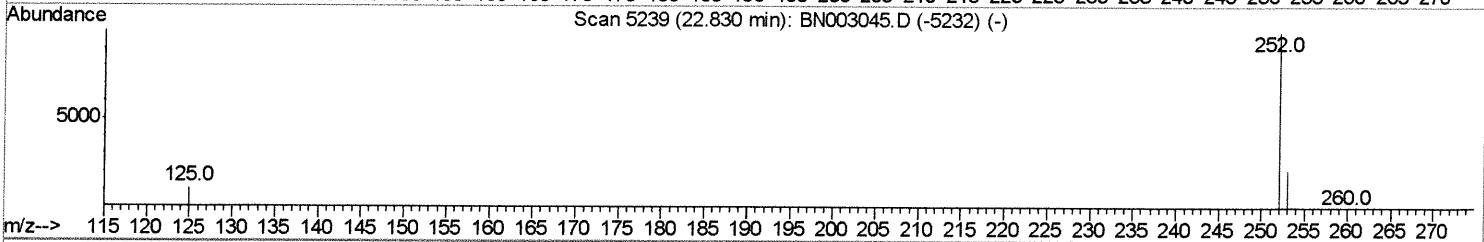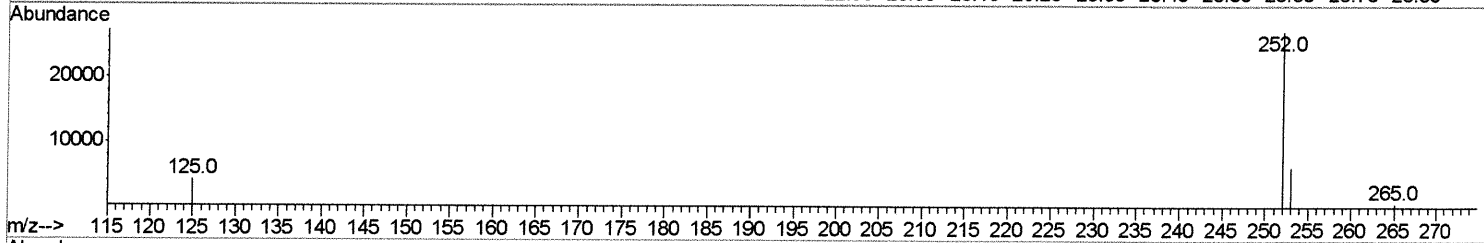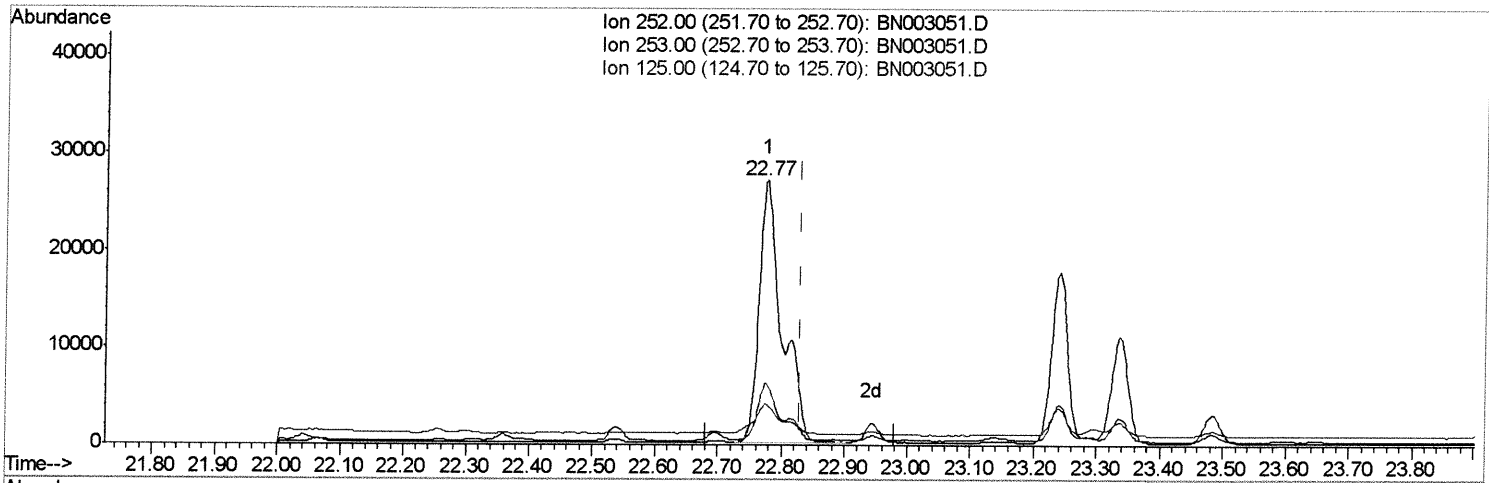

TIC: BN003051.D

(22) Benzo(k)fluoranthene

22.775min (-0.056) 3.27ng/ul

response 68797

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	23.36
125.00	17.60	15.32
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
Data File : BN003051.D
Acq On : 10 Oct 2018 05:30
Operator : MJ/SJ
Sample : J5115-18
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC61

Manual Integrations
APPROVED

Sohil
10/10/2018 4:58:39 PM

Quant Time: Oct 10 09:09:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 10 08:36:11 2018
Response via : Initial Calibration

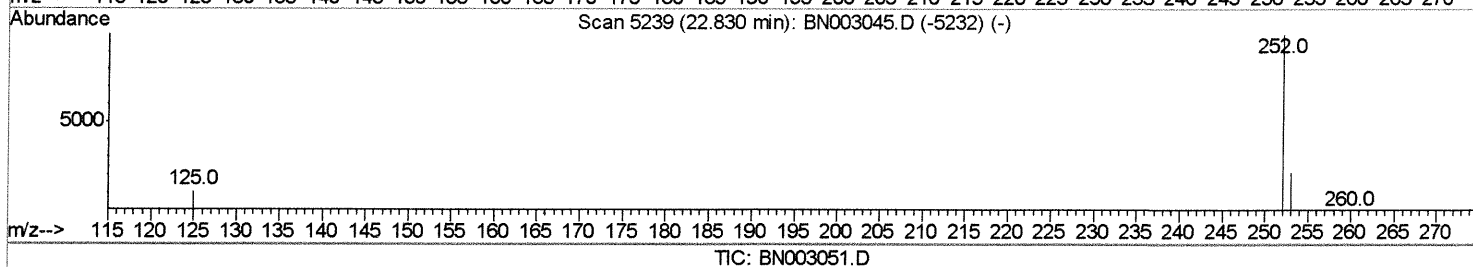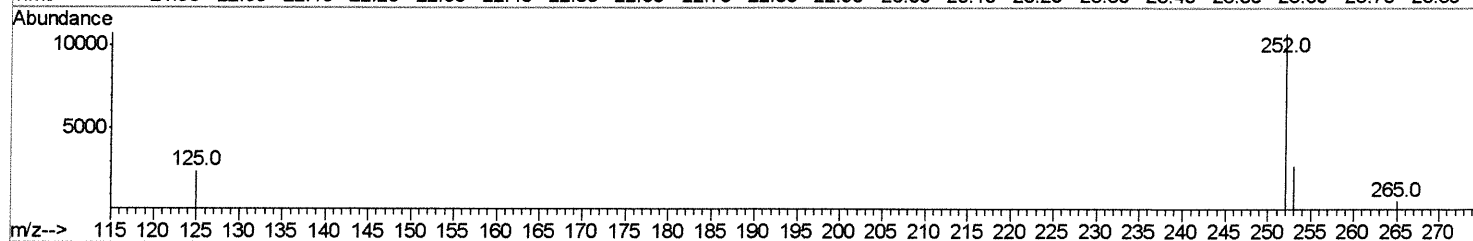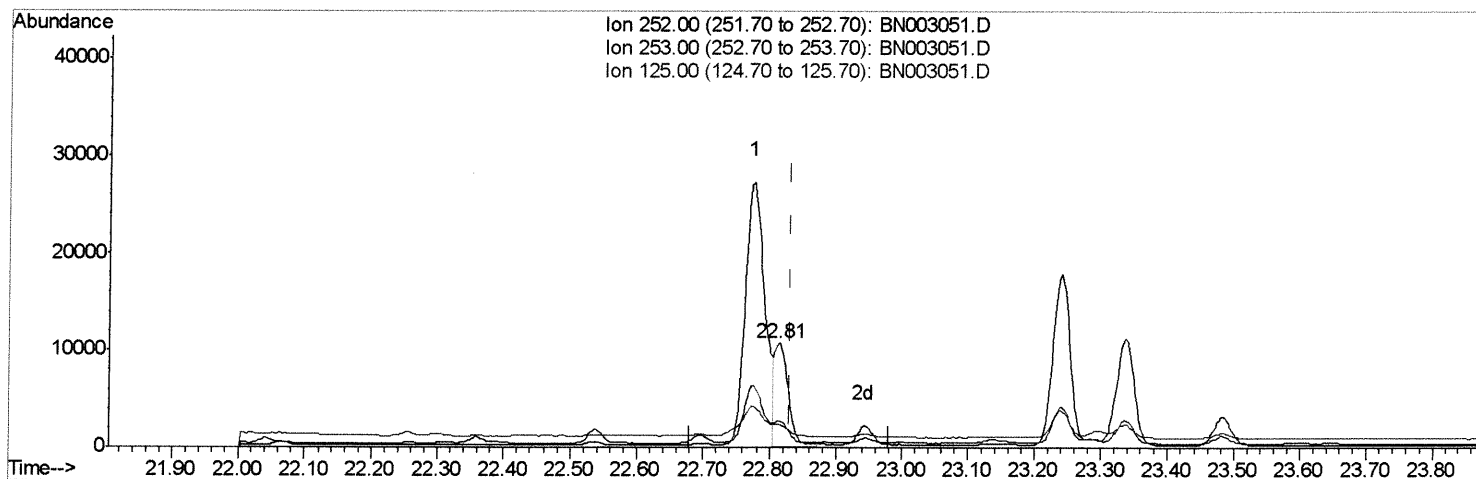

(22) Benzo(k)fluoranthene

22.813min (-0.018) 0.71ng/ul m

SJ 10/12/18

response 14957

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	25.59
125.00	17.60	22.35#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101018\
 Data File : BN003051.D
 Acq On : 10 Oct 2018 05:30
 Operator : MJ/SJ
 Sample : J5115-18
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC61

Manual Integrations
 APPROVED

Sohil
 10/10/2018 4:58:39 PM

Quant Time: Oct 10 09:10:34 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 10 08:36:11 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	1907	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.39	136	7930	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.26	164	4419	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.01	188	9507m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.22	240	6100m	0.40	ng/ul	-0.01
20) Perylene-d12	23.44	264	5633	0.40	ng/ul	-0.01

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.00	152	2605	0.21	ng/ul	-0.01
14) Fluoranthene-d10	19.05	212	5457m	0.20	ng/ul	-0.01

Target Compounds

					Ovalue	
3) Naphthalene	10.44	128	1711	0.084	ng/ul#	91
5) 2-Methylnaphthalene	12.07	142	638	0.046	ng/ul	95
7) Acenaphthylene	13.98	152	893	0.044	ng/ul#	71
8) Acenaphthene	14.32	153	1232	0.080	ng/ul	97
9) Fluorene	15.32	166	1132	0.064	ng/ul#	95
11) Pentachlorophenol	16.72	266	106m	0.115	ng/ul	
12) Phenanthrene	17.06	178	21272	0.803	ng/ul	99
13) Anthracene	17.15	178	4169m	0.167	ng/ul	
15) Fluoranthene	19.09	202	51154m	1.645	ng/ul	
17) Pyrene	19.45	202	51497m	2.174	ng/ul	
18) Benzo(a)anthracene	21.21	228	25511	1.300	ng/ul	98
19) Chrysene	21.26	228	42334	2.124	ng/ul	99
21) Benzo(b)fluoranthene	22.77	252	55080m	2.715	ng/ul	
22) Benzo(k)fluoranthene	22.81	252	14957m	0.711	ng/ul	
23) Benzo(a)pyrene	23.34	252	20792	1.144	ng/ul	96
24) Indeno(1,2,3-cd)pyrene	25.64	276	19959	0.955	ng/ul#	94
25) Dibenzo(a,h)anthracene	25.64	278	5423	0.324	ng/ul#	82
26) Benzo(a,h,i)perylene	26.32	276	22580	1.282	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed