
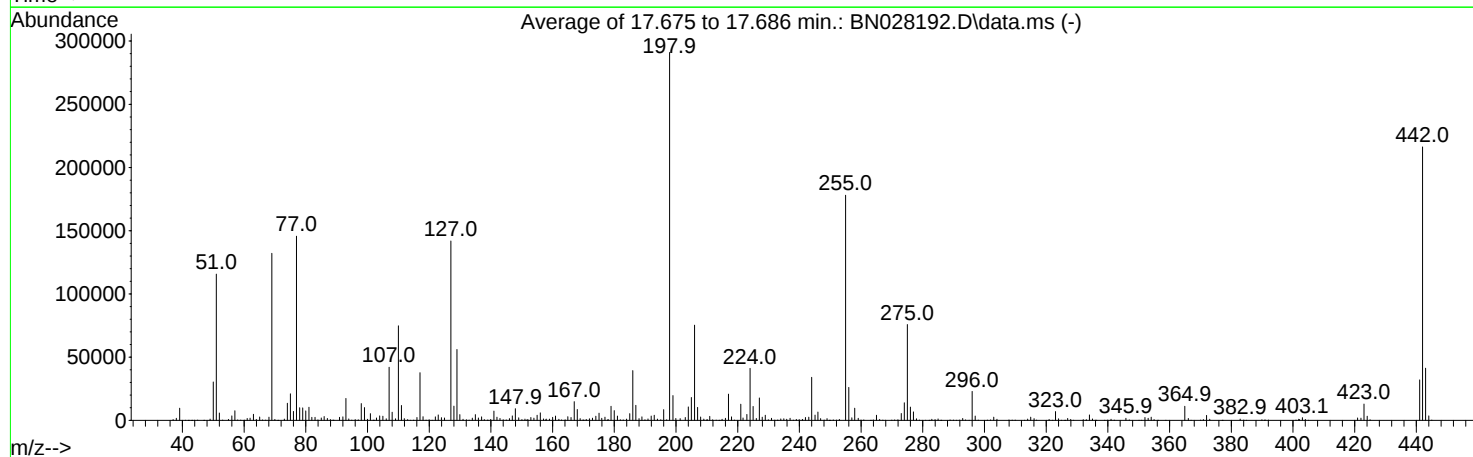


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101023\
Data File : BN028192.D
Acq On : 10 Oct 2023 12:00
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN100223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 11 18:40:16 2023

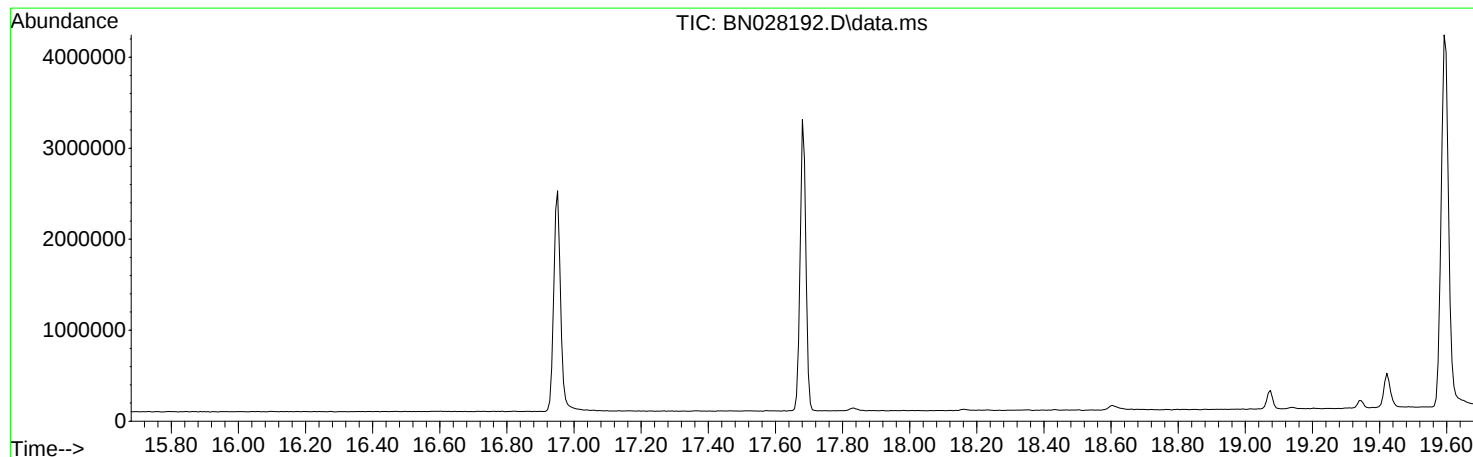




AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.8	115708	PASS
68	69	0.00	2	1.9	2569	PASS
69	198	0.00	100	45.4	132171	PASS
70	69	0.00	2	0.5	715	PASS
127	198	10	80	48.8	141931	PASS
197	198	0.00	2	0.2	514	PASS
198	198	100	100	100.0	290944	PASS
199	198	5	9	6.7	19622	PASS
275	198	10	60	26.0	75781	PASS
365	198	1	100	3.8	11141	PASS
441	198	0.01	100	11.0	32077	PASS
442	442	50	100	100.0	216336	PASS
443	442	15	24	19.1	41272	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101023\
Data File : BN028192.D
Acq On : 10 Oct 2023 12:00
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 11 06:03:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 06:03:31 2023
Response via : Initial Calibration

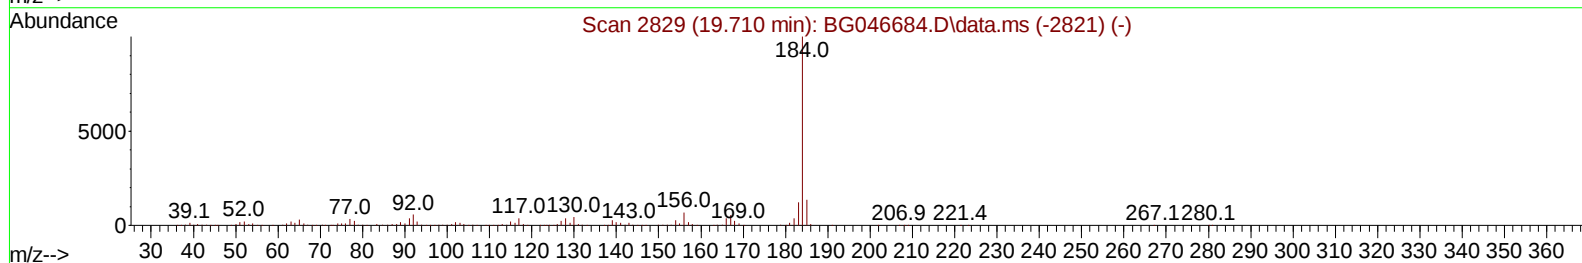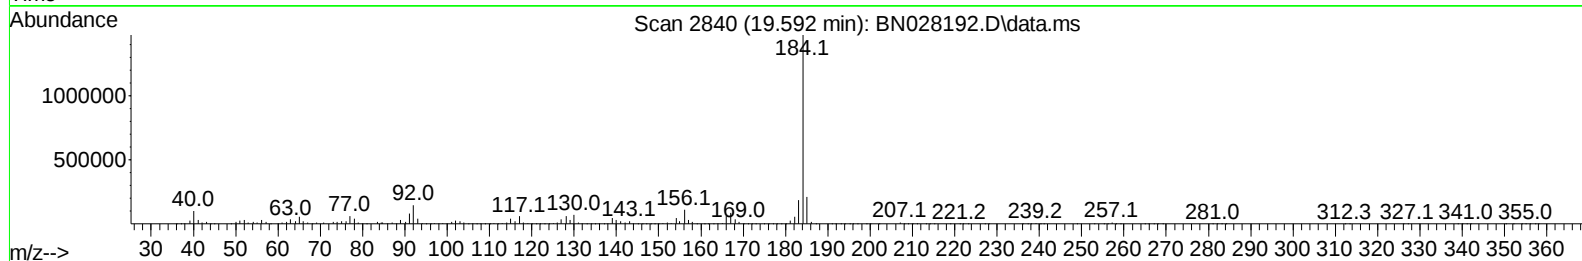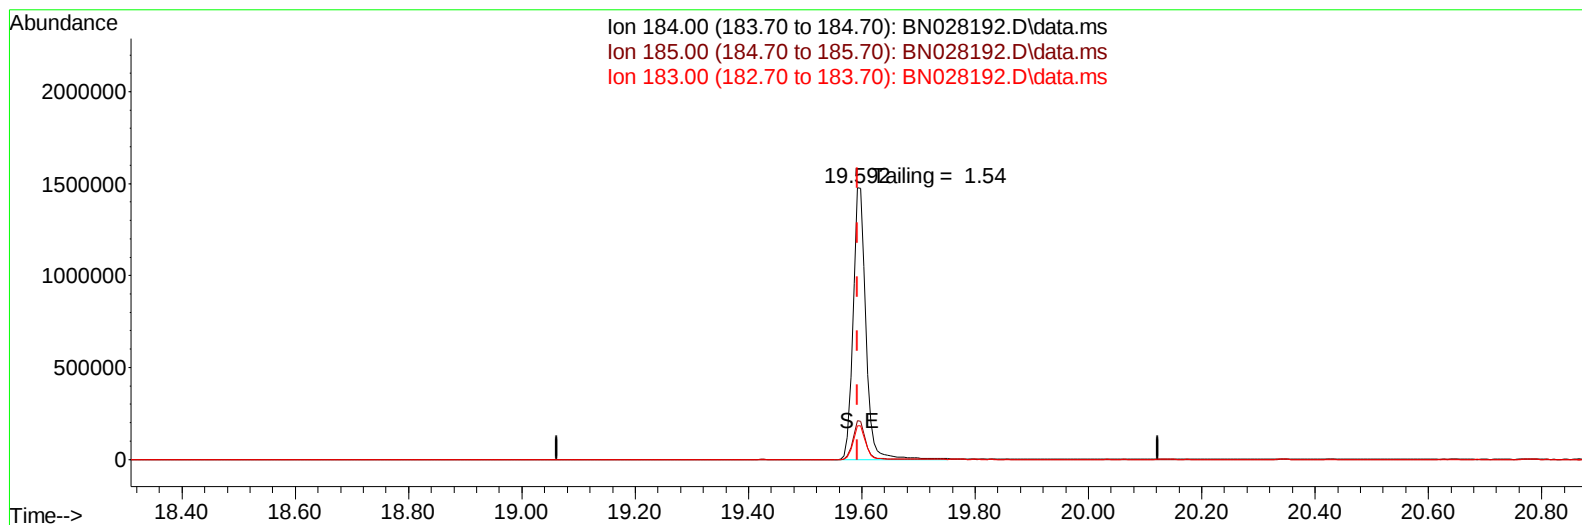

TIC: BN028192.D\data.ms

(77) Benzidine

19.592min (0.000) 257721.81 ng

response 2335645

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.36
183.00	13.20	12.45
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/10/2023	BNA_N	<u>BN028192.D</u>
Compound Name	Response	Retention Time
DDT	667744	20.78
DDD	284939	20.345
DDE	14604	19.827
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
299543	967287	30.97

Instrument :
BNA_N
ClientSampleId :
DFTPP