
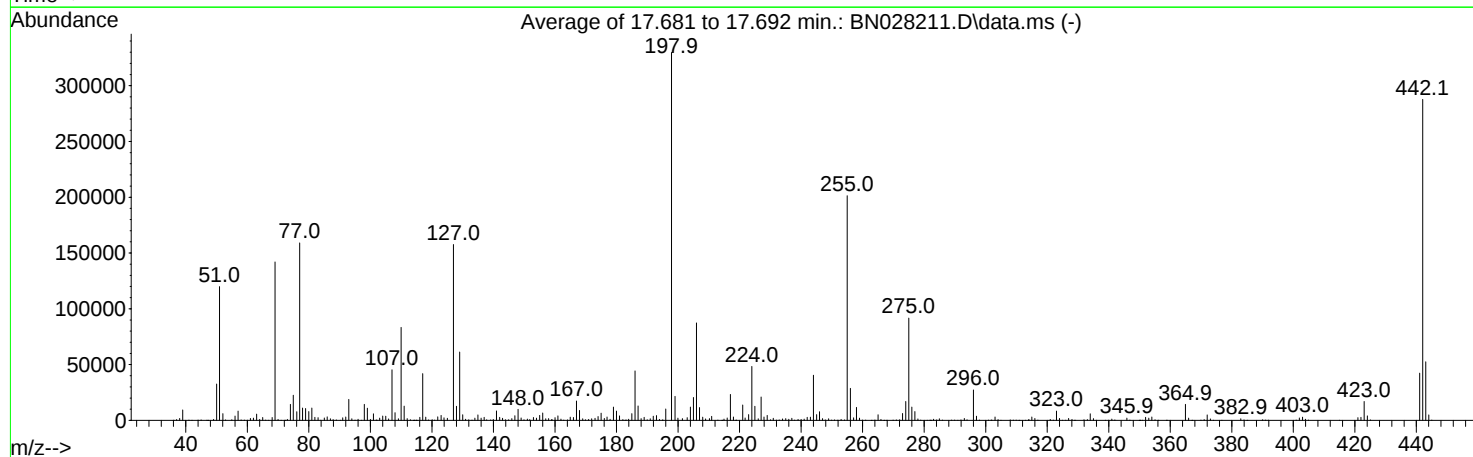


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101023\
Data File : BN028211.D
Acq On : 11 Oct 2023 00:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN100223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 11 18:40:16 2023

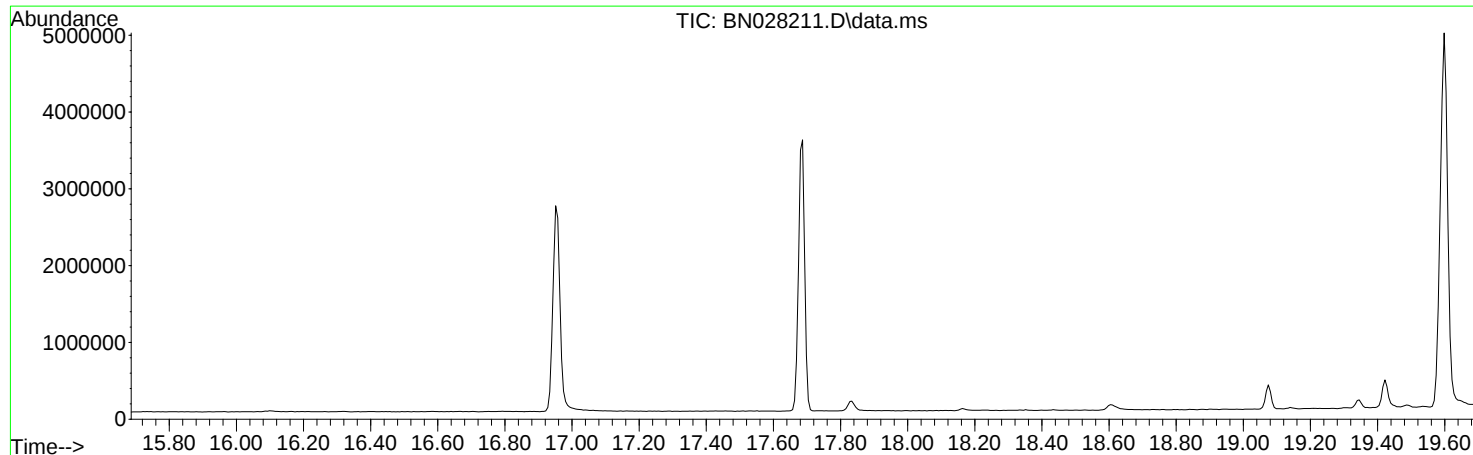




AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	119947	PASS
68	69	0.00	2	1.9	2649	PASS
69	198	0.00	100	43.1	142002	PASS
70	69	0.00	2	0.6	820	PASS
127	198	10	80	47.8	157688	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	329749	PASS
199	198	5	9	6.5	21460	PASS
275	198	10	60	27.8	91653	PASS
365	198	1	100	4.3	14324	PASS
441	198	0.01	100	12.8	42355	PASS
442	442	50	100	100.0	287701	PASS
443	442	15	24	18.2	52467	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101023\
Data File : BN028211.D
Acq On : 11 Oct 2023 00:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 11 06:05:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 06:03:31 2023
Response via : Initial Calibration

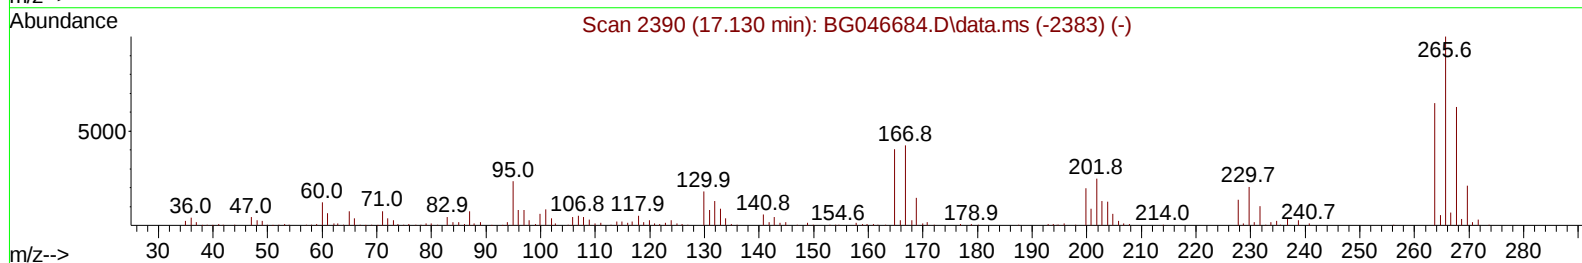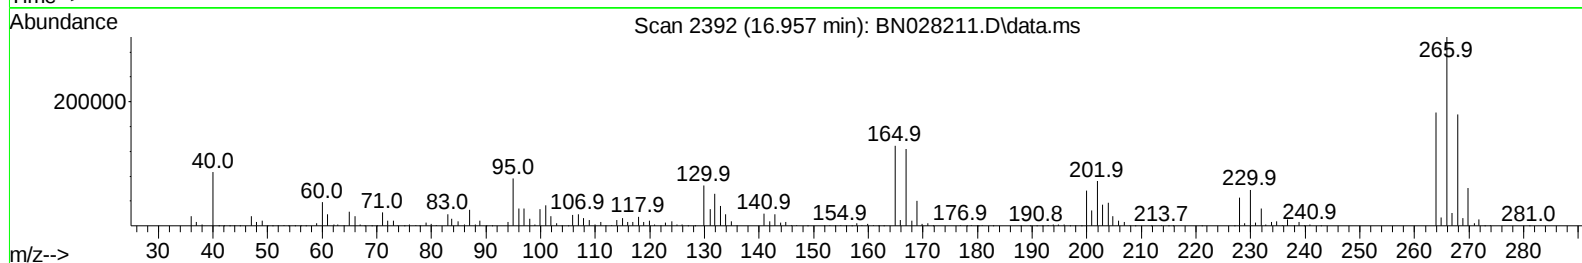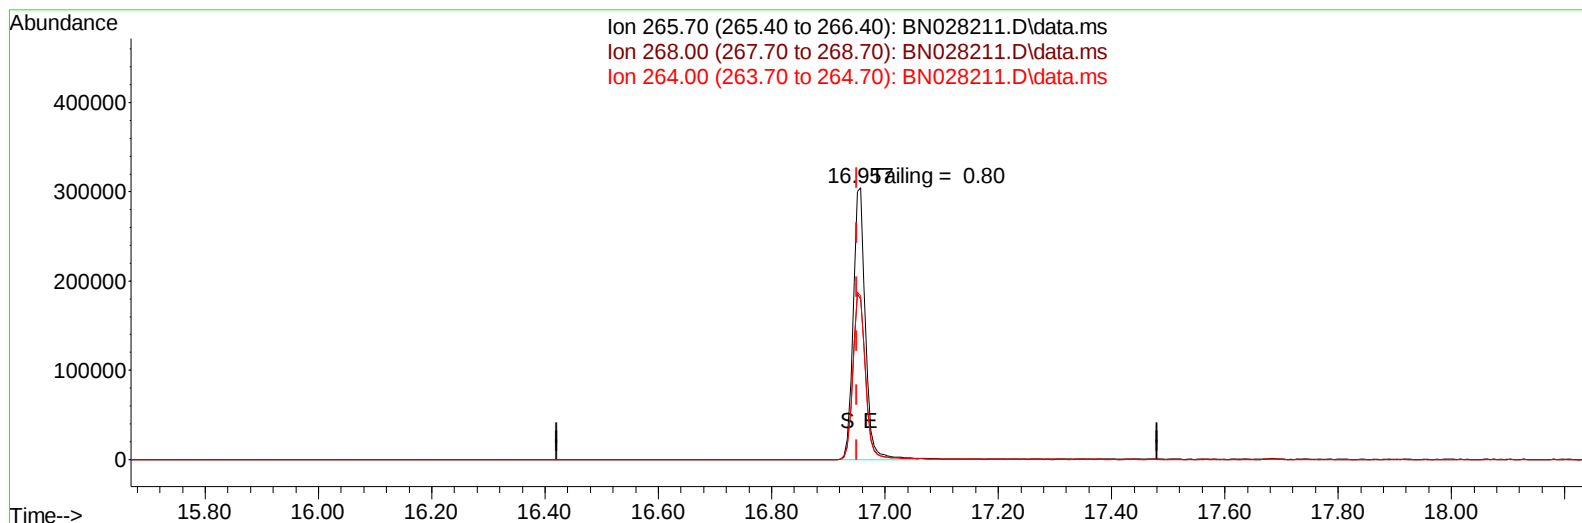

TIC: BN028211.D\data.ms

(70) Pentachlorophenol (C)

16.957min (+ 0.006) 25683.00 ng




response 459341

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.96
264.00	61.60	60.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101023\
Data File : BN028211.D
Acq On : 11 Oct 2023 00:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 11 06:05:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 06:03:31 2023
Response via : Initial Calibration

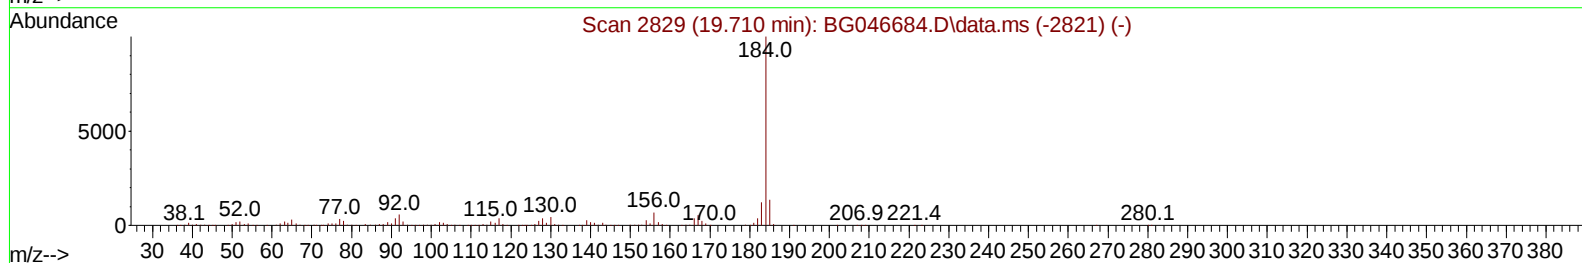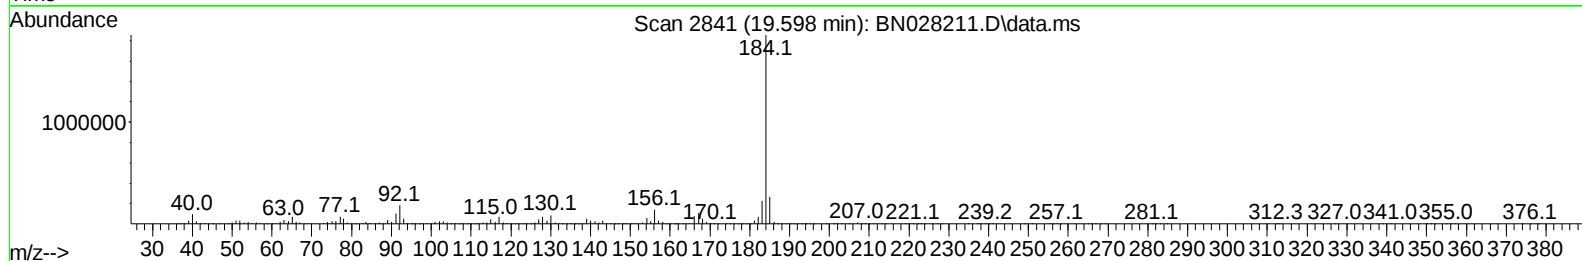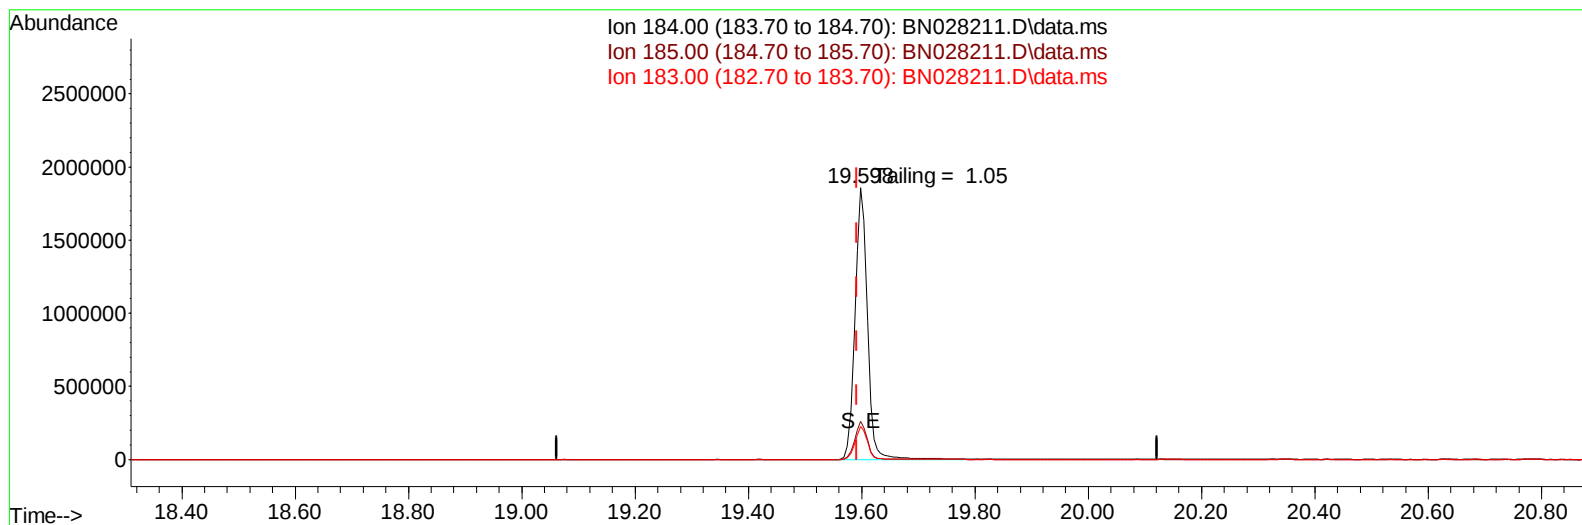

TIC: BN028211.D\data.ms

(77) Benzidine

19.598min (+ 0.006) 564044.77 ng

response 2834063

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.10
183.00	13.20	12.18
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/10/2023	BNA_N	<u>BN028211.D</u>
Compound Name	Response	Retention Time
DDT	430944	20.78
DDD	536824	20.345
DDE	2551	19.828
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
539375	970319	55.59

Instrument :
BNA_N
ClientSampleId :
DFTPP