

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101118\
 Data File : BN003090.D
 Acq On : 11 Oct 2018 06:29
 Operator : MJ/SJ
 Sample : J5234-05
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Oct 11 08:14:23 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 08:10:30 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	1657	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.39	136	6968	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.26	164	3929	0.40	ng/ul	-0.01
10) Phenanthrene-d10	17.11	188	372413	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.24
20) Perylene-d12	23.44	264	4806	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.01	152	2711	0.25	ng/ul	-0.01
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
21) Benzo(b)fluoranthene	22.78	252	411	0.024	ng/ul#	1
23) Benzo(a)pyrene	23.29	252	1033	0.067	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101118\
Data File : BN003090.D
Acq On : 11 Oct 2018 06:29
Operator : MJ/SJ
Sample : J5234-05
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Oct 11 08:14:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 08:10:30 2018
Response via : Initial Calibration



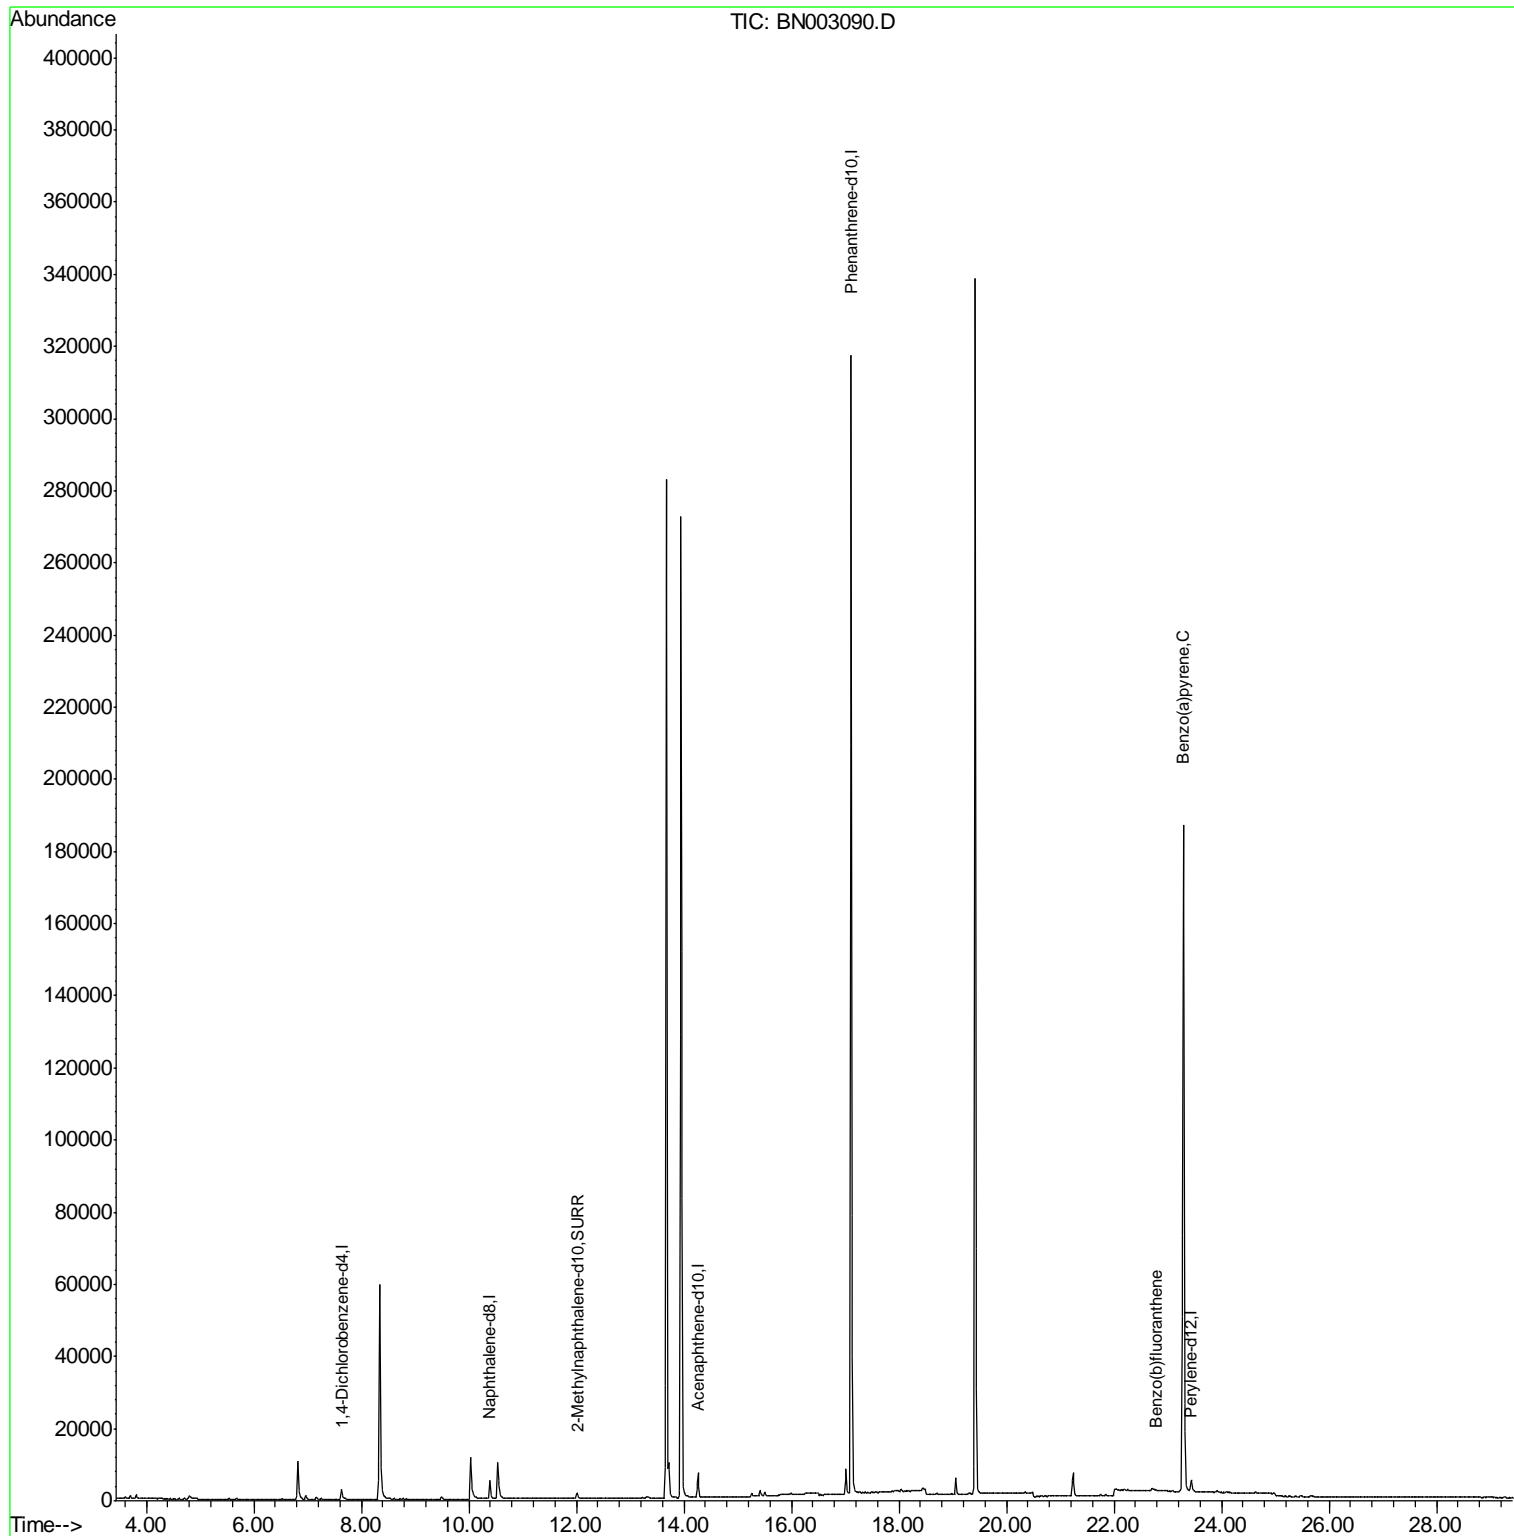


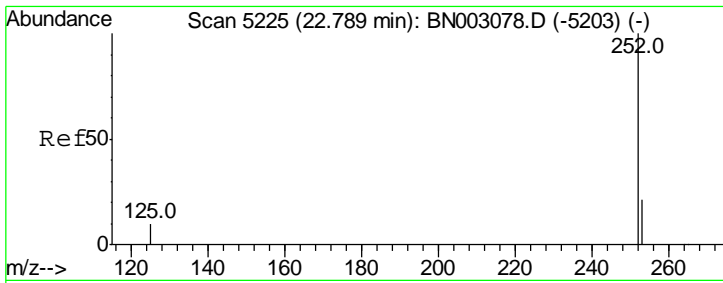

#21
 Benzo(b)fluoranthene
 Concen: 0.024 ng/ul
 RT: 22.78 min Scan# 5223
 Delta R.T. -0.01 min
 Lab File: BN003090.D
 Acq: 11 Oct 2018 06:29

Instrument :
 BNA_N
 ClientSampled :

Tgt Ion	Resp	Lower	Upper
252	411		
253	97.2	0.0	53.2#
125	462.9	0.0	34.2#

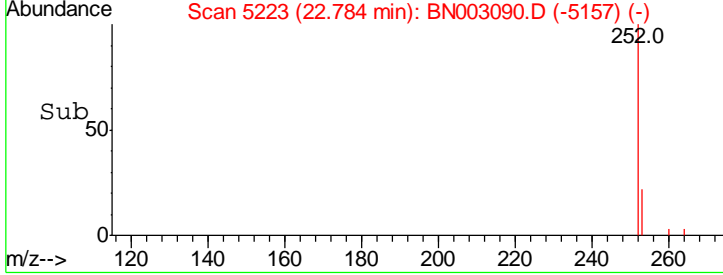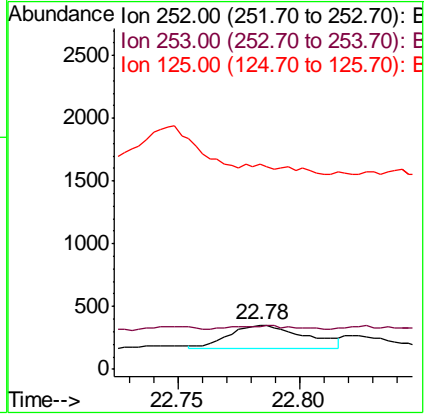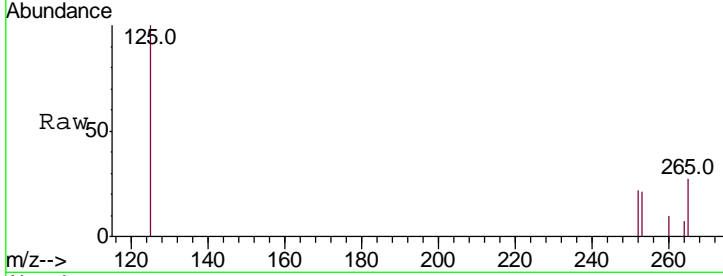

#23
 Benzo(a)pyrene
 Concen: 0.067 ng/ul
 RT: 23.29 min Scan# 5397
 Delta R.T. -0.07 min
 Lab File: BN003090.D
 Acq: 11 Oct 2018 06:29

Tgt Ion	Resp	Lower	Upper
252	1033		
253	70.4	23.1	34.7#
125	274.1	16.9	25.3#

