

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101118\
 Data File : BN003091.D
 Acq On : 11 Oct 2018 07:04
 Operator : MJ/SJ
 Sample : J5230-07
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Oct 11 08:14:26 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 08:10:30 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	1623	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.39	136	6592	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.26	164	3609	0.40	ng/ul	-0.01
10) Phenanthrene-d10	17.11	188	562669	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.24
20) Perylene-d12	23.44	264	5416	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.01	152	4512	0.44	ng/ul	-0.01
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.26	166	1055	0.074	ng/ul#	16
23) Benzo(a)pyrene	23.29	252	1870	0.107	ng/ul#	10


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101118\
Data File : BN003091.D
Acq On : 11 Oct 2018 07:04
Operator : MJ/SJ
Sample : J5230-07
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Oct 11 08:14:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 08:10:30 2018
Response via : Initial Calibration




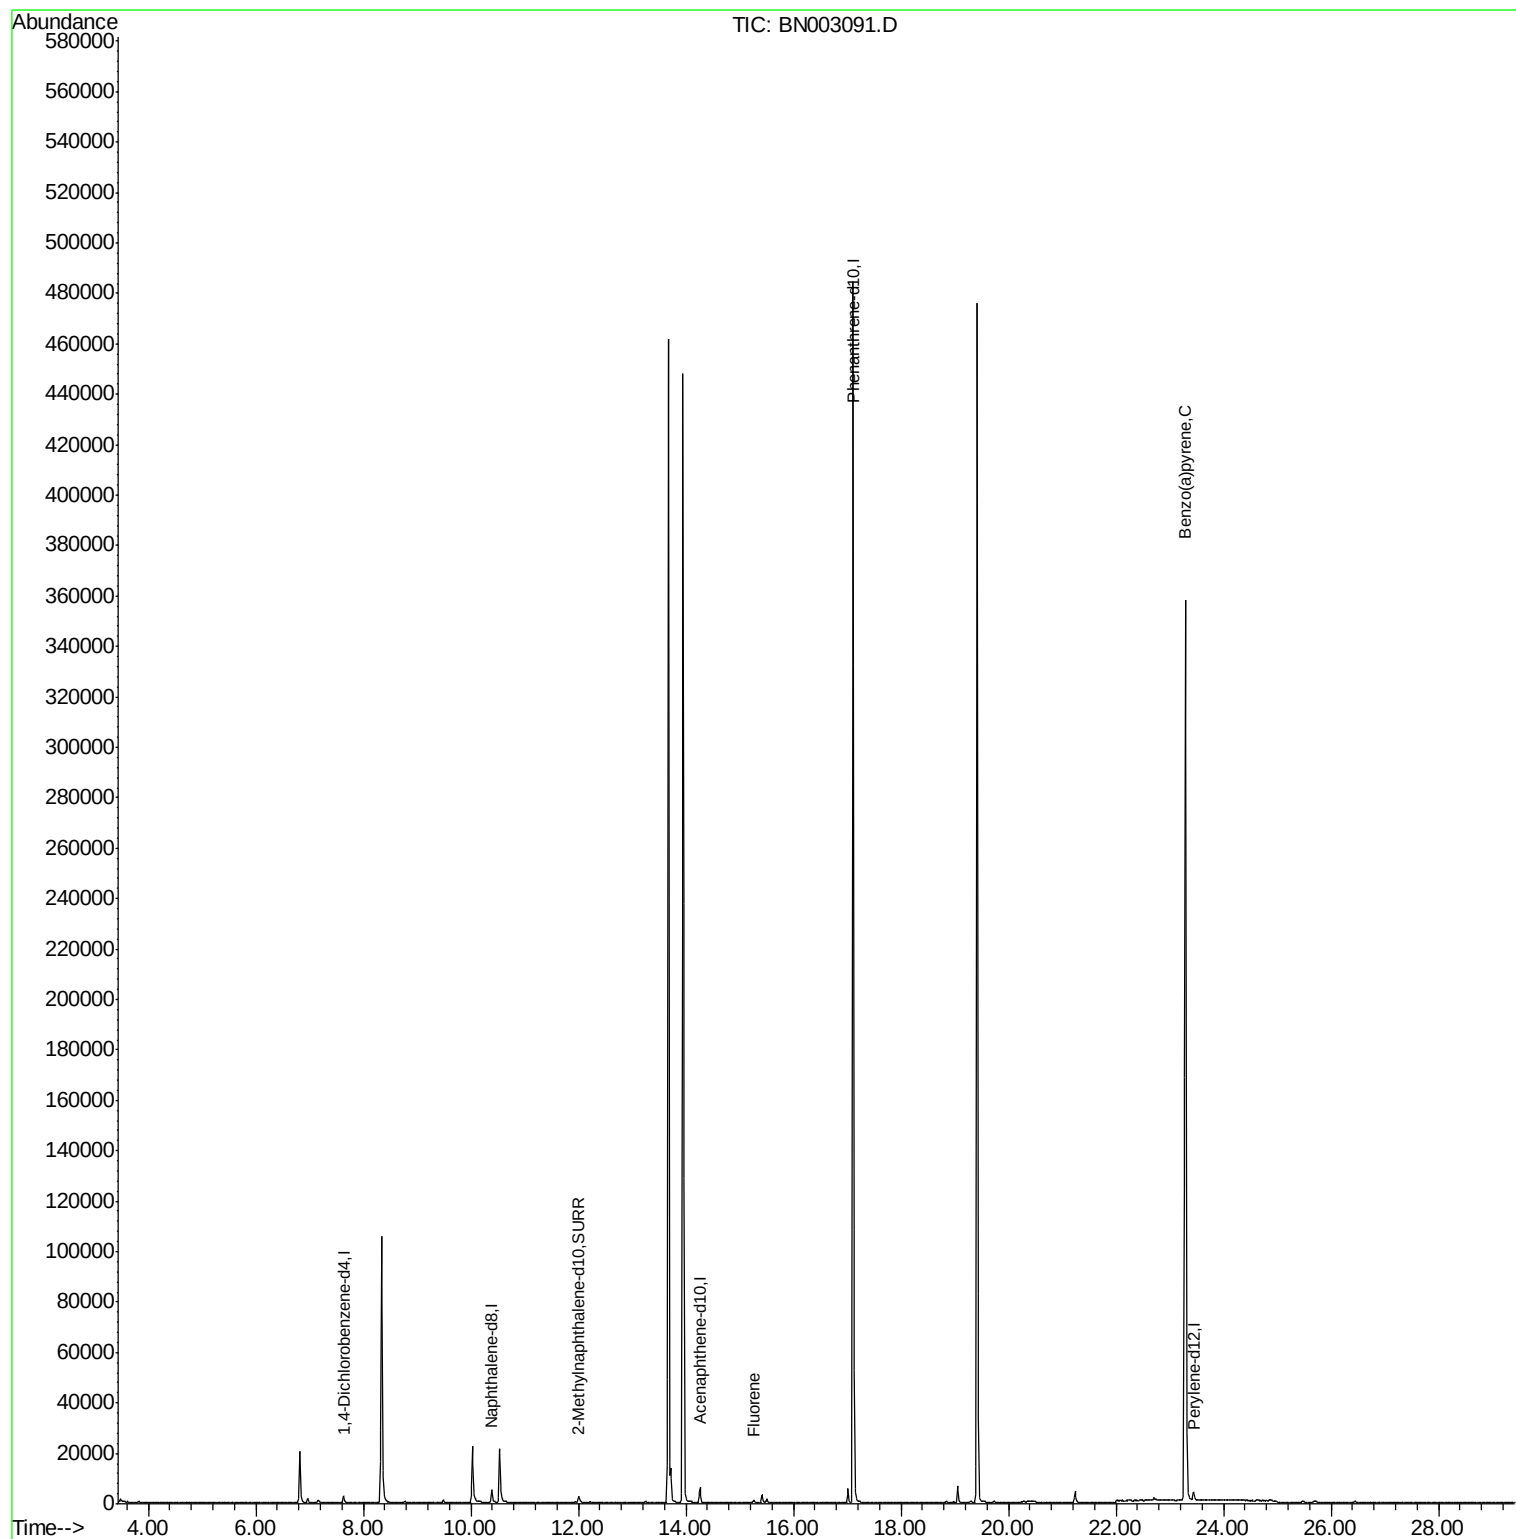


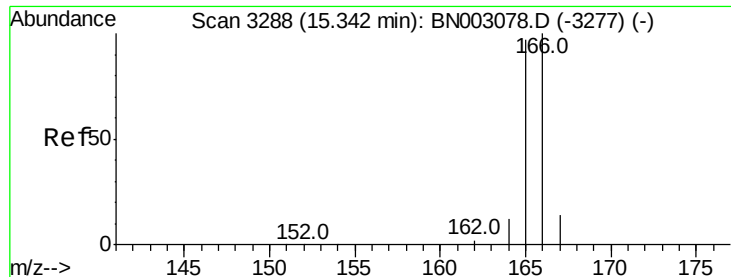

#9
Fluorene
 Concen: 0.074 ng/ul
 RT: 15.26 min Scan# 3270
 Delta R.T. -0.08 min
 Lab File: BN003091.D
 Acq: 11 Oct 2018 07:04

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion:166 Resp: 1055
 Ion Ratio Lower Upper
 166 100
 165 10.2 78.5 117.7#
 167 35.0 11.6 17.4#

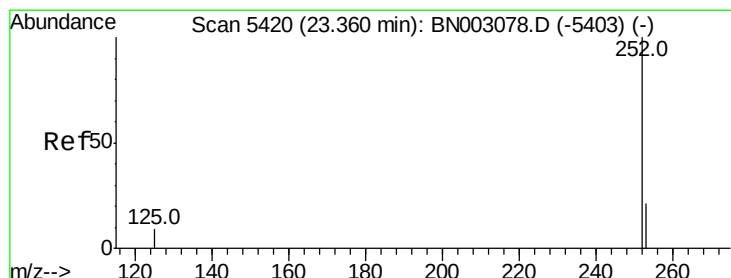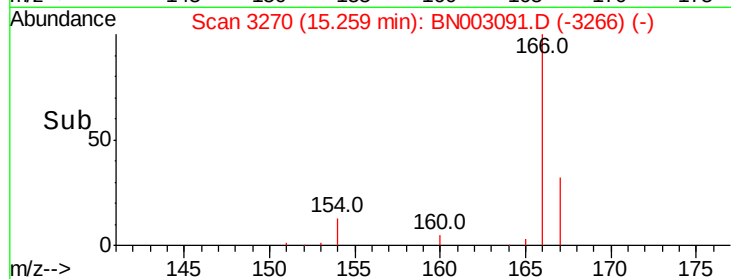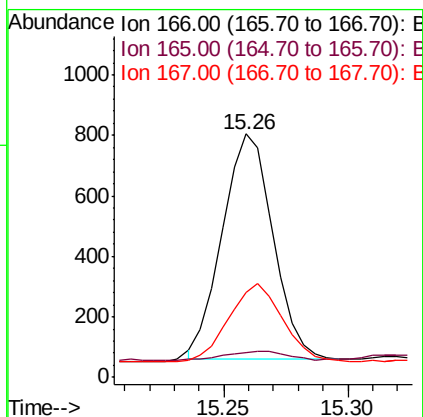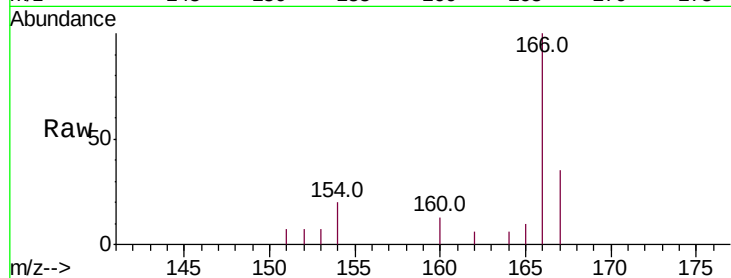

#23
Benzo(a)pyrene
 Concen: 0.107 ng/ul
 RT: 23.29 min Scan# 5396
 Delta R.T. -0.07 min
 Lab File: BN003091.D
 Acq: 11 Oct 2018 07:04

Tgt Ion:252 Resp: 1870
 Ion Ratio Lower Upper
 252 100
 253 48.4 23.1 34.7#
 125 97.7 16.9 25.3#

