

(QT Reviewed)


```
Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101118\
Data File : BN003075.D
Acq On    : 10 Oct 2018   21:41
Operator  : MJ/SJ
Sample    : J5157-19
Misc      :
ALS Vial  : 13      Sample Multiplier: 1
```

Instrument :
BNA_N
ClientSampleId :
C0AE1

Manual Integrations
APPROVED

Sohil
10/11/2018 5:45:41 PM

Quant Time: Oct 11 08:00:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 07:04:52 2018
Response via : Initial Calibration

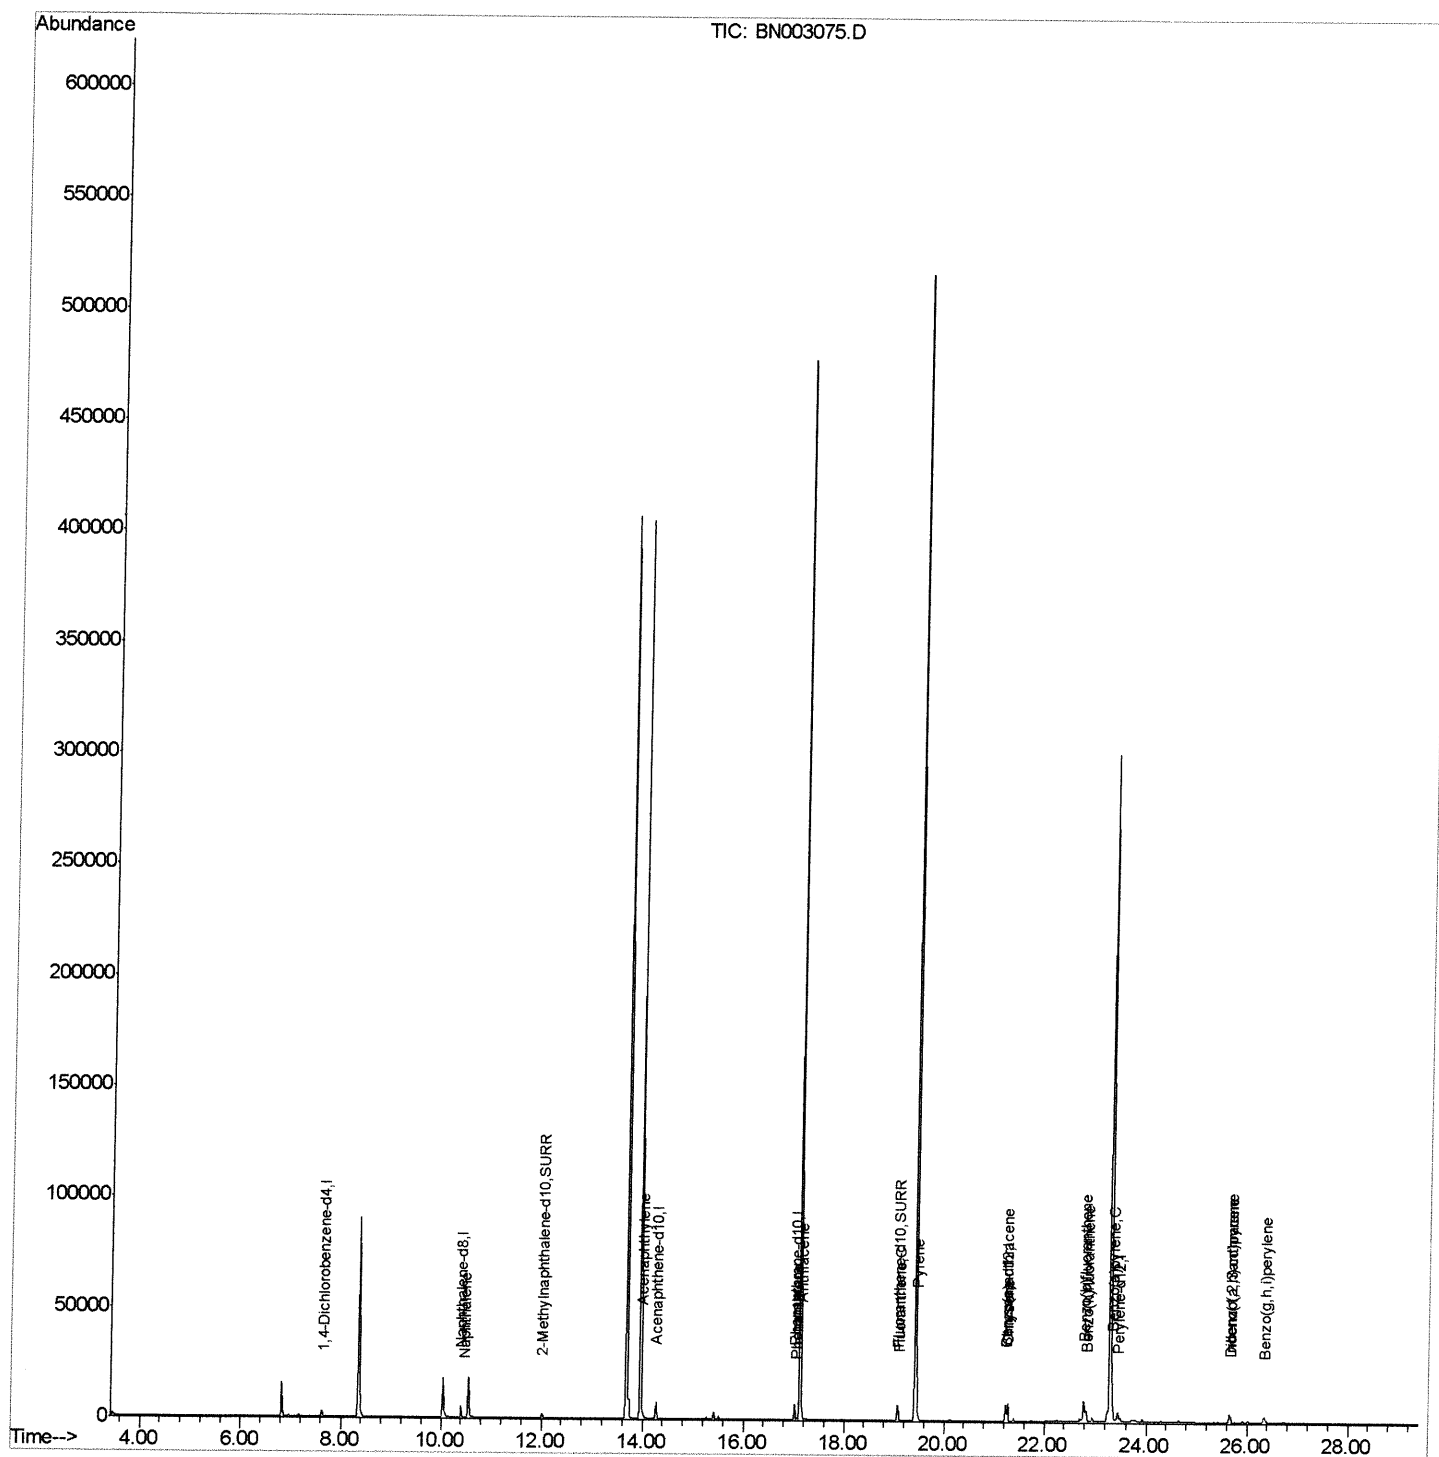

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101118\
 Data File : BN003075.D
 Acq On : 10 Oct 2018 21:41
 Operator : MJ/SJ
 Sample : J5157-19
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 C0AE1

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:45:41 PM

Quant Time: Oct 11 07:08:15 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 07:04:52 2018
 Response via : Initial Calibration

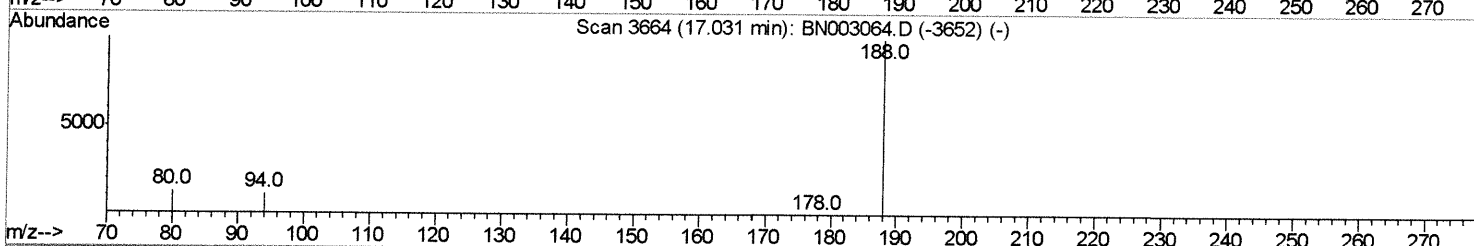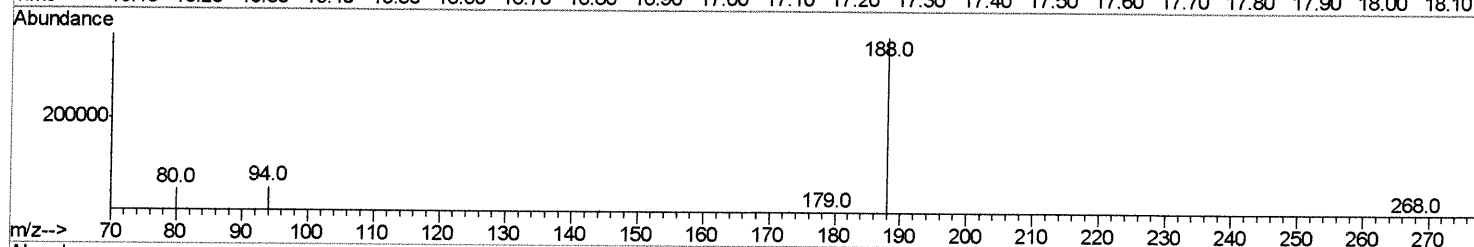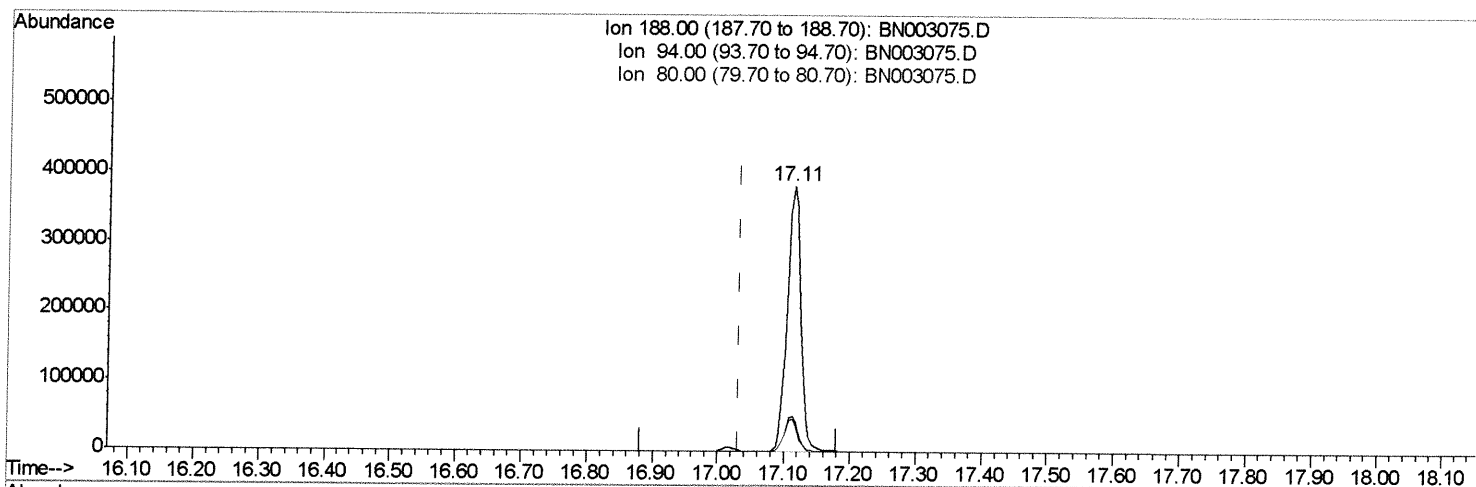

TIC: BN003075.D

(10) Phenanthrene-d10 (I)
 17.112min (+0.080) 0.40ng/ul
 response 563144

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	13.29
80.00	12.70	12.12
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101118\
 Data File : BN003075.D
 Acq On : 10 Oct 2018 21:41
 Operator : MJ/SJ
 Sample : J5157-19
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AE1

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:45:41 PM

Quant Time: Oct 11 07:08:15 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 07:04:52 2018
 Response via : Initial Calibration

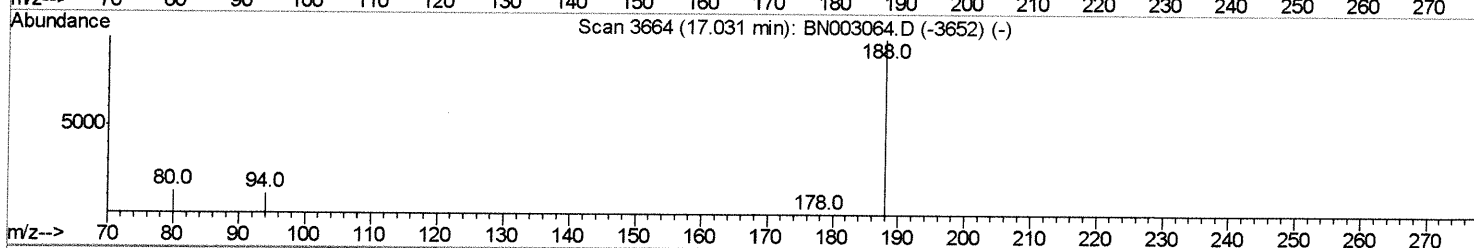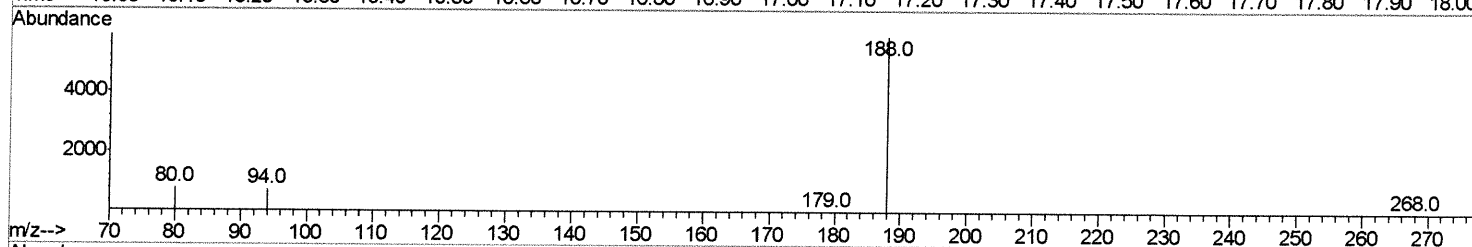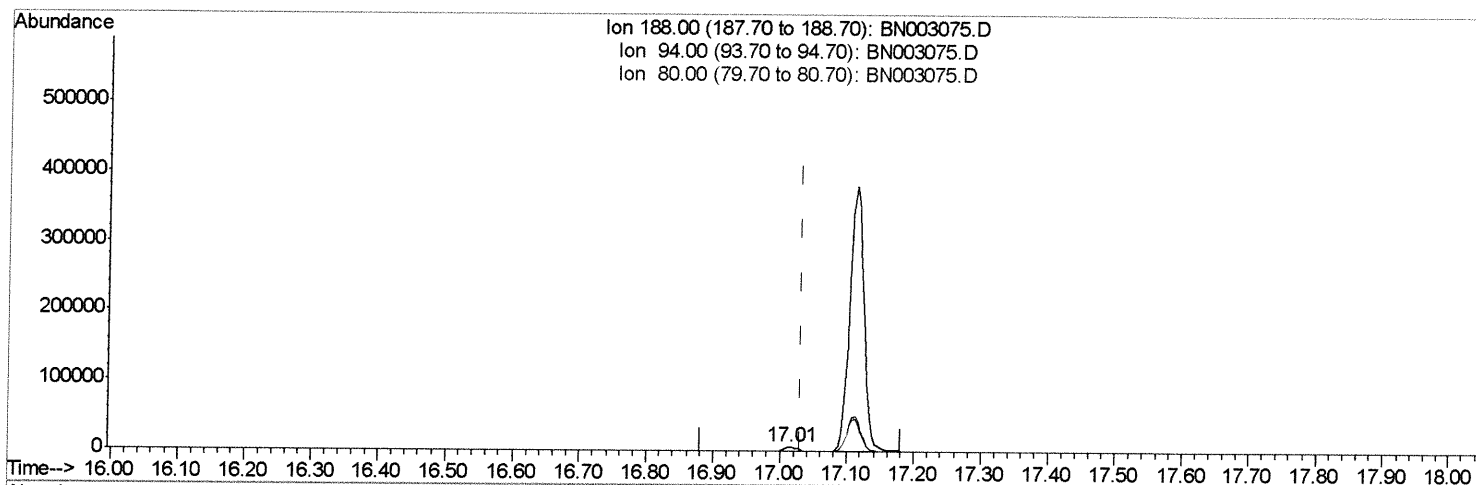

TIC: BN003075.D

(10) Phenanthrene-d10 (I)

17.014min (-0.017) 0.40ng/ul m

response 8389

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	12.46
80.00	12.70	13.47
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101118\
Data File : BN003075.D
Acq On : 10 Oct 2018 21:41
Operator : MJ/SJ
Sample : J5157-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE1

Manual Integrations
APPROVED

Sohil
10/11/2018 5:45:41 PM

Quant Time: Oct 11 07:57:57 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 07:04:52 2018
Response via : Initial Calibration

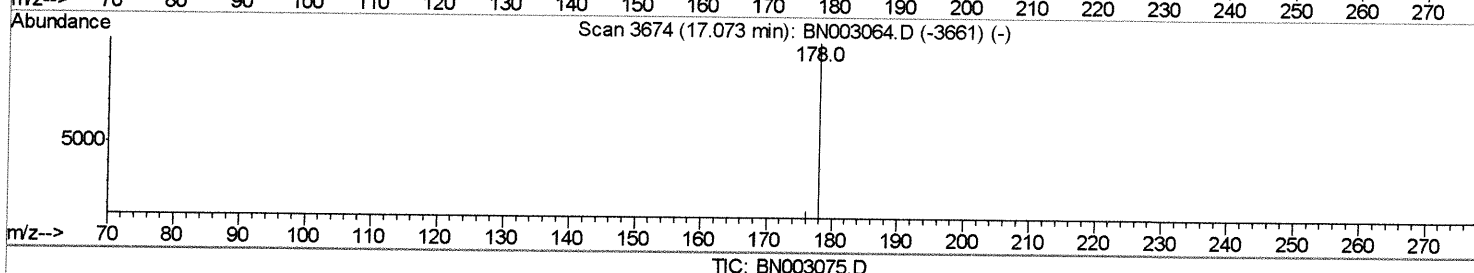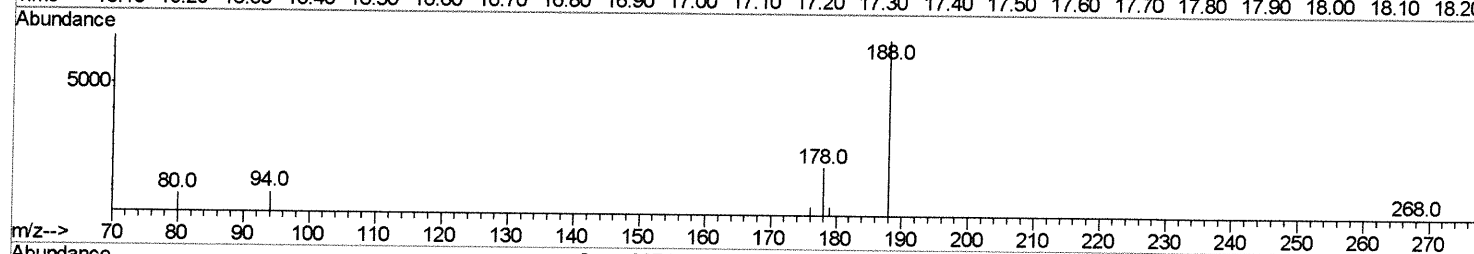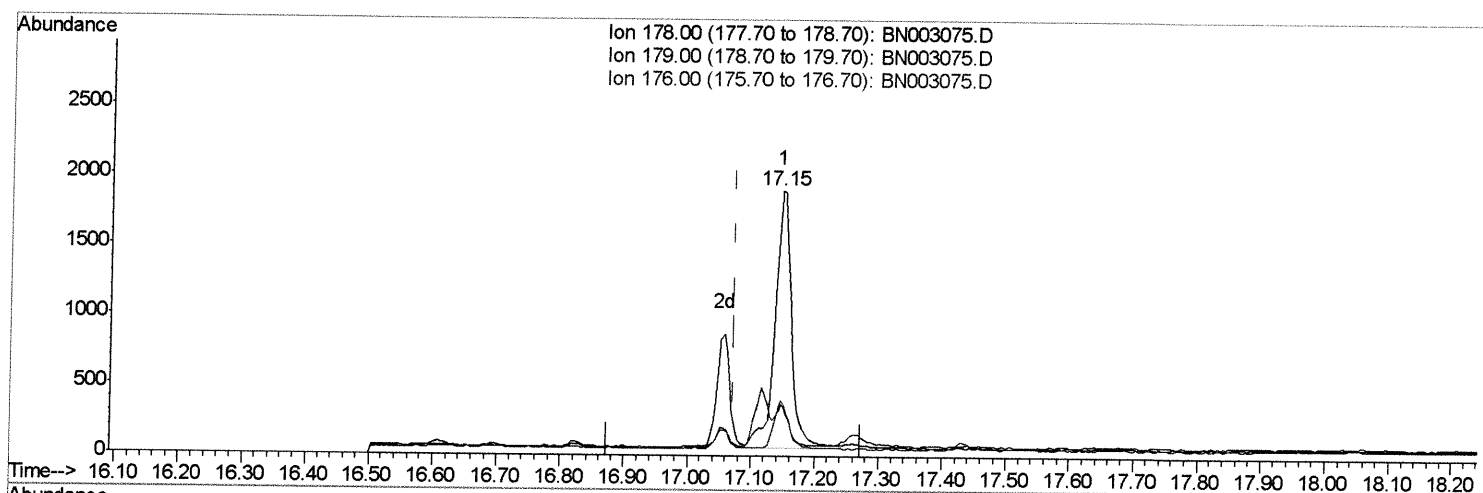

(12) Phenanthrene

17.145min (+0.072) 0.14ng/ul

response 3310

Ion	Exp%	Act%
178.00	100	100
179.00	16.10	19.48#
176.00	19.30	20.75
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101118\
Data File : BN003075.D
Acq On : 10 Oct 2018 21:41
Operator : MJ/SJ
Sample : J5157-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE1

Manual Integrations
APPROVED

Sohil
10/11/2018 5:45:41 PM

Quant Time: Oct 11 07:57:57 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 07:04:52 2018
Response via : Initial Calibration

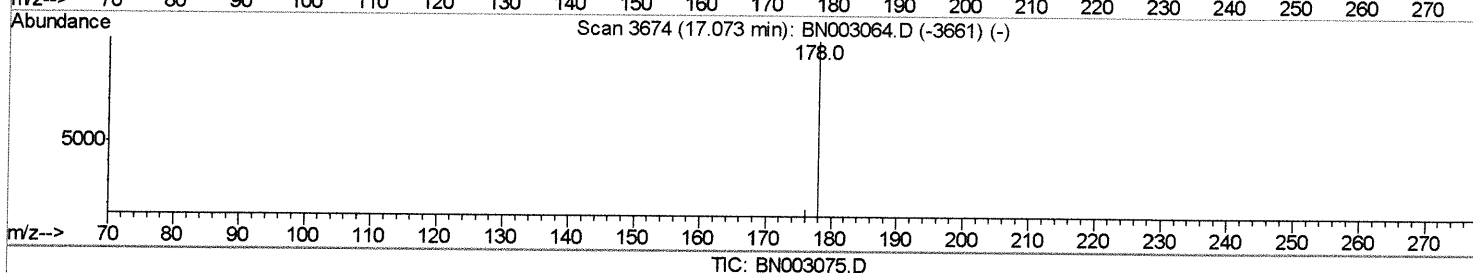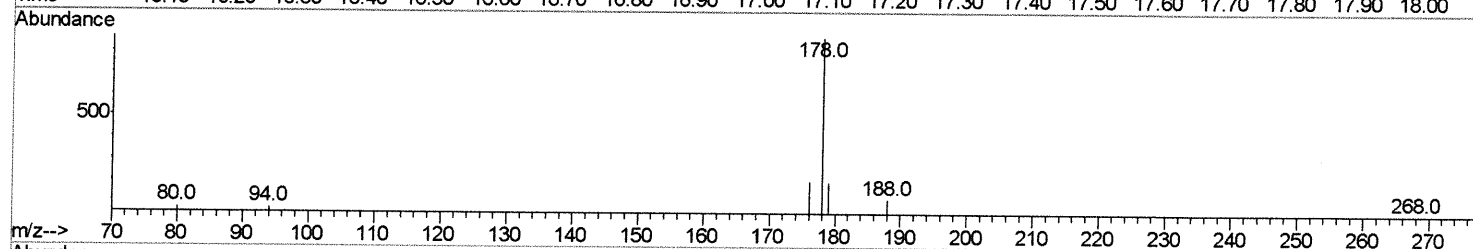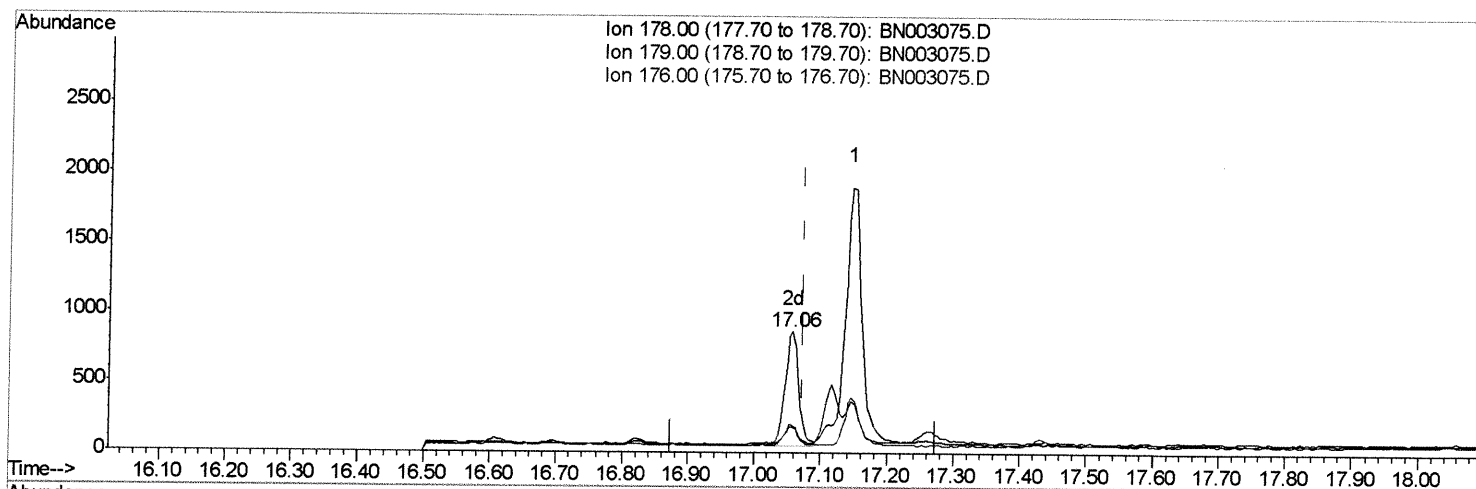

(12) Phenanthrene

17.057min (-0.017) 0.05ng/ul m

response 1173

Ion	Exp%	Act%
178.00	100	100
179.00	16.10	21.89#
176.00	19.30	23.04
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101118\
 Data File : BN003075.D
 Acq On : 10 Oct 2018 21:41
 Operator : MJ/SJ
 Sample : J5157-19
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AE1

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:45:41 PM

Quant Time: Oct 11 07:57:57 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 07:04:52 2018
 Response via : Initial Calibration

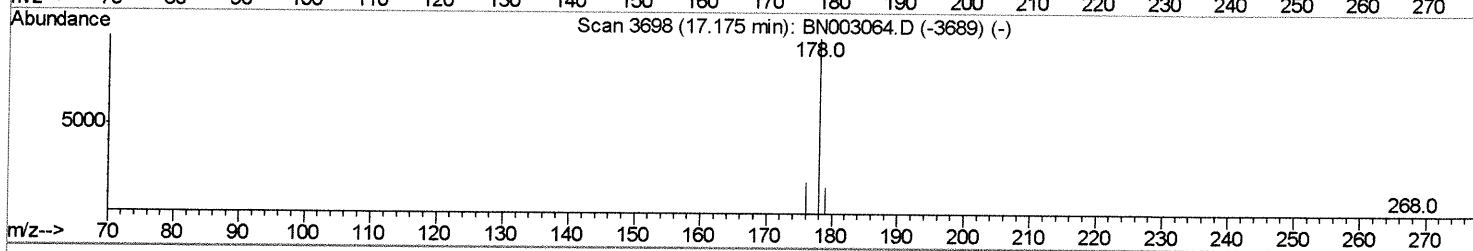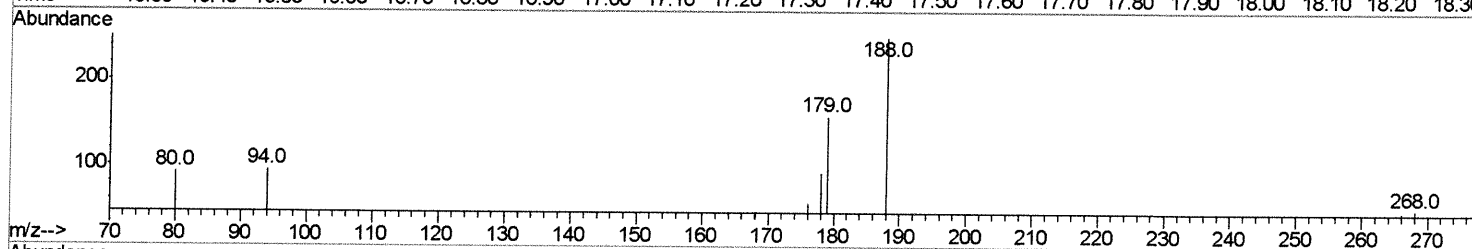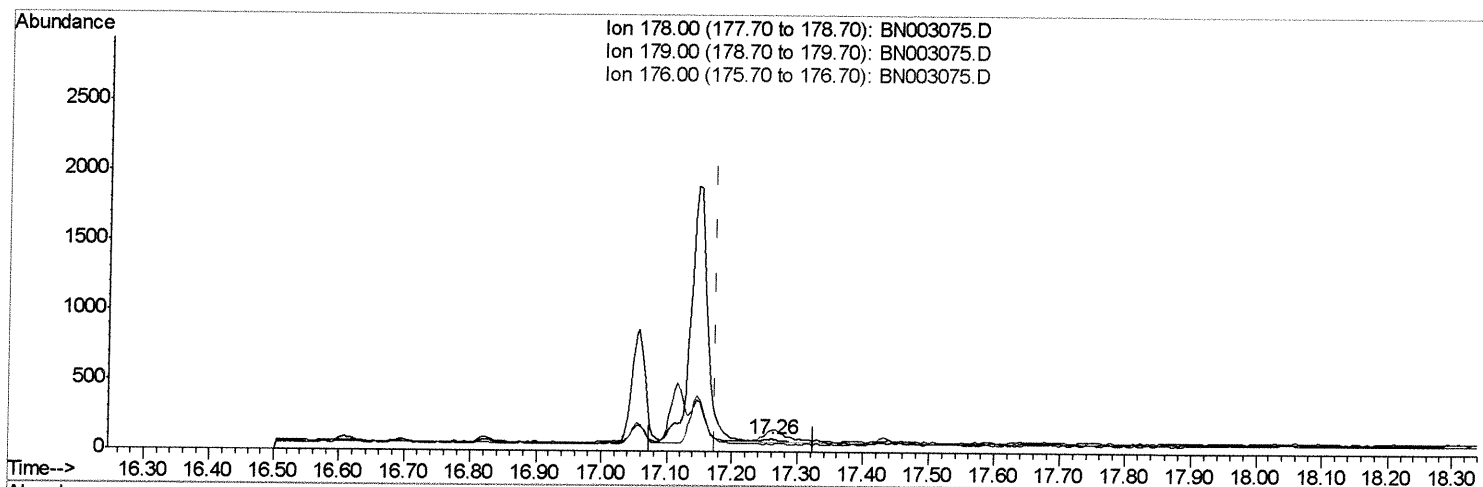

TIC: BN003075.D

(13) Anthracene

17.259min (+0.085) 0.00ng/ul

response 61

Ion	Exp%	Act%
178.00	100	100
179.00	16.30	173.63#
176.00	19.10	61.54#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101118\
 Data File : BN003075.D
 Acq On : 10 Oct 2018 21:41
 Operator : MJ/SJ
 Sample : J5157-19
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AE1

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:45:41 PM

Quant Time: Oct 11 07:57:57 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 07:04:52 2018
 Response via : Initial Calibration

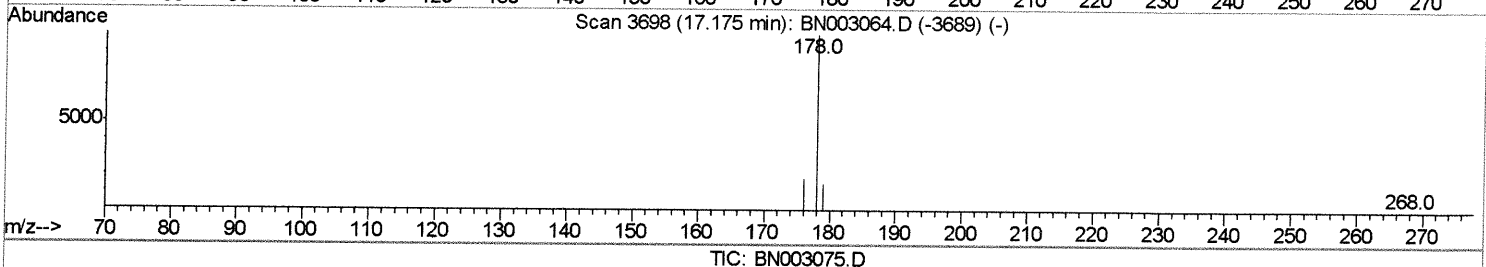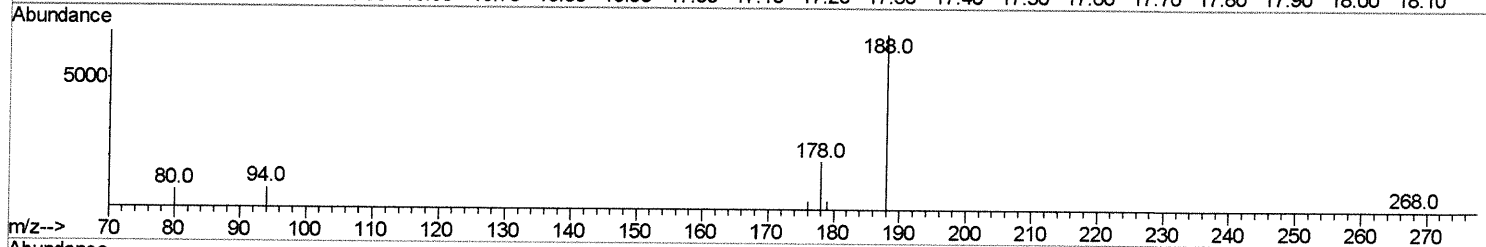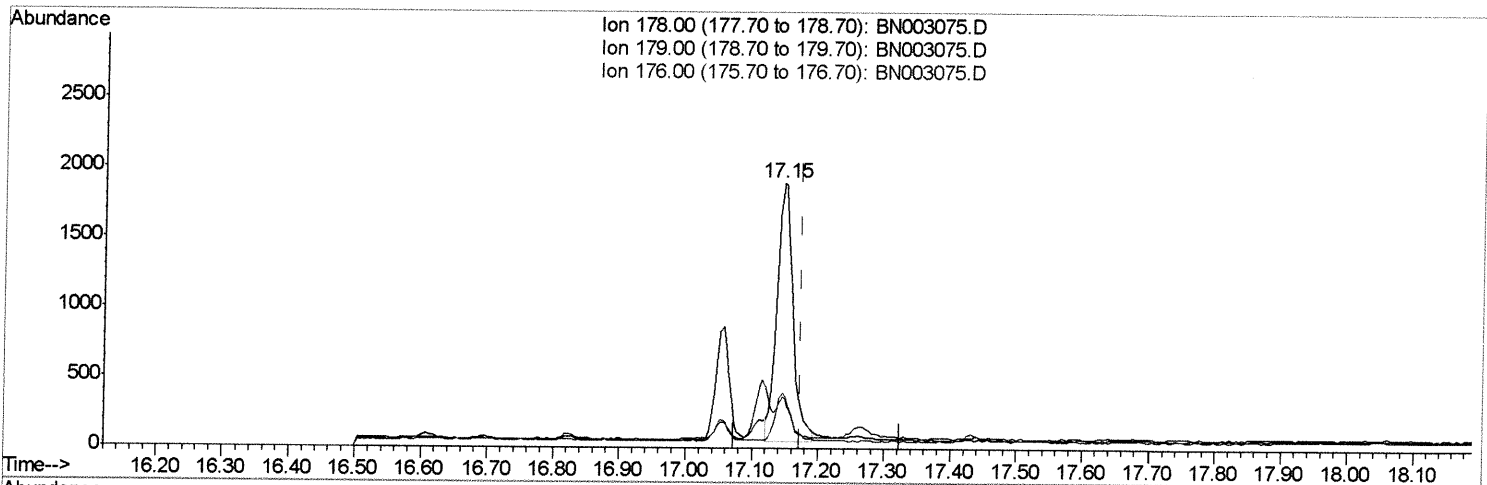

TIC: BN003075.D

(13) Anthracene

17.145min (-0.029) 0.14ng/ul m

response 3086

Ion	Exp%	Act%
178.00	100	100
179.00	16.30	19.48
176.00	19.10	20.75
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101118\
Data File : BN003075.D
Acq On : 10 Oct 2018 21:41
Operator : MJ/SJ
Sample : J5157-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE1

Manual Integrations
APPROVED

Sohil
10/11/2018 5:45:41 PM

Quant Time: Oct 11 07:57:57 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 07:04:52 2018
Response via : Initial Calibration

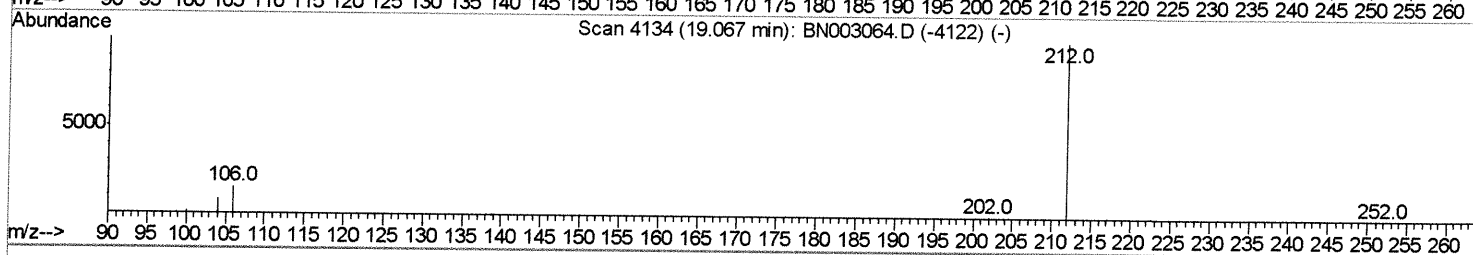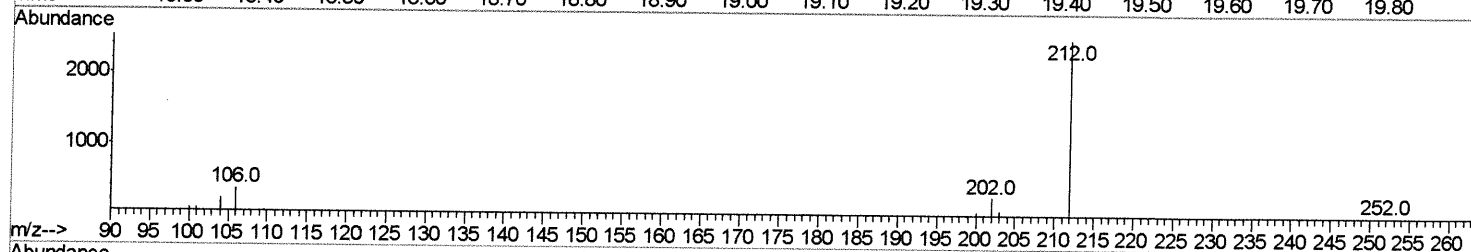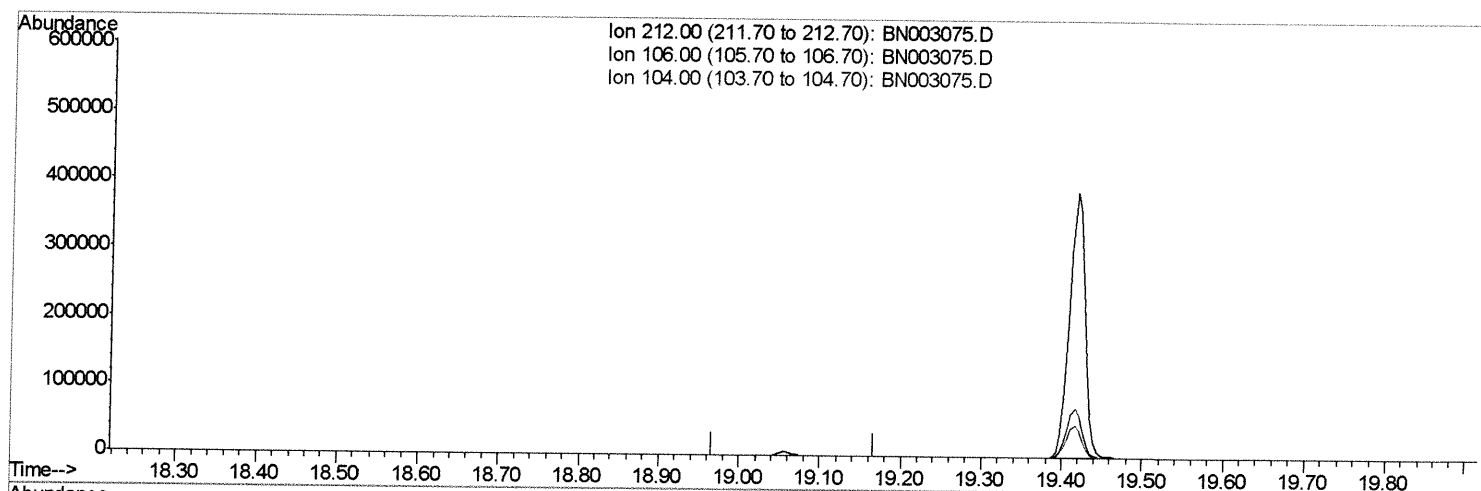

TIC: BN003075.D

(14) Fluoranthene-d10 (SURR)

19.067min (-19.067) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	15.40	0.00#
104.00	8.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101118\
Data File : BN003075.D
Acq On : 10 Oct 2018 21:41
Operator : MJ/SJ
Sample : J5157-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE1

Manual Integrations
APPROVED

Sohil
10/11/2018 5:45:41 PM

Quant Time: Oct 11 07:57:57 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 07:04:52 2018
Response via : Initial Calibration

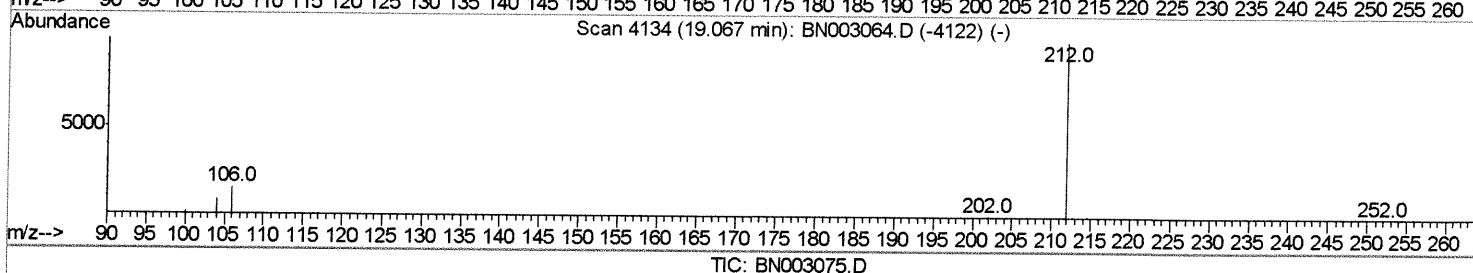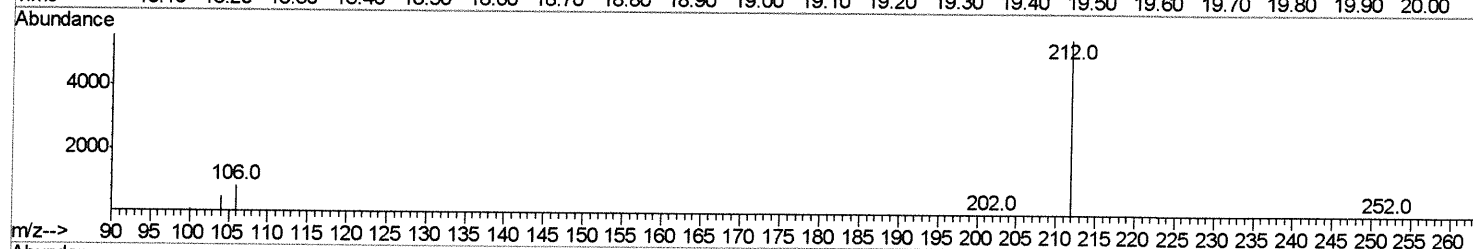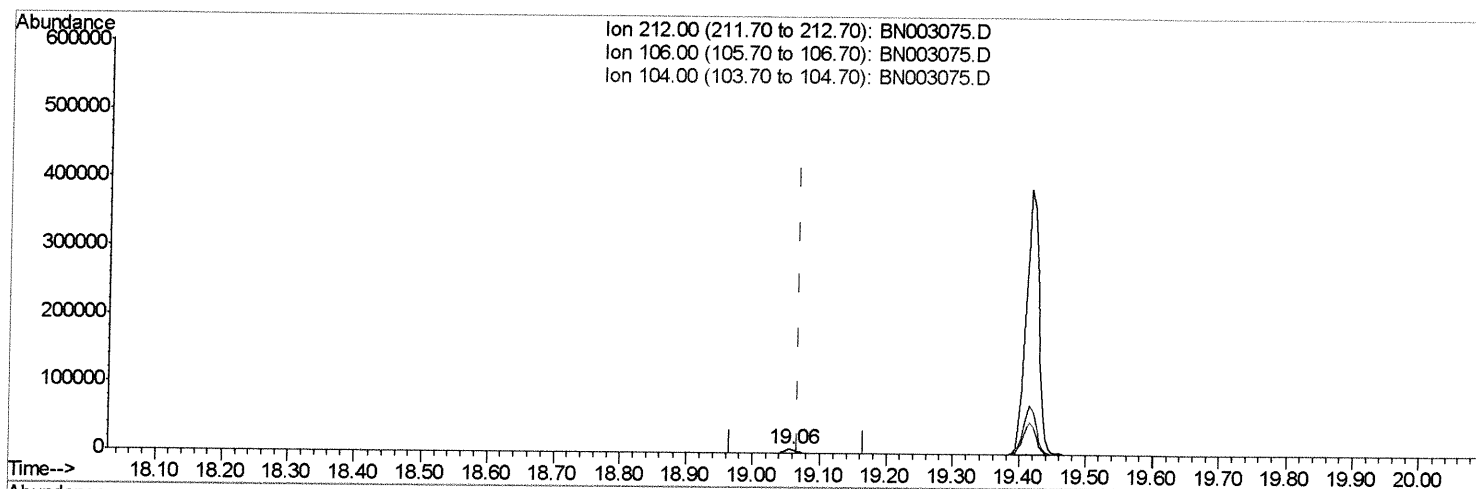

(14) Fluoranthene-d10 (SURR)

19.058min (-0.009) 0.31ng/ul m

response 7552

Ion	Exp%	Act%
212.00	100	100
106.00	15.40	0.00#
104.00	8.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101118\
Data File : BN003075.D
Acq On : 10 Oct 2018 21:41
Operator : MJ/SJ
Sample : J5157-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE1

Manual Integrations
APPROVED

Sohil
10/11/2018 5:45:41 PM

Quant Time: Oct 11 07:57:57 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 07:04:52 2018
Response via : Initial Calibration

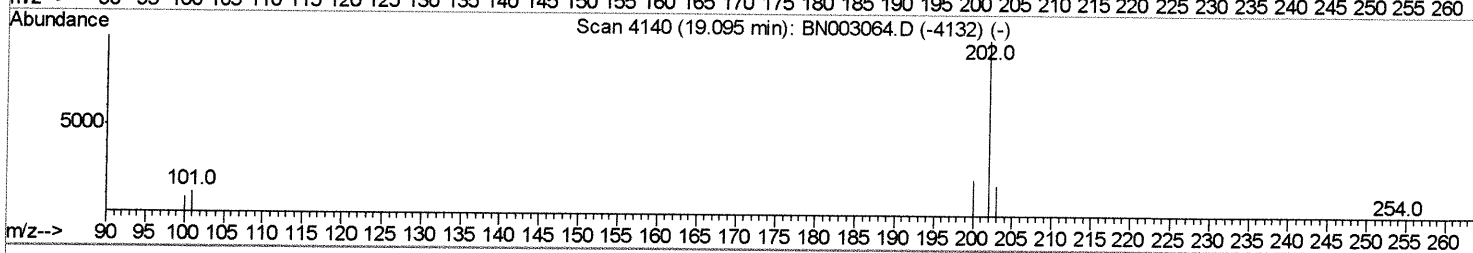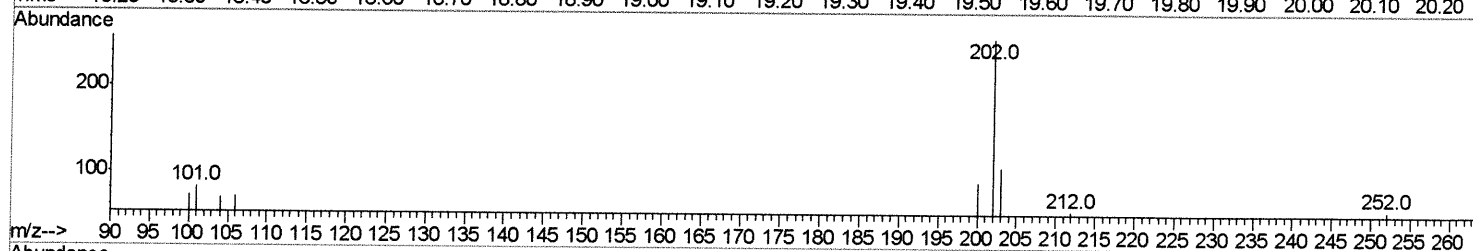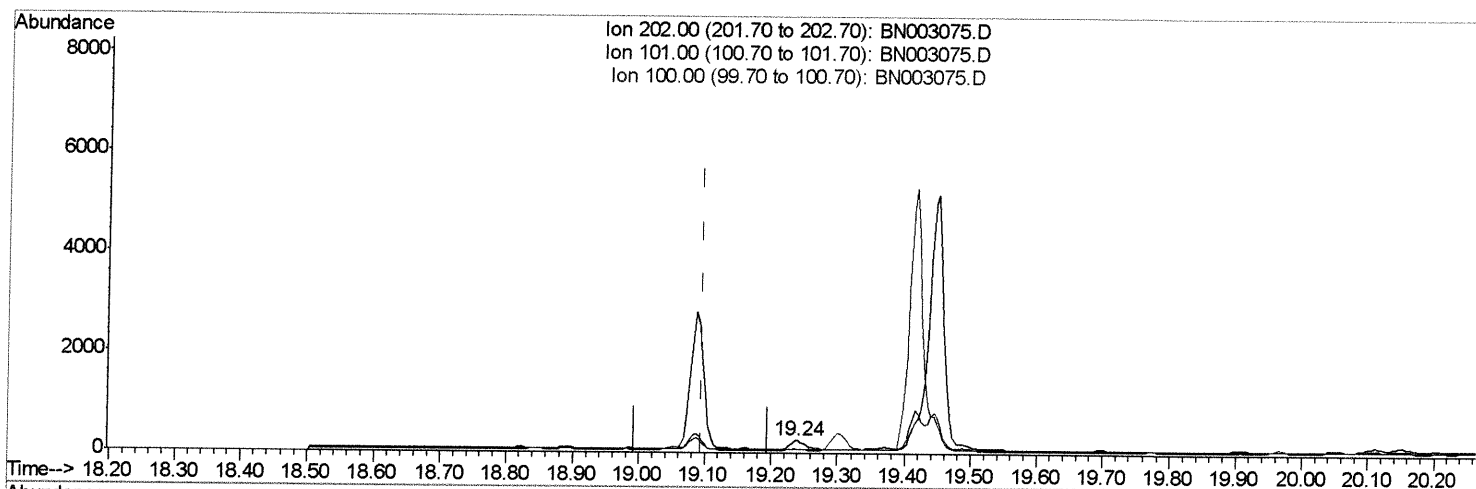

TIC: BN003075.D

(15) Fluoranthene (C)

19.239min (+0.144) 0.01ng/ul

response 286

Ion	Exp%	Act%
202.00	100	100
101.00	12.30	31.40
100.00	9.10	27.91
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101118\
 Data File : BN003075.D
 Acq On : 10 Oct 2018 21:41
 Operator : MJ/SJ
 Sample : J5157-19
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AE1

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:45:41 PM

Quant Time: Oct 11 07:57:57 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 07:04:52 2018
 Response via : Initial Calibration

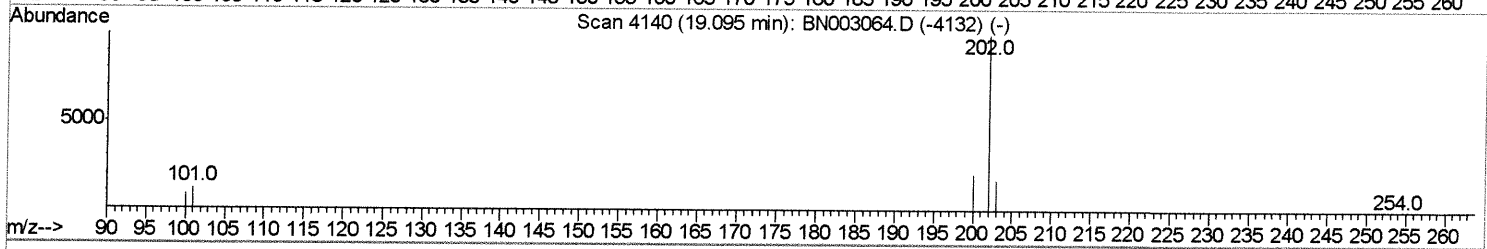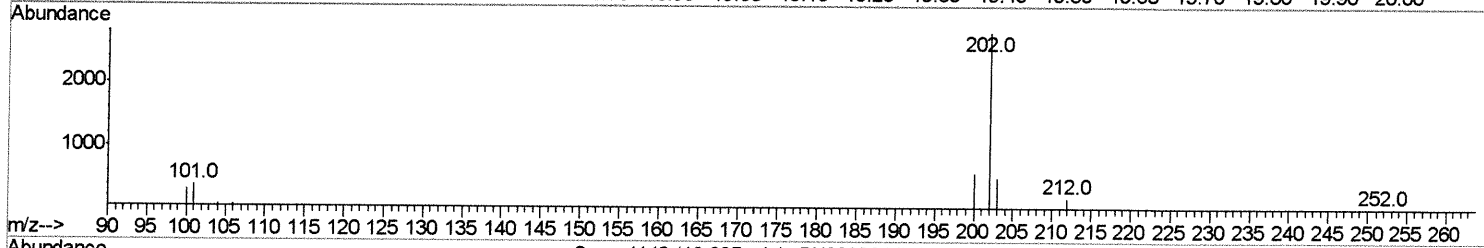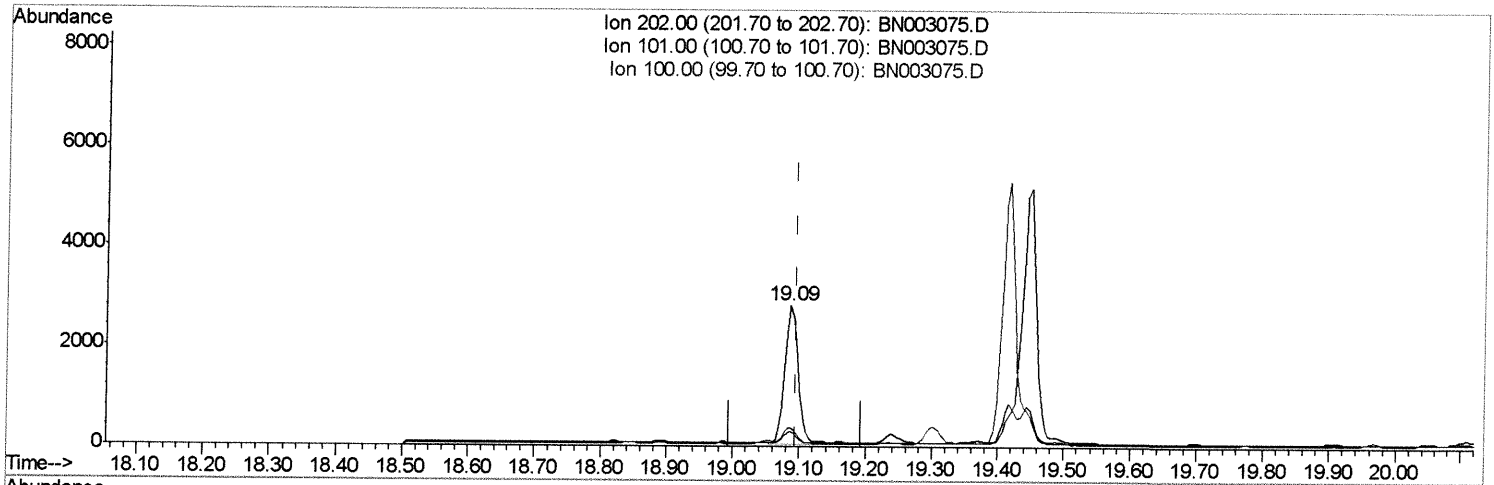

TIC: BN003075.D

(15) Fluoranthene (C)

19.086min (-0.009) 0.14ng/ul m

response 3880

Ion	Exp%	Act%
202.00	100	100
101.00	12.30	13.74
100.00	9.10	11.07
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101118\
 Data File : BN003075.D
 Acq On : 10 Oct 2018 21:41
 Operator : MJ/SJ
 Sample : J5157-19
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AE1

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:45:41 PM

Quant Time: Oct 11 07:57:57 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 07:04:52 2018
 Response via : Initial Calibration

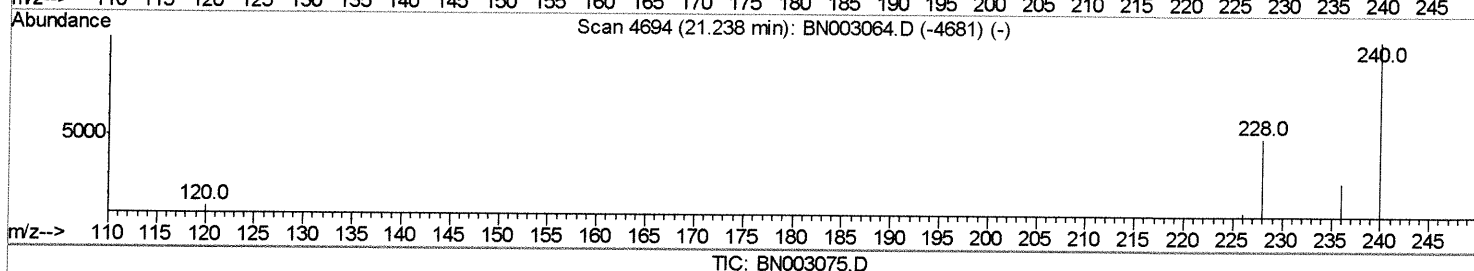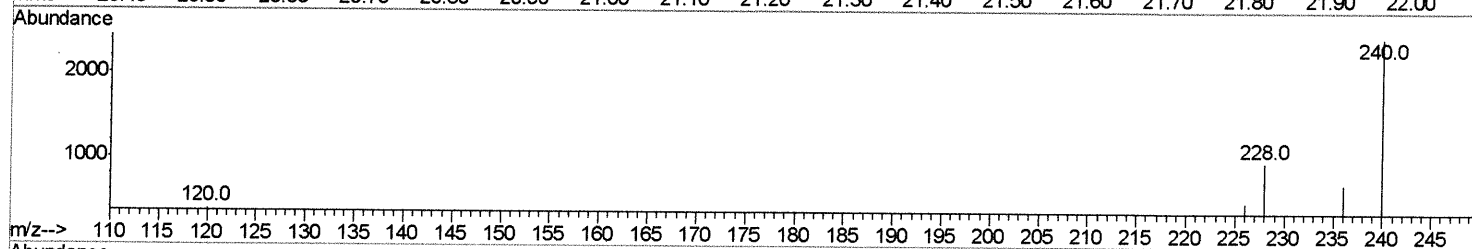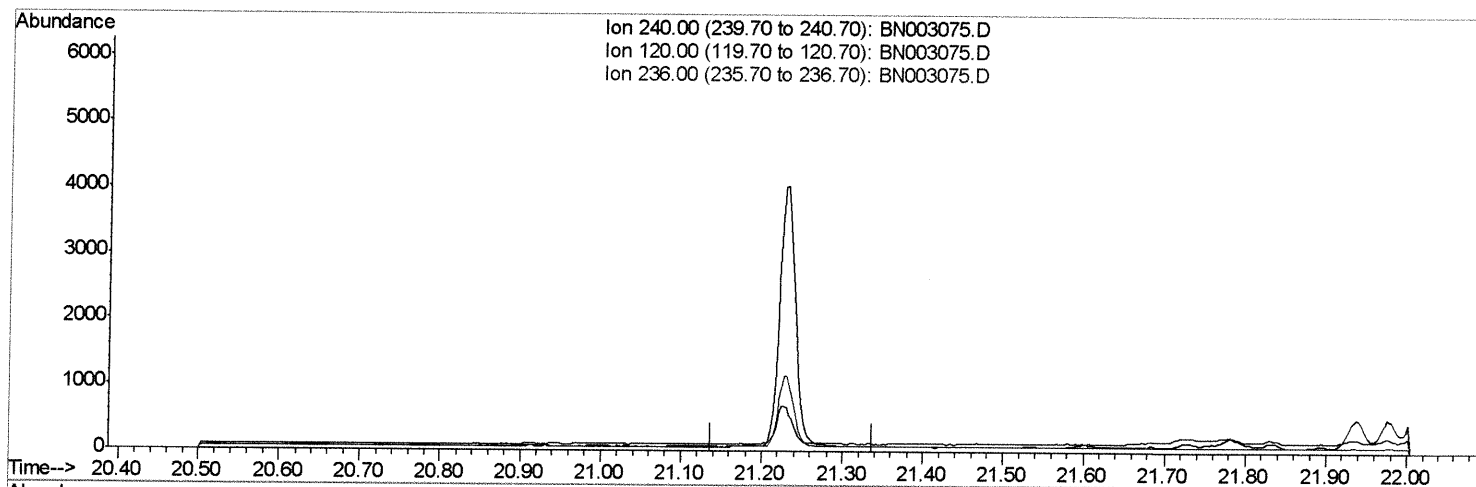

(16) Chrysene-d12 (I)

21.238min (-21.238) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	16.40	0.00#
236.00	28.10	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101118\
 Data File : BN003075.D
 Acq On : 10 Oct 2018 21:41
 Operator : MJ/SJ
 Sample : J5157-19
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AE1

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:45:41 PM

Quant Time: Oct 11 07:57:57 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 07:04:52 2018
 Response via : Initial Calibration

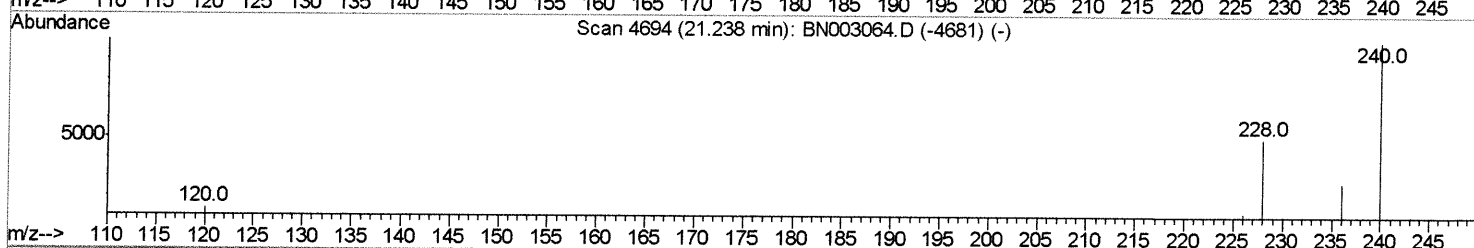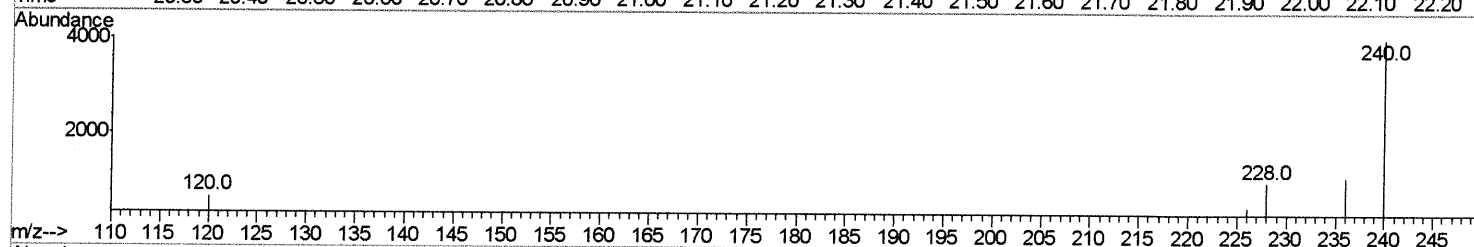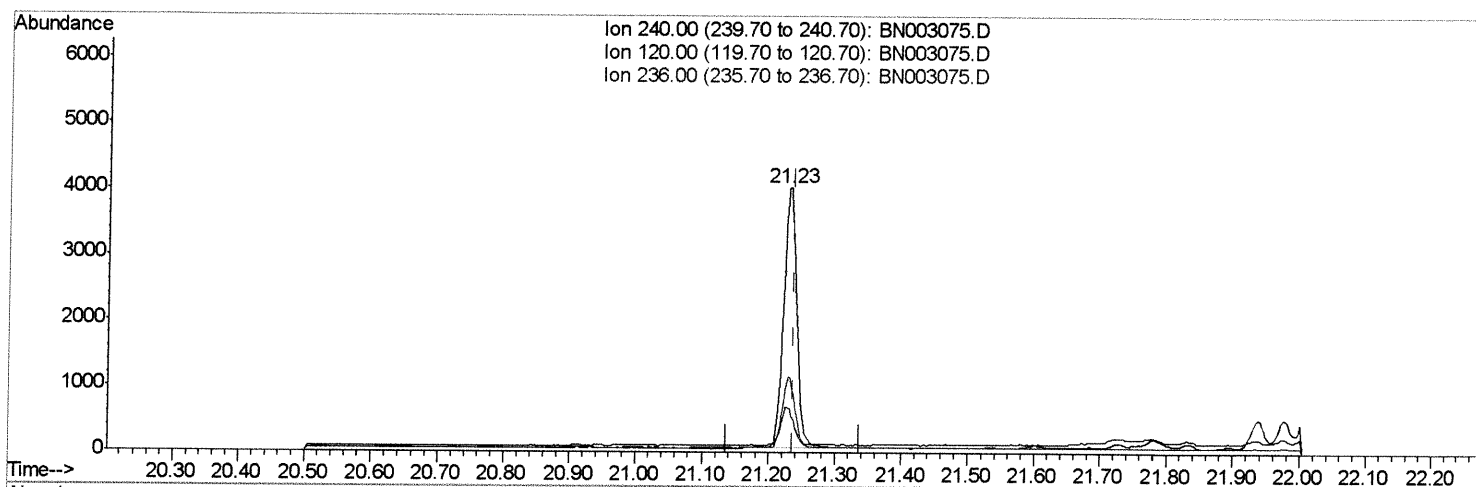

TIC: BN003075.D

(16) Chrysene-d12 (I)

21.230min (-0.007) 0.40ng/ul m

response 5461

Ion	Exp%	Act%
240.00	100	100
120.00	16.40	16.53
236.00	28.10	27.97
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101118\
Data File : BN003075.D
Acq On : 10 Oct 2018 21:41
Operator : MJ/SJ
Sample : J5157-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE1

Manual Integrations
APPROVED

Sohil
10/11/2018 5:45:41 PM

Quant Time: Oct 11 07:59:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 07:04:52 2018
Response via : Initial Calibration

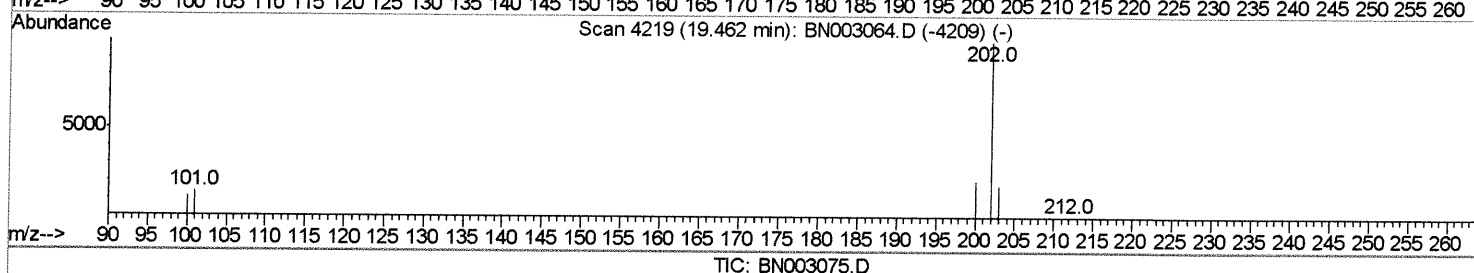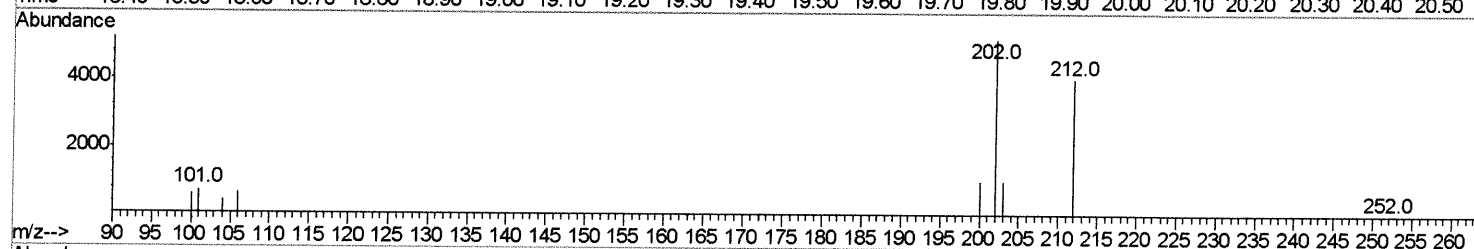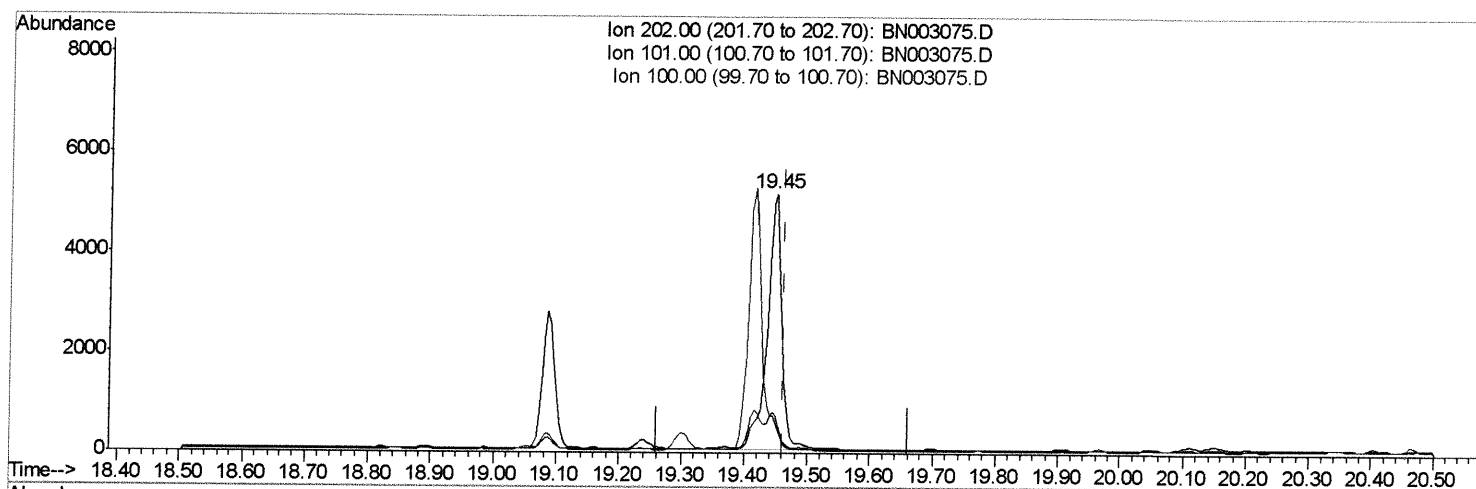

(17) Pyrene

19.448min (-0.014) 0.40ng/ul

response 8404

Ion	Exp%	Act%
202.00	100	100
101.00	14.90	14.22
100.00	12.40	11.69
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101118\
 Data File : BN003075.D
 Acq On : 10 Oct 2018 21:41
 Operator : MJ/SJ
 Sample : J5157-19
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 C0AE1

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:45:41 PM

Quant Time: Oct 11 07:59:10 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 07:04:52 2018
 Response via : Initial Calibration

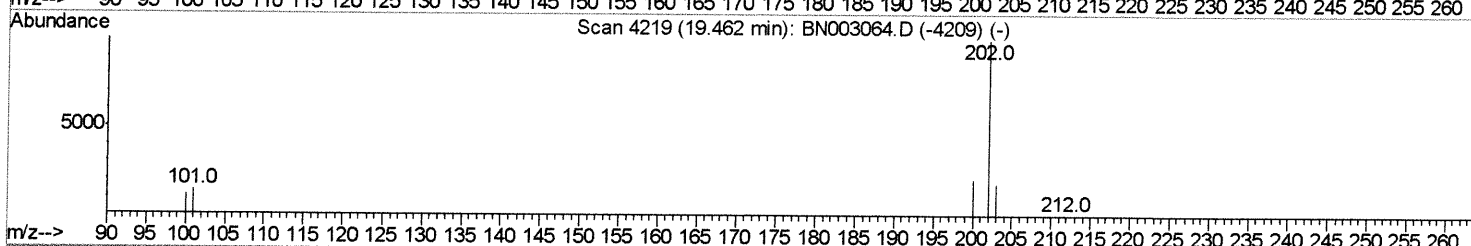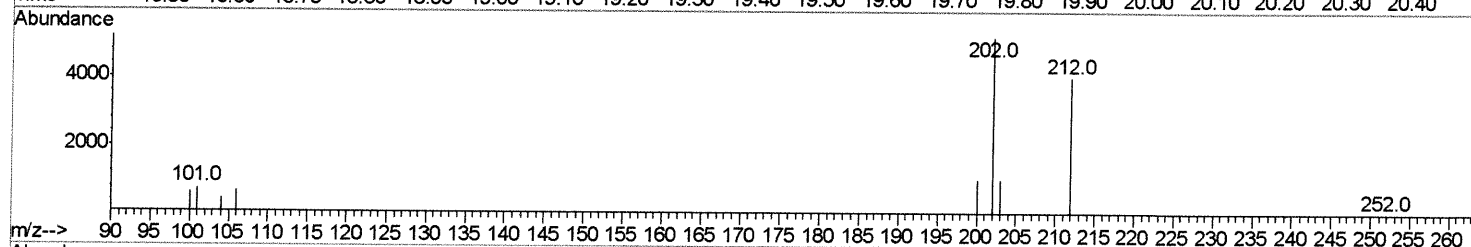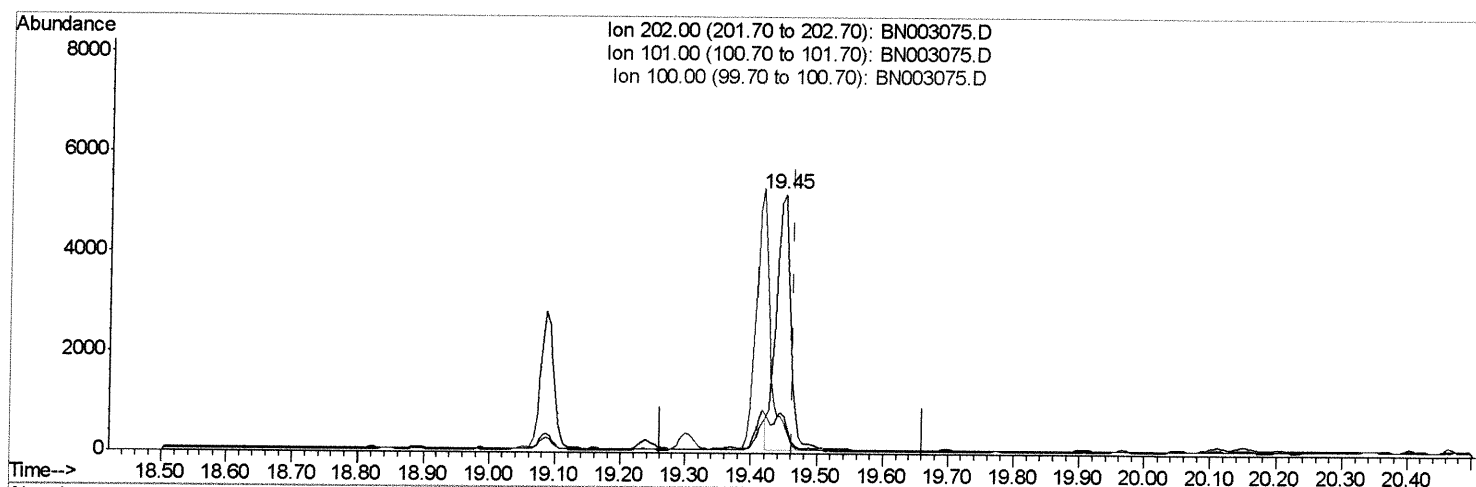

TIC: BN003075.D

(17) Pyrene

19.448min (-0.014) 0.37ng/ul m

response 7777

Ion	Exp%	Act%
202.00	100	100
101.00	14.90	14.22
100.00	12.40	11.69
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101118\
Data File : BN003075.D
Acq On : 10 Oct 2018 21:41
Operator : MJ/SJ
Sample : J5157-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE1

Manual Integrations
APPROVED

Sohil
10/11/2018 5:45:41 PM

Quant Time: Oct 11 07:59:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 07:04:52 2018
Response via : Initial Calibration

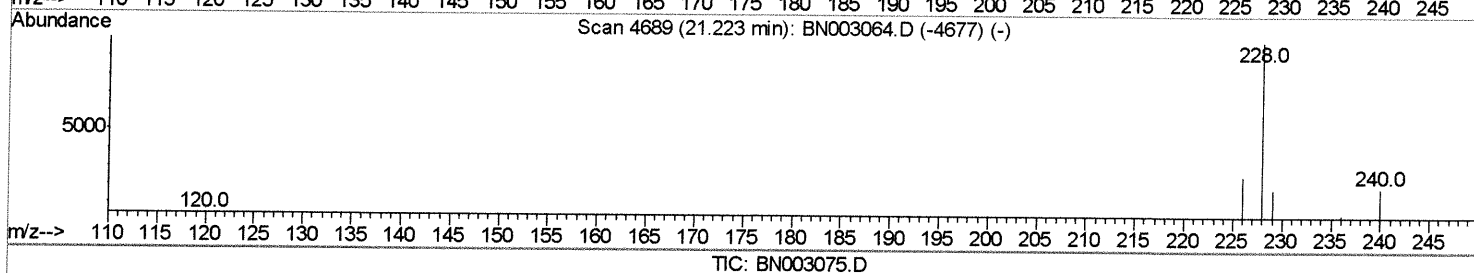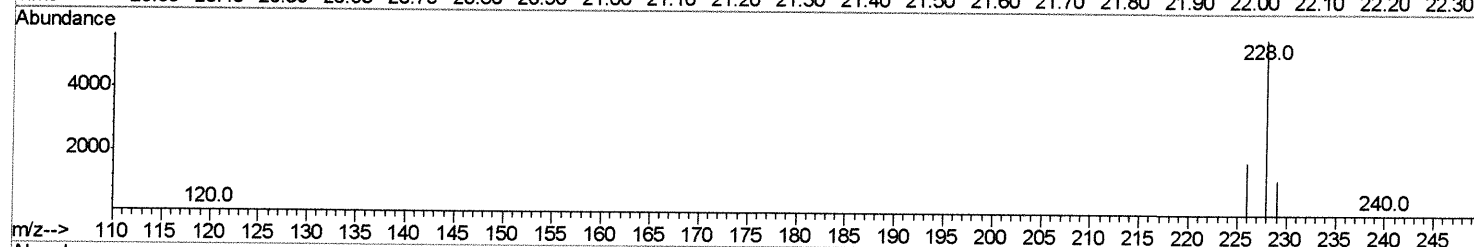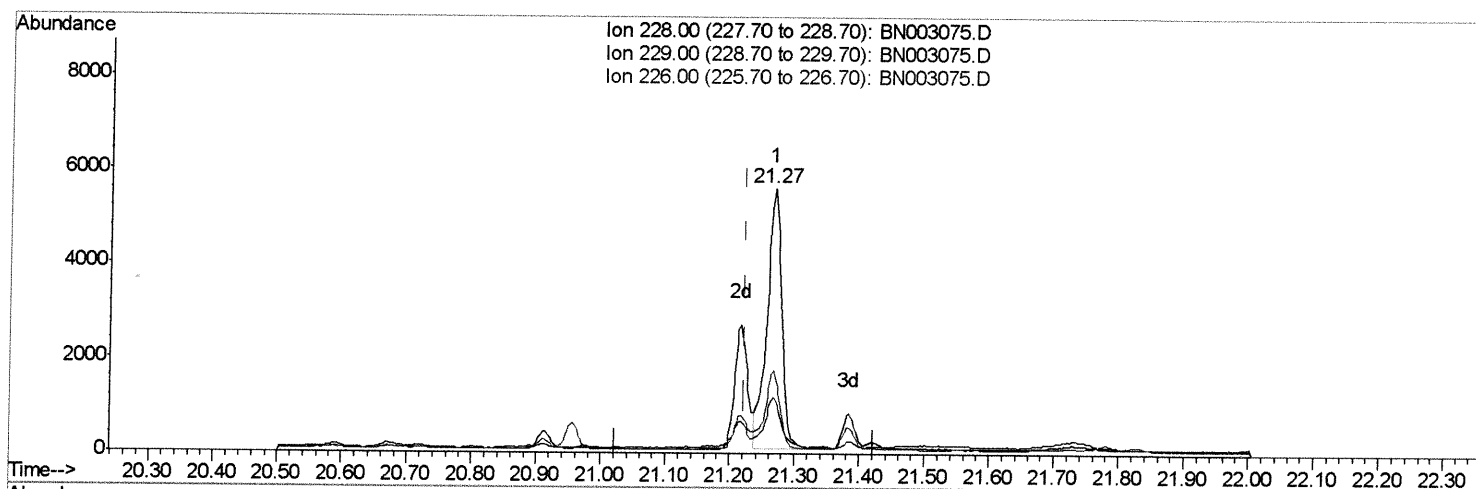

(18) Benzo(a)anthracene

21.265min (+0.042) 0.50ng/ul

response 8721

Ion	Exp%	Act%
228.00	100	100
229.00	20.20	21.39
226.00	27.90	31.16
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101118\
Data File : BN003075.D
Acq On : 10 Oct 2018 21:41
Operator : MJ/SJ
Sample : J5157-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE1

Manual Integrations
APPROVED

Sohil
10/11/2018 5:45:41 PM

Quant Time: Oct 11 07:59:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 07:04:52 2018
Response via : Initial Calibration

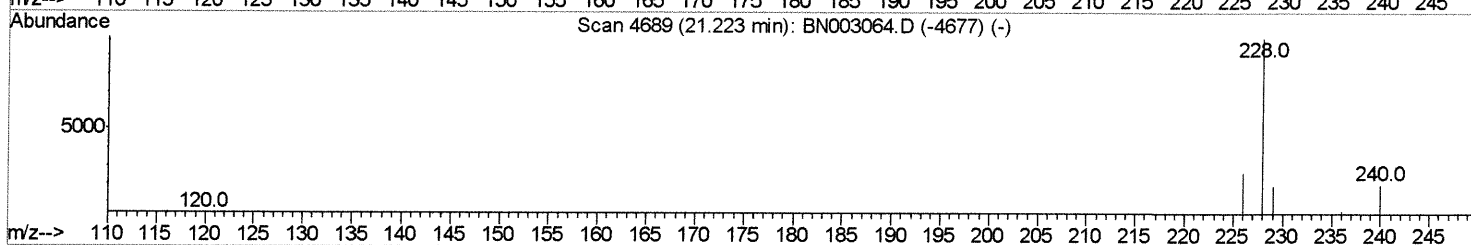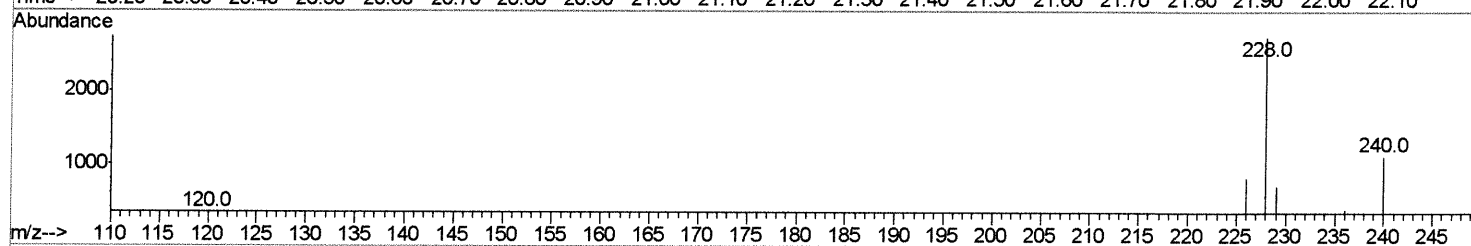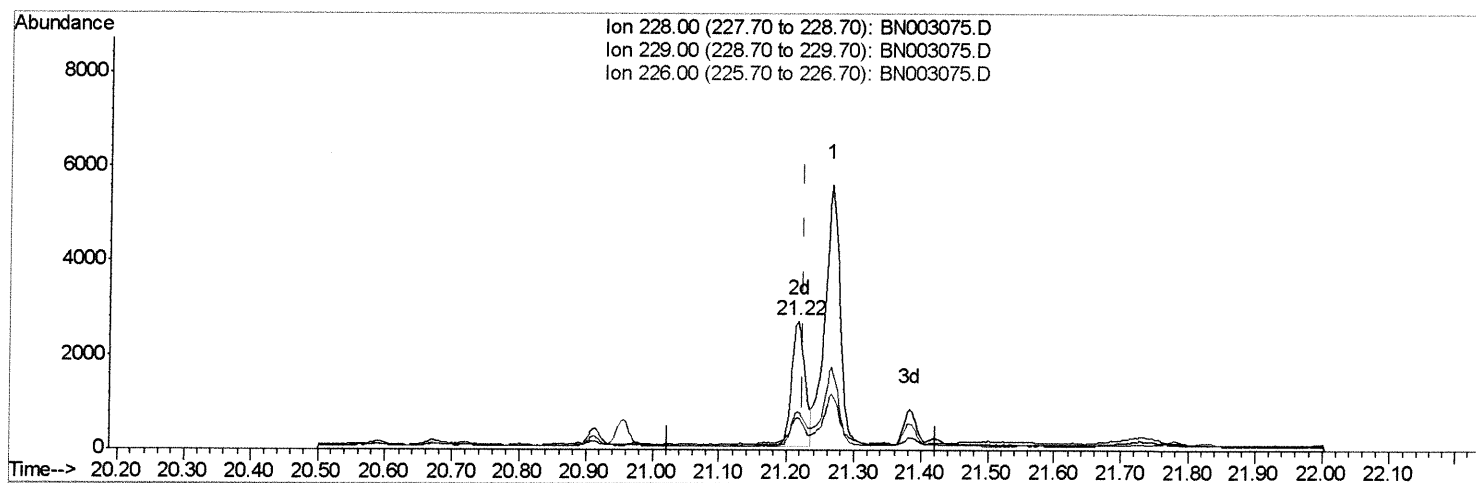

TIC: BN003075.D

(18) Benzo(a)anthracene

21.216min (-0.007) 0.22ng/ul m

response 3779

Ion	Exp%	Act%
228.00	100	100
229.00	20.20	25.67#
226.00	27.90	29.76
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101118\
 Data File : BN003075.D
 Acq On : 10 Oct 2018 21:41
 Operator : MJ/SJ
 Sample : J5157-19
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AE1

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:45:41 PM

Quant Time: Oct 11 07:59:10 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 07:04:52 2018
 Response via : Initial Calibration

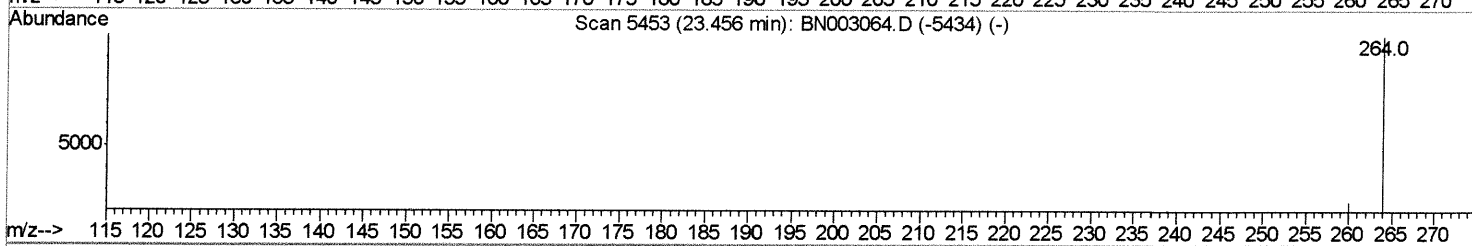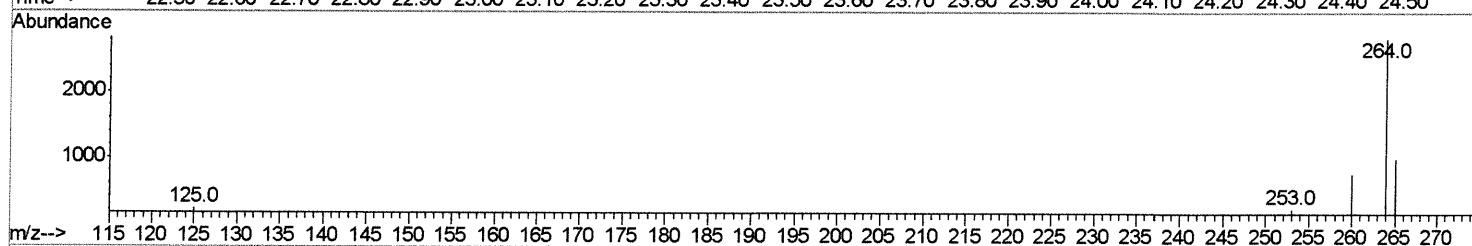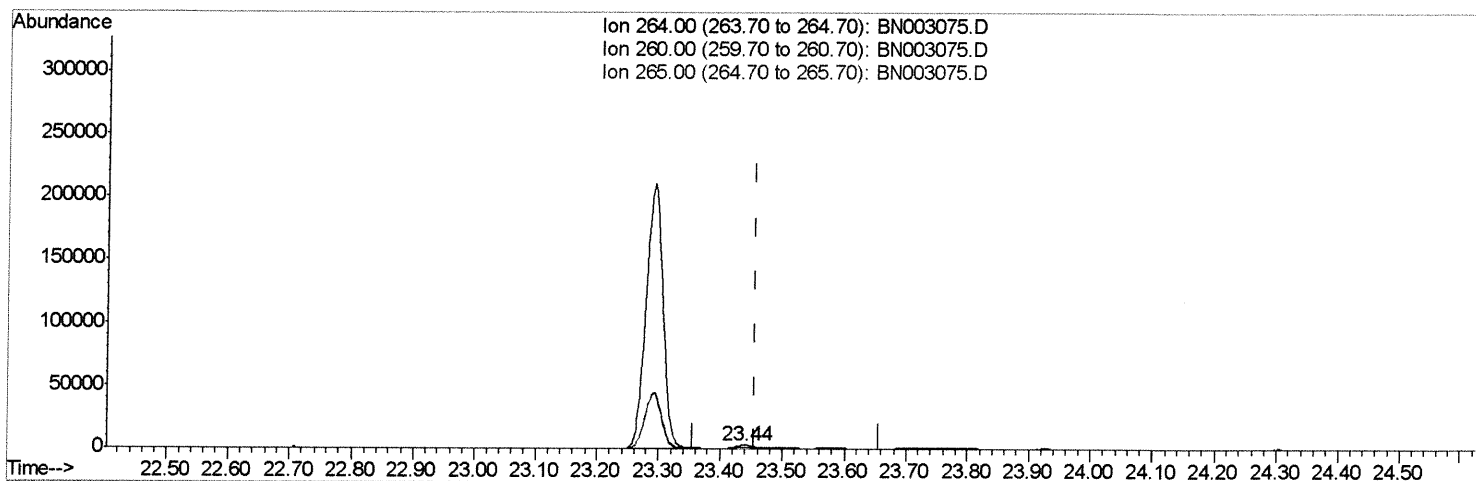

TIC: BN003075.D

(20) Perylene-d12 (I)

23.440min (-0.016) 0.40ng/ul

response 6058

Ion	Exp%	Act%
264.00	100	100
260.00	28.70	26.46
265.00	45.40	35.10#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101118\
 Data File : BN003075.D
 Acq On : 10 Oct 2018 21:41
 Operator : MJ/SJ
 Sample : J5157-19
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AE1

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:45:41 PM

Quant Time: Oct 11 07:59:10 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 07:04:52 2018
 Response via : Initial Calibration

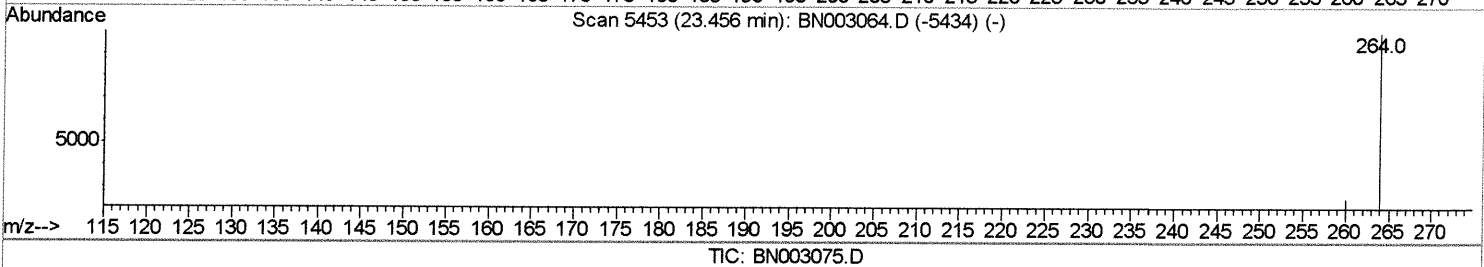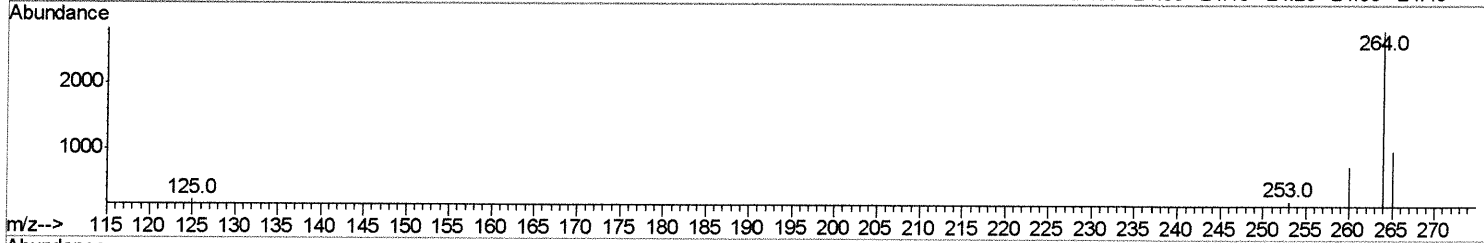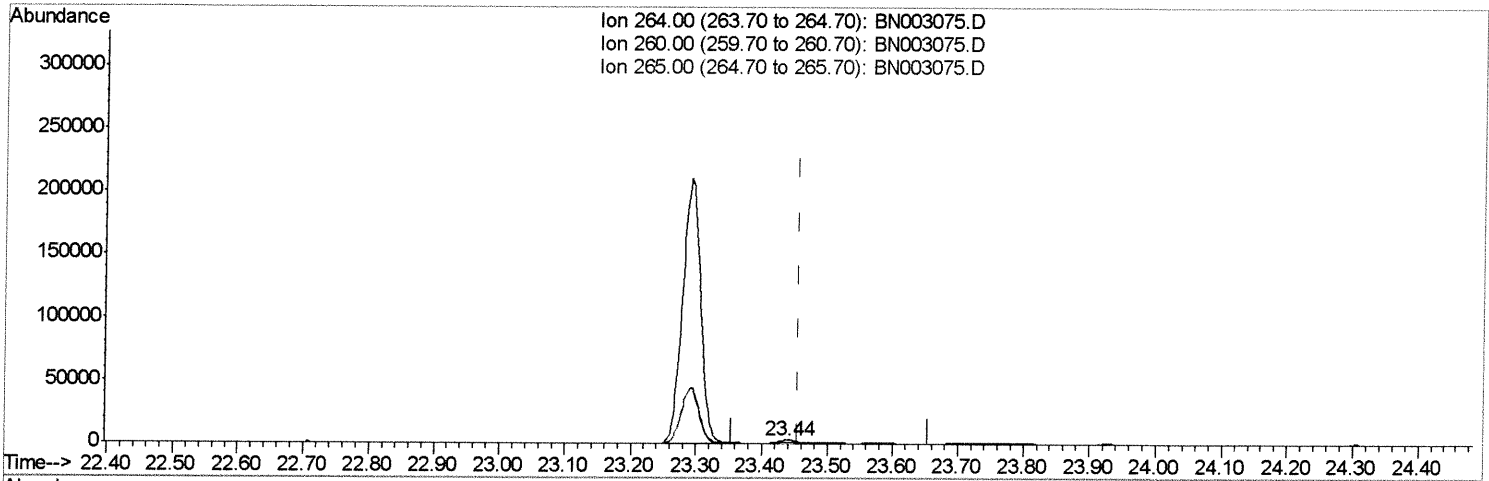

TIC: BN003075.D

(20) Perylene-d12 (I)

23.440min (-0.016) 0.40ng/ul m

Handwritten signature and date: 10/12/18

response 4973

Ion	Exp%	Act%
264.00	100	100
260.00	28.70	26.46
265.00	45.40	35.10#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101118\
Data File : BN003075.D
Acq On : 10 Oct 2018 21:41
Operator : MJ/SJ
Sample : J5157-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE1

Manual Integrations
APPROVED

Sohil
10/11/2018 5:45:41 PM

Quant Time: Oct 11 08:00:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 07:04:52 2018
Response via : Initial Calibration

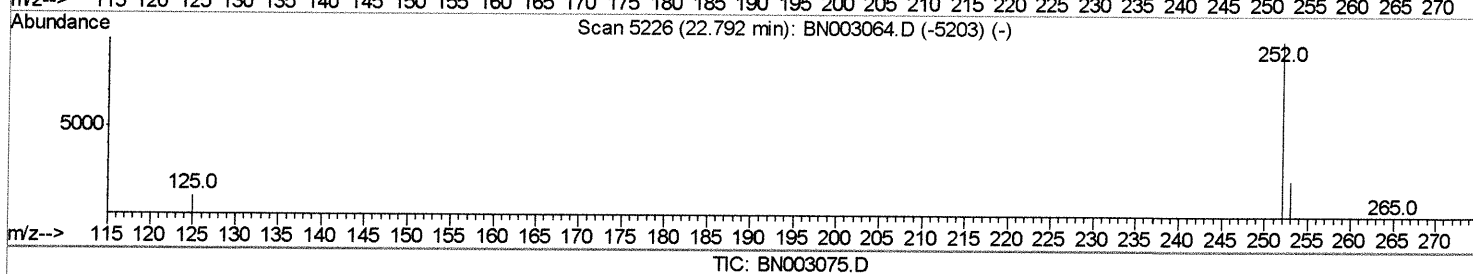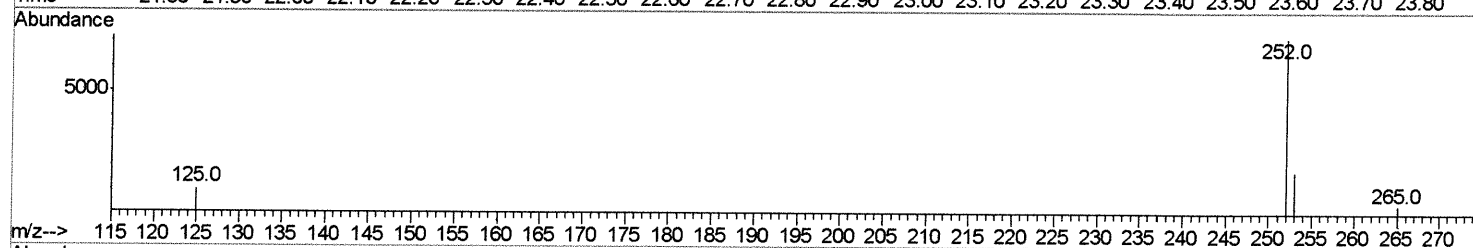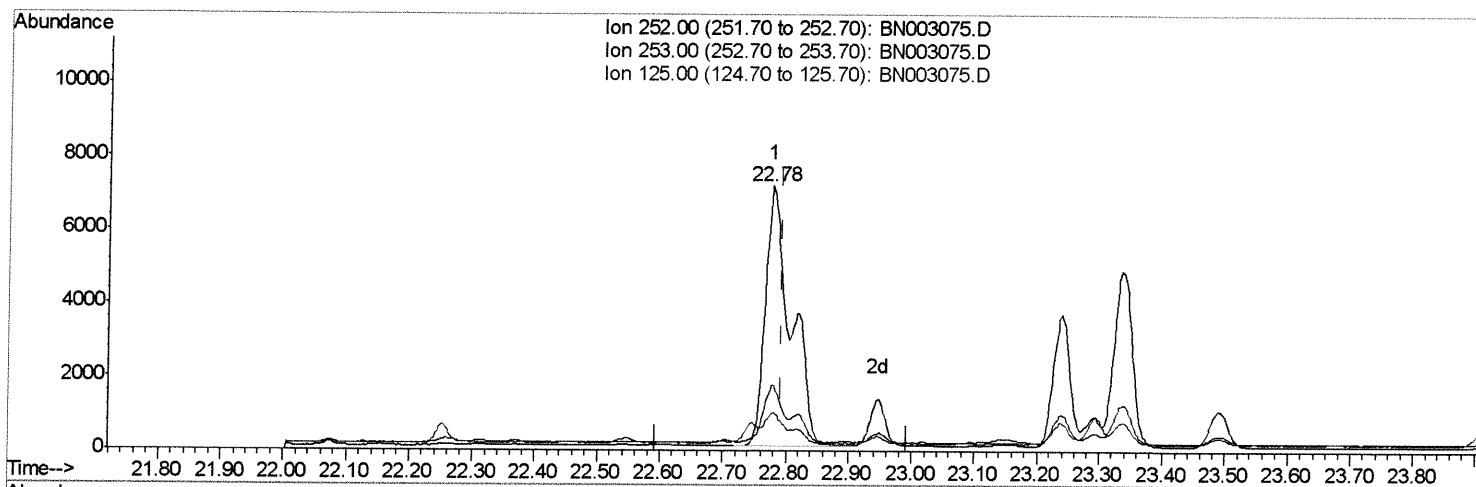

(21) Benzo(b)fluoranthene

22.776min (-0.016) 1.12ng/ul

response 20069

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	24.56
125.00	17.10	14.13
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101118\
 Data File : BN003075.D
 Acq On : 10 Oct 2018 21:41
 Operator : MJ/SJ
 Sample : J5157-19
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 C0AE1

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:45:41 PM

Quant Time: Oct 11 08:00:12 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 07:04:52 2018
 Response via : Initial Calibration

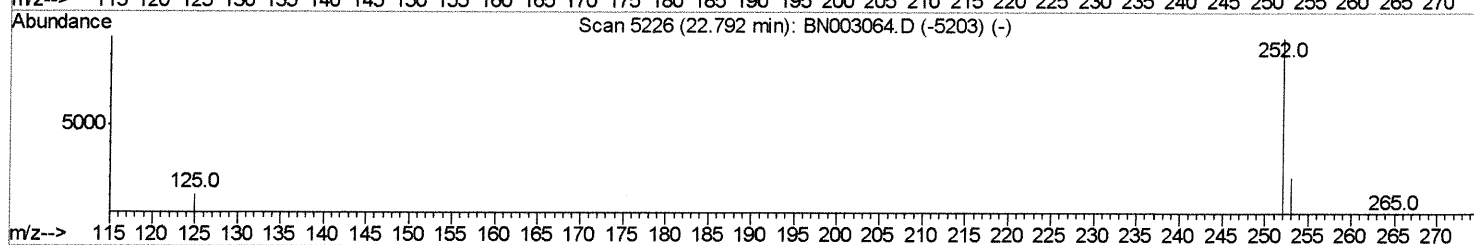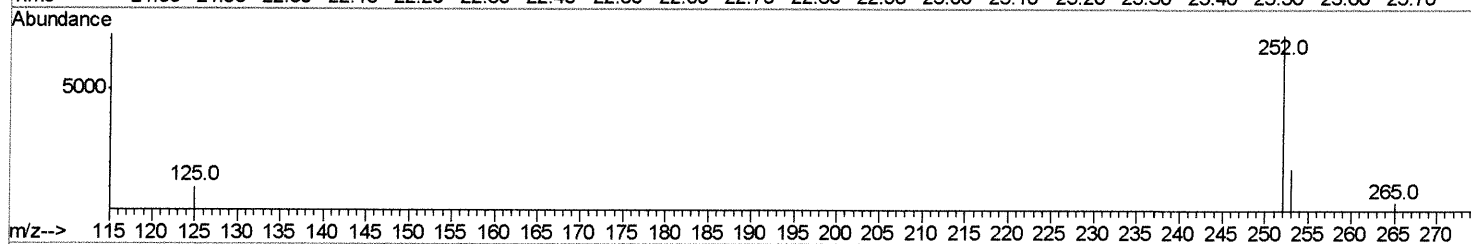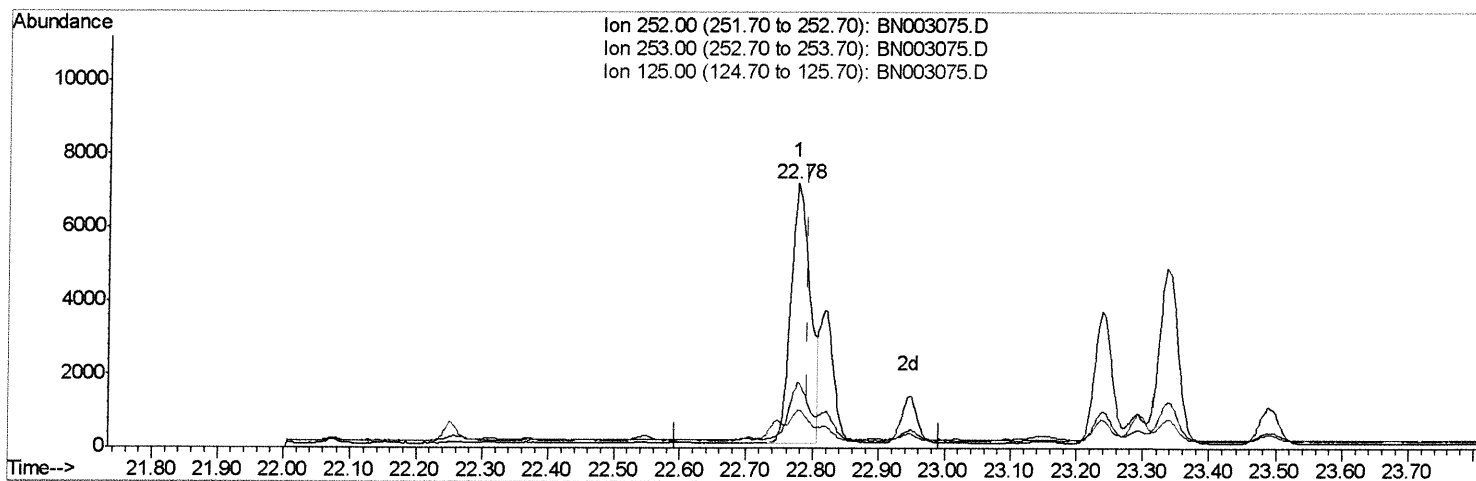

(21) Benzo(b)fluoranthene

22.776min (-0.016) 0.81ng/ul m

response 14443

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	24.56
125.00	17.10	14.13
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101118\
Data File : BN003075.D
Acq On : 10 Oct 2018 21:41
Operator : MJ/SJ
Sample : J5157-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE1

Manual Integrations
APPROVED

Sohil
10/11/2018 5:45:41 PM

Quant Time: Oct 11 08:00:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 07:04:52 2018
Response via : Initial Calibration

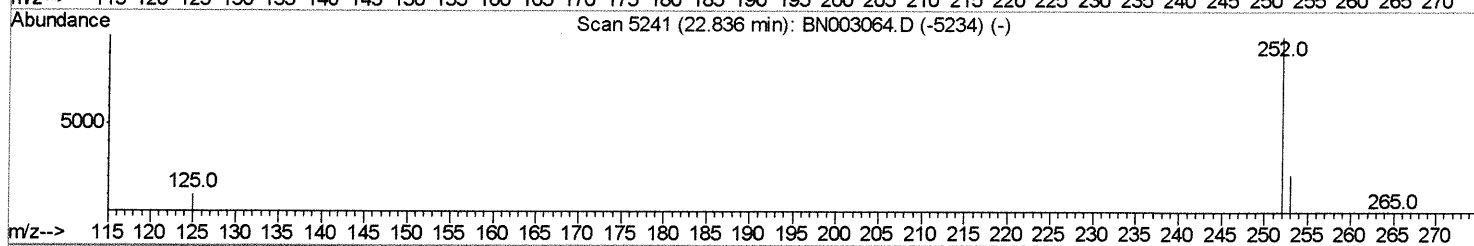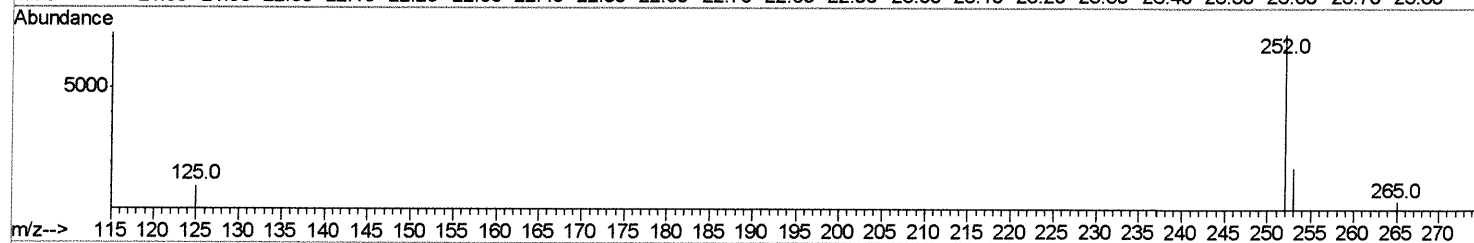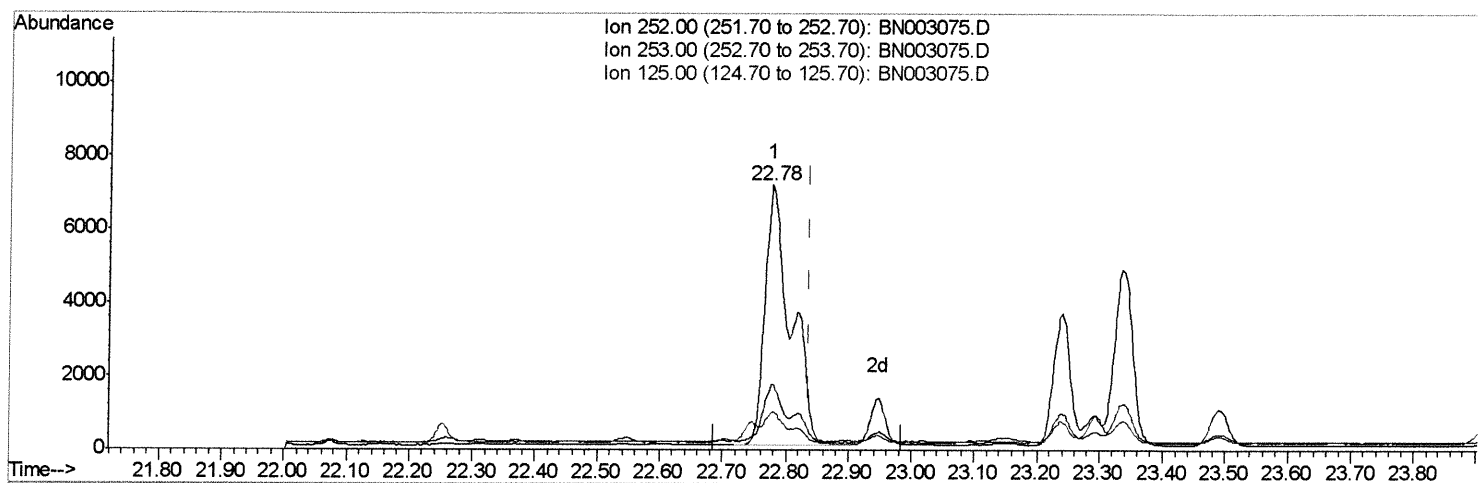

TIC: BN003075.D

(22) Benzo(k)fluoranthene

22.776min (-0.060) 1.08ng/ul

response 20069

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	24.56
125.00	17.60	14.13
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101118\
 Data File : BN003075.D
 Acq On : 10 Oct 2018 21:41
 Operator : MJ/SJ
 Sample : J5157-19
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 C0AE1

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:45:41 PM

Quant Time: Oct 11 08:00:12 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 07:04:52 2018
 Response via : Initial Calibration

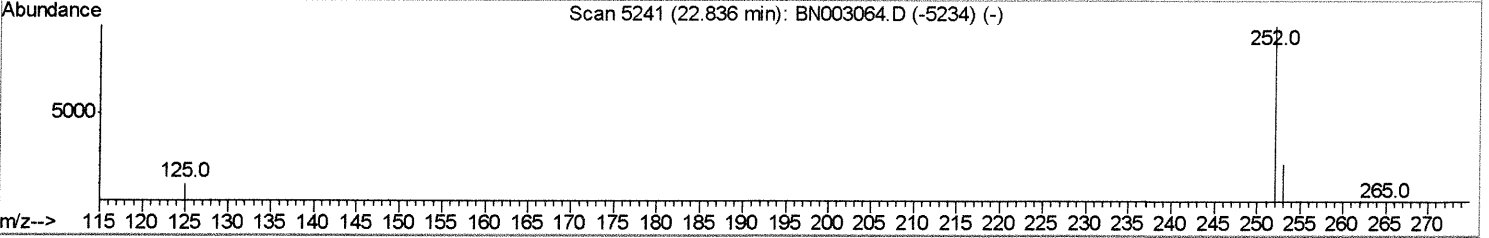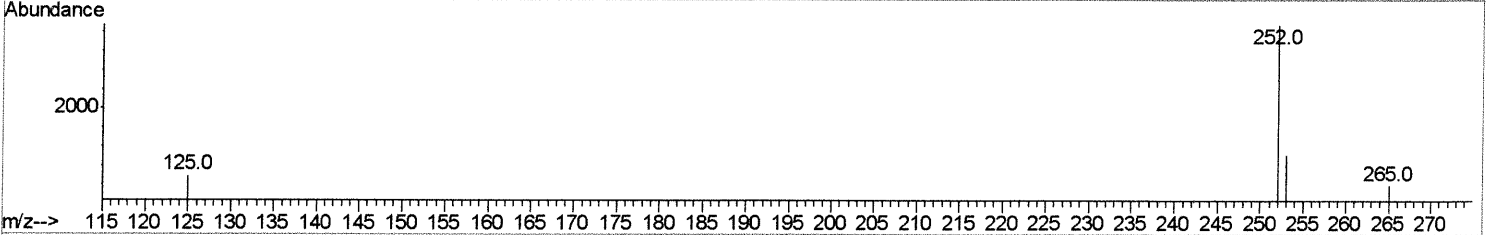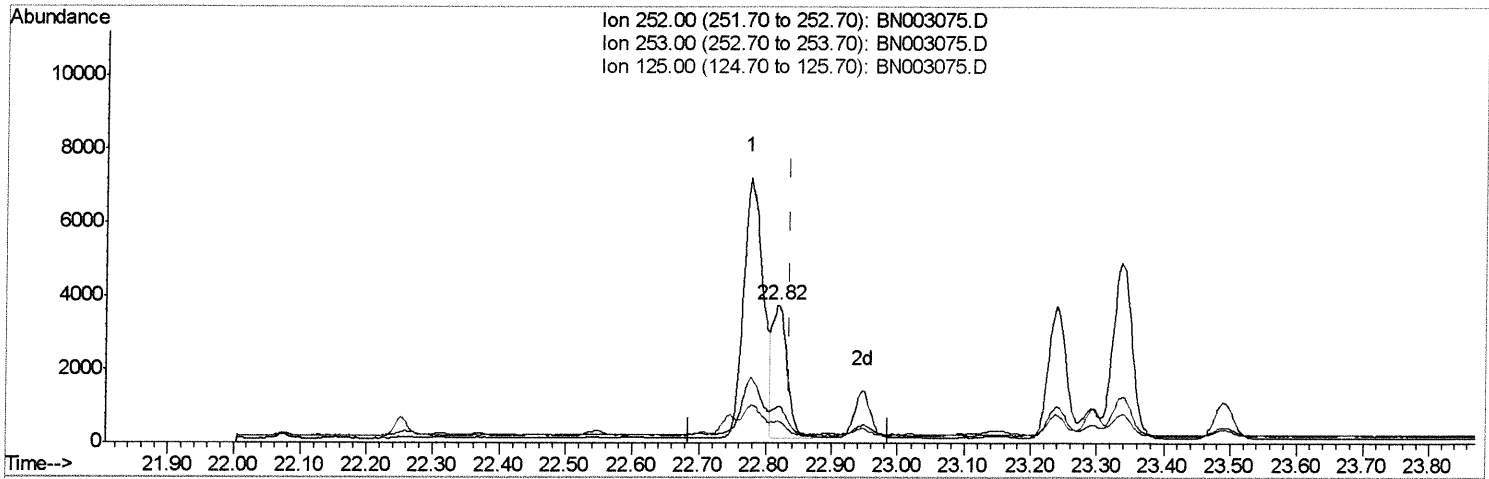

TIC: BN003075.D

(22) Benzo(k)fluoranthene

22.820min (-0.016) 0.30ng/ul m

response 5641

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	27.19
125.00	17.60	15.50
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101118\
 Data File : BN003075.D
 Acq On : 10 Oct 2018 21:41
 Operator : MJ/SJ
 Sample : J5157-19
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AE1

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:45:41 PM

Quant Time: Oct 11 08:00:46 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 07:04:52 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	1834	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.39	136	7536	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.26	164	4241	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.01	188	8389m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.23	240	5461m	0.40	ng/ul	0.00
20) Perylene-d12	23.44	264	4973m	0.40	ng/ul	-0.02
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.01	152	3921	0.34	ng/ul	-0.01
14) Fluoranthene-d10	19.06	212	7552m	0.31	ng/ul	0.00
Target Compounds						
					Ovalue	
3) Naphthalene	10.44	128	710	0.037	ng/ul#	80
7) Acenaphthylene	13.98	152	1841	0.095	ng/ul#	92
12) Phenanthrene	17.06	178	1173m	0.050	ng/ul	
13) Anthracene	17.15	178	3086m	0.140	ng/ul	
15) Fluoranthene	19.09	202	3880m	0.141	ng/ul	
17) Pyrene	19.45	202	7777m	0.367	ng/ul	
18) Benzo(a)anthracene	21.22	228	3779m	0.215	ng/ul	
19) Chrysene	21.27	228	8750	0.490	ng/ul	99
21) Benzo(b)fluoranthene	22.78	252	14443m	0.806	ng/ul	
22) Benzo(k)fluoranthene	22.82	252	5641m	0.304	ng/ul	
23) Benzo(a)pyrene	23.33	252	9761	0.608	ng/ul#	92
24) Indeno(1,2,3-cd)pyrene	25.66	276	5787	0.314	ng/ul#	95
25) Dibenzo(a,h)anthracene	25.66	278	1844	0.125	ng/ul#	80
26) Benzo(a,h,i)perylene	26.34	276	5549	0.357	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed