

Quantitation Report (QT Reviewed)


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101118\
 Data File : BN003094.D
 Acq On : 11 Oct 2018 09:14
 Operator : MJ/SJ
 Sample : J5157-16DL 2X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD8DL

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:45:12 PM

Quant Time: Oct 11 13:37:31 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 08:10:30 2018
 Response via : Initial Calibration

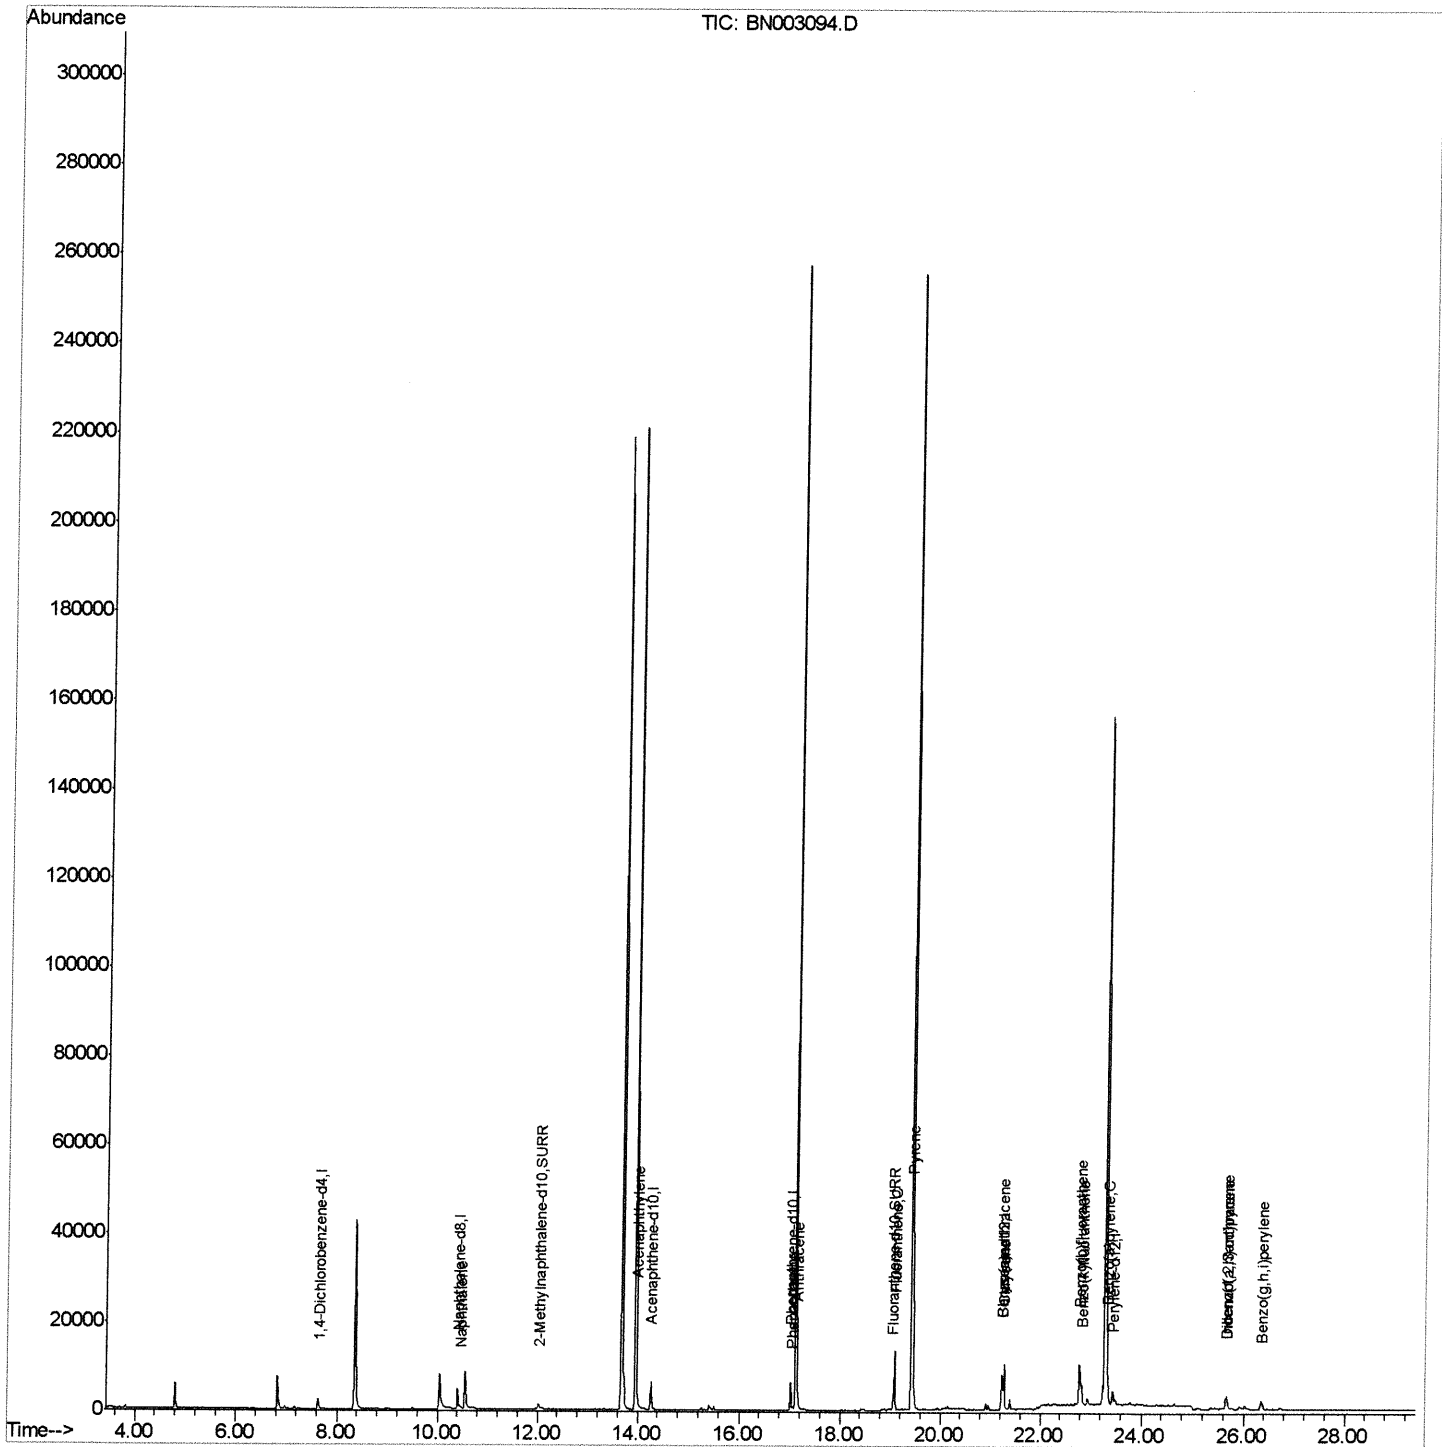

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101118\
Data File : BN003094.D
Acq On : 11 Oct 2018 09:14
Operator : MJ/SJ
Sample : J5157-16DL 2X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD8DL

Manual Integrations
APPROVED

Sohil
10/11/2018 5:45:12 PM

Quant Time: Oct 11 13:32:40 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 08:10:30 2018
Response via : Initial Calibration

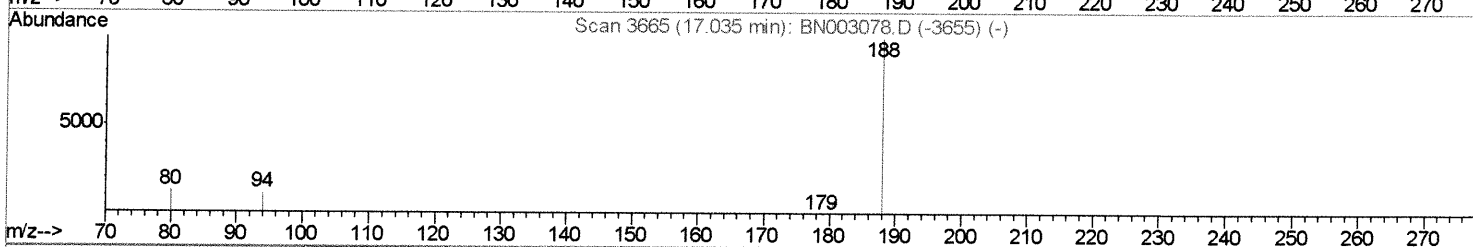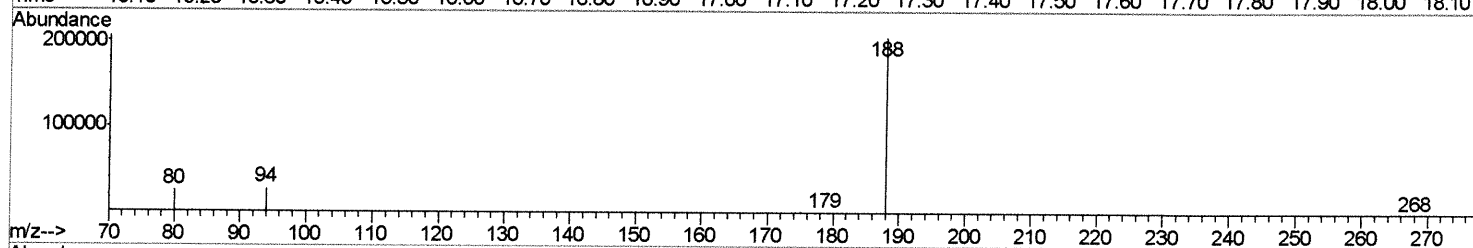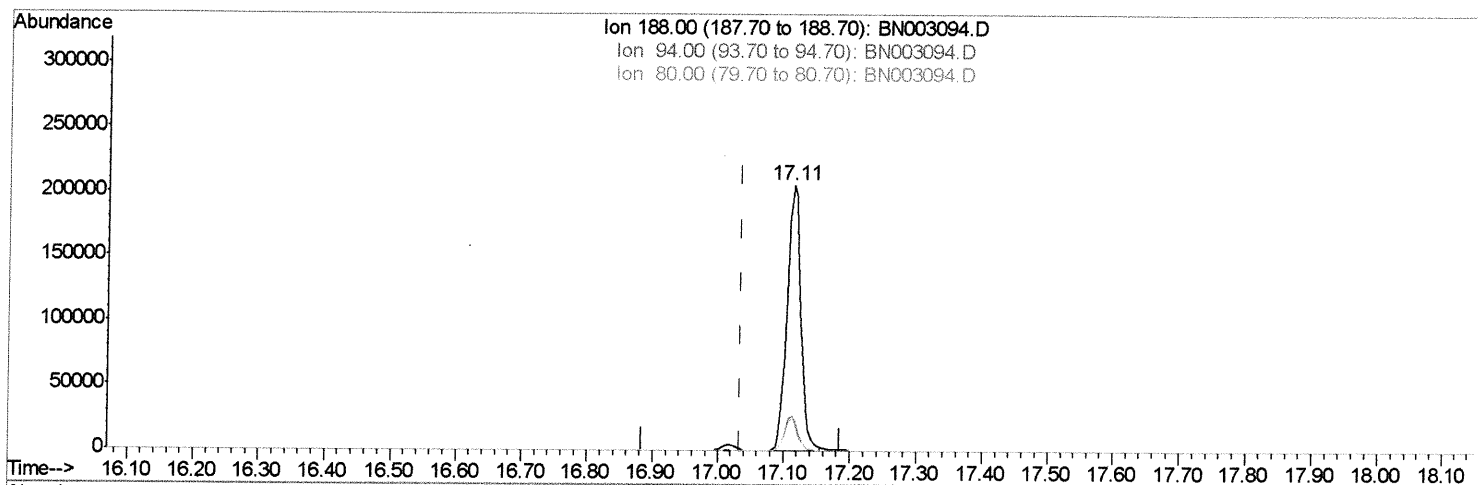

TIC: BN003094.D

(10) Phenanthrene-d10 (I)

17.111min (+0.076) 0.40ng/ul

response 305558

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	13.15
80.00	12.70	12.12
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101118\
 Data File : BN003094.D
 Acq On : 11 Oct 2018 09:14
 Operator : MJ/SJ
 Sample : J5157-16DL 2X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD8DL

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:45:12 PM

Quant Time: Oct 11 13:32:40 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 08:10:30 2018
 Response via : Initial Calibration

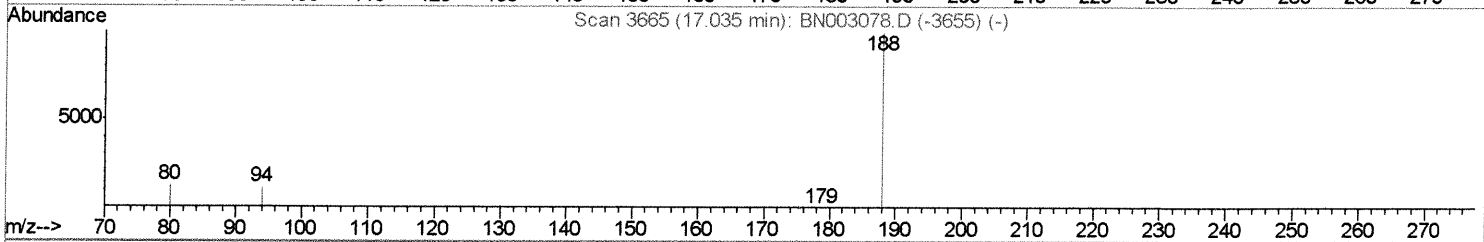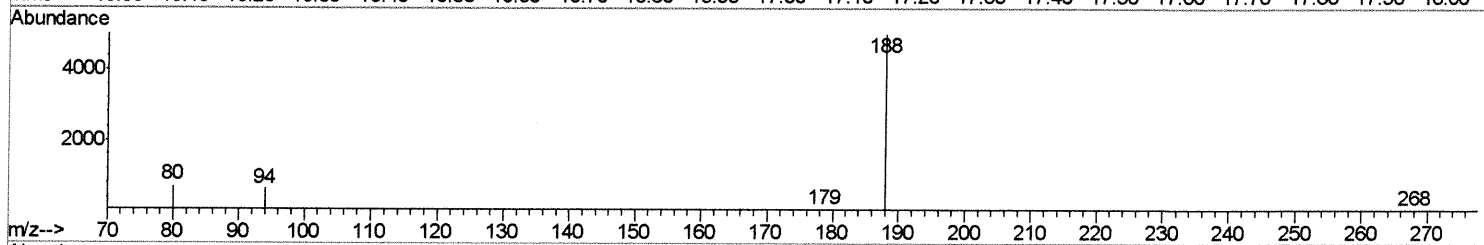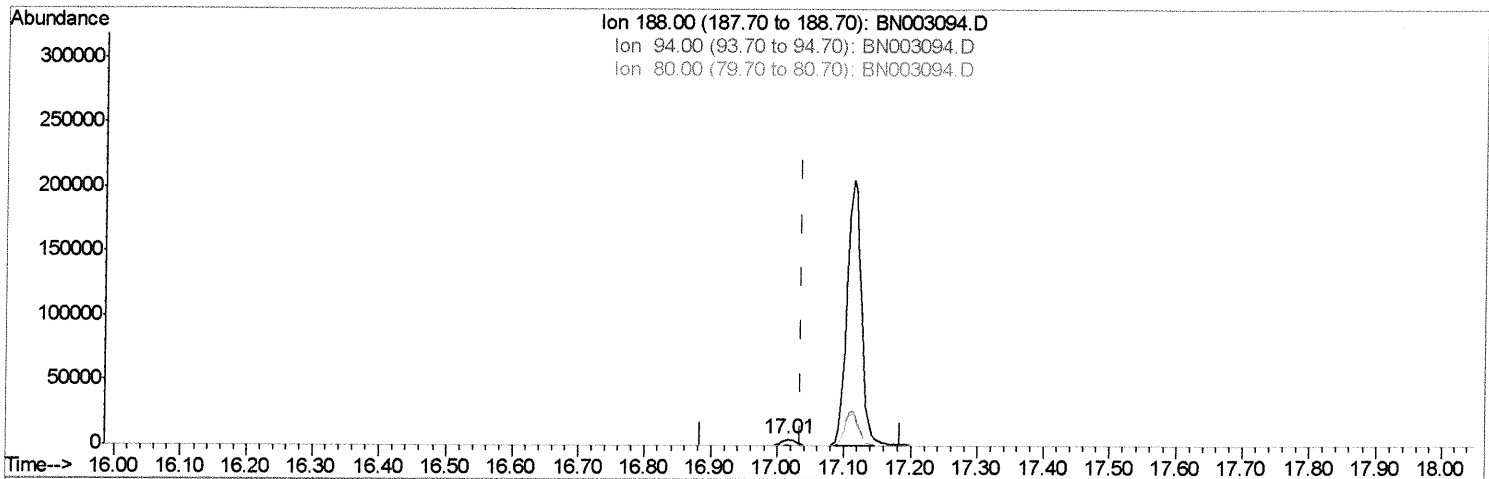

TIC: BN003094.D

(10) Phenanthrene-d10 (I)

17.014min (-0.021) 0.40ng/ul m

response 7409

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	12.43
80.00	12.70	13.96
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101118\
Data File : BN003094.D
Acq On : 11 Oct 2018 09:14
Operator : MJ/SJ
Sample : J5157-16DL 2X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD8DL

Manual Integrations
APPROVED

Sohil
10/11/2018 5:45:12 PM

Quant Time: Oct 11 13:33:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 08:10:30 2018
Response via : Initial Calibration

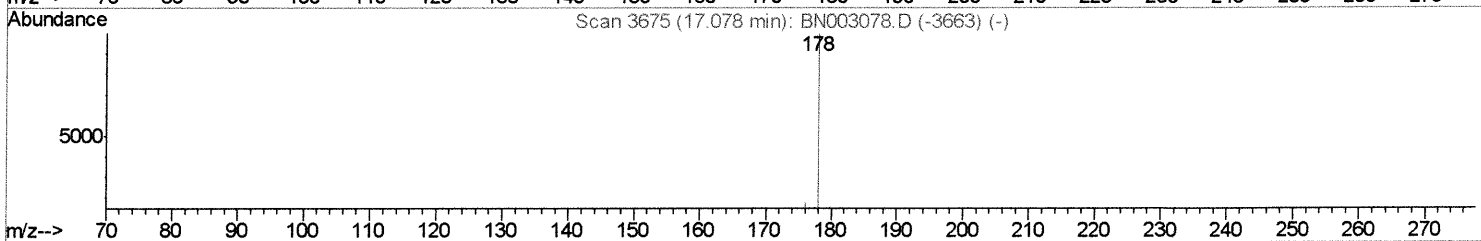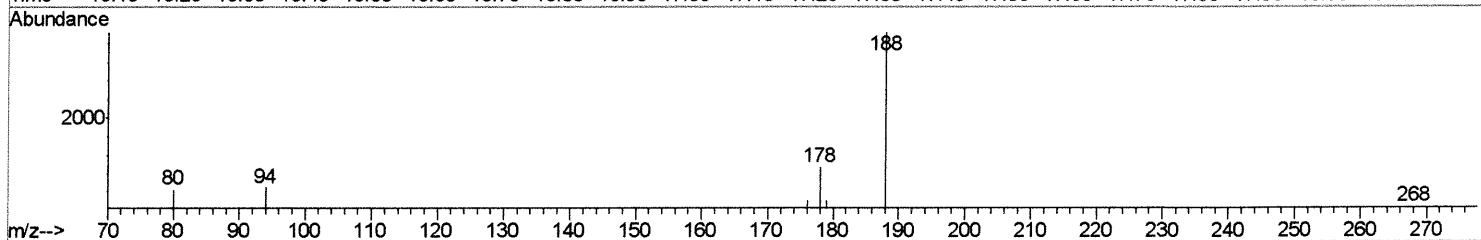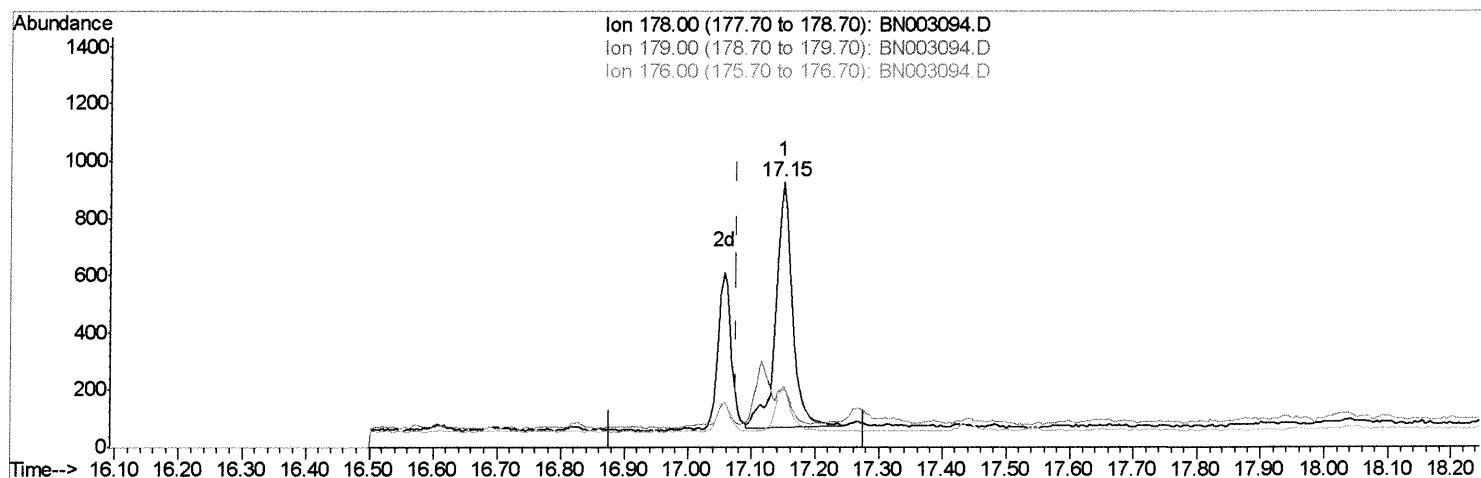

TIC: BN003094.D

(12) Phenanthrene

17.149min (+0.072) 0.08ng/ul

response 1553

Ion	Exp%	Act%
178.00	100	100
179.00	16.10	23.05#
176.00	19.30	22.29
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101118\
 Data File : BN003094.D
 Acq On : 11 Oct 2018 09:14
 Operator : MJ/SJ
 Sample : J5157-16DL 2X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD8DL

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:45:12 PM

Quant Time: Oct 11 13:33:55 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 08:10:30 2018
 Response via : Initial Calibration

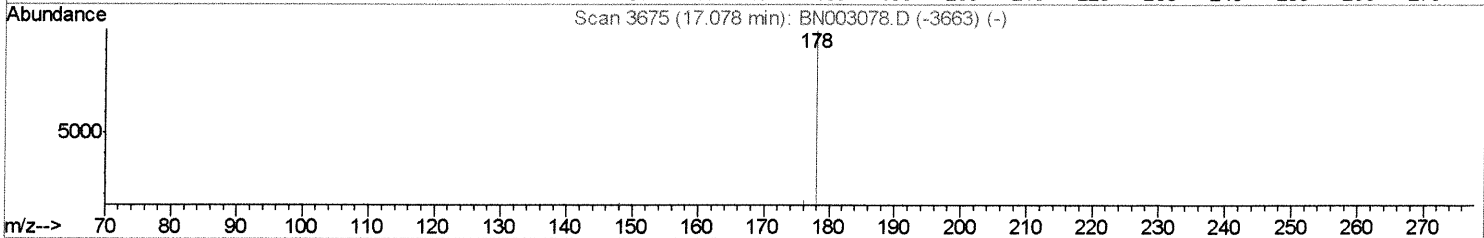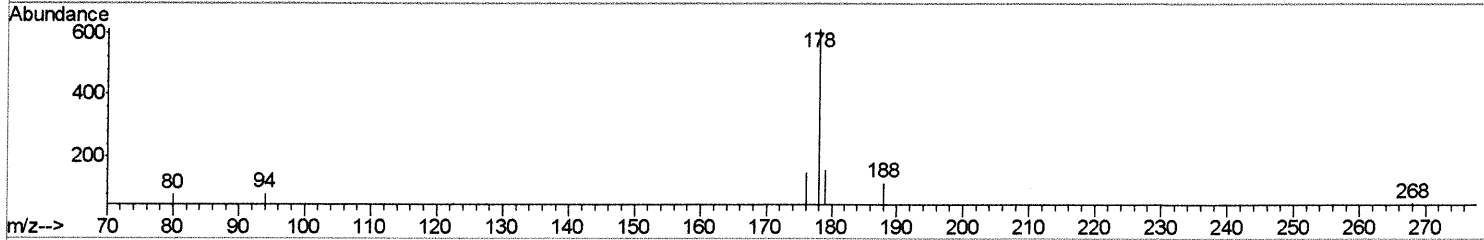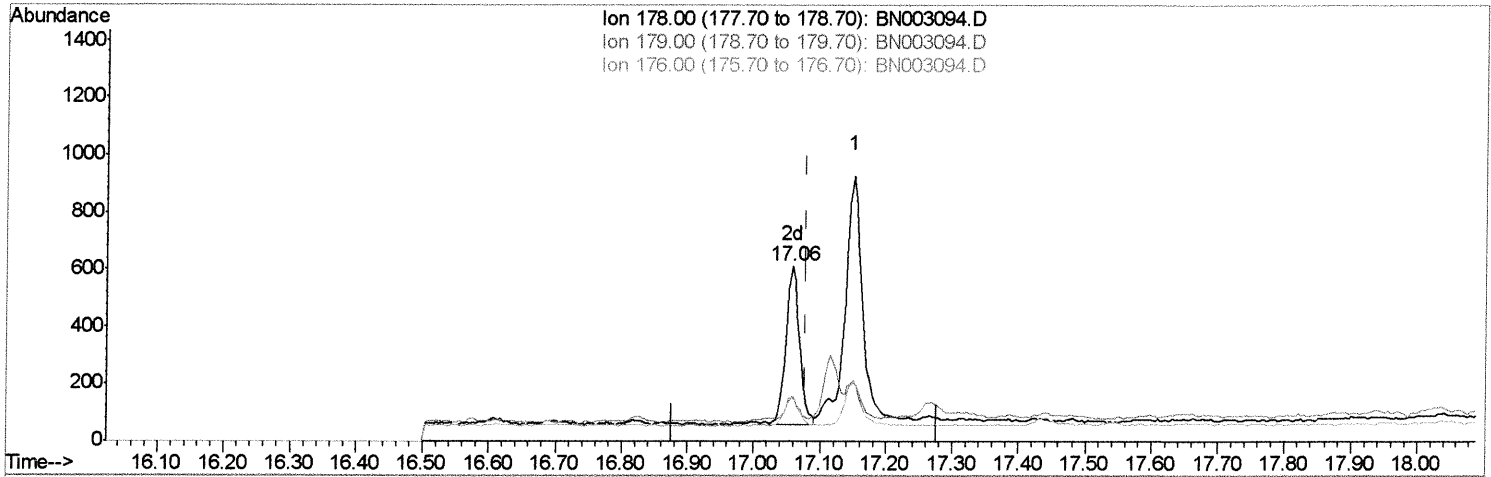

TIC: BN003094.D

(12) Phenanthrene

17.056min (-0.021) 0.04ng/ul m

response 804

Ion	Exp%	Act%
178.00	100	100
179.00	16.10	25.90#
176.00	19.30	24.92#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101118\
 Data File : BN003094.D
 Acq On : 11 Oct 2018 09:14
 Operator : MJ/SJ
 Sample : J5157-16DL 2X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD8DL

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:45:12 PM

Quant Time: Oct 11 13:33:55 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 08:10:30 2018
 Response via : Initial Calibration

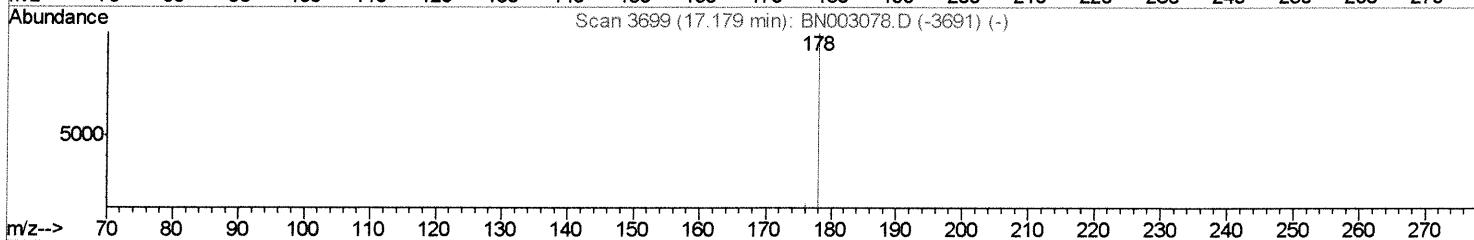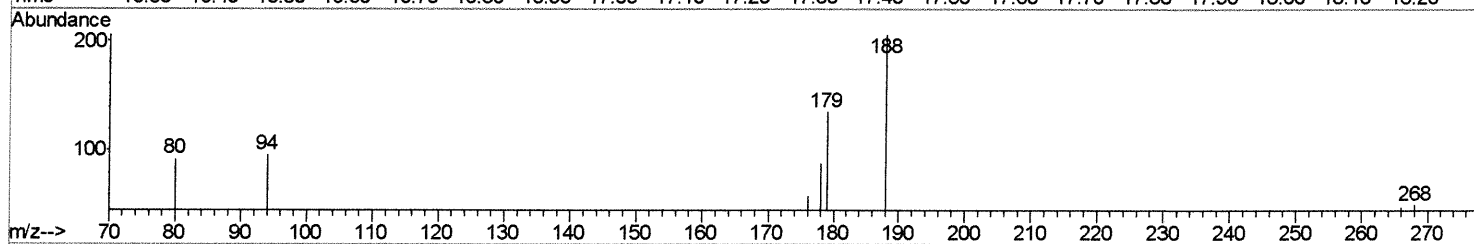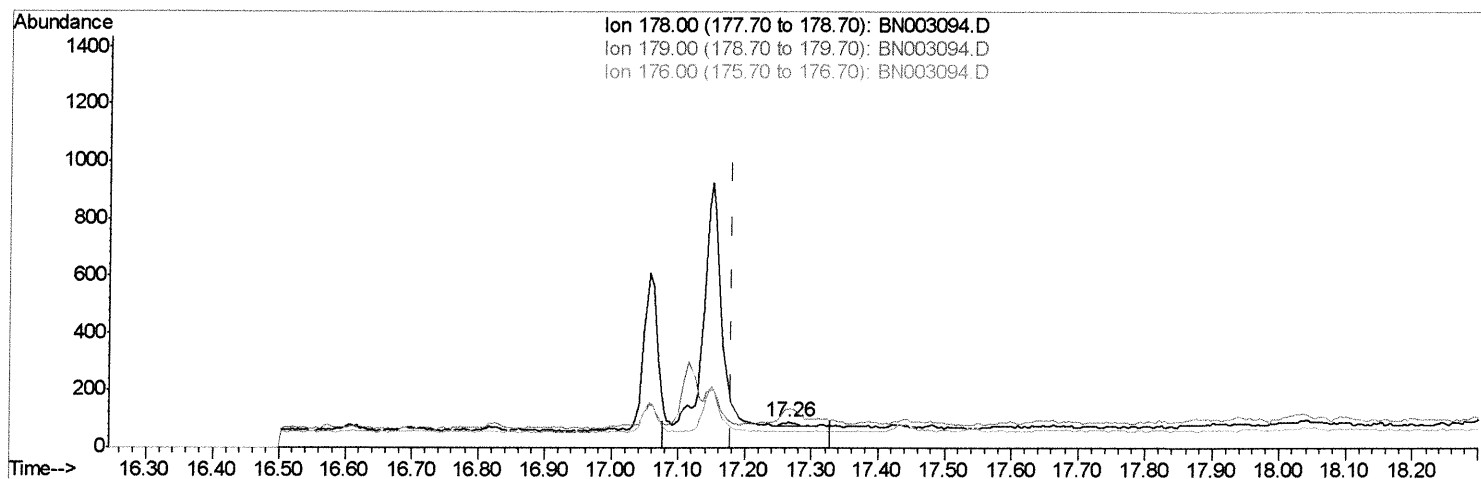

TIC: BN003094.D

(13) Anthracene

17.263min (+0.084) 0.00ng/ul

response 23

Ion	Exp%	Act%
178.00	100	100
179.00	16.30	151.69#
176.00	19.10	66.29#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101118\
 Data File : BN003094.D
 Acq On : 11 Oct 2018 09:14
 Operator : MJ/SJ
 Sample : J5157-16DL 2X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD8DL

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:45:12 PM

Quant Time: Oct 11 13:33:55 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 08:10:30 2018
 Response via : Initial Calibration

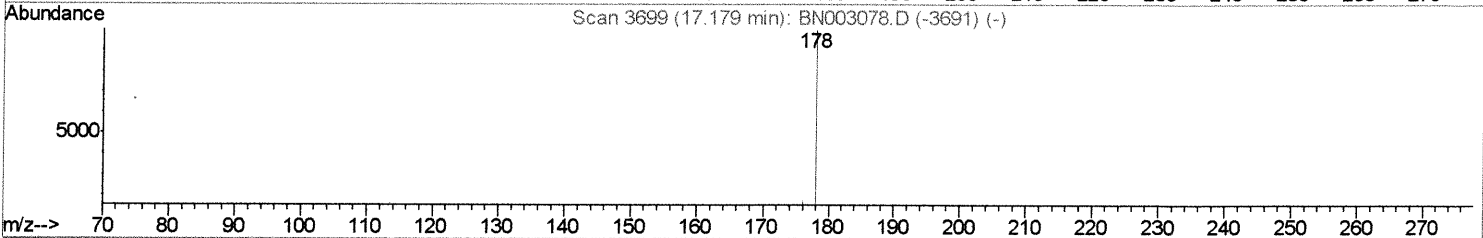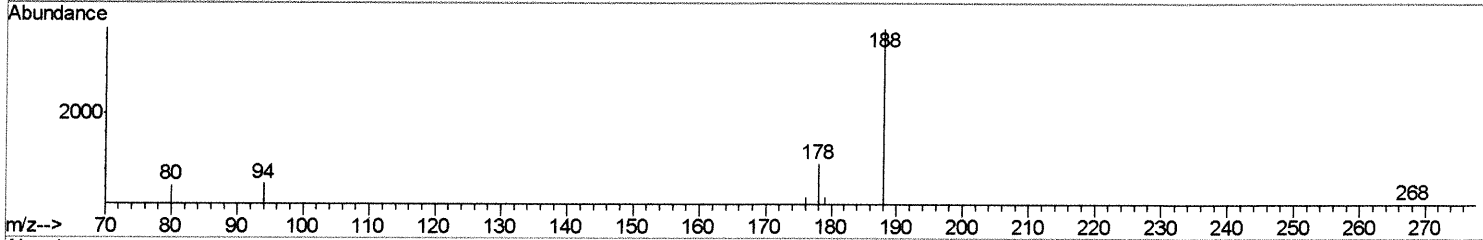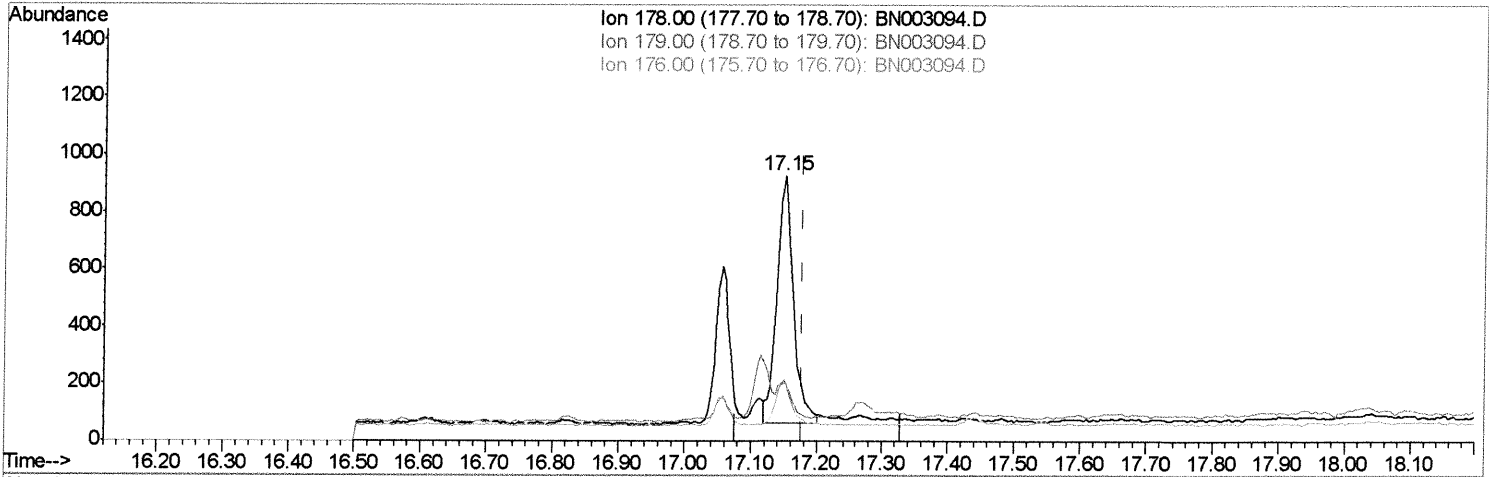

TIC: BN003094.D

(13) Anthracene

17.149min (-0.030) 0.08ng/ul m

response 1474

Ion Exp% Act%

178.00 100 100

179.00 16.30 23.05#

176.00 19.10 22.29

0.00 0.00 0.00

85 10/12/18

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101118\
 Data File : BN003094.D
 Acq On : 11 Oct 2018 09:14
 Operator : MJ/SJ
 Sample : J5157-16DL 2X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD8DL

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:45:12 PM

Quant Time: Oct 11 13:33:55 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 08:10:30 2018
 Response via : Initial Calibration

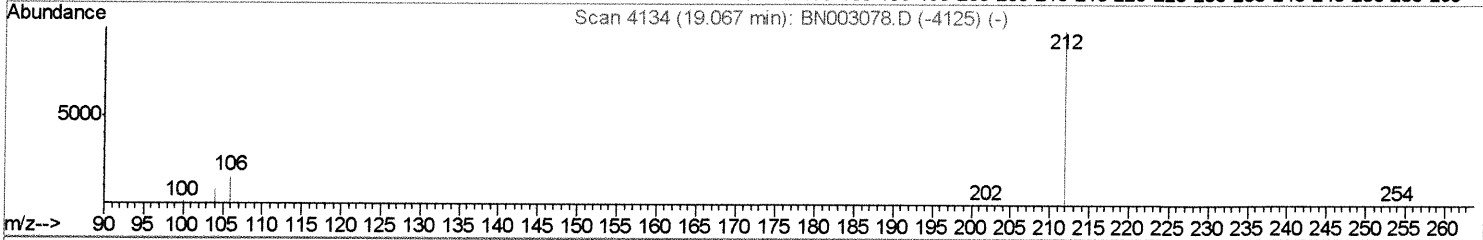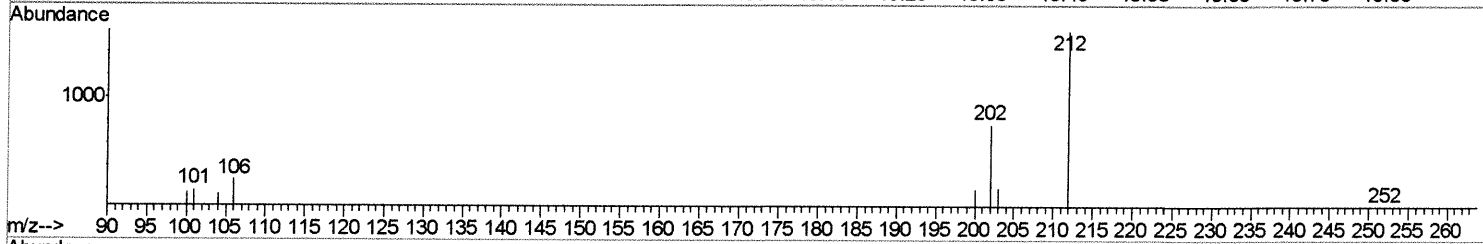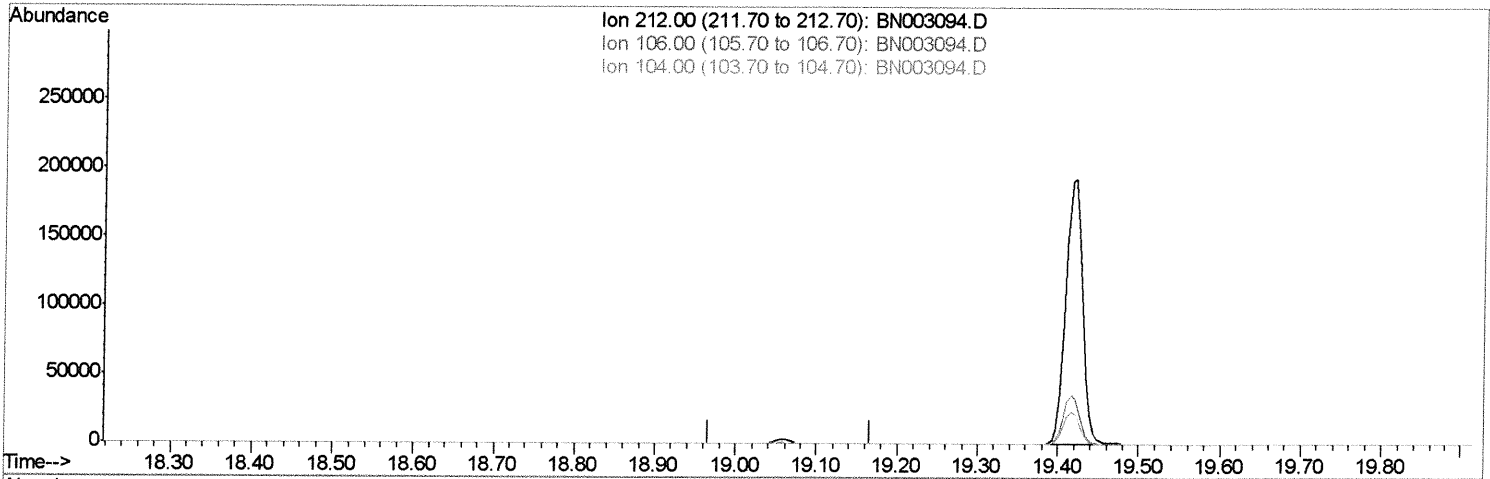

TIC: BN003094.D

(14) Fluoranthene-d10 (SURR)

19.067min (-19.067) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	15.40	0.00#
104.00	8.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101118\
Data File : BN003094.D
Acq On : 11 Oct 2018 09:14
Operator : MJ/SJ
Sample : J5157-16DL 2X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD8DL

Manual Integrations
APPROVED

Sohil
10/11/2018 5:45:12 PM

Quant Time: Oct 11 13:33:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 08:10:30 2018
Response via : Initial Calibration

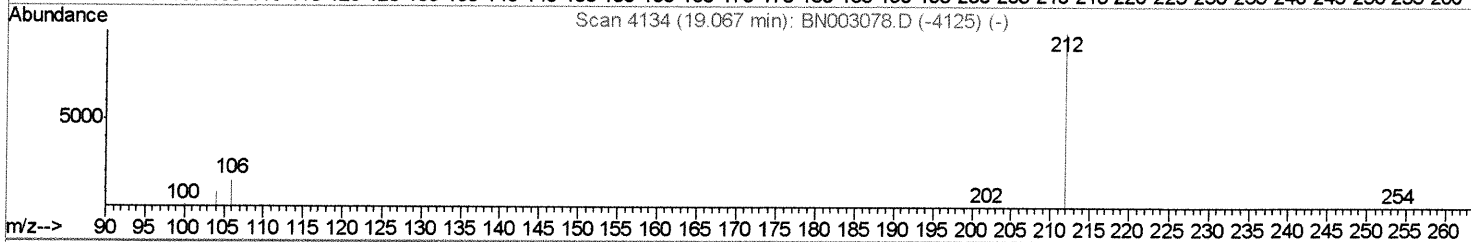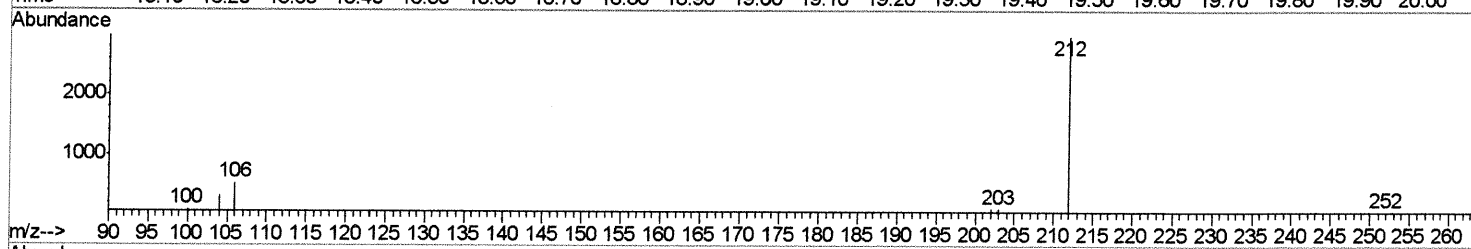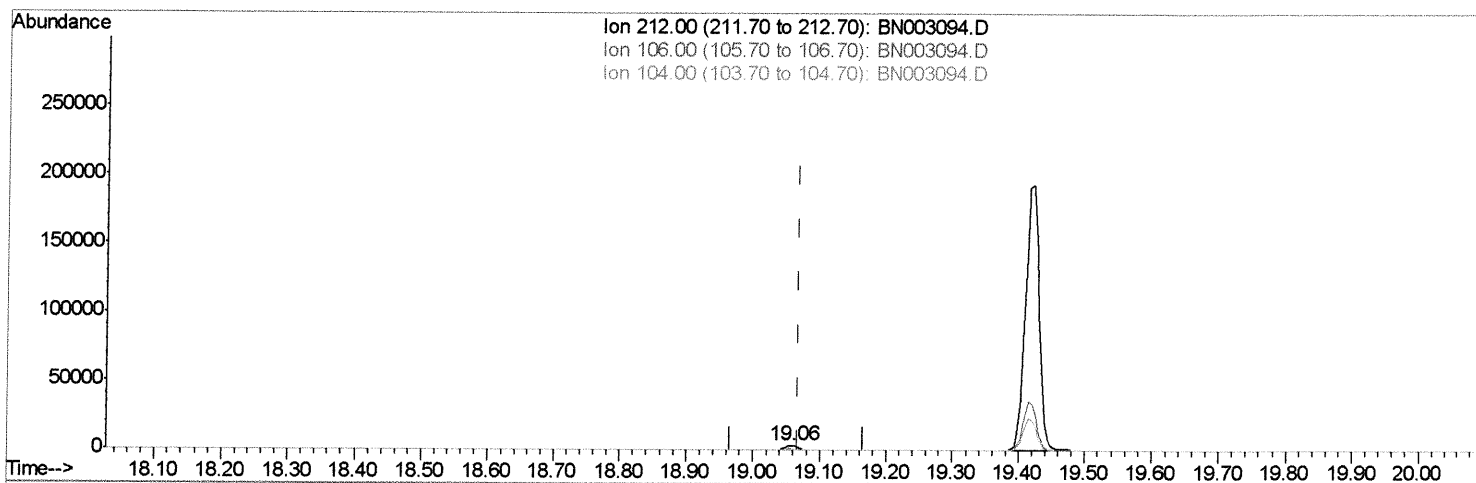

TIC: BN003094.D

(14) Fluoranthene-d10 (SURR)

19.058min (-0.009) 0.19ng/ul m

response 4115

Ion	Exp%	Act%
212.00	100	100
106.00	15.40	0.00#
104.00	8.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101118\
Data File : BN003094.D
Acq On : 11 Oct 2018 09:14
Operator : MJ/SJ
Sample : J5157-16DL 2X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD8DL

Manual Integrations
APPROVED

Sohil
10/11/2018 5:45:12 PM

Quant Time: Oct 11 13:33:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 08:10:30 2018
Response via : Initial Calibration

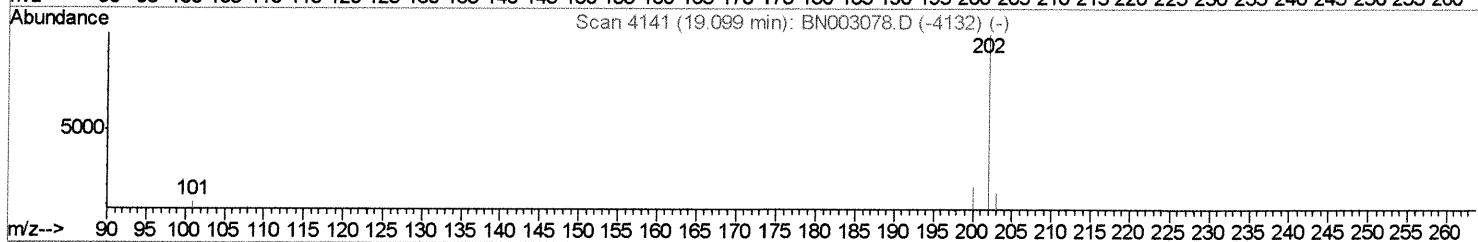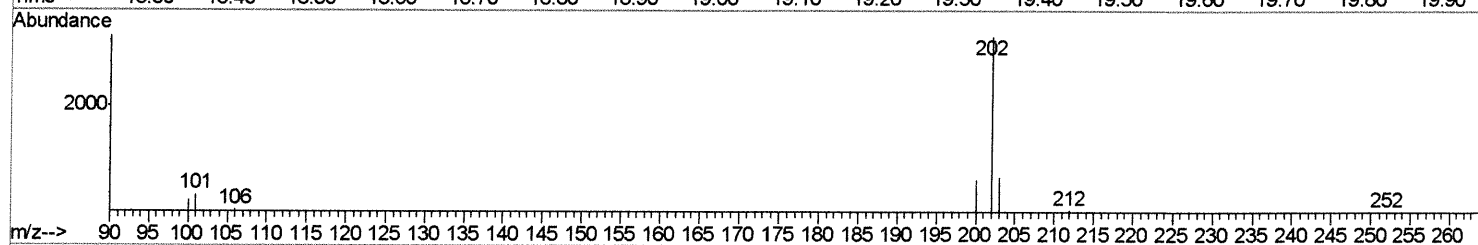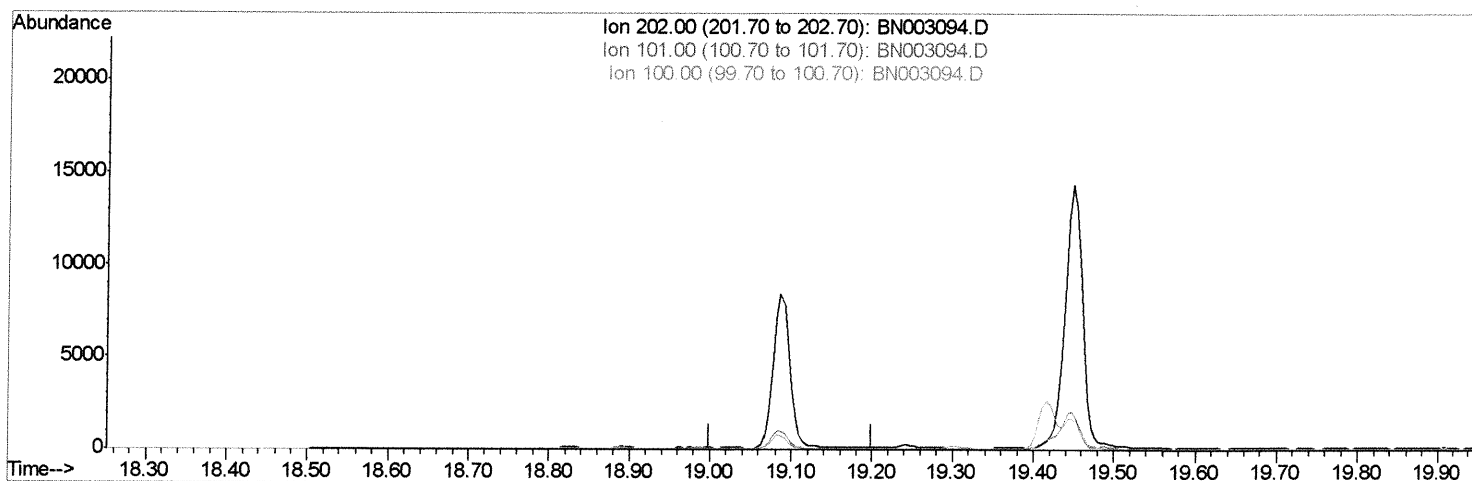

TIC: BN003094.D

(15) Fluoranthene (C)

19.099min (-19.099) 0.00ng/ul

response 0

Ion	Exp%	Act%
202.00	100	0.00
101.00	12.30	0.00
100.00	9.10	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101118\
 Data File : BN003094.D
 Acq On : 11 Oct 2018 09:14
 Operator : MJ/SJ
 Sample : J5157-16DL 2X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD8DL

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:45:12 PM

Quant Time: Oct 11 13:33:55 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 08:10:30 2018
 Response via : Initial Calibration

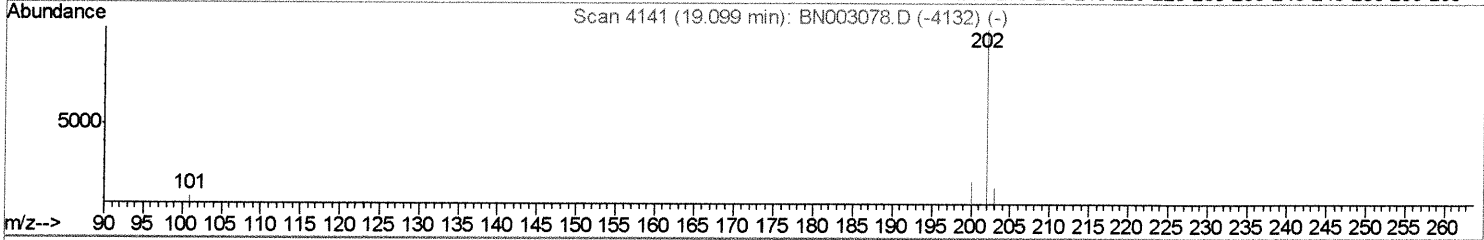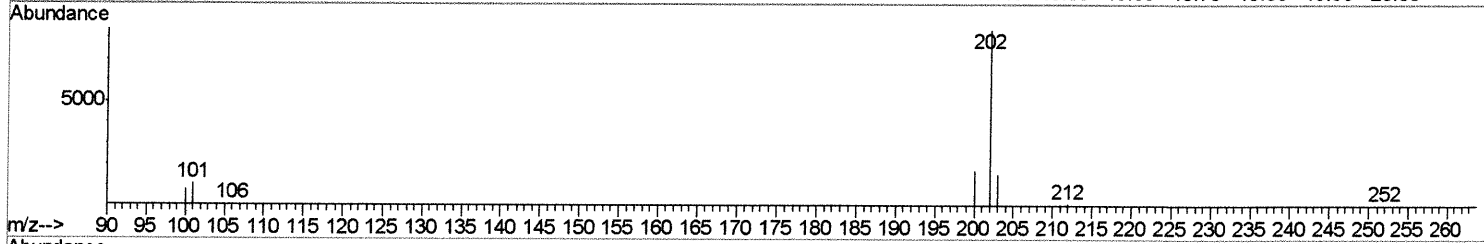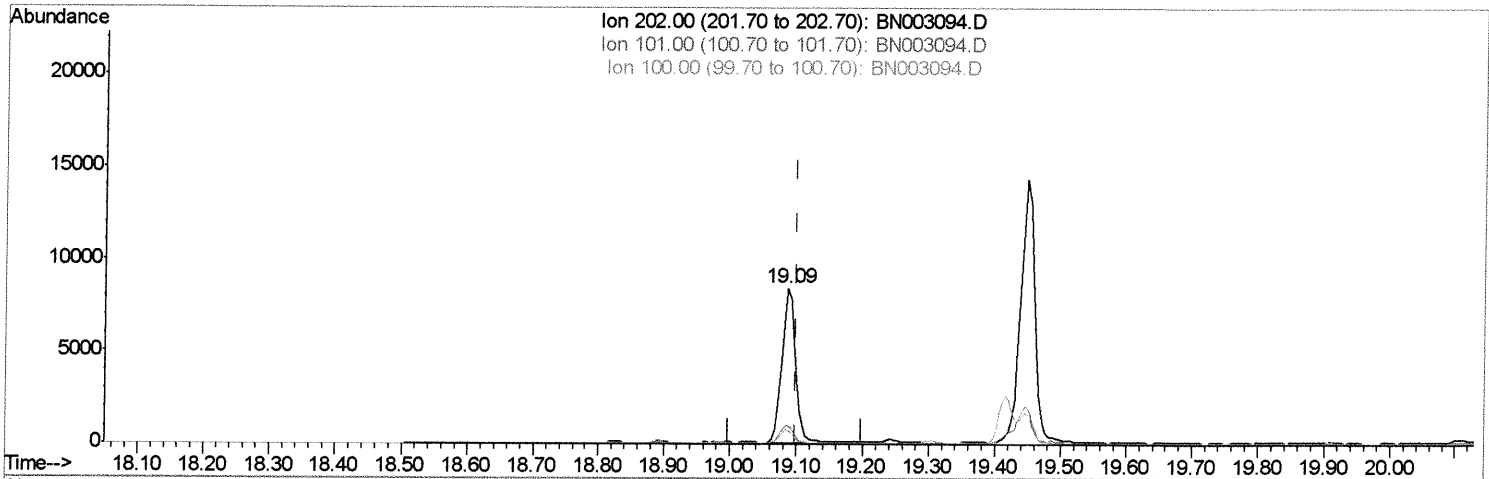

TIC: BN003094.D

(15) Fluoranthene (C)

19.085min (-0.014) 0.49ng/ul m

response 11950

Ion	Exp%	Act%
202.00	100	100
101.00	12.30	12.66
100.00	9.10	9.68
0.00	0.00	0.00

856112/18

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101118\
 Data File : BN003094.D
 Acq On : 11 Oct 2018 09:14
 Operator : MJ/SJ
 Sample : J5157-16DL 2X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 C0AD8DL

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:45:12 PM

Quant Time: Oct 11 13:33:55 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 08:10:30 2018
 Response via : Initial Calibration

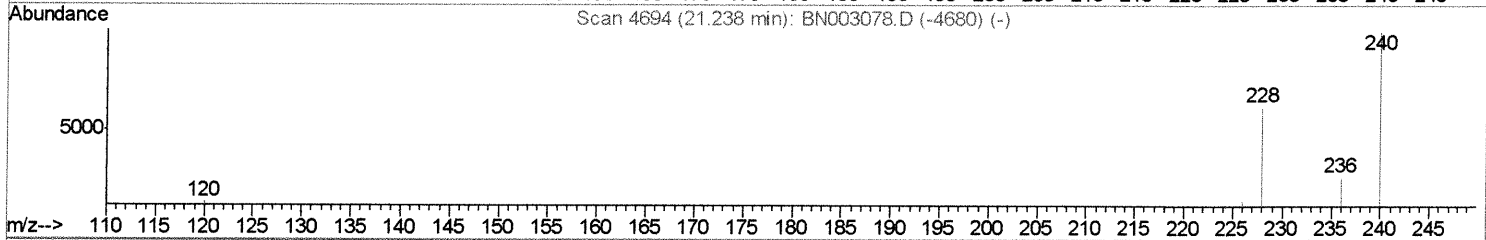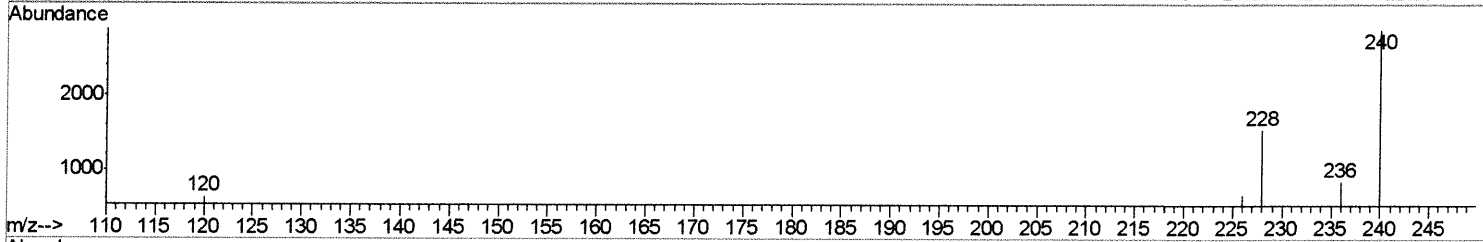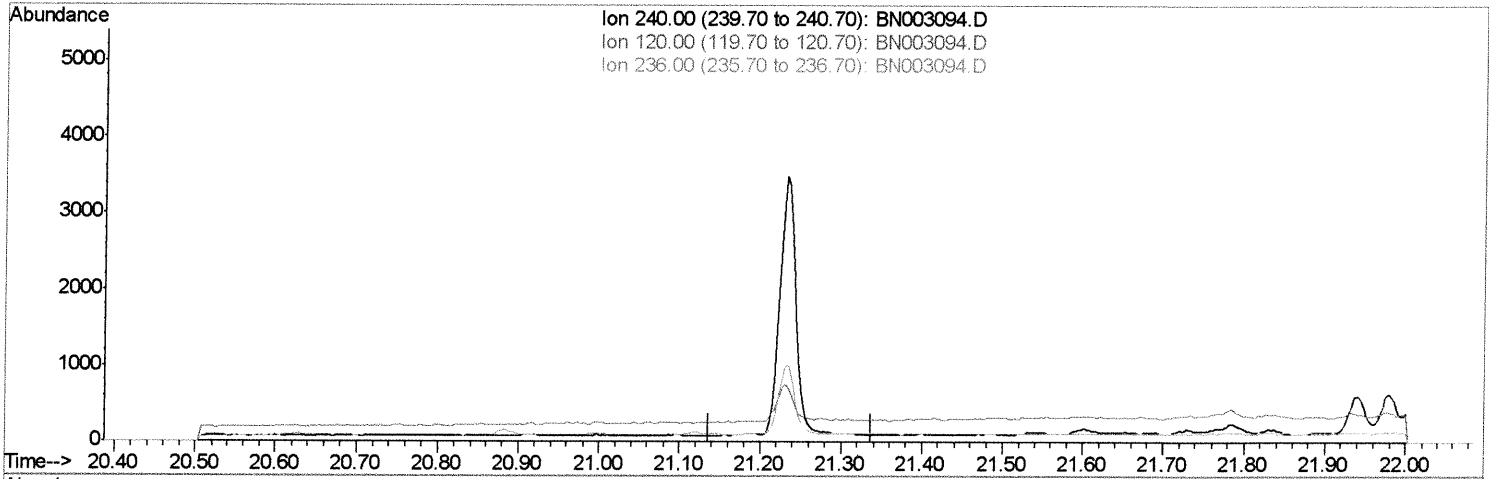

(16) Chrysene-d12 (I)

21.238min (-21.238) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	16.40	0.00#
236.00	28.10	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101118\
Data File : BN003094.D
Acq On : 11 Oct 2018 09:14
Operator : MJ/SJ
Sample : J5157-16DL 2X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
C0AD8DL

Manual Integrations
APPROVED

Sohil
10/11/2018 5:45:12 PM

Quant Time: Oct 11 13:33:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 08:10:30 2018
Response via : Initial Calibration

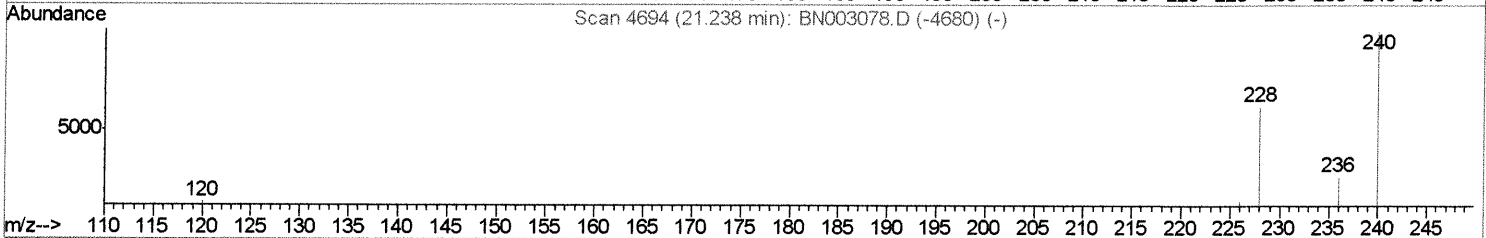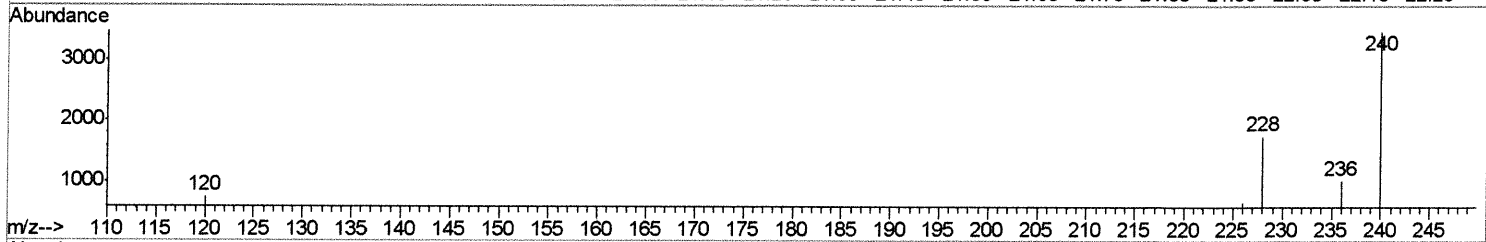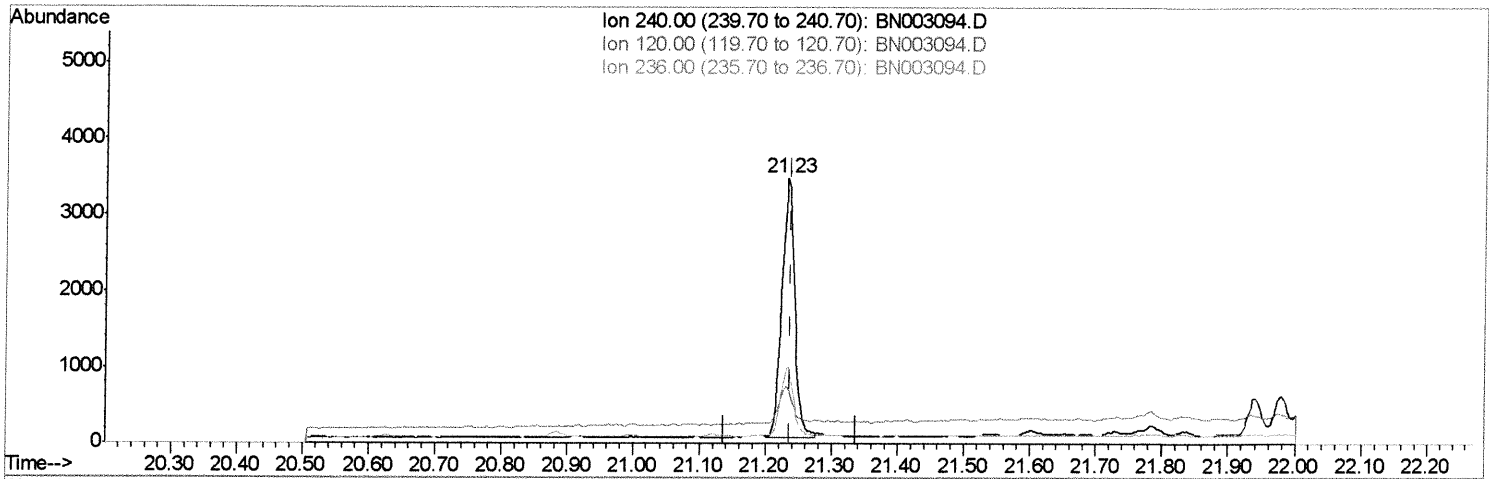

TIC: BN003094.D

(16) Chrysene-d12 (I)

21.232min (-0.006) 0.40ng/ul m

response 4588

Ion	Exp%	Act%
240.00	100	100
120.00	16.40	21.18#
236.00	28.10	29.29
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101118\
 Data File : BN003094.D
 Acq On : 11 Oct 2018 09:14
 Operator : MJ/SJ
 Sample : J5157-16DL 2X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD8DL

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:45:12 PM

Quant Time: Oct 11 13:36:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 08:10:30 2018
 Response via : Initial Calibration

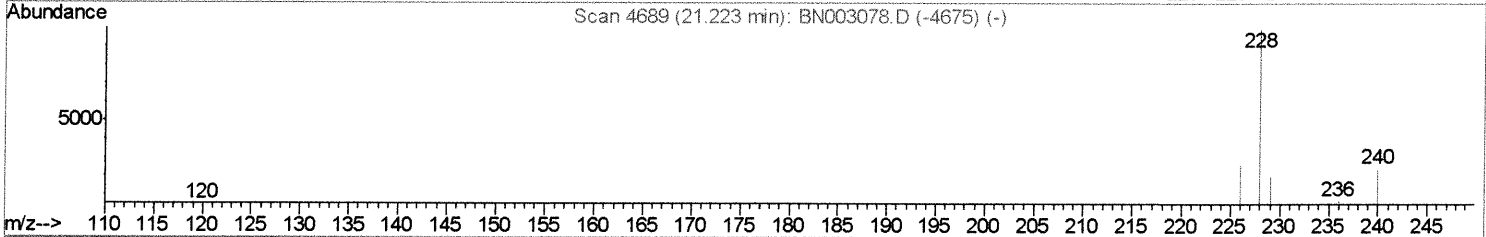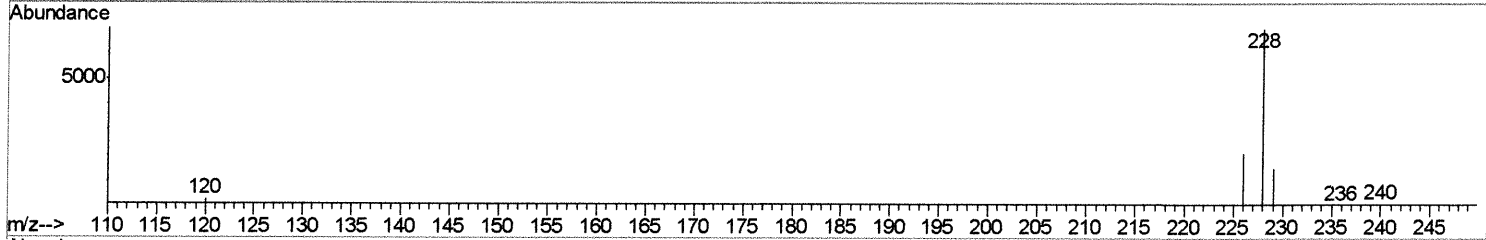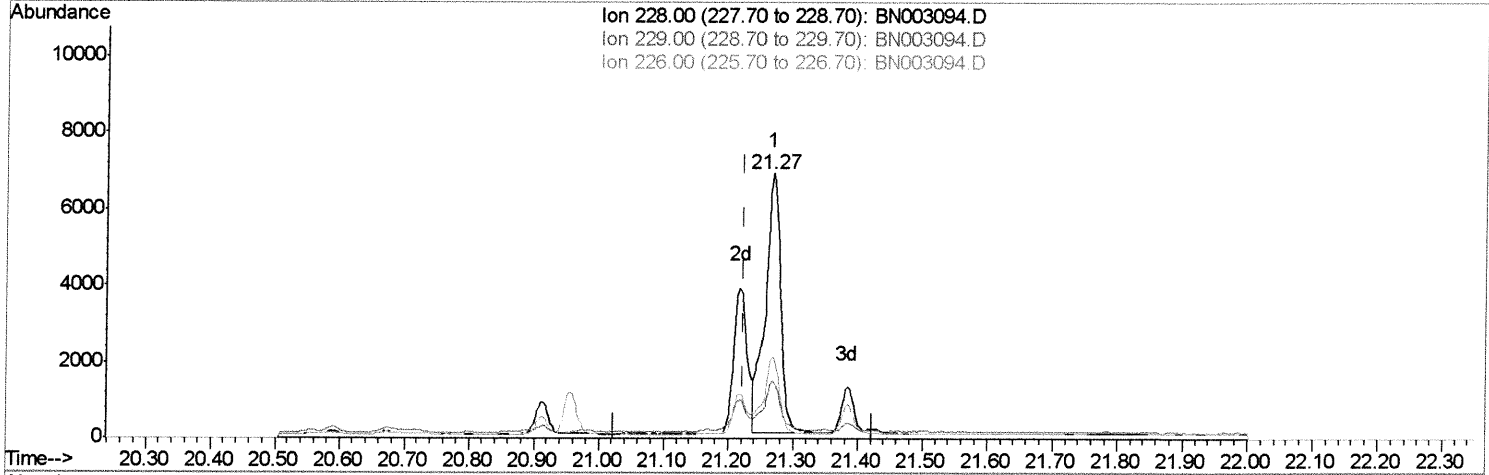

TIC: BN003094.D

(18) Benzo(a)anthracene
 21.267min (+0.044) 0.77ng/ul
 response 11378

Ion	Exp%	Act%
228.00	100	100
229.00	20.20	21.79
226.00	27.90	30.78
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101118\
 Data File : BN003094.D
 Acq On : 11 Oct 2018 09:14
 Operator : MJ/SJ
 Sample : J5157-16DL 2X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD8DL

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:45:12 PM

Quant Time: Oct 11 13:36:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 08:10:30 2018
 Response via : Initial Calibration

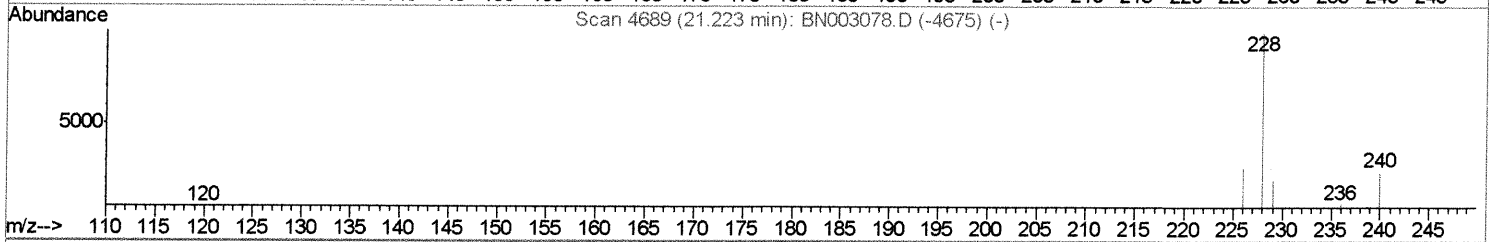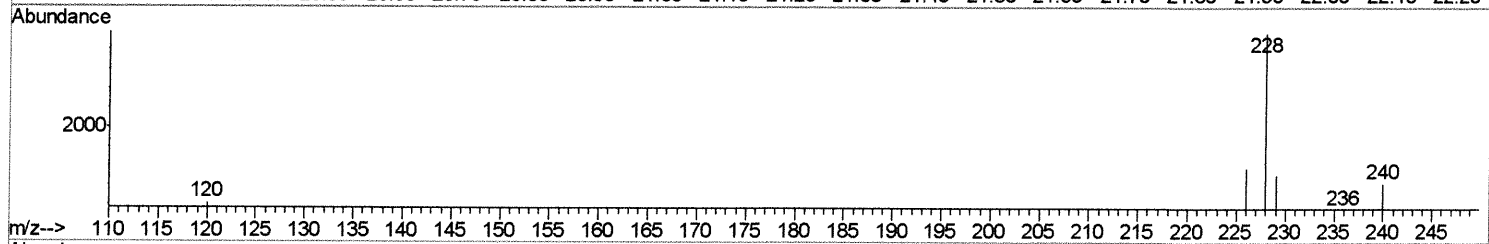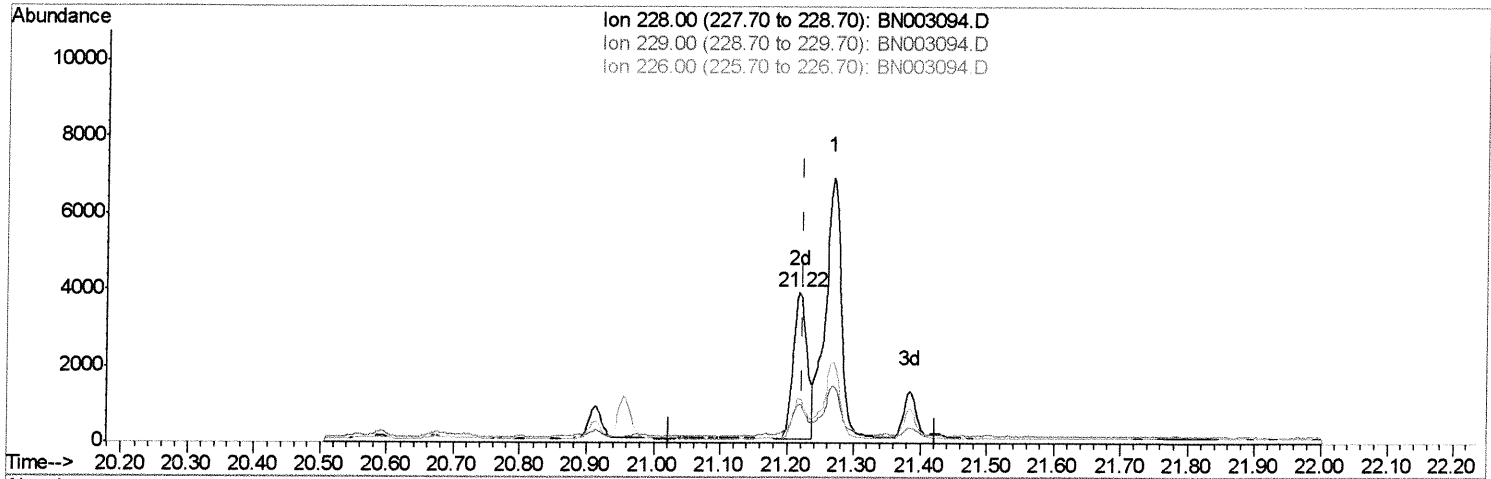

TIC: BN003094.D

(18) Benzo(a)anthracene

21.217min (-0.006) 0.39ng/ul m

response 5730

Ion Exp% Act%

228.00 100 100

229.00 20.20 25.62#

226.00 27.90 29.38

0.00 0.00 0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101118\
Data File : BN003094.D
Acq On : 11 Oct 2018 09:14
Operator : MJ/SJ
Sample : J5157-16DL 2X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD8DL

Manual Integrations
APPROVED

Sohil
10/11/2018 5:45:12 PM

Quant Time: Oct 11 13:36:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 08:10:30 2018
Response via : Initial Calibration

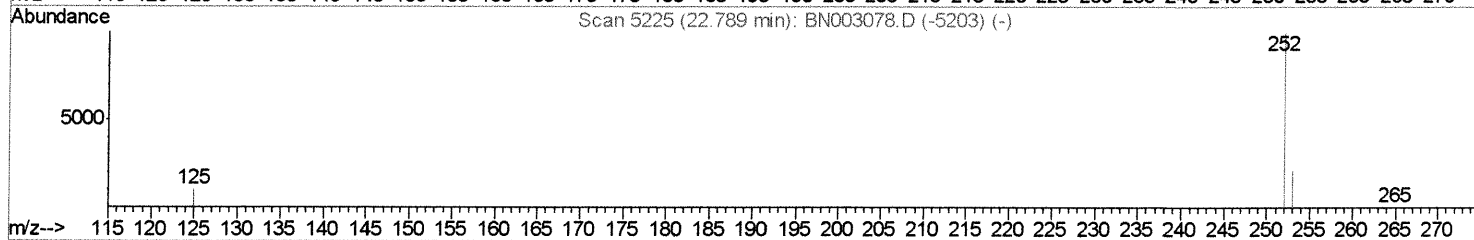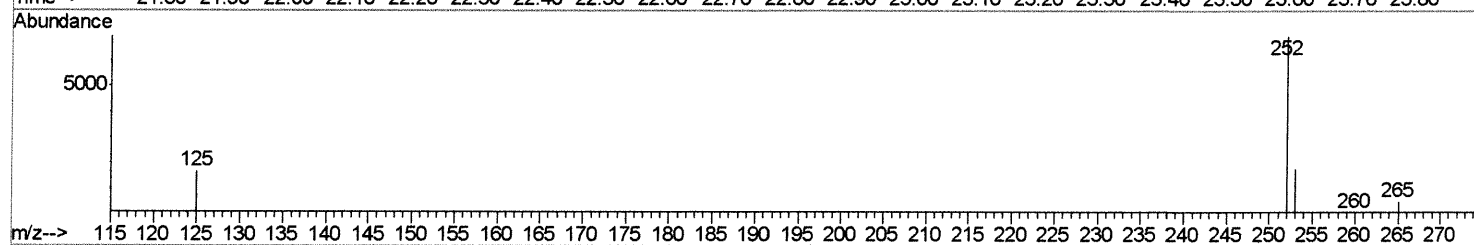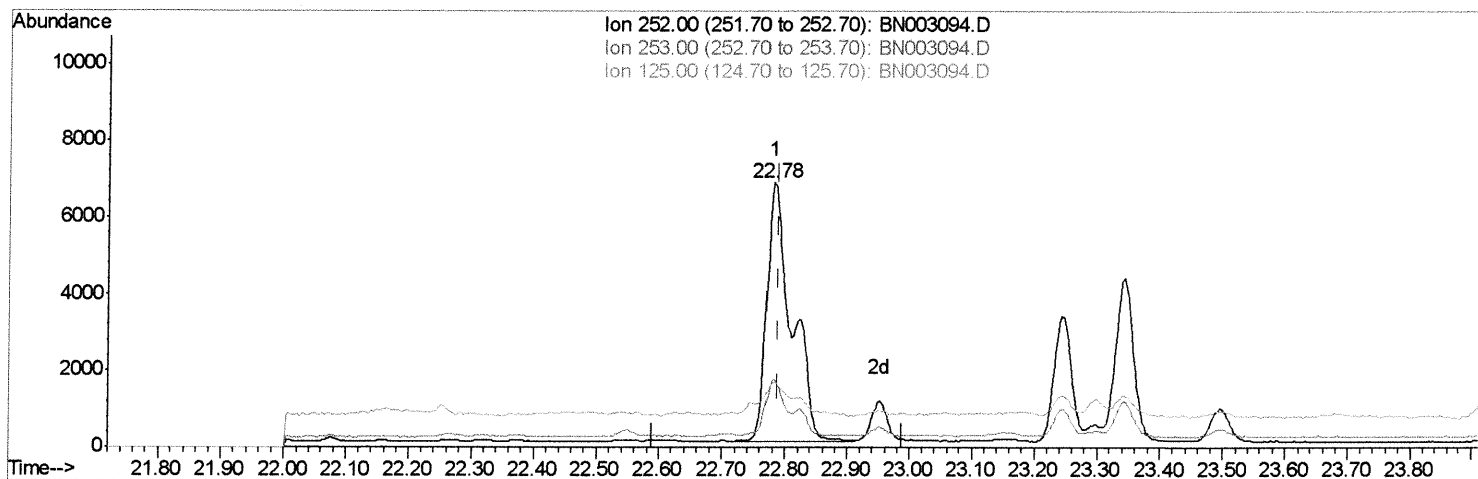

TIC: BN003094.D

(21) Benzo(b)fluoranthene

22.781min (-0.009) 1.07ng/ul

response 18587

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	26.12
125.00	17.10	24.34
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101118\
 Data File : BN003094.D
 Acq On : 11 Oct 2018 09:14
 Operator : MJ/SJ
 Sample : J5157-16DL 2X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD8DL

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:45:12 PM

Quant Time: Oct 11 13:36:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 08:10:30 2018
 Response via : Initial Calibration

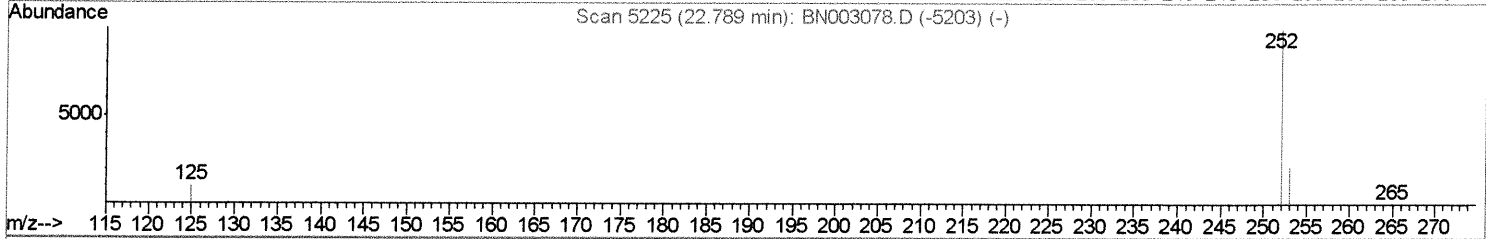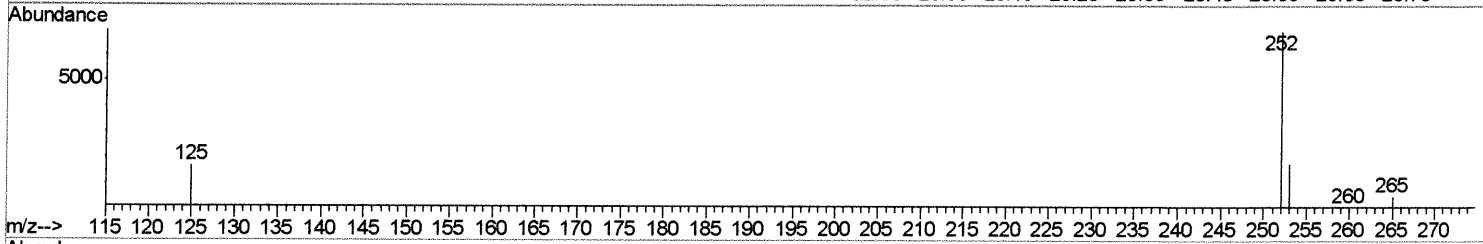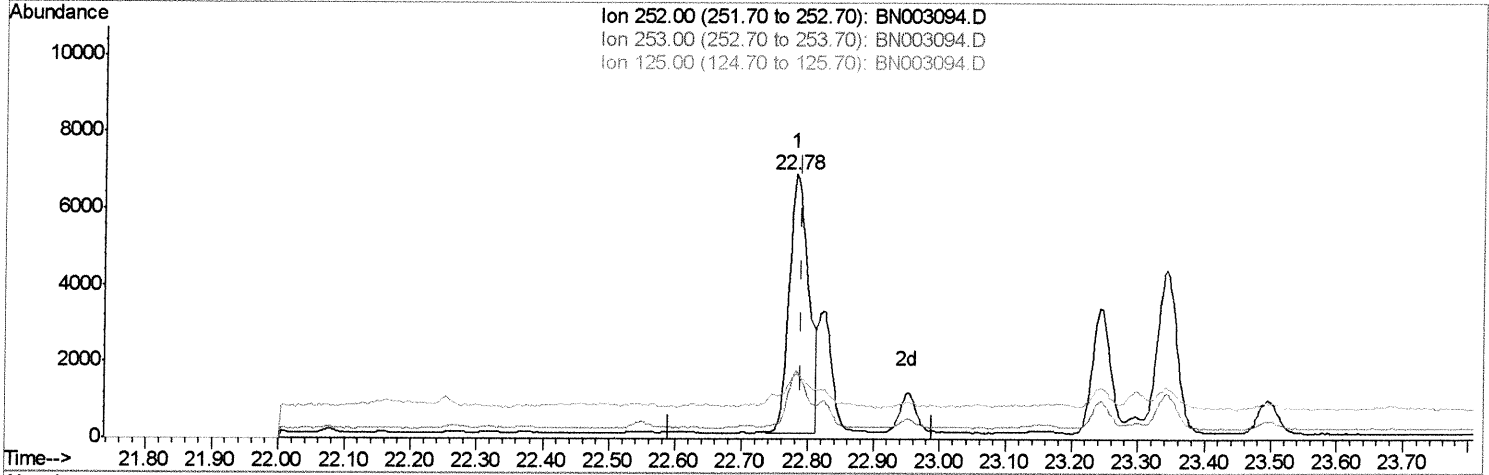

TIC: BN003094.D

(21) Benzo(b)fluoranthene

22.781min (-0.009) 0.79ng/ul m

response 13702

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	26.12
125.00	17.10	24.34
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101118\
 Data File : BN003094.D
 Acq On : 11 Oct 2018 09:14
 Operator : MJ/SJ
 Sample : J5157-16DL 2X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD8DL

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:45:12 PM

Quant Time: Oct 11 13:36:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 08:10:30 2018
 Response via : Initial Calibration

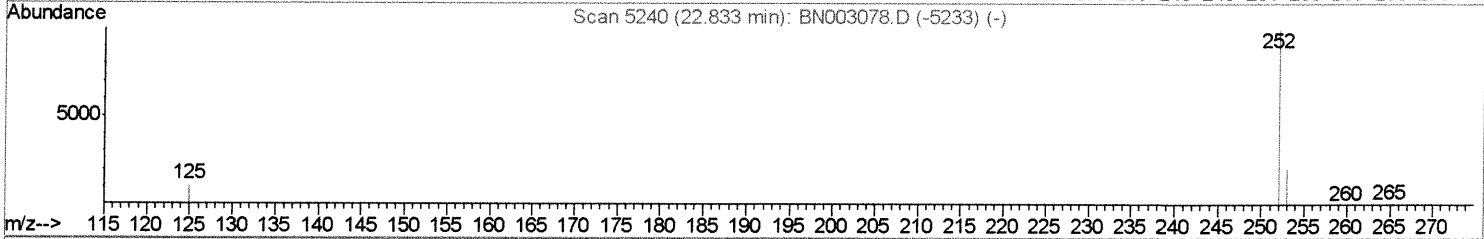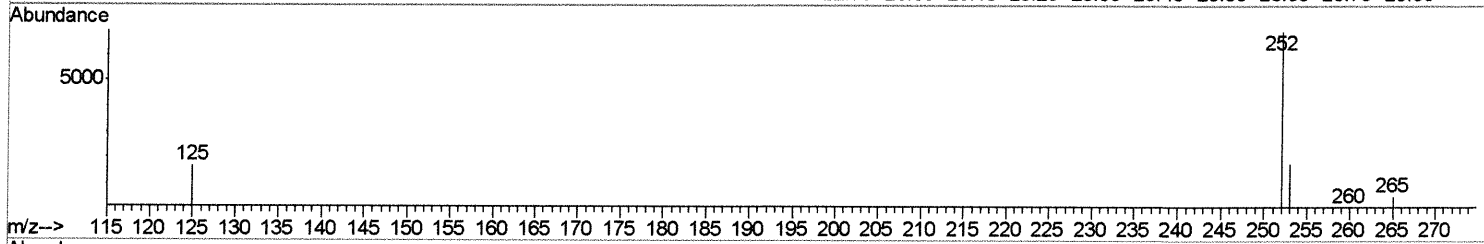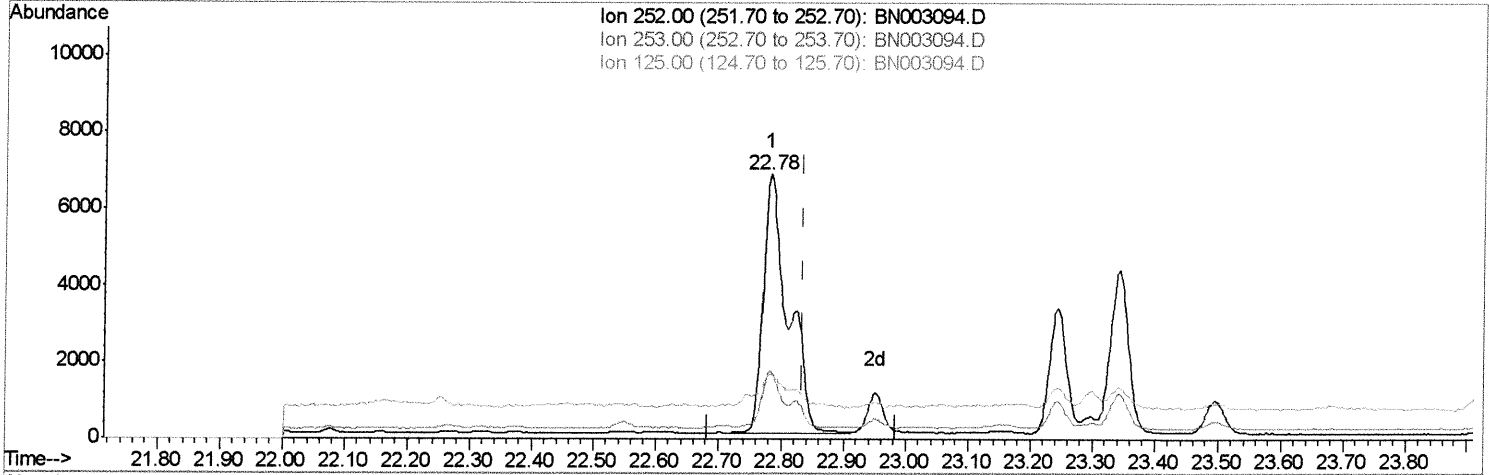

(22) Benzo(k)fluoranthene
 22.781min (-0.053) 1.03ng/ul
 response 18587

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	26.12
125.00	17.60	24.34#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101118\
 Data File : BN003094.D
 Acq On : 11 Oct 2018 09:14
 Operator : MJ/SJ
 Sample : J5157-16DL 2X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD8DL

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:45:12 PM

Quant Time: Oct 11 13:36:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 08:10:30 2018
 Response via : Initial Calibration

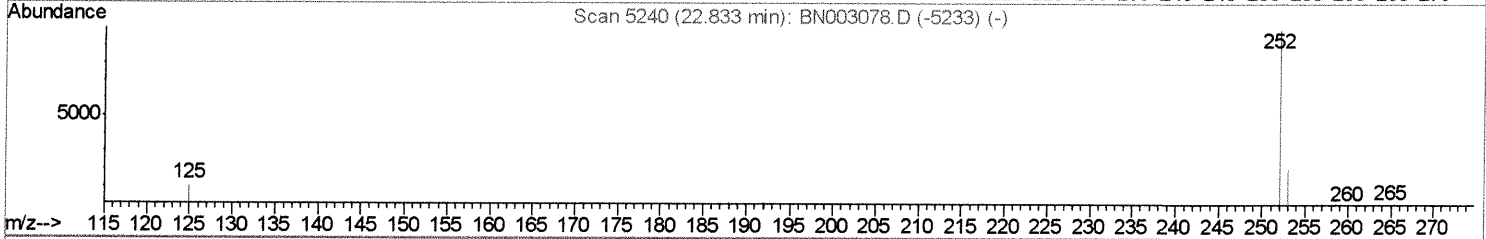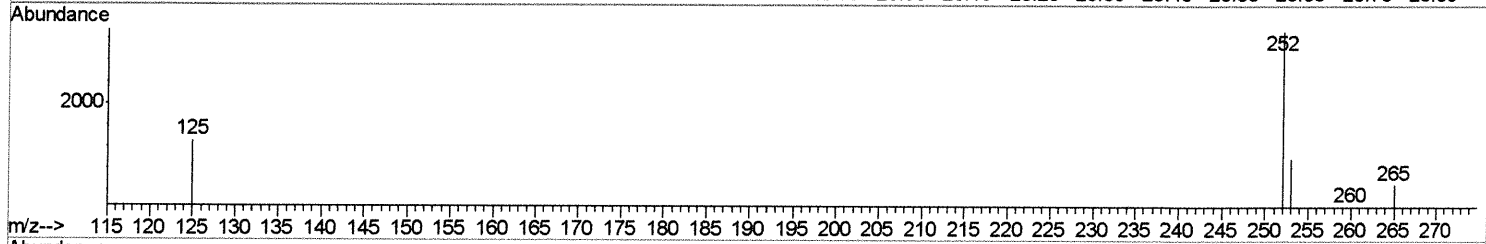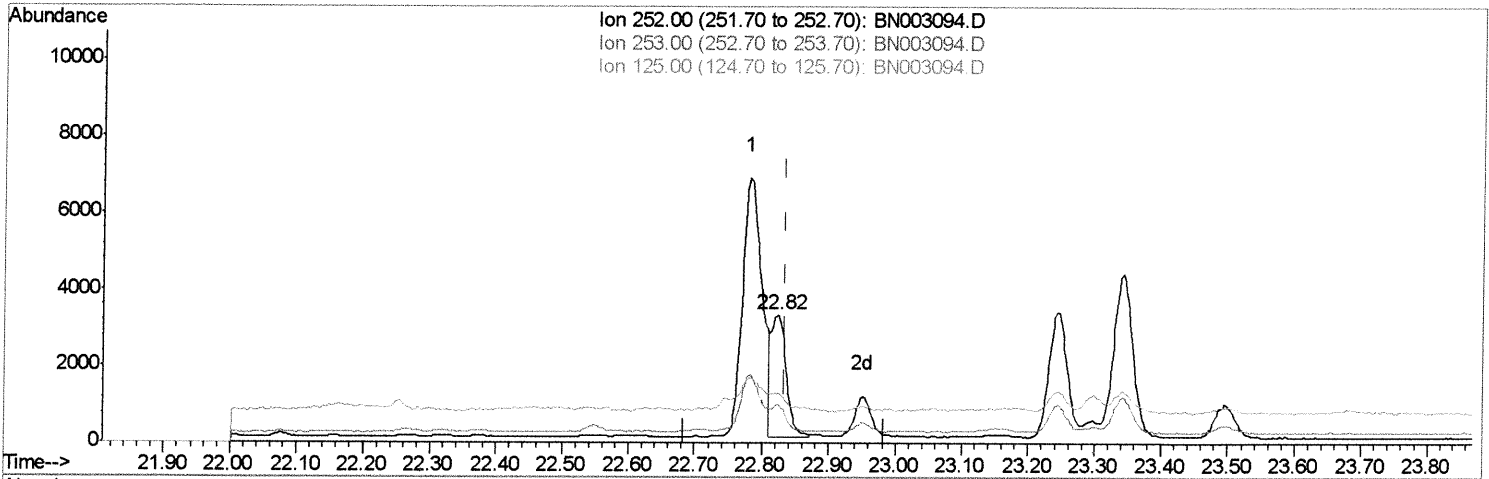

TIC: BN003094.D

(22) Benzo(k)fluoranthene

22.824min (-0.009) 0.27ng/ul m

response 4890

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	29.75
125.00	17.60	39.19#
0.00	0.00	0.00

JS 10/12/18

Quantitation Report (QT Reviewed)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101118\
 Data File : BN003094.D
 Acq On : 11 Oct 2018 09:14
 Operator : MJ/SJ
 Sample : J5157-16DL 2X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD8DL

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:45:12 PM

Quant Time: Oct 11 13:37:31 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN100918.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Oct 11 08:10:30 2018

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	1494	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.39	136	6209	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.26	164	3541	0.40	ng/ul	-0.01
10) Phenanthrene-d10	17.01	188	7409m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.23	240	4588m	0.40	ng/ul	0.00
20) Perylene-d12	23.44	264	4813	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.02	152	2029	0.21	ng/ul	0.00
14) Fluoranthene-d10	19.06	212	4115m	0.19	ng/ul	0.00

Target Compounds

					Qvalue	
3) Naphthalene	10.44	128	795	0.050	ng/ul#	81
7) Acenaphthylene	13.98	152	1029	0.064	ng/ul#	87
12) Phenanthrene	17.06	178	804m	0.039	ng/ul	
13) Anthracene	17.15	178	1474m	0.076	ng/ul	
15) Fluoranthene	19.09	202	11950m	0.493	ng/ul	
17) Pyrene	19.45	202	21841	1.226	ng/ul	99
18) Benzo(a)anthracene	21.22	228	5730m	0.388	ng/ul	99
19) Chrysene	21.27	228	11420	0.762	ng/ul	99
21) Benzo(b)fluoranthene	22.78	252	13702m	0.790	ng/ul	
22) Benzo(k)fluoranthene	22.82	252	4890m	0.272	ng/ul	
23) Benzo(a)pyrene	23.34	252	8596	0.553	ng/ul#	89
24) Indeno(1,2,3-cd)pyrene	25.67	276	4818	0.270	ng/ul#	93
25) Dibenzo(a,h)anthracene	25.66	278	1421	0.099	ng/ul#	25
26) Benzo(g,h,i)perylene	26.35	276	3794	0.252	ng/ul#	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed