

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101118\
 Data File : BN003086.D
 Acq On : 11 Oct 2018 04:08
 Operator : MJ/SJ
 Sample : J5230-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A3YT3

Manual Integrations
 APPROVED

Sohil
 10/11/2018 5:44:52 PM

Quant Time: Oct 11 08:50:47 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 08:10:30 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	1475	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.39	136	5928	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.26	164	3397	0.40	ng/ul	-0.01
10) Phenanthrene-d10	17.01	188	6125m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.24	240	4279m	0.40	ng/ul	0.00
20) Perylene-d12	23.44	264	3852m	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.01	152	4497	0.49	ng/ul	-0.01
14) Fluoranthene-d10	19.06	212	7300m	0.42	ng/ul	0.00
Target Compounds						
8) Acenaphthene	14.34	153	1606	0.136	ng/ul#	Ovalue 26

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101118\
Data File : BN003086.D
Acq On : 11 Oct 2018 04:08
Operator : MJ/SJ
Sample : J5230-01
Misc :
ALS Vial : 23 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
A3YT3

Manual Integrations
APPROVED

Sohil
10/11/2018 5:44:52 PM

Quant Time: Oct 11 08:50:47 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 08:10:30 2018
Response via : Initial Calibration

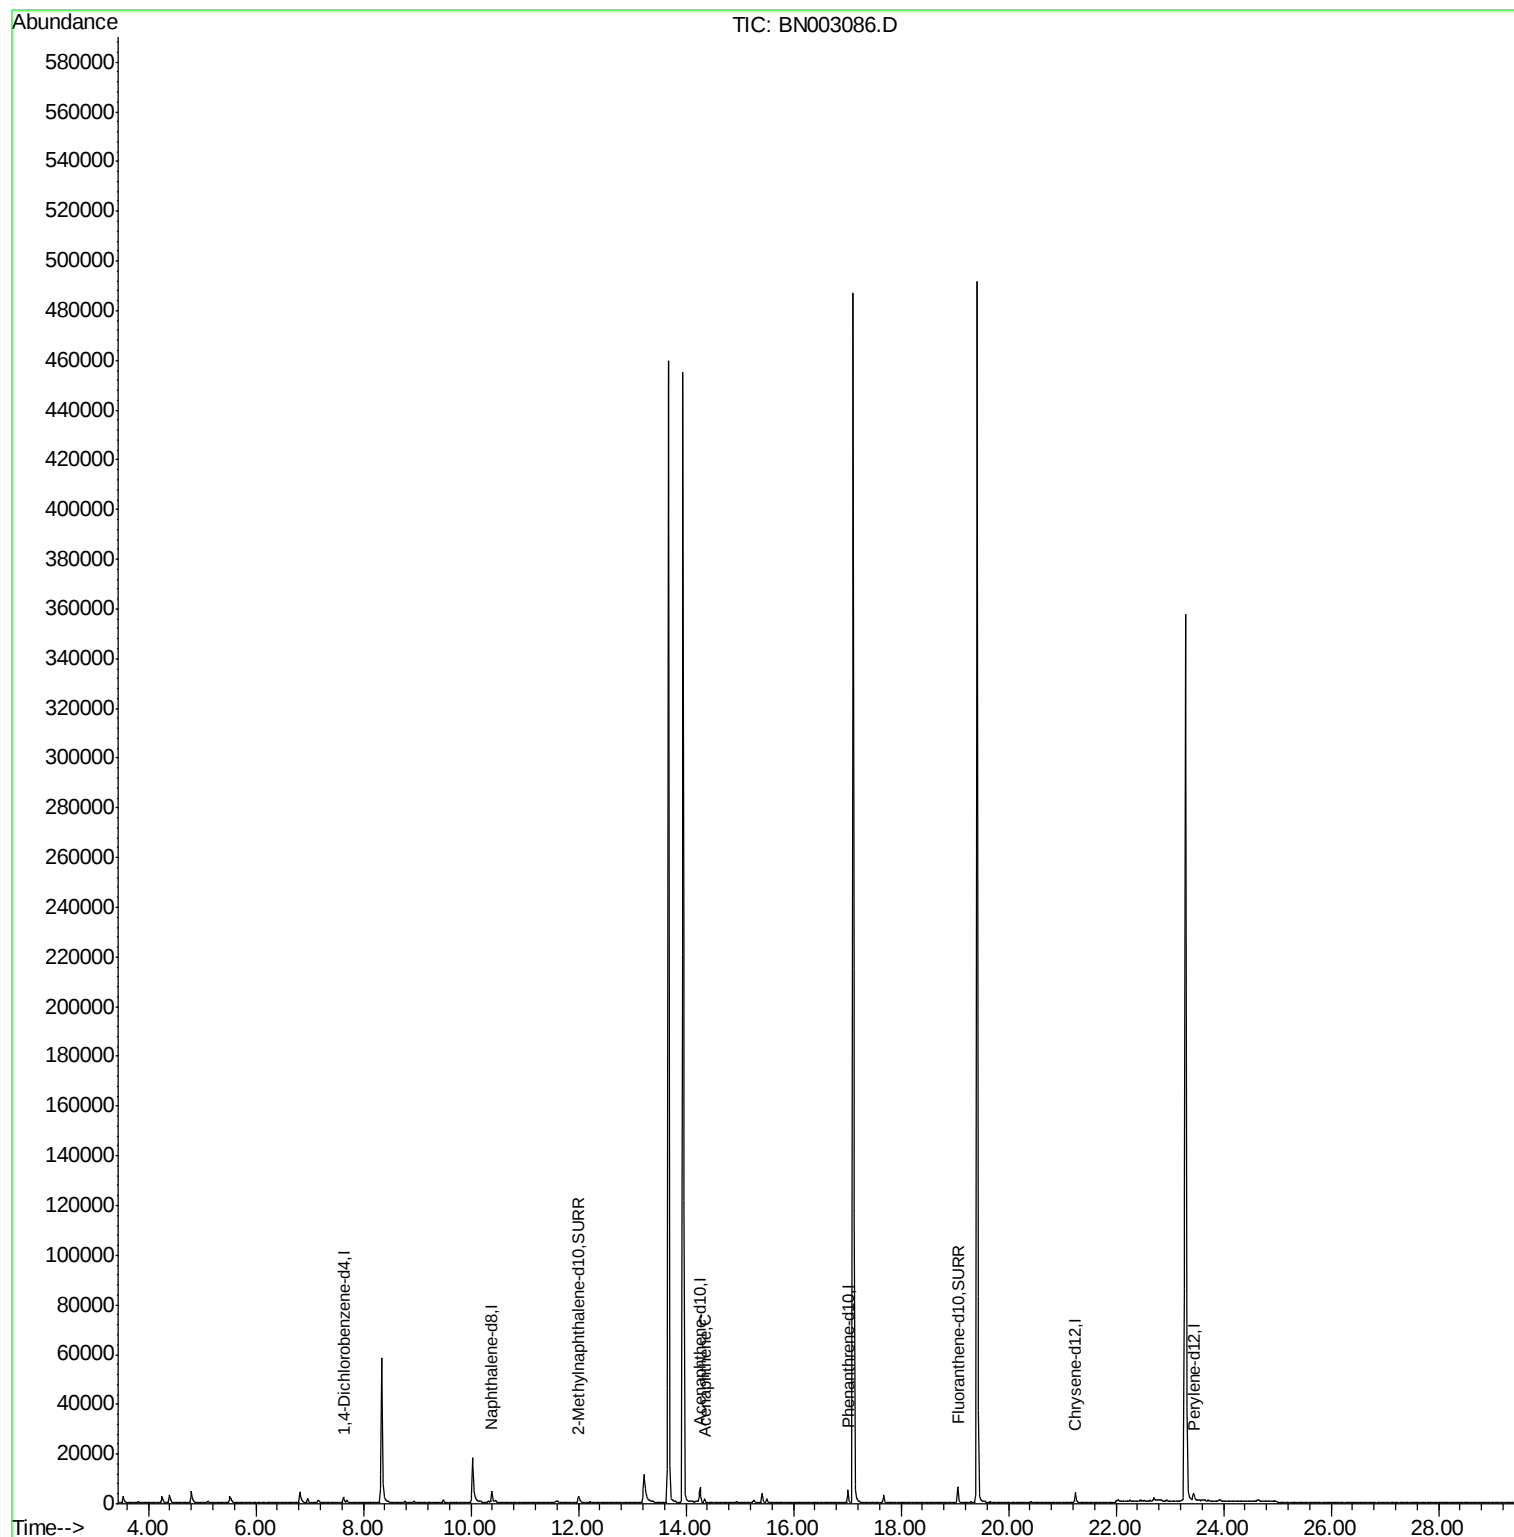

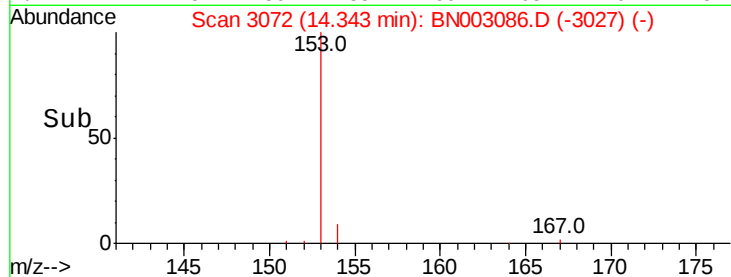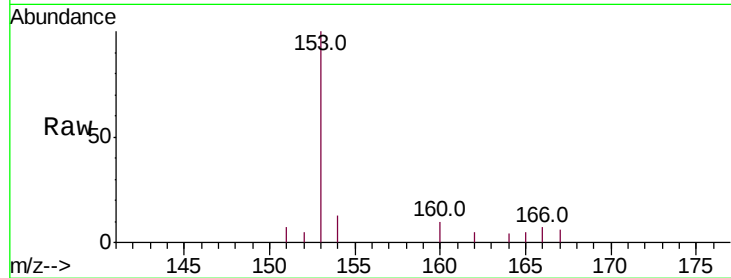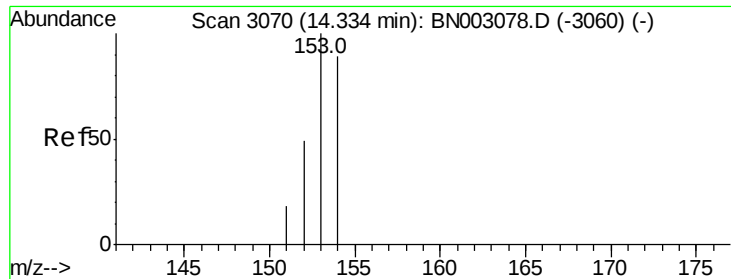

#8

Acenaphthene

Concen: 0.136 ng/ul

RT: 14.34 min Scan# 3072

Delta R.T. 0.01 min

Lab File: BN003086.D

Acq: 11 Oct 2018 04:08

Instrument :

BNA_N

ClientSampleId :

A3YT3

Tot Ion:153 Resp: 1606

Ion Ratio Lower Upper

153 100

152 5.4 38.2 57.4#

154 12.9 70.2 105.2#

Manual Integrations

APPROVED

Sohil

10/11/2018 5:44:52 PM

