

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101119\
 Data File : BN008079.D
 Acq On : 11 Oct 2019 16:07
 Operator : JU
 Sample : K5050-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Oct 11 23:16:00 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 11 19:05:54 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	3002	0.40	ng/ul	0.00
2) Naphthalene-d8	10.40	136	13810	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.26	164	9005	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.11	188	1284722	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.22
20) Perylene-d12	23.40	264	26176	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.00	152	5809	0.25	ng/ul	0.00
14) Fluoranthene-d10	19.12	212	431	0.00	ng/ul	0.07
Target Compounds						
23) Benzo(a)pyrene	23.26	252	5419	0.060	ng/ul#	Ovalue 70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101119\
Data File : BN008079.D
Acq On : 11 Oct 2019 16:07
Operator : JU
Sample : K5050-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Oct 11 23:16:00 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 11 19:05:54 2019
Response via : Initial Calibration

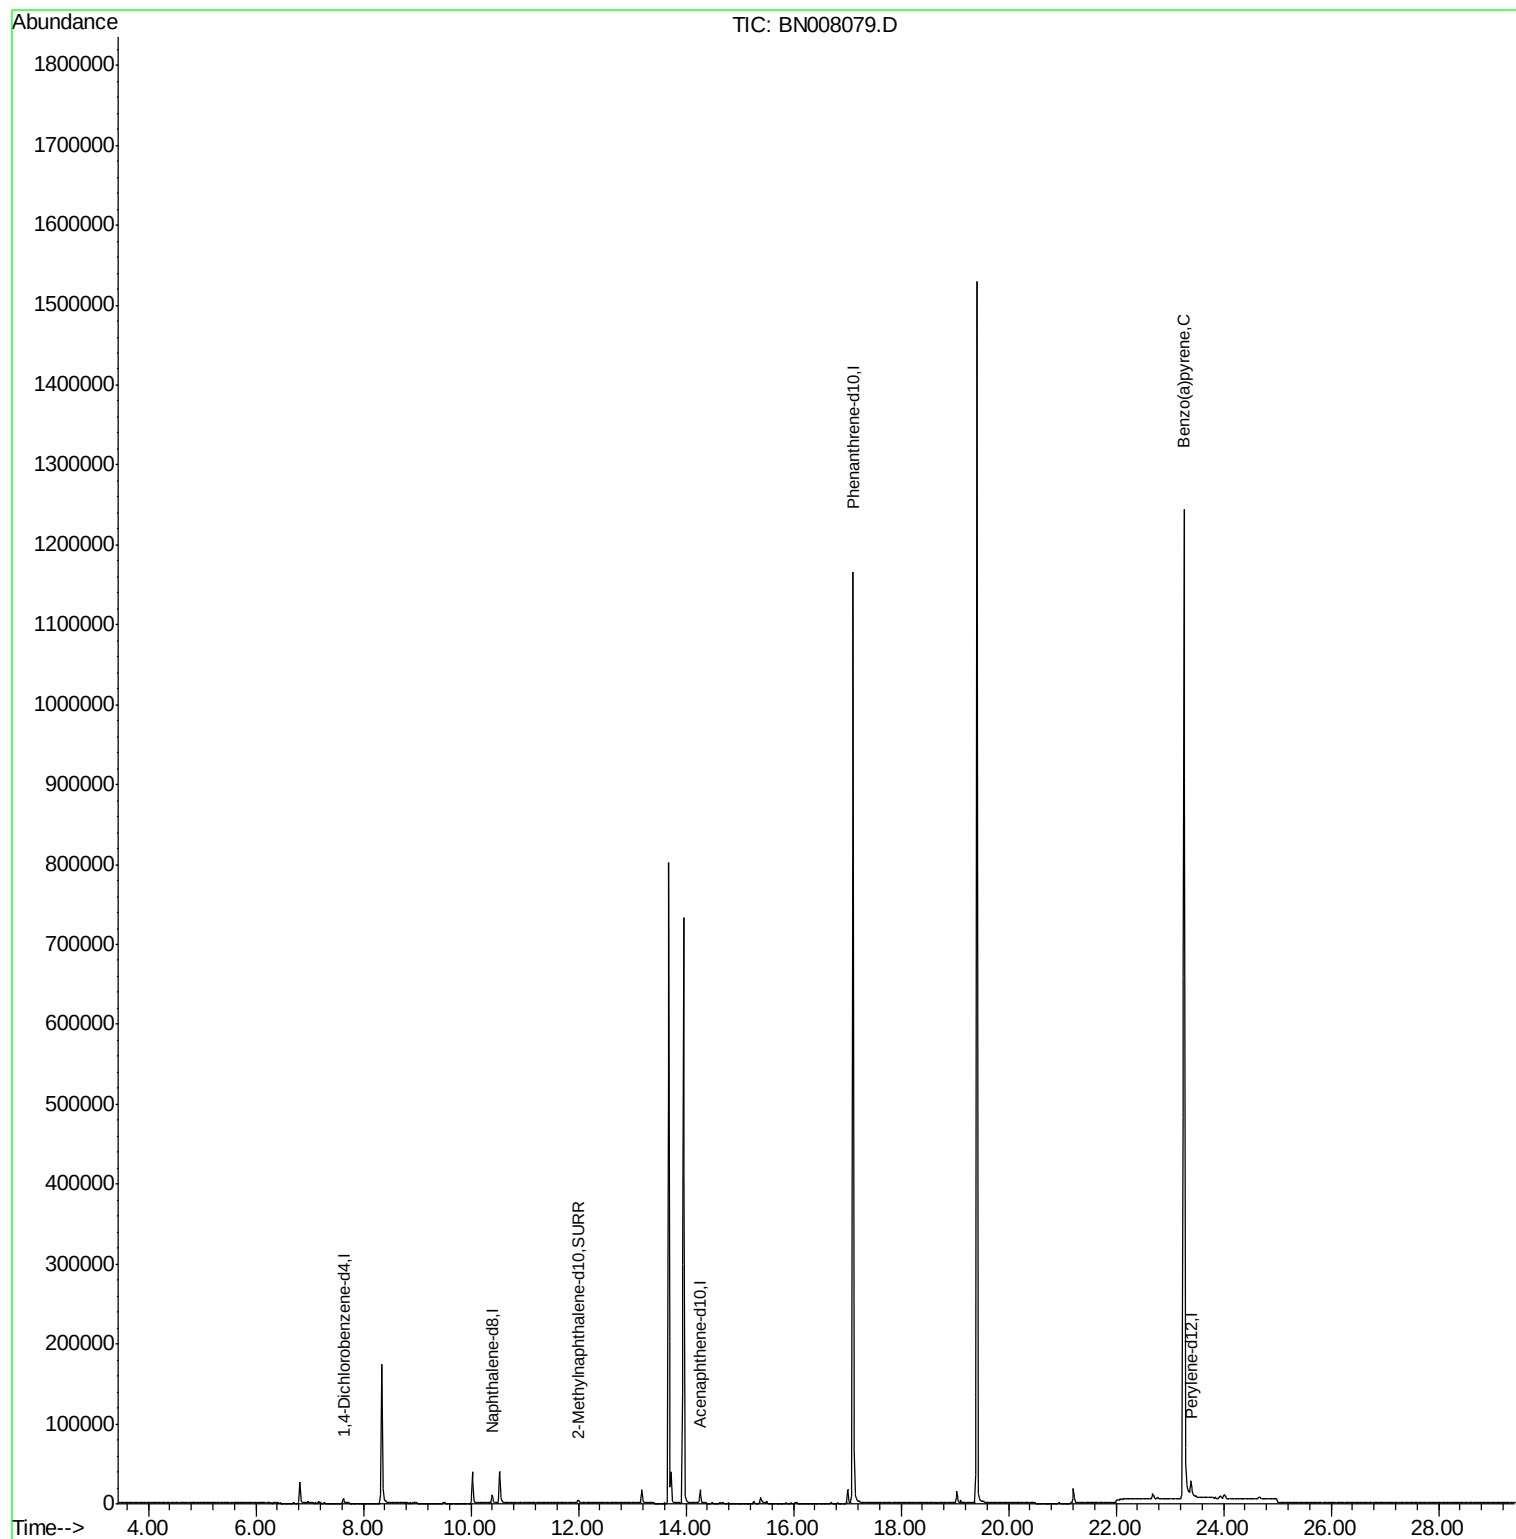

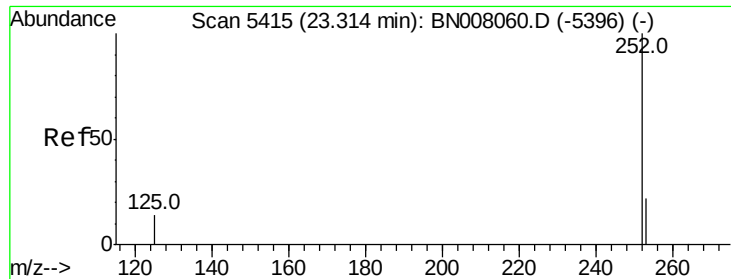

#23

Benzo(a)pyrene

Concen: 0.060 ng/ul

RT: 23.26 min Scan# 5397

Delta R.T. -0.05 min

Lab File: BN008079.D

Acq: 11 Oct 2019 16:07

Instrument :

BNA_N

ClientSampleId :


Tot Ion:252 Resp: 5419

Ion Ratio Lower Upper

252 100

253 42.8 22.8 34.2#

125 38.9 18.4 27.6#

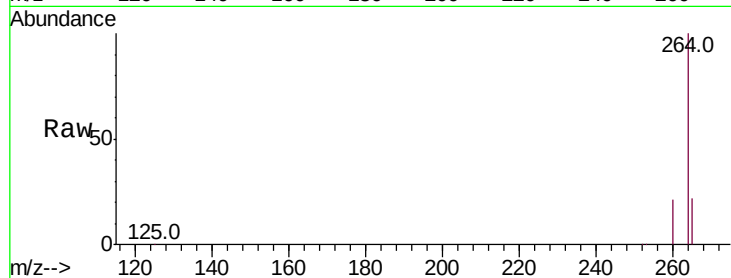

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

