

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101119\
 Data File : BN008087.D
 Acq On : 11 Oct 2019 20:53
 Operator : JU
 Sample : K5050-18
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Oct 11 23:16:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 11 19:05:54 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	2413	0.40	ng/ul	0.00
2) Naphthalene-d8	10.40	136	11018	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.26	164	7093	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.11	188	975572	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.22
20) Perylene-d12	23.40	264	22719	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.00	152	4455	0.24	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
3) Naphthalene	10.44	128	845	0.027	ng/ul#	74
5) 2-Methylnaphthalene	12.07	142	800	0.037	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101119\
Data File : BN008087.D
Acq On : 11 Oct 2019 20:53
Operator : JU
Sample : K5050-18
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Oct 11 23:16:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 11 19:05:54 2019
Response via : Initial Calibration

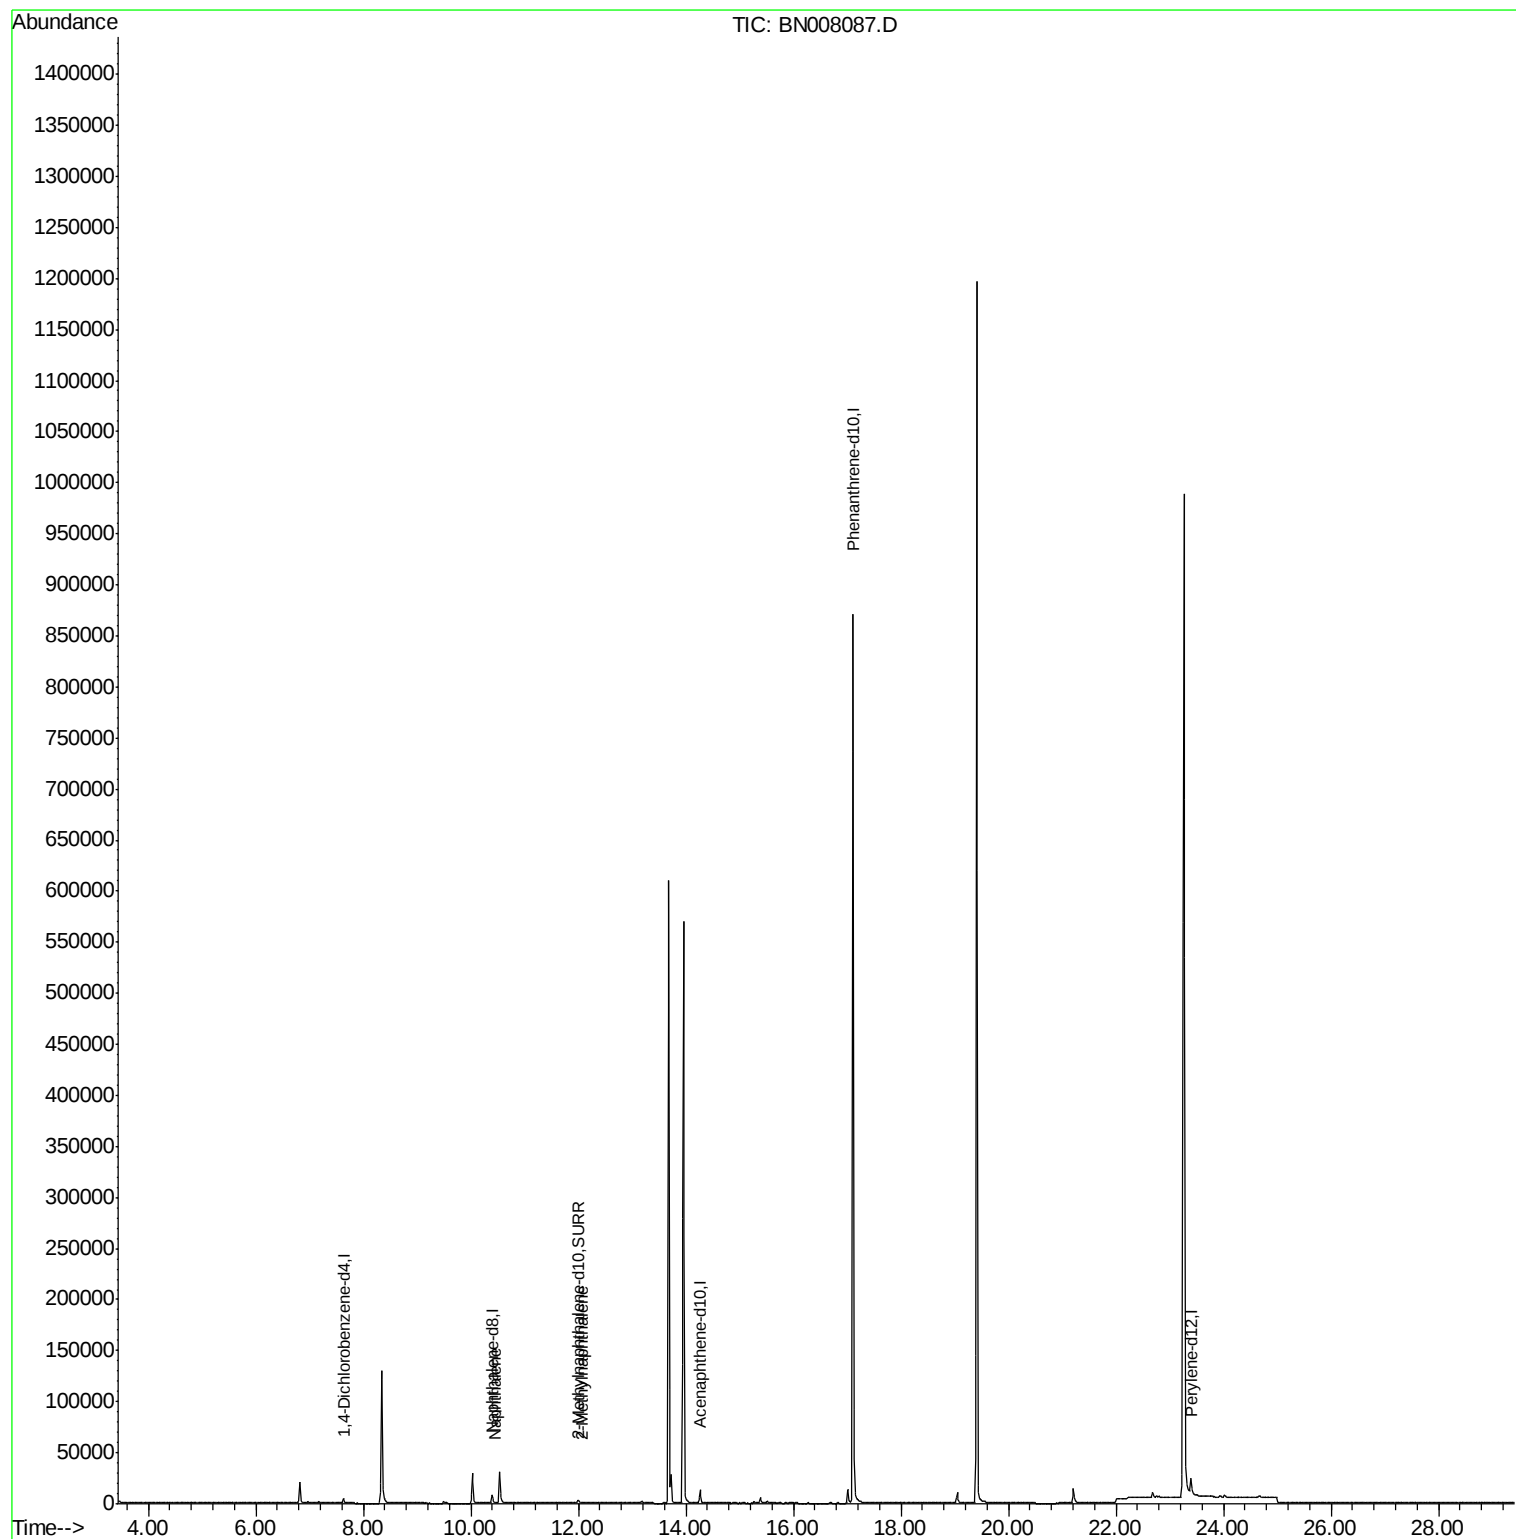

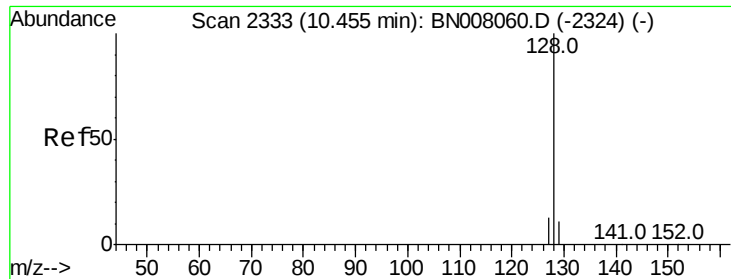

#3

Naphthalene

Concen: 0.027 ng/ul

RT: 10.44 min Scan# 2331

Delta R.T. -0.01 min

Lab File: BN008087.D

Acq: 11 Oct 2019 20:53

Instrument :

BNA_N

ClientSampleId :


Tot Ion:128 Resp: 845

Ion Ratio Lower Upper

128 100

129 25.7 9.8 14.8#




127 21.8 11.1 16.7#

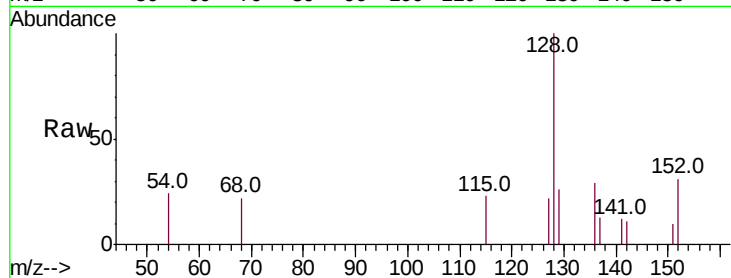

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

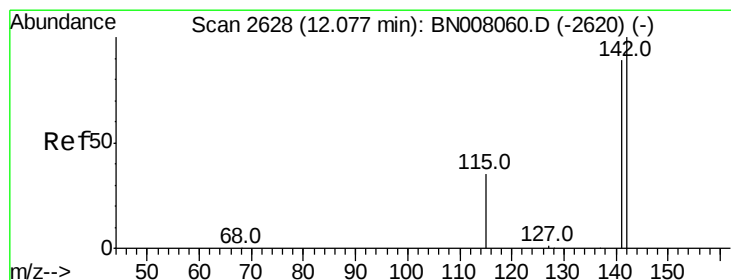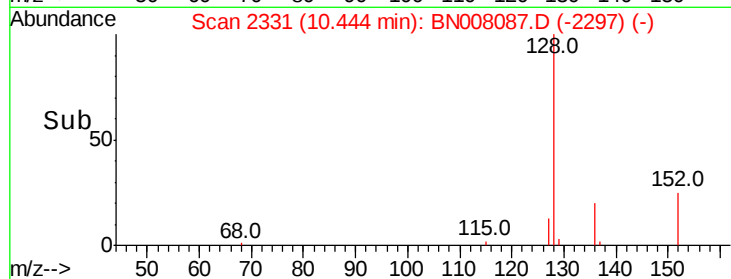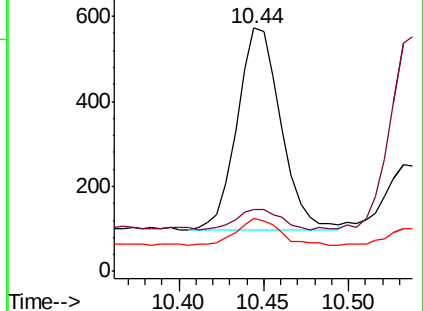

#5

2-Methylnaphthalene

Concen: 0.037 ng/ul

RT: 12.07 min Scan# 2627

Delta R.T. -0.01 min

Lab File: BN008087.D


Acq: 11 Oct 2019 20:53

Tgt Ion:142 Resp: 800

Ion Ratio Lower Upper

142 100

141 93.4 71.4 107.2

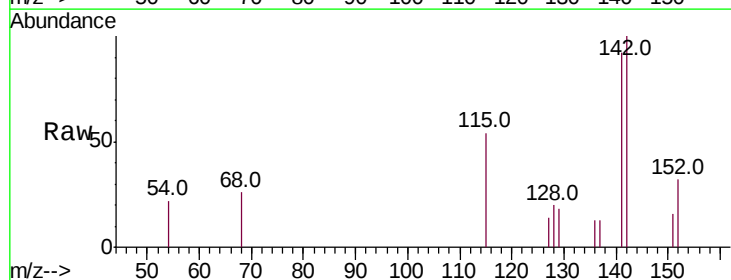

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

