

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101119\
 Data File : BN008128.D
 Acq On : 13 Oct 2019 01:30
 Operator : JU
 Sample : K5178-19
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Oct 14 01:02:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 11 19:05:54 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	2699	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.39	136	13242	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.26	164	8611	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.11	188	854249	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.22
20) Perylene-d12	23.39	264	18792	0.40	ng/ul	-0.02
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.99	152	3419	0.15	ng/ul	-0.01
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.25	252	2568	0.040	ng/ul#	Ovalue 42


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101119\
Data File : BN008128.D
Acq On : 13 Oct 2019 01:30
Operator : JU
Sample : K5178-19
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Oct 14 01:02:16 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 11 19:05:54 2019
Response via : Initial Calibration

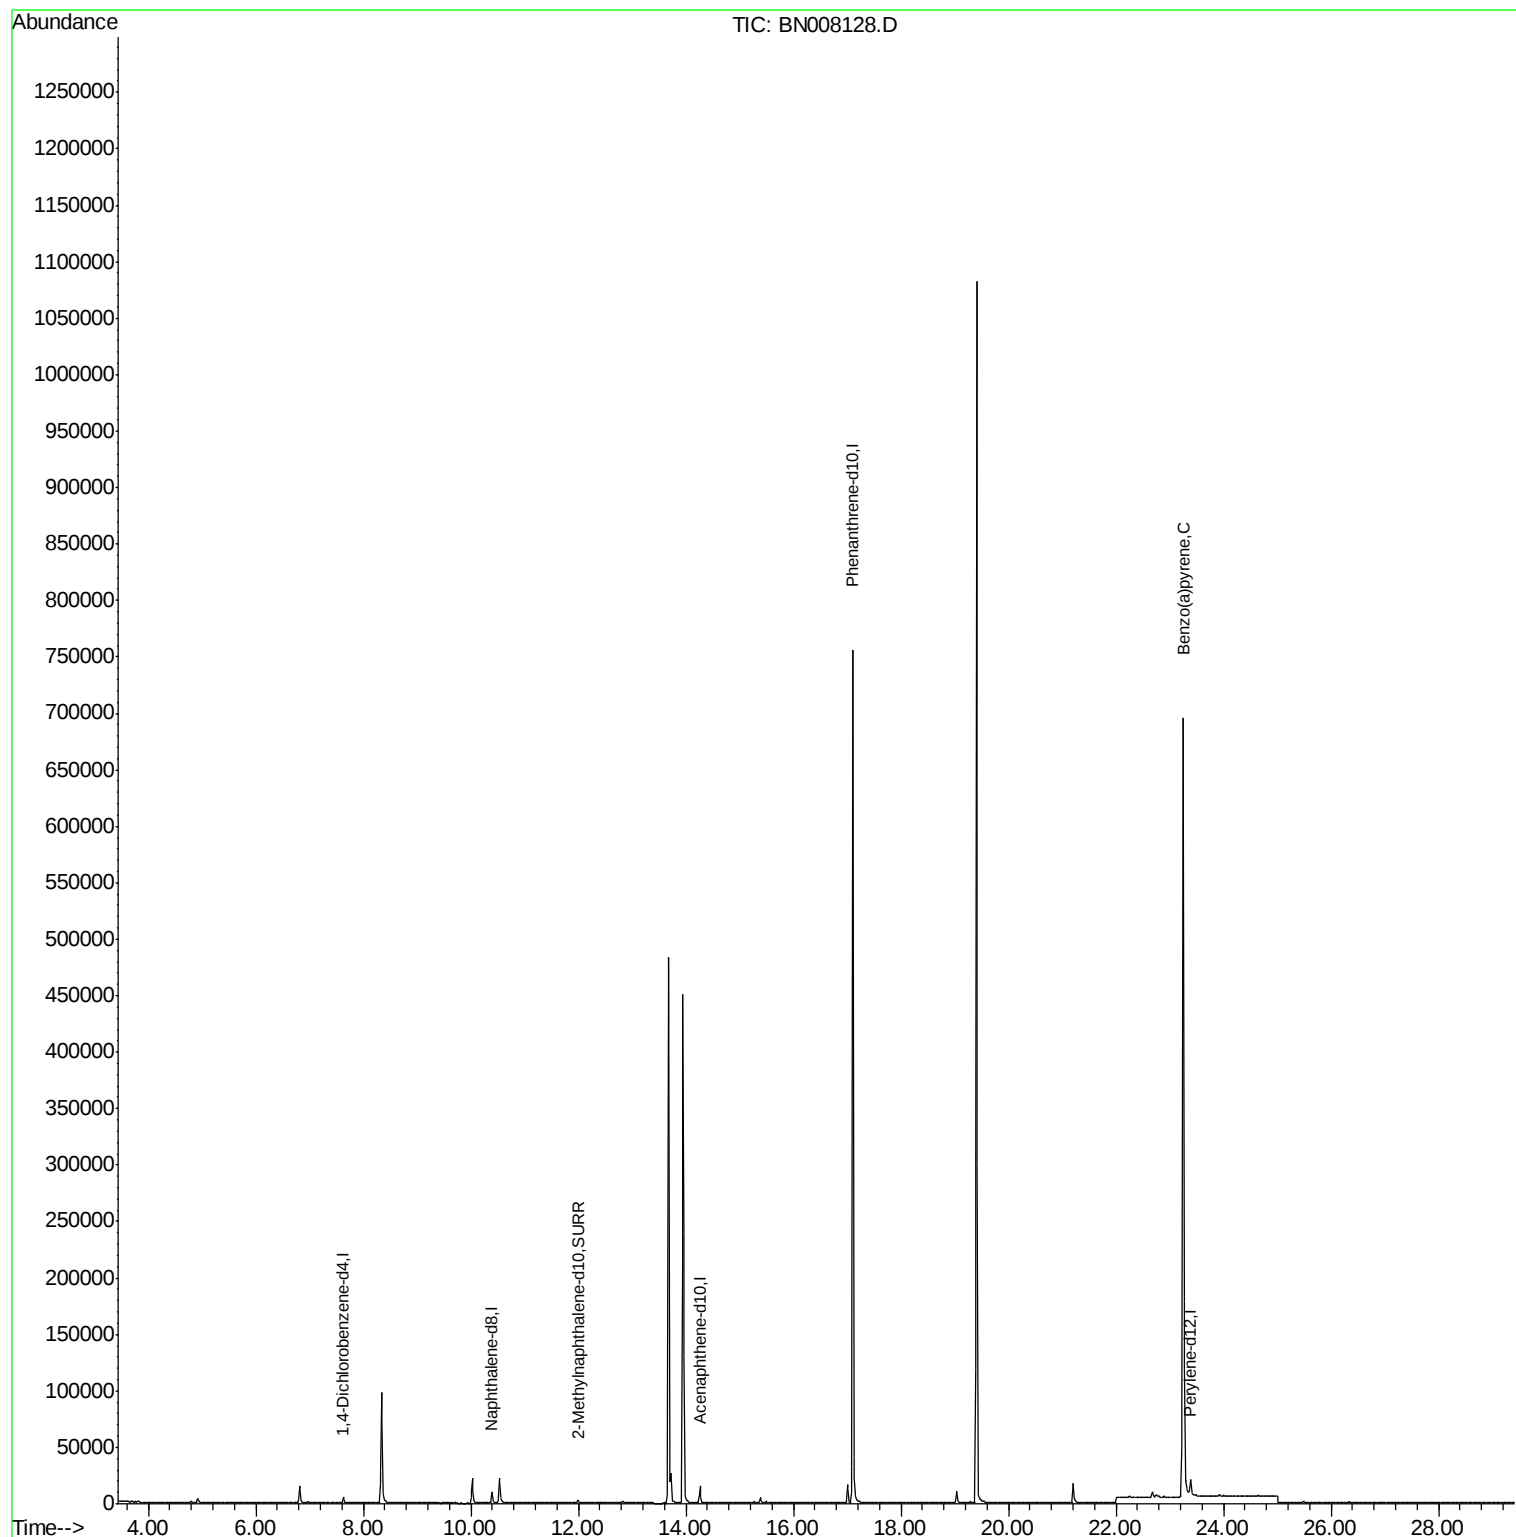

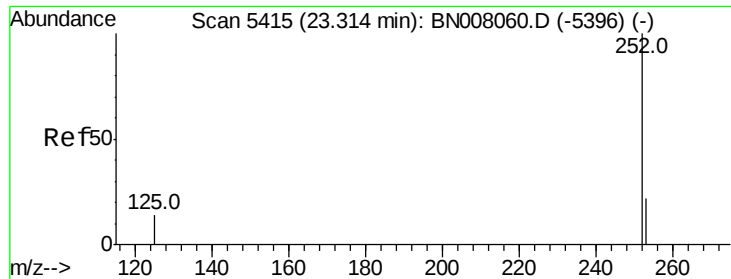

#23

Benzo(a)pyrene

Concen: 0.040 ng/ul

RT: 23.25 min Scan# 5393

Delta R.T. -0.06 min


Lab File: BN008128.D

Acq: 13 Oct 2019 01:30

Instrument :

BNA_N

ClientSampleId :

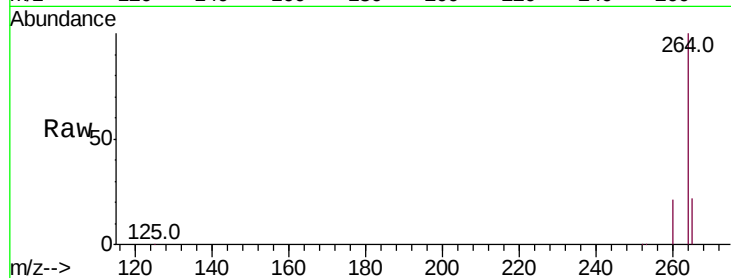

Tot Ion: 252 Resp: 2568

Ion Ratio Lower Upper

252 100

253 54.0 22.8 34.2#

125 56.6 18.4 27.6#

