


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101119\
Data File : BN008097.D
Acq On : 12 Oct 2019 04:01
Operator : JU
Sample : K5124-08
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLM78

Manual Integrations
APPROVED

mohammad
10/15/2019 7:57:55 AM

Quant Time: Oct 14 15:29:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 11 19:05:54 2019
Response via : Initial Calibration

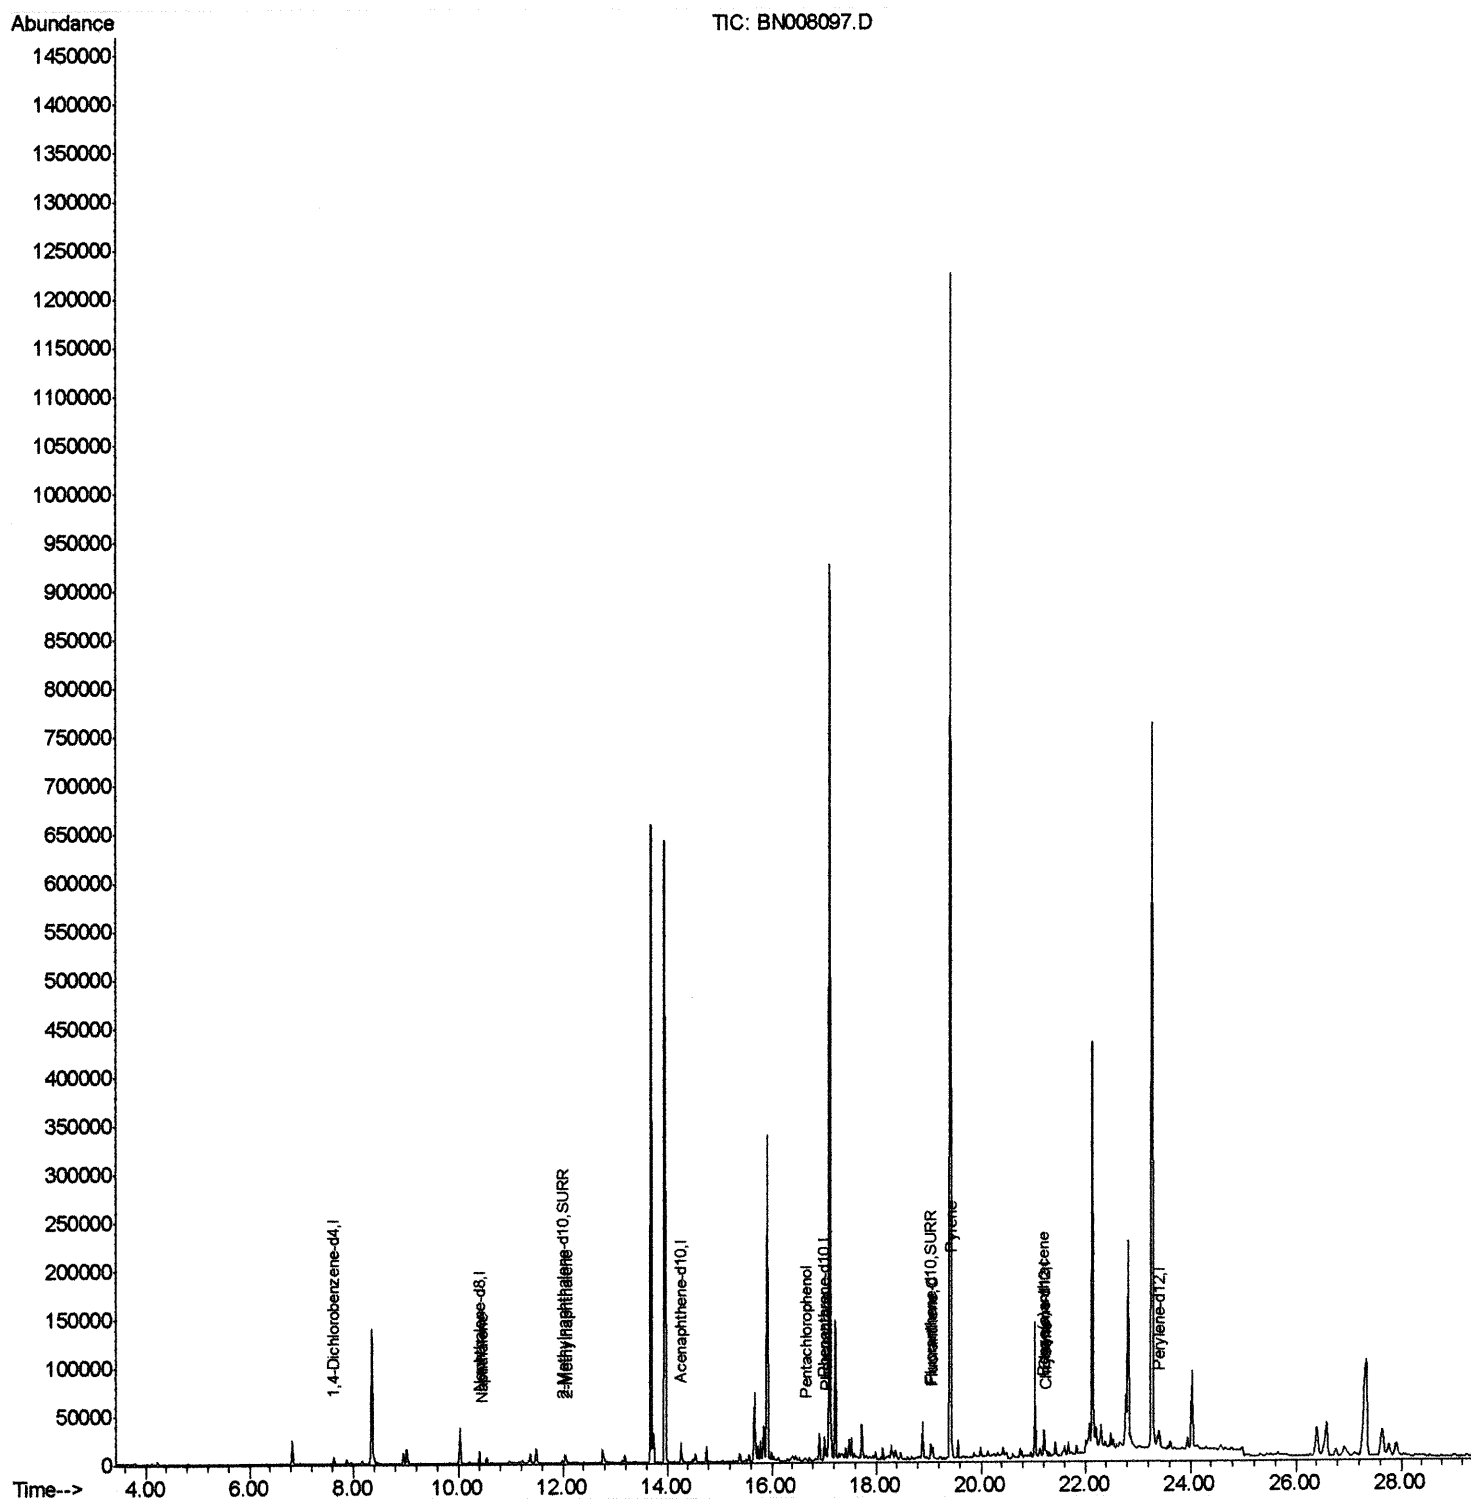

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101119\
 Data File : BN008097.D
 Acq On : 12 Oct 2019 04:01
 Operator : JU
 Sample : K5124-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLM78

Manual Integrations
 APPROVED

mohammad
 10/15/2019 7:57:55 AM

Quant Time: Oct 14 15:25:31 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 11 19:05:54 2019
 Response via : Initial Calibration

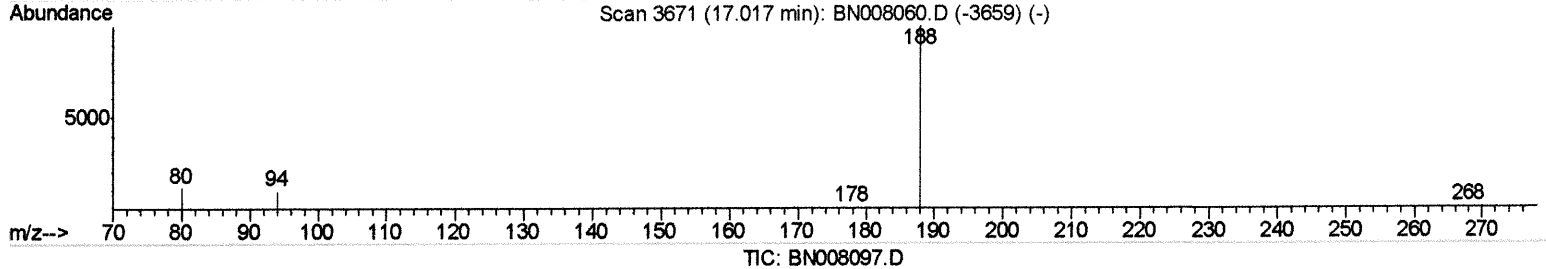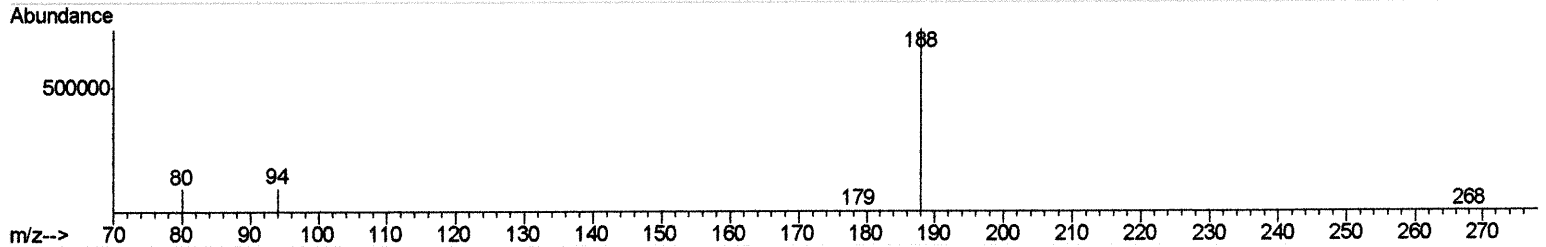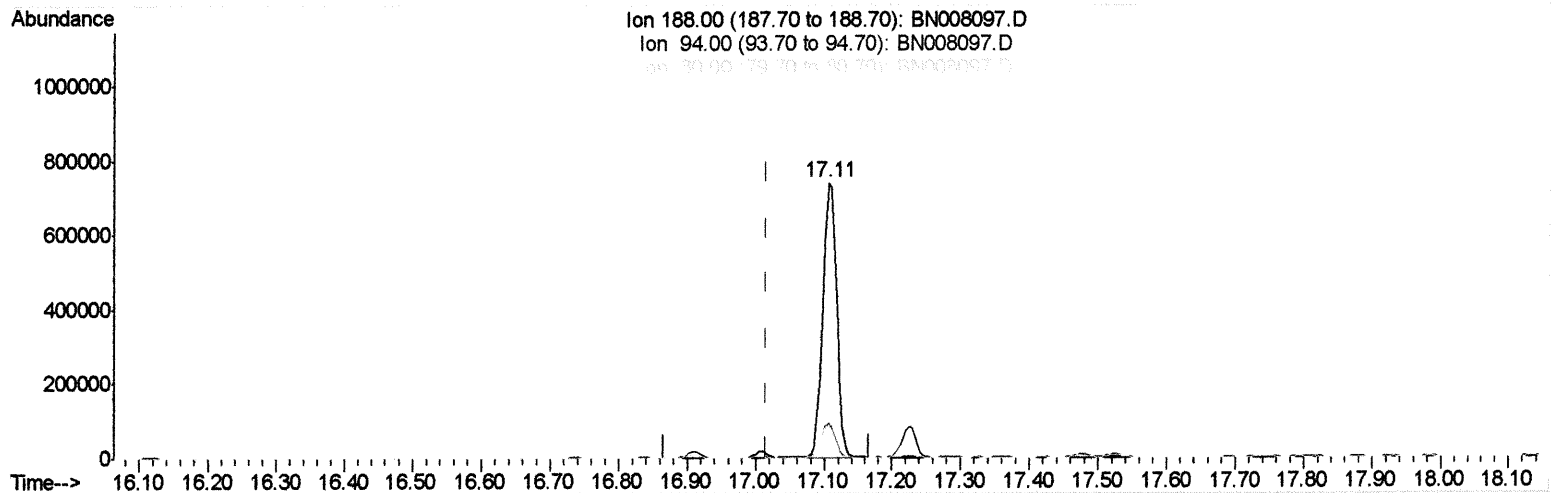

TIC: BN008097.D

(10) Phenanthrene-d10 (I)
 17.106min (+0.089) 0.40ng/ul
 response 1036674

Ion	Exp%	Act%
188.00	100	100
94.00	10.90	12.66
80.00	12.60	12.22
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101119\
 Data File : BN008097.D
 Acq On : 12 Oct 2019 04:01
 Operator : JU
 Sample : K5124-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLM78

Manual Integrations
 APPROVED

mohammad
 10/15/2019 7:57:55 AM

Quant Time: Oct 14 15:25:31 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 11 19:05:54 2019
 Response via : Initial Calibration

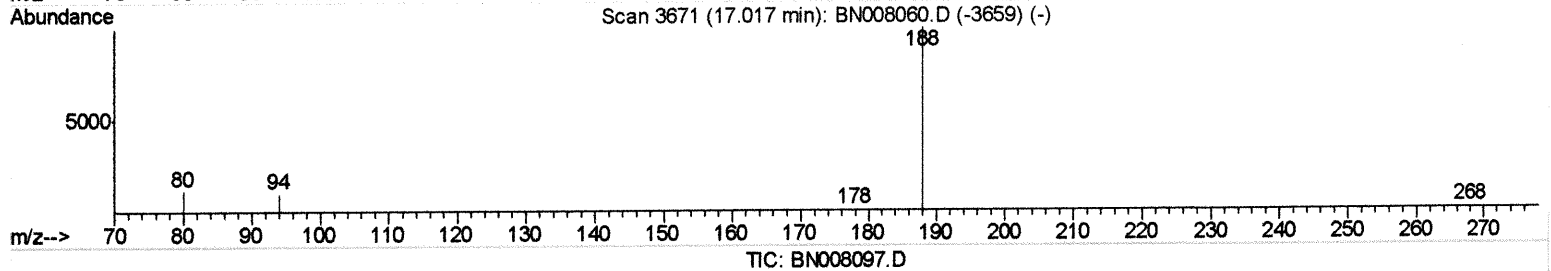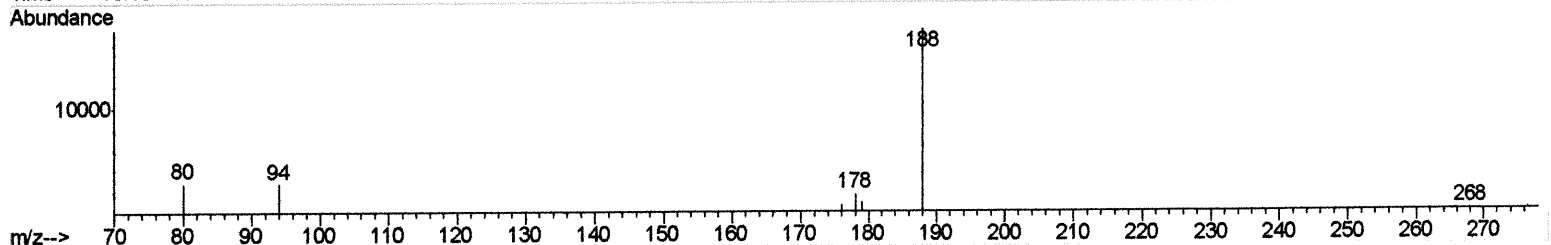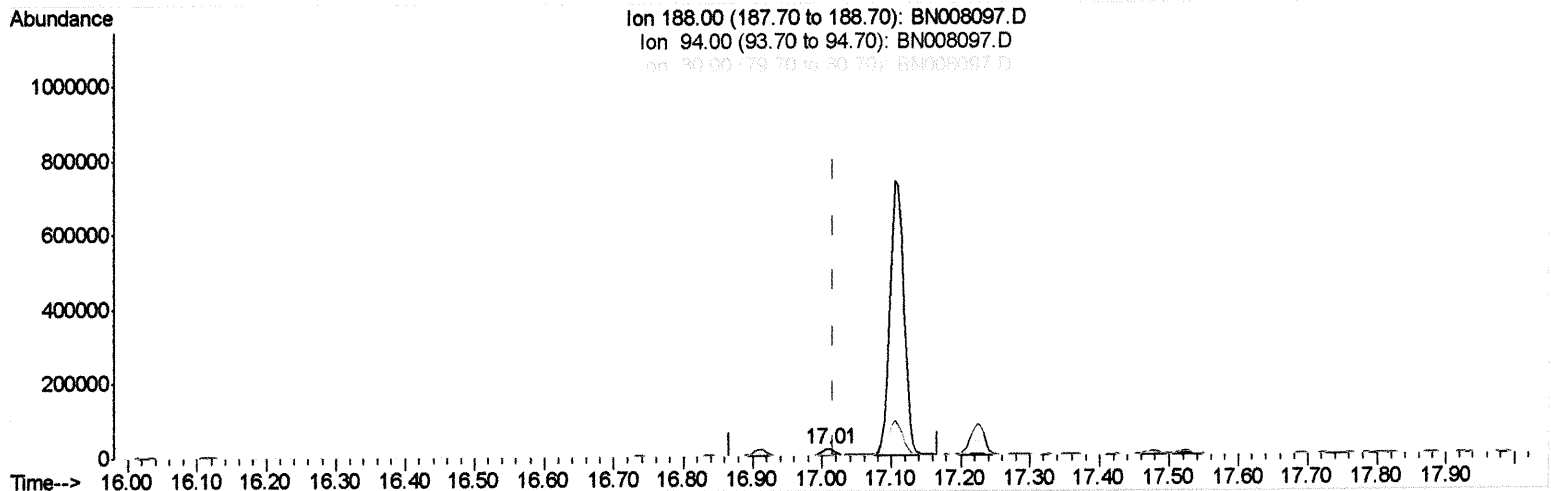

(10) Phenanthrene-d10 (I)

17.009min (-0.008) 0.40ng/ul m

Re 10/16/19

response 24310

Ion	Exp%	Act%
188.00	100	100
94.00	10.90	15.85#
80.00	12.60	16.11#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101119\
 Data File : BN008097.D
 Acq On : 12 Oct 2019 04:01
 Operator : JU
 Sample : K5124-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLM78

Manual Integrations
 APPROVED

mohammad
 10/15/2019 7:57:55 AM

Quant Time: Oct 14 15:26:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 11 19:05:54 2019
 Response via : Initial Calibration

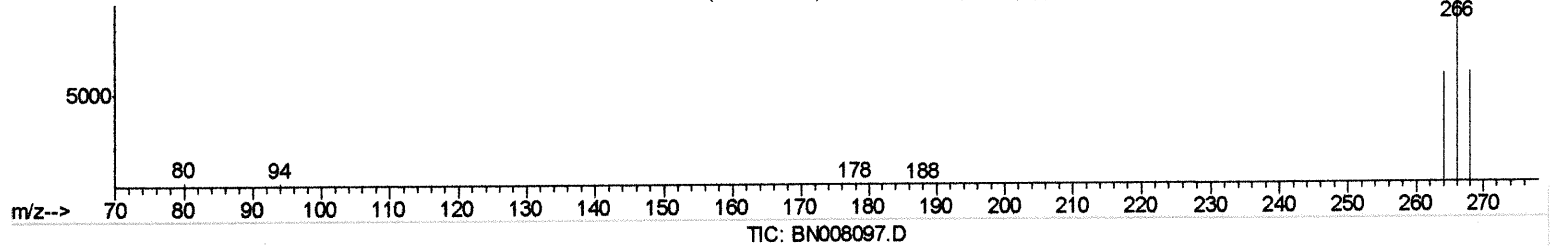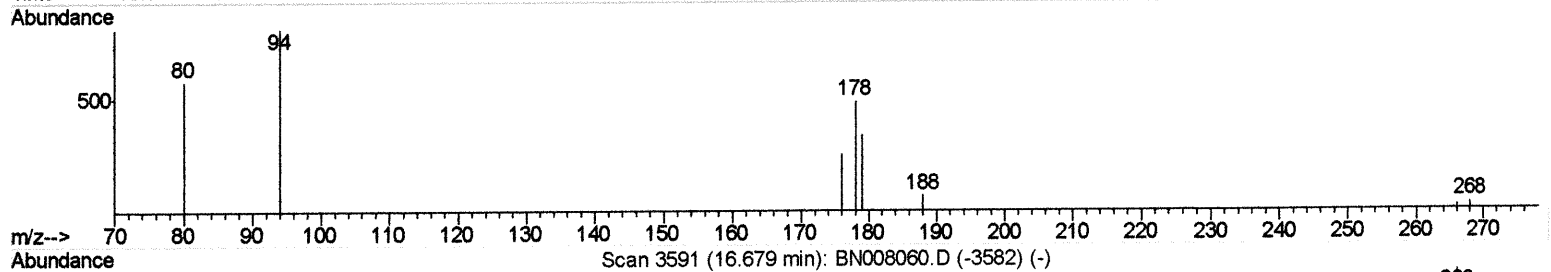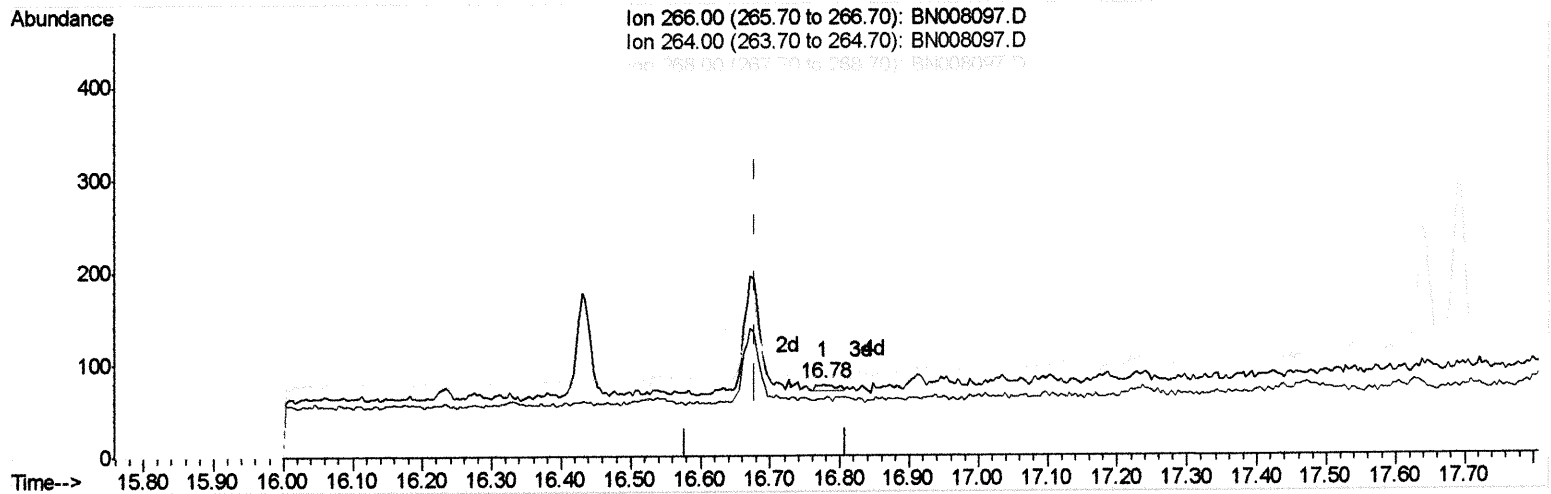

(11) Pentachlorophenol

16.776min (+0.097) 0.00ng/ul

response 13

Ion	Exp%	Act%
266.00	100	100
264.00	62.60	46.15#
268.00	64.90	30.77#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101119\
 Data File : BN008097.D
 Acq On : 12 Oct 2019 04:01
 Operator : JU
 Sample : K5124-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLM78

Manual Integrations
 APPROVED

mohammad
 10/15/2019 7:57:55 AM

Quant Time: Oct 14 15:26:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 11 19:05:54 2019
 Response via : Initial Calibration

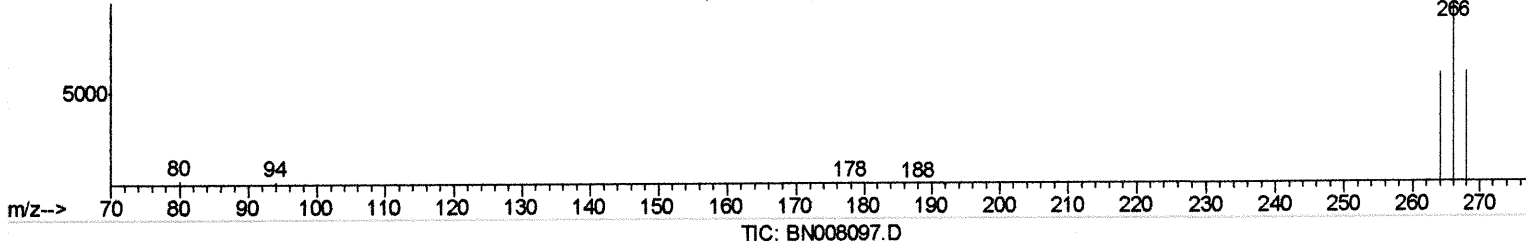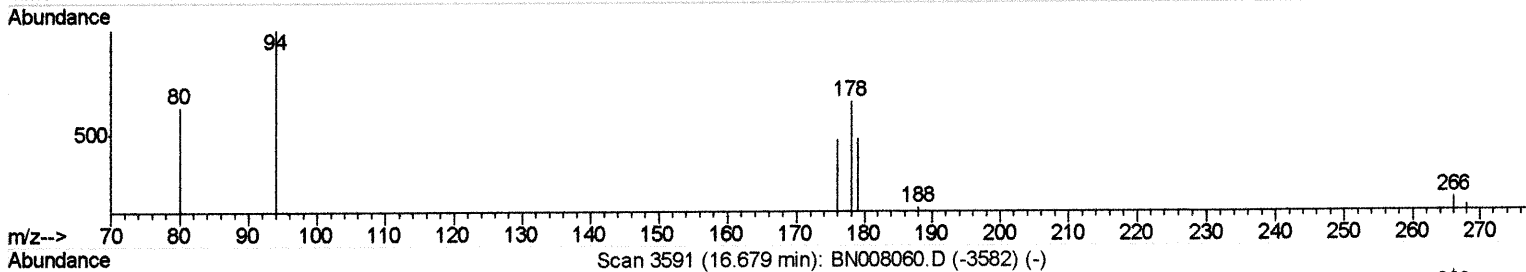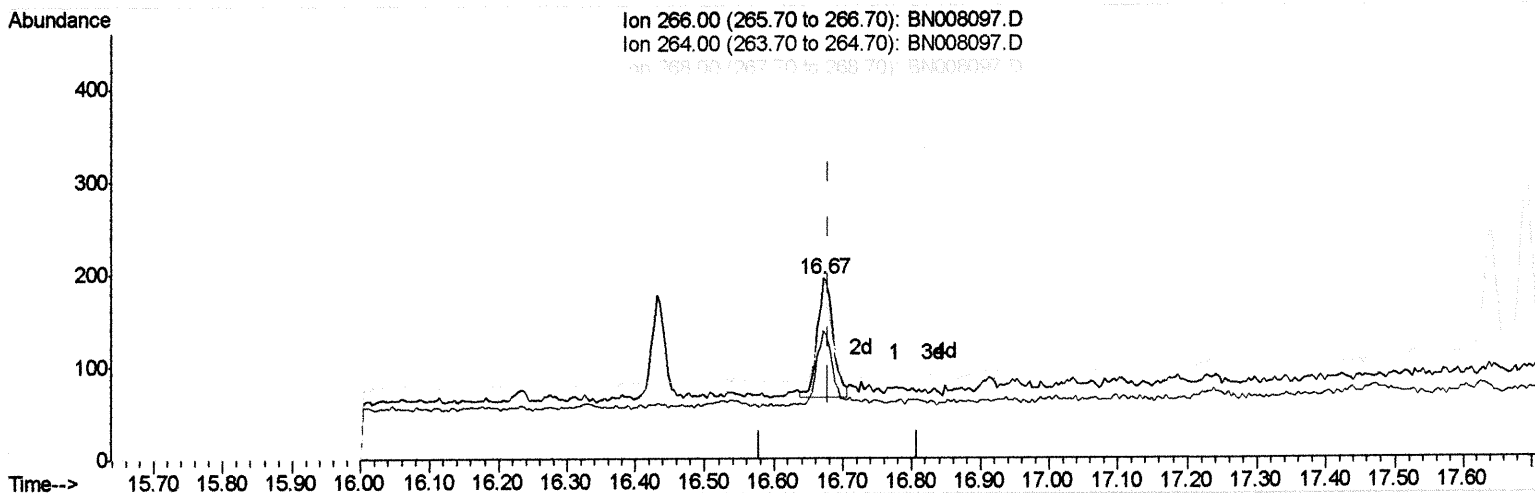

(11) Pentachlorophenol

16.671min (-0.008) 0.03ng/ul m JU 10/16/19

response 204

Ion	Exp%	Act%
266.00	100	100
264.00	62.60	2.94#
268.00	64.90	1.96#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101119\
 Data File : BN008097.D
 Acq On : 12 Oct 2019 04:01
 Operator : JU
 Sample : K5124-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLM78

Manual Integrations
 APPROVED

mohammad
 10/15/2019 7:57:55 AM

Quant Time: Oct 14 15:26:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 11 19:05:54 2019
 Response via : Initial Calibration

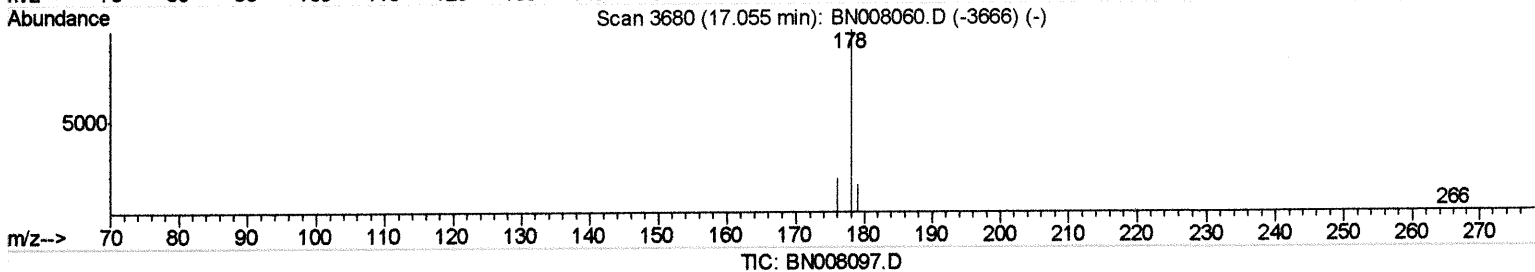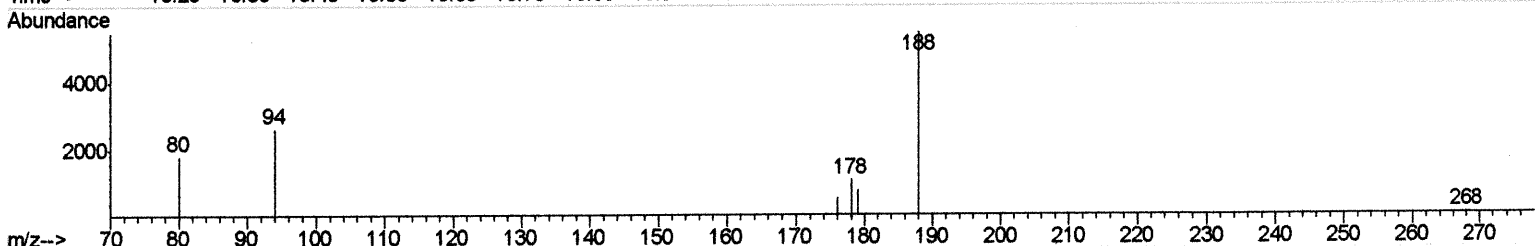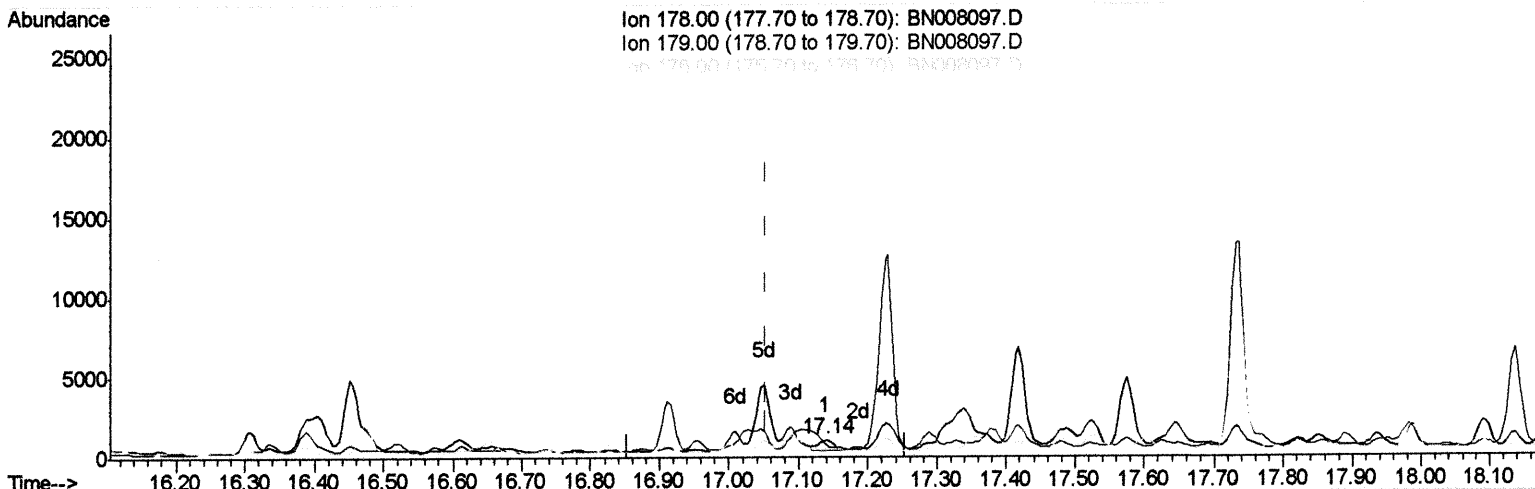

(12) Phenanthrene

17.140min (+0.085) 0.01ng/ul

response 1066

Ion	Exp%	Act%
178.00	100	100
179.00	16.00	69.07#
176.00	19.30	49.27#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101119\
 Data File : BN008097.D
 Acq On : 12 Oct 2019 04:01
 Operator : JU
 Sample : K5124-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLM78

Manual Integrations
 APPROVED

mohammad
 10/15/2019 7:57:55 AM

Quant Time: Oct 14 15:26:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 11 19:05:54 2019
 Response via : Initial Calibration

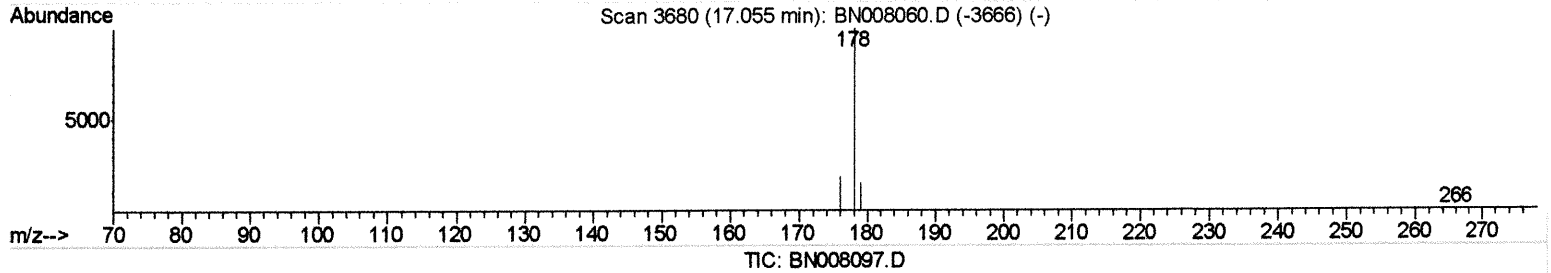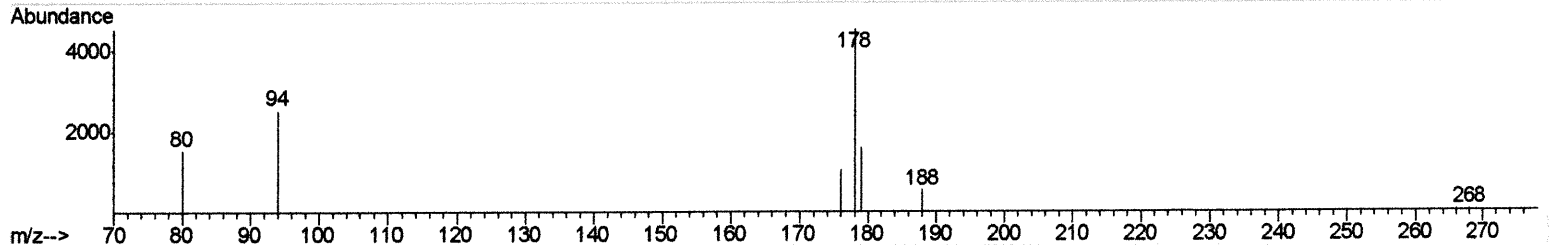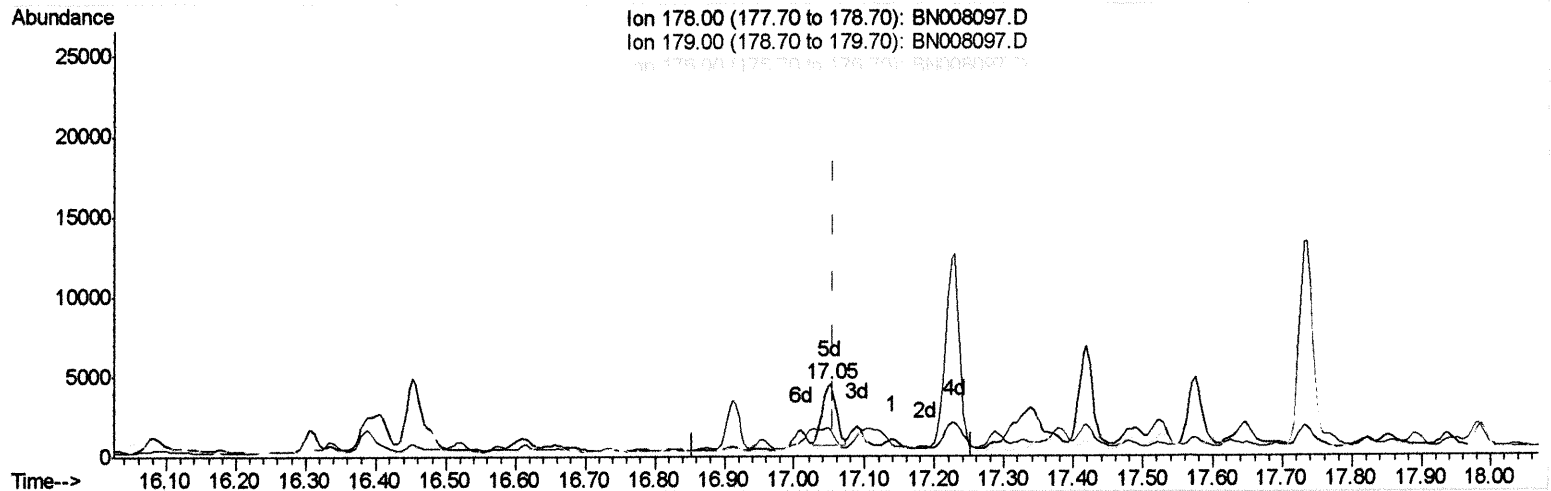

(12) Phenanthrene

17.051min (-0.004) 0.07ng/ul m JU 10/16/19

response 5308

Ion	Exp%	Act%
178.00	100	100
179.00	16.00	35.69#
176.00	19.30	23.59#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101119\
 Data File : BN008097.D
 Acq On : 12 Oct 2019 04:01
 Operator : JU
 Sample : K5124-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLM78

Manual Integrations
 APPROVED

mohammad
 10/15/2019 7:57:55 AM

Quant Time: Oct 14 15:26:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 11 19:05:54 2019
 Response via : Initial Calibration

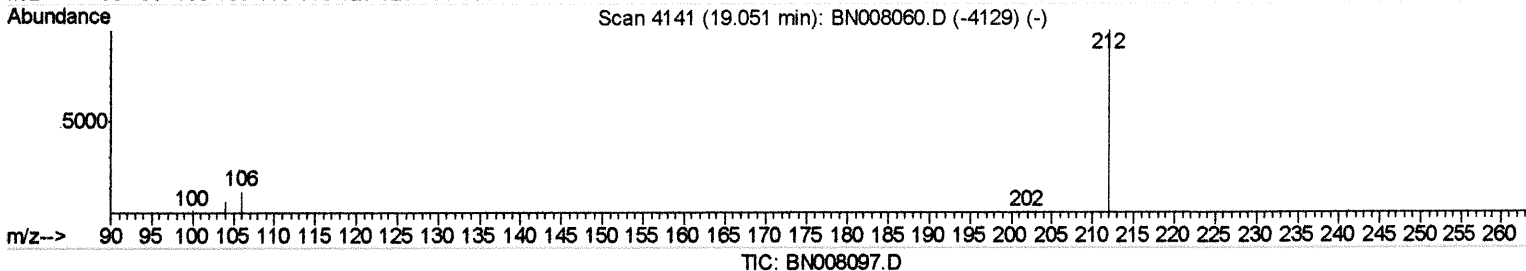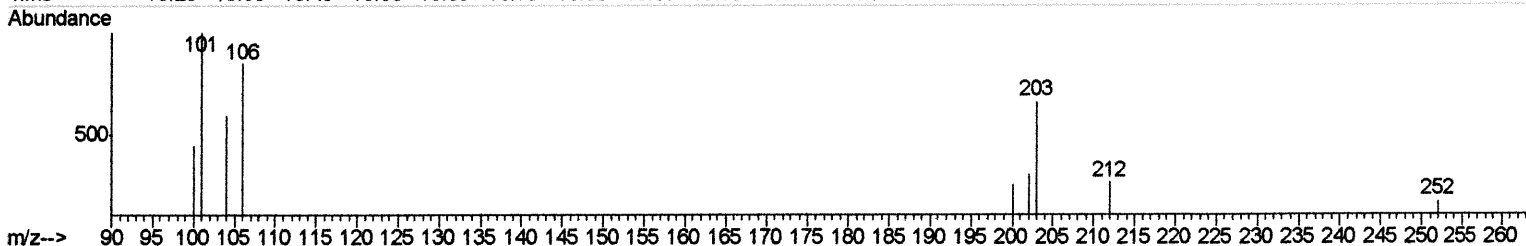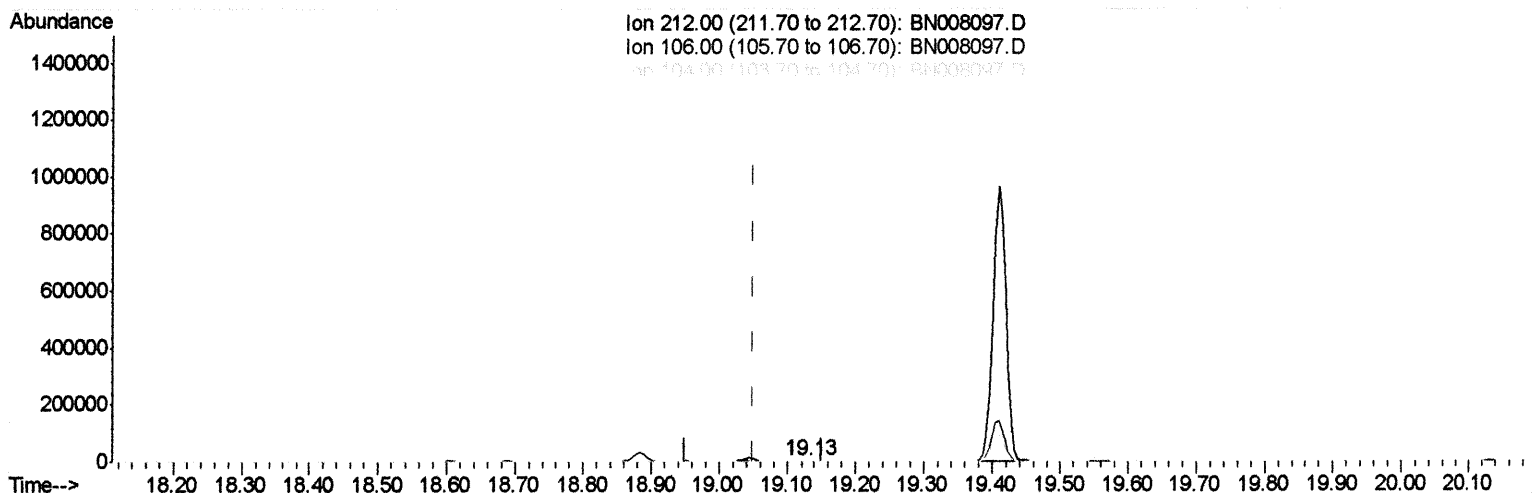

(14) Fluoranthene-d10 (SURR)

19.130min (+0.079) 0.00ng/ul

response 290

Ion	Exp%	Act%
212.00	100	100
106.00	12.70	163.10#
104.00	7.20	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101119\
 Data File : BN008097.D
 Acq On : 12 Oct 2019 04:01
 Operator : JU
 Sample : K5124-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLM78

Manual Integrations
 APPROVED

mohammad
 10/15/2019 7:57:55 AM

Quant Time: Oct 14 15:26:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 11 19:05:54 2019
 Response via : Initial Calibration

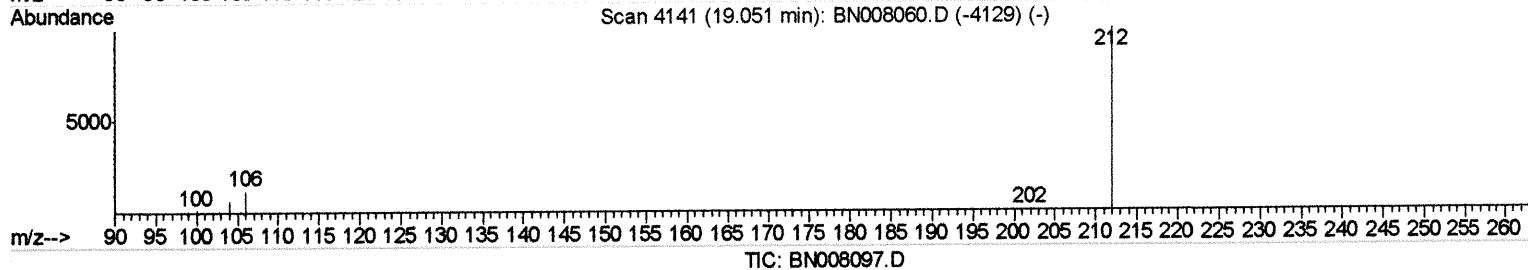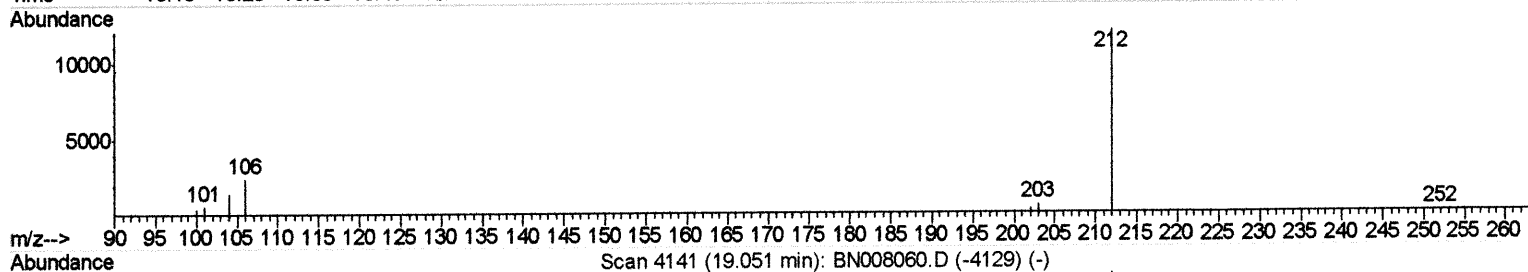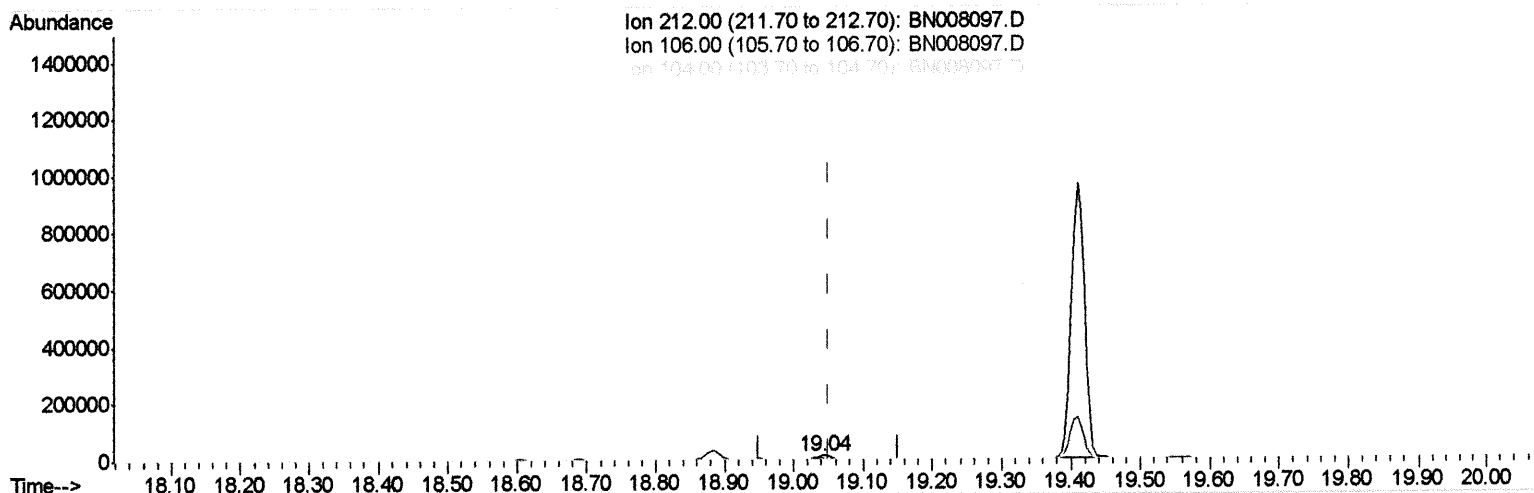

(14) Fluoranthene-d10 (SURR)

19.042min (-0.009) 0.19ng/ul m JU 10/16/19

response 16118

Ion	Exp%	Act%
212.00	100	100
106.00	12.70	2.93#
104.00	7.20	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101119\
 Data File : BN008097.D
 Acq On : 12 Oct 2019 04:01
 Operator : JU
 Sample : K5124-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLM78

Manual Integrations
 APPROVED

mohammad
 10/15/2019 7:57:55 AM

Quant Time: Oct 14 15:26:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 11 19:05:54 2019
 Response via : Initial Calibration

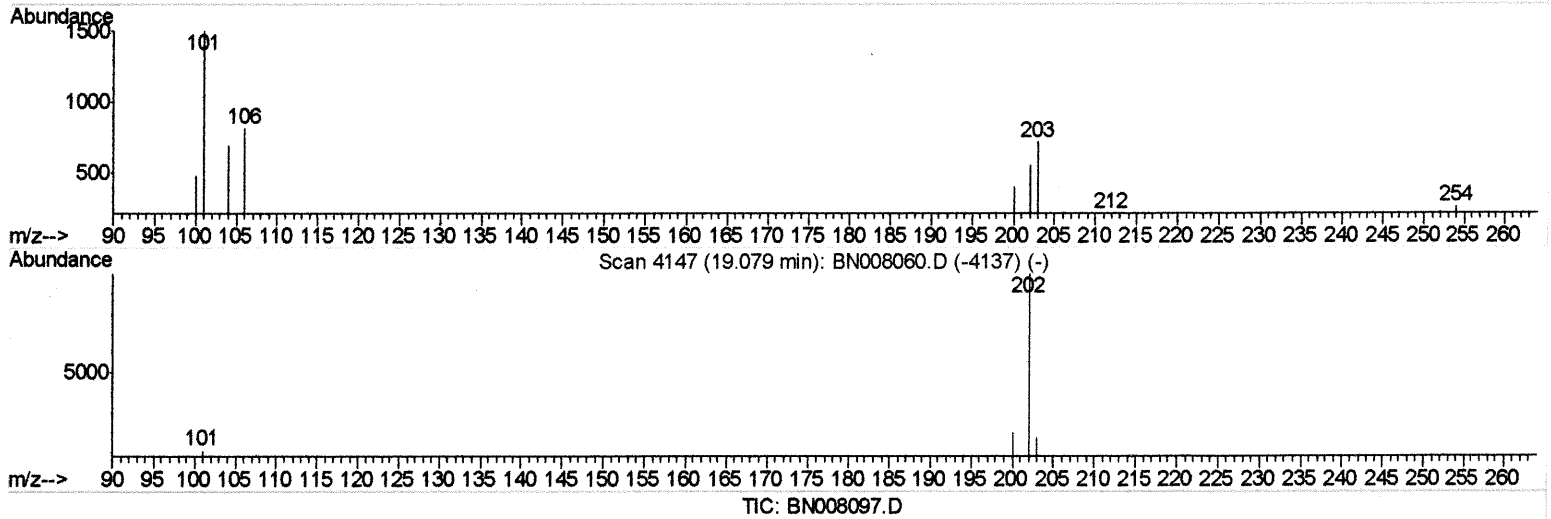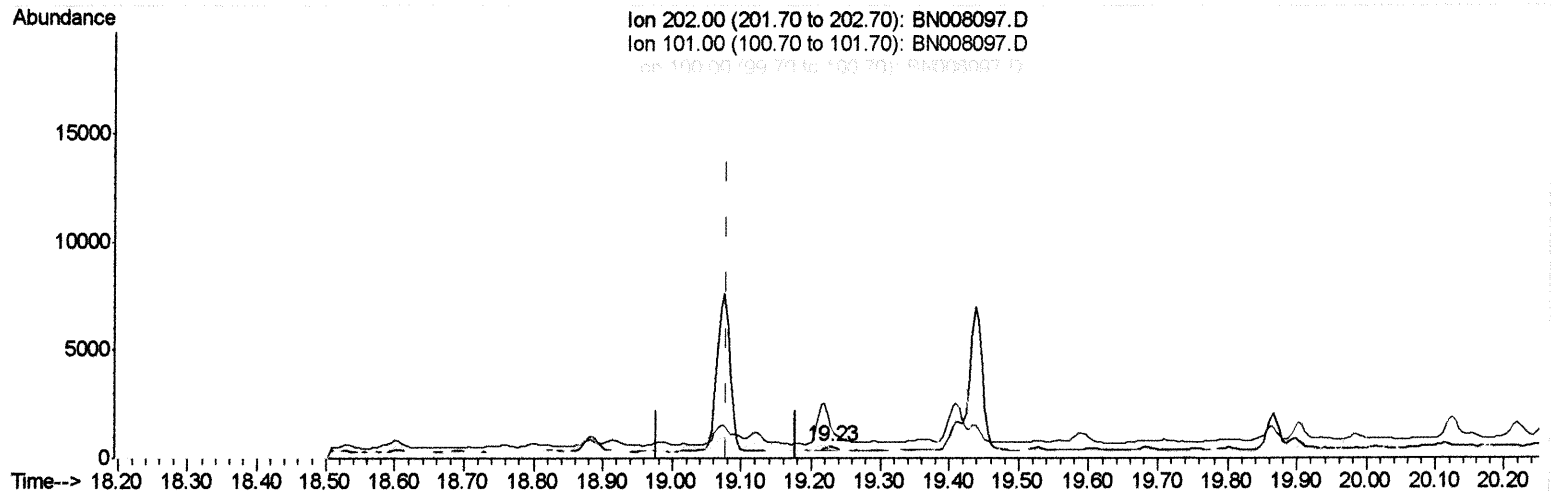

(15) Fluoranthene (C)
 19.228min (+0.149) 0.00ng/ul
 response 277

Ion	Exp%	Act%
202.00	100	100
101.00	11.20	268.69#
100.00	8.50	87.30#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101119\
 Data File : BN008097.D
 Acq On : 12 Oct 2019 04:01
 Operator : JU
 Sample : K5124-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLM78

Manual Integrations
 APPROVED

mohammad
 10/15/2019 7:57:55 AM

Quant Time: Oct 14 15:26:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 11 19:05:54 2019
 Response via : Initial Calibration

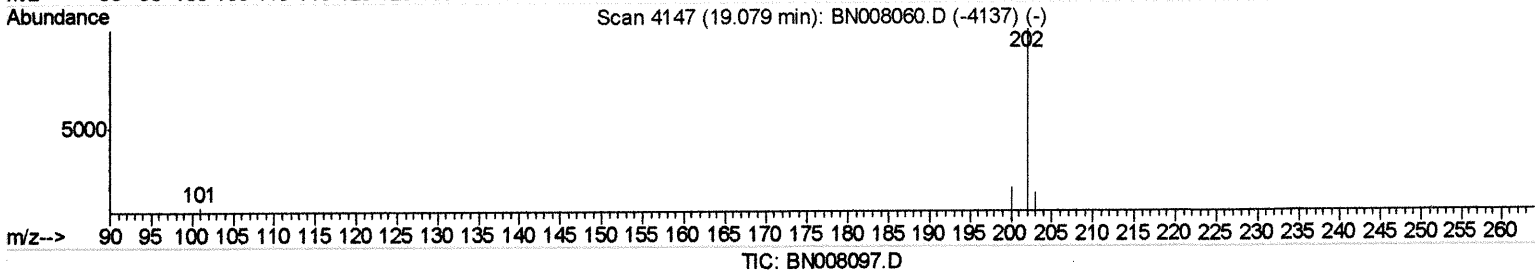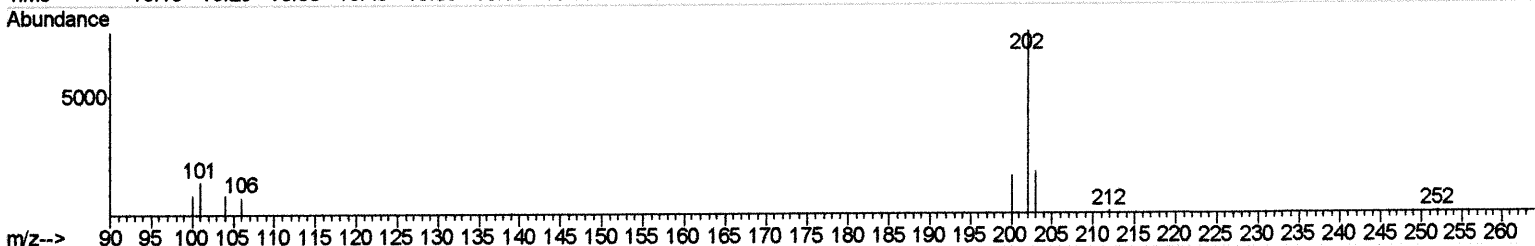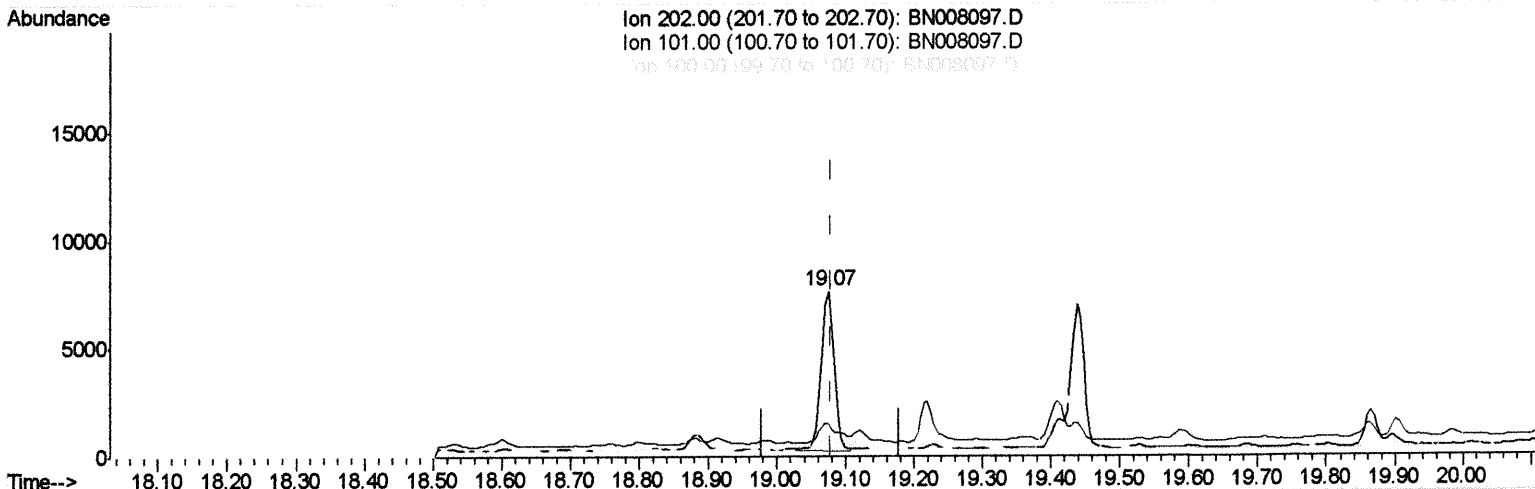

(15) Fluoranthene (C)

19.074min (-0.004) 0.11ng/ul m

24/10/16/19

response 9887

Ion	Exp%	Act%
202.00	100	100
101.00	11.20	19.39
100.00	8.50	12.17
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101119\
 Data File : BN008097.D
 Acq On : 12 Oct 2019 04:01
 Operator : JU
 Sample : K5124-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLM78

Manual Integrations
 APPROVED

mohammad
 10/15/2019 7:57:55 AM

Quant Time: Oct 14 15:26:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 11 19:05:54 2019
 Response via : Initial Calibration

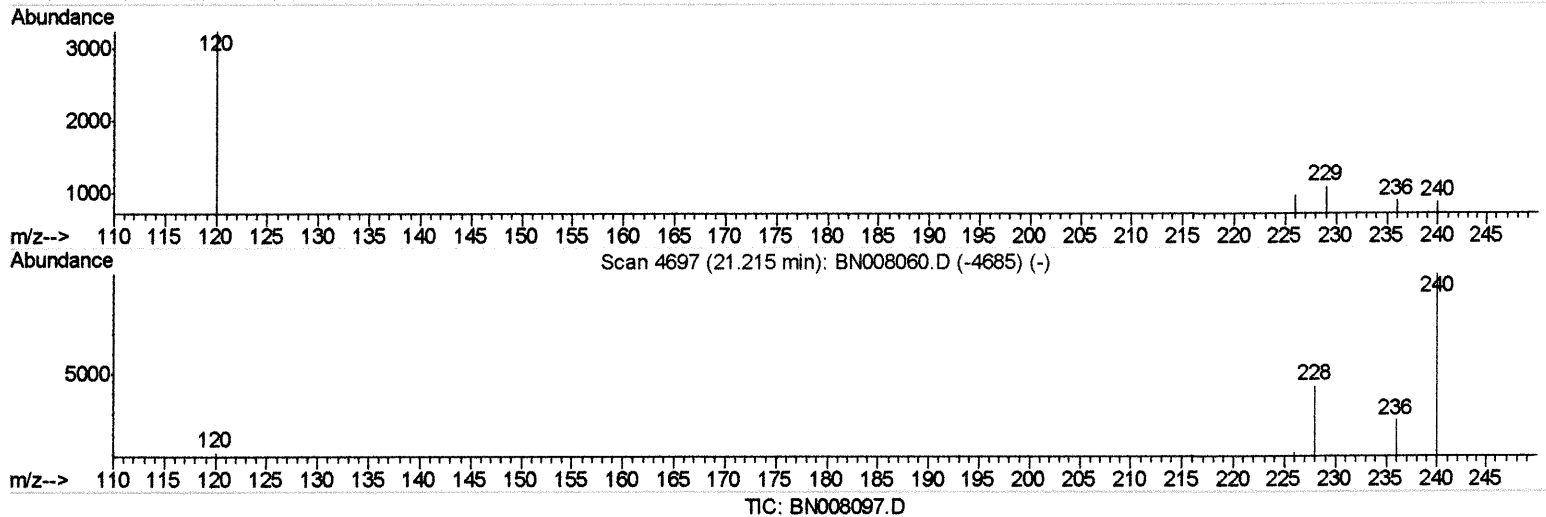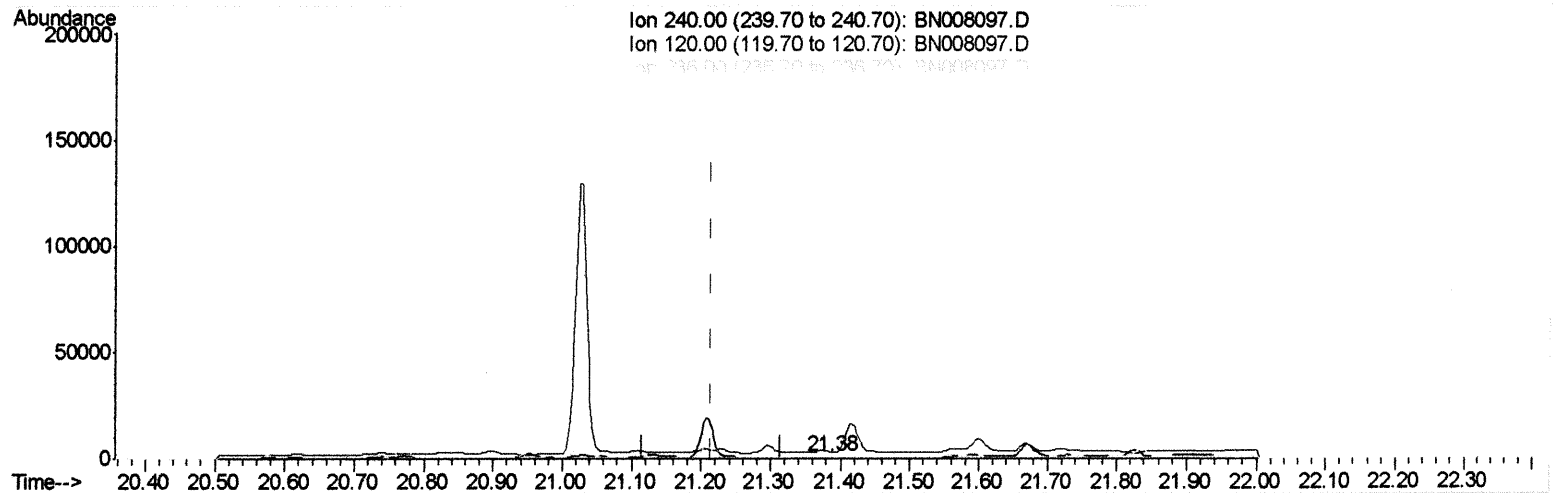

(16) Chrysene-d12 (I)

21.385min (+0.170) 0.40ng/ul

response 273

Ion	Exp%	Act%
240.00	100	100
120.00	14.70	372.76#
236.00	28.40	101.49#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101119\
 Data File : BN008097.D
 Acq On : 12 Oct 2019 04:01
 Operator : JU
 Sample : K5124-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLM78

Manual Integrations
 APPROVED

mohammad
 10/15/2019 7:57:55 AM

Quant Time: Oct 14 15:26:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 11 19:05:54 2019
 Response via : Initial Calibration

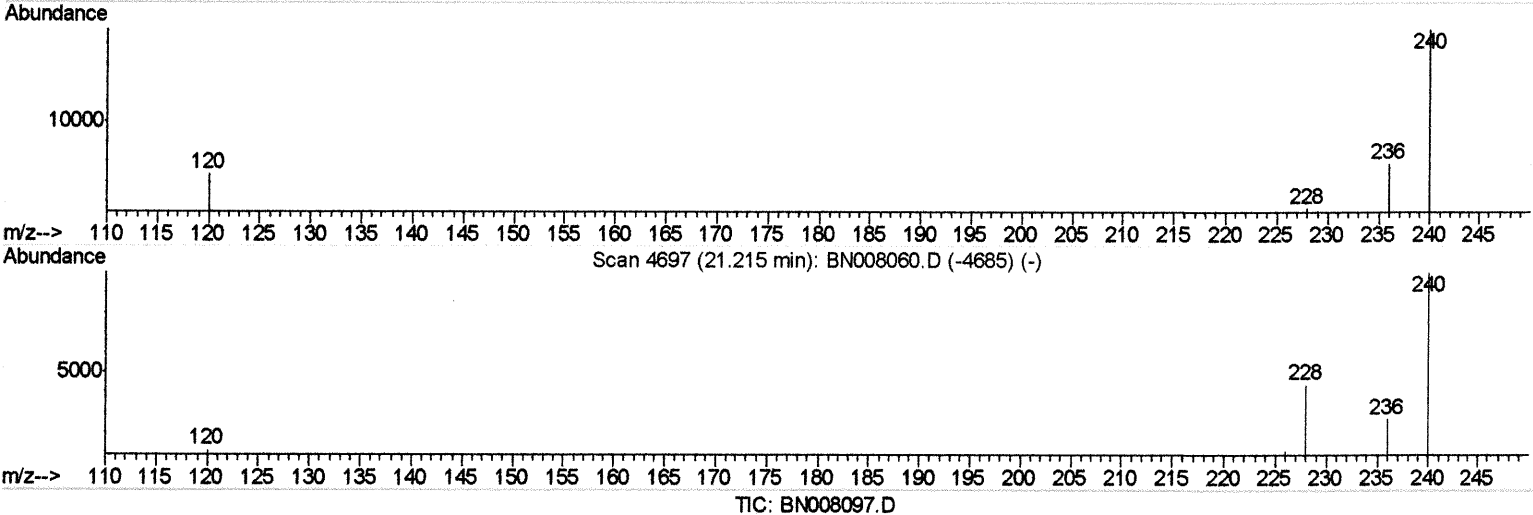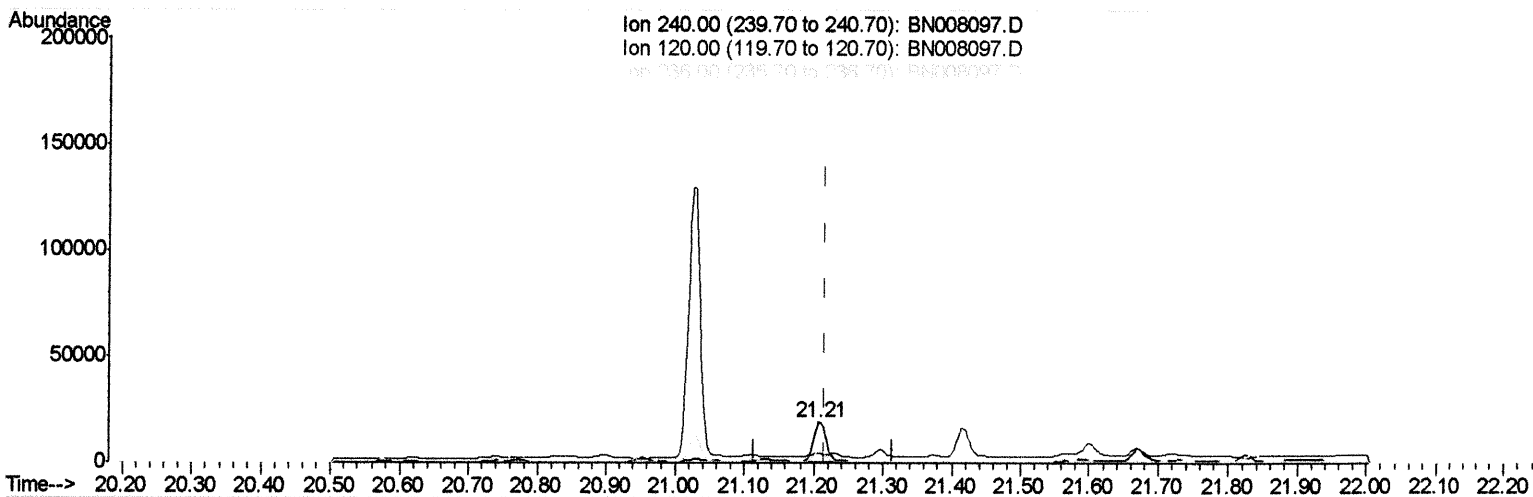

(16) Chrysene-d12 (I)

21.207min (-0.009) 0.40ng/ul m JU 10/16/19

response 22770

Ion	Exp%	Act%
240.00	100	100
120.00	14.70	24.43#
236.00	28.40	29.82
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101119\
 Data File : BN008097.D
 Acq On : 12 Oct 2019 04:01
 Operator : JU
 Sample : K5124-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLM78

Manual Integrations
 APPROVED

mohammad
 10/15/2019 7:57:55 AM

Quant Time: Oct 14 15:26:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 11 19:05:54 2019
 Response via : Initial Calibration

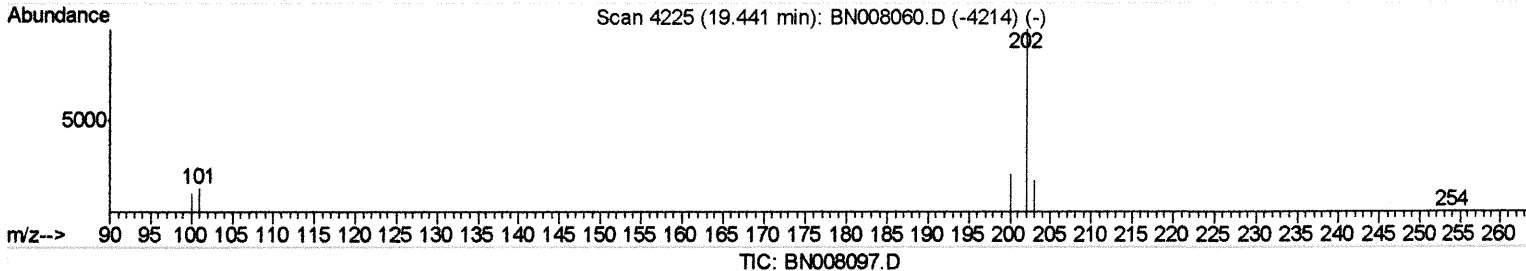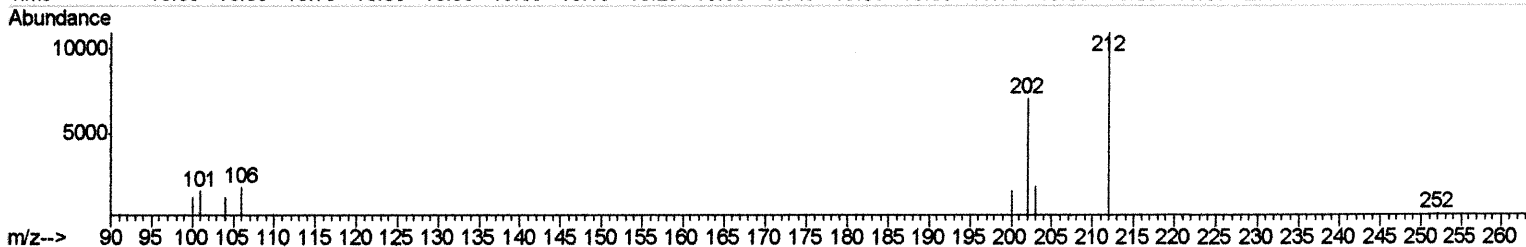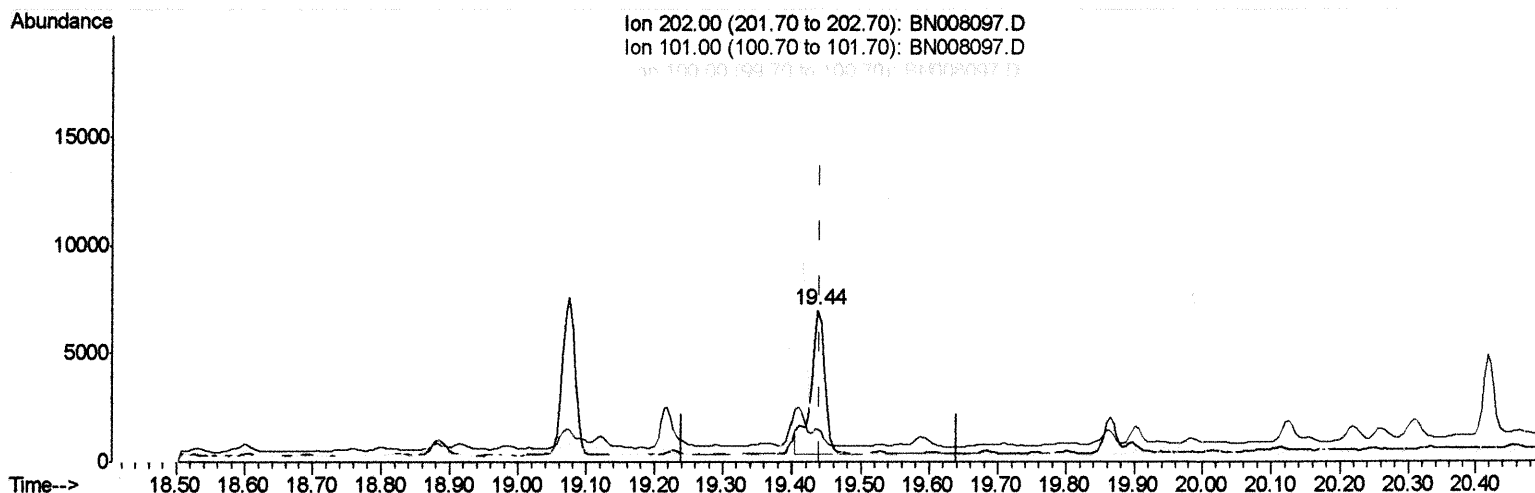

(17) Pyrene

19.437min (-0.004) 0.11ng/ul

response 9539

Ion	Exp%	Act%
202.00	100	100
101.00	13.60	22.35#
100.00	10.90	17.64#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101119\
Data File : BN008097.D
Acq On : 12 Oct 2019 04:01
Operator : JU
Sample : K5124-08
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLM78

Manual Integrations
APPROVED

mohammad
10/15/2019 7:57:55 AM

Quant Time: Oct 14 15:26:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 11 19:05:54 2019
Response via : Initial Calibration

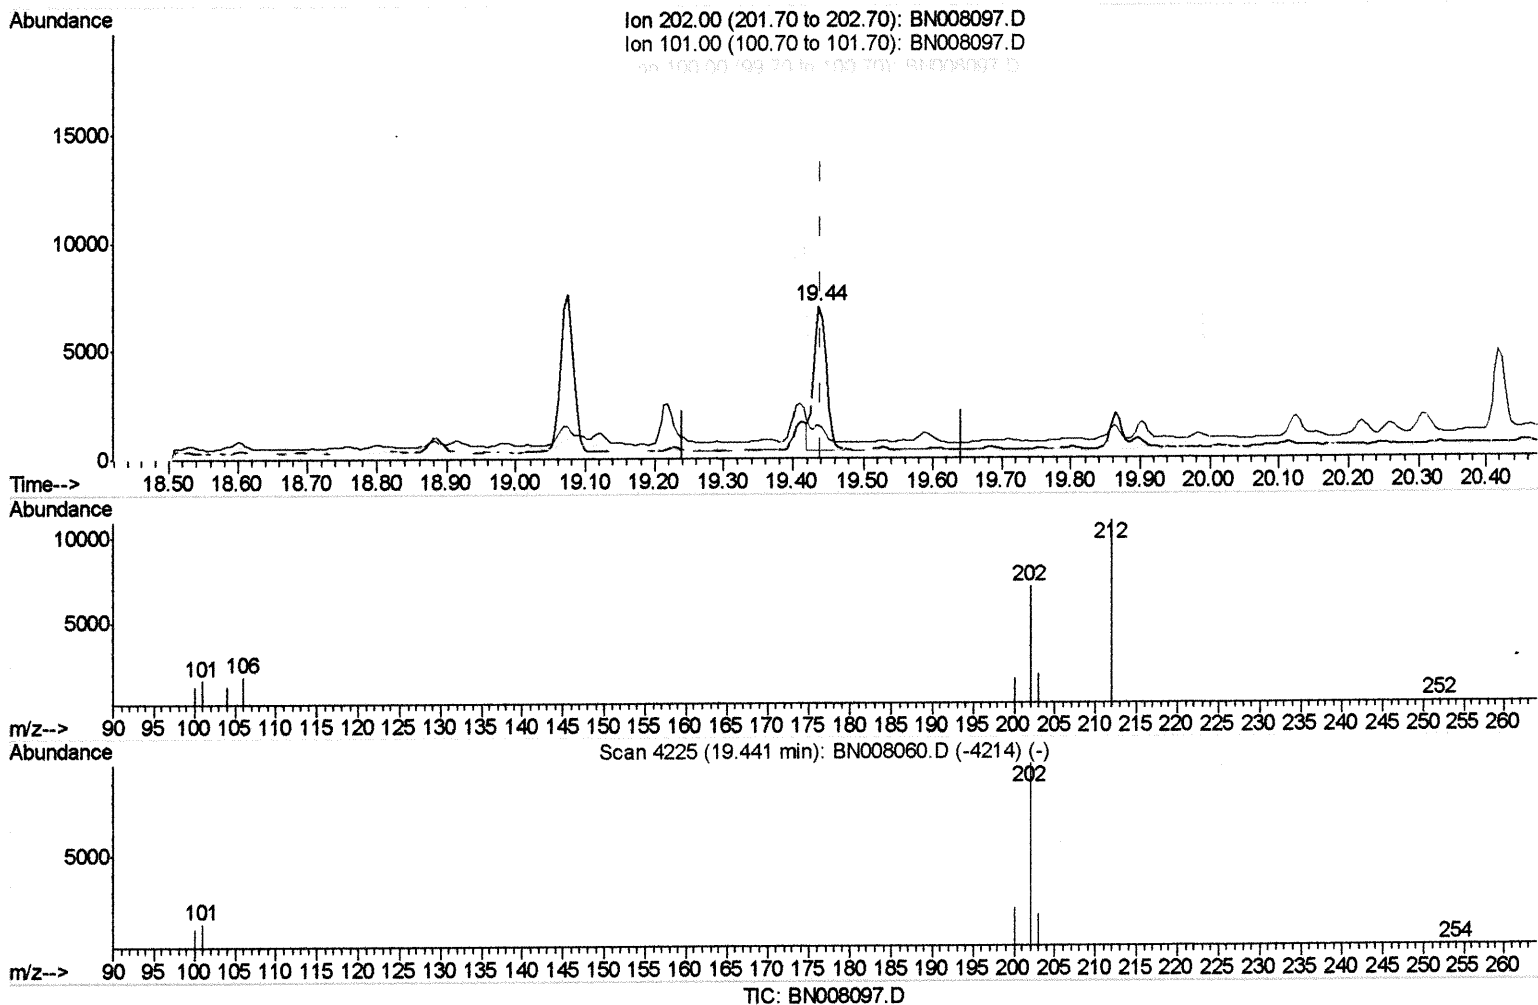

(17) Pyrene

19.437min (-0.004) 0.09ng/ul m *JU 10/16/19*

response 8454

Ion	Exp%	Act%
202.00	100	100
101.00	13.60	22.35#
100.00	10.90	17.64#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101119\
 Data File : BN008097.D
 Acq On : 12 Oct 2019 04:01
 Operator : JU
 Sample : K5124-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLM78

Manual Integrations
 APPROVED

mohammad
 10/15/2019 7:57:55 AM

Quant Time: Oct 14 15:26:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 11 19:05:54 2019
 Response via : Initial Calibration

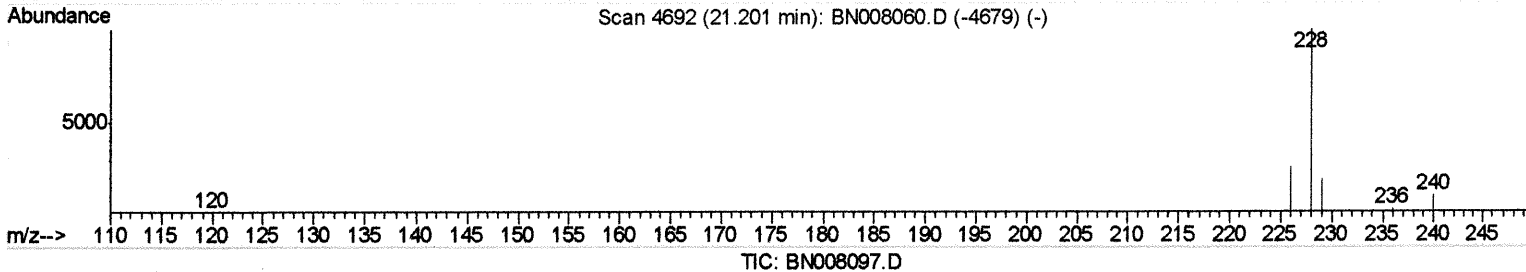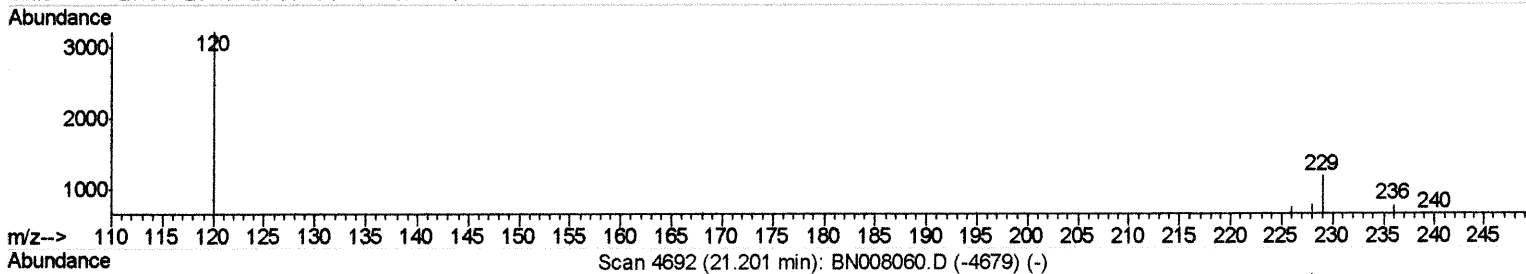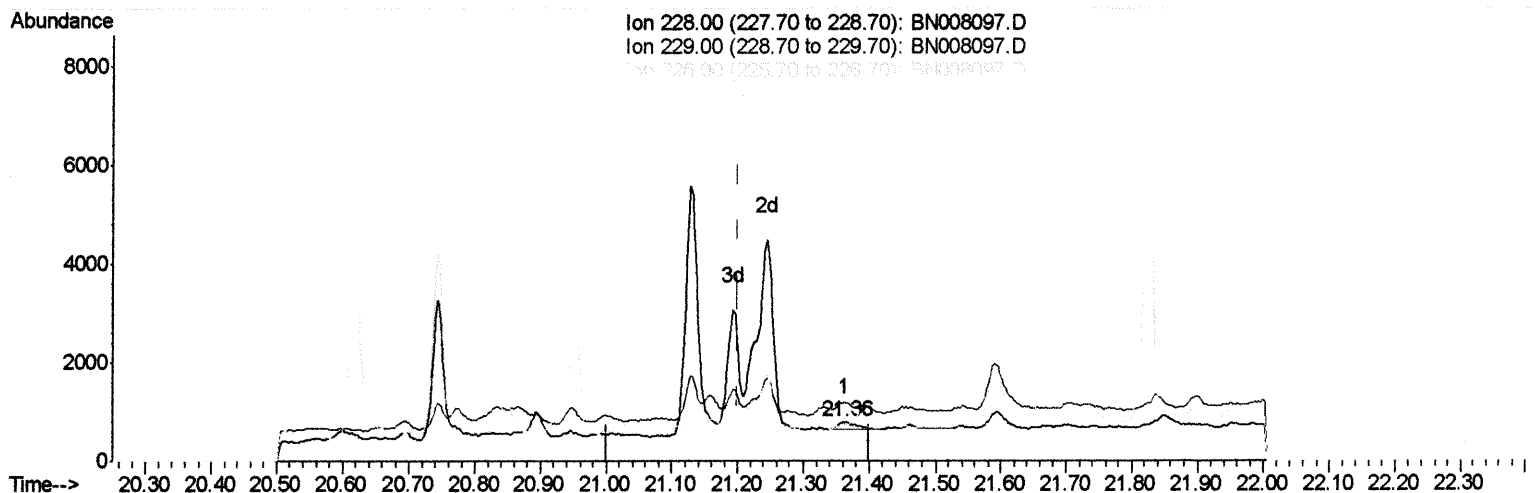

(18) Benzo(a)anthracene
 21.364min (+0.164) 0.00ng/ul
 response 354

Ion	Exp%	Act%
228.00	100	100
229.00	20.20	149.75#
226.00	26.70	93.98#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101119\
 Data File : BN008097.D
 Acq On : 12 Oct 2019 04:01
 Operator : JU
 Sample : K5124-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 JLM78

Manual Integrations
 APPROVED

mohammad
 10/15/2019 7:57:55 AM

Quant Time: Oct 14 15:26:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 11 19:05:54 2019
 Response via : Initial Calibration

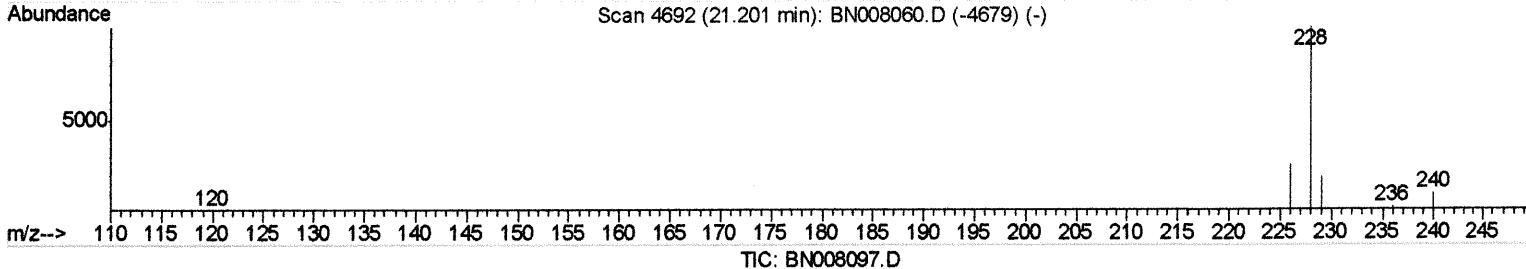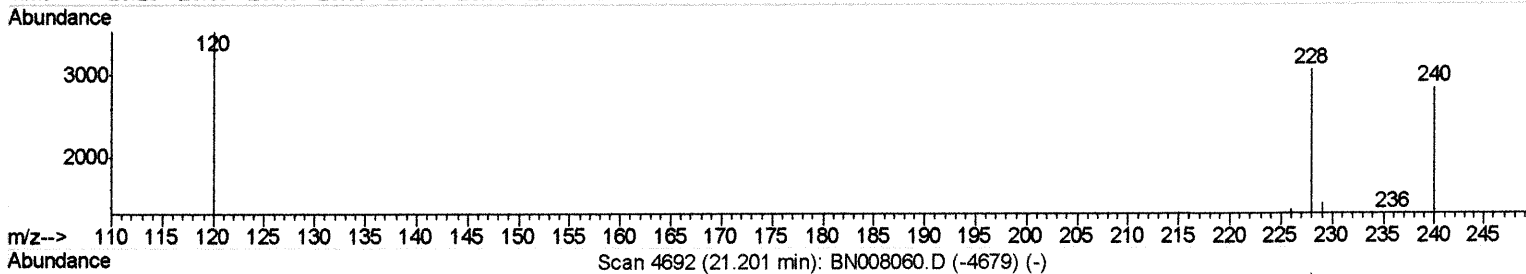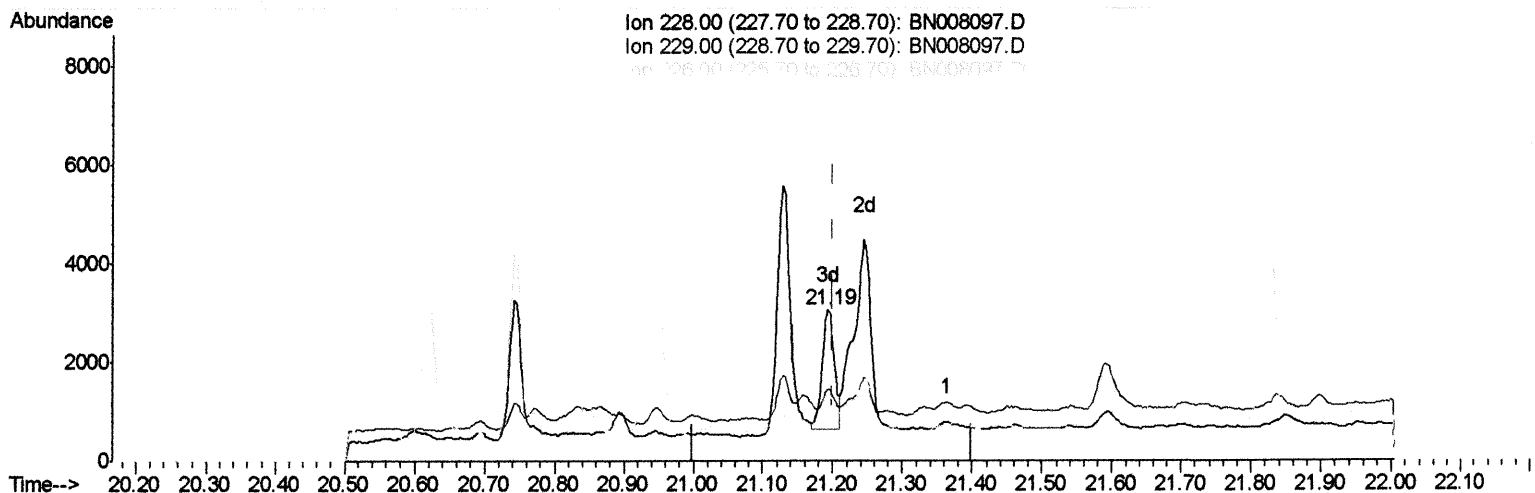

(18) Benzo(a)anthracene

21.192min (-0.009) 0.04ng/ul m 24/10/16/19

response 2972

Ion	Exp%	Act%
228.00	100	100
229.00	20.20	46.87#
226.00	26.70	44.35#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101119\
 Data File : BN008097.D
 Acq On : 12 Oct 2019 04:01
 Operator : JU
 Sample : K5124-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLM78

Manual Integrations
 APPROVED

mohammad
 10/15/2019 7:57:55 AM

Quant Time: Oct 14 15:26:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 11 19:05:54 2019
 Response via : Initial Calibration

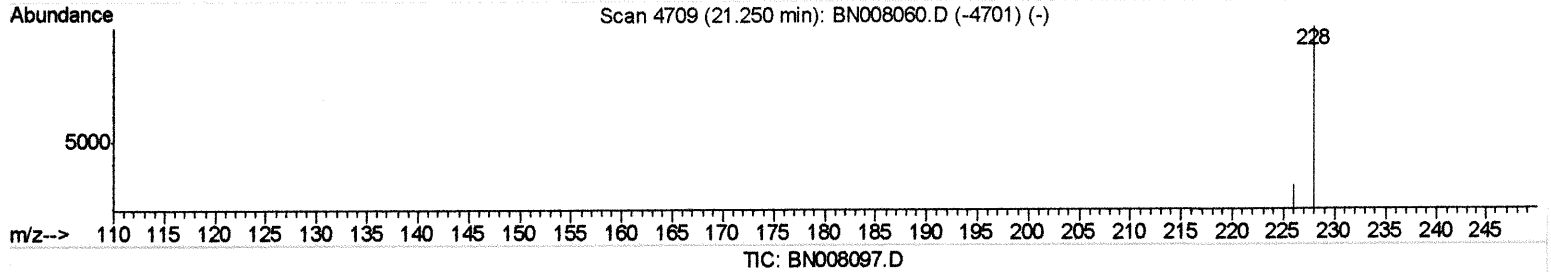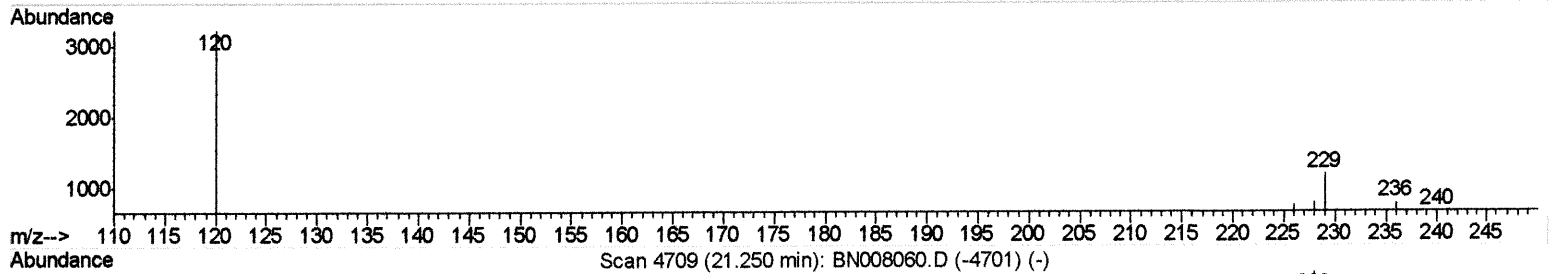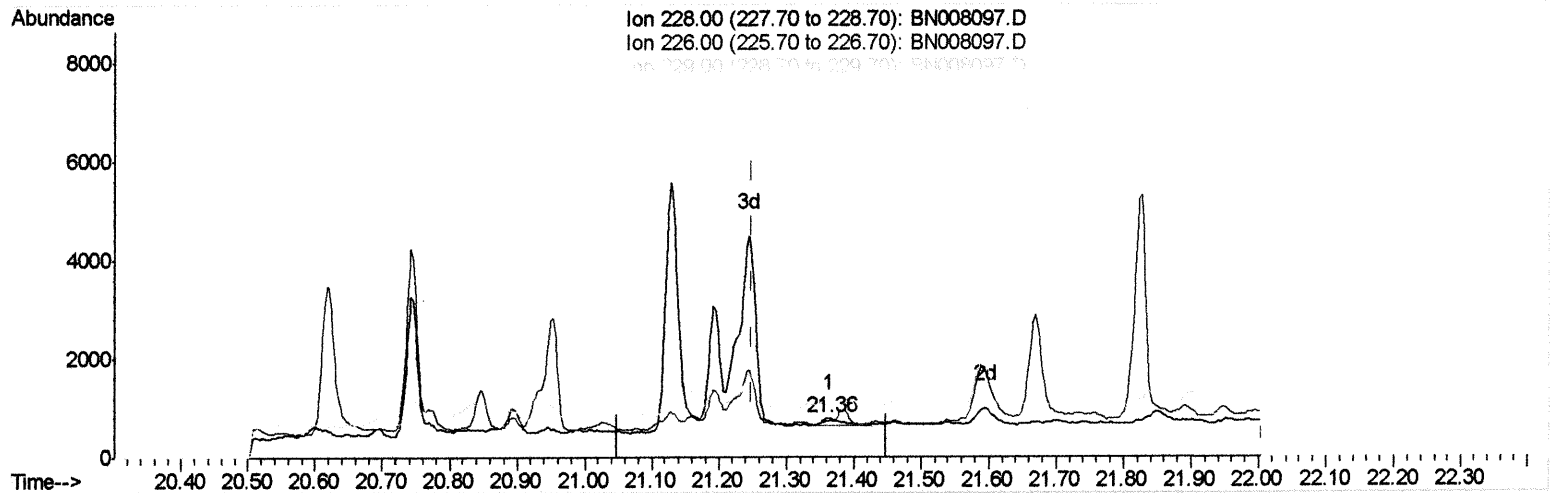

(19) Chrysene

21.364min (+0.114) 0.00ng/ul

response 354

Ion	Exp%	Act%
228.00	100	100
226.00	30.10	93.98#
229.00	20.20	149.75#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101119\
 Data File : BN008097.D
 Acq On : 12 Oct 2019 04:01
 Operator : JU
 Sample : K5124-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLM78

Manual Integrations
 APPROVED

mohammad
 10/15/2019 7:57:55 AM

Quant Time: Oct 14 15:26:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 11 19:05:54 2019
 Response via : Initial Calibration

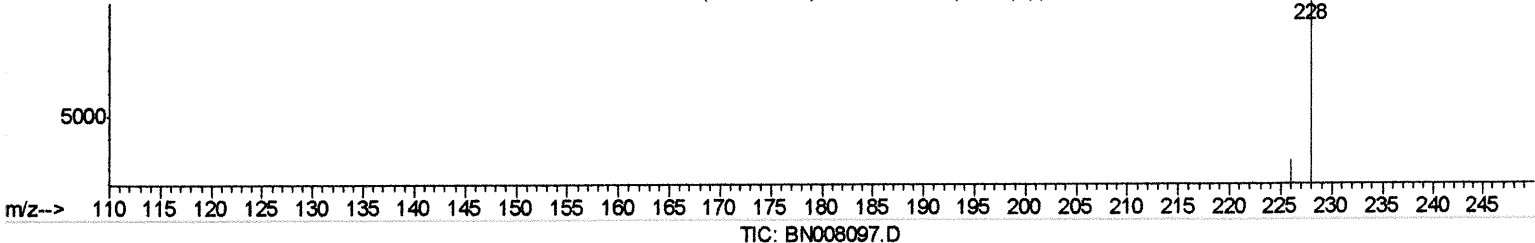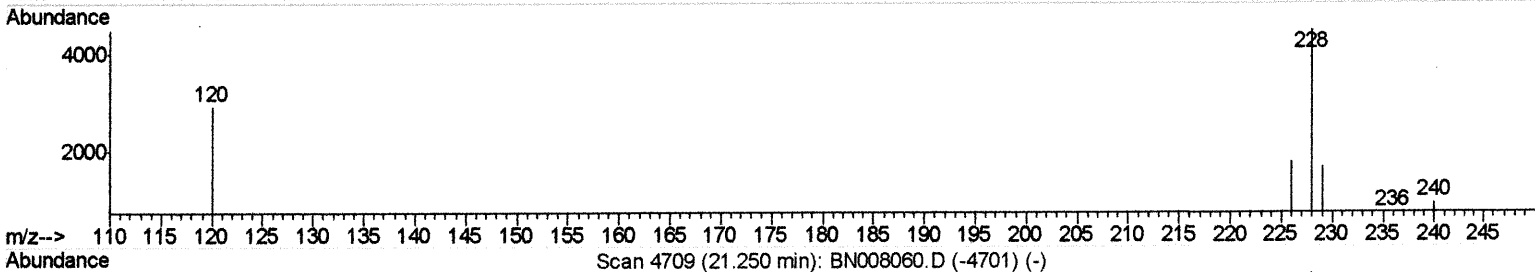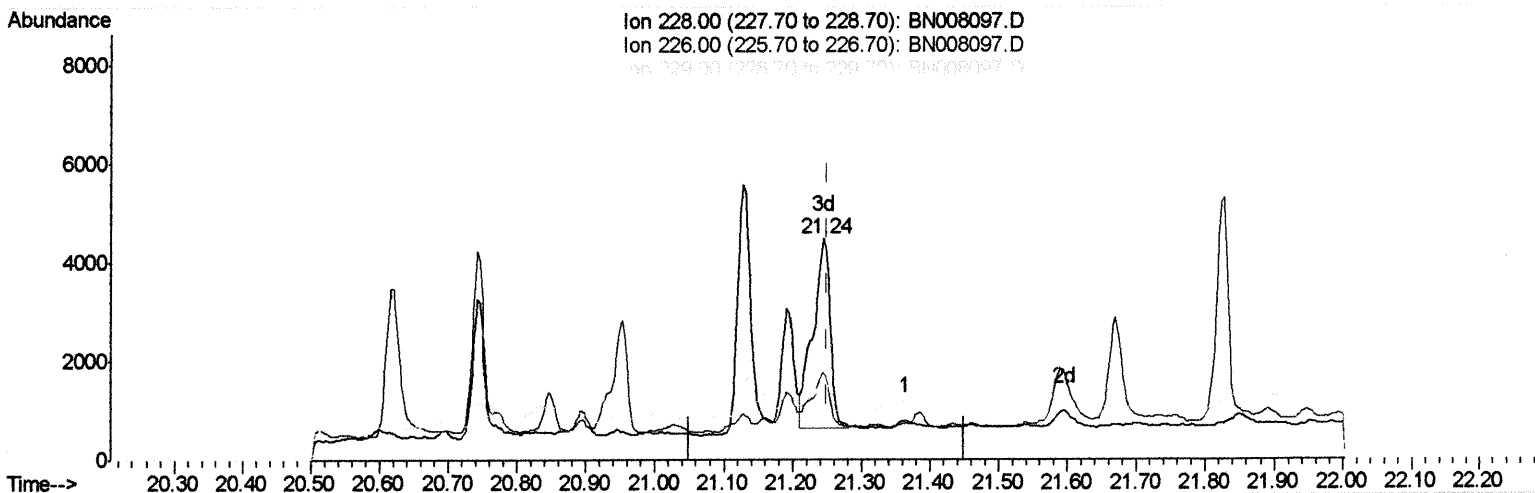

(19) Chrysene

21.245min (-0.006) 0.07ng/ul m 10/16/19

response 6778

Ion	Exp%	Act%
228.00	100	100
226.00	30.10	39.41#
229.00	20.20	37.22#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101119\
 Data File : BN008097.D
 Acq On : 12 Oct 2019 04:01
 Operator : JU
 Sample : K5124-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLM78

Manual Integrations
 APPROVED

mohammad
 10/15/2019 7:57:55 AM

Quant Time: Oct 14 15:26:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 11 19:05:54 2019
 Response via : Initial Calibration

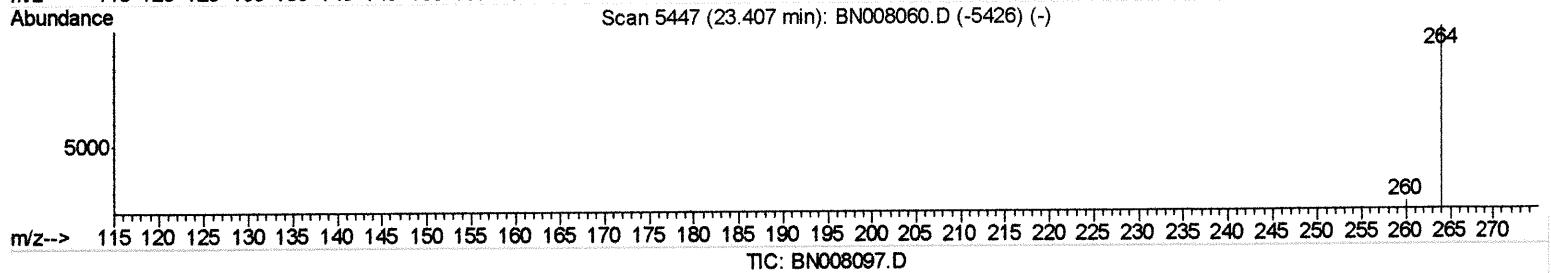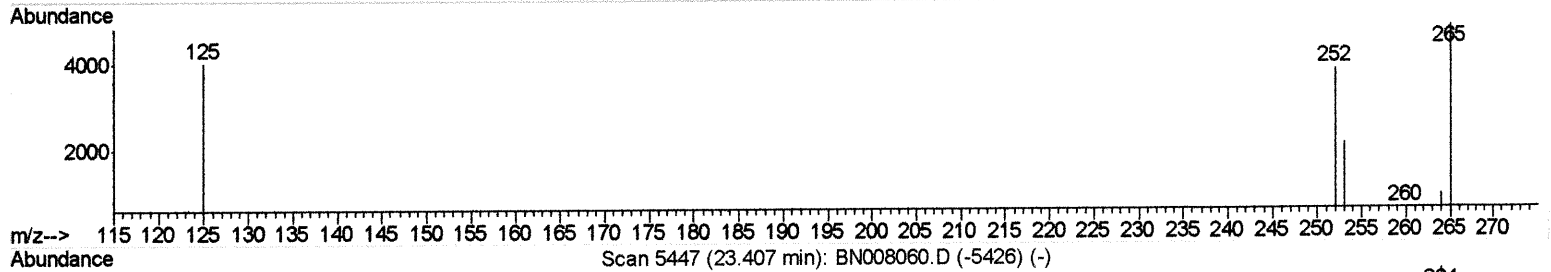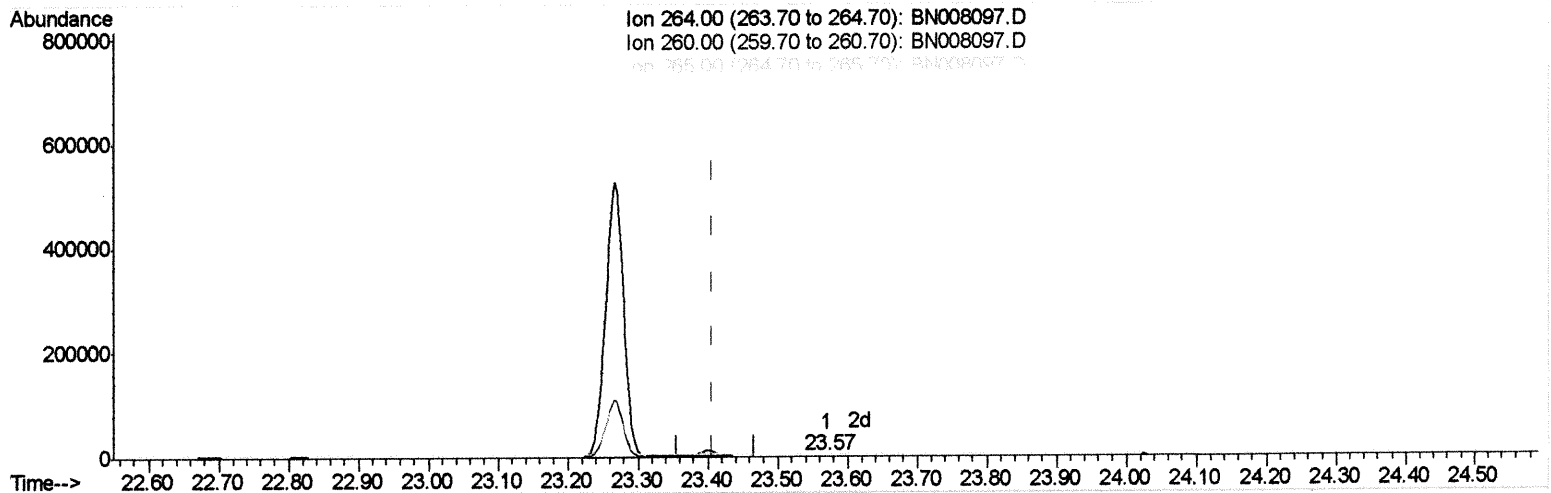

(20) Perylene-d12 (I)

23.571min (+0.164) 0.40ng/ul

response 199

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	65.56#
265.00	74.00	535.65#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101119\
Data File : BN008097.D
Acq On : 12 Oct 2019 04:01
Operator : JU
Sample : K5124-08
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLM78

Manual Integrations
APPROVED

mohammad
10/15/2019 7:57:55 AM

Quant Time: Oct 14 15:26:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 11 19:05:54 2019
Response via : Initial Calibration

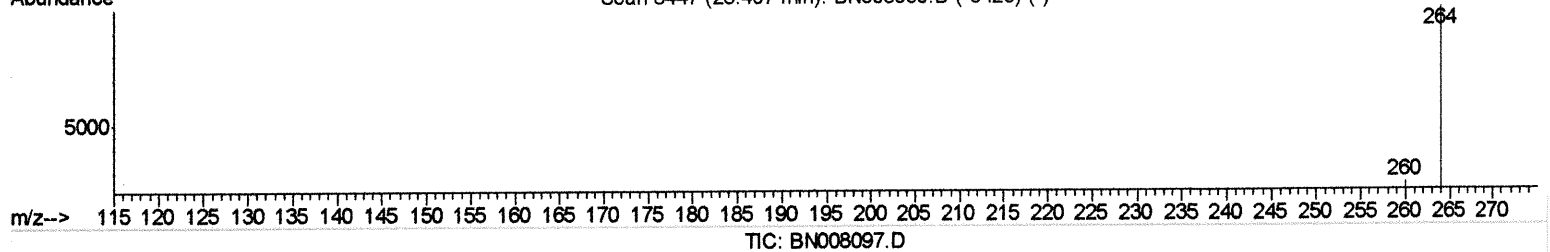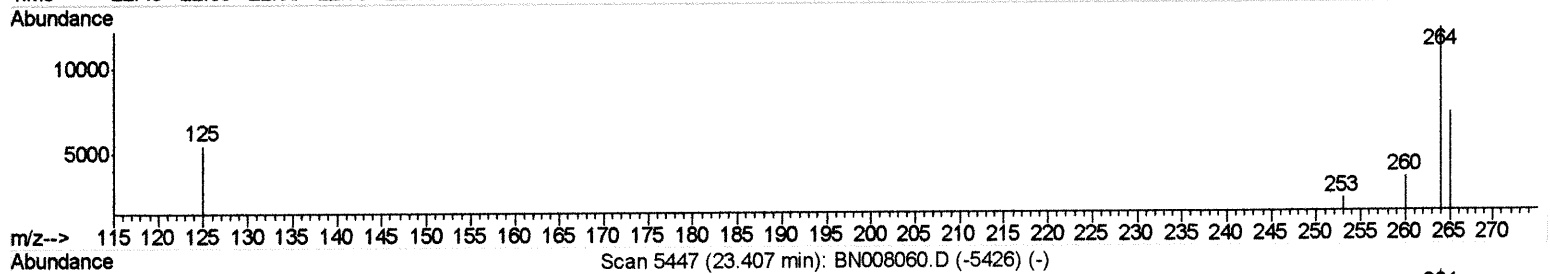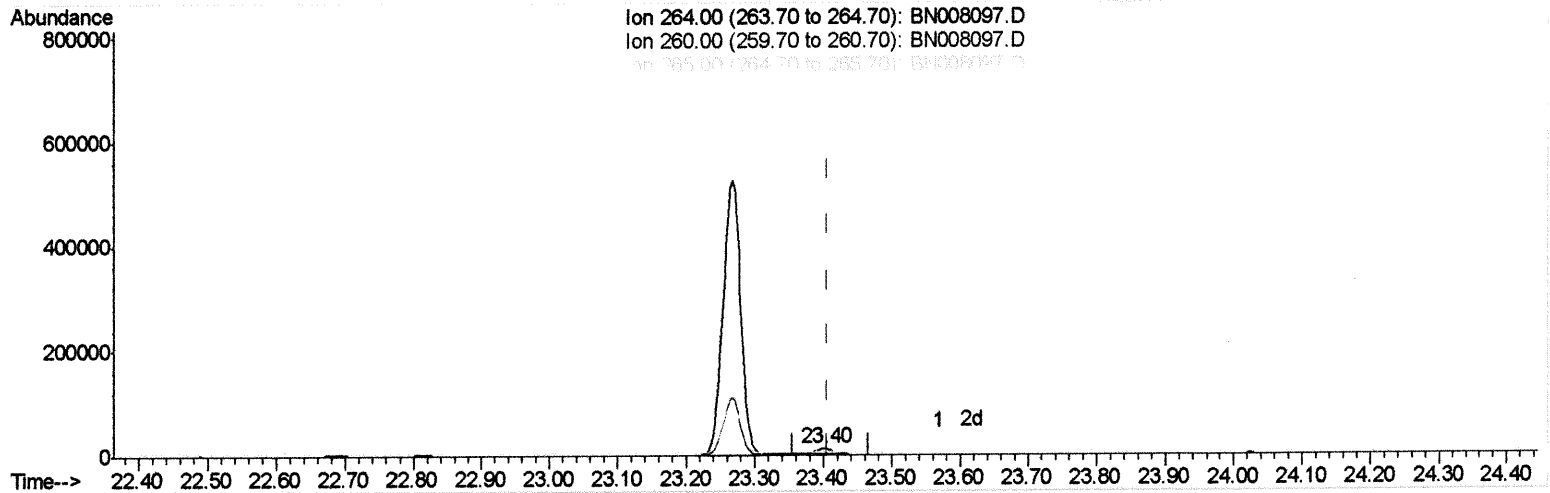

(20) Perylene-d12 (I)

23.402min (-0.005) 0.40ng/ul m

JU 10/16/19

response 18540

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	28.01
265.00	74.00	58.90#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101119\
 Data File : BN008097.D
 Acq On : 12 Oct 2019 04:01
 Operator : JU
 Sample : K5124-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLM78

Manual Integrations
 APPROVED

mohammad
 10/15/2019 7:57:55 AM

Quant Time: Oct 14 15:29:55 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 11 19:05:54 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	3736	0.40	ng/ul	0.00
2) Naphthalene-d8	10.39	136	16765	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.26	164	11537	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.01	188	24310m	0.40	ng/ul	0.00
16) Chrysene-d12	21.21	240	22770m	0.40	ng/ul	0.00
20) Perylene-d12	23.40	264	18540m	0.40	ng/ul	0.00

JU 10/16/19

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.99	152	5446	0.19	ng/ul	-0.01
14) Fluoranthene-d10	19.04	212	16118m	0.19	ng/ul	0.00

JU 10/16/19

Target Compounds

					Qvalue	
3) Naphthalene	10.44	128	1267	0.027	ng/ul#	78
5) 2-Methylnaphthalene	12.07	142	1041	0.032	ng/ul	97
11) Pentachlorophenol	16.67	266	204m	0.035	ng/ul	
12) Phenanthrene	17.05	178	5308m	0.075	ng/ul	
15) Fluoranthene	19.07	202	9887m	0.105	ng/ul	
17) Pyrene	19.44	202	8454m	0.093	ng/ul	
18) Benzo(a)anthracene	21.19	228	2972m	0.036	ng/ul	
19) Chrysene	21.24	228	6778m	0.067	ng/ul	

JU 10/16/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed