
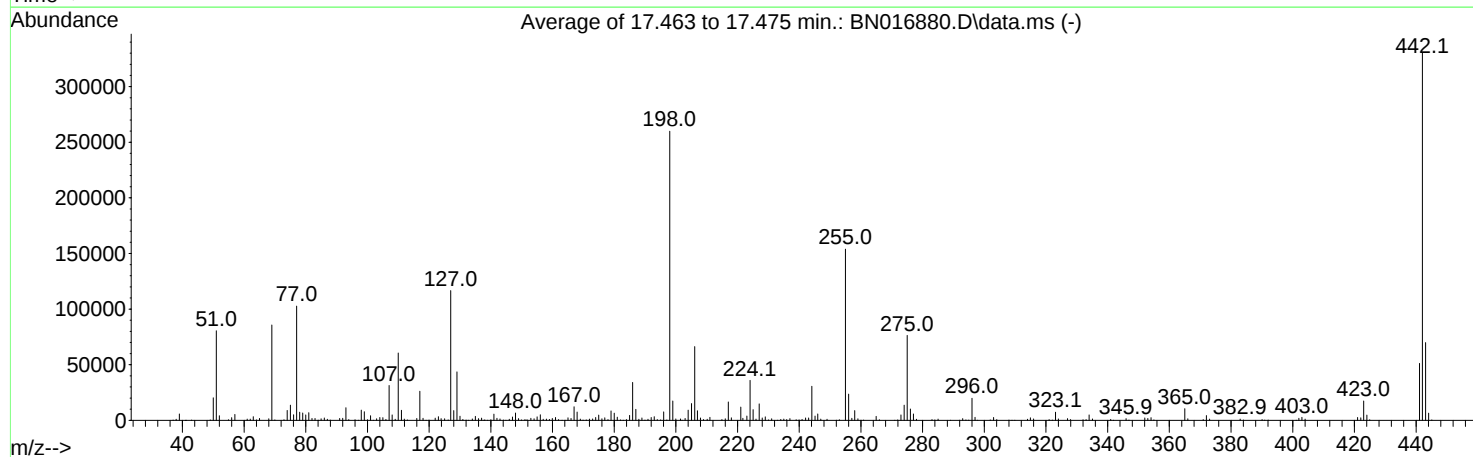


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101121\
 Data File : BN016880.D
 Acq On : 11 Oct 2021 11:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 08 15:46:07 2021

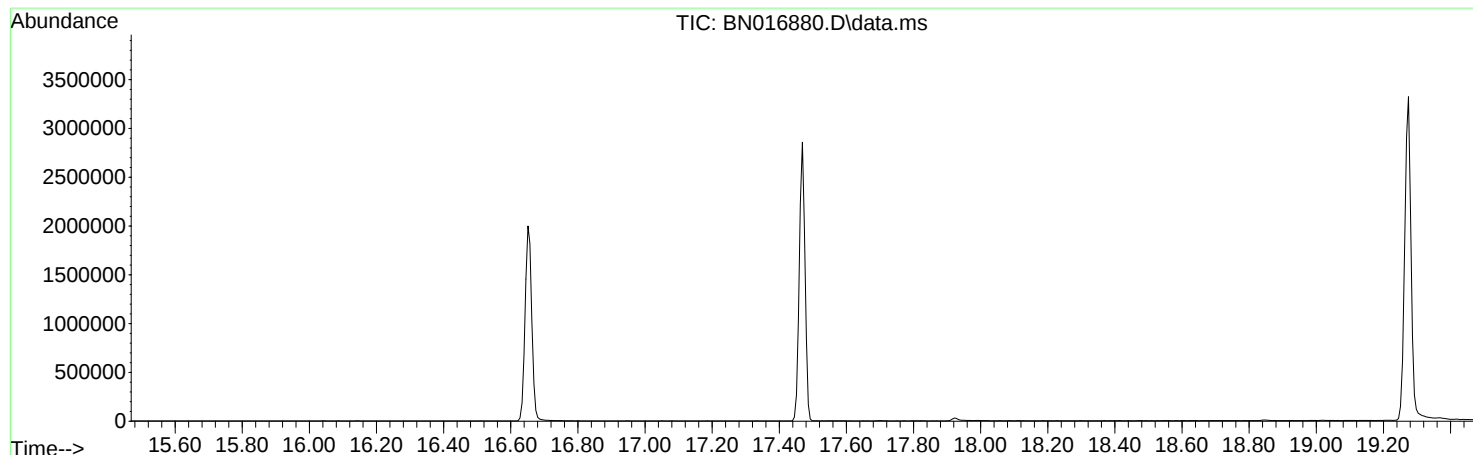

AutoFind: Scans 2444, 2445, 2446; Background Corrected with Scan 2437

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.0	80589	PASS
68	69	0.00	2	1.8	1501	PASS
69	198	0.00	100	33.0	85757	PASS
70	69	0.00	2	0.6	496	PASS
127	198	10	80	44.9	116621	PASS
197	198	0.00	2	0.2	451	PASS
198	198	100	100	100.0	259947	PASS
199	198	5	9	6.7	17378	PASS
275	198	10	60	29.4	76336	PASS
365	198	1	100	4.0	10472	PASS
441	198	0.01	100	19.7	51232	PASS
442	442	50	100	100.0	330645	PASS
443	442	15	24	21.1	69907	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/11/2021	BNA_N	<u>BN016880.D</u>
Compound Name	Response	Retention Time
DDT	907305	20.51
DDD	46861	20.07
DDE	497	19.56
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
47358	954663	4.96

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101121\
 Data File : BN016880.D
 Acq On : 11 Oct 2021 11:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Oct 11 13:04:36 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 30 18:14:09 2021
 Response via : Initial Calibration

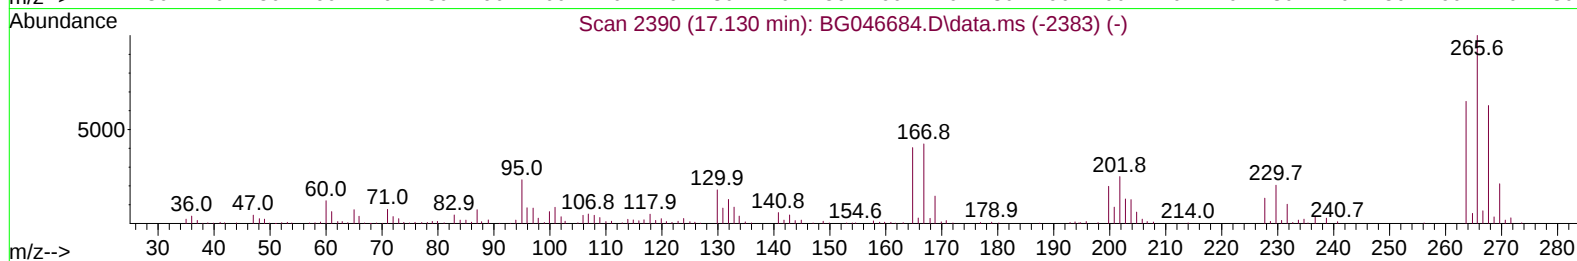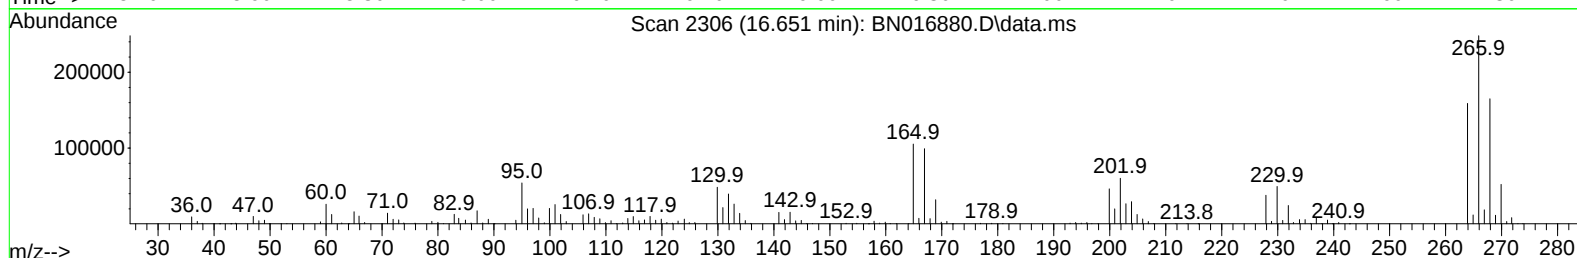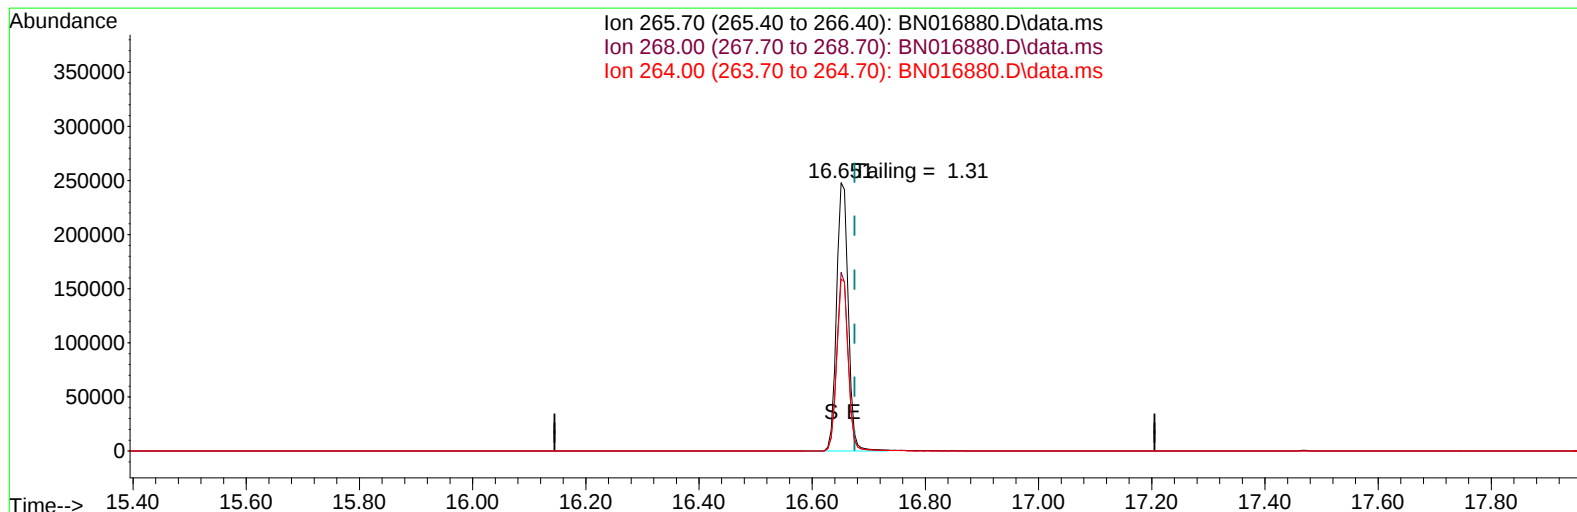

TIC: BN016880.D\data.ms

(70) Pentachlorophenol (C)

16.651min (-0.024) 34327.99 ng m




response 355874

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.54
264.00	61.60	64.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101121\
Data File : BN016880.D
Acq On : 11 Oct 2021 11:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 11 13:04:36 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 18:14:09 2021
Response via : Initial Calibration

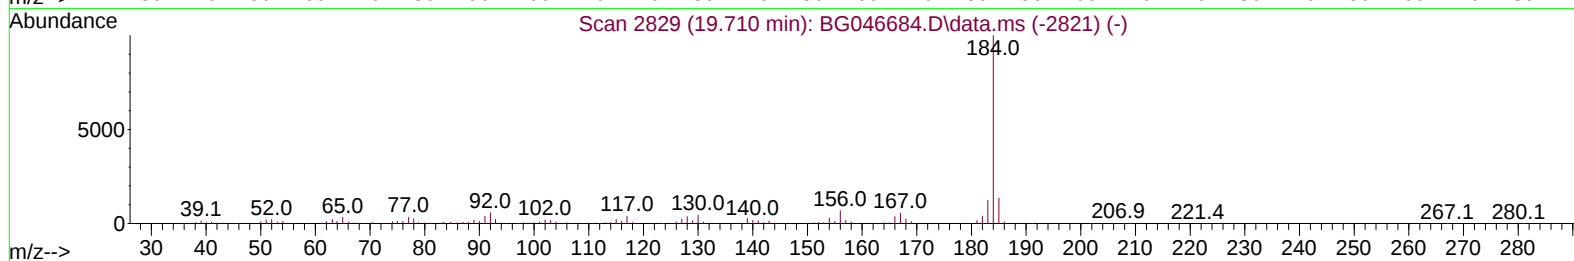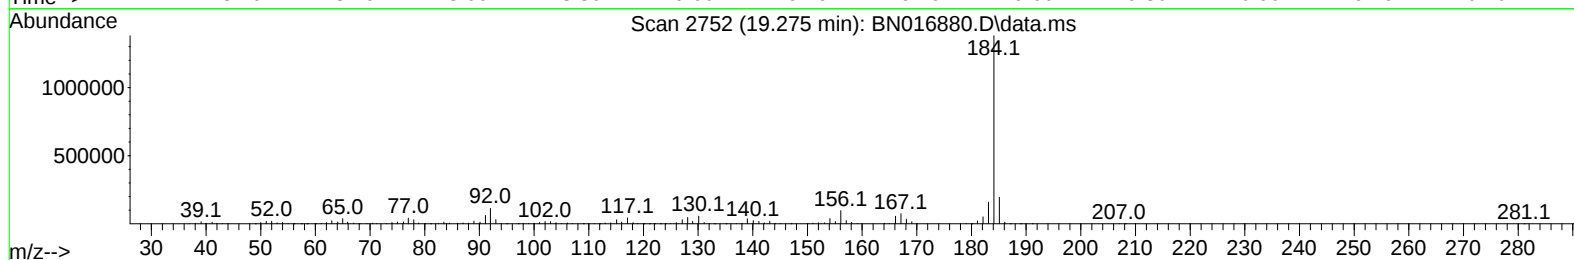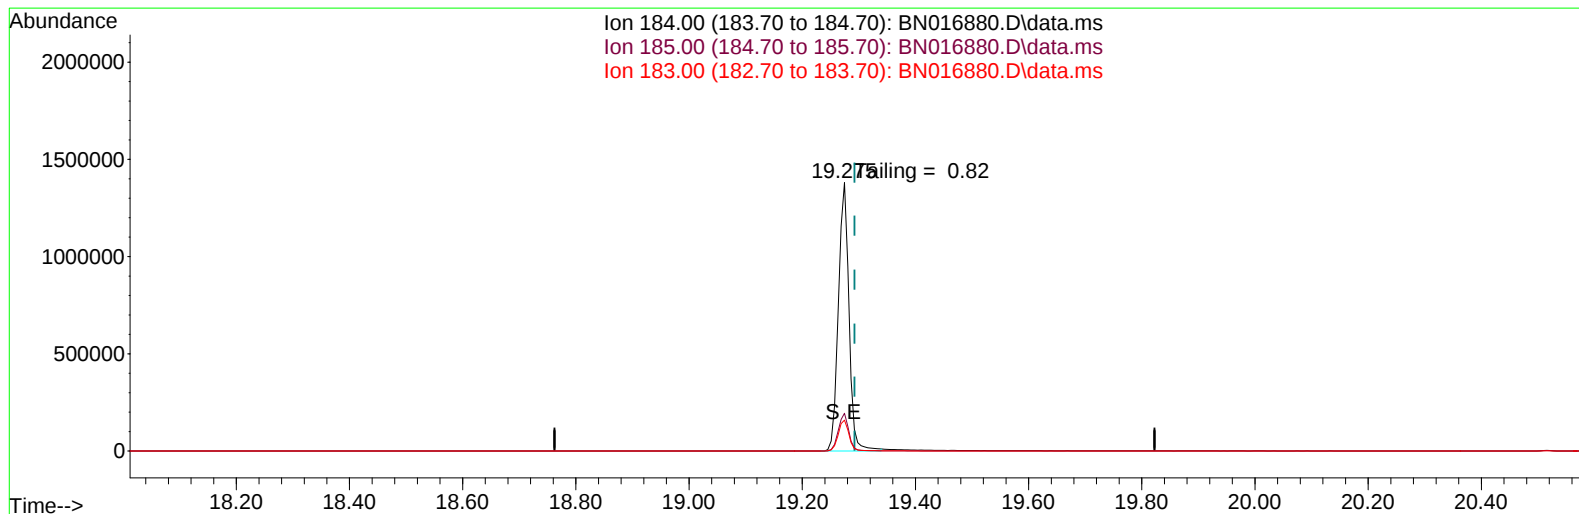

TIC: BN016880.D\data.ms

(77) Benzidine

19.275min (-0.018) 0.00 ng

response 1832815

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.08
183.00	13.20	11.52
0.00	0.00	0.00