

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101123\
 Data File : BN028241.D
 Acq On : 11 Oct 2023 20:15
 Operator : MA/JU
 Sample : 04819-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SW-AP-01-100923-FD

Quant Time: Oct 12 04:06:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN100223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 12 04:03:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.922	152	2792	0.400	ng	0.00
7) Naphthalene-d8	10.735	136	9620	0.400	ng	# 0.00
13) Acenaphthene-d10	14.566	164	6057	0.400	ng	0.00
19) Phenanthrene-d10	17.319	188	14089	0.400	ng	0.00
29) Chrysene-d12	21.524	240	13658	0.400	ng	0.00
35) Perylene-d12	23.993	264	14844	0.400	ng	0.02
System Monitoring Compounds						
4) 2-Fluorophenol	5.459	112	1030	0.124	ng	0.00
5) Phenol-d6	7.098	99	779	0.074	ng	0.00
8) Nitrobenzene-d5	9.123	82	2060	0.252	ng	0.00
11) 2-Methylnaphthalene-d10	12.321	152	4205	0.295	ng	0.00
14) 2,4,6-Tribromophenol	16.065	330	1096	0.395	ng	-0.01
15) 2-Fluorobiphenyl	13.187	172	6031	0.276	ng	0.00
27) Fluoranthene-d10	19.356	212	13913	0.393	ng	0.00
31) Terphenyl-d14	19.946	244	12151	0.381	ng	0.00
Target Compounds						
						Qvalue
3) n-Nitrosodimethylamine	3.769	42	99	0.028	ng	# 1
20) 4,6-Dinitro-2-methylph...	16.773	198	4	0.021	ng	# 1
28) Fluoranthene	19.388	202	1373	0.031	ng	# 67
30) Pyrene	19.755	202	1277	0.025	ng	95
32) Benzo(a)anthracene	21.507	228	1367	0.029	ng	# 56
33) Chrysene	21.560	228	1875	0.042	ng	# 66
34) Bis(2-ethylhexyl)phtha...	21.372	149	13950	0.456	ng	99
36) Indeno(1,2,3-cd)pyrene	26.595	276	1344	0.027	ng	# 81
37) Benzo(b)fluoranthene	23.233	252	2520	0.053	ng	# 1
39) Benzo(a)pyrene	23.885	252	942	0.021	ng	# 1
41) Benzo(g,h,i)perylene	27.408	276	1363	0.033	ng	# 18


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101123\
Data File : BN028241.D
Acq On : 11 Oct 2023 20:15
Operator : MA/JU
Sample : 04819-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SW-AP-01-100923-FD


Quant Time: Oct 12 04:06:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN100223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 12 04:03:12 2023
Response via : Initial Calibration

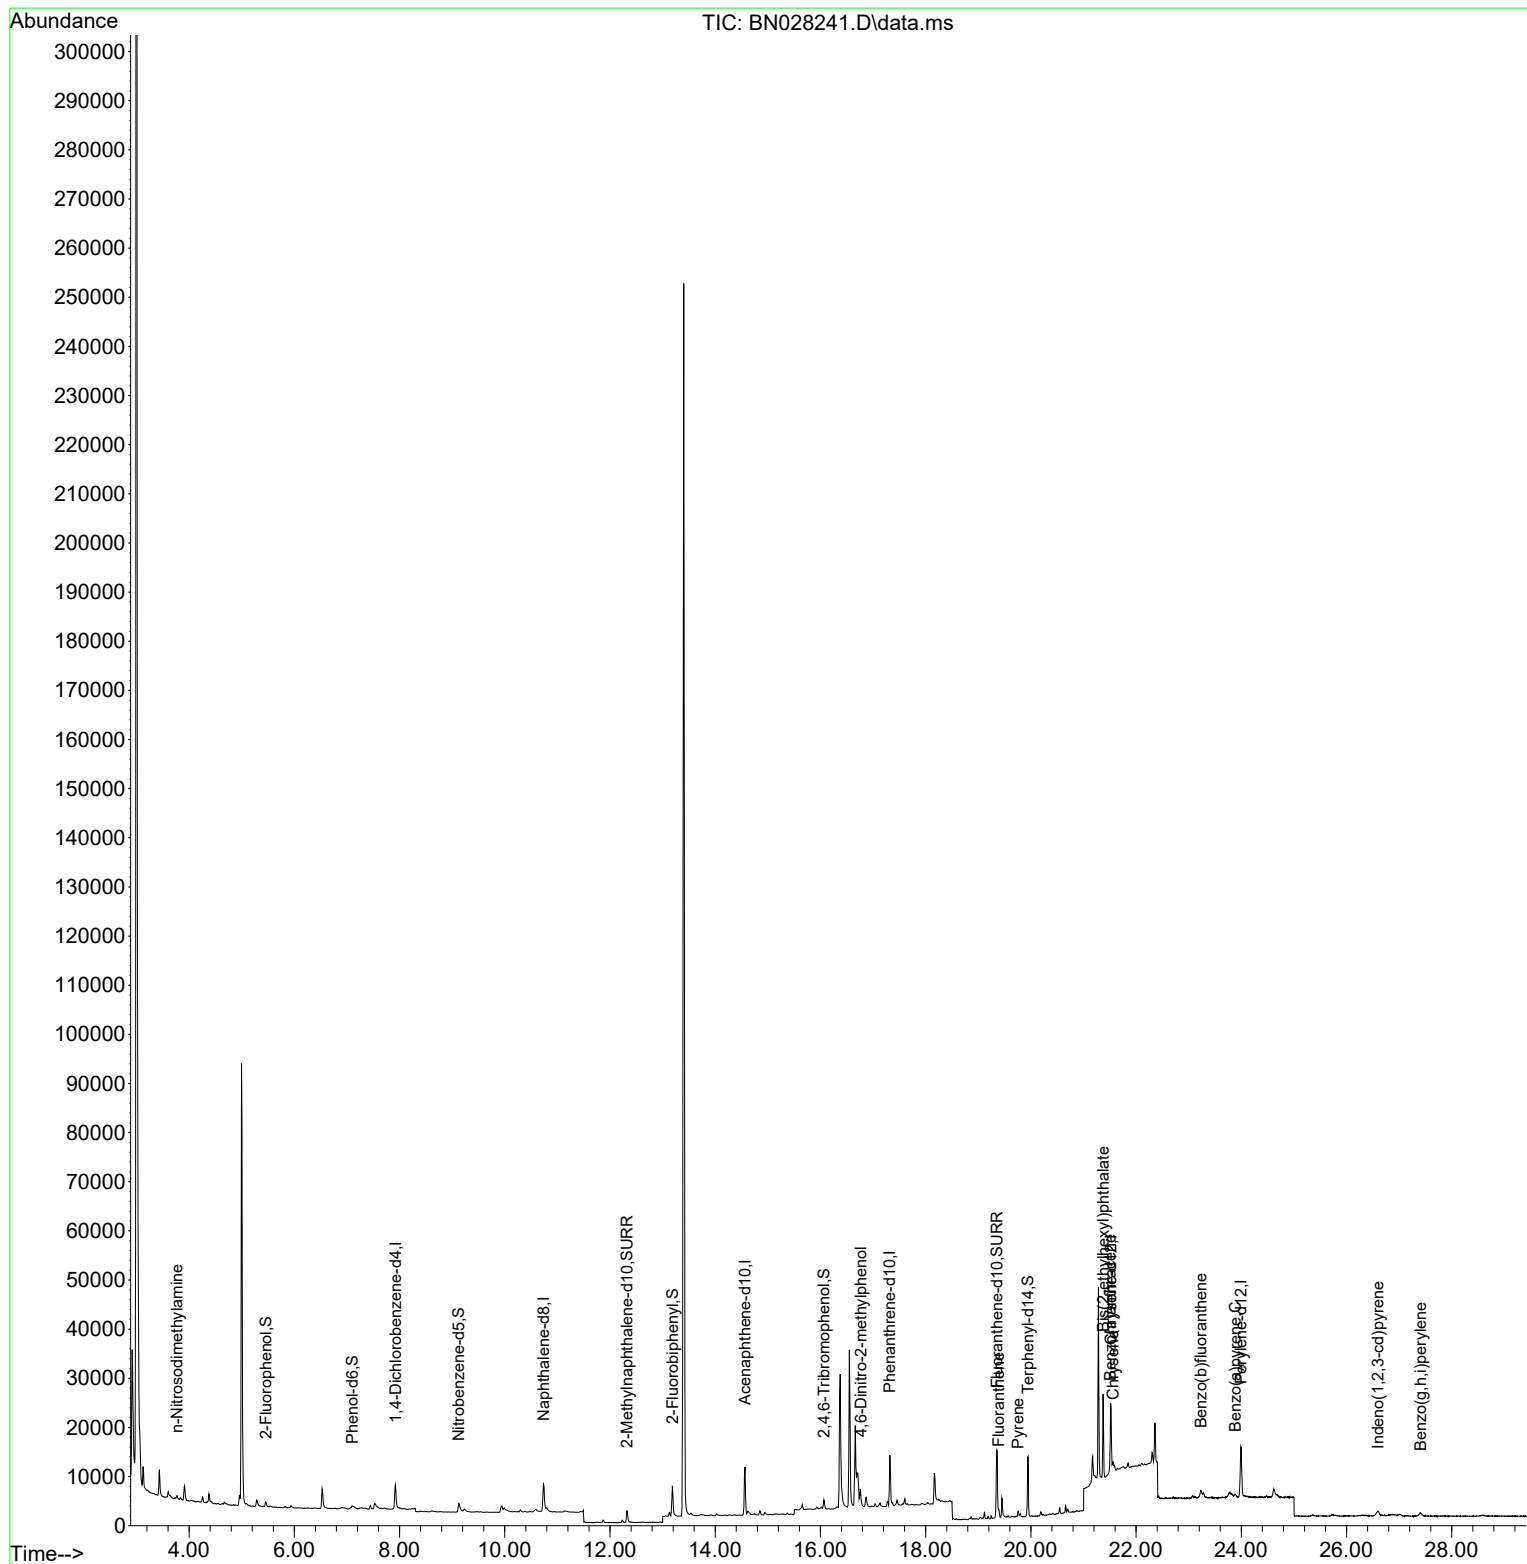



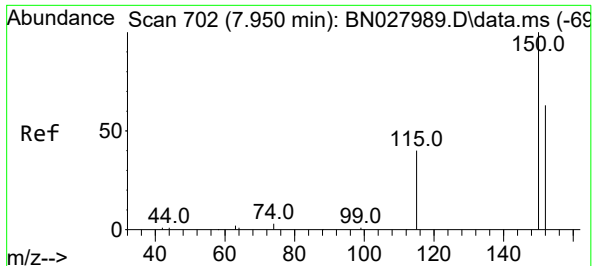


#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.922 min Scan# 61
Delta R.T. -0.000 min
Lab File: BN028241.D
Acq: 11 Oct 2023 20:15

Instrument :
BNA_N
ClientSampleId :
SW-AP-01-100923-FD



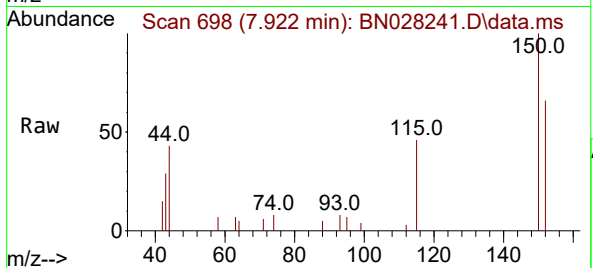



Tgt Ion:152 Resp: 2792
Ion Ratio Lower Upper
152 100
150 150.5 125.6 188.4
115 69.4 54.8 82.2

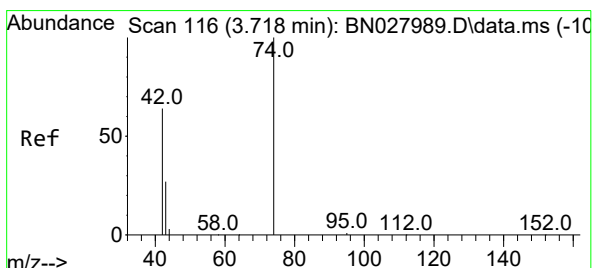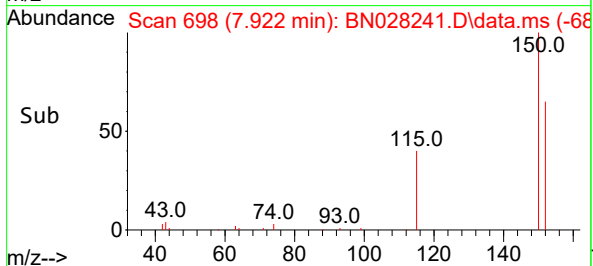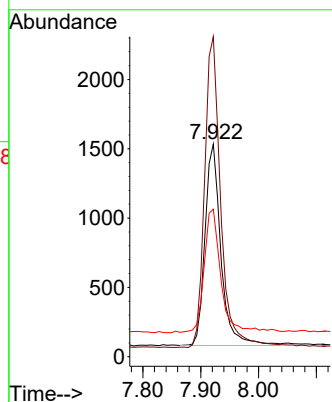

#3
n-Nitrosodimethylamine
Concen: 0.028 ng
RT: 3.769 min Scan# 123
Delta R.T. 0.058 min
Lab File: BN028241.D
Acq: 11 Oct 2023 20:15

Tgt Ion: 42 Resp: 99
Ion Ratio Lower Upper
42 100
74 6.1 115.9 173.9#
44 19.2 8.0 12.0#

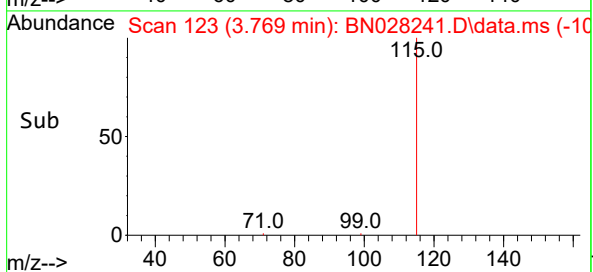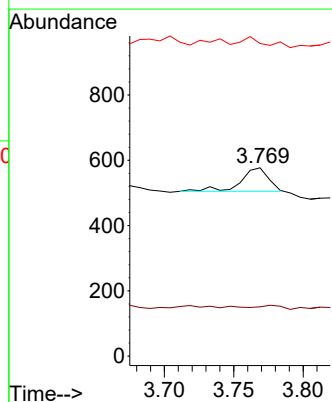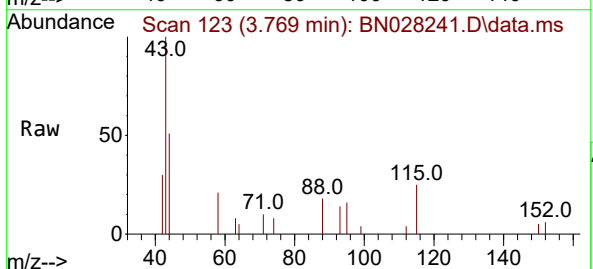

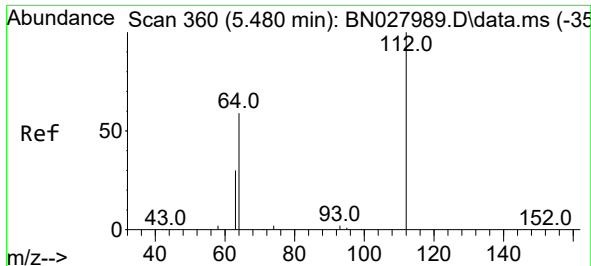

#4

2-Fluorophenol

Concen: 0.124 ng

RT: 5.459 min Scan# 3

Delta R.T. -0.007 min

Lab File: BN028241.D

Acq: 11 Oct 2023 20:15

Instrument :

BNA_N

ClientSampleId :

SW-AP-01-100923-FD





Tgt Ion:112 Resp: 1030

Ion Ratio Lower Upper

112 100

64 58.6 45.0 67.6

63 35.3 23.4 35.0#

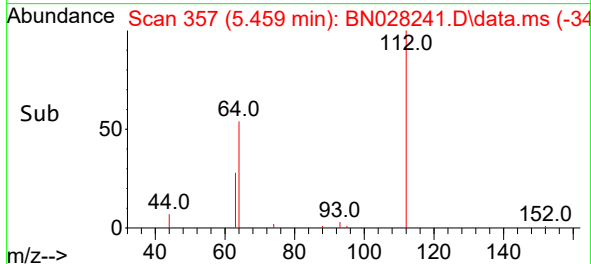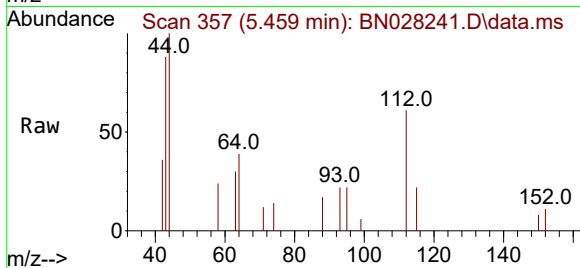

#5

Phenol-d6

Concen: 0.074 ng

RT: 7.098 min Scan# 584

Delta R.T. 0.007 min

Lab File: BN028241.D

Acq: 11 Oct 2023 20:15




Tgt Ion: 99 Resp: 779


Ion Ratio Lower Upper

99 100

42 0.0 14.6 22.0#

71 46.3 28.3 42.5#

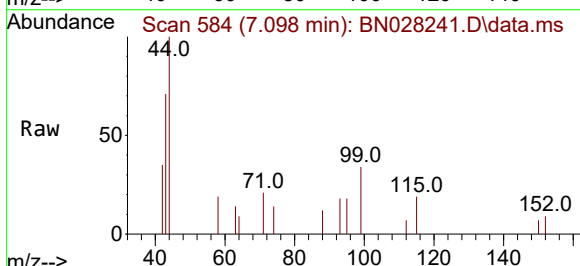



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.735 min Scan# 91

Delta R.T. 0.000 min

Lab File: BN028241.D

Acq: 11 Oct 2023 20:15

Instrument :

BNA_N

ClientSampleId :

SW-AP-01-100923-FD

Tgt Ion:136 Resp: 9620





Ion Ratio Lower Upper

136 100

137 12.1 9.4 14.0

54 10.3 7.0 10.6

68 9.7 6.4 9.6#

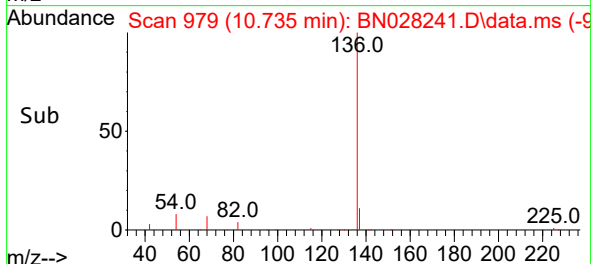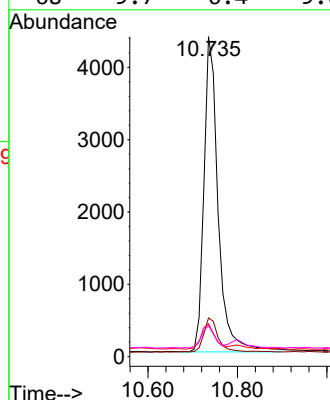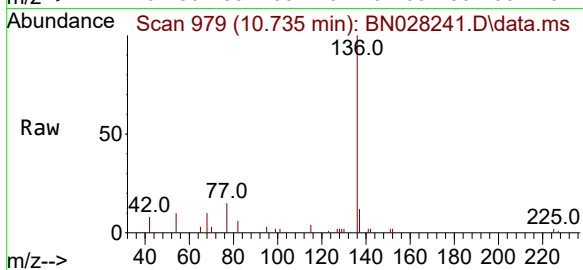

#8

Nitrobenzene-d5

Concen: 0.252 ng

RT: 9.123 min Scan# 828

Delta R.T. 0.000 min

Lab File: BN028241.D

Acq: 11 Oct 2023 20:15




Tgt Ion: 82 Resp: 2060


Ion Ratio Lower Upper

82 100

128 43.9 32.7 49.1

54 55.2 38.7 58.1

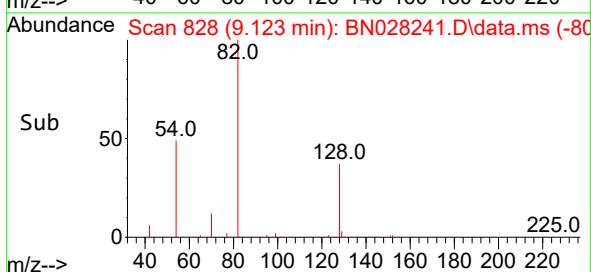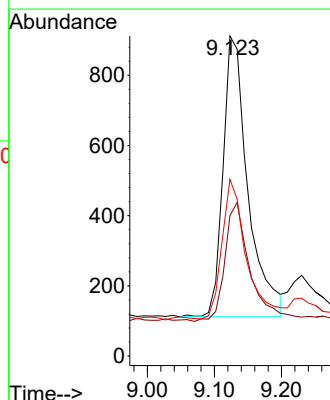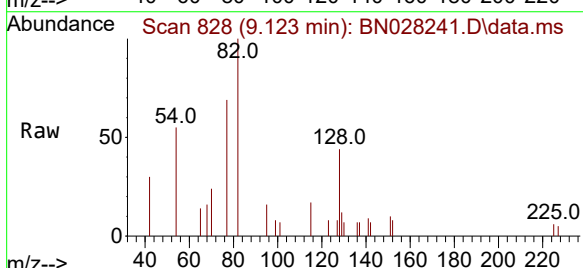

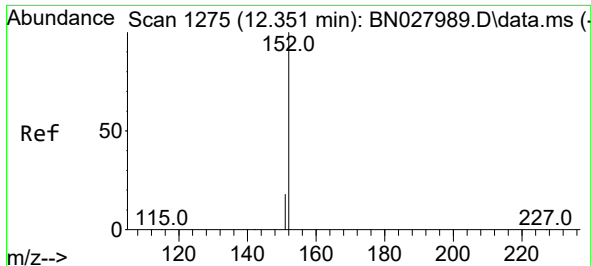

#11

2-Methylnaphthalene-d10

Concen: 0.295 ng

RT: 12.321 min Scan# 11

Delta R.T. -0.004 min

Lab File: BN028241.D

Acq: 11 Oct 2023 20:15

Instrument :

BNA_N

ClientSampleId :





SW-AP-01-100923-FD

Tgt Ion:152 Resp: 4205

Ion Ratio Lower Upper

152 100

151 19.1 16.5 24.7

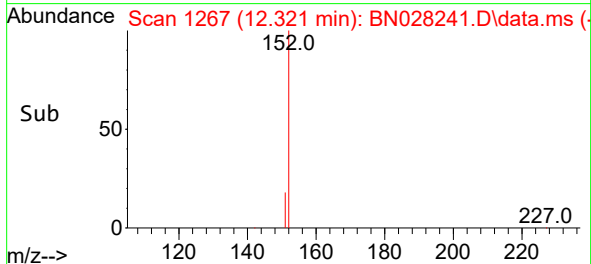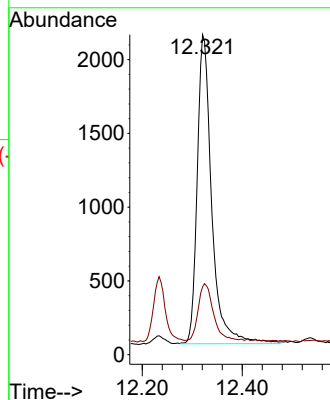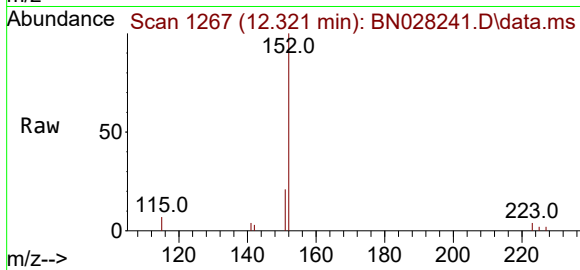

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.566 min Scan# 1594

Delta R.T. 0.000 min

Lab File: BN028241.D

Acq: 11 Oct 2023 20:15




Tgt Ion:164 Resp: 6057


Ion Ratio Lower Upper

164 100

162 101.3 80.8 121.2

160 45.9 36.4 54.6



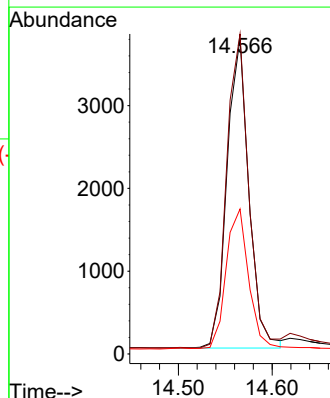
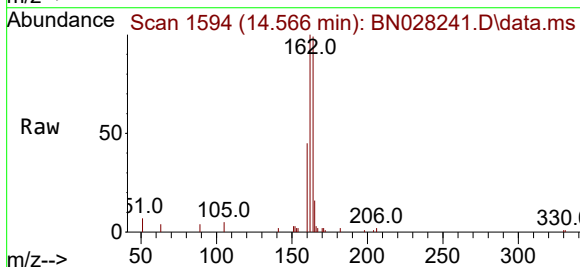


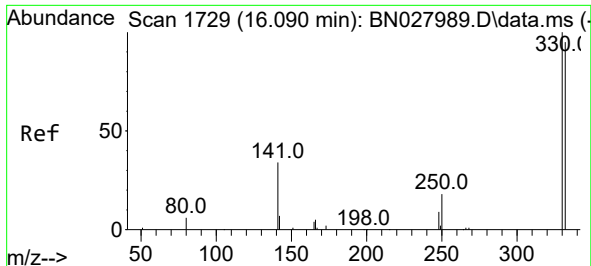

#14
2,4,6-Tribromophenol
Concen: 0.395 ng
RT: 16.065 min Scan# 11
Delta R.T. -0.012 min
Lab File: BN028241.D
Acq: 11 Oct 2023 20:15




Instrument :
BNA_N
ClientSampleId :
SW-AP-01-100923-FD


Tgt Ion:330 Resp: 1096
Ion Ratio Lower Upper
330 100
332 95.9 78.1 117.1
141 42.0 33.4 50.2

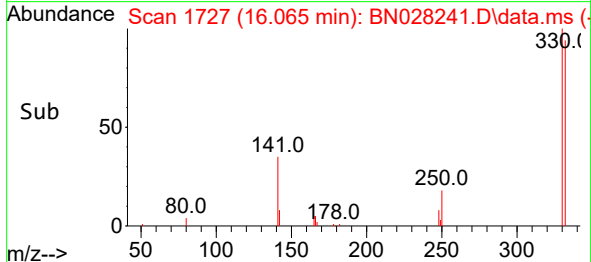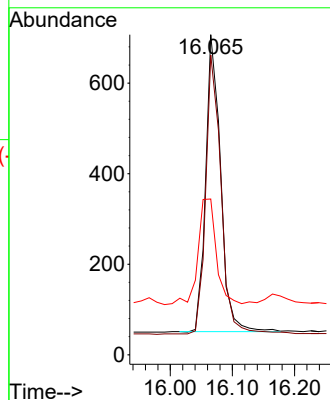

#15
2-Fluorobiphenyl
Concen: 0.276 ng
RT: 13.187 min Scan# 1465
Delta R.T. 0.000 min
Lab File: BN028241.D
Acq: 11 Oct 2023 20:15

Tgt Ion:172 Resp: 6031
Ion Ratio Lower Upper
172 100
171 36.4 28.1 42.1
170 24.3 18.4 27.6

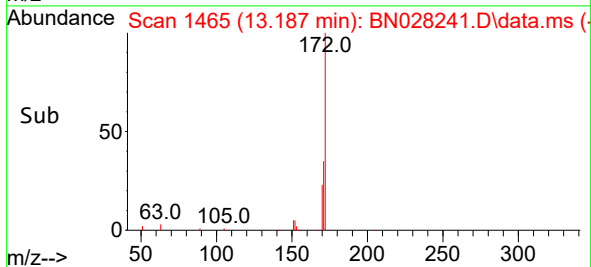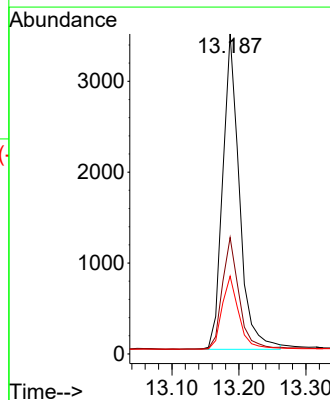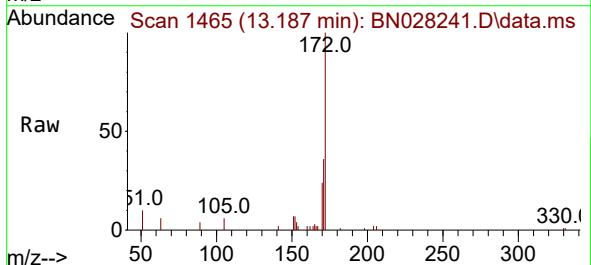



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.319 min Scan# 1828

Delta R.T. 0.000 min

Lab File: BN028241.D

Acq: 11 Oct 2023 20:15

Instrument :

BNA_N

ClientSampleId :

SW-AP-01-100923-FD





Tgt Ion:188 Resp: 14089

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 14.8 10.2 15.4

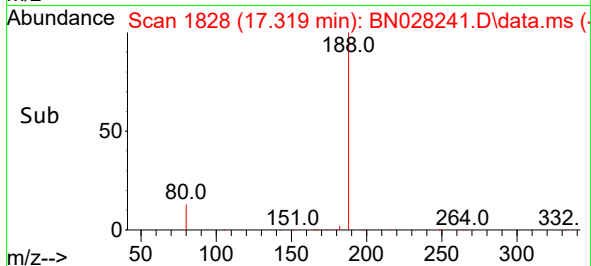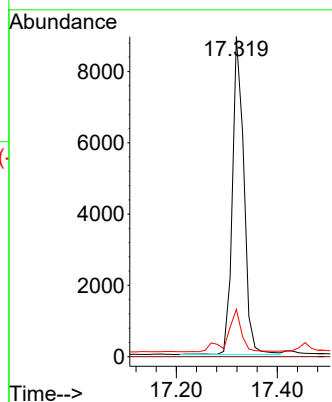

#20

4,6-Dinitro-2-methylphenol

Concen: 0.021 ng

RT: 16.773 min Scan# 1784

Delta R.T. -0.012 min

Lab File: BN028241.D

Acq: 11 Oct 2023 20:15




Tgt Ion:198 Resp: 4


Ion Ratio Lower Upper

198 100

51 656.5 180.7 271.1#

105 2301.6 222.2 333.2#


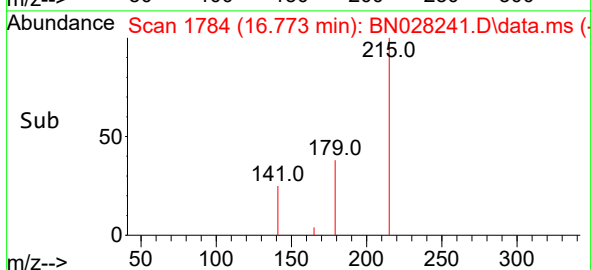

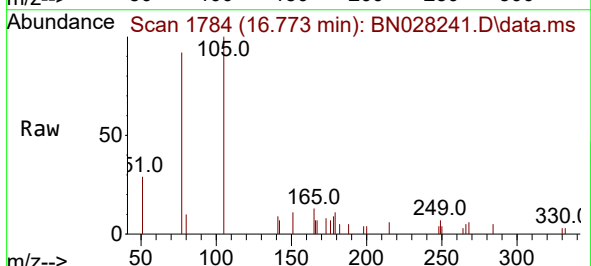


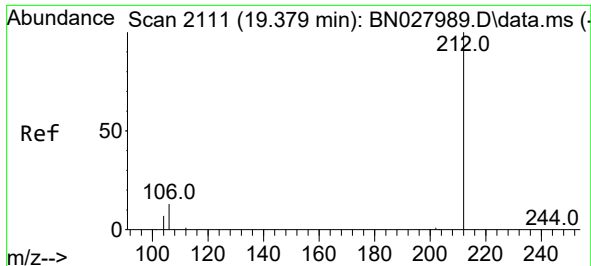

#27
Fluoranthene-d10
Concen: 0.393 ng
RT: 19.356 min Scan# 2113
Delta R.T. 0.000 min
Lab File: BN028241.D
Acq: 11 Oct 2023 20:15




Instrument :
BNA_N
ClientSampleId :
SW-AP-01-100923-FD


Tgt Ion:212 Resp: 13913
Ion Ratio Lower Upper
212 100
106 14.1 11.3 16.9
104 8.8 6.4 9.6

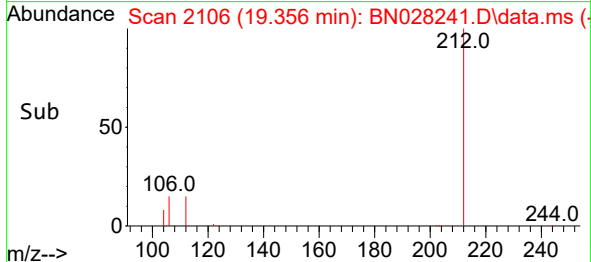

#28
Fluoranthene
Concen: 0.031 ng
RT: 19.388 min Scan# 2113
Delta R.T. 0.005 min
Lab File: BN028241.D
Acq: 11 Oct 2023 20:15

Tgt Ion:202 Resp: 1373
Ion Ratio Lower Upper
202 100
101 41.1 9.8 14.6#
203 15.2 13.8 20.8

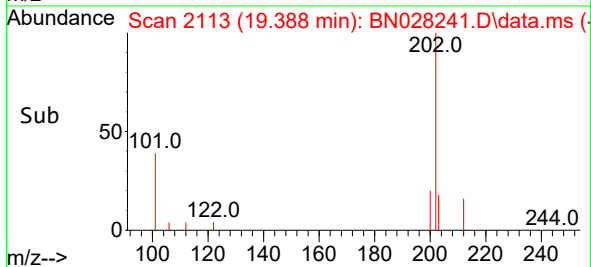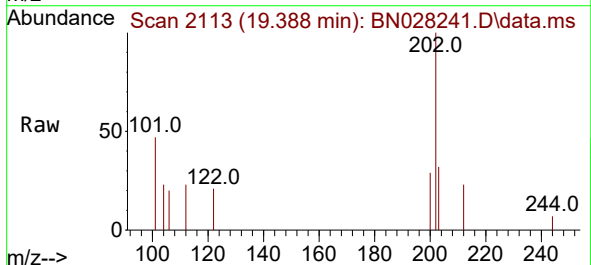

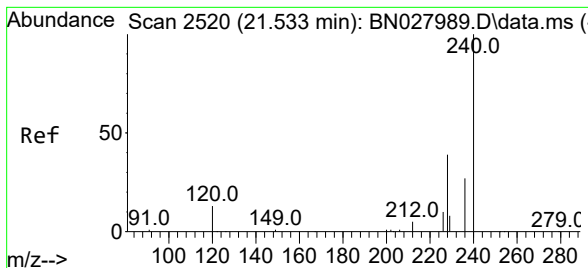

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.524 min Scan# 2119

Delta R.T. 0.009 min

Lab File: BN028241.D

Acq: 11 Oct 2023 20:15

Instrument :

BNA_N

ClientSampleId :

SW-AP-01-100923-FD





Tgt Ion:240 Resp: 13658

Ion Ratio Lower Upper

240 100

120 14.0 13.8 20.6

236 28.2 22.6 33.8

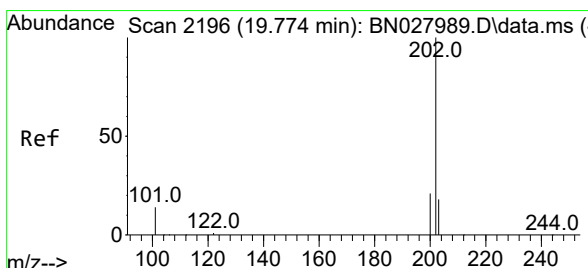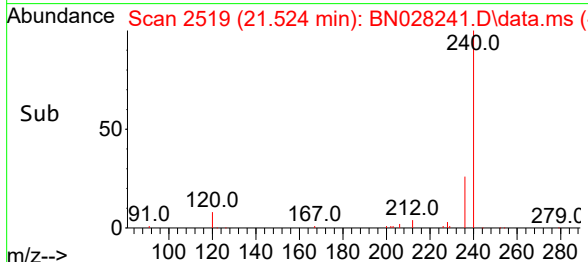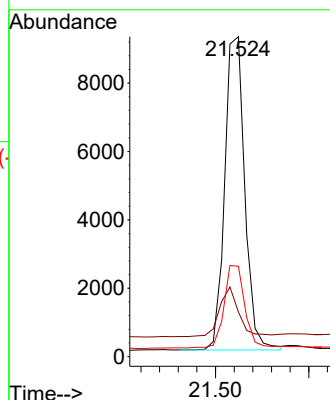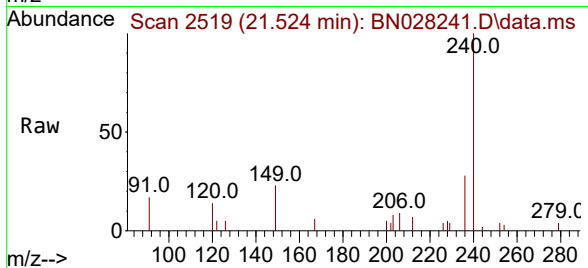

#30

Pyrene

Concen: 0.025 ng

RT: 19.755 min Scan# 2192

Delta R.T. 0.005 min

Lab File: BN028241.D

Acq: 11 Oct 2023 20:15




Tgt Ion:202 Resp: 1277


Ion Ratio Lower Upper

202 100

200 22.2 16.5 24.7

203 15.3 14.7 22.1


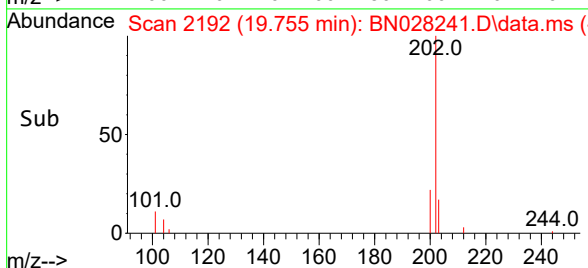
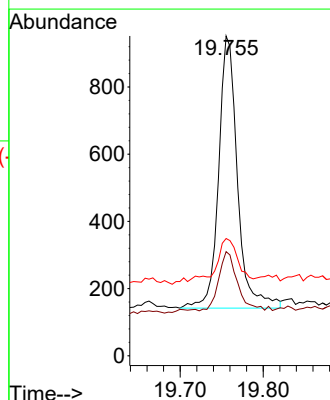
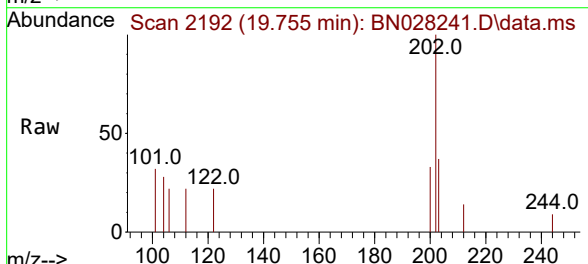


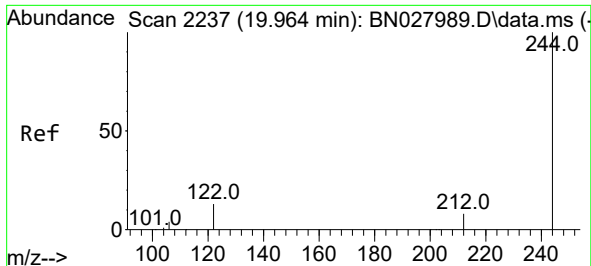

#31
 Terphenyl-d14
 Concen: 0.381 ng
 RT: 19.946 min Scan# 21
 Delta R.T. 0.005 min
 Lab File: BN028241.D
 Acq: 11 Oct 2023 20:15




Instrument :
 BNA_N
 ClientSampleId :
 SW-AP-01-100923-FD


Tgt Ion:244 Resp: 12151
 Ion Ratio Lower Upper
 244 100
 212 8.9 6.6 9.8
 122 14.7 11.4 17.0

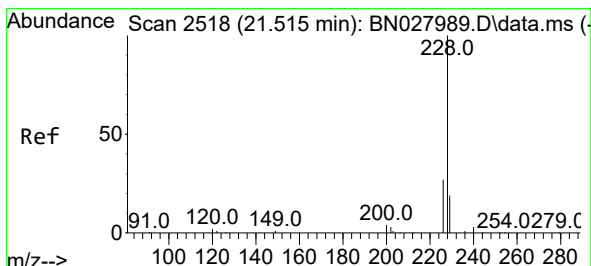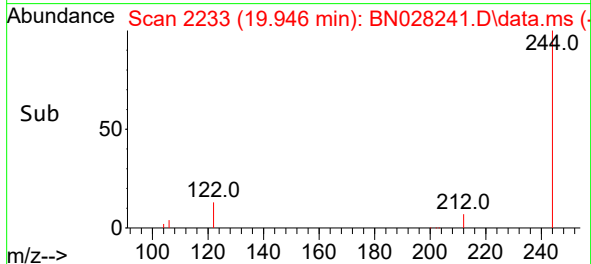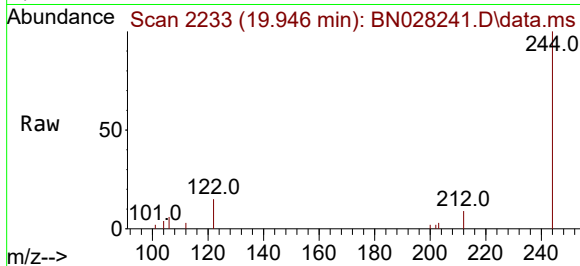

#32
 Benzo(a)anthracene
 Concen: 0.029 ng
 RT: 21.507 min Scan# 2517
 Delta R.T. 0.009 min
 Lab File: BN028241.D
 Acq: 11 Oct 2023 20:15

Tgt Ion:228 Resp: 1367
 Ion Ratio Lower Upper
 228 100
 226 46.0 22.0 33.0#
 229 45.3 16.0 24.0#

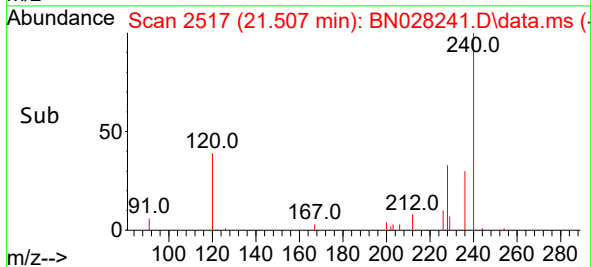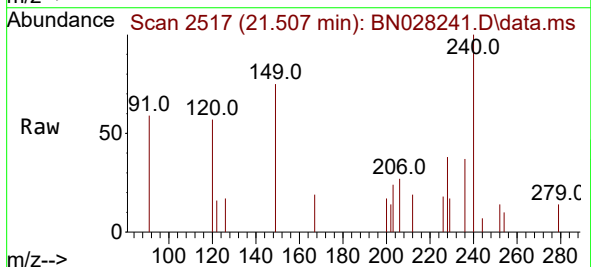

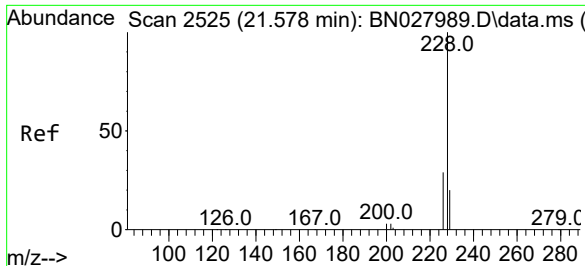

#33

Chrysene

Concen: 0.042 ng

RT: 21.560 min Scan# 21

Delta R.T. 0.009 min

Lab File: BN028241.D

Acq: 11 Oct 2023 20:15

Instrument :

BNA_N

ClientSampleId :

SW-AP-01-100923-FD





Tgt Ion:228 Resp: 1875

Ion Ratio Lower Upper

228 100

226 44.3 23.8 35.8#

229 41.2 16.6 25.0#

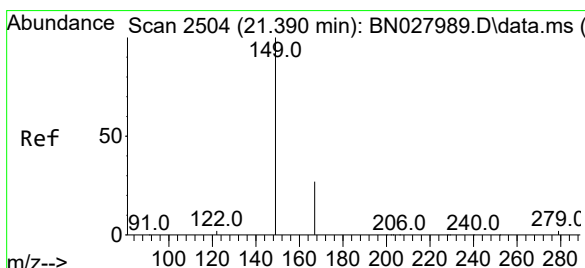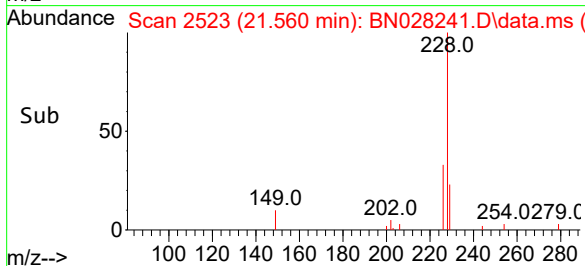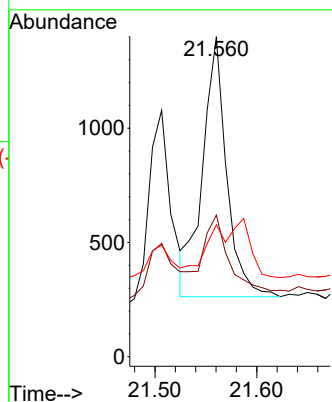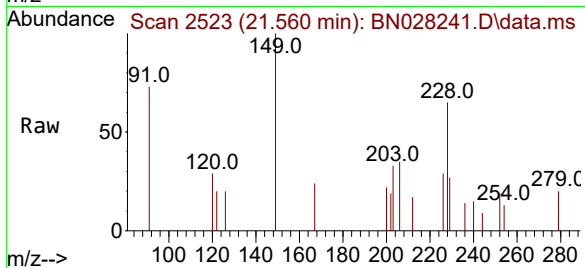

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.456 ng

RT: 21.372 min Scan# 2502

Delta R.T. 0.009 min

Lab File: BN028241.D

Acq: 11 Oct 2023 20:15




Tgt Ion:149 Resp: 13950


Ion Ratio Lower Upper

149 100

167 28.3 22.1 33.1

279 4.0 3.4 5.0


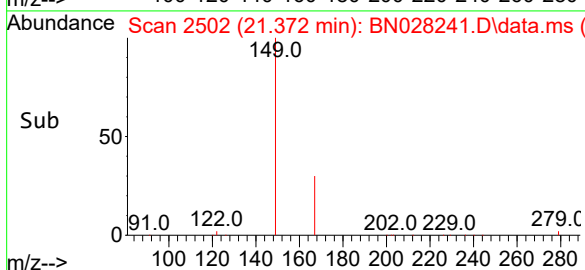

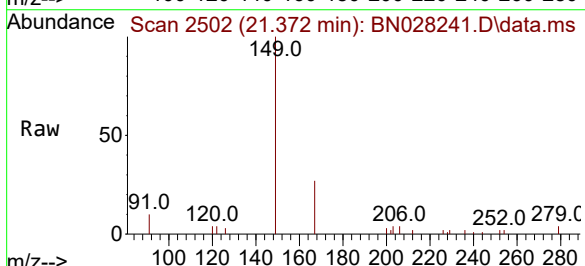


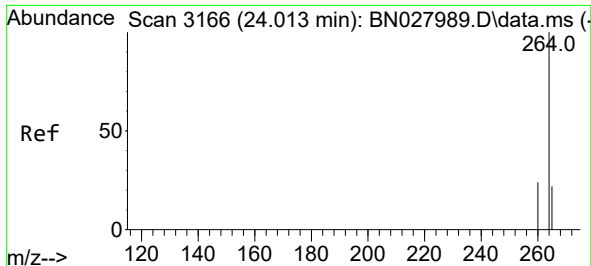

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.993 min Scan# 3166
Delta R.T. 0.018 min
Lab File: BN028241.D
Acq: 11 Oct 2023 20:15




Instrument :
BNA_N
ClientSampleId :
SW-AP-01-100923-FD


Tgt Ion:264 Resp: 14844
Ion Ratio Lower Upper
264 100
260 26.3 20.2 30.4
265 56.1 54.8 82.2

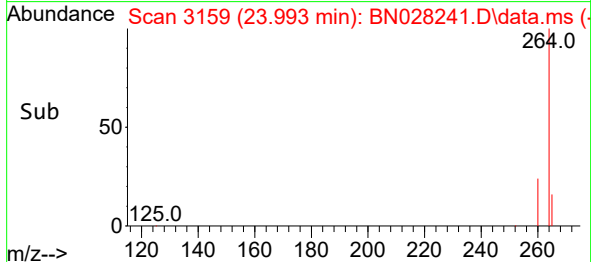

#36
Indeno(1,2,3-cd)pyrene
Concen: 0.027 ng
RT: 26.595 min Scan# 4049
Delta R.T. 0.038 min
Lab File: BN028241.D
Acq: 11 Oct 2023 20:15

Tgt Ion:276 Resp: 1344
Ion Ratio Lower Upper
276 100
138 20.3 20.9 31.3#
277 11.2 19.8 29.6#

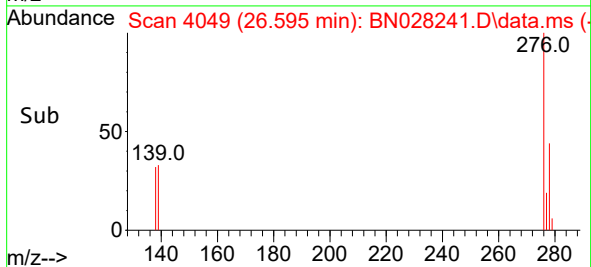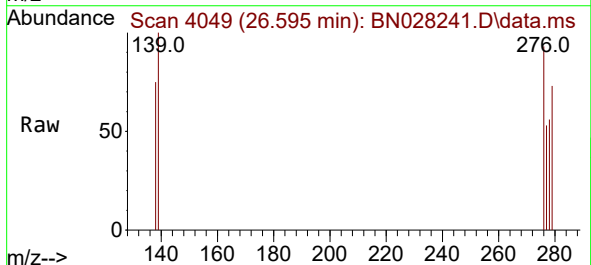



#37

Benzo(b)fluoranthene

Concen: 0.053 ng

RT: 23.233 min Scan# 21

Delta R.T. 0.021 min

Lab File: BN028241.D

Acq: 11 Oct 2023 20:15

Instrument :

BNA_N

ClientSampleId :

SW-AP-01-100923-FD





Tgt Ion:252 Resp: 2520

Ion Ratio Lower Upper

252 100

253 72.7 22.9 34.3#

125 93.3 13.8 20.8#

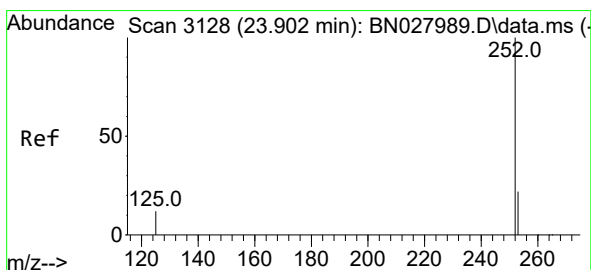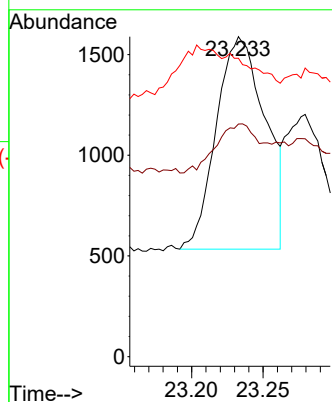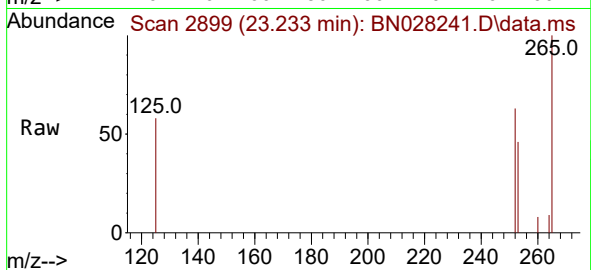

#39

Benzo(a)pyrene

Concen: 0.021 ng

RT: 23.885 min Scan# 3122

Delta R.T. 0.021 min

Lab File: BN028241.D

Acq: 11 Oct 2023 20:15




Tgt Ion:252 Resp: 942


Ion Ratio Lower Upper

252 100

253 105.9 25.0 37.4#

125 135.6 16.6 24.8#

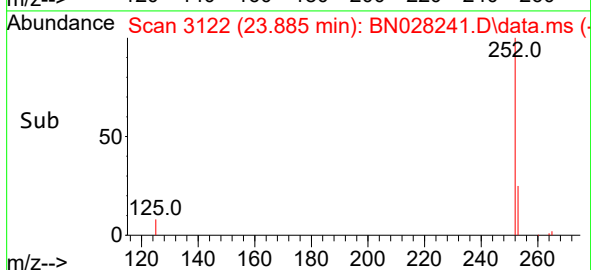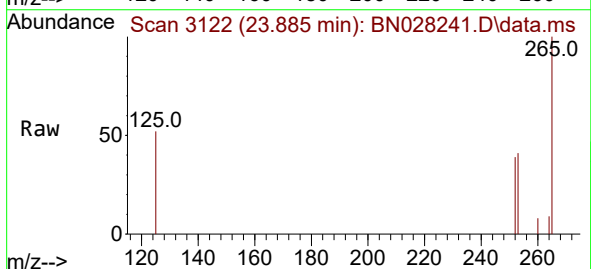

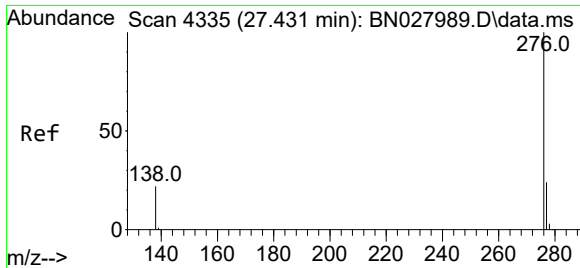

#41

Benzo(g,h,i)perylene

Concen: 0.033 ng

RT: 27.408 min Scan# 41

Delta R.T. 0.041 min

Lab File: BN028241.D


Acq: 11 Oct 2023 20:15

Instrument :

BNA_N

ClientSampleId :

SW-AP-01-100923-FD

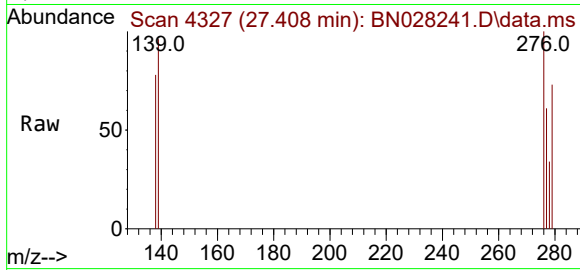

Tgt Ion:276 Resp: 1363

Ion Ratio Lower Upper

276 100

277 60.5 22.1 33.1#

138 78.1 20.8 31.2#

