
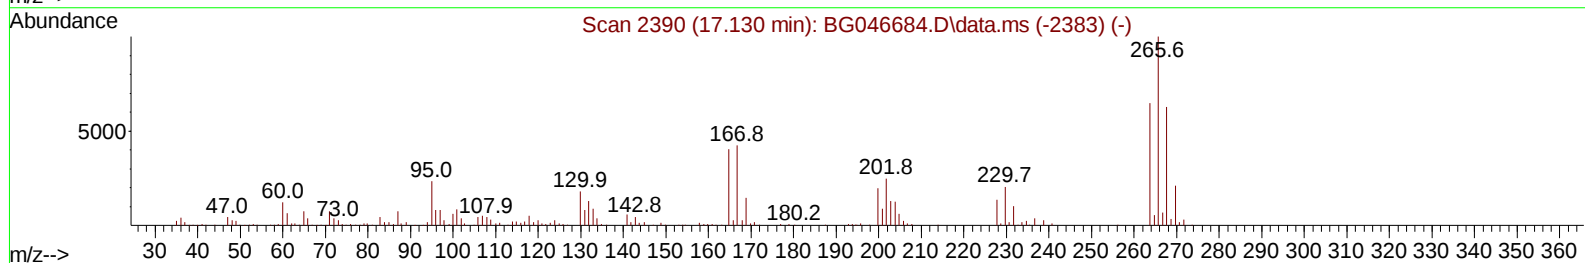
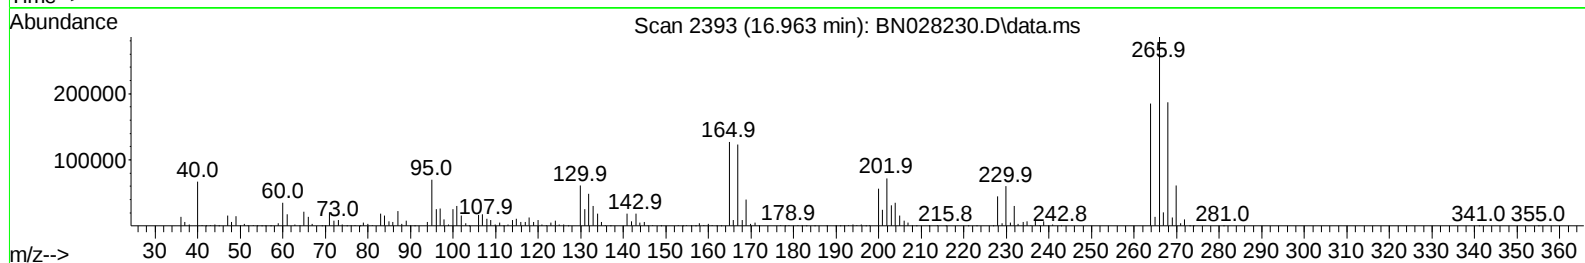


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN101123\  
Data File : BN028230.D  
Acq On : 11 Oct 2023 13:35  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 05:03:02 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Oct 12 05:02:54 2023  
Response via : Initial Calibration

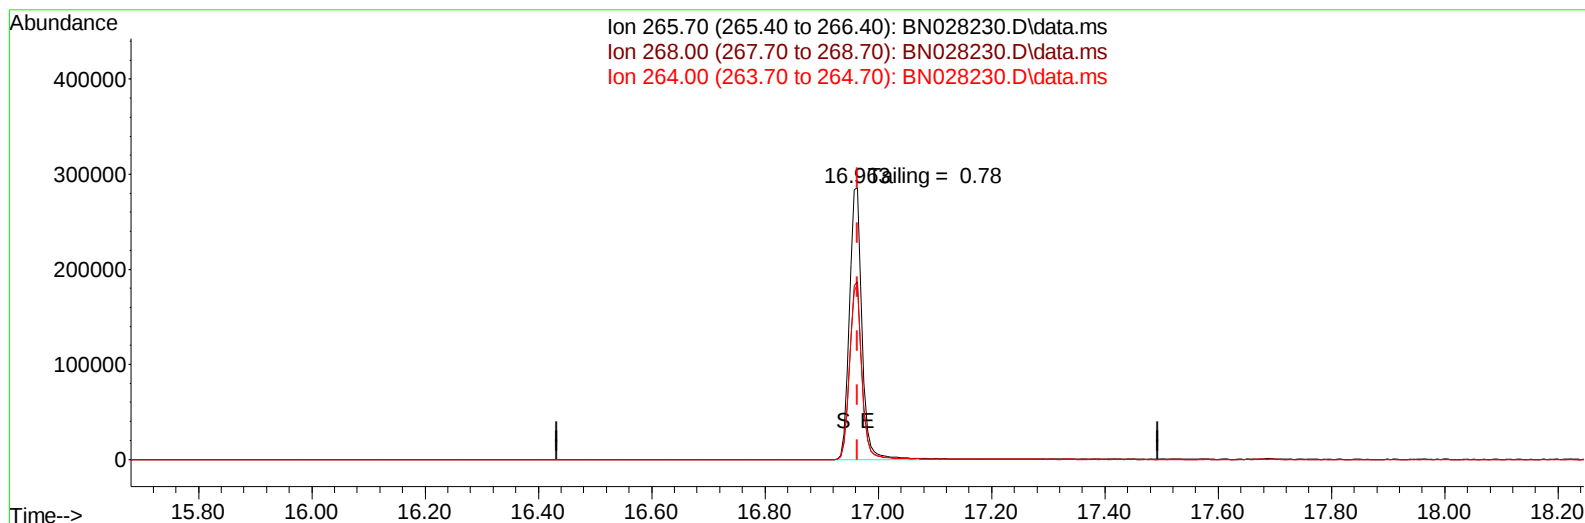

TIC: BN028230.D\data.ms

**(70) Pentachlorophenol (C)**




**16.963min ( 0.000) 23247.31 ng**

**response 442962**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 65.54  |
| 264.00 | 61.60  | 64.80  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN101123\  
Data File : BN028230.D  
Acq On : 11 Oct 2023 13:35  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 05:03:02 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Oct 12 05:02:54 2023  
Response via : Initial Calibration

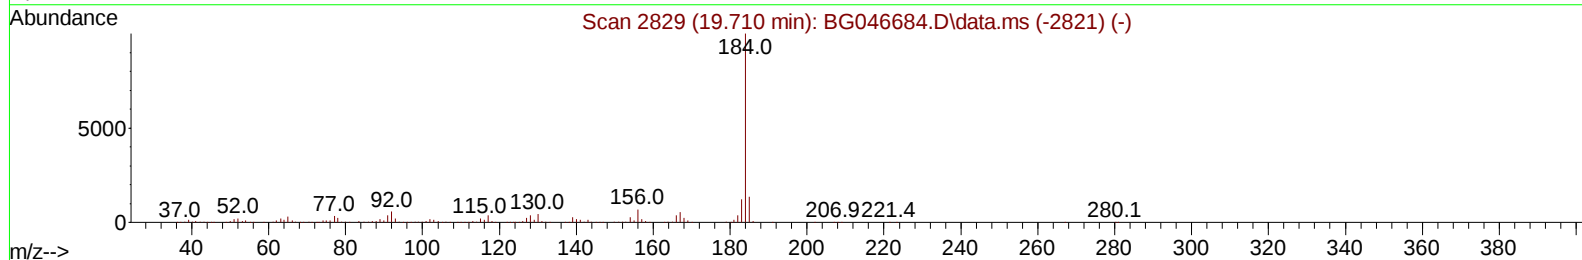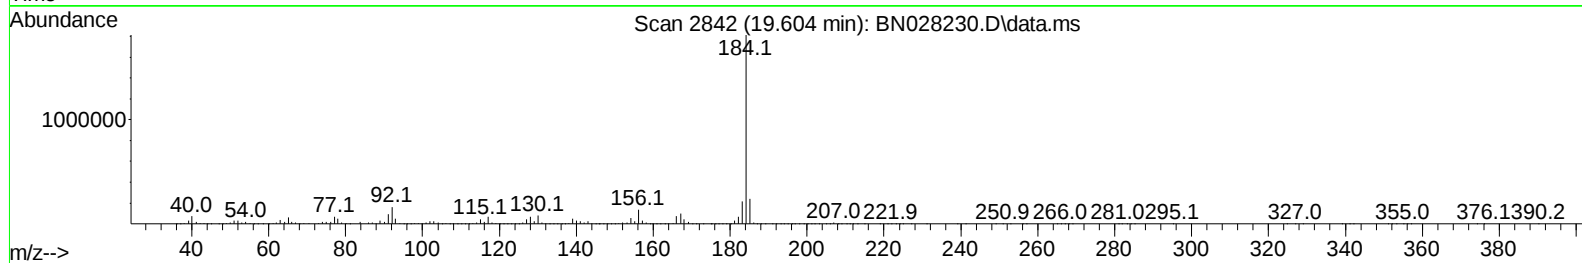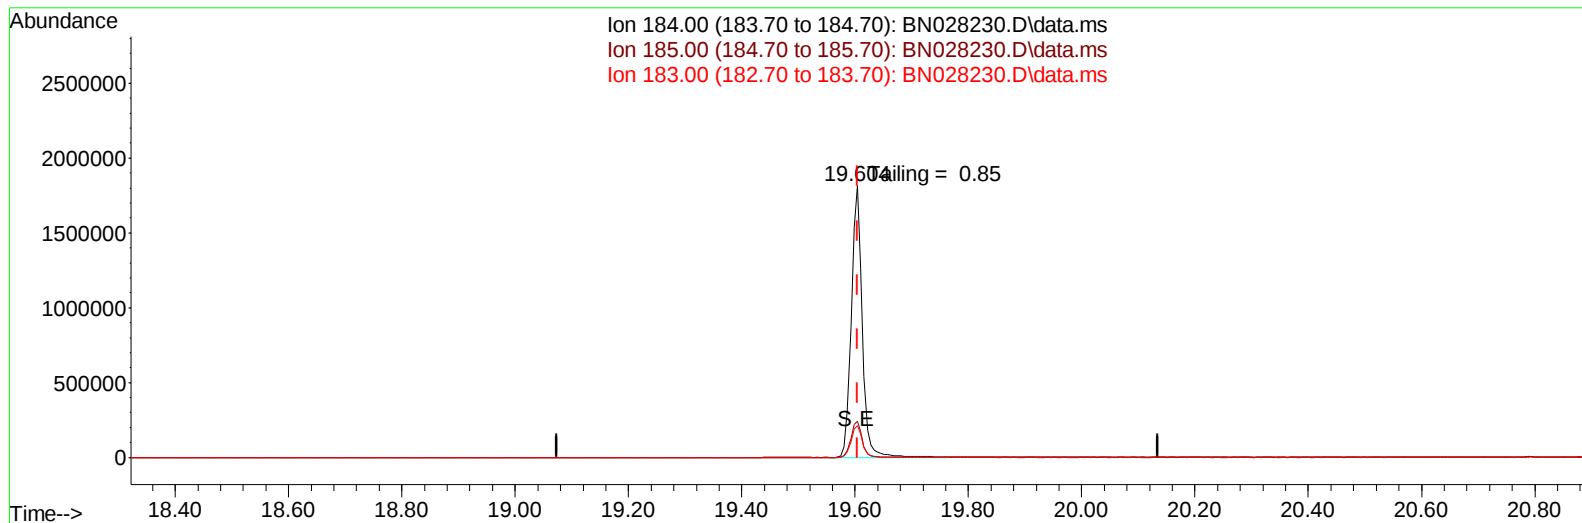

TIC: BN028230.D\data.ms

**(77) Benzidine****19.604min ( 0.000) 627488.78 ng****response 2456507**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.36  |
| 183.00 | 13.20  | 11.74  |
| 0.00   | 0.00   | 0.00   |