
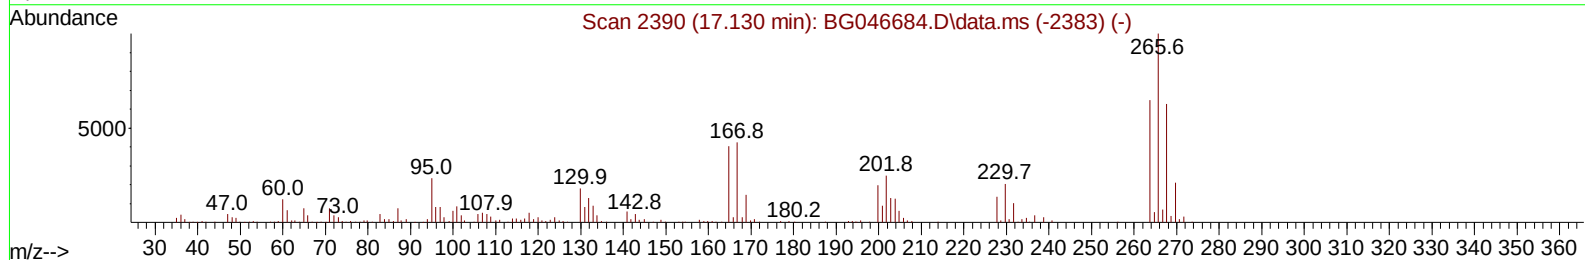
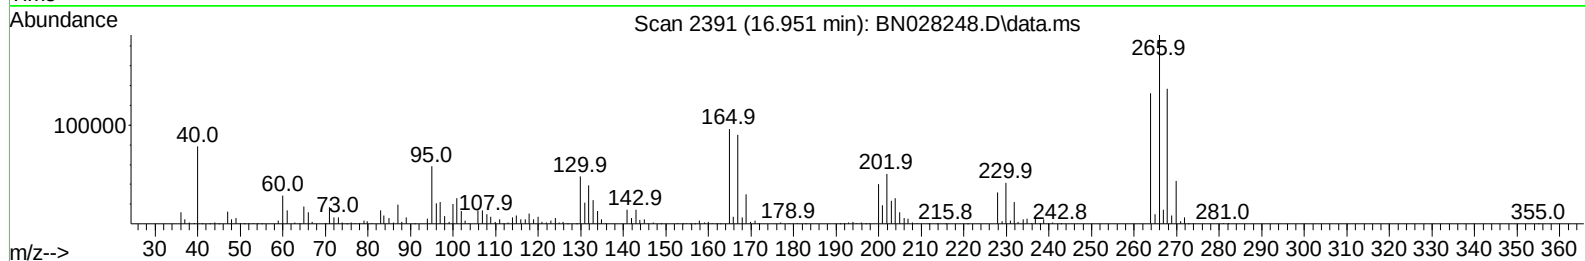


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101123\
Data File : BN028248.D
Acq On : 12 Oct 2023 01:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 05:05:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 12 05:02:54 2023
Response via : Initial Calibration

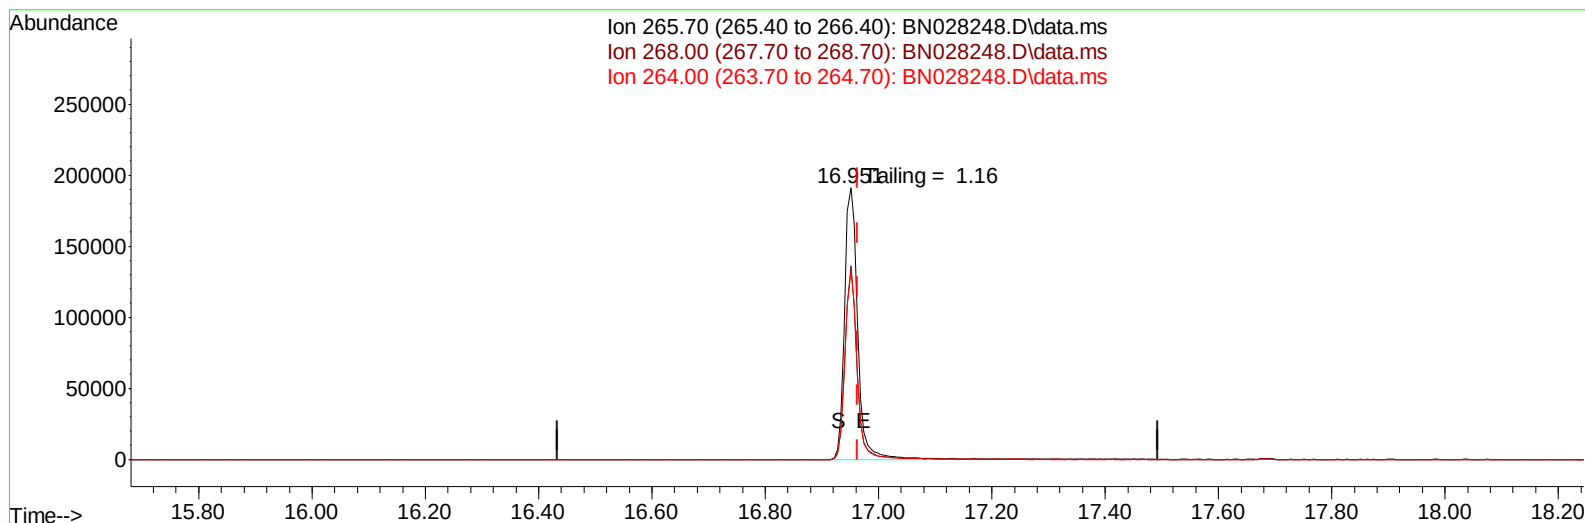

TIC: BN028248.D\data.ms

(70) Pentachlorophenol (C)




16.951min (-0.012) 21295.39 ng

response 304160

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	71.40
264.00	61.60	69.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101123\
Data File : BN028248.D
Acq On : 12 Oct 2023 01:03
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 05:05:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 12 05:02:54 2023
Response via : Initial Calibration

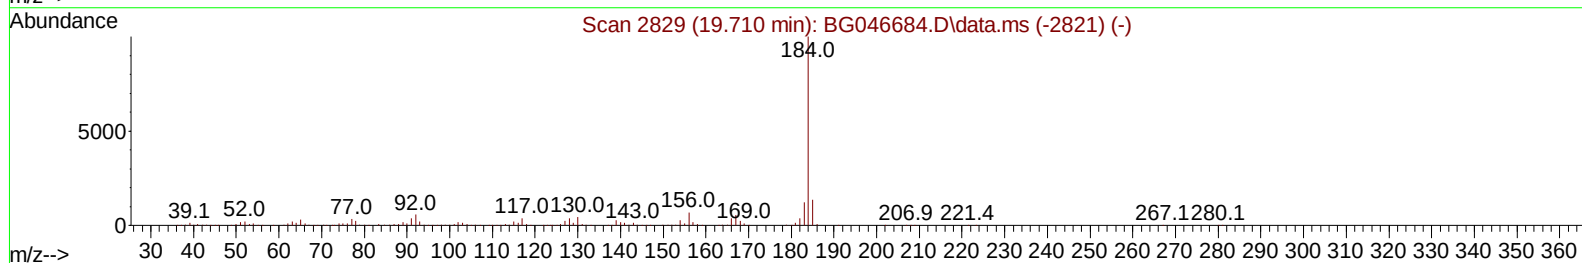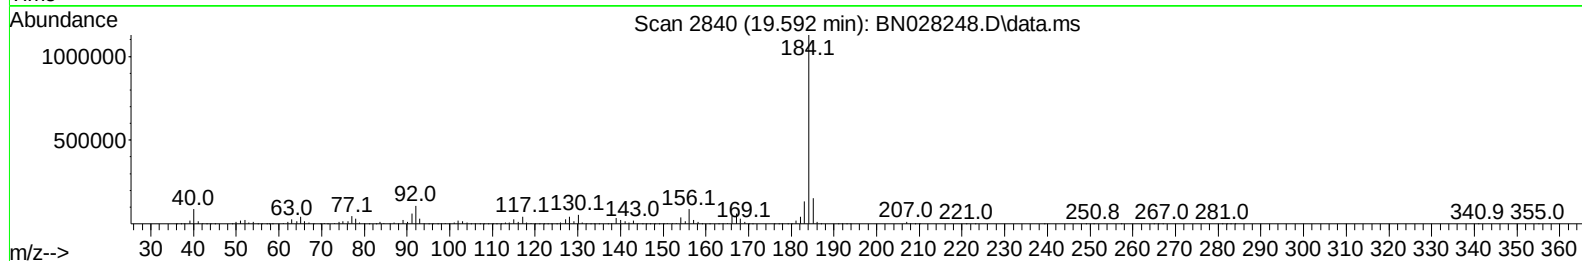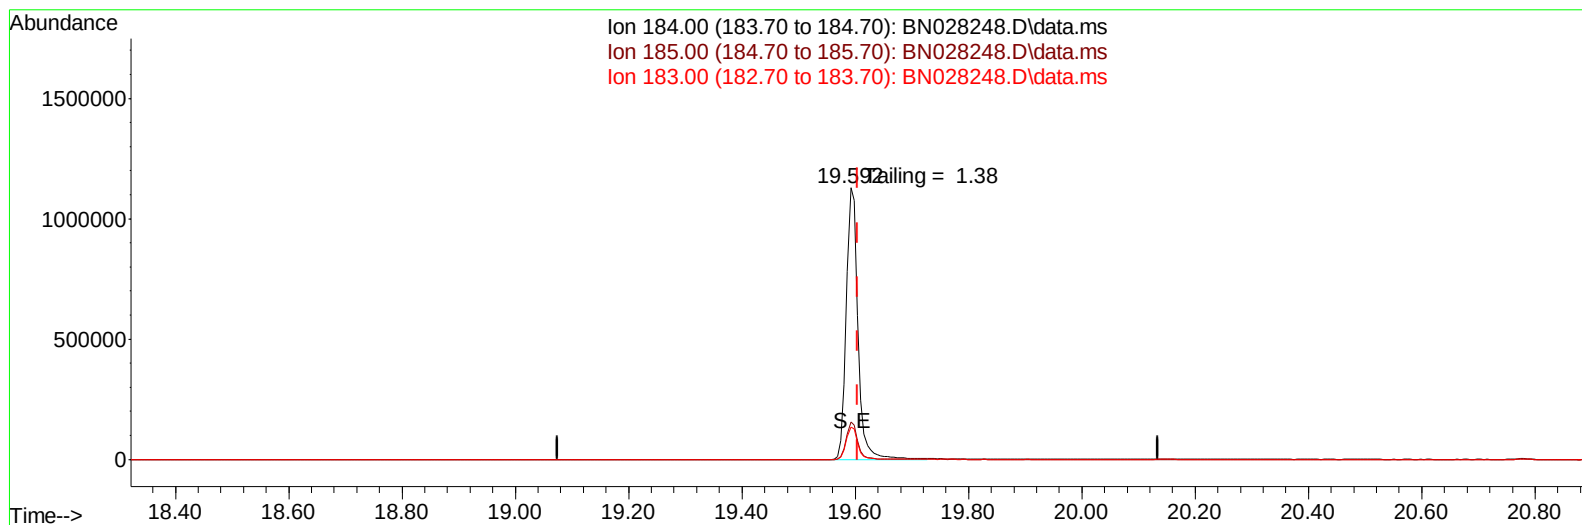

TIC: BN028248.D\data.ms

(77) Benzidine

19.592min (-0.012) 982937.29 ng

response 1636168

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.71
183.00	13.20	12.02
0.00	0.00	0.00