
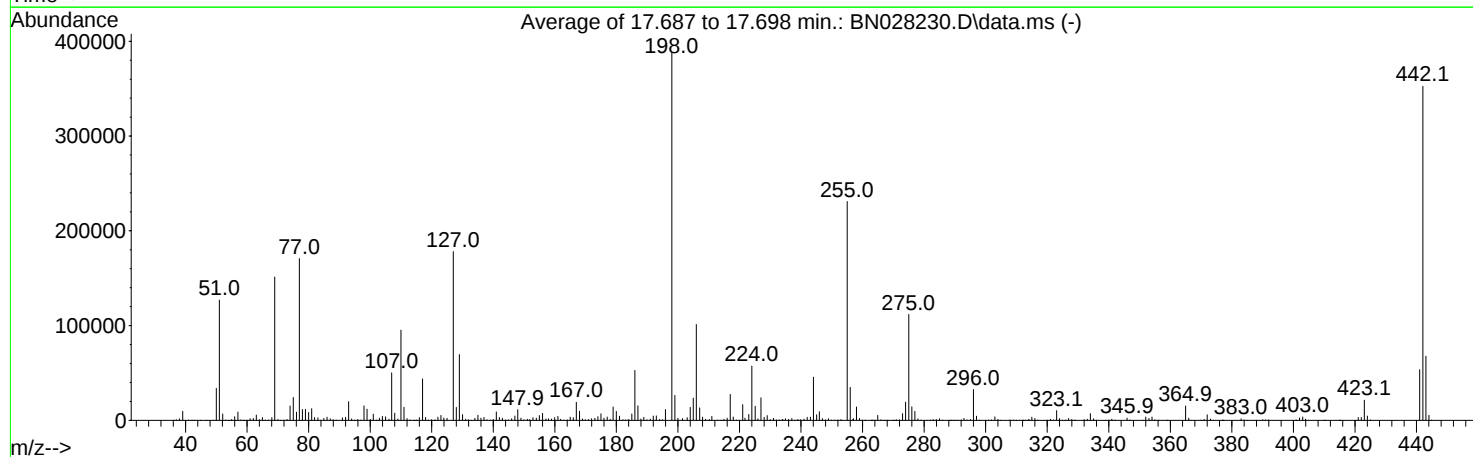


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101123\
Data File : BN028230.D
Acq On : 11 Oct 2023 13:35
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN100223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 12 11:45:56 2023

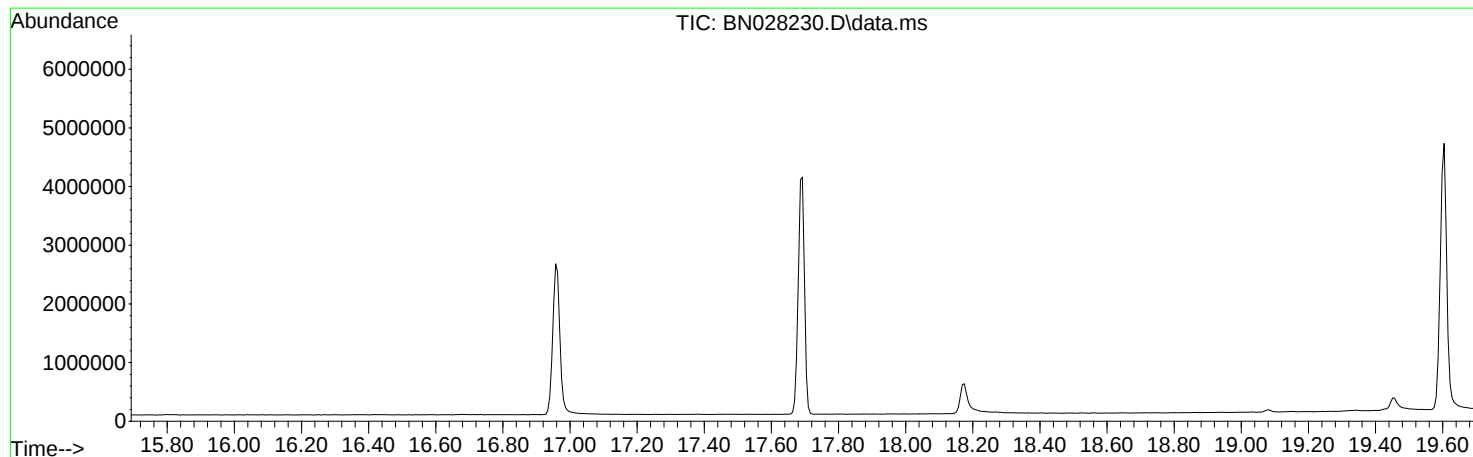




AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.7	127034	PASS
68	69	0.00	2	1.9	2886	PASS
69	198	0.00	100	39.0	151280	PASS
70	69	0.00	2	0.5	820	PASS
127	198	10	80	45.9	178205	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	388139	PASS
199	198	5	9	6.8	26355	PASS
275	198	10	60	28.8	111749	PASS
365	198	1	100	3.9	15245	PASS
441	198	0.01	100	13.8	53445	PASS
442	442	50	100	100.0	352533	PASS
443	442	15	24	19.2	67779	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101123\
Data File : BN028230.D
Acq On : 11 Oct 2023 13:35
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 12 05:03:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 12 05:02:54 2023
Response via : Initial Calibration

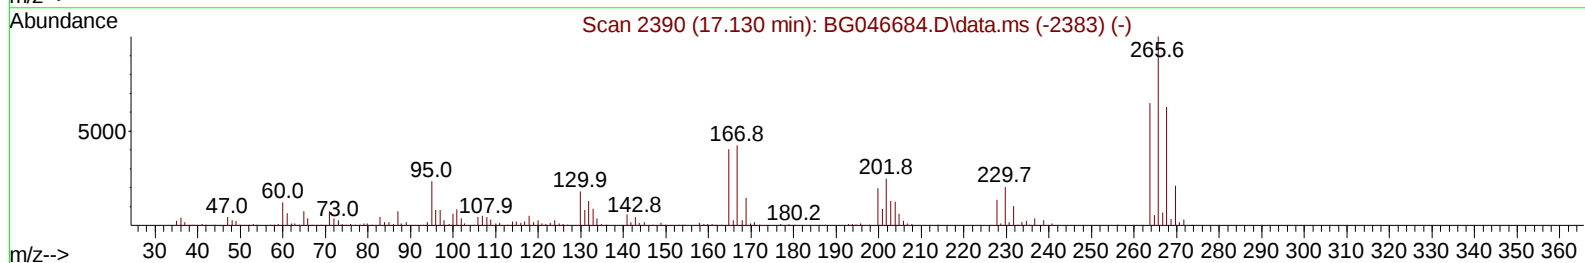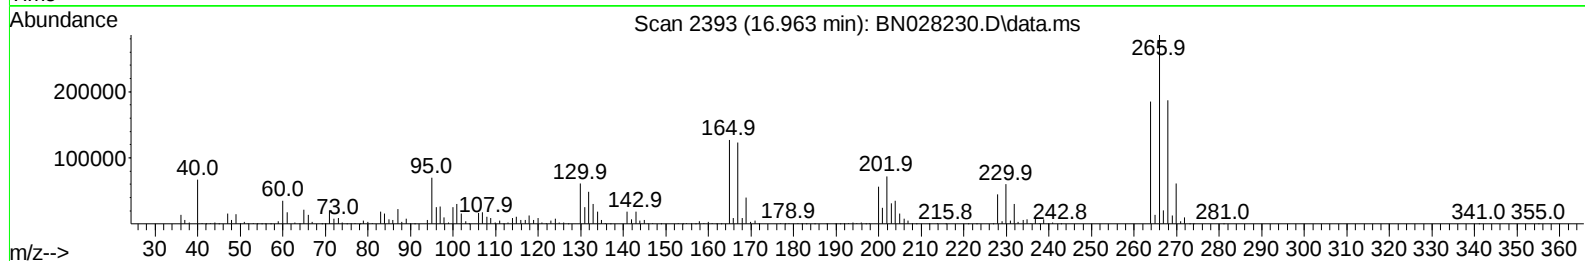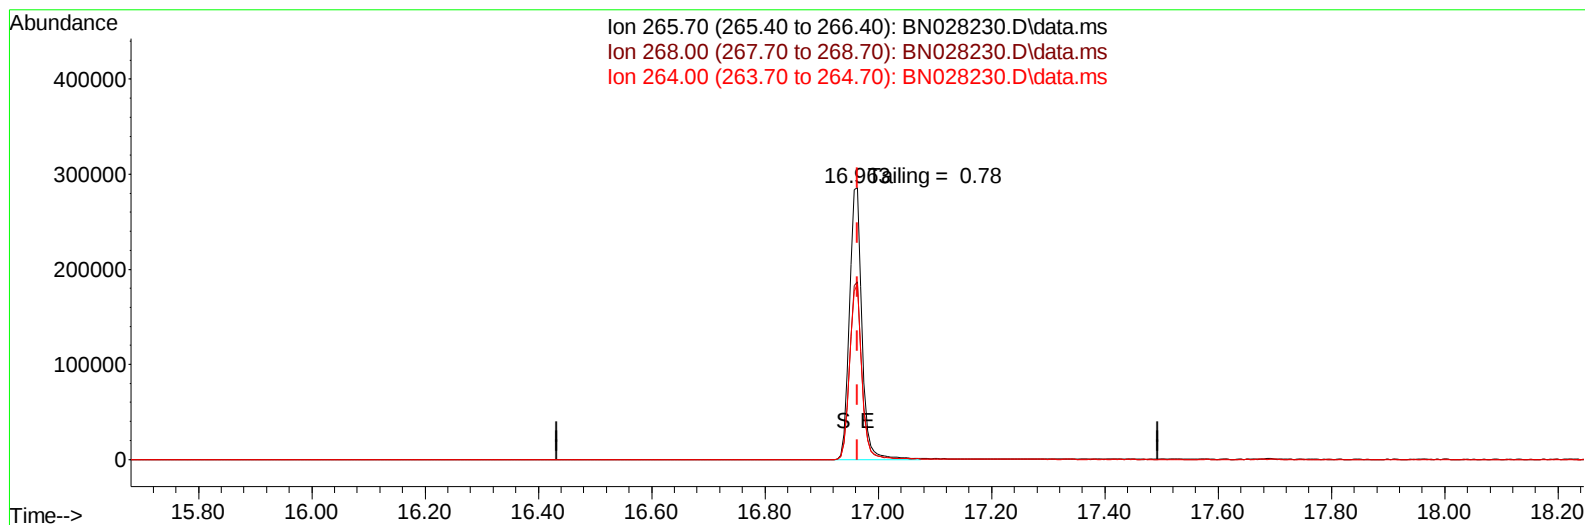

TIC: BN028230.D\data.ms

(70) Pentachlorophenol (C)

16.963min (0.000) 23247.31 ng




response 442962

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.54
264.00	61.60	64.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101123\
Data File : BN028230.D
Acq On : 11 Oct 2023 13:35
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 12 05:03:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 12 05:02:54 2023
Response via : Initial Calibration

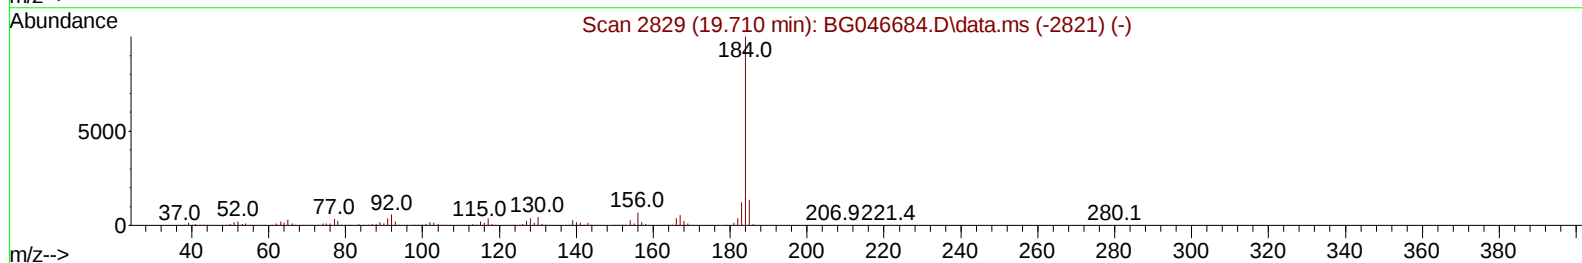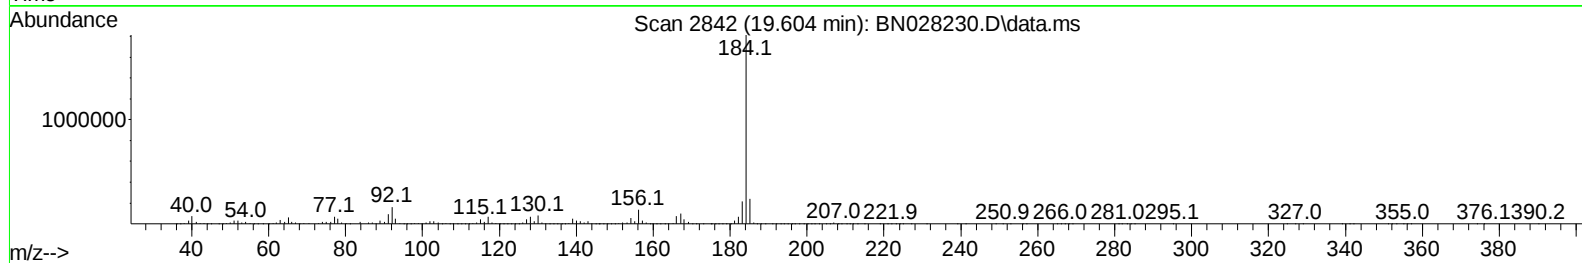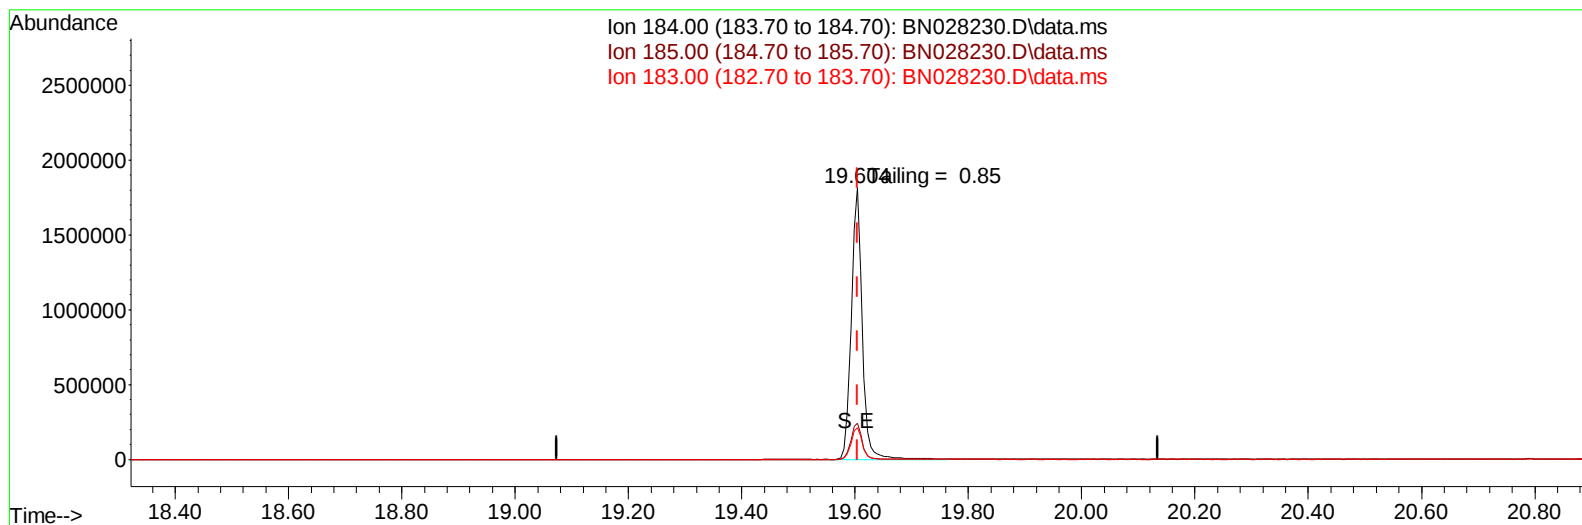

TIC: BN028230.D\data.ms

(77) Benzidine

19.604min (0.000) 627488.78 ng

response 2456507

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.36
183.00	13.20	11.74
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/11/2023	BNA_N	<u>BN028230.D</u>
Compound Name	Response	Retention Time
DDT	1347555	20.792
DDD	35765	20.357
DDE	1452	19.834
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
37217	1384772	2.69

Instrument :
BNA_N
ClientSampleId :
DFTPP