
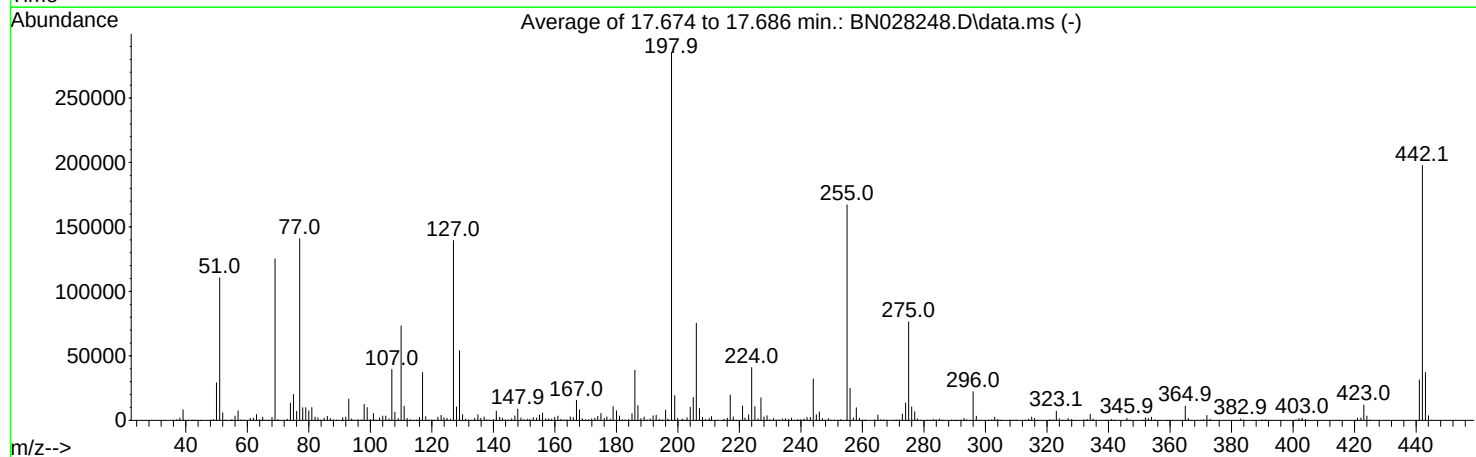


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101123\
Data File : BN028248.D
Acq On : 12 Oct 2023 01:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN100223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 12 11:45:56 2023

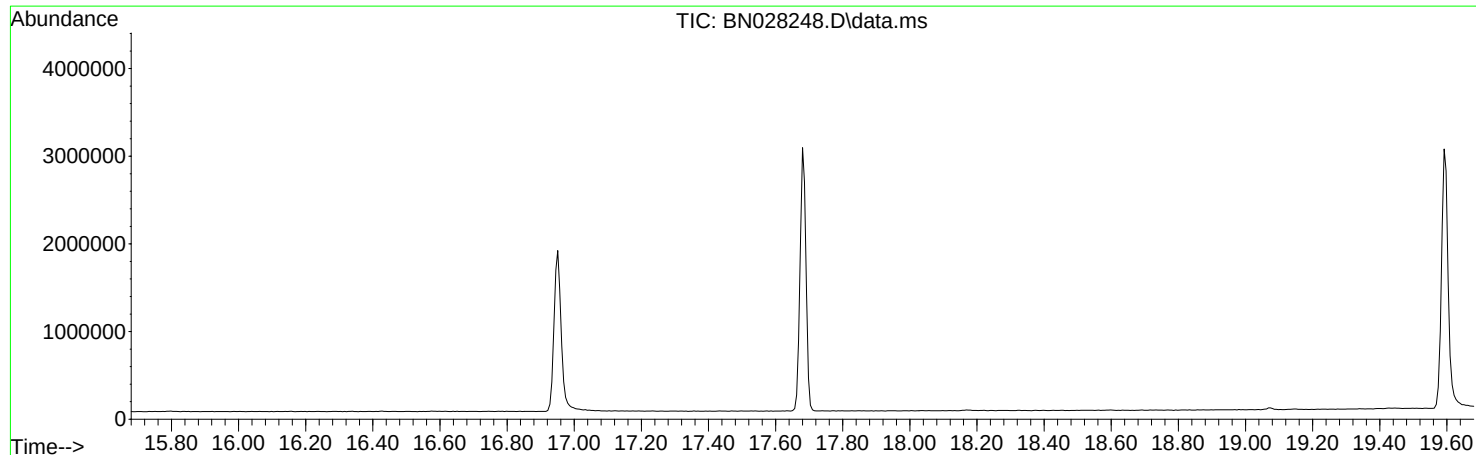




AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	110536	PASS
68	69	0.00	2	1.9	2401	PASS
69	198	0.00	100	44.0	125405	PASS
70	69	0.00	2	0.5	604	PASS
127	198	10	80	48.9	139477	PASS
197	198	0.00	2	0.4	1000	PASS
198	198	100	100	100.0	285312	PASS
199	198	5	9	6.7	19227	PASS
275	198	10	60	26.8	76395	PASS
365	198	1	100	3.9	11090	PASS
441	198	0.01	100	11.0	31424	PASS
442	442	50	100	100.0	197664	PASS
443	442	15	24	18.8	37104	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101123\
Data File : BN028248.D
Acq On : 12 Oct 2023 01:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 12 05:05:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 12 05:02:54 2023
Response via : Initial Calibration

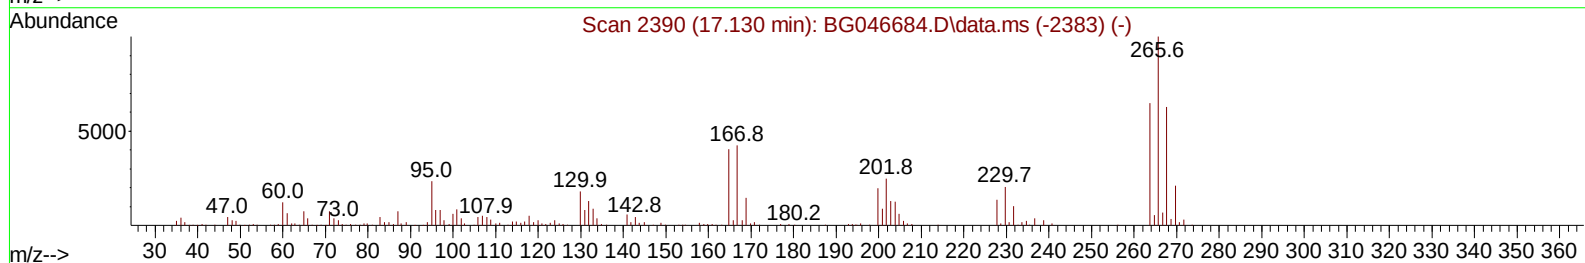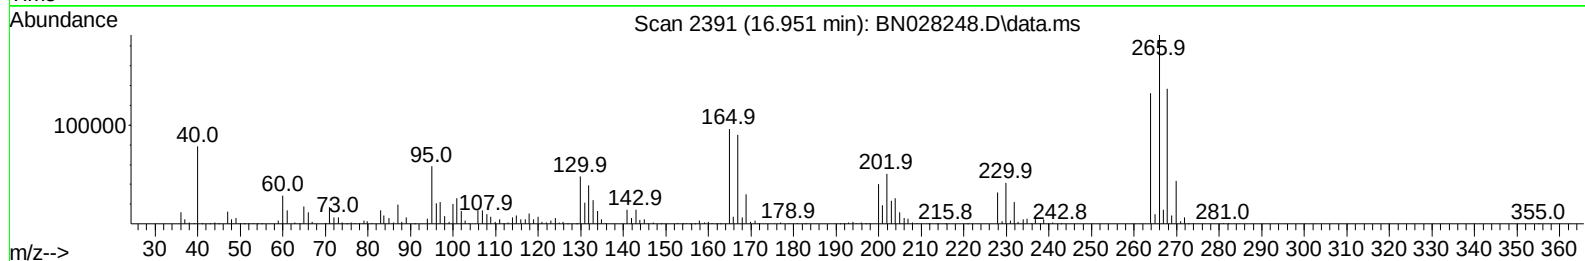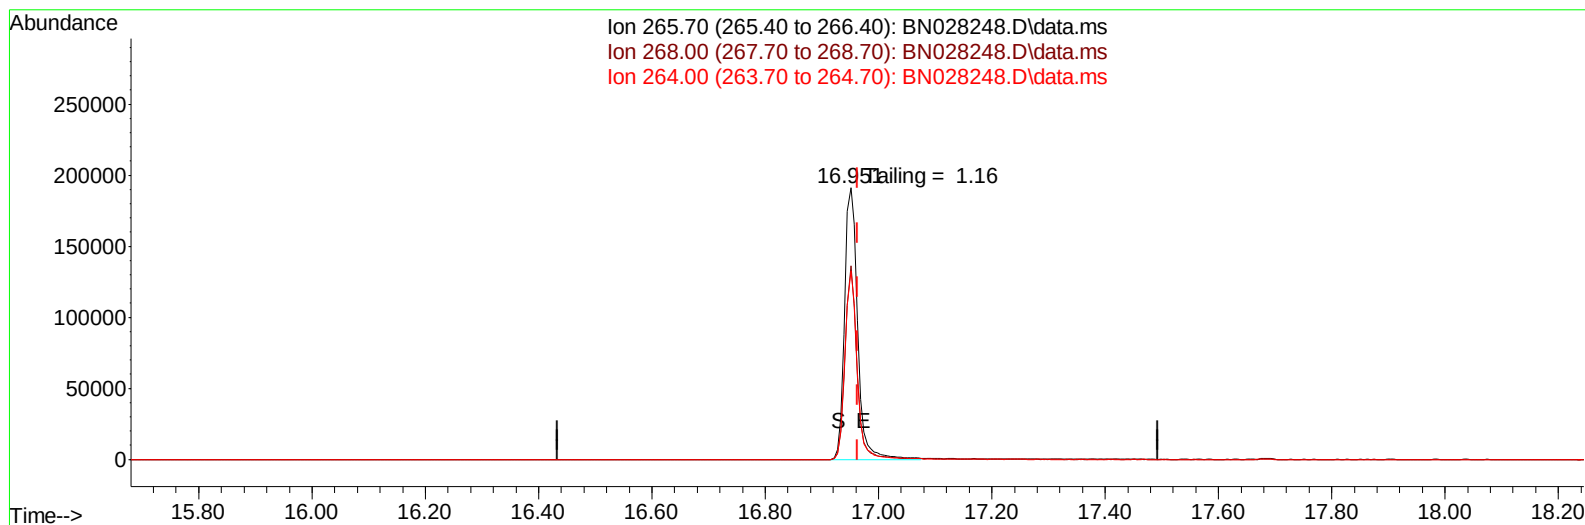

TIC: BN028248.D\data.ms

(70) Pentachlorophenol (C)

16.951min (-0.012) 21295.39 ng

response 304160

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	71.40
264.00	61.60	69.36
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/11/2023	BNA_N	<u>BN028248.D</u>
Compound Name	Response	Retention Time
DDT	889690	20.78
DDD	90984	20.345
DDE	2903	19.827
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
93887	983577	9.55

Instrument :
BNA_N
ClientSampleId :
DFTPP