
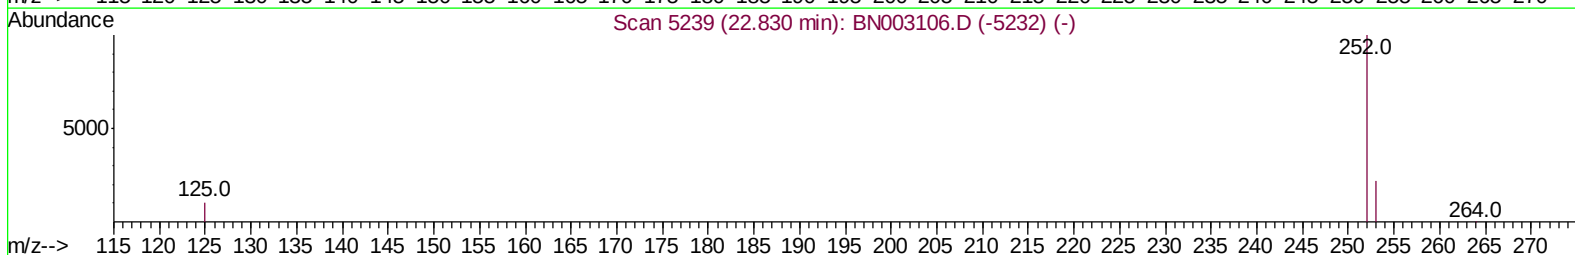
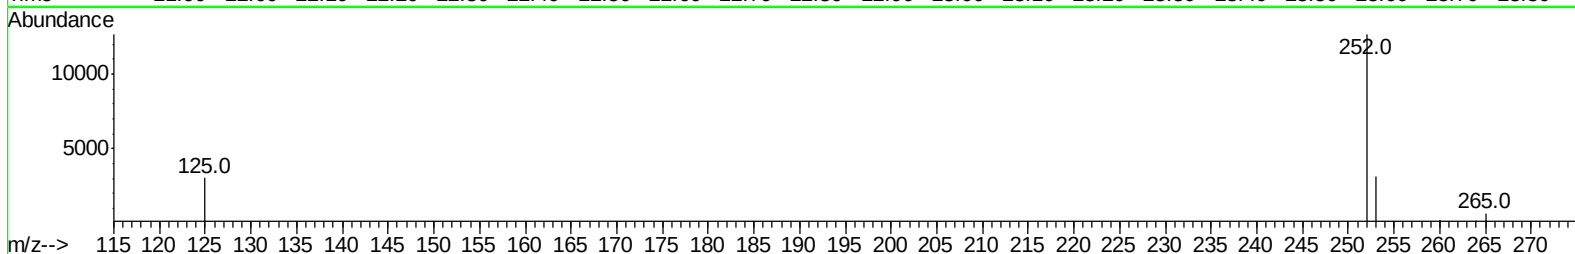


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003109.D
Acq On : 11 Oct 2018 18:51
Operator : MJ/SJ
Sample : J5368-07MS
Misc :
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Oct 12 05:37:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

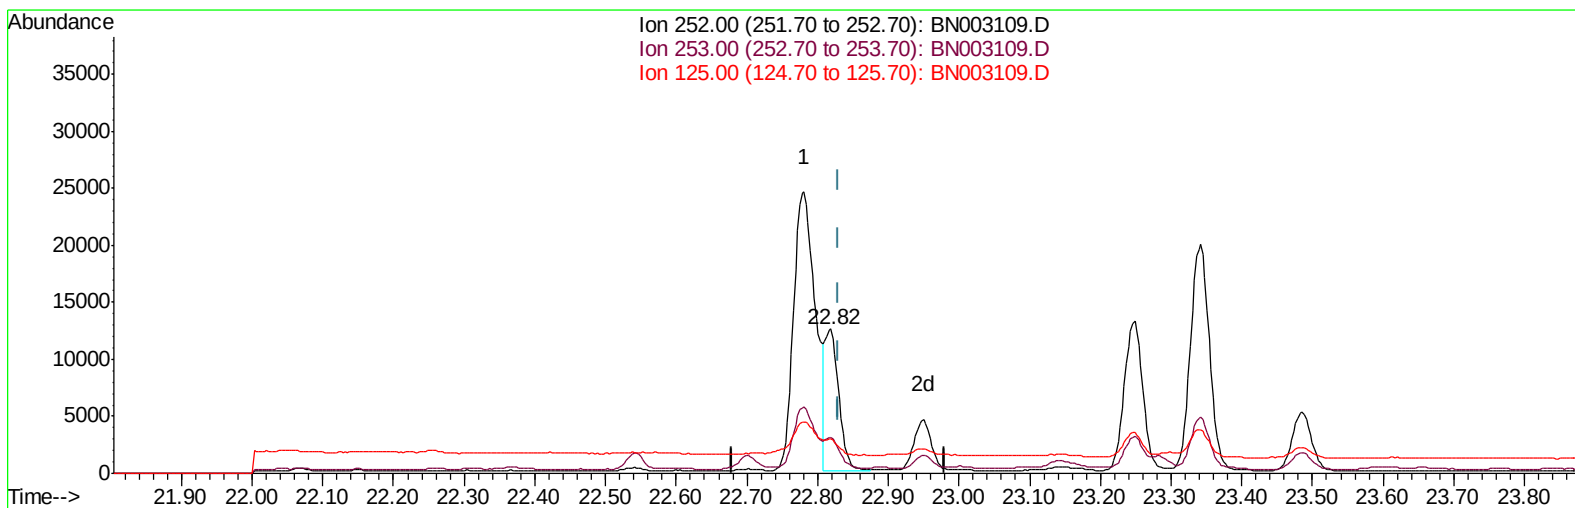

TIC: BN003109.D

(22) Benzo(k)fluoranthene

22.819min (-0.012) 0.98ng/ul m

response 17438

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	25.00
125.00	17.60	23.86#
0.00	0.00	0.00