
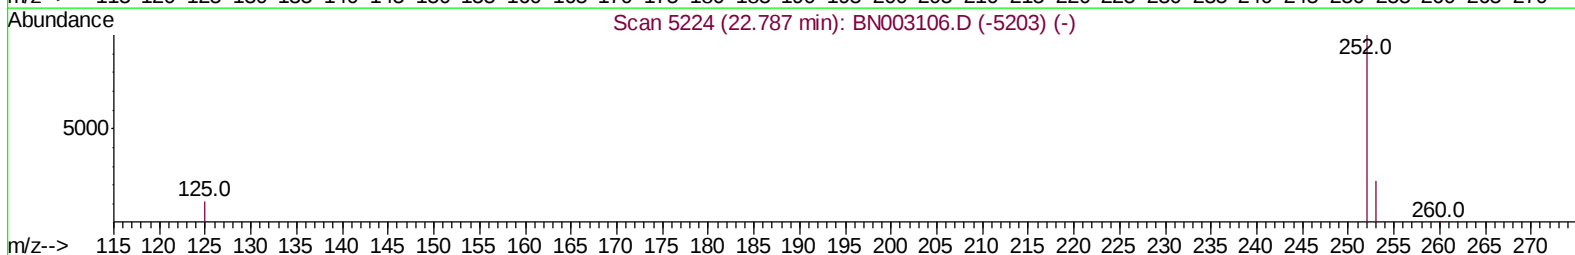
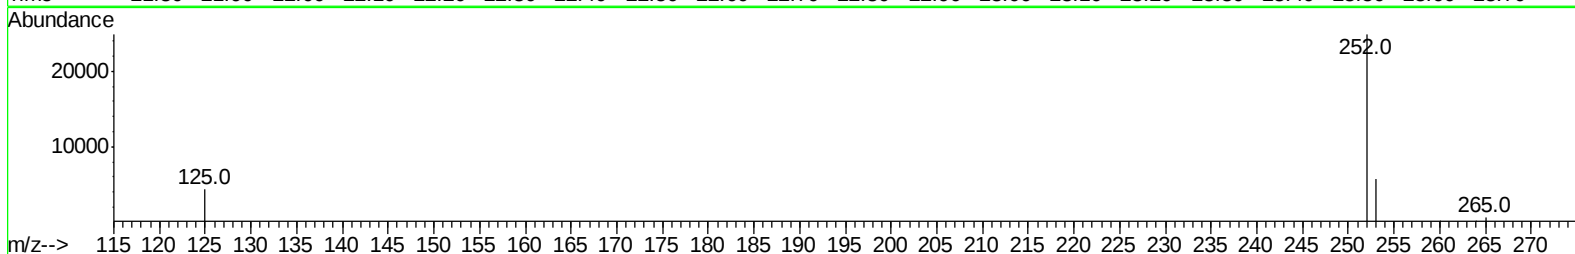


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003110.D
Acq On : 11 Oct 2018 19:26
Operator : MJ/SJ
Sample : J5368-08MSD
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Oct 12 05:37:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

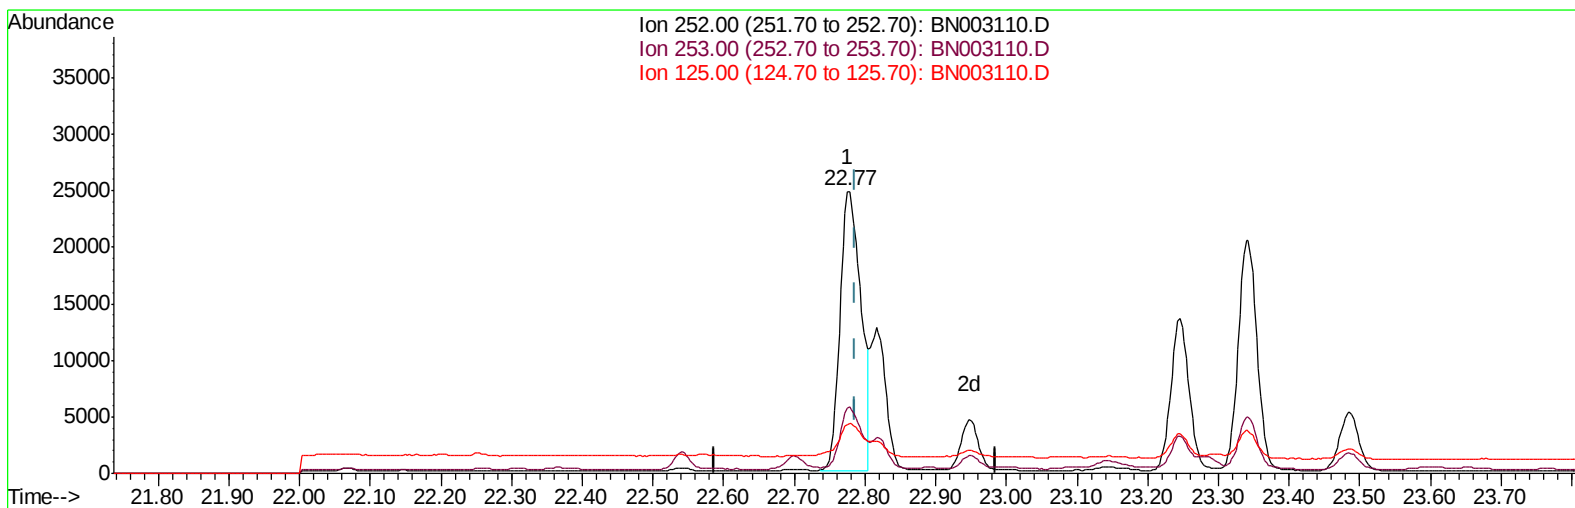

TIC: BN003110.D

(21) Benzo(b)fluoranthene

22.775min (-0.012) 3.11ng/ul m

response 50917

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	23.26
125.00	17.10	17.32
0.00	0.00	0.00