
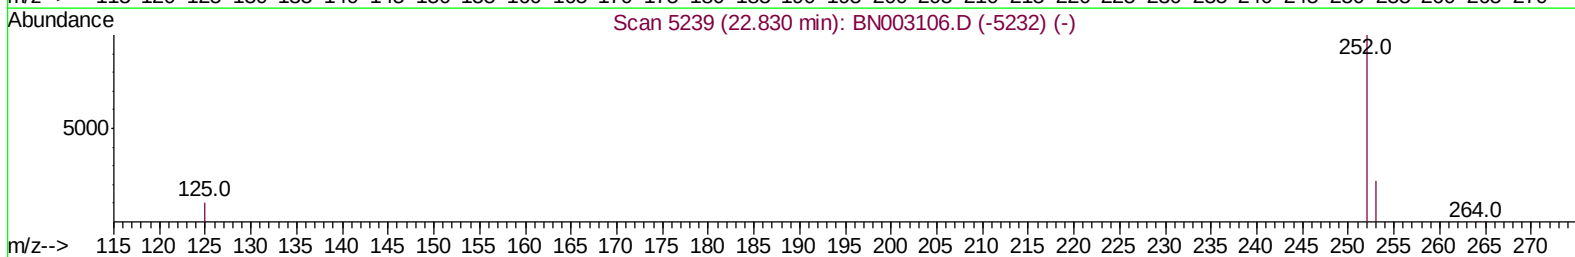
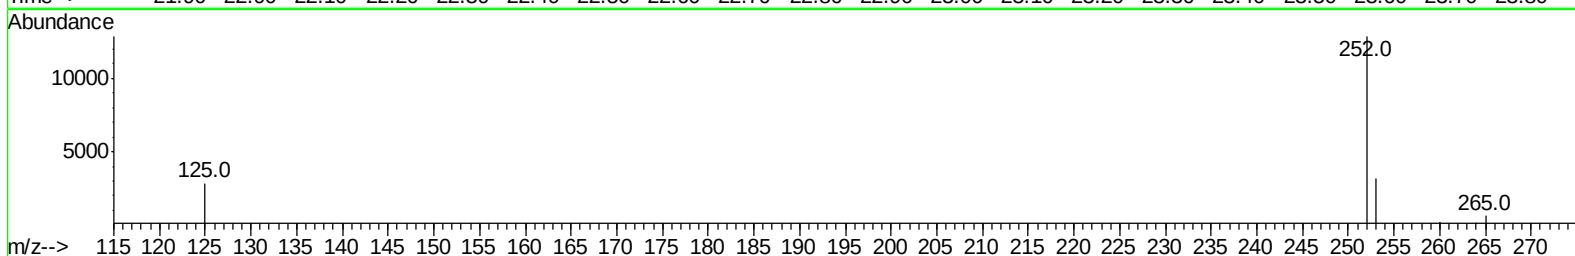


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003110.D
Acq On : 11 Oct 2018 19:26
Operator : MJ/SJ
Sample : J5368-08MSD
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Oct 12 05:37:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

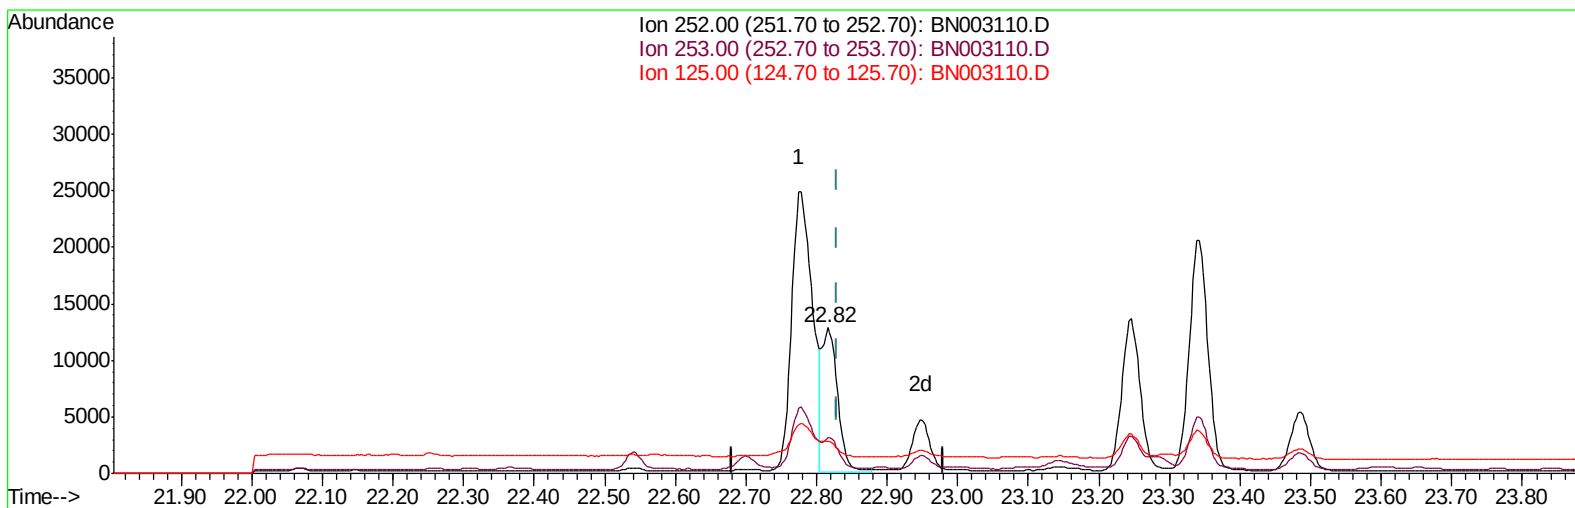

TIC: BN003110.D

(22) Benzo(k)fluoranthene

22.816min (-0.015) 1.17ng/ul m

response 19838

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	24.82
125.00	17.60	22.27#
0.00	0.00	0.00