
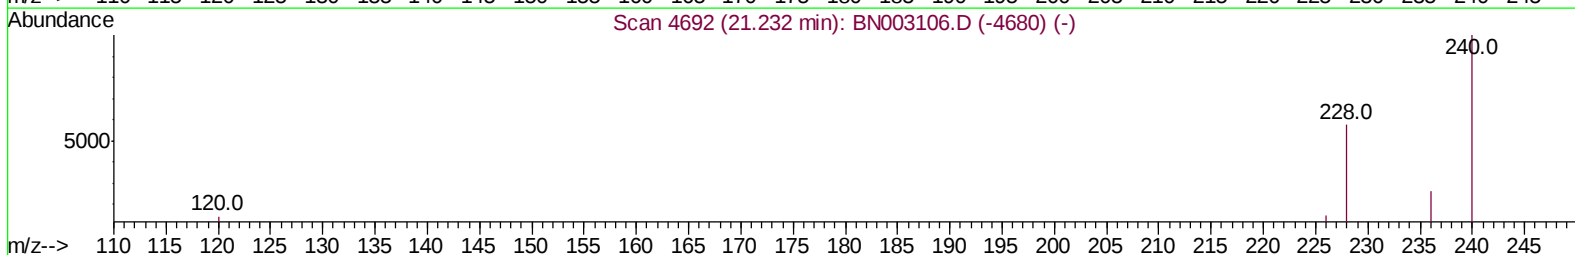
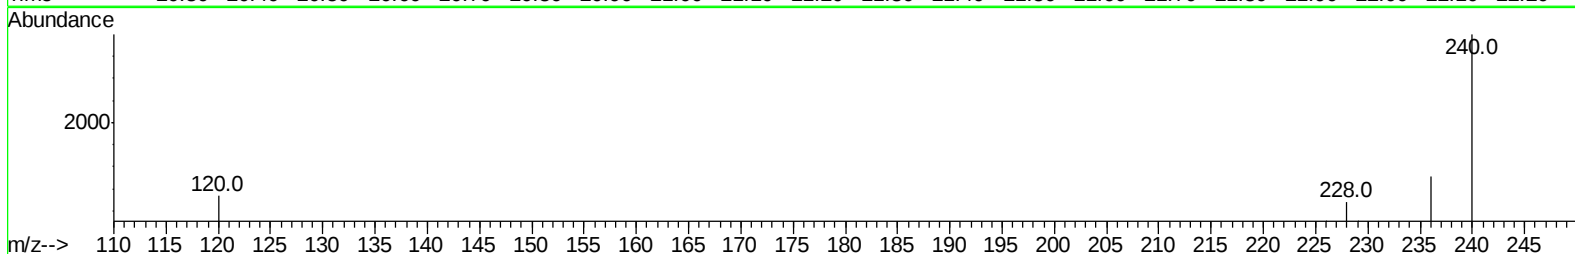


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003111.D
Acq On : 11 Oct 2018 20:01
Operator : MJ/SJ
Sample : J5368-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Oct 12 06:02:24 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

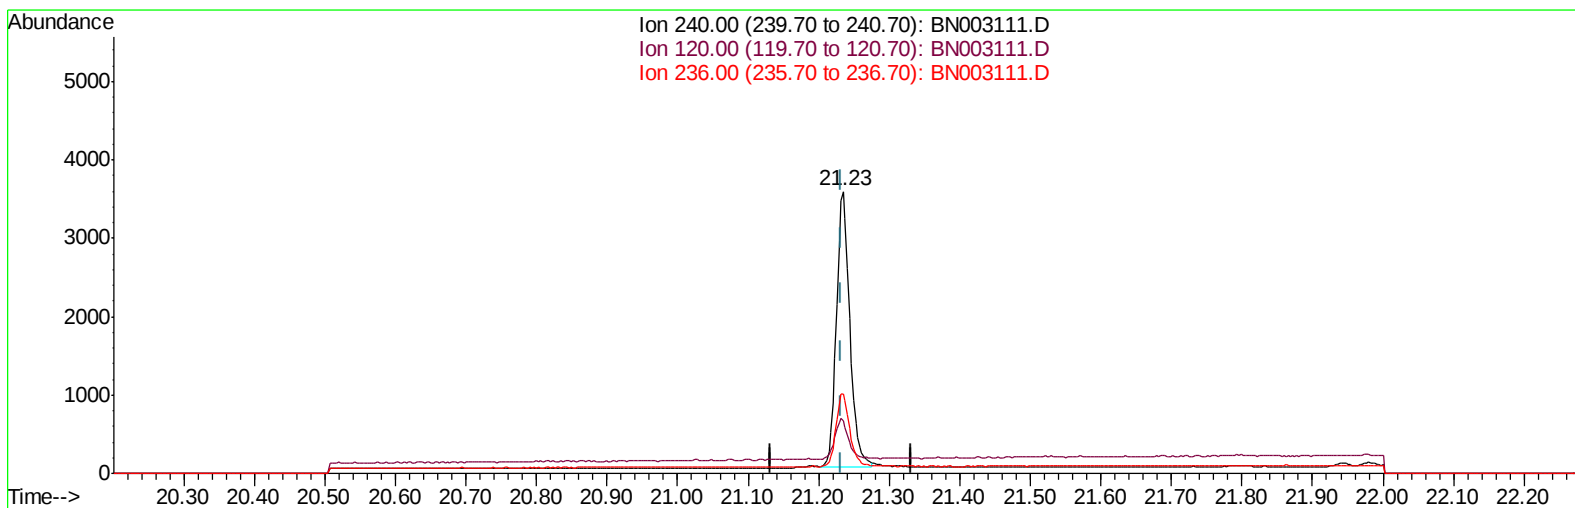

TIC: BN003111.D

(16) Chrysene-d12 (I)

21.235min (+0.003) 0.40ng/ul m

response 4639

Ion	Exp%	Act%
240.00	100	100
120.00	16.40	18.70
236.00	28.10	28.33
0.00	0.00	0.00