
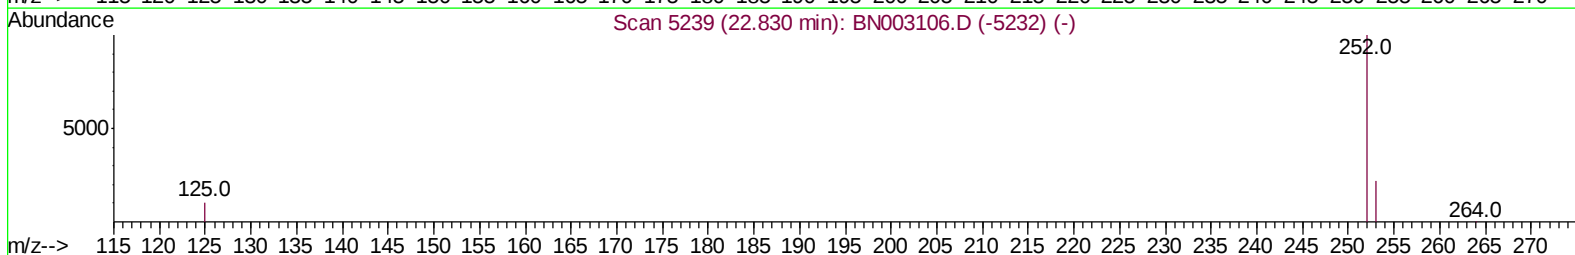
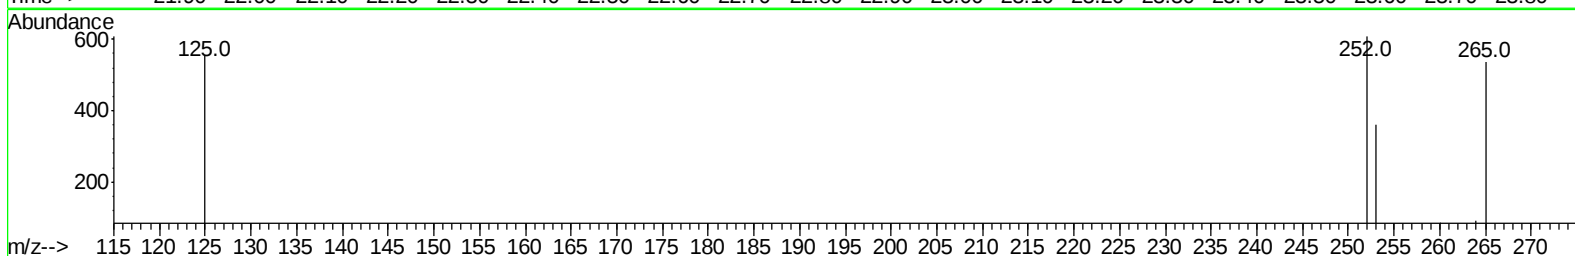


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003111.D
Acq On : 11 Oct 2018 20:01
Operator : MJ/SJ
Sample : J5368-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Oct 12 06:04:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

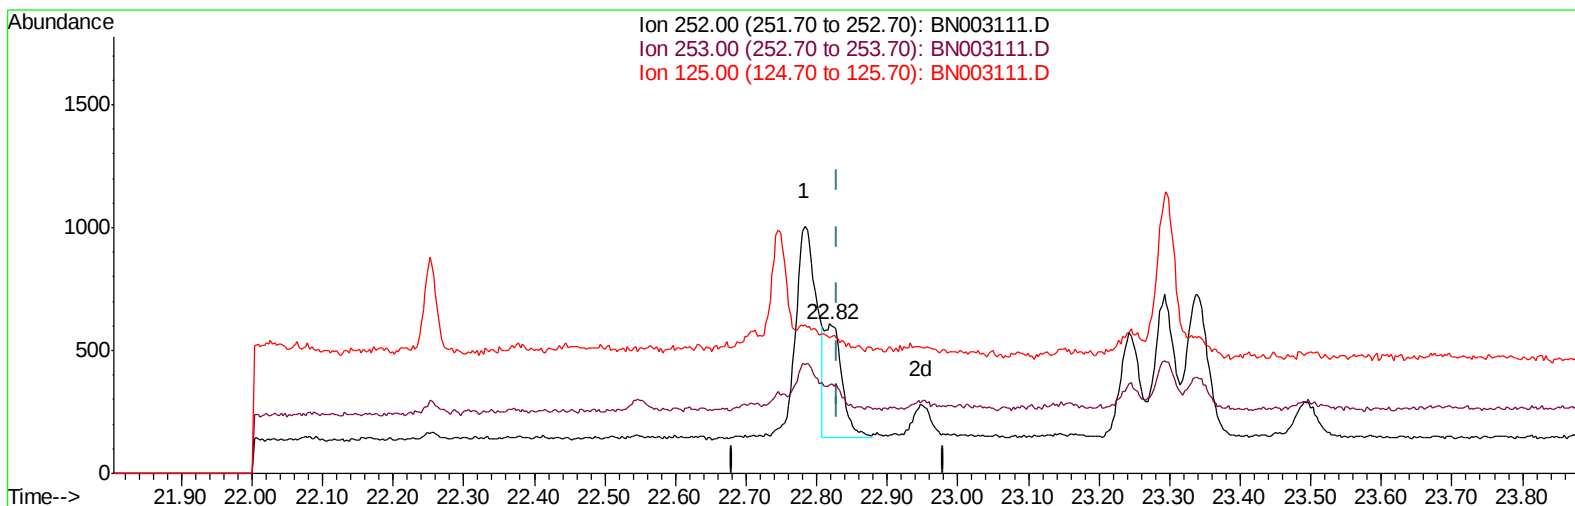

TIC: BN003111.D

(22) Benzo(k)fluoranthene

22.819min (-0.012) 0.05ng/ul m

response 820

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	59.05#
125.00	17.60	90.95#
0.00	0.00	0.00