
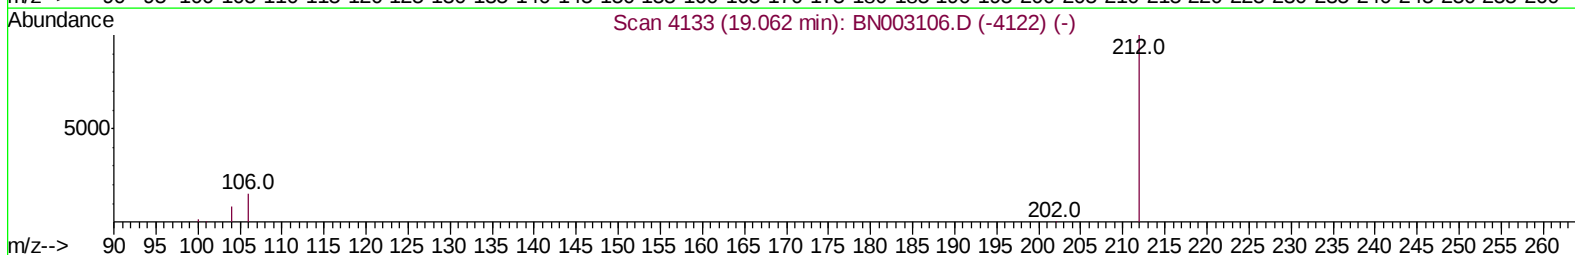
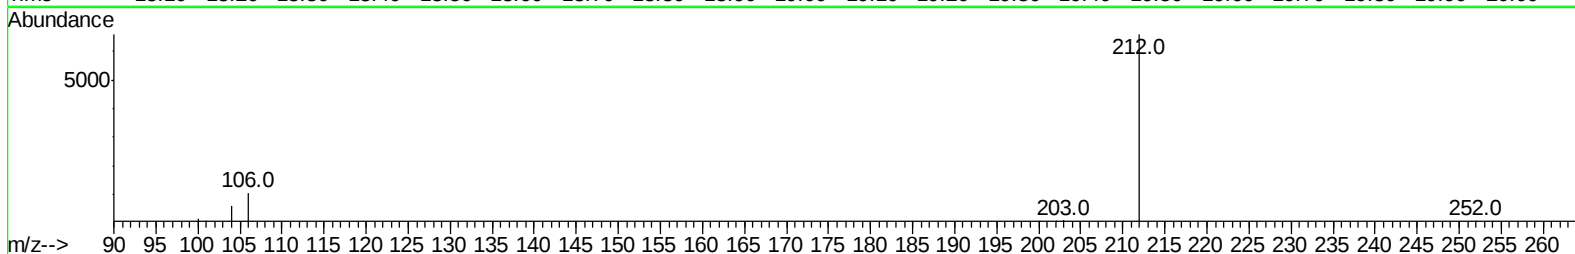


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003112.D
Acq On : 11 Oct 2018 20:36
Operator : MJ/SJ
Sample : J5368-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Oct 12 06:45:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

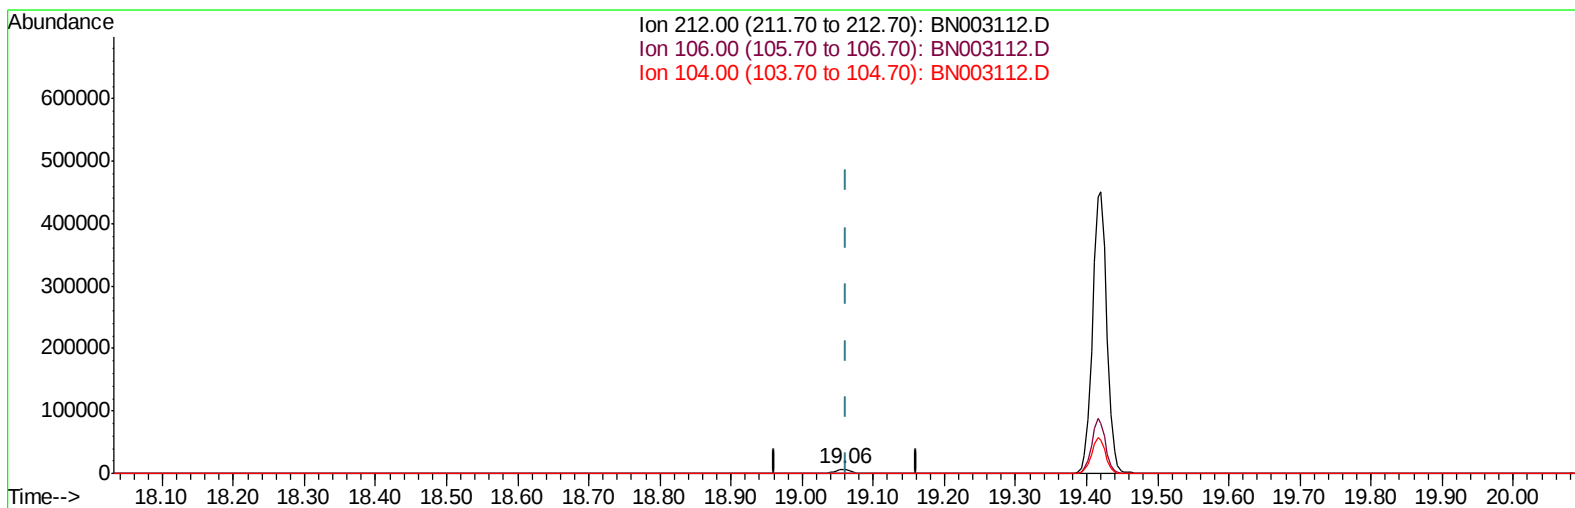

TIC: BN003112.D

(14) Fluoranthene-d10 (SURR)

19.058min (-0.005) 0.37ng/ul m

response 9367

Ion	Exp%	Act%
212.00	100	100
106.00	15.40	0.00#
104.00	8.60	0.00#
0.00	0.00	0.00