
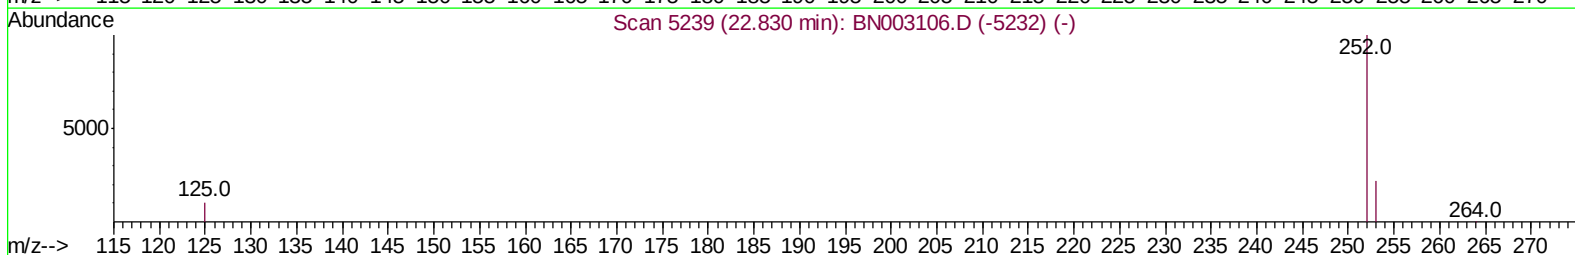
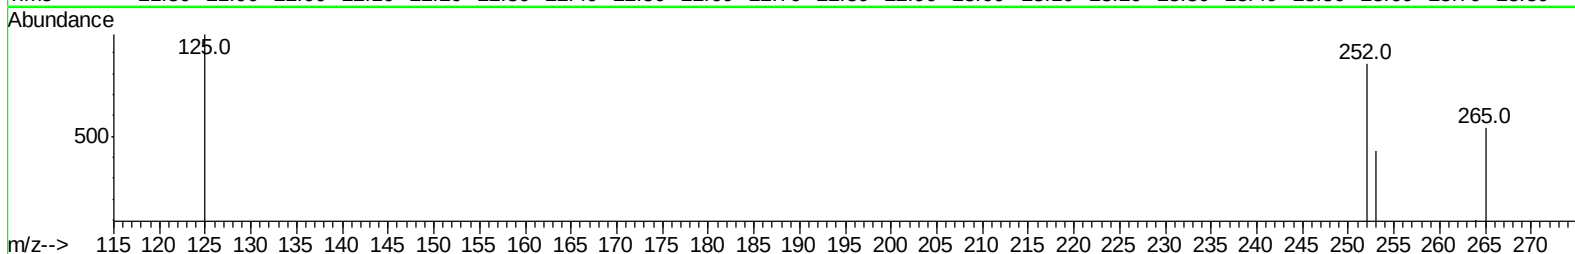


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003112.D
Acq On : 11 Oct 2018 20:36
Operator : MJ/SJ
Sample : J5368-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Oct 12 06:46:51 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

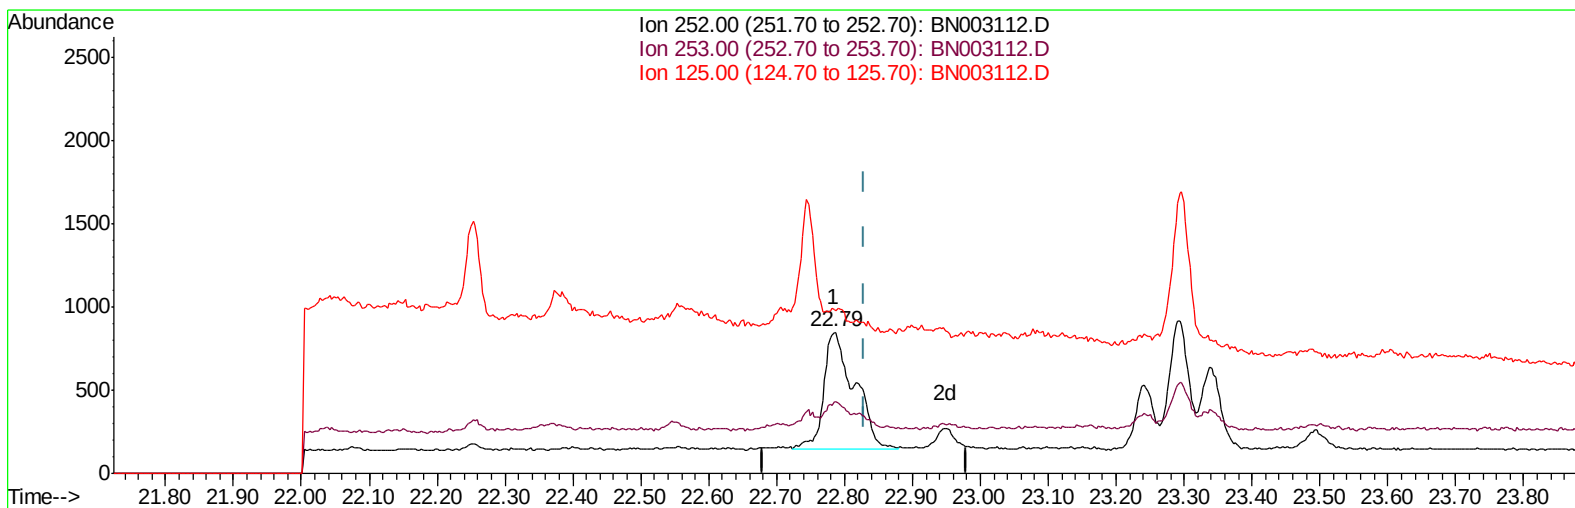

TIC: BN003112.D

(22) Benzo(k)fluoranthene

22.785min (-0.045) 0.13ng/ul

response 2202

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	50.53#
125.00	17.60	116.65#
0.00	0.00	0.00