
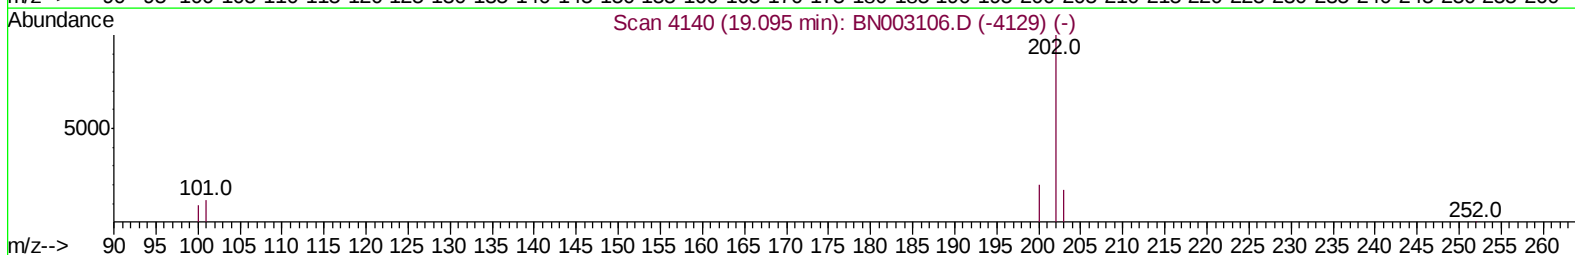
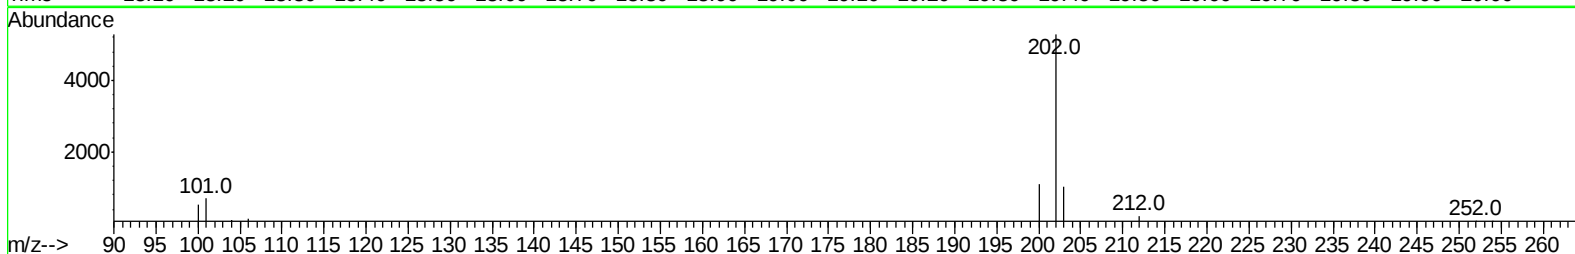


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003113.D
Acq On : 11 Oct 2018 21:12
Operator : MJ/SJ
Sample : J5368-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Oct 12 06:48:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

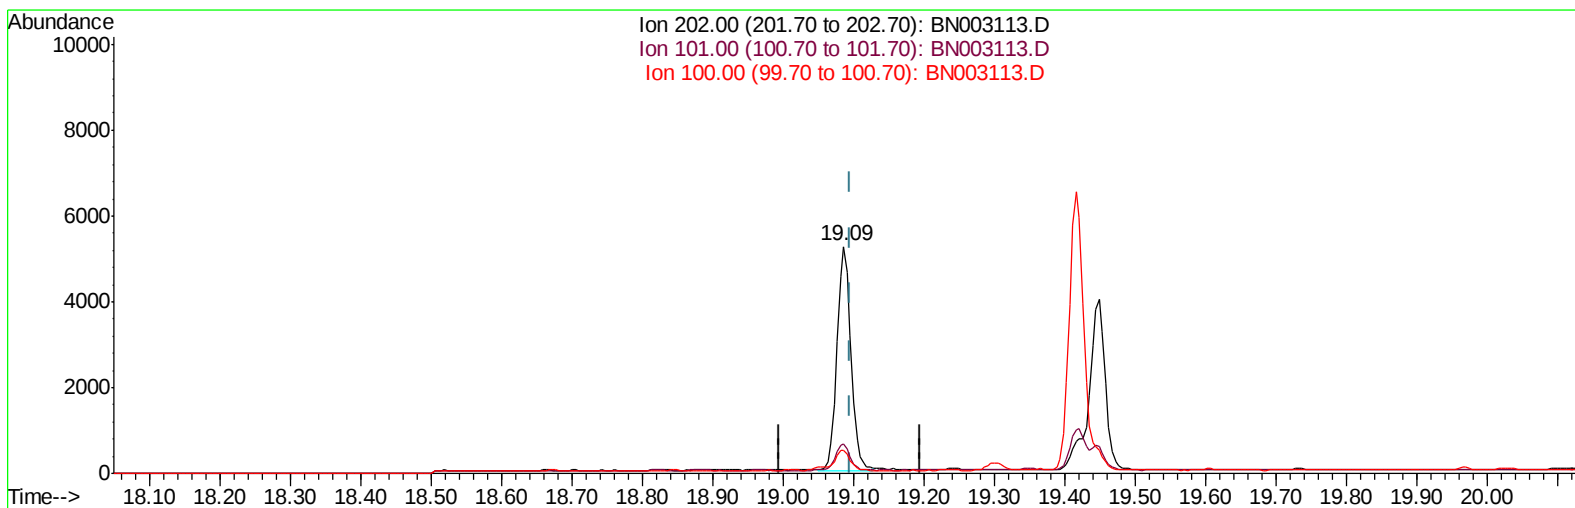

TIC: BN003113.D

(15) Fluoranthene (C)

19.085min (-0.009) 0.24ng/ul m

response 7332

Ion	Exp%	Act%
202.00	100	100
101.00	12.30	13.19
100.00	9.10	10.05
0.00	0.00	0.00