
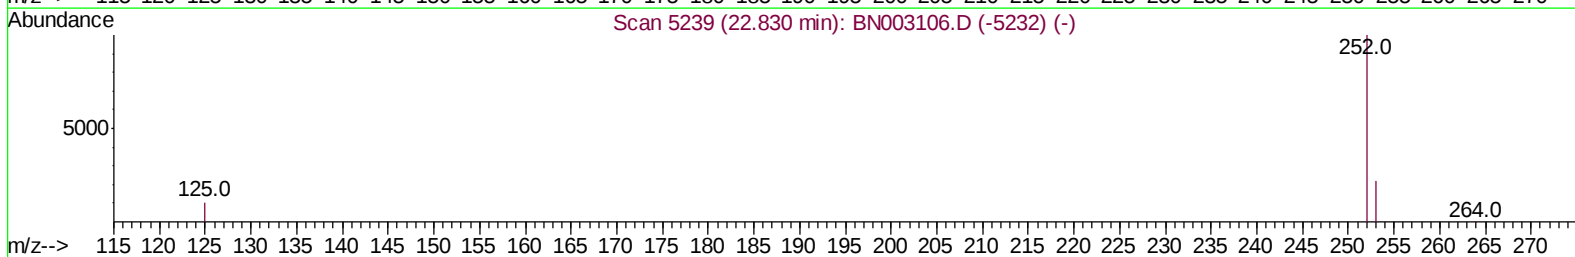
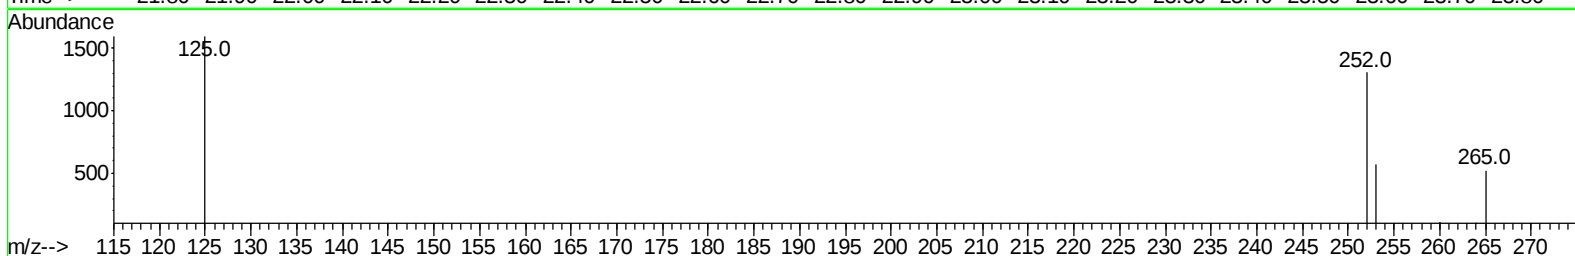


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\  
Data File : BN003113.D  
Acq On : 11 Oct 2018 21:12  
Operator : MJ/SJ  
Sample : J5368-02  
Misc :  
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Oct 12 06:50:44 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Oct 12 05:29:36 2018  
Response via : Initial Calibration

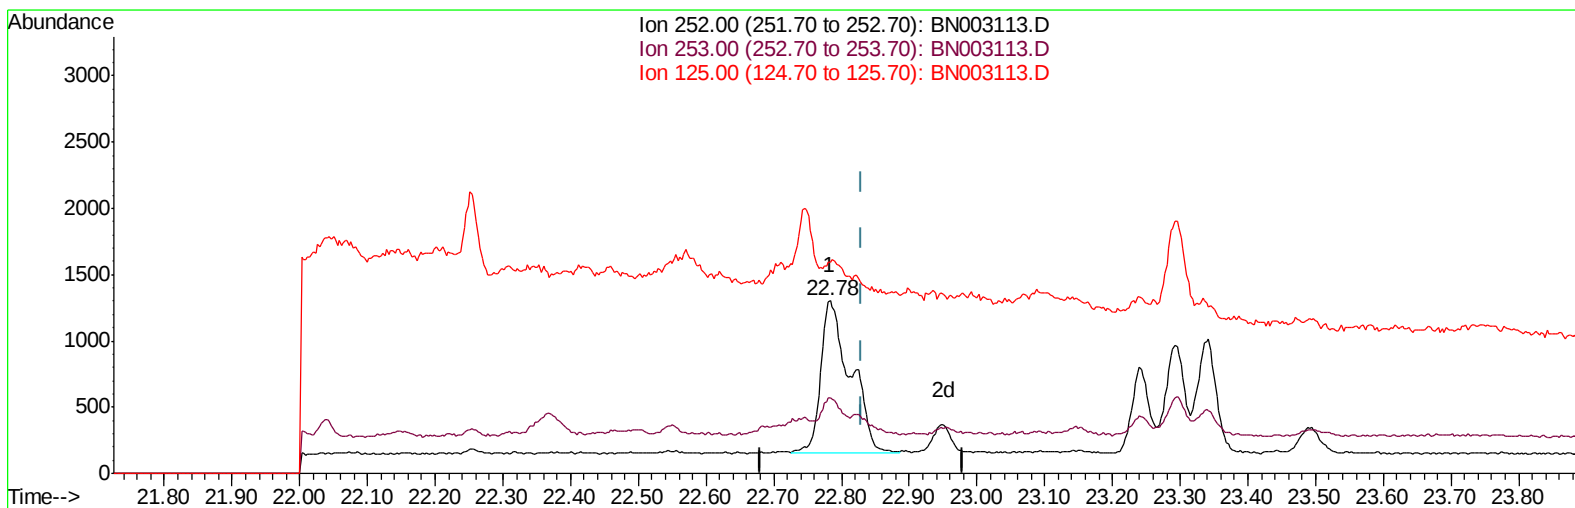

TIC: BN003113.D

(22) Benzo(k)fluoranthene

22.784min (-0.047) 0.19ng/ul

response 3490

| Ion    | Exp%  | Act%    |
|--------|-------|---------|
| 252.00 | 100   | 100     |
| 253.00 | 26.60 | 43.75#  |
| 125.00 | 17.60 | 122.26# |
| 0.00   | 0.00  | 0.00    |