
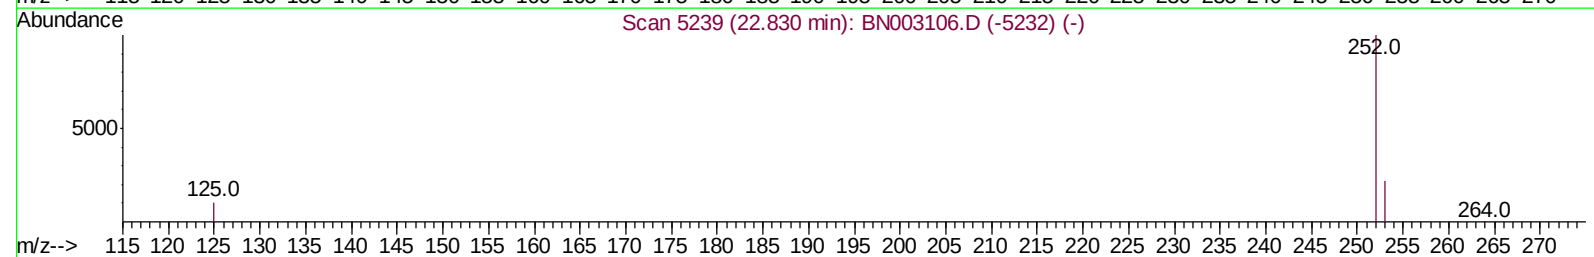
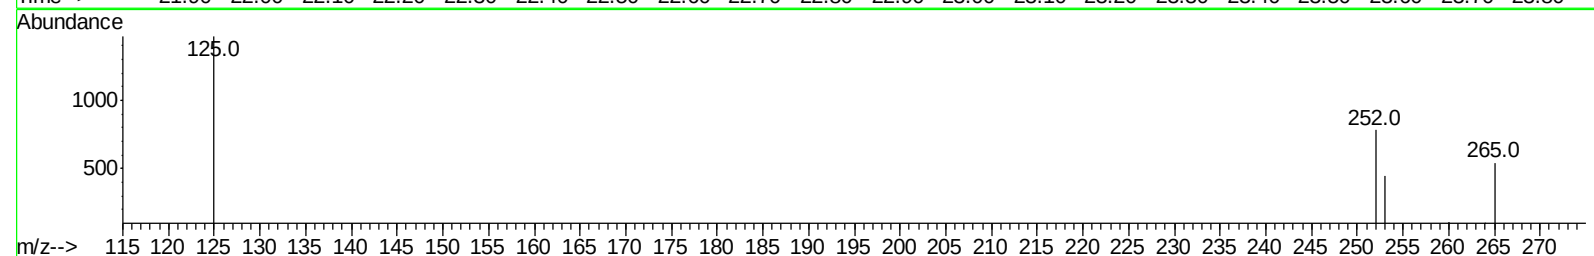


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003113.D
Acq On : 11 Oct 2018 21:12
Operator : MJ/SJ
Sample : J5368-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Oct 12 06:50:44 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

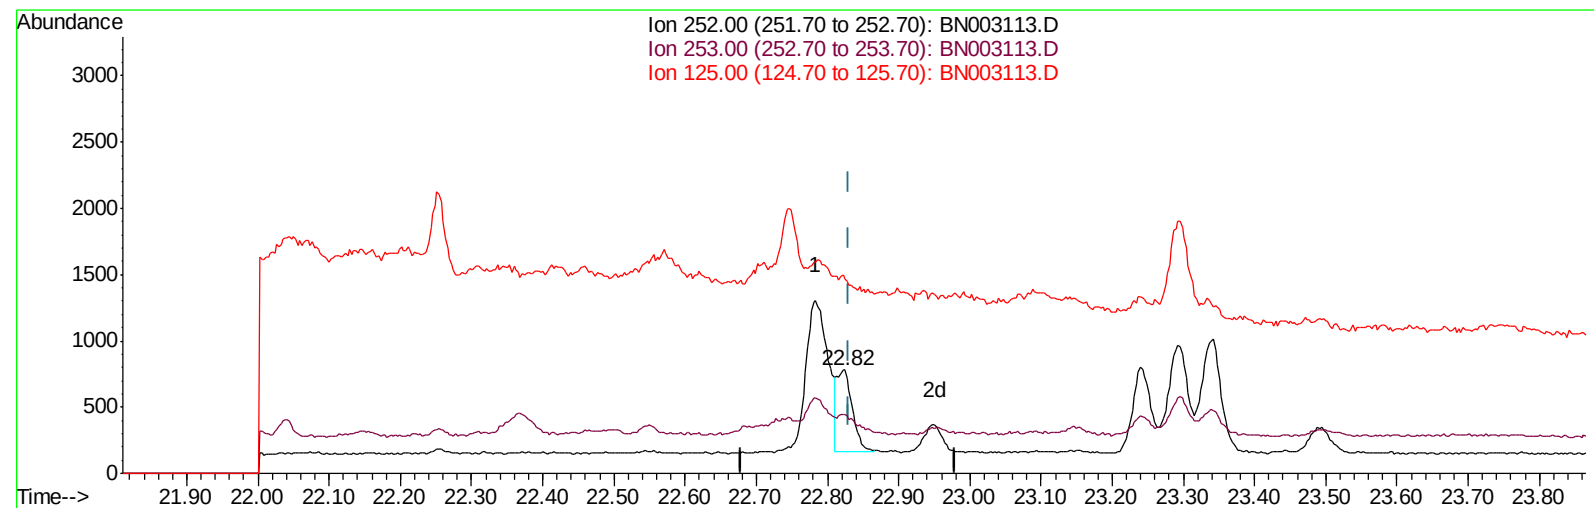

TIC: BN003113.D

(22) Benzo(k)fluoranthene

22.825min (-0.006) 0.05ng/ul m

response 940

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	57.03#
125.00	17.60	187.98#
0.00	0.00	0.00