
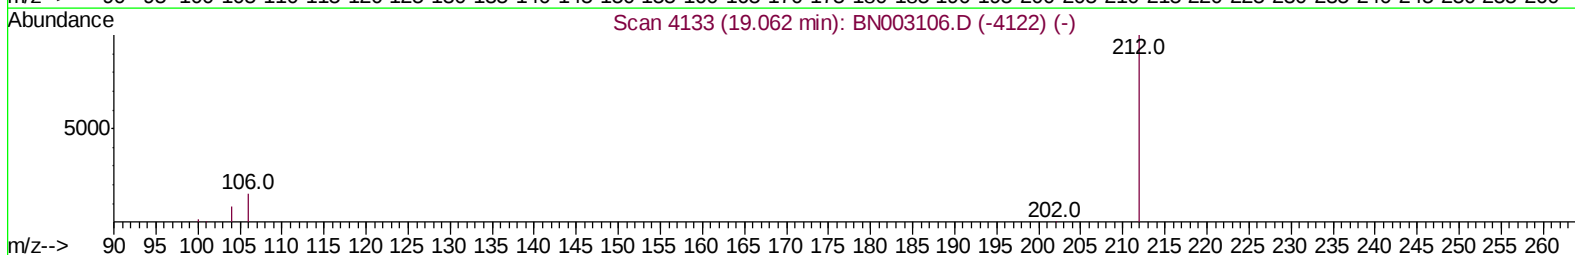
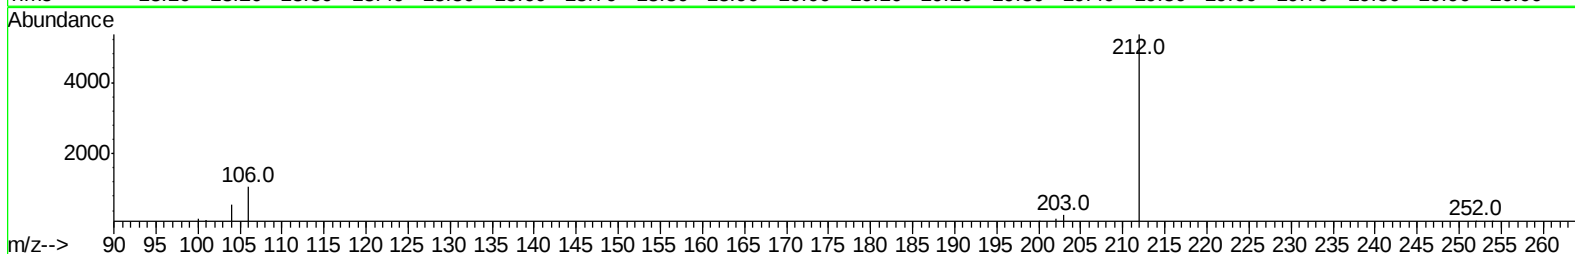


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003114.D
Acq On : 11 Oct 2018 21:47
Operator : MJ/SJ
Sample : J5368-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Oct 12 06:53:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

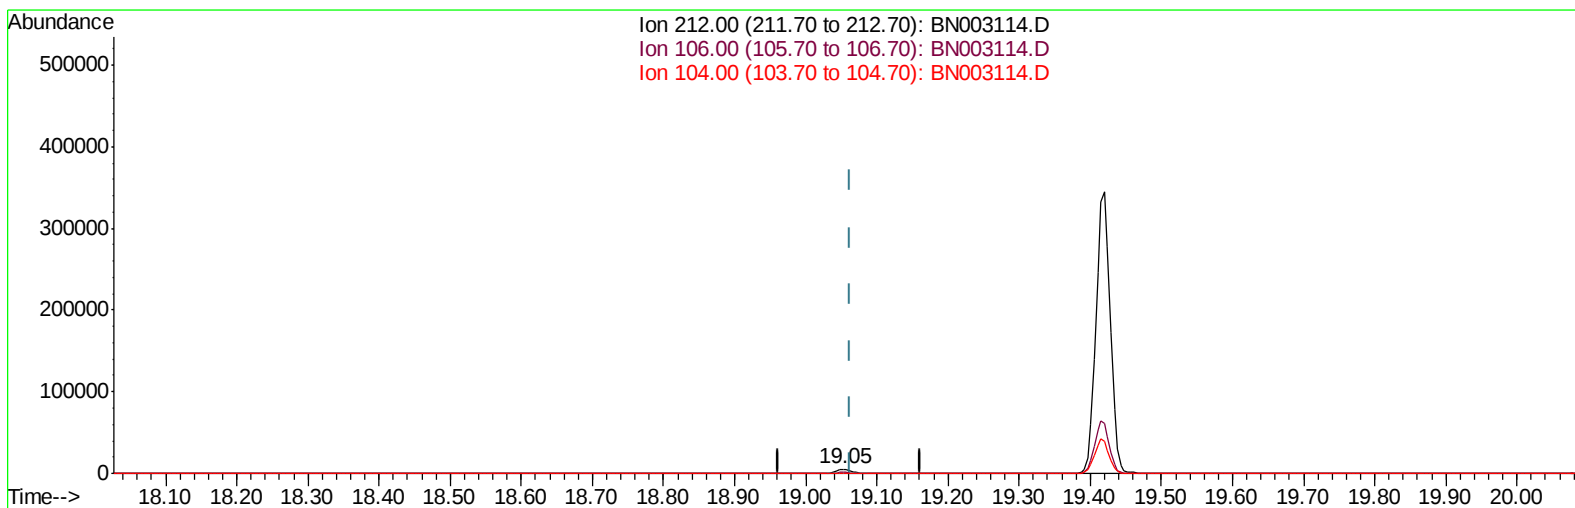

TIC: BN003114.D

(14) Fluoranthene-d10 (SURR)

19.053min (-0.010) 0.29ng/ul m

response 7384

Ion	Exp%	Act%
212.00	100	100
106.00	15.40	0.00#
104.00	8.60	0.00#
0.00	0.00	0.00