
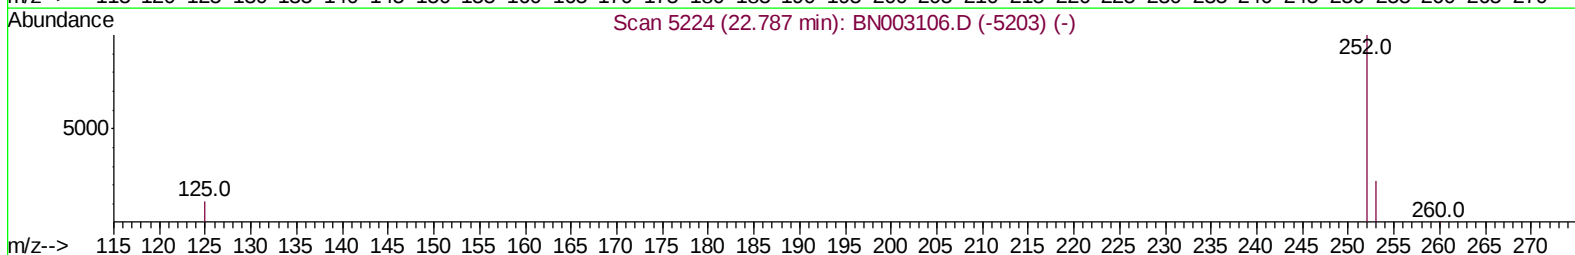
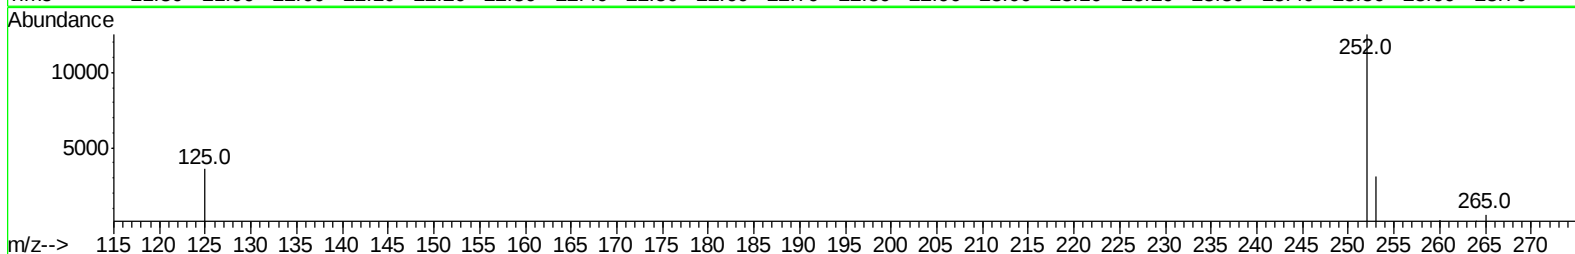


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003114.D
Acq On : 11 Oct 2018 21:47
Operator : MJ/SJ
Sample : J5368-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Oct 12 06:55:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

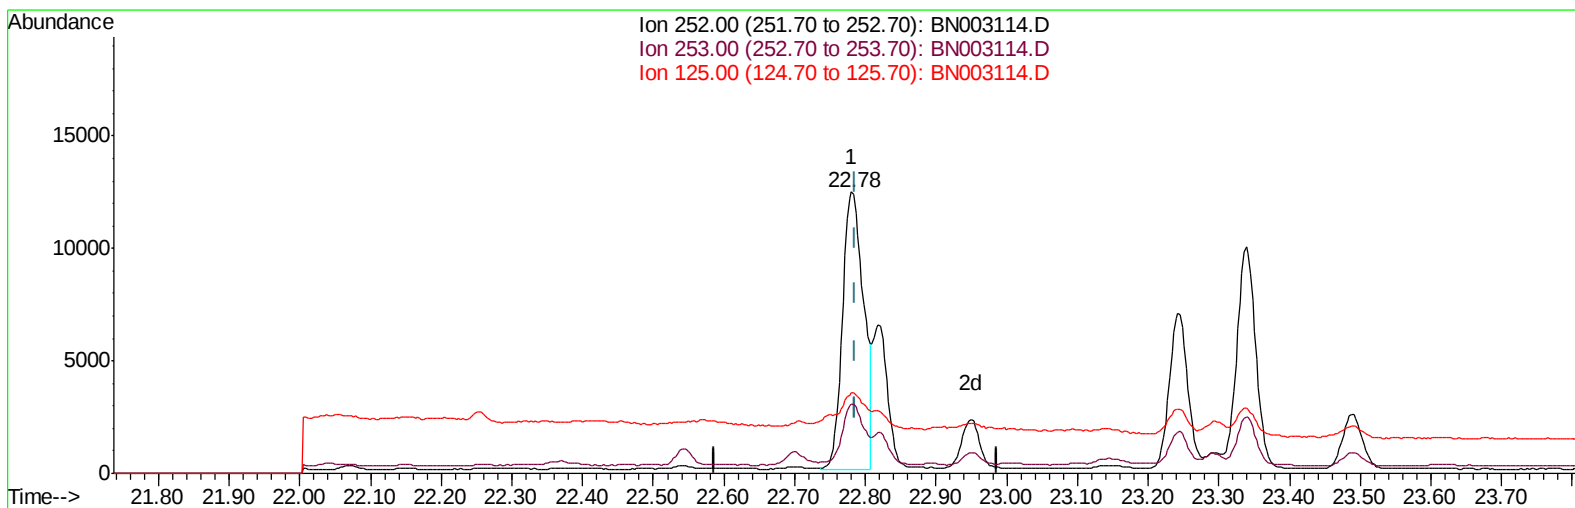

TIC: BN003114.D

(21) Benzo(b)fluoranthene

22.780min (-0.006) 1.52ng/ul m

response 25401

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	24.72
125.00	17.10	28.80
0.00	0.00	0.00