
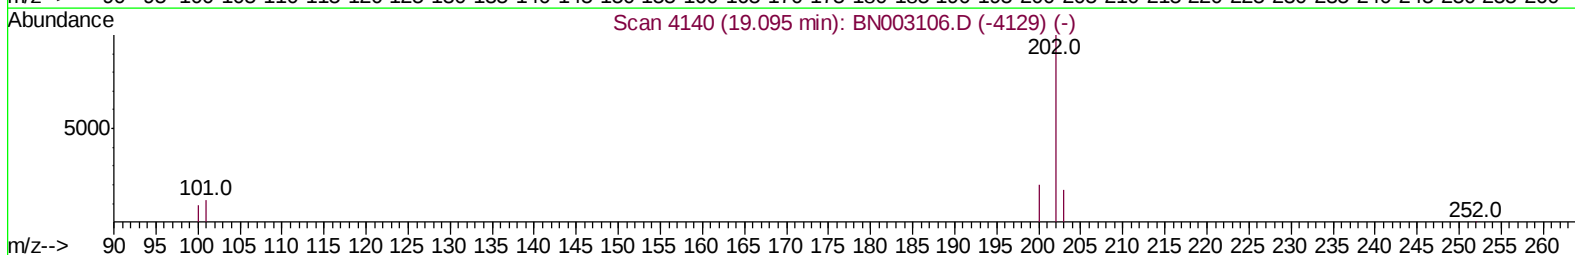
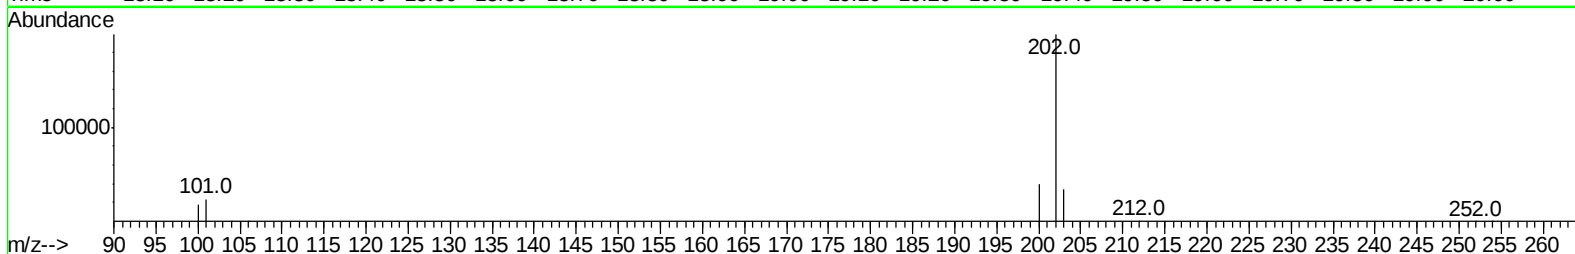


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003115.D
Acq On : 11 Oct 2018 22:22
Operator : MJ/SJ
Sample : J5368-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Oct 12 06:57:04 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

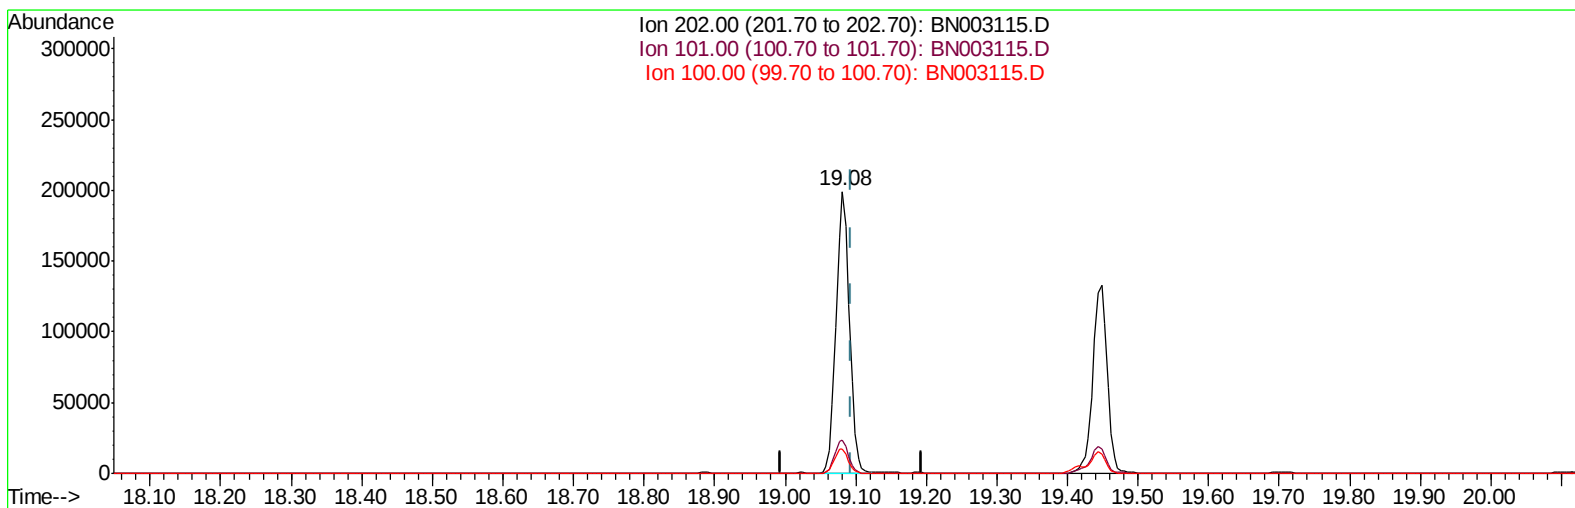

TIC: BN003115.D

(15) Fluoranthene (C)

19.081min (-0.014) 9.52ng/ul m

response 262815

Ion	Exp%	Act%
202.00	100	100
101.00	12.30	11.81
100.00	9.10	8.78
0.00	0.00	0.00