
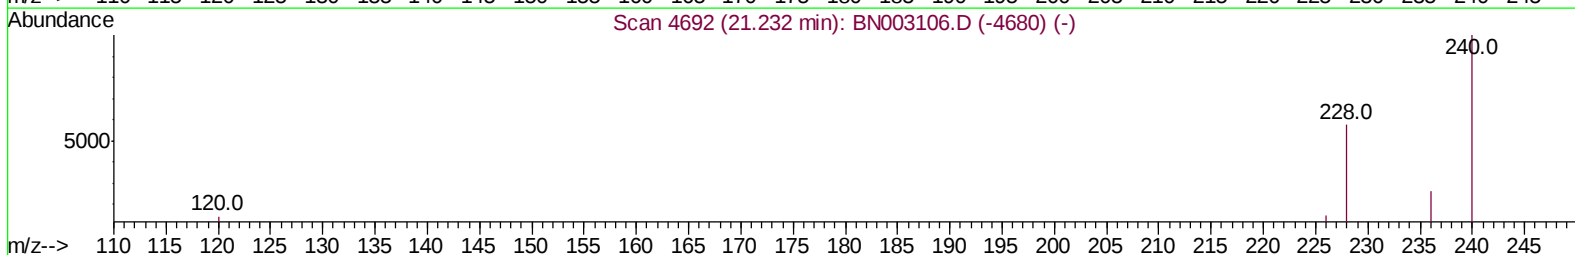
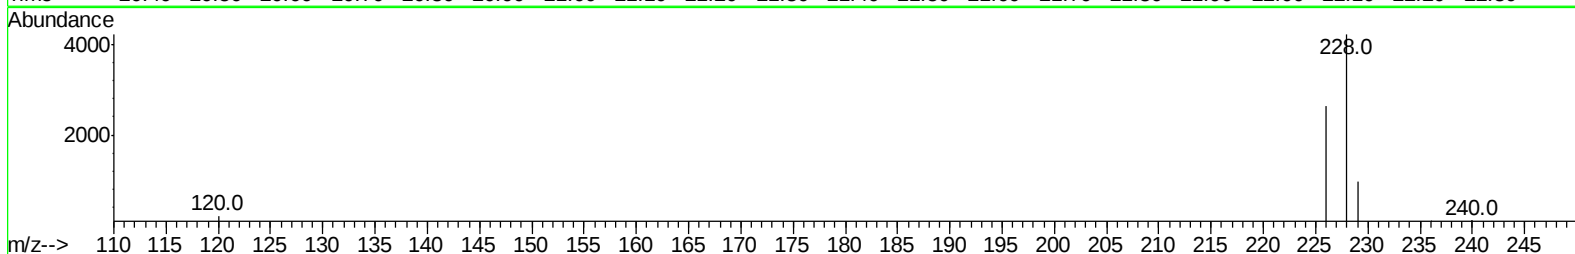


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003115.D
Acq On : 11 Oct 2018 22:22
Operator : MJ/SJ
Sample : J5368-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Oct 12 06:57:04 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

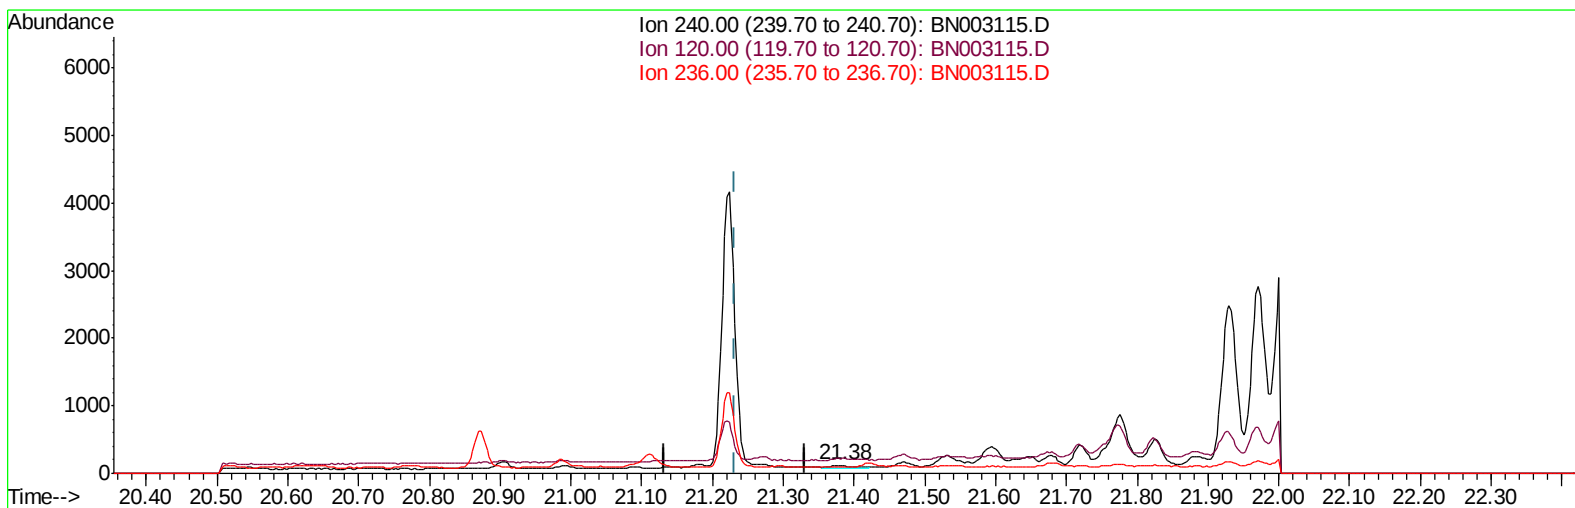

TIC: BN003115.D

(16) Chrysene-d12 (I)

21.384min (+0.152) 0.40ng/ul

response 63

Ion	Exp%	Act%
240.00	100	100
120.00	16.40	190.43#
236.00	28.10	80.87#
0.00	0.00	0.00