
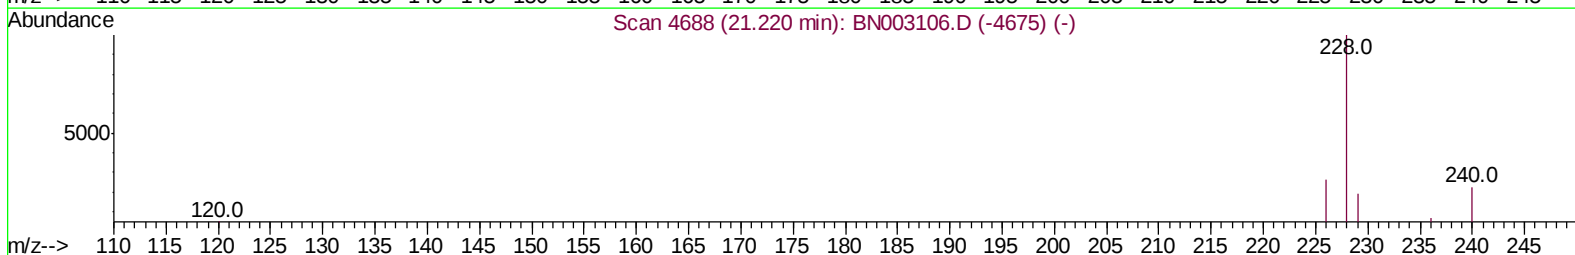
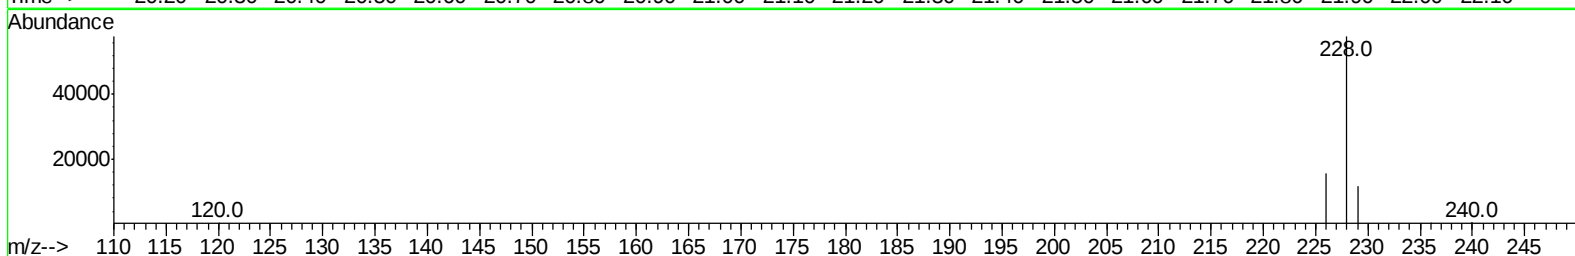


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003115.D
Acq On : 11 Oct 2018 22:22
Operator : MJ/SJ
Sample : J5368-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Oct 12 06:58:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

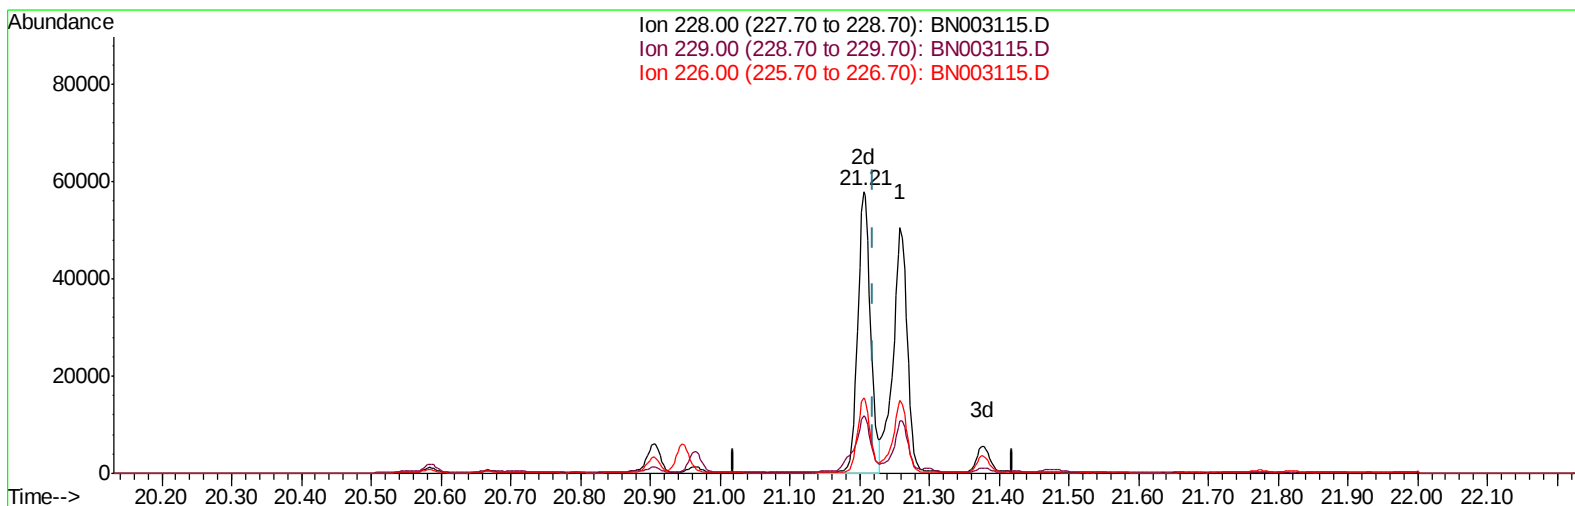

TIC: BN003115.D

(18) Benzo(a)anthracene

21.206min (-0.015) 4.62ng/ul m

response 75614

Ion	Exp%	Act%
228.00	100	100
229.00	20.20	20.26
226.00	27.90	27.04
0.00	0.00	0.00