
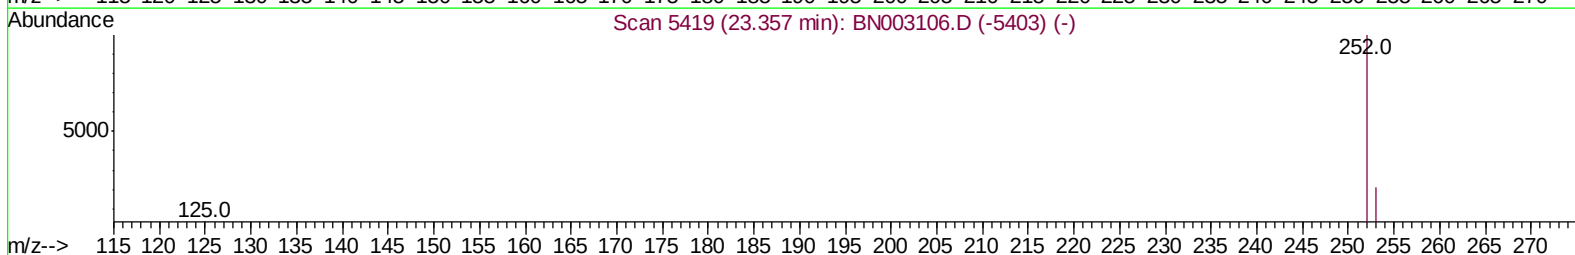
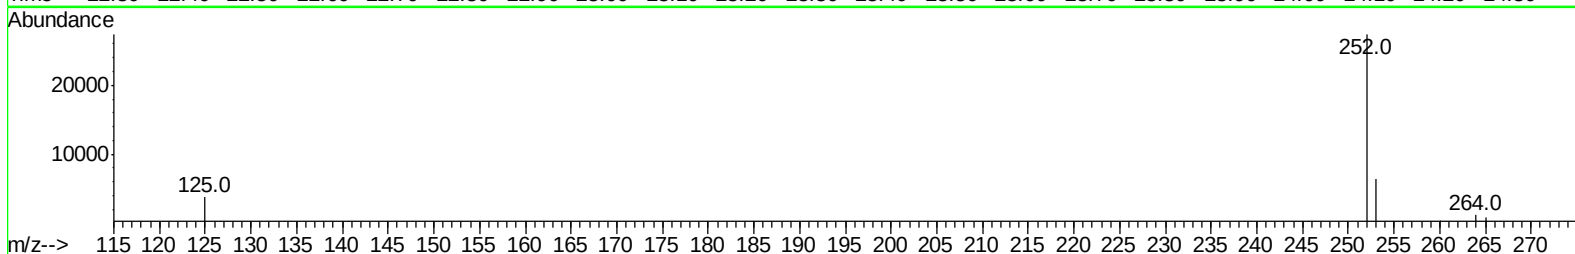


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003115.D
Acq On : 11 Oct 2018 22:22
Operator : MJ/SJ
Sample : J5368-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Oct 12 06:59:40 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

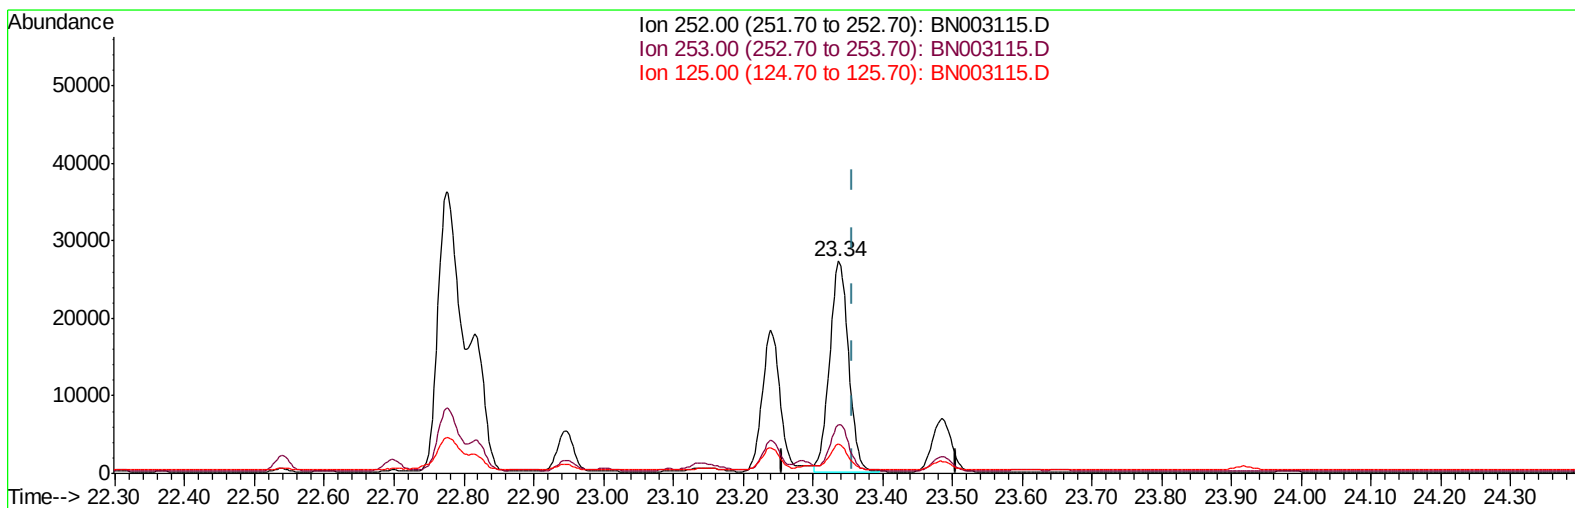

TIC: BN003115.D

(23) Benzo(a)pyrene (C)

23.336min (-0.020) 3.43ng/ul m

response 51567

Ion	Exp%	Act%
252.00	100	100
253.00	28.90	23.24
125.00	21.10	13.66#
0.00	0.00	0.00