
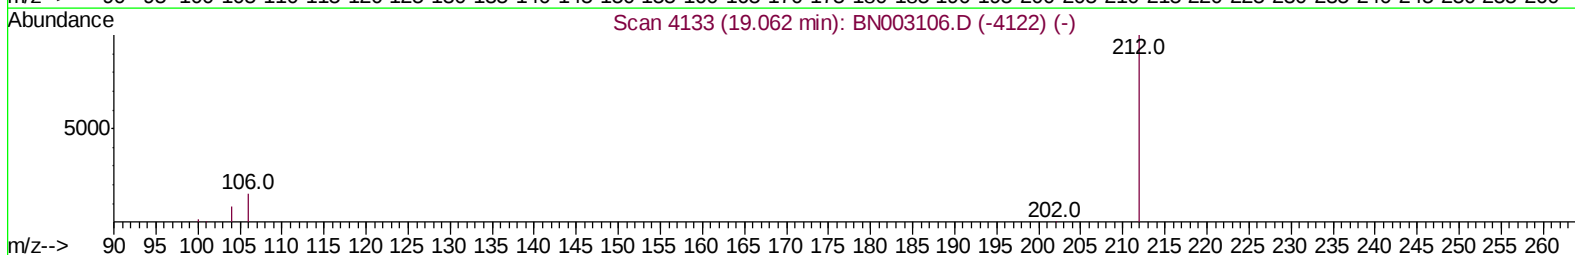
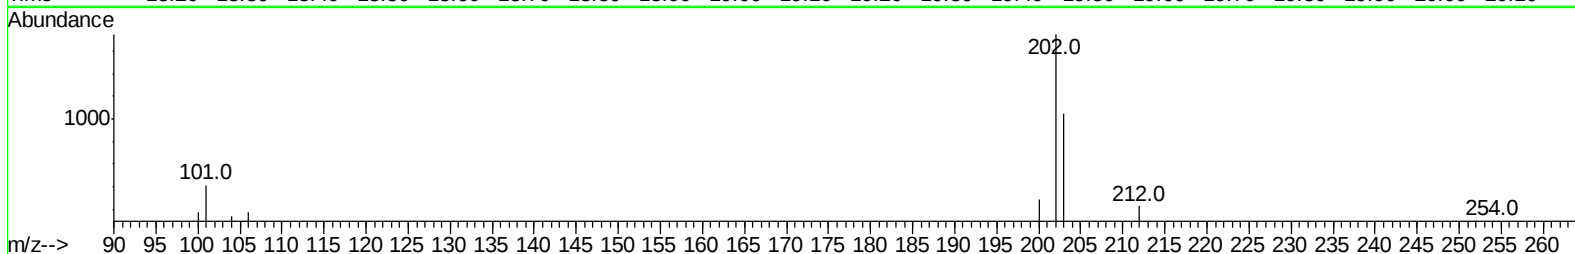


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\  
Data File : BN003116.D  
Acq On : 11 Oct 2018 22:57  
Operator : MJ/SJ  
Sample : J5230-04  
Misc :  
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Oct 12 07:03:09 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Oct 12 05:29:36 2018  
Response via : Initial Calibration

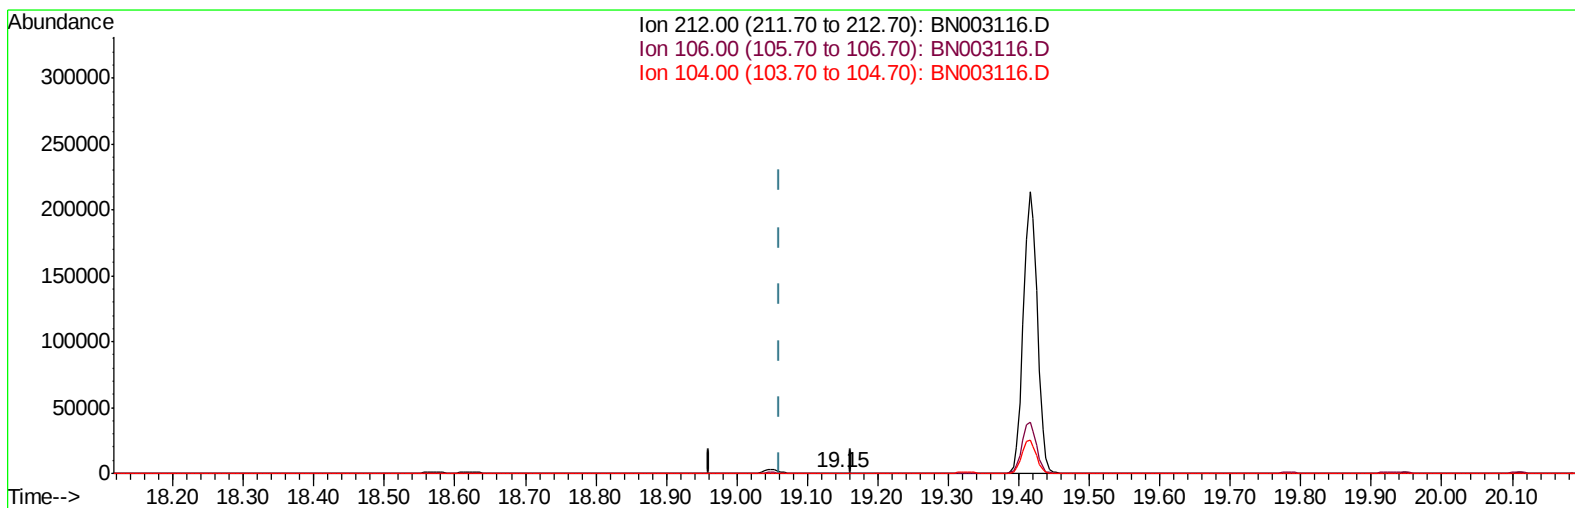

TIC: BN003116.D

(14) Fluoranthene-d10 (SURR)

19.146min (+0.084) 0.01ng/ul

response 211

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 212.00 | 100   | 100    |
| 106.00 | 15.40 | 34.60# |
| 104.00 | 8.60  | 21.80# |
| 0.00   | 0.00  | 0.00   |