
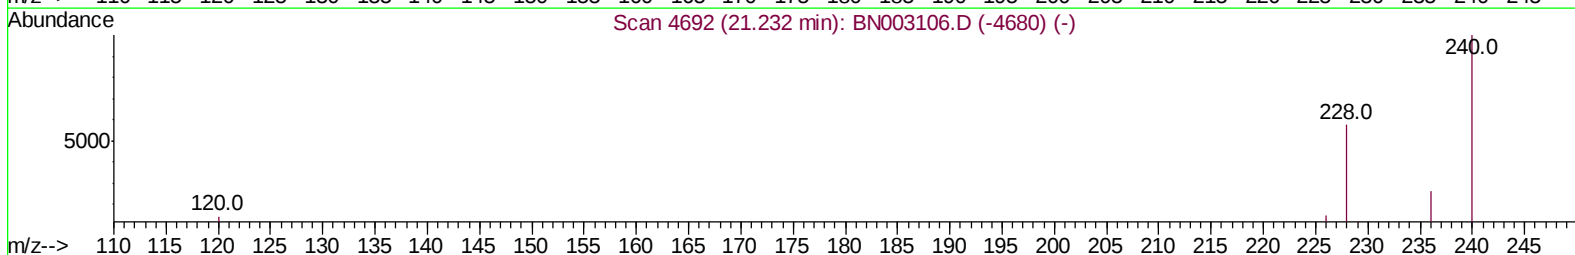
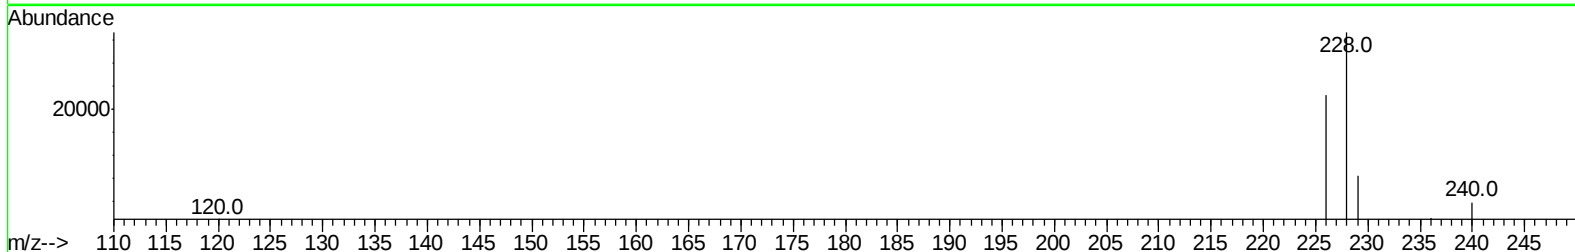


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
 Data File : BN003116.D
 Acq On : 11 Oct 2018 22:57
 Operator : MJ/SJ
 Sample : J5230-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Quant Time: Oct 12 07:03:09 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 12 05:29:36 2018
 Response via : Initial Calibration

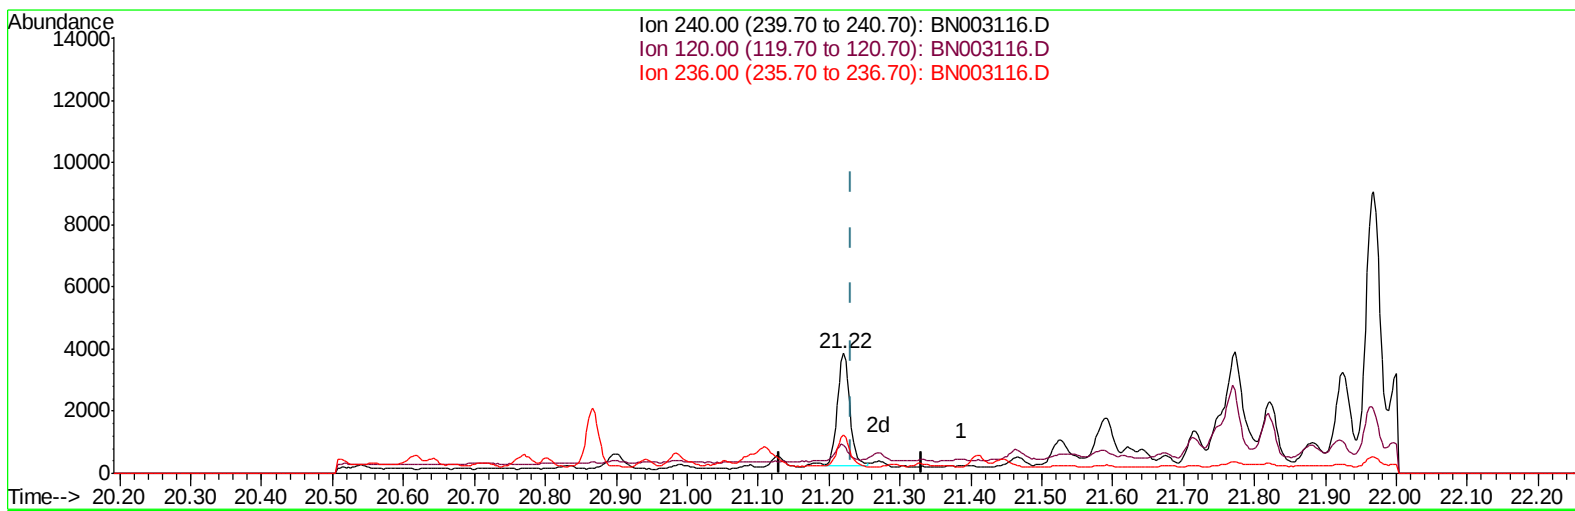

TIC: BN003116.D

(16) Chrysene-d12 (I)

21.220min (-0.012) 0.40ng/ul m

response 4432

Ion	Exp%	Act%
240.00	100	100
120.00	16.40	23.78#
236.00	28.10	31.60
0.00	0.00	0.00