
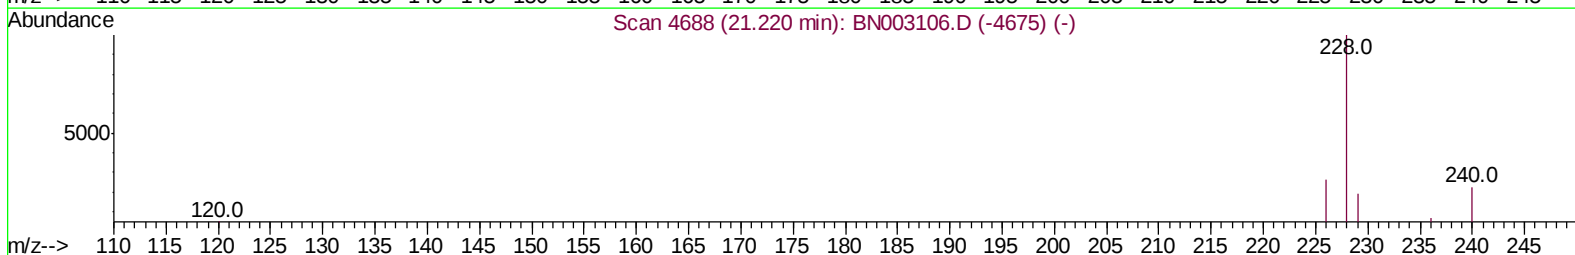
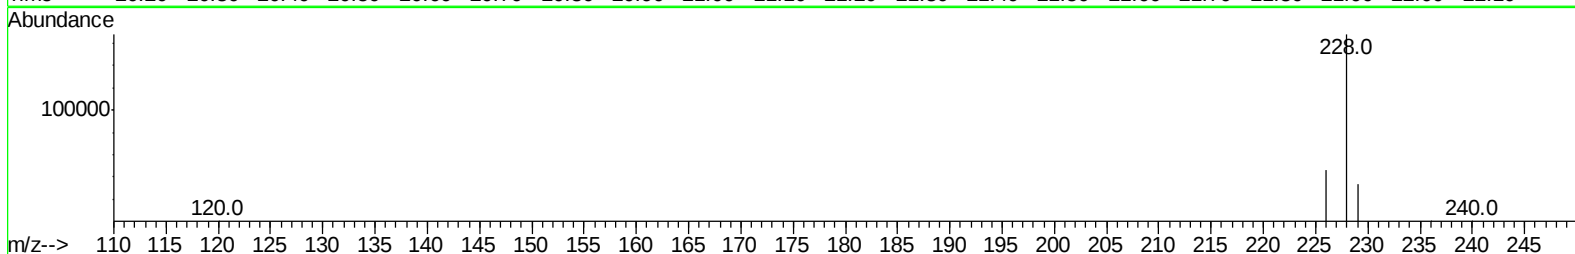


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003116.D
Acq On : 11 Oct 2018 22:57
Operator : MJ/SJ
Sample : J5230-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Oct 12 07:04:25 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

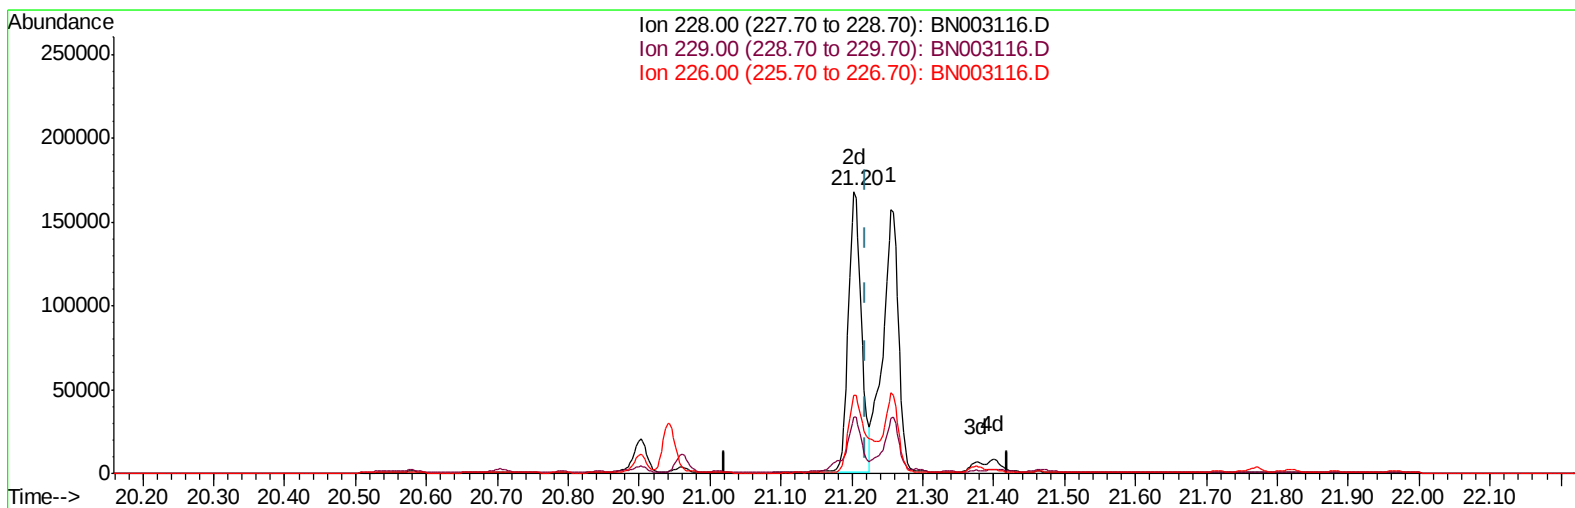

TIC: BN003116.D

(18) Benzo(a)anthracene

21.203min (-0.017) 14.89ng/ul m

response 212340

Ion	Exp%	Act%
228.00	100	100
229.00	20.20	20.15
226.00	27.90	27.85
0.00	0.00	0.00