
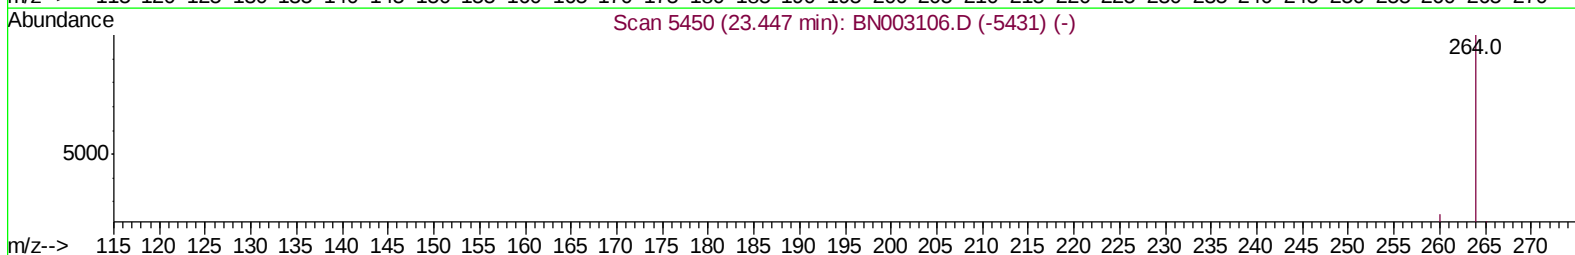
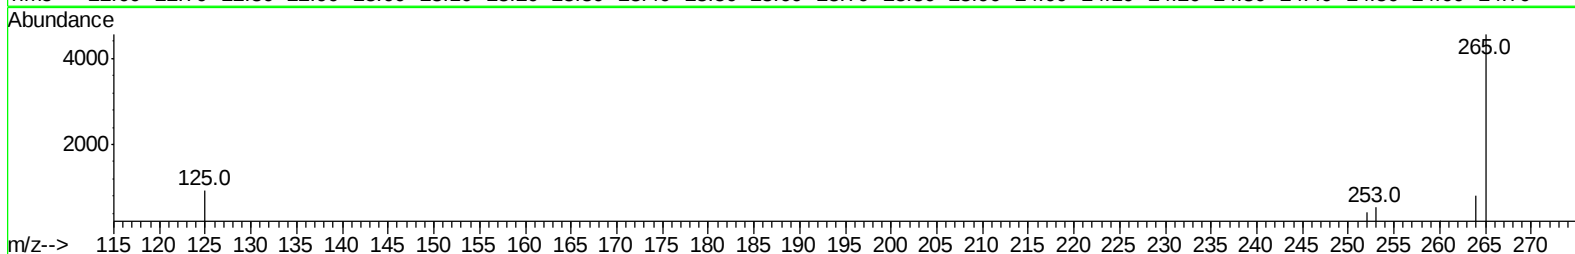


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003116.D
Acq On : 11 Oct 2018 22:57
Operator : MJ/SJ
Sample : J5230-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Oct 12 07:04:25 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

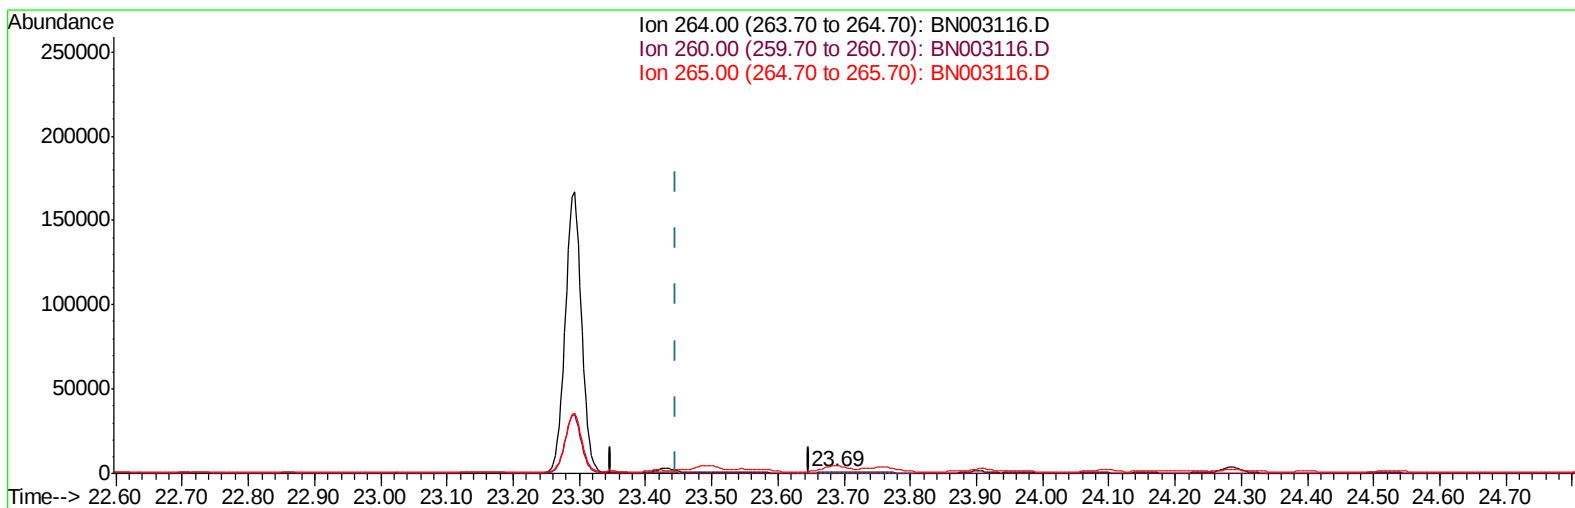

TIC: BN003116.D

(20) Perylene-d12 (I)

23.687min (+0.240) 0.40ng/ul

response 2886

Ion	Exp%	Act%
264.00	100	100
260.00	28.70	26.78
265.00	45.40	559.46#
0.00	0.00	0.00