
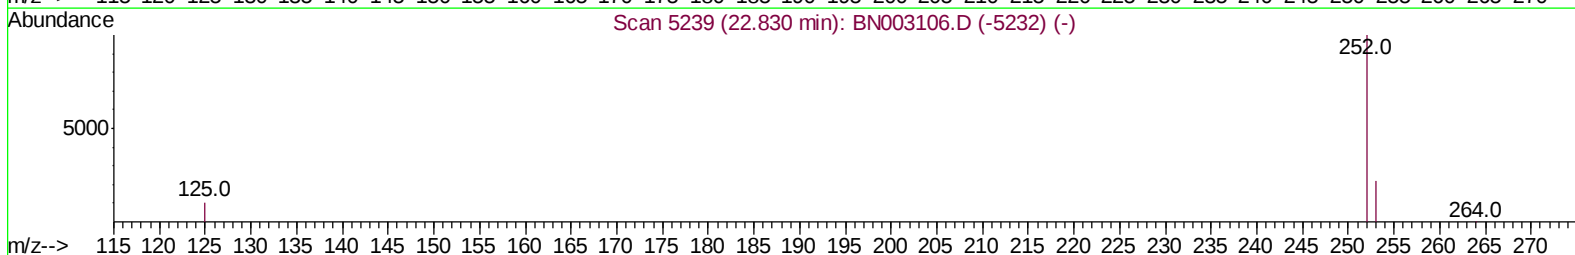
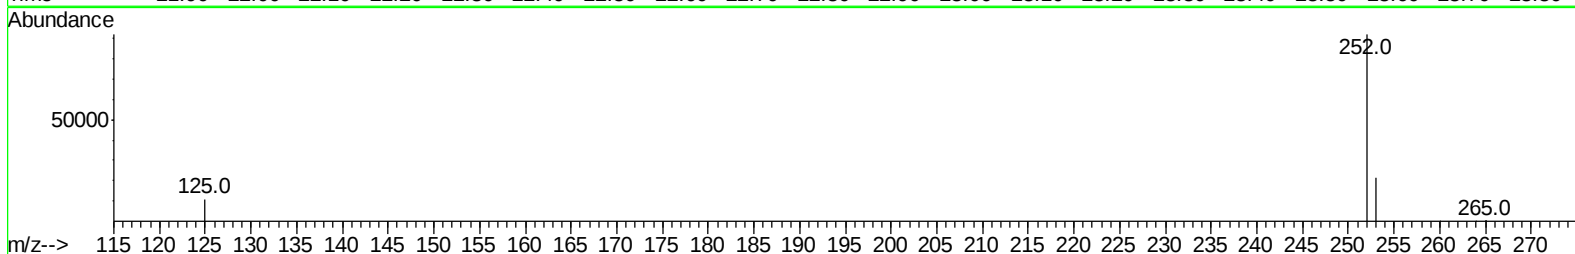


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003116.D
Acq On : 11 Oct 2018 22:57
Operator : MJ/SJ
Sample : J5230-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Oct 12 07:05:36 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

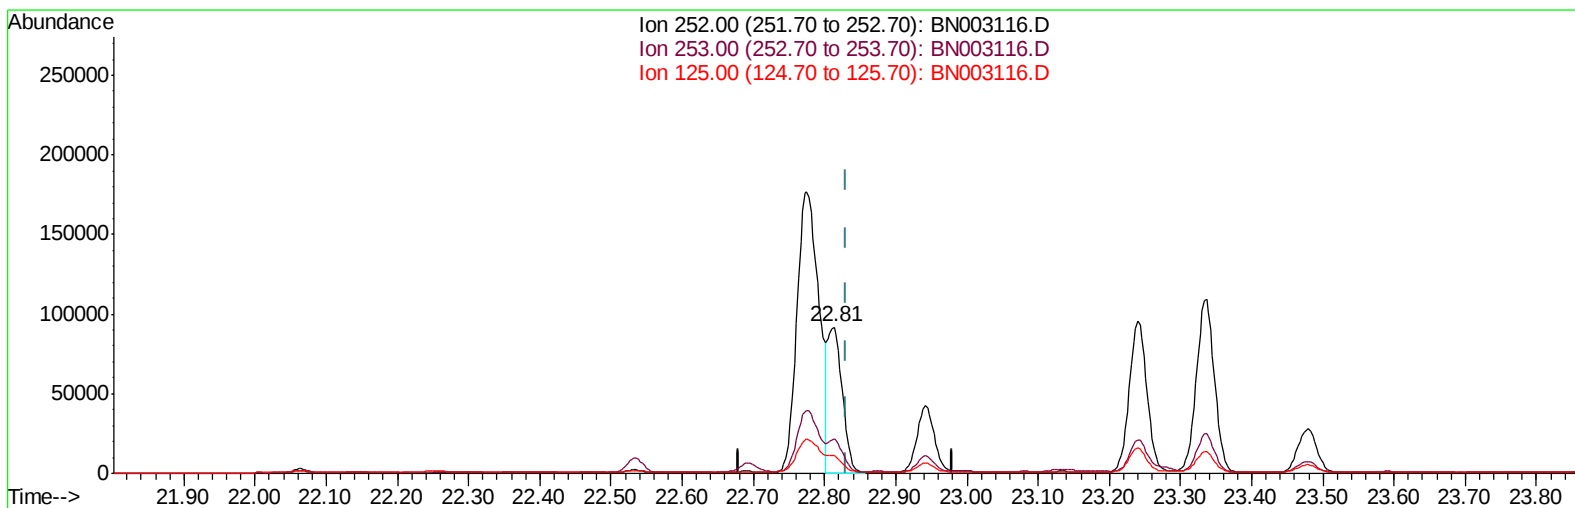

TIC: BN003116.D

(22) Benzo(k)fluoranthene

22.813min (-0.017) 7.13ng/ul m

response 131422

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	23.40
125.00	17.60	11.93#
0.00	0.00	0.00