
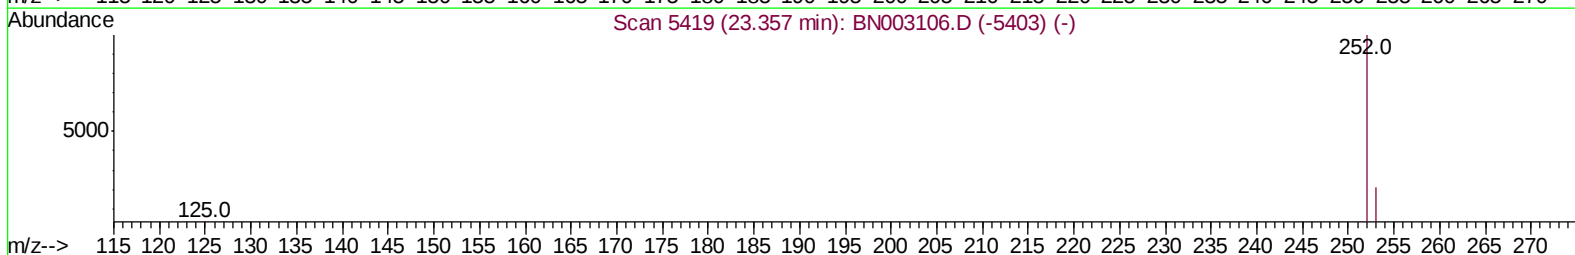
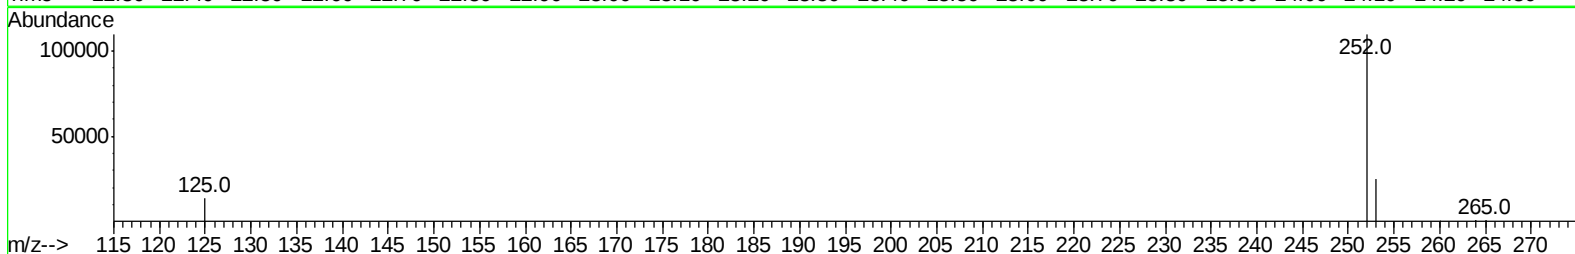


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003116.D
Acq On : 11 Oct 2018 22:57
Operator : MJ/SJ
Sample : J5230-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Oct 12 07:05:36 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

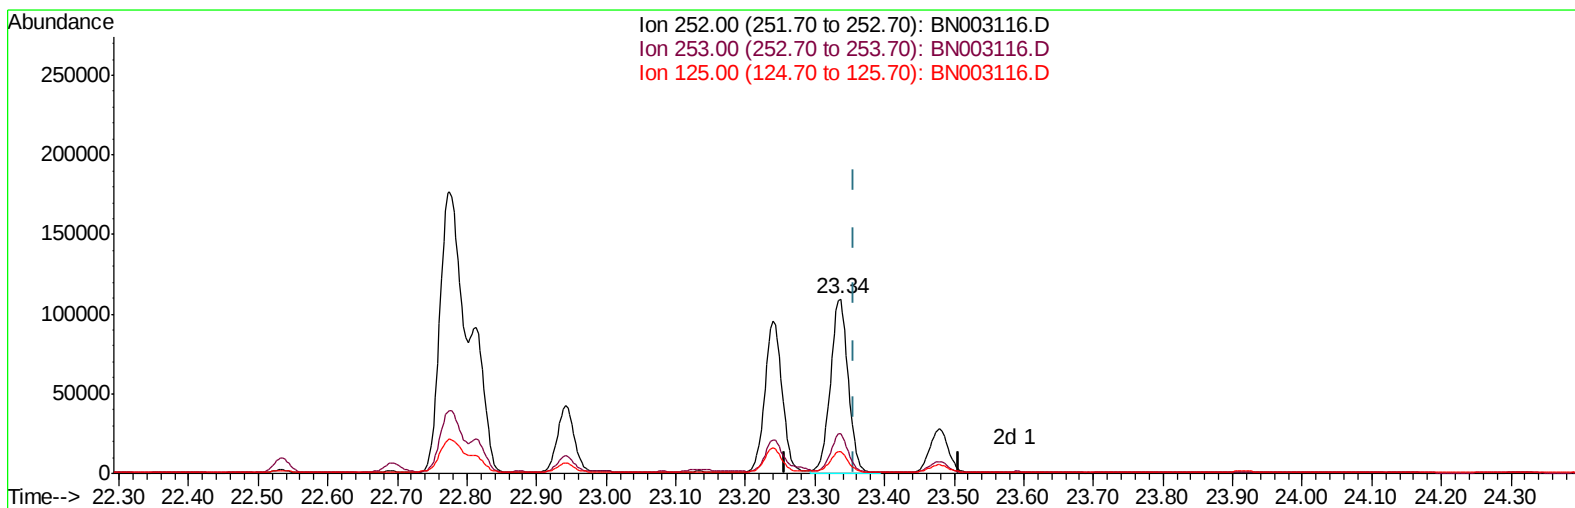

TIC: BN003116.D

(23) Benzo(a)pyrene (C)

23.336min (-0.020) 12.10ng/ul m

response 192761

Ion	Exp%	Act%
252.00	100	100
253.00	28.90	22.67#
125.00	21.10	12.71#
0.00	0.00	0.00