
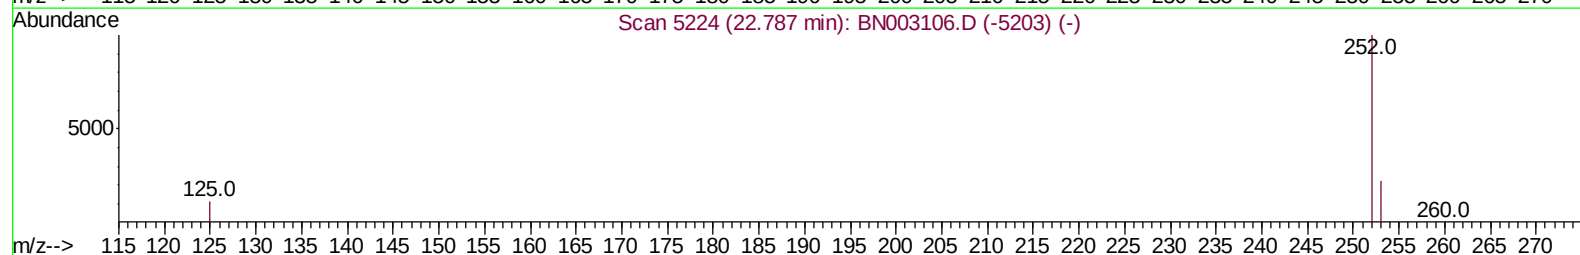
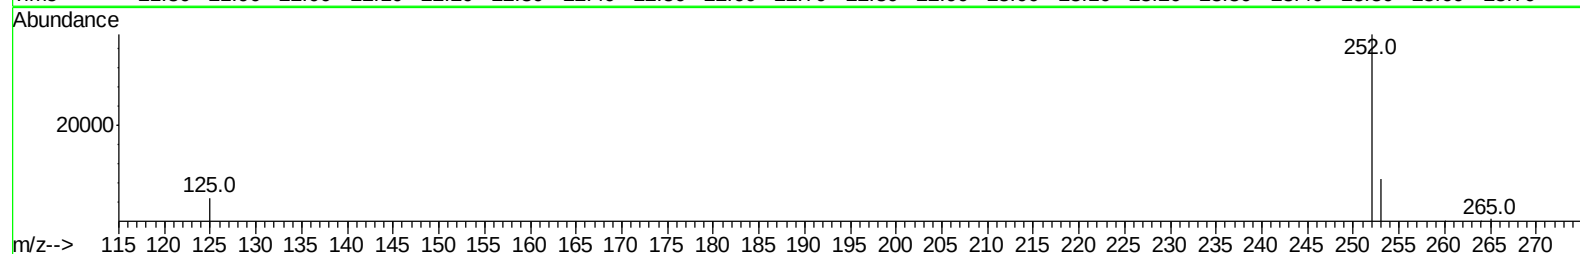


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003117.D
Acq On : 11 Oct 2018 23:32
Operator : MJ/SJ
Sample : J5230-04DL 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Oct 12 05:38:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

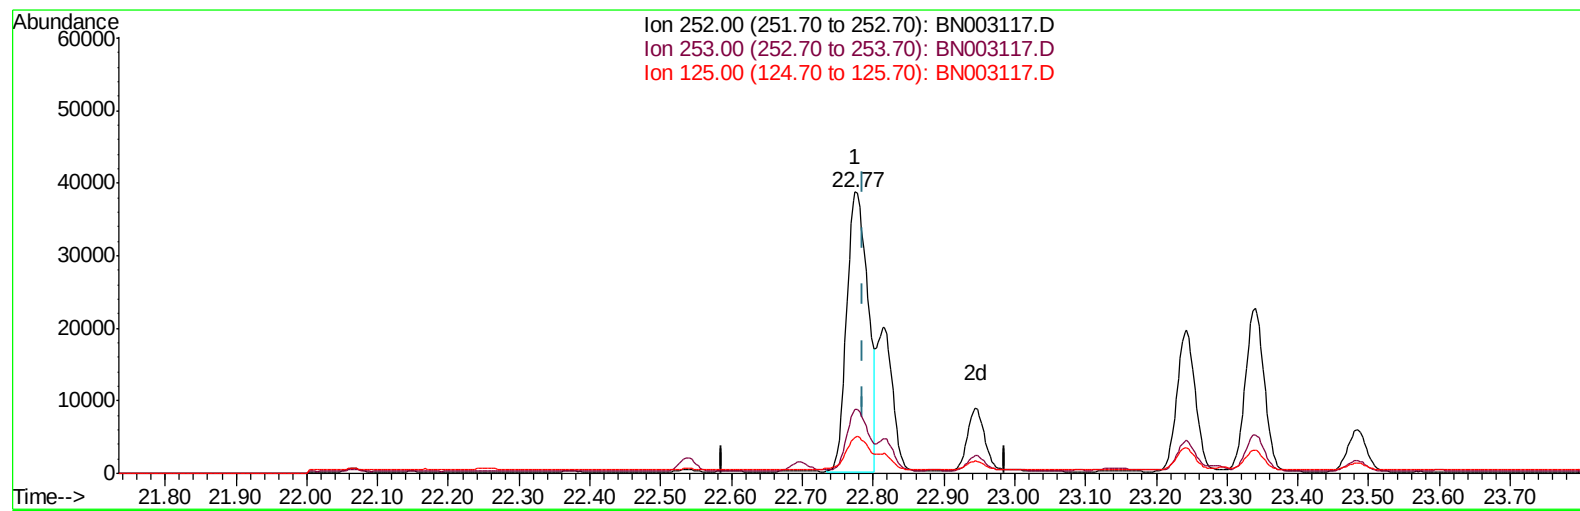

TIC: BN003117.D

(21) Benzo(b)fluoranthene

22.775min (-0.012) 4.06ng/ul m

response 80302

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	22.62
125.00	17.10	12.80
0.00	0.00	0.00