
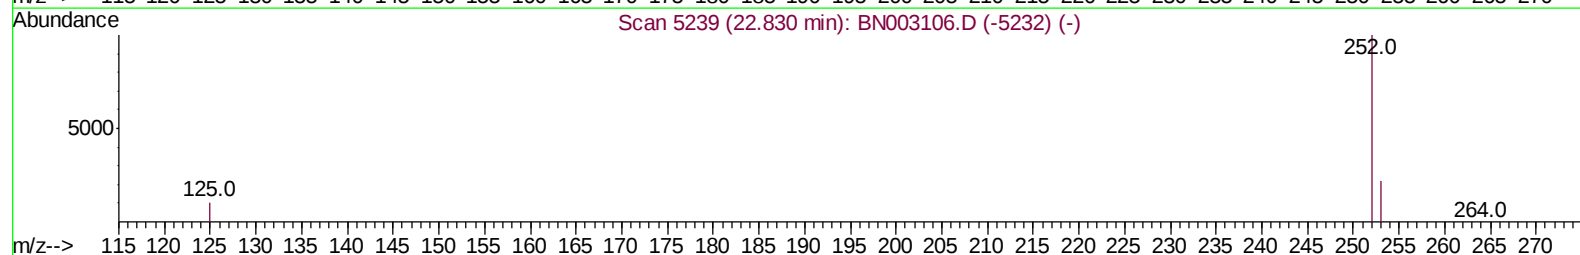
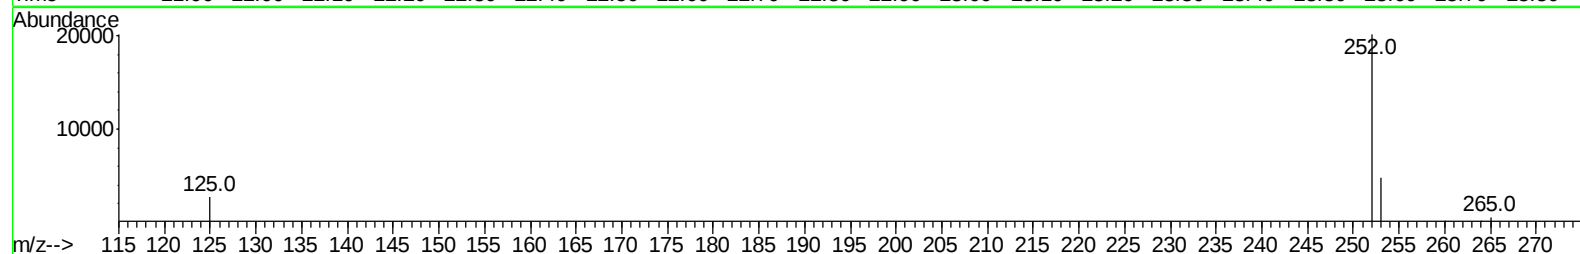


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003117.D
Acq On : 11 Oct 2018 23:32
Operator : MJ/SJ
Sample : J5230-04DL 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Oct 12 05:38:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

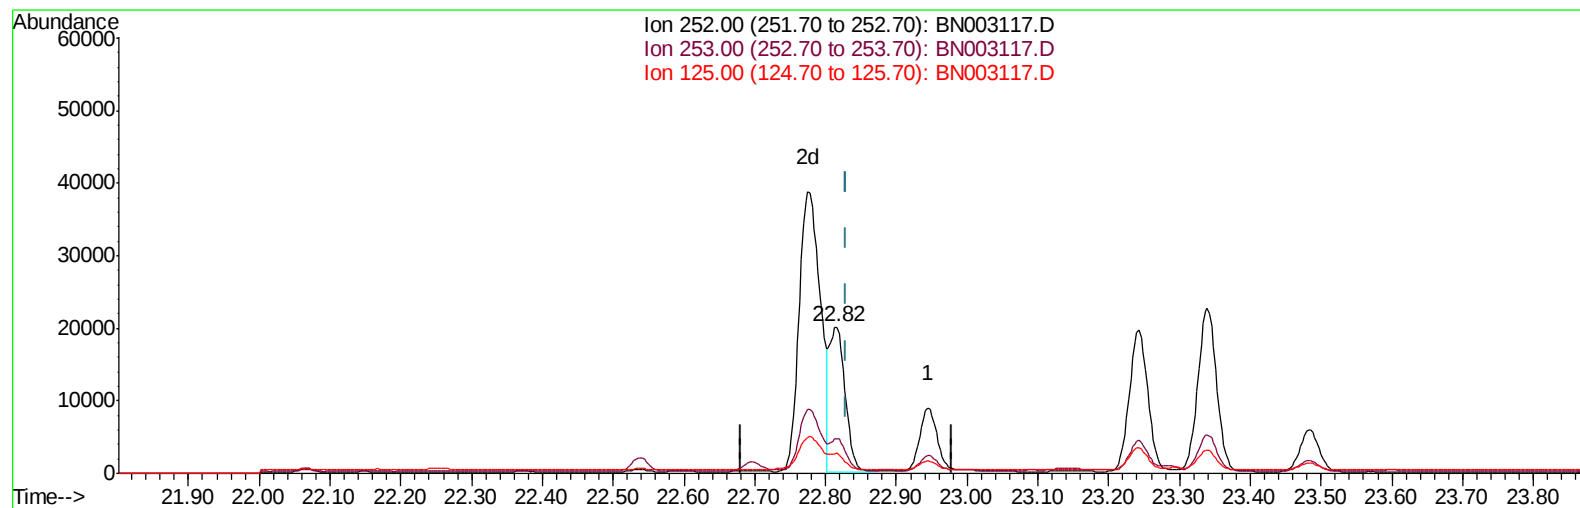

TIC: BN003117.D

(22) Benzo(k)fluoranthene

22.816min (-0.014) 1.52ng/ul m

response 31191

Ion	Exp%	Act%
252.00	100	100
253.00	26.60	23.95
125.00	17.60	13.63#
0.00	0.00	0.00