
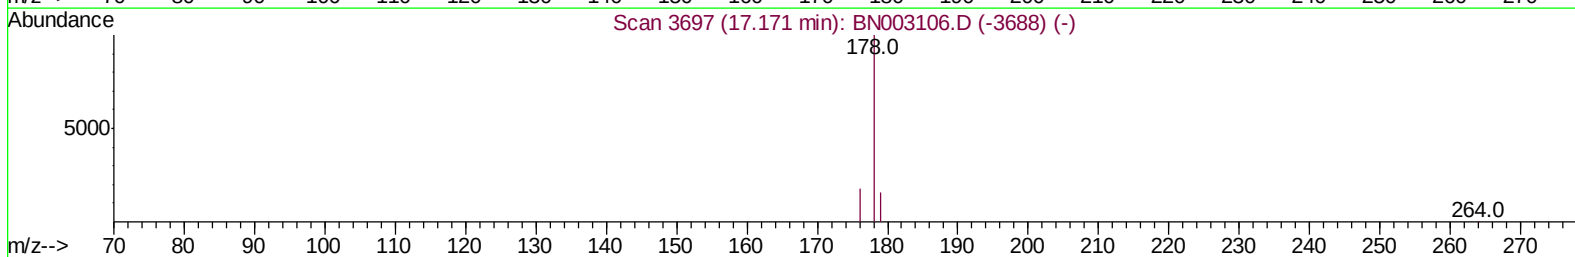
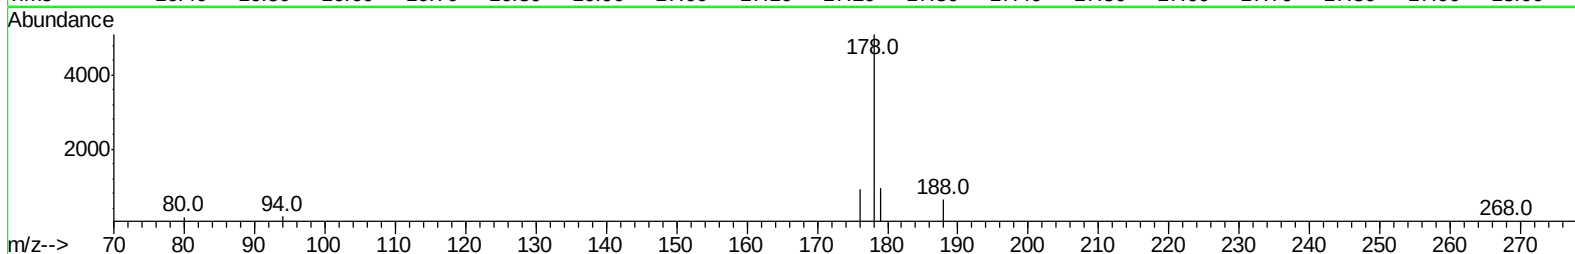


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003118.D
Acq On : 12 Oct 2018 00:08
Operator : MJ/SJ
Sample : J5230-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Oct 12 07:13:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

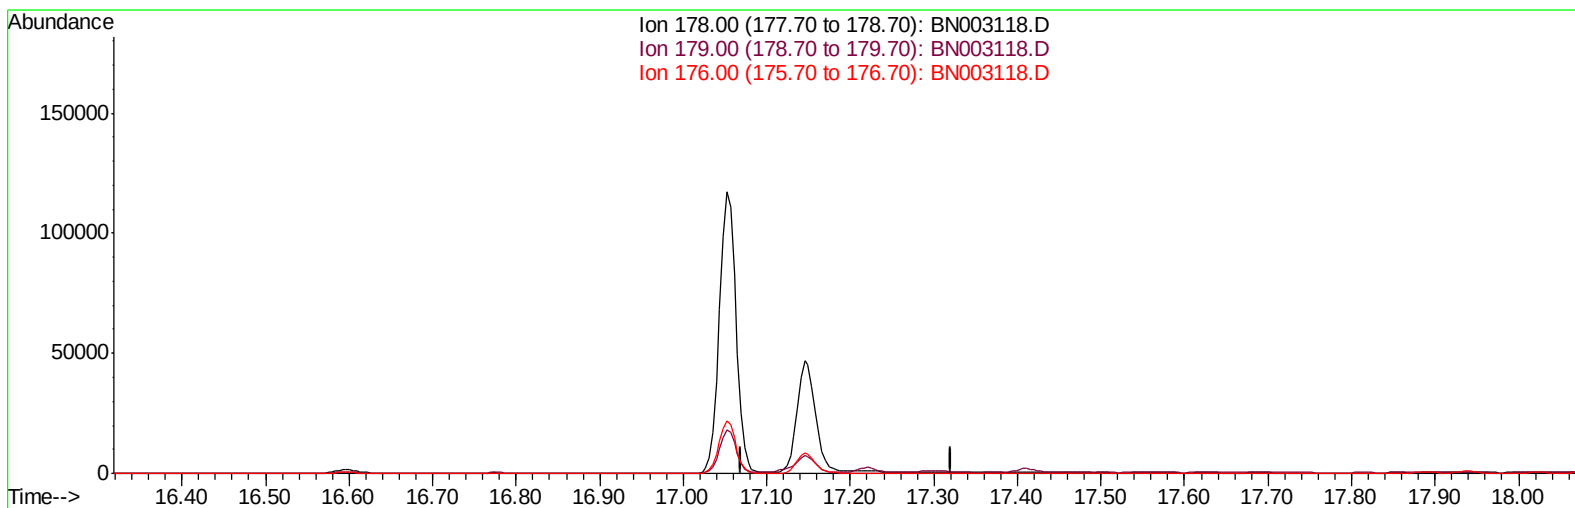

TIC: BN003118.D

(13) Anthracene

17.171min (-17.171) 0.00ng/ul

response 0

Ion	Exp%	Act%
178.00	100	0.00
179.00	16.30	0.00#
176.00	19.10	0.00#
0.00	0.00	0.00