
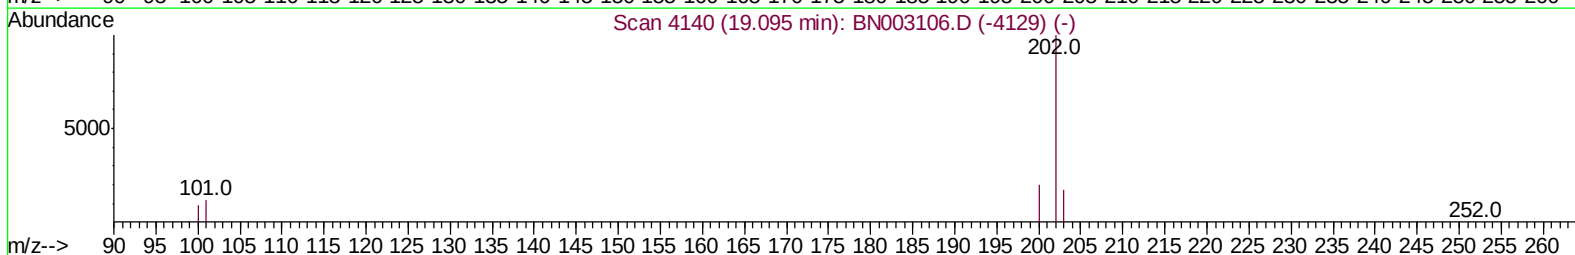
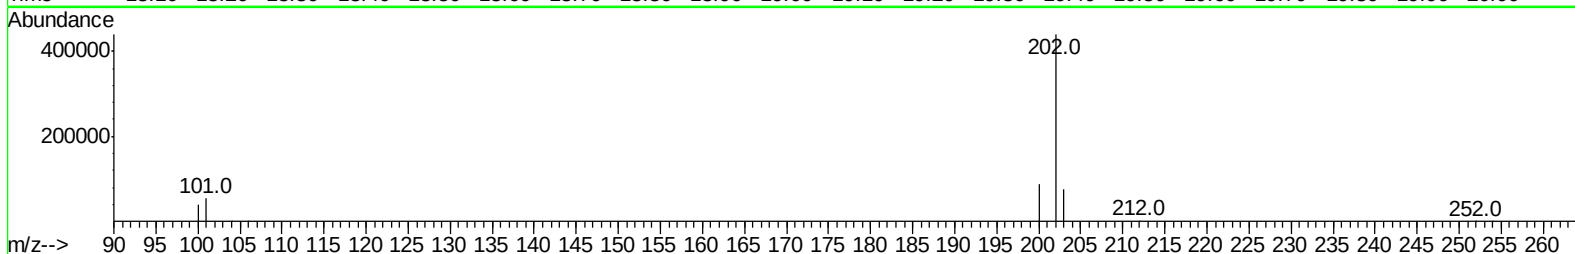


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101218\
Data File : BN003118.D
Acq On : 12 Oct 2018 00:08
Operator : MJ/SJ
Sample : J5230-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Oct 12 07:13:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN100918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 12 05:29:36 2018
Response via : Initial Calibration

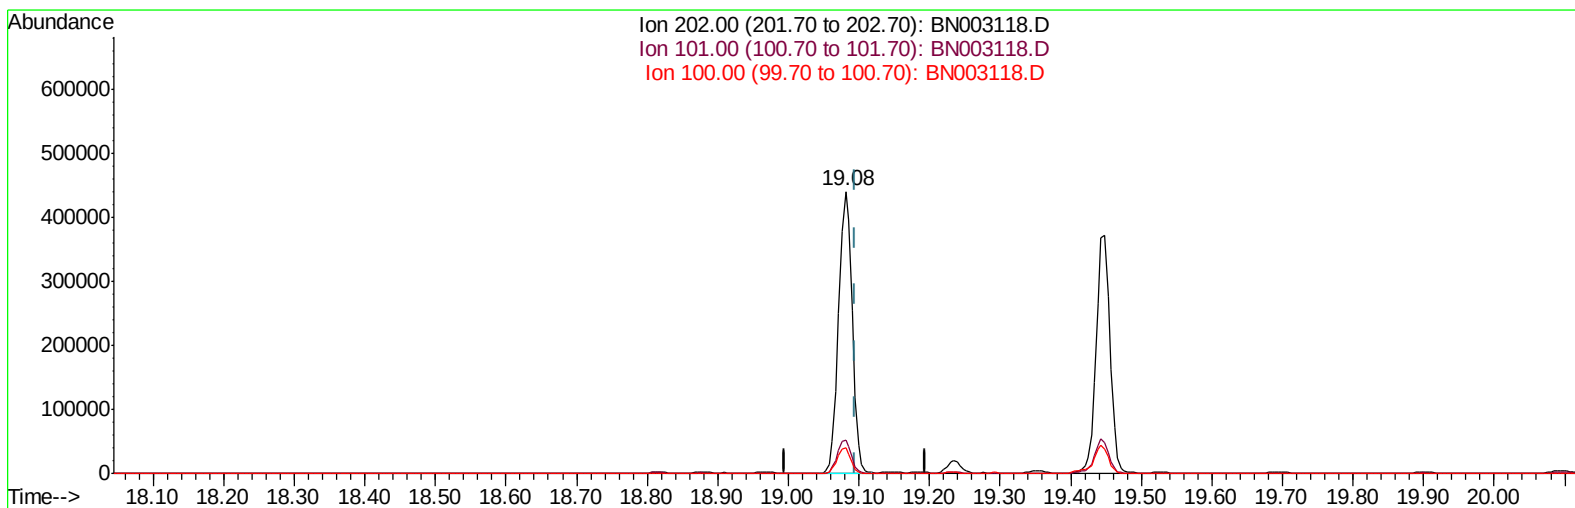

TIC: BN003118.D

(15) Fluoranthene (C)

19.081min (-0.014) 19.38ng/ul m

response 584659

Ion	Exp%	Act%
202.00	100	100
101.00	12.30	12.05
100.00	9.10	8.89
0.00	0.00	0.00